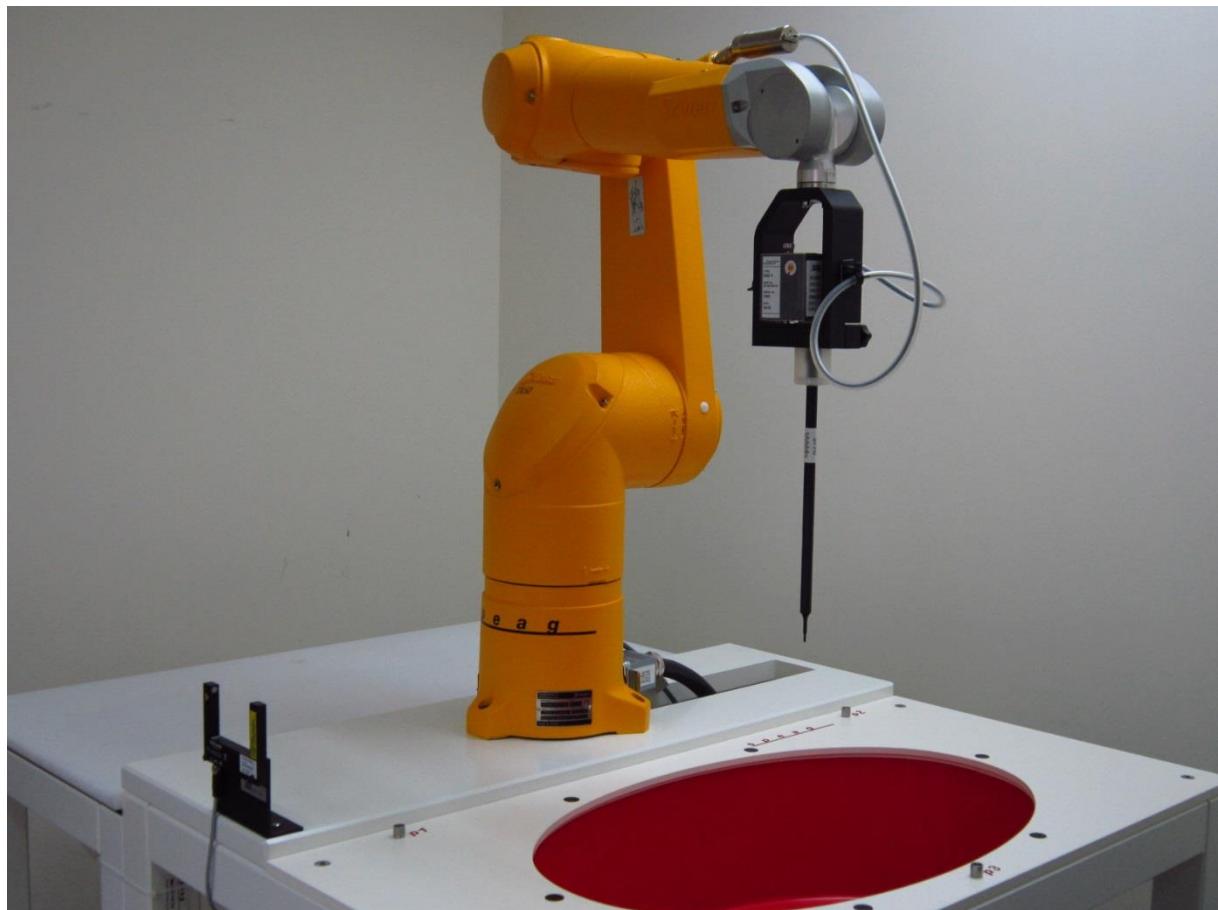


Appendix D

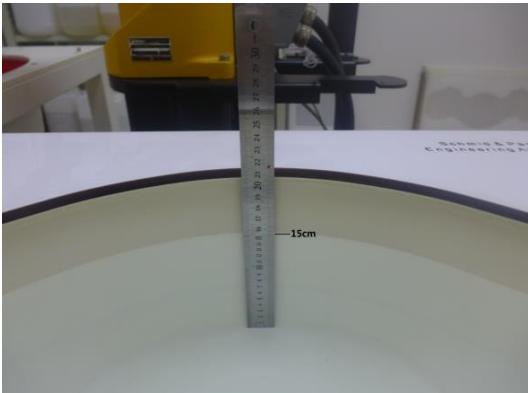
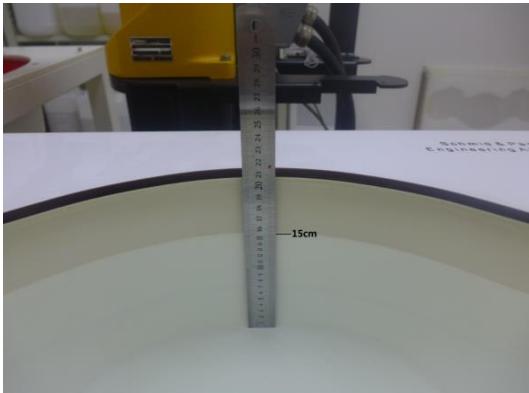
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Tissue Simulant Liquid for Head 2450	Tissue Simulant Liquid for Head 5GHz
 A photograph showing a shallow, curved pool of tissue simulant liquid in a white container. A vertical ruler is positioned next to the container, with the 15cm mark clearly visible. The liquid surface is slightly irregular, reflecting the light.	 A photograph showing a shallow, curved pool of tissue simulant liquid in a white container. A vertical ruler is positioned next to the container, with the 15cm mark clearly visible. The liquid surface is slightly irregular, reflecting the light.

3. Photographs of EUT test position

Photo 1: Front side 0mm	Photo 2: Back side 0mm
Photo 3: Left side 0mm	Photo 4: Right side 0mm
Photo 5: Top side 0mm	Photo 6: Bottom side 0mm

4. EUT Constructional Details

Details please Refer to the <External Photos> & <Internal Photos>.