



Itamar Medical

Antenna Return Loss

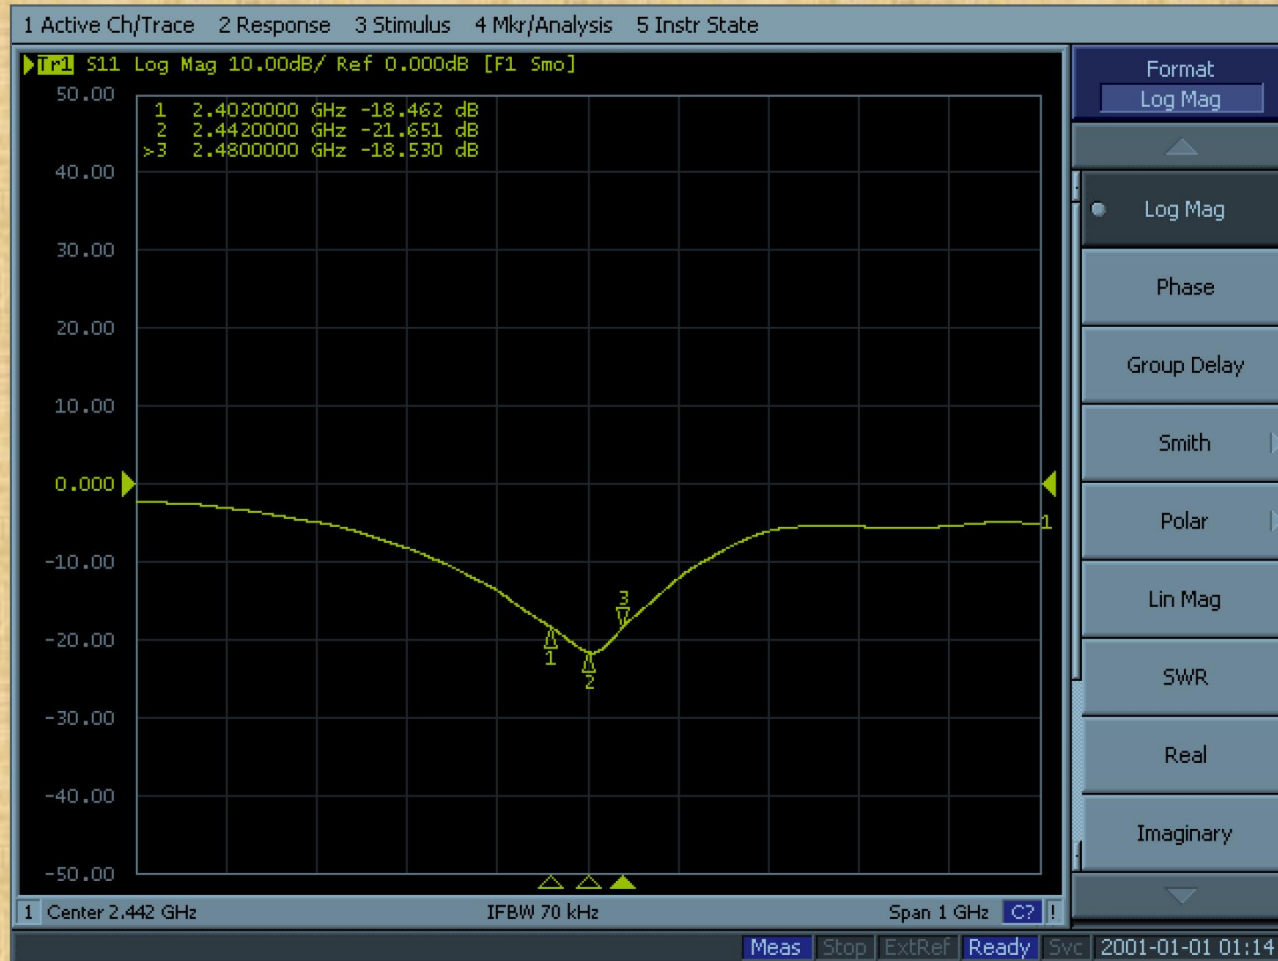


Itamar Medical

Antenna VSWR

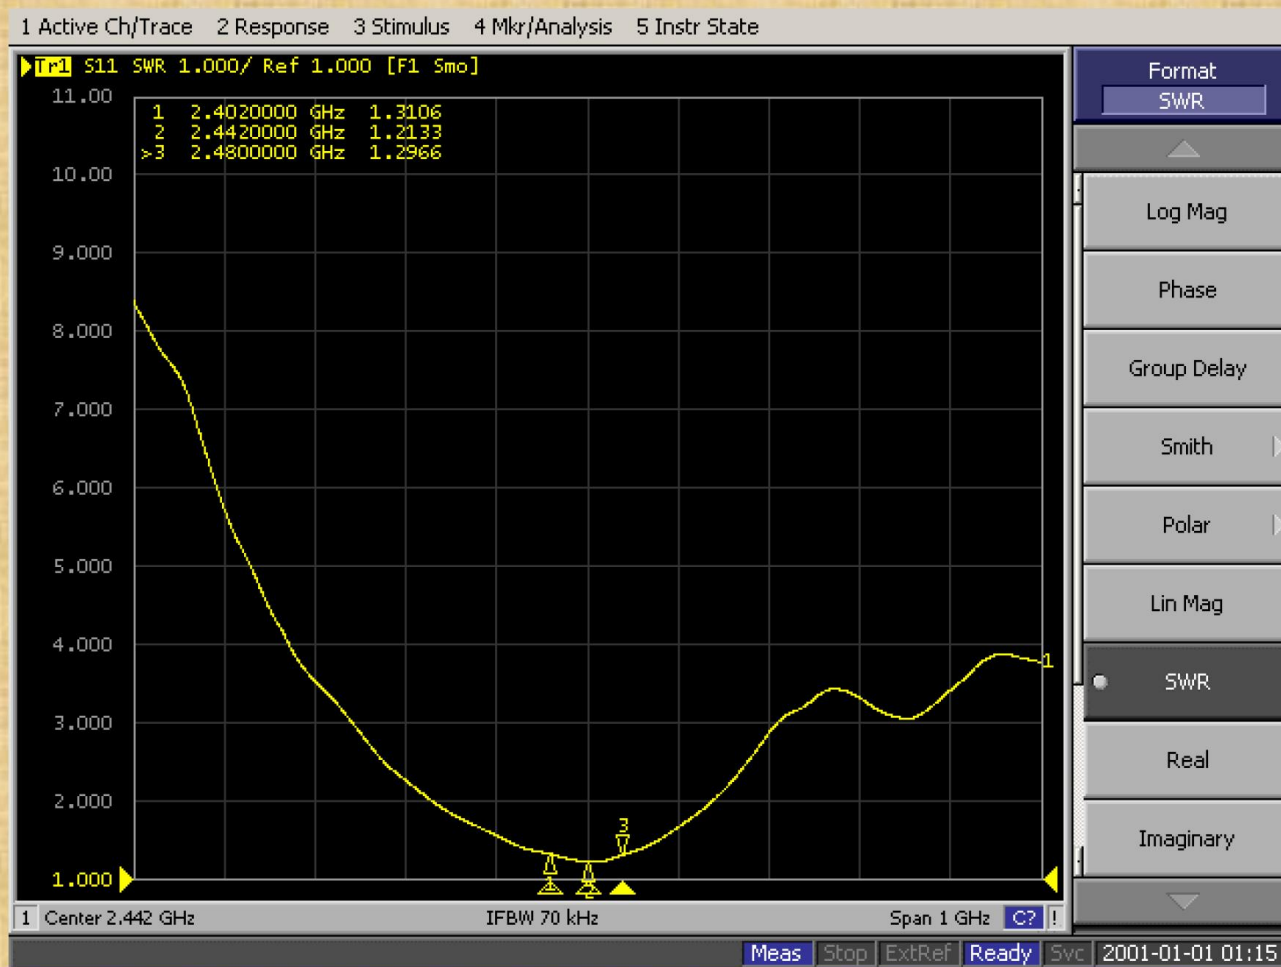

Itamar Medical

Antenna Smith Chart

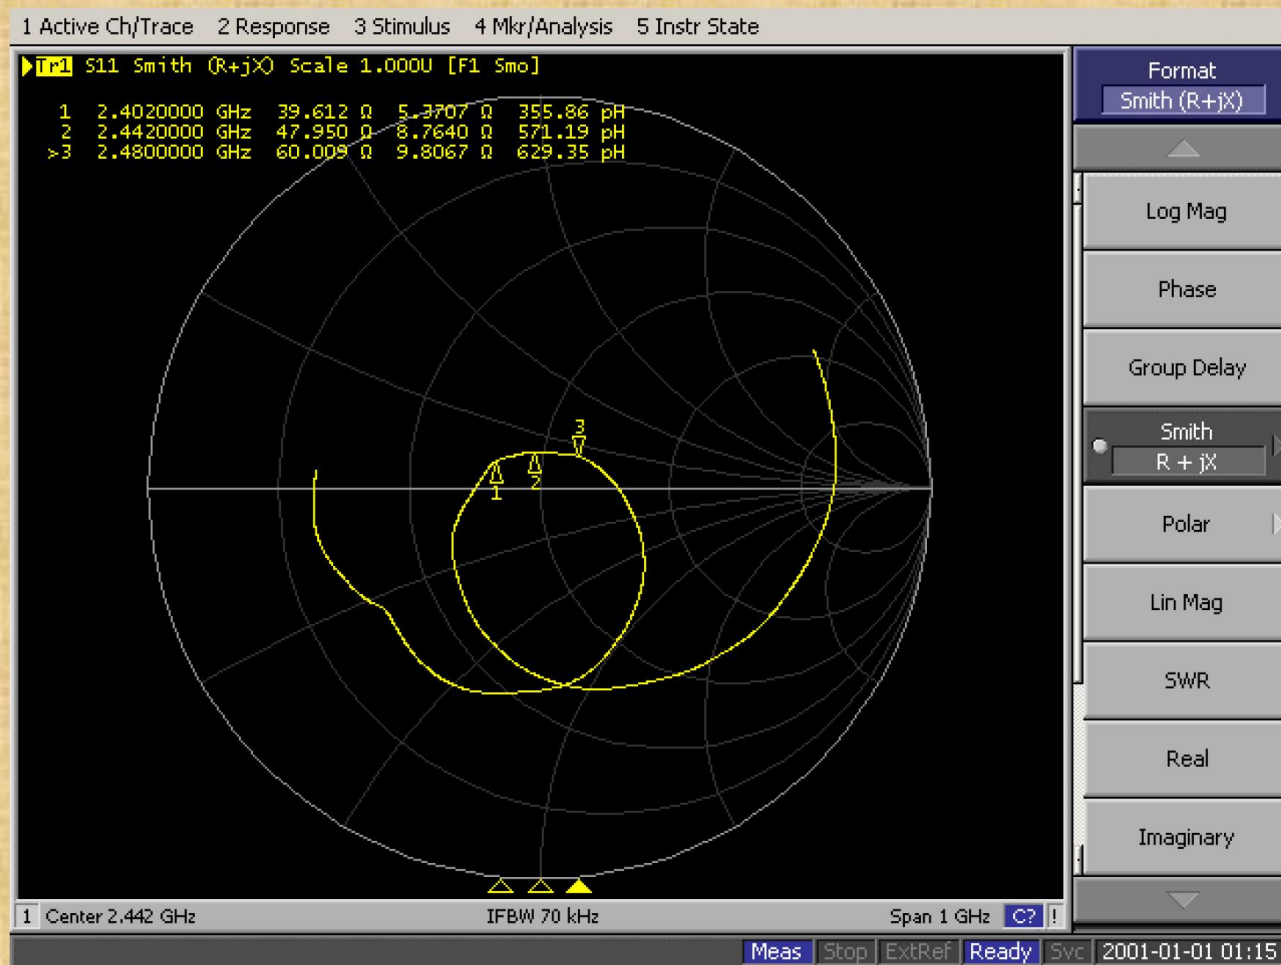


Itamar Medical

WP400 Free Space 3D Chamber Efficiency Antenna Test Results

Band	Frequency [MHz]	Ant EFF [%]	Ant 3D EFF [dbi]	Peak Gain [dBi]
BT	2402	63.24	-1.99	+3.50
BT	2440	44.16	-3.55	+2.77
BT	2480	44.06	-3.71	+3.71


Itamar Medical

WP400 Free Space 3D Chamber Efficiency Antenna Pattern Test Results

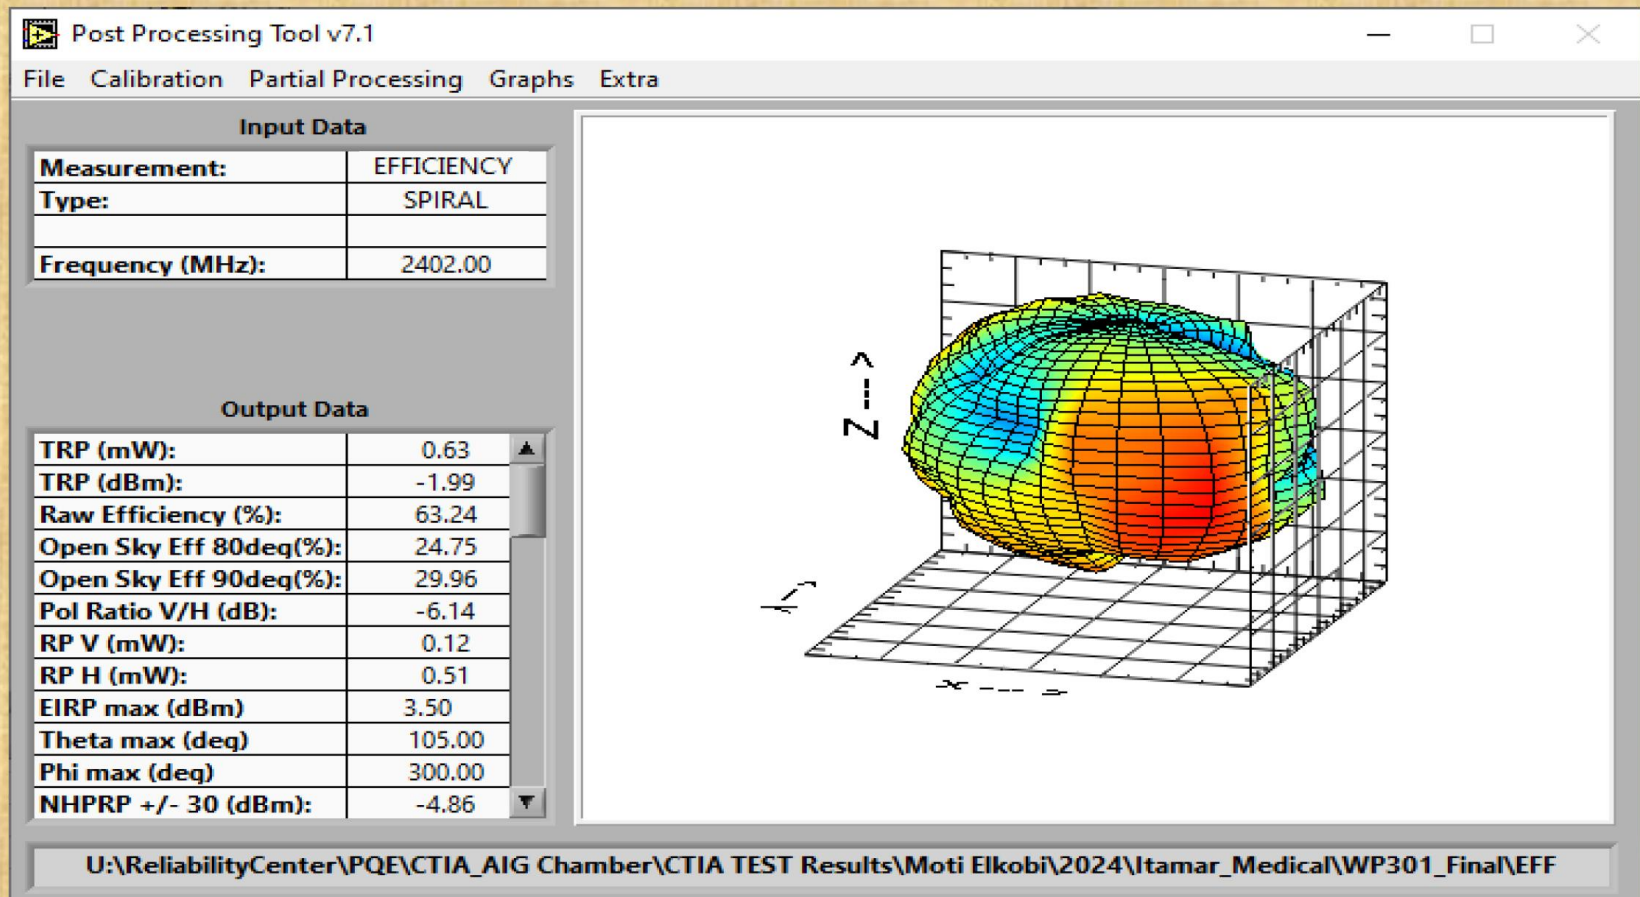

Itamar Medical

WP400 Free Space 3D Chamber Efficiency Antenna Pattern Test Results

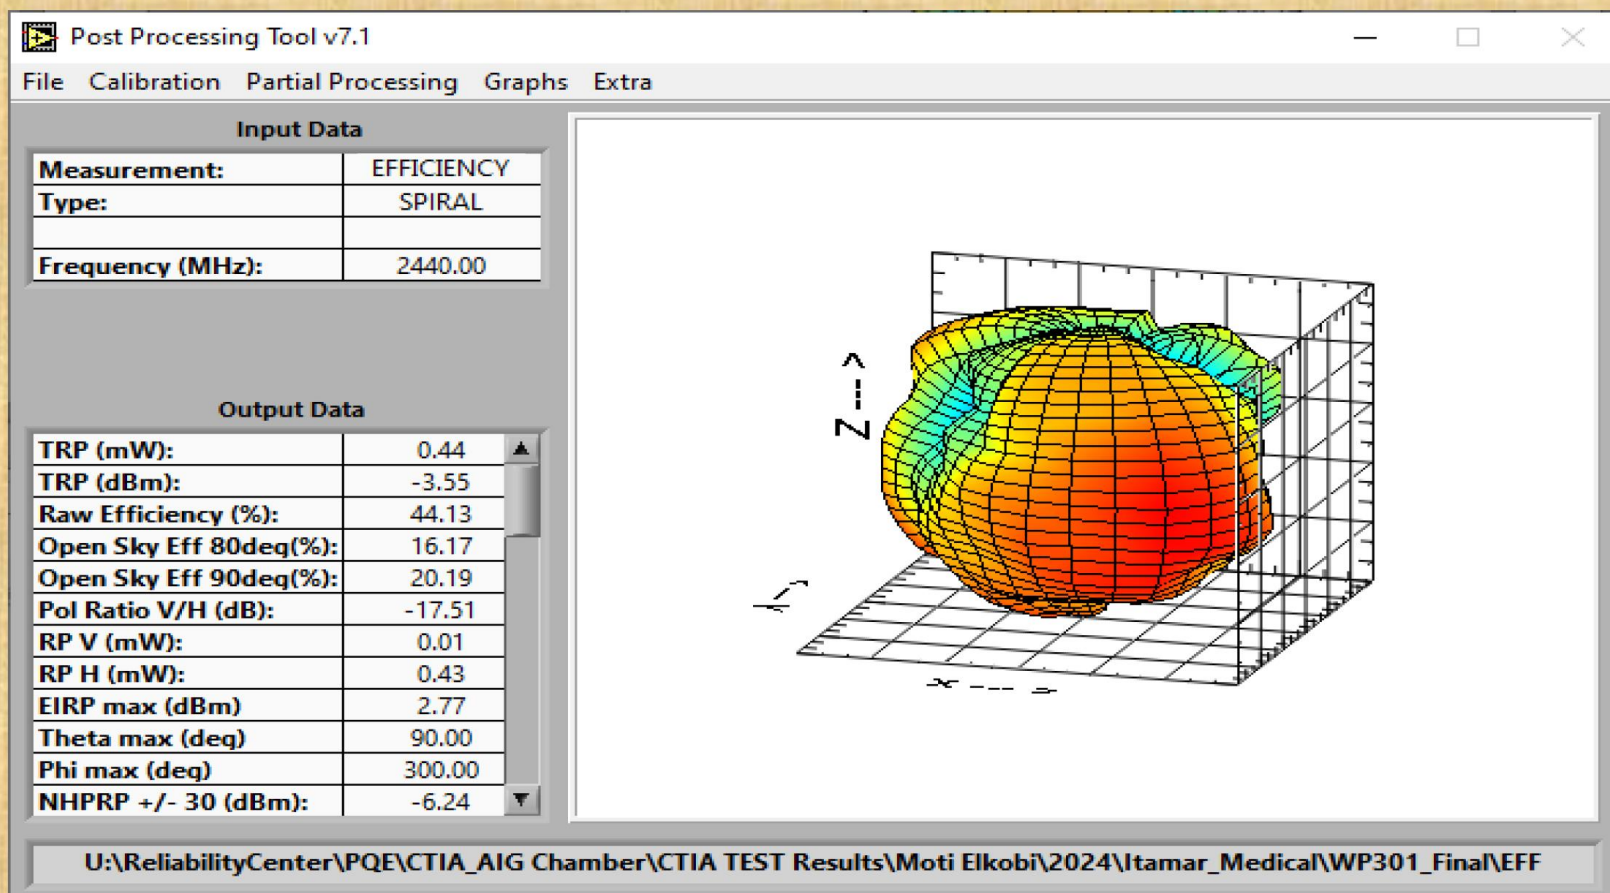

Itamar Medical

WP400 Free Space 3D Chamber Efficiency Antenna Pattern Test Results

