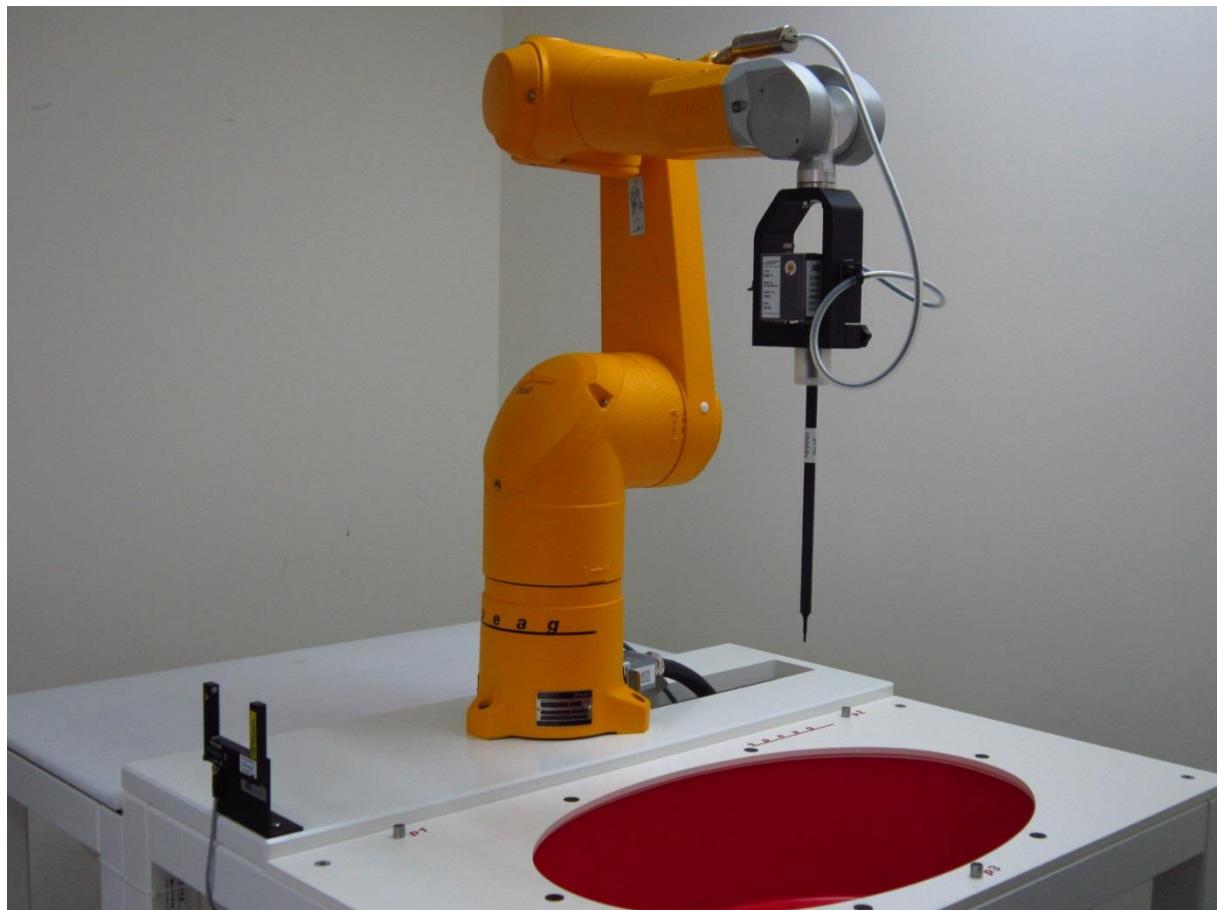


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

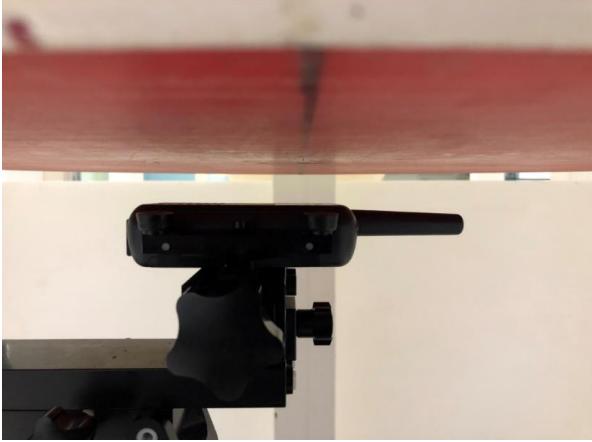
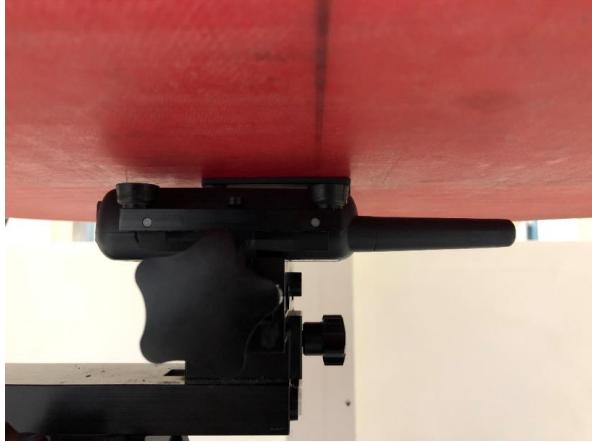


2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 450MHz



3. Photographs of EUT test position

Photo 2: Front side 25mm	Photo 3: Back side 0mm with Back Splint
 A photograph showing a black device mounted on a stand, positioned in front of a red wall. The device is angled slightly to the left. The background is a plain, light-colored wall.	 A photograph showing the same black device from a different angle, positioned directly behind the red wall. The device is mounted on a stand and appears to be facing the wall. A black back splint is visible behind the device.

4. EUT Constructional Details

Details please Refer to the <External Photos>&<Internal Photos>.