


450 Head

Calibrated impedance: $55.7\Omega - 5.3j\Omega$; Measurement impedance: $58.4\Omega + 6.5j\Omega$ (within 5Ω)



Calibrated return loss: -22.6dB; Measurement return loss: -22.7dB (within 20%)

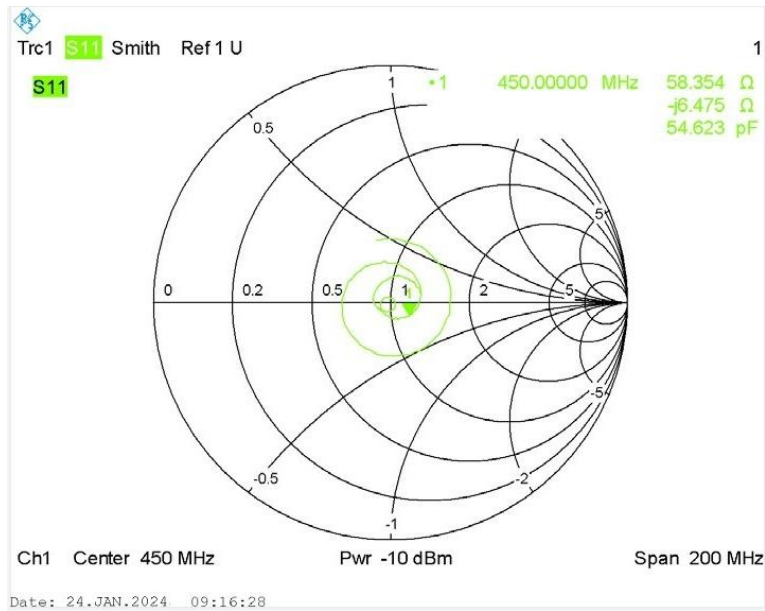