




MedicSMART
WHEN SECONDS COUNT, COUNT ON US

User Manual


REV: A.4 . Draft

1. Installation
2. General safety notes.
3. FCC Compliance Statement

1. AMD Cabinet
2. Wall Mounting
3. Cable power


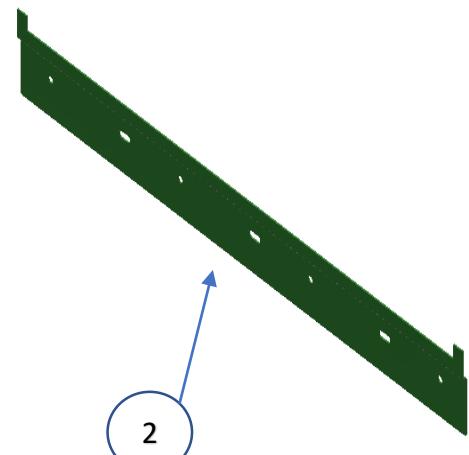


Step 1: Fit the Wall Mounting on the Wall, Use 4 Screw #12 x 1 ¼ in

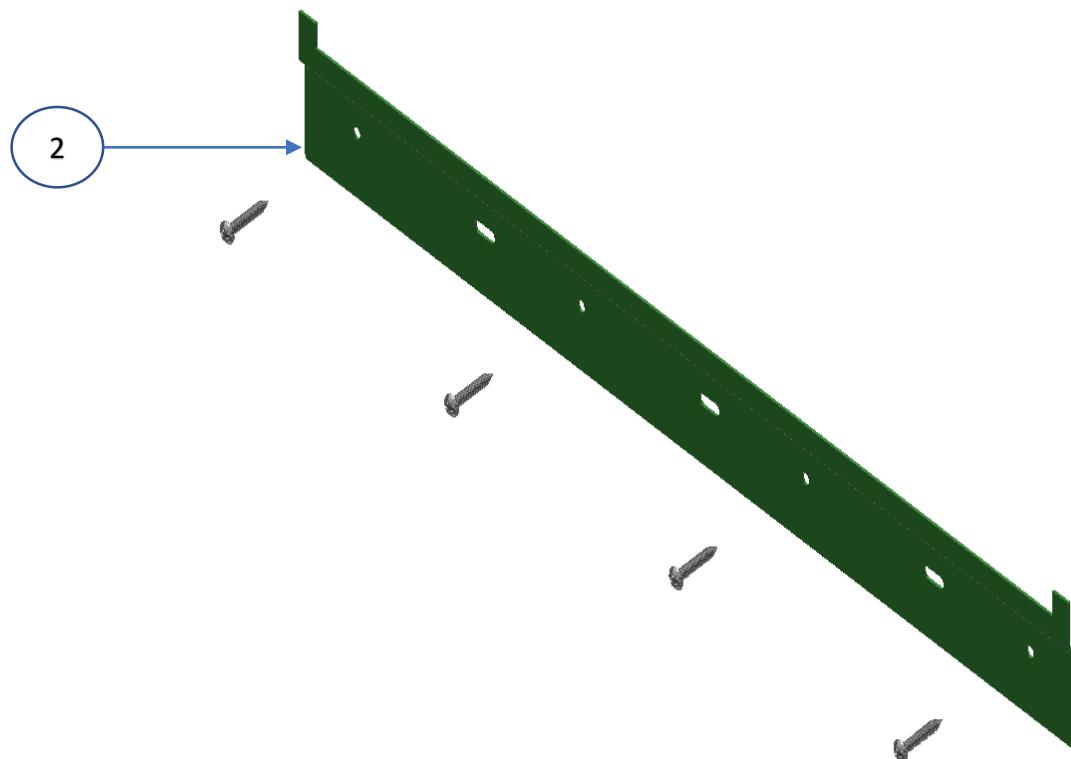


Tools: Screwdriver Phillips

Step 2: Hang the AMD Cabinet on Wall put the Box mounting over the Wall Mounting.

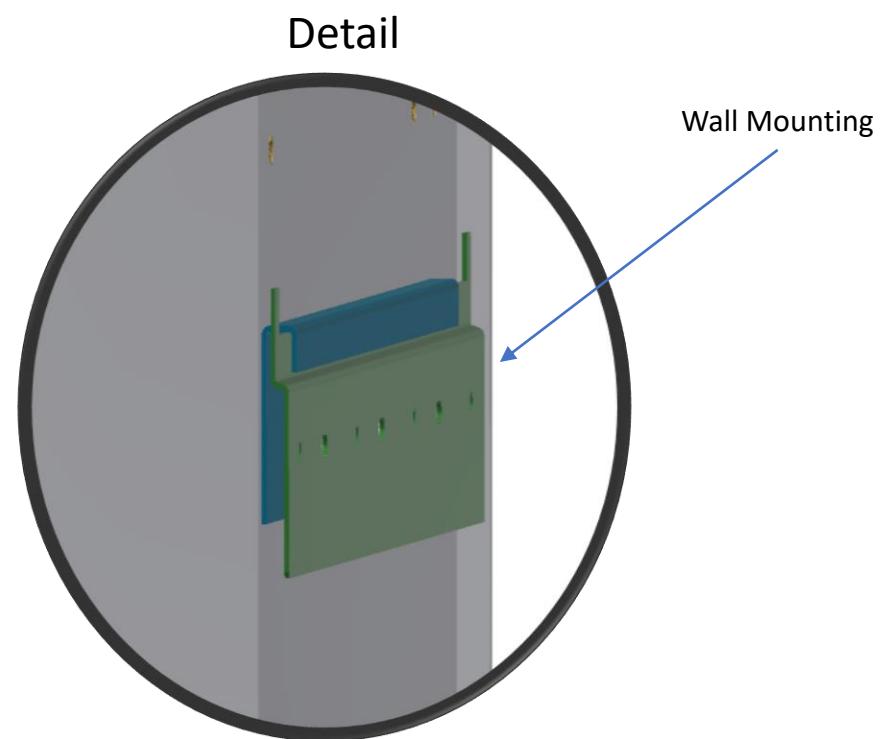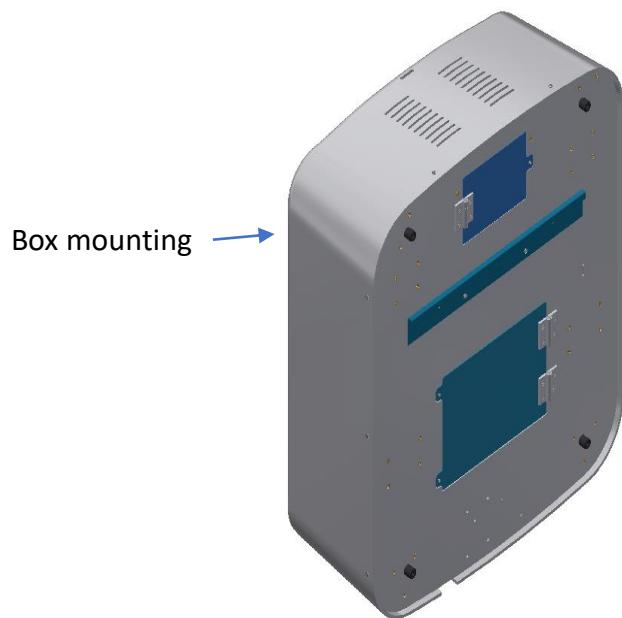


Tools: Screwdriver Hex Key 1/4

Step 3: Put in the Cable power in the power Conector, Insert the Cable Male ends in the Blade Receptacles and Turn on the switch in the AMD Cabinet.

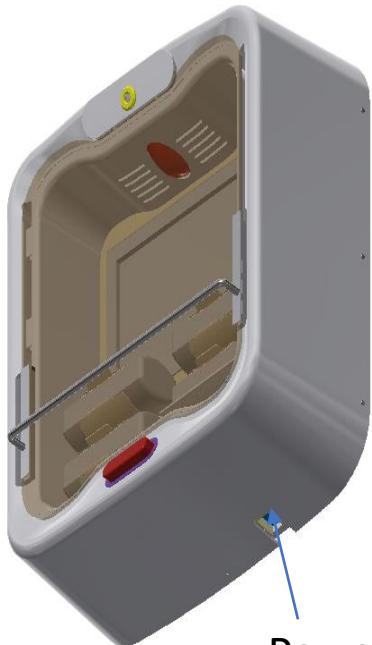

Power Connector

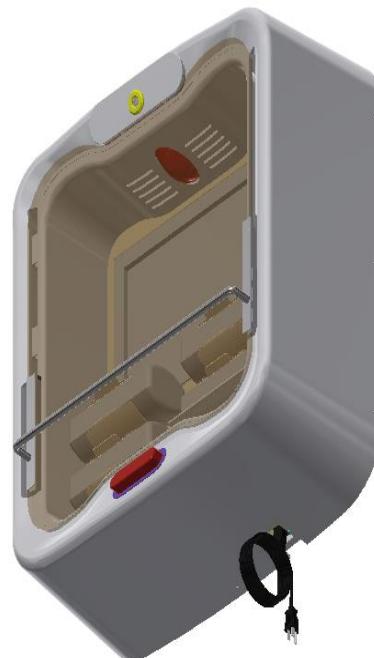

To avoid malfunction or damage to MedicSmart please observe the following:

- Do not expose it to water, moisture or place on a conductive surface whilst in operation.
- Do not expose it to heat from any source; MedicSmart is designed for reliable operation at normal ambient room temperatures.
- Take care whilst handling to avoid mechanical or electrical damage to the product.
- Avoid handling MedicSmart cabinet while it is powered.

All peripherals used with the MedicSmart should comply with relevant standards for the country of use and be marked accordingly to ensure that safety and performance requirements are met. These articles include but are not limited to keyboards, monitors and mice used in conjunction with MedicSmart.

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- *—Reorient or relocate the receiving antenna.*
- *—Increase the separation between the equipment and receiver.*
- *—Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.*
- *—Consult the dealer or an experienced radio/ TV technician for help.*

This equipment complies with the FCC RF radiation exposure limits set forth for an uncontrolled environment. This equipment should be installed and operated with a minimum distance of 20 centimeters between the radiator and your body.