




2Mbps

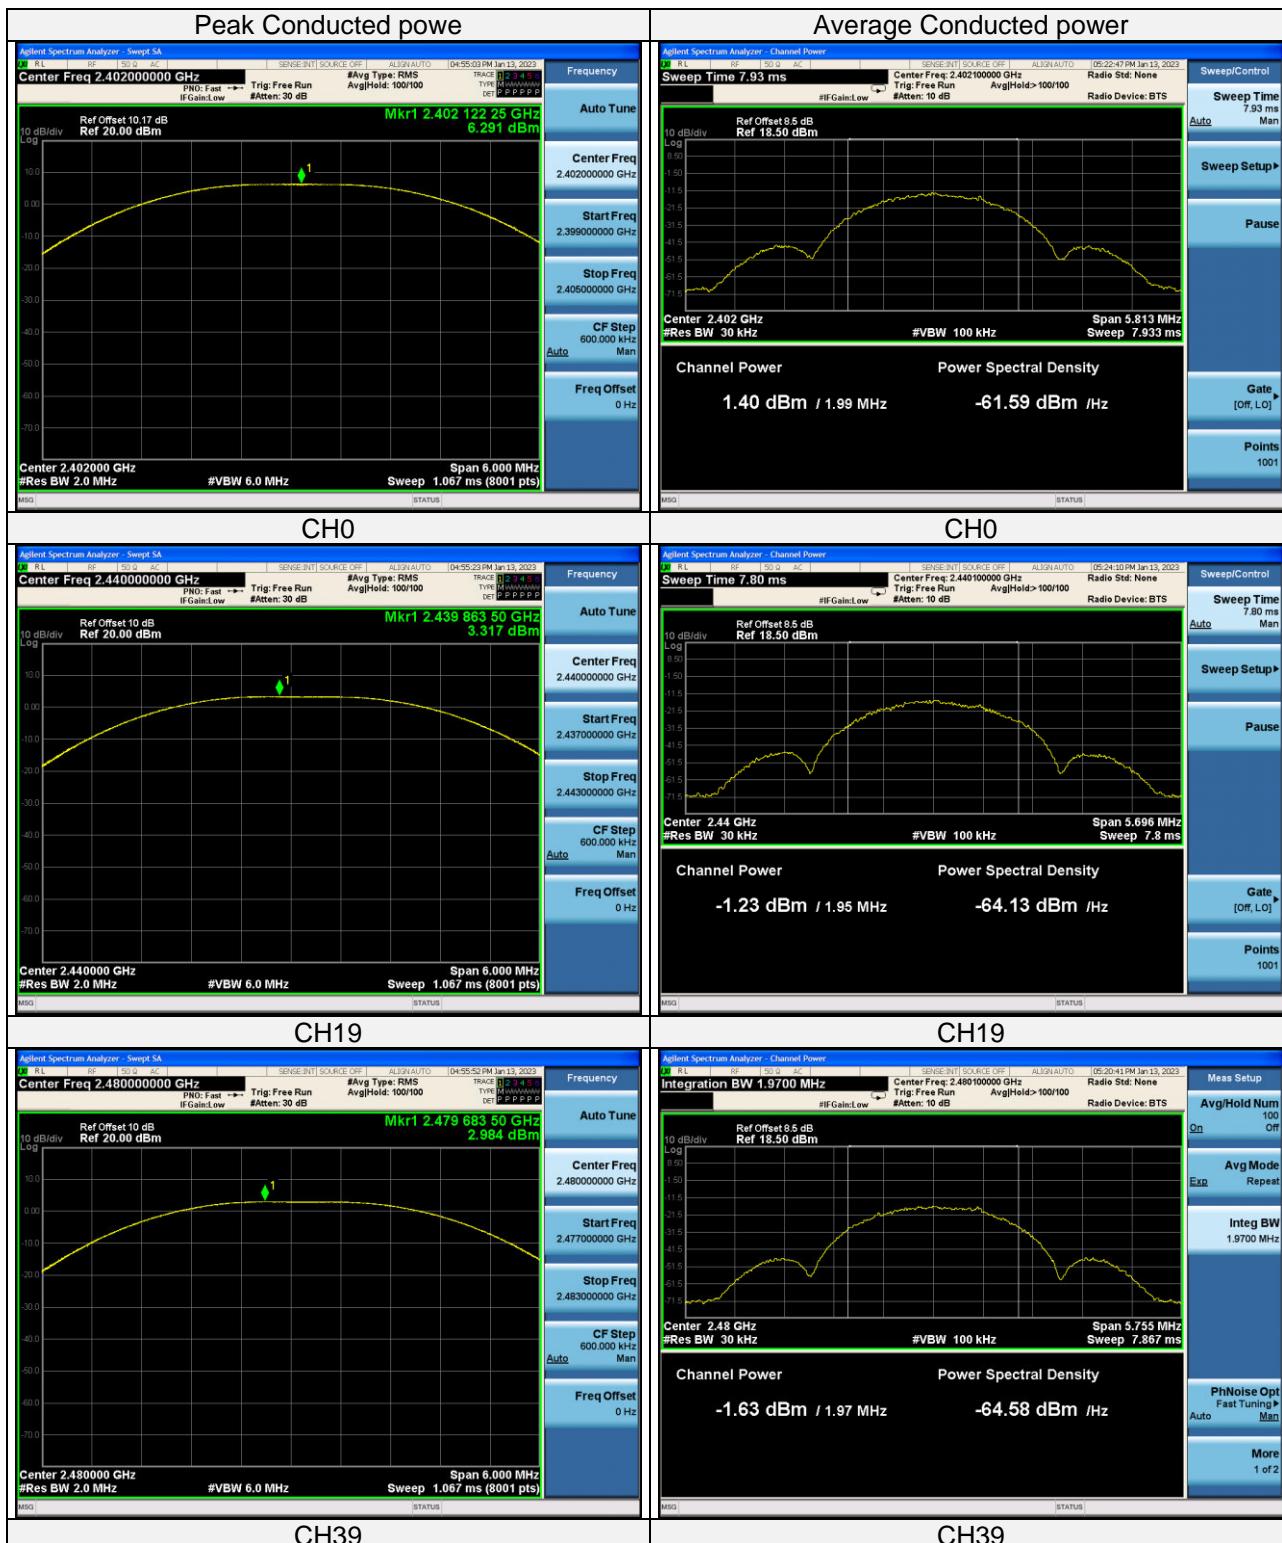


3.5 Power Spectral Density Measurement

3.5.1 Limits of Power Spectral Density Measurement

The Maximum of Power Spectral Density Measurement is 8dBm/3kHz.

3.5.2 Test Setup

- DTS maximum power spectral density level in the fundamental emission Subclause 11.10 of ANSI C63.10 is applicable

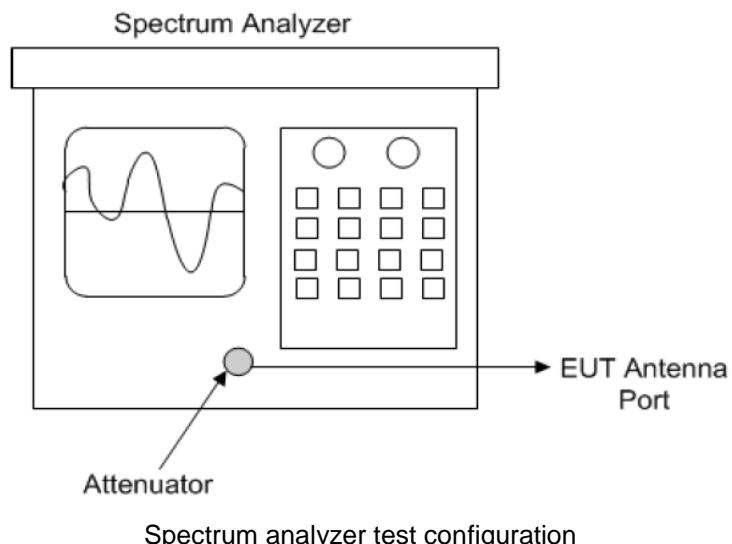

3.5.3 Test Instruments

Refer to section 5 to get information of above instrument.



3.5.4 Test Procedure

- a. **Method AVGPSD-1 or method AVGPSD-1A (alternative)** shall be applied if either of the following conditions can be satisfied:
 - 1) The EUT transmits continuously (or with a D $\geq 98\%$).
 - 2) Sweep triggering can be implemented in such a way that the device transmits at the maximum power control level throughout the duration of each of the instrument sweeps to be averaged. This condition can generally be achieved by triggering the instrument's sweep if the duration of the sweep is equal to or shorter than the duration I of each transmission from the EUT, and if those transmissions exhibit full power throughout these durations.
- b. **Method AVGPSD-2 or method AVGPSD-2A (alternative)** shall be applied if the conditions of the preceding item a) cannot be achieved. and the transmissions exhibit a constant duty cycle during the measurement duration. Duty cycle will be considered to be constant if variations are less than $\pm 2\%$.
- c. **Method AVGPSD-3 or method AVGPSD-3A (alternative)** shall be applied if the conditions of the preceding paragraphs a) and b) cannot be achieved.

Method AVGPSD-3:

Method AVGPSD-3 uses mms detection across ON and OFE times of the EUT with max hold. The following procedure is applicable when the EUT cannot be configured to transmit continuously (i.e. D<98%), when sweep triggering/signal gating cannot be used to measure only when the EUT is transmitting at its maximum power control level. and when the transmission duty cycle is not constant (i.e., duty cycle variations exceed $\pm 2\%$),

SA Setting:

- a. Set the instrument span to a minimum of 1.5 times the OBW.
- b. Set sweep trigger to "free run."
- c. Set the RBW = 3 kHz, VBW = 10 kHz,
- d. Detector = RMS (power averaging).
- e. Sweep time = Auto couple,
- f. Allow max hold to run for at least 60 s or longer as needed to allow the trace to stabilize.
- g. Use the peak marker function to determine the maximum PSD level

- If the measured value exceeds requirement, then reduce RBW (but no less than 3 kHz) and repeat (note that this may require zooming in on the emission of interest and reducing the span to meet the minimum measurement point requirement as the RBW is reduced).

3.5.5 Deviation from Test Standard

No deviation.

3.5.6 EUT Operating Condition


The software provided by client to enable the EUT under transmission condition continuously at lowest, middle and highest channel frequencies individually.



3.5.7 Test Results

BLE-1Mbps		Power Density	
Test Channel	Channel Frequency	Test Result (dBm/3kHz)	Limit (dBm/3kHz)
0	2402MHz	-5.55	<8
19	2440MHz	-7.67	<8
39	2480MHz	-7.40	<8

BLE-2Mbps		Power Density	
Test Channel	Channel Frequency	Test Result (dBm/3kHz)	Limit (dBm/3kHz)
0	2402MHz	-8.42	<8
19	2440MHz	-10.51	<8
39	2480MHz	-10.53	<8

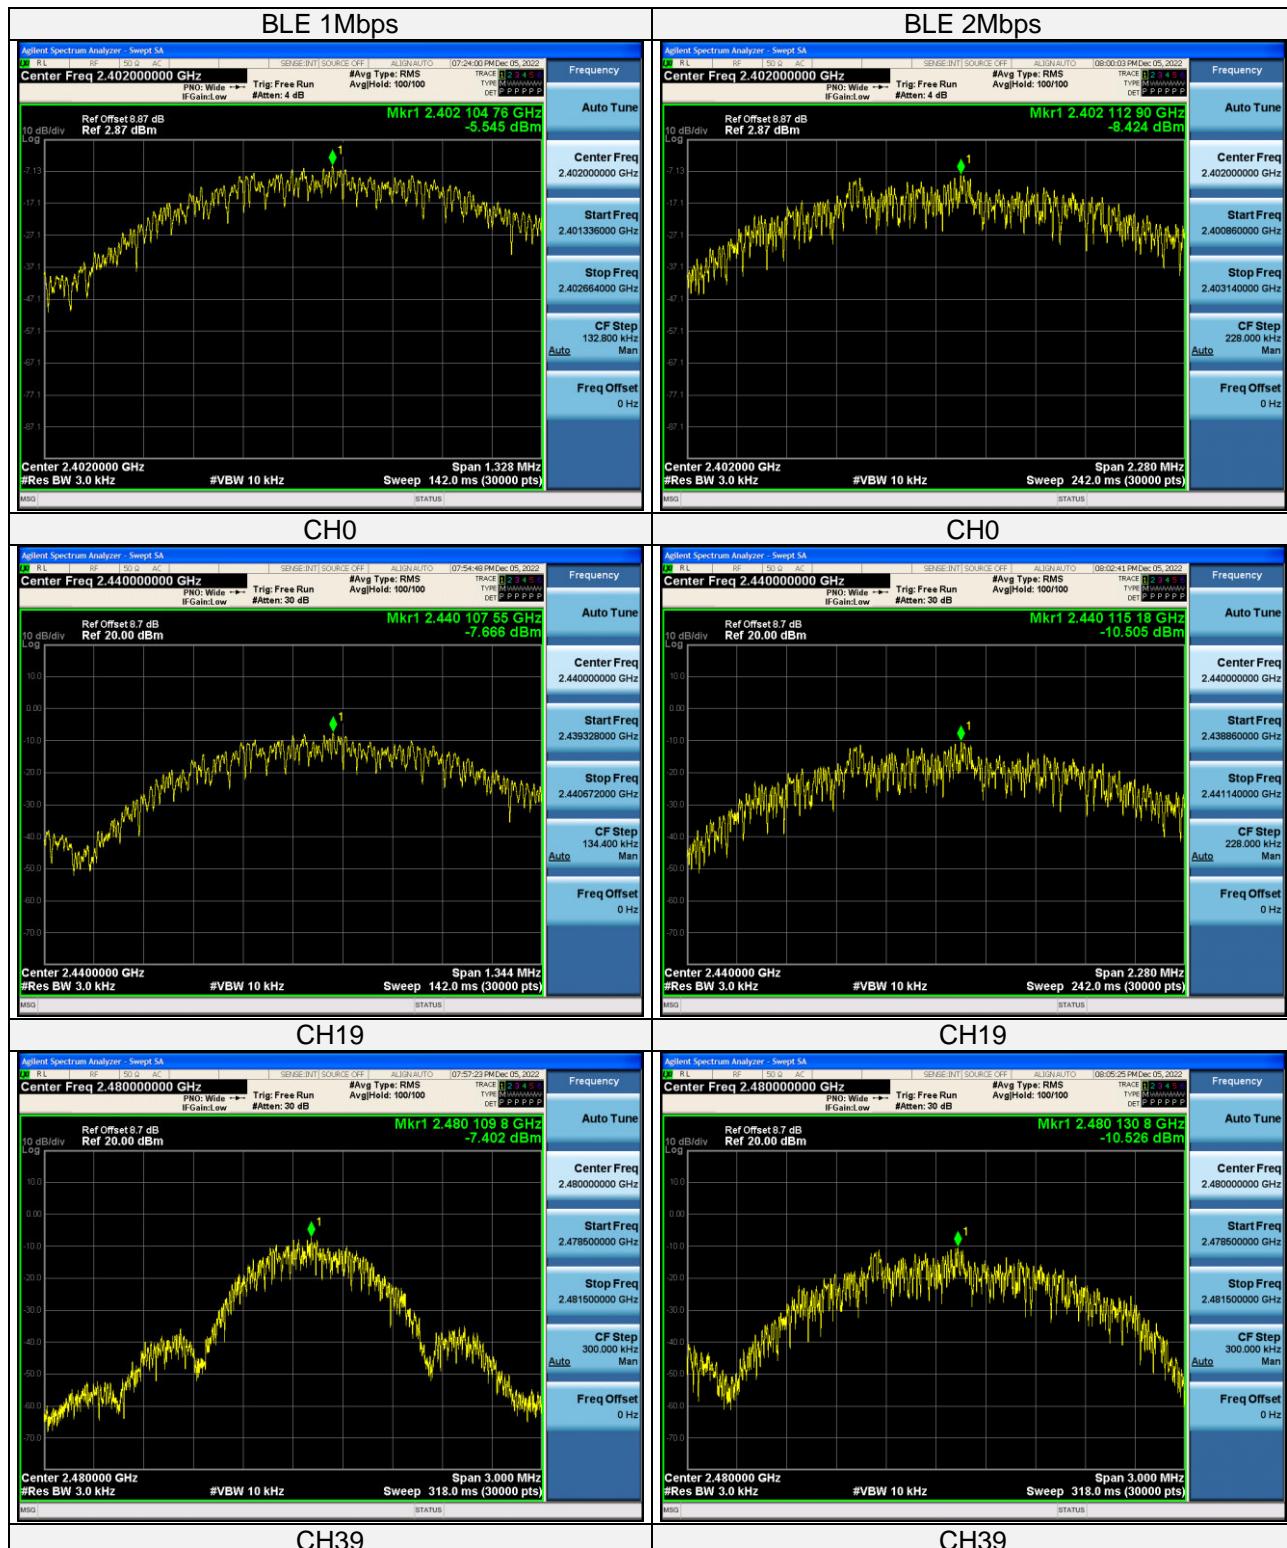


3.6 Conducted Out of Band Emission Measurement

3.6.1 Limits of Conducted Out of Band Emission Measurement

- a. **If the maximum peak conducted output power procedure was used to determine compliance as described in 11.9.1**, then the peak output power measured in any 100 kHz bandwidth outside of the authorized frequency band shall be attenuated by at least 20 dB relative to the maximum in-band peak PSD level in 100 kHz (i.e., 20 dBc).
- b. **If maximum conducted (average) output power was used to determine compliance as described in 11.9.2**, then the peak power in any 100 kHz bandwidth outside of the authorized frequency band shall be attenuated by at least 30 dB relative to the maximum in-band peak PSD level in 100 kHz (i.e., 30 dBc).

3.6.2 Test Setup

- DTS emissions in non-restricted frequency bands Subclause 11.11 of ANSI C63.10 is applicable.
- DTS emissions in restricted frequency bands Subclause 11.12 of ANSI C63.10 is applicable

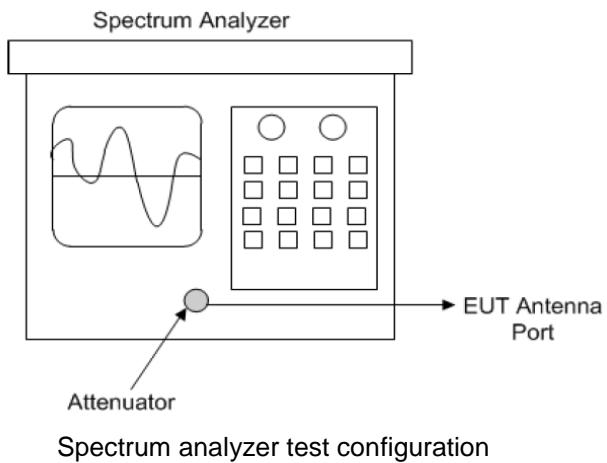

3.6.3 Test Instruments

Refer to section 5 to get information of above instrument.



3.6.4 Test Procedure

- a. Establish a reference level by using the following procedure:
 - 1) Set instrument center frequency to DTS channel center frequency.
 - 2) Set the span to 21.5 times the DTS bandwidth)
 - 3) Set the RBW= 100 kHz)
 - 4) Set the VBW $\geq 3 \times$ RBW
 - 5) Detector = peak
 - 6) Sweep time = auto coupling
 - 7) Trace mode =max hold
 - 8) Allow trace to fully stabilize
 - 9) Use the peak marker function to determine the maximum PSD level.

Note that the channel found to contain the maximum PSD level can be used to establish the reference level.

- b. Establish an emission level by using the following procedure:

- 1) Set the center frequency and span to encompass frequency range to be measured.
 - 2) Set the RBW = 100 kHz
 - 3) Set the VBW ≥ 300 kHz.
 - 4) Detector = peak.
 - 5) Sweep time = auto couple.
 - 6) Trace mode = max hold.
 - 7) Allow trace to fully stabilize.
 - 8) Use the peak marker function to determine the maximum power level in any 100 kHz band segment within the fundamental EBW.

3.6.5 Deviation from Test Standard


No deviation.


3.6.6 EUT Operating Condition


The software provided by client to enable the EUT under transmission condition continuously at lowest, middle and highest channel frequencies individually.




3.6.7 Test results

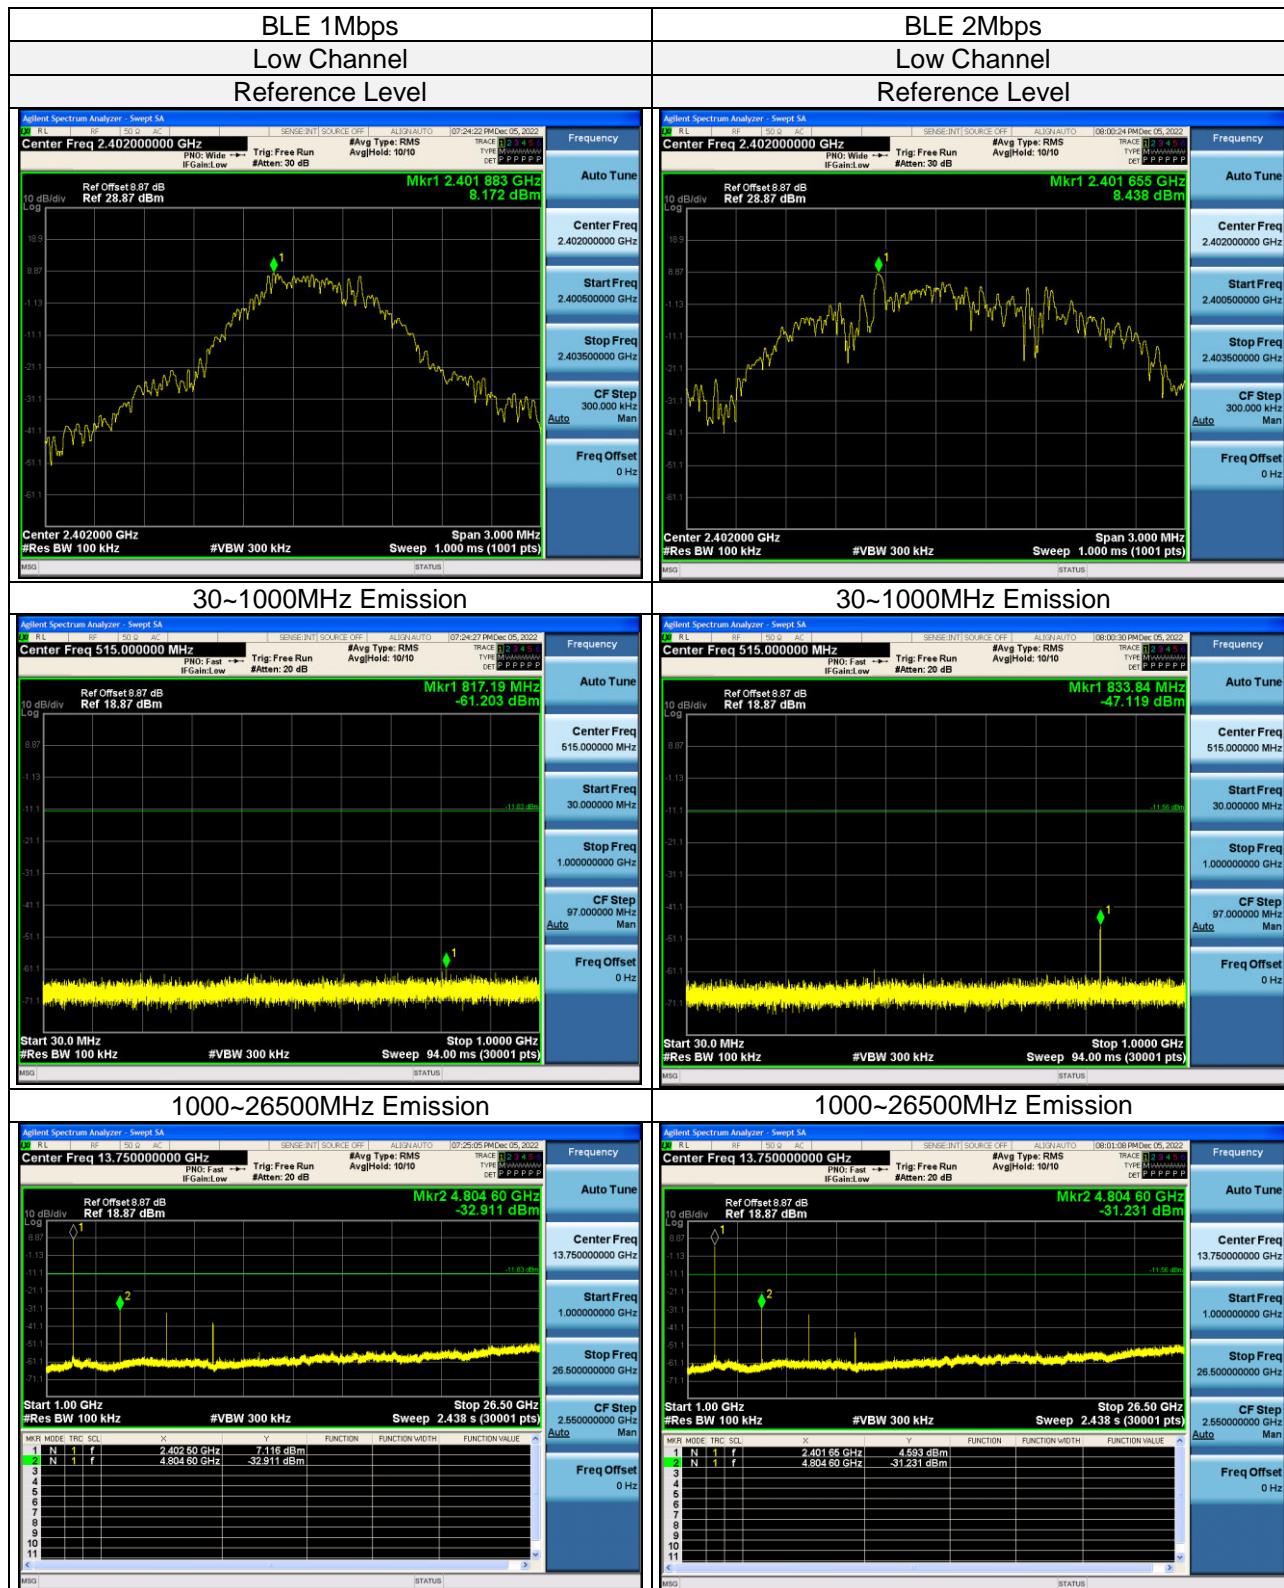

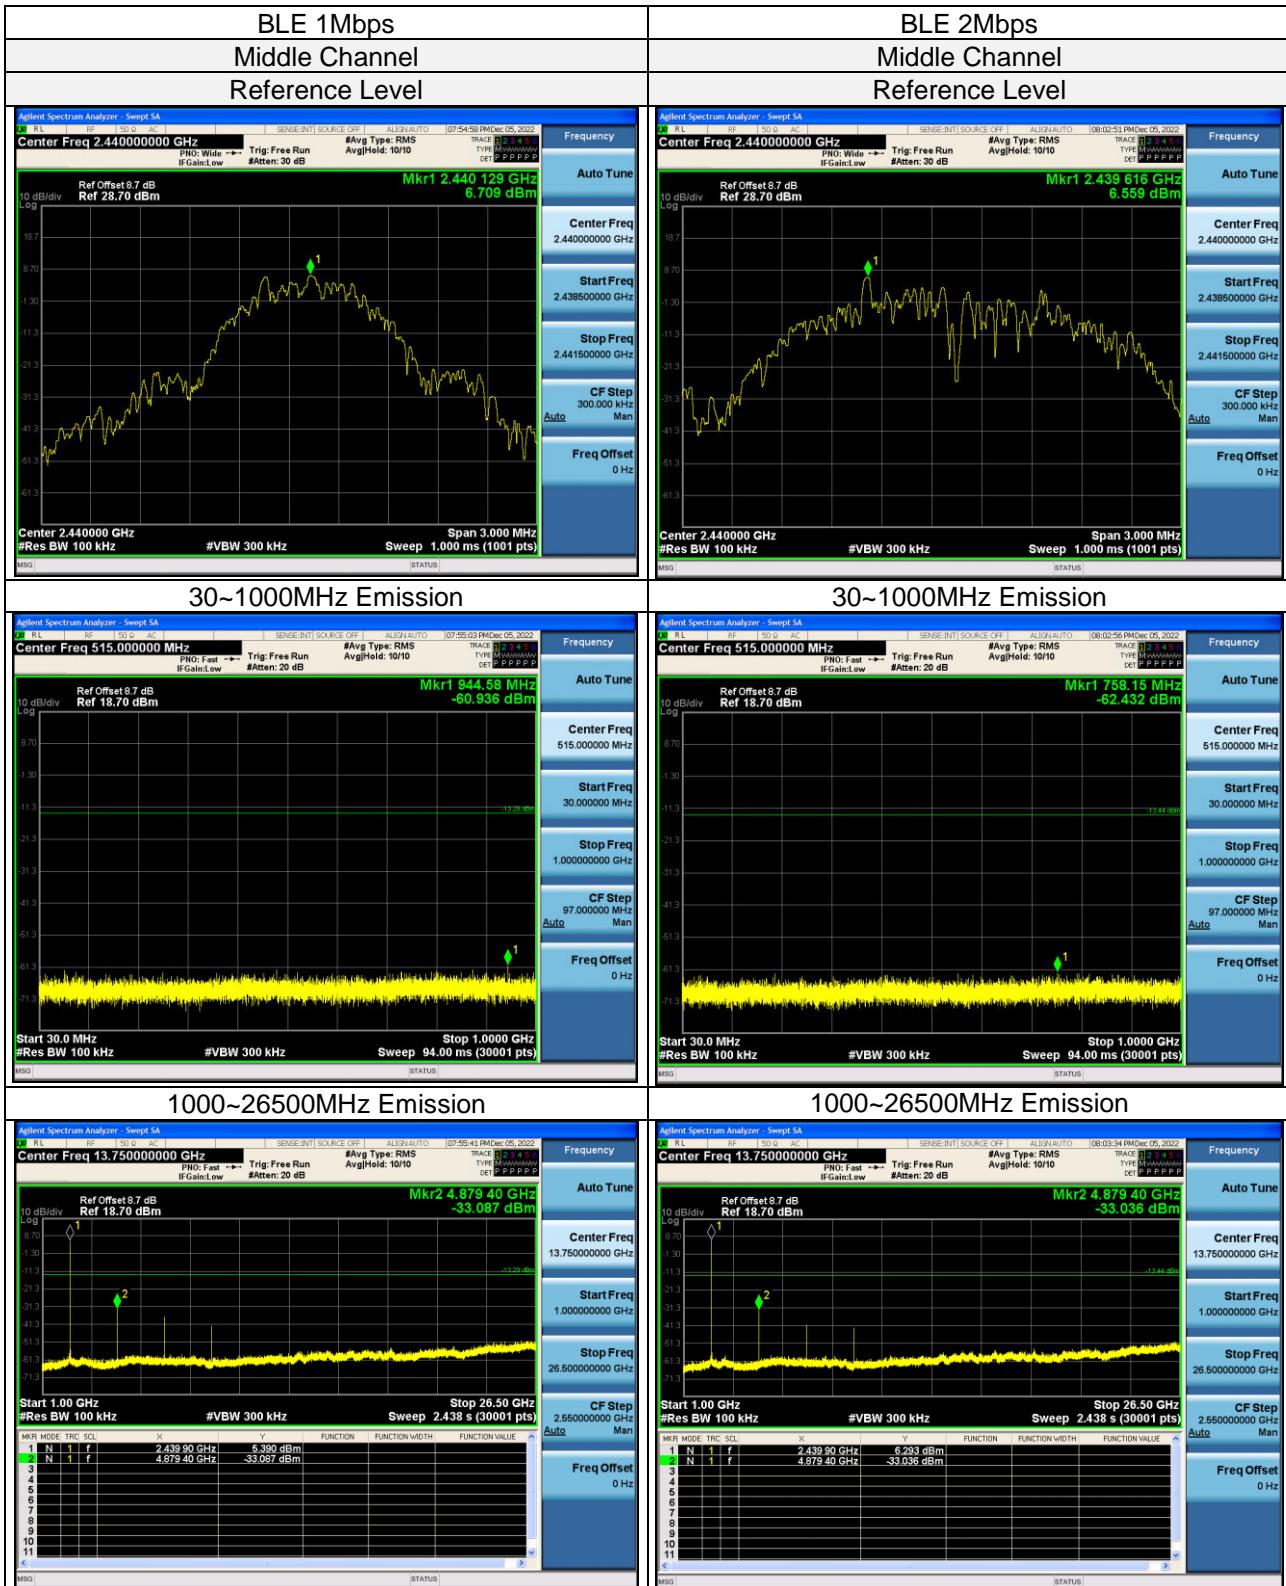

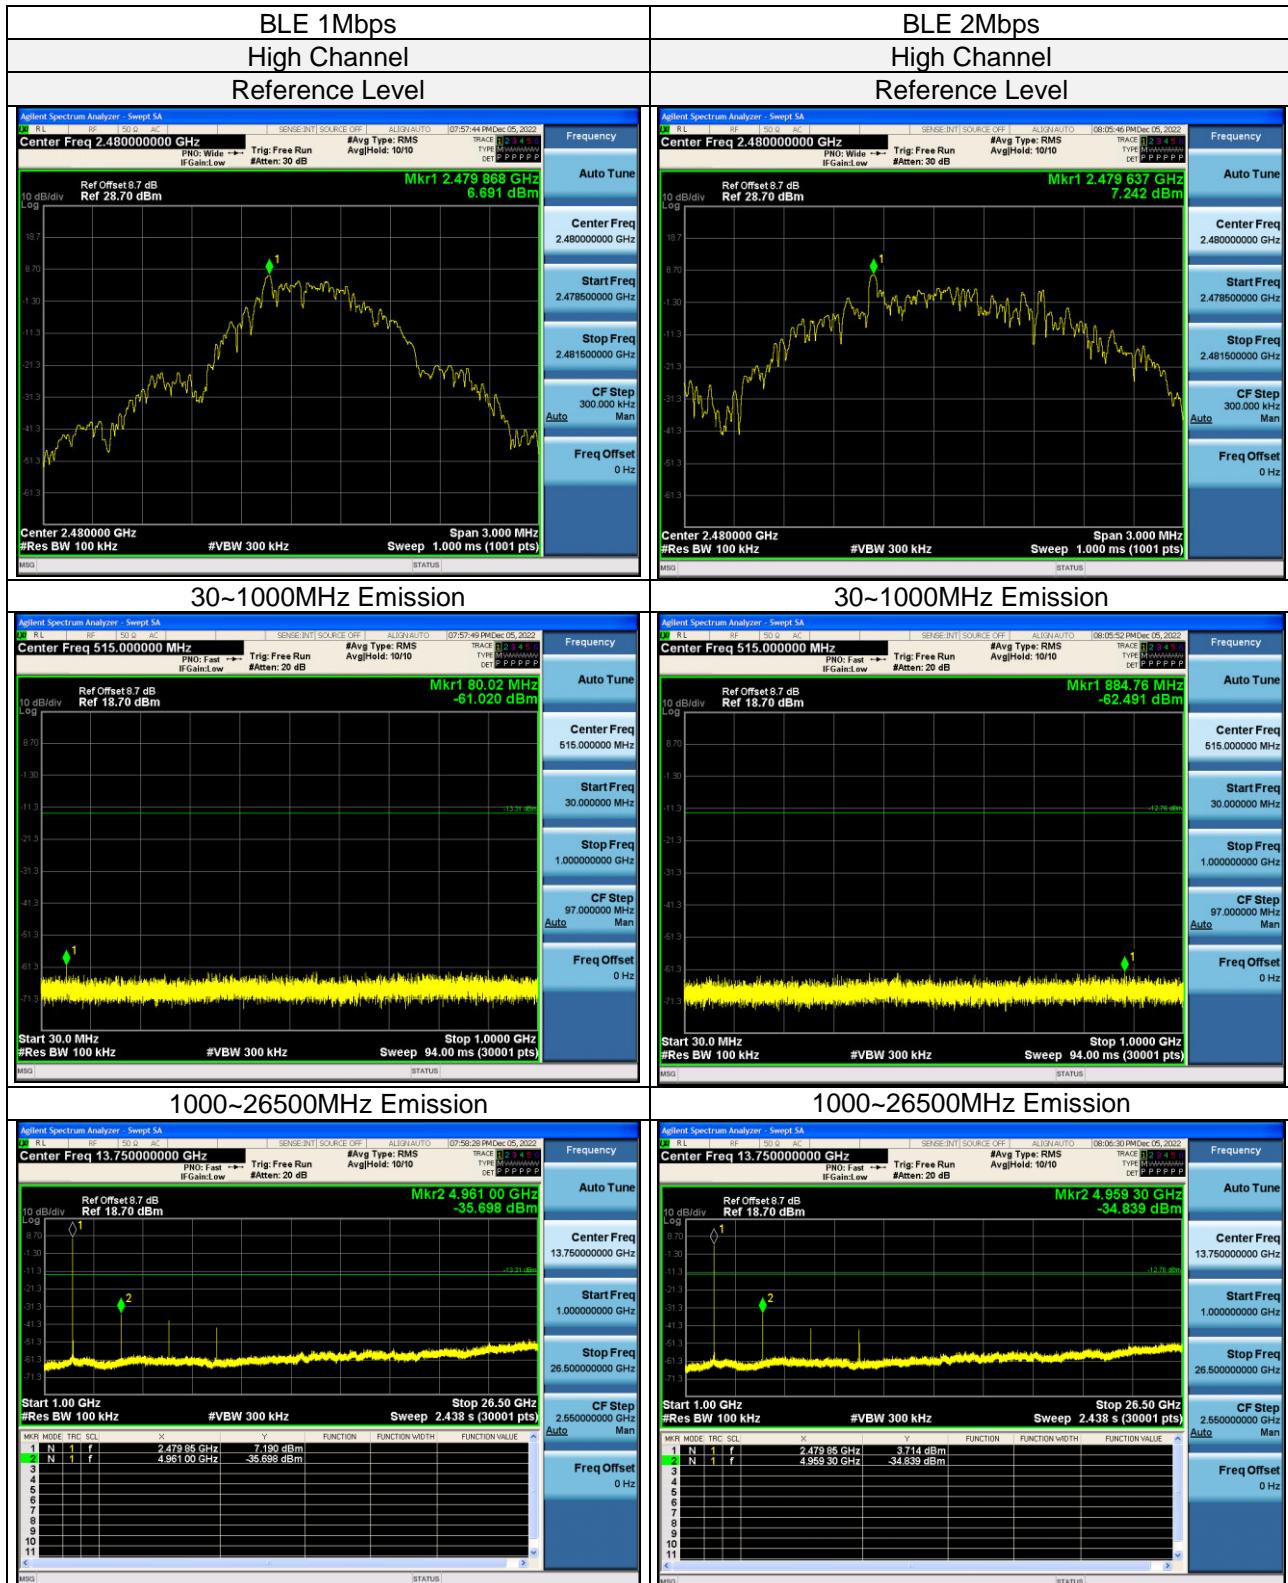

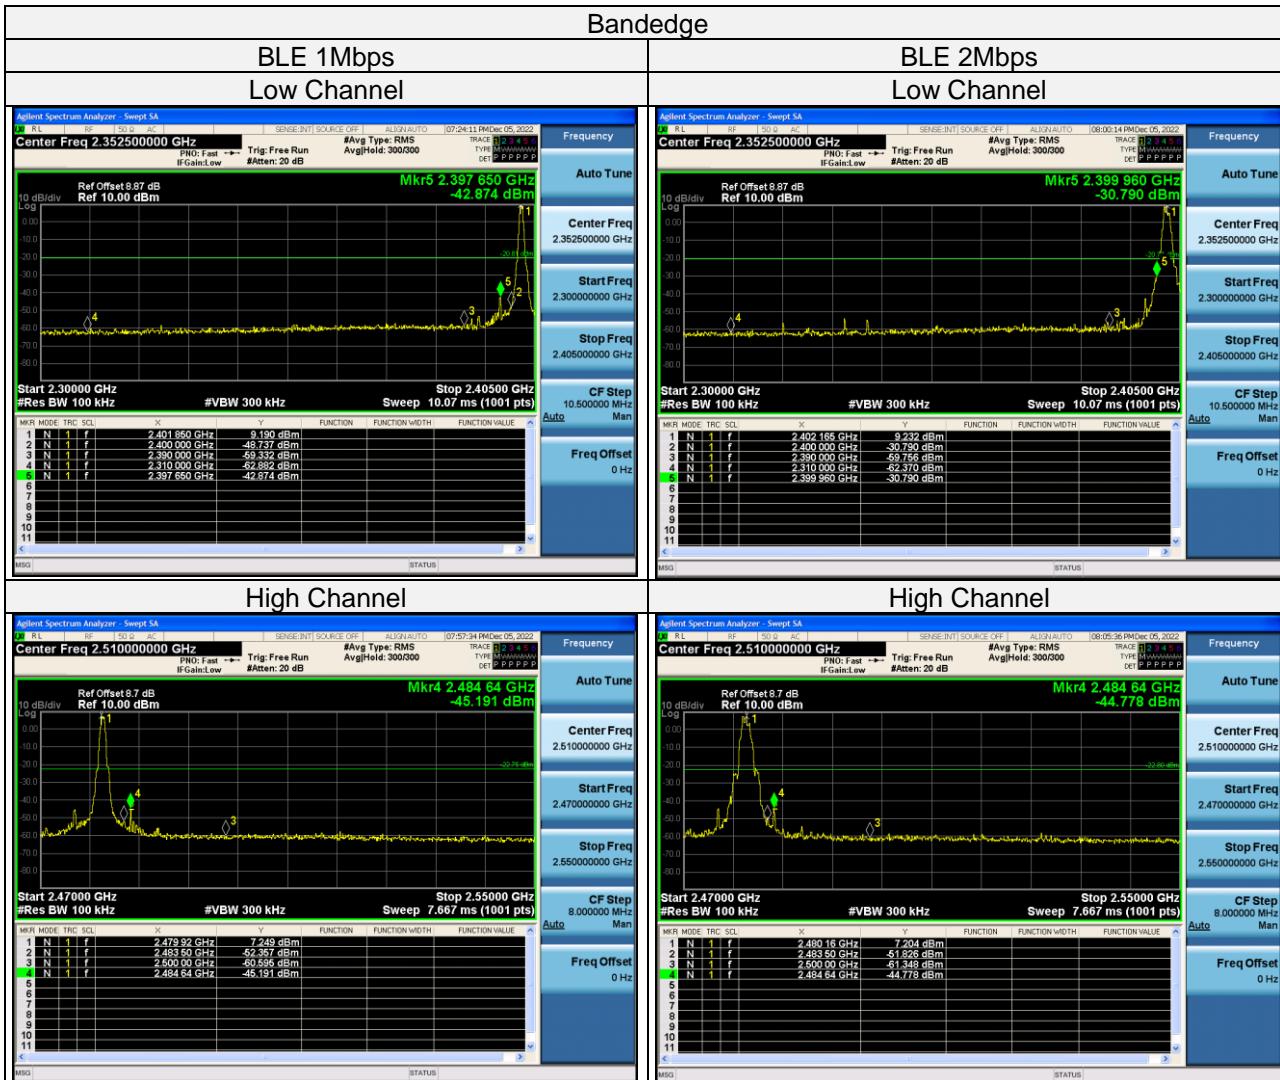



4. Pictures of Test Arrangements

Please refer to the attached file (Test Setup Photo).



5. Test Instruments

Description & Manufacturer	Model No.	Serial No.	Due Date of Calibration
Spectrum Keysight	N9020A	MY51240612	2023-08-25
Spectrum Analyzer Rohde&Schwarz	FSV-40N	101783	2023-01-12
Power Meter 10Hz~18GHz Tonscend	JS0806-2	188060126	2023-08-25
Signal generator Keysight	E4421B	GB40051020	2023-08-25
Signal generator Keysight	N5182A	MY47420944	2023-08-25
Test Software Tonscend	JS0806-2	NA	NA
Hygrothermograph Yuhuaze	HTC-1	NA	2023-08-25

Note:

1. The calibration interval of the above test instruments is 12 months and the calibrations are traceable to CEPREI/CHINA.
2. The test was performed in Chamber 1.



Appendix – Information on The Testing Laboratories

We, [Hwa-Hsing \(Dongguan\) Co., Ltd.](#), A global provider of TESTING and CERTIFICATION services for consumer products, electronic products and wireless information technology products. Adhering to the core values “HONEST and TRUSTWORTHY, OBJECTIVE and IMPARTIALITY, RIGOROUS and AFFICIENT”, commitment to provide professional, perfect and efficient comprehensive ONE-STOP solution of TESTING and CERTIFICATION services for Manufacturers, Buyers, Traders, Brands, Retailers. Assist client to better manage risk, protect their brands, reduce costs and cut time to over 150 markets in global. Our laboratories are FCC recognized accredited test firms and accredited and approved according to ISO/IEC 17025.

If you have any comments, please feel free to contact us at the following:

Lab Address: [No.101, Bld N1, Yuyuan 2Rd, Yuyuan Industrial Park, HuangJiang Town, Dongguan, China](#)

Contact Tel: [0769-83078199](#)

Email: CustomerService.dg@hwa-hsing.com

Web Site: www.hwa-hsing.com

--- END ---