



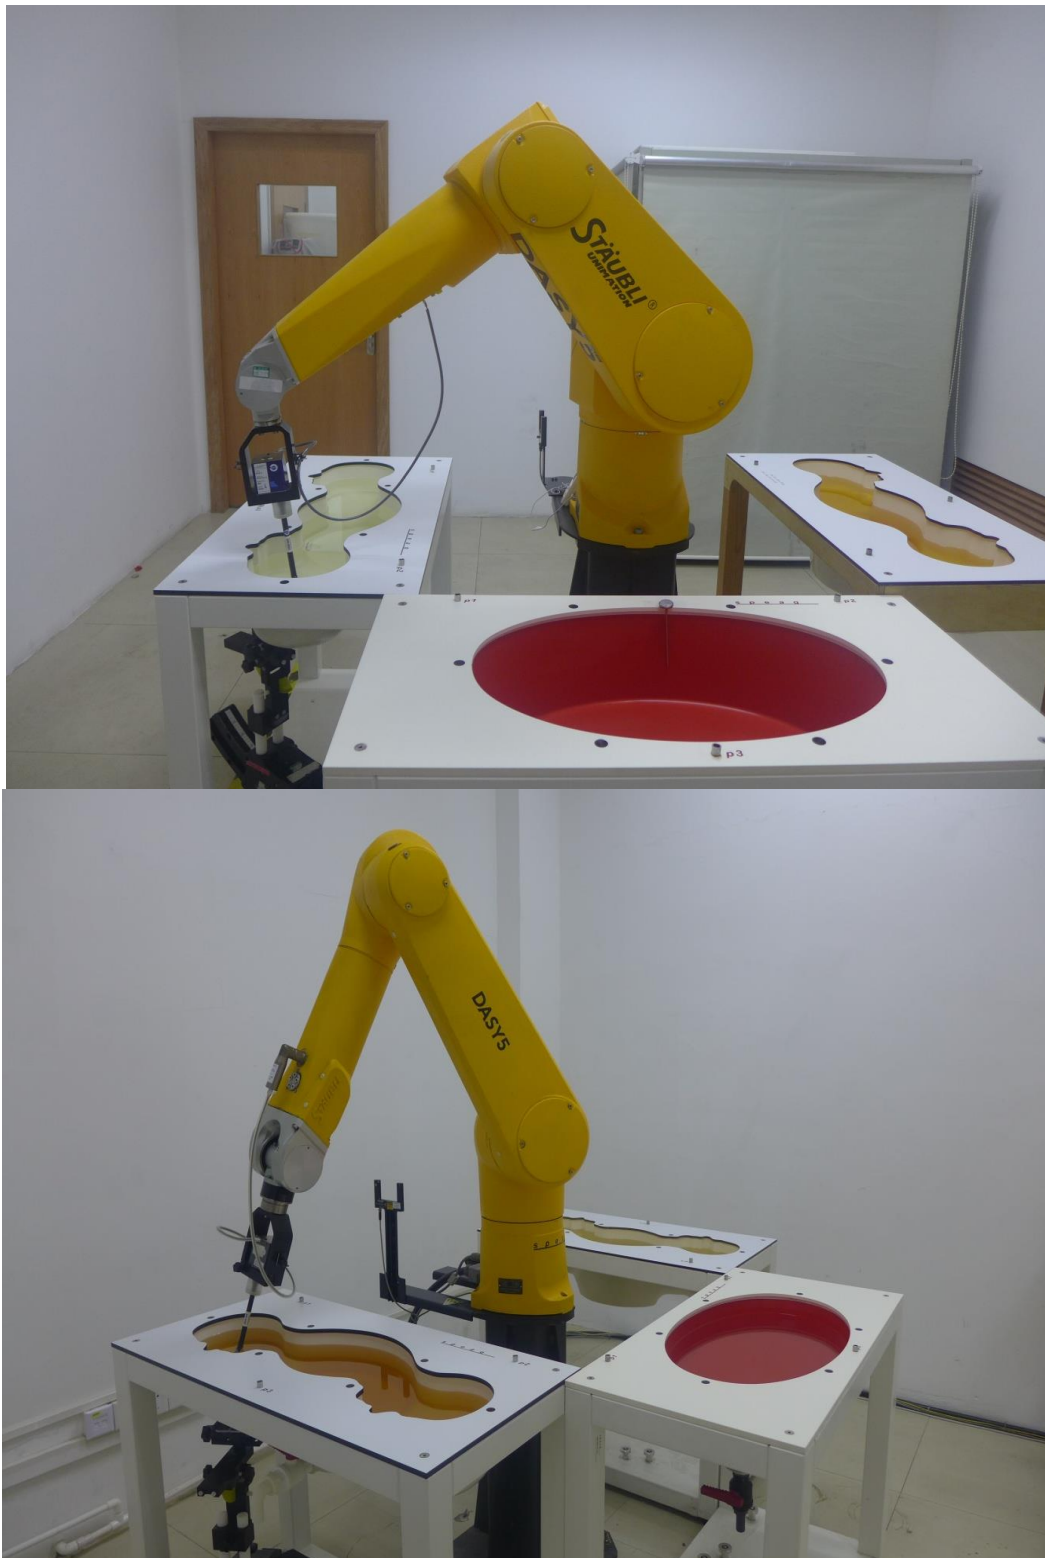
Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details
5. Serial Number of EUT



1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

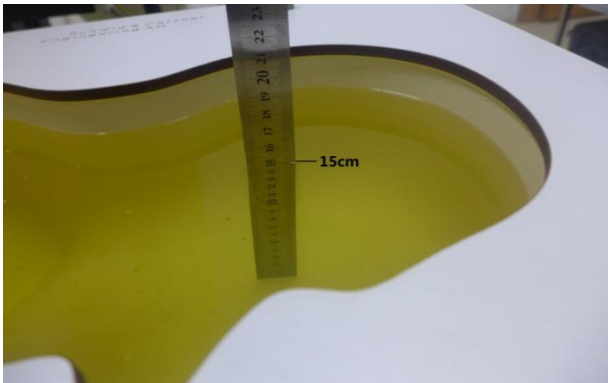
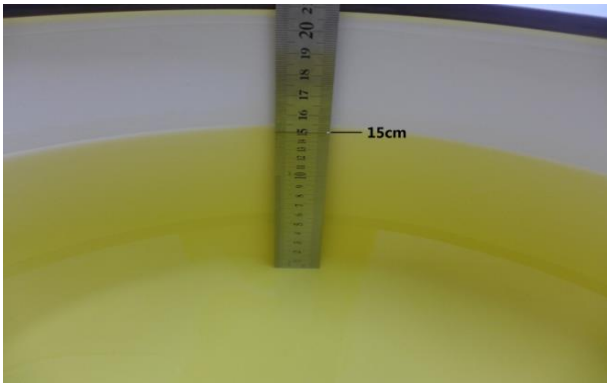
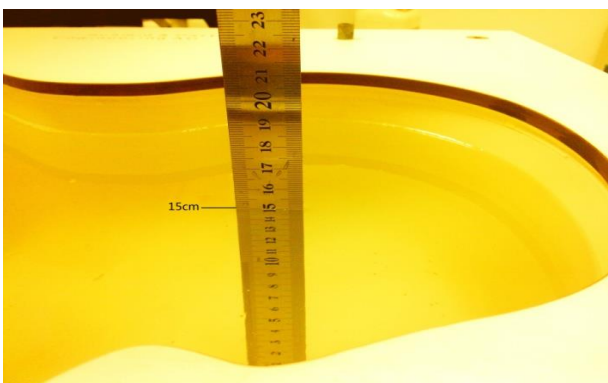
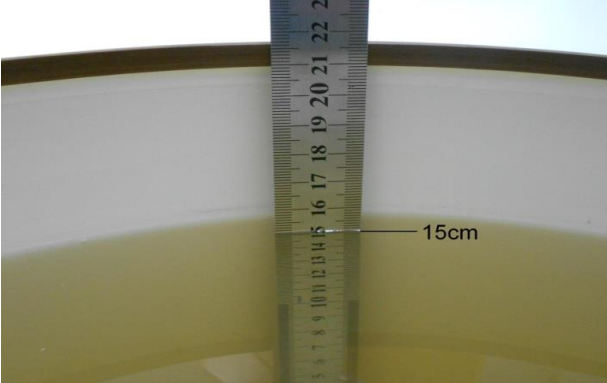
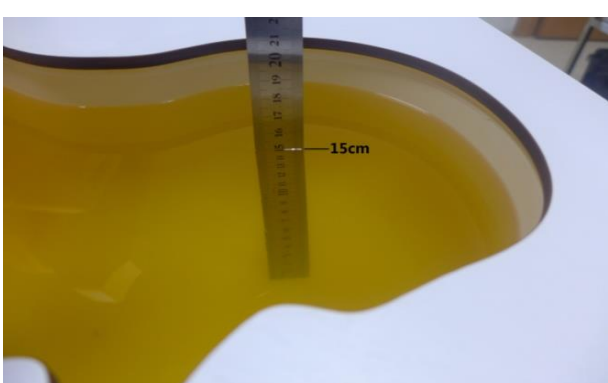
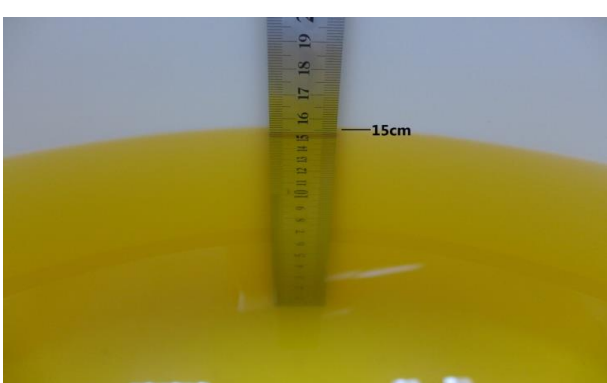
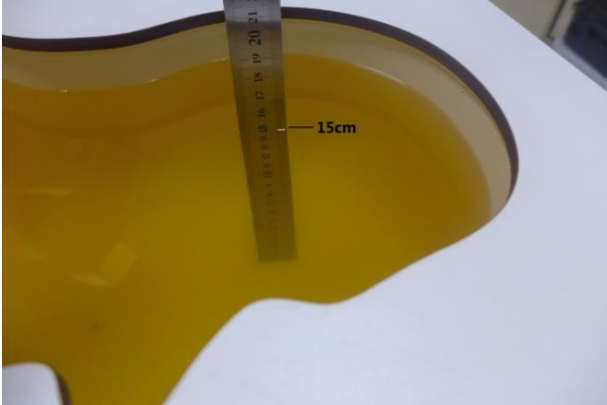
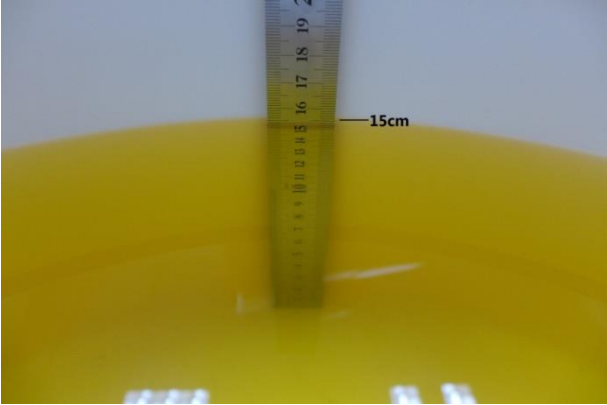
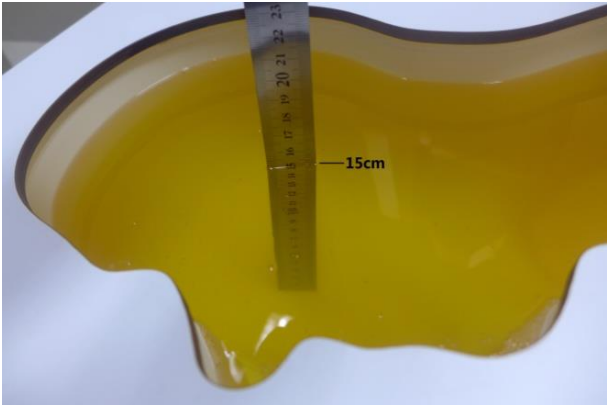
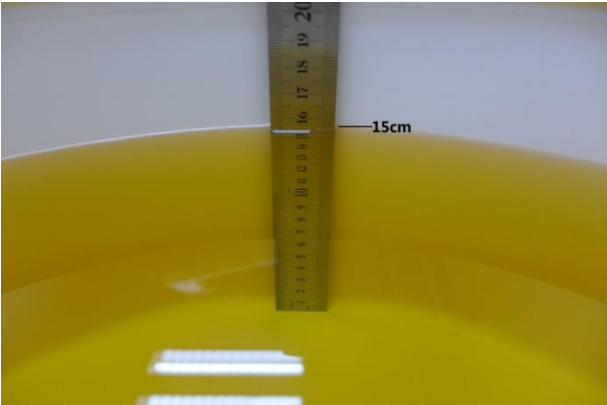
Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Body 750
	
Photo 3: Tissue Simulant Liquid for Head 835	Photo 4: Tissue Simulant Liquid for Body 835
	
Photo 5: Tissue Simulant Liquid for Head 1750	Photo 6: Tissue Simulant Liquid for Body 1750
	



Photo 7: Tissue Simulant Liquid for Head 1900 	Photo 8: Tissue Simulant Liquid for Body 1900 
Photo 9: Tissue Simulant Liquid for Head 2450 	Photo 10: Tissue Simulant Liquid for Body 2450 

3. Photographs of EUT test position


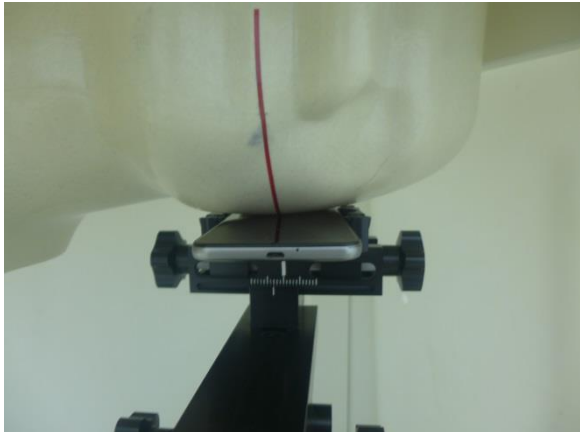
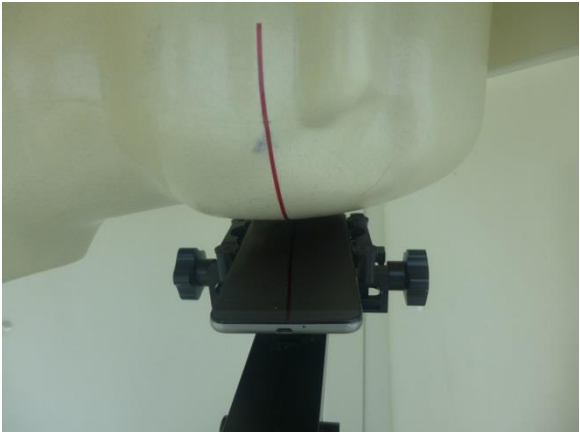
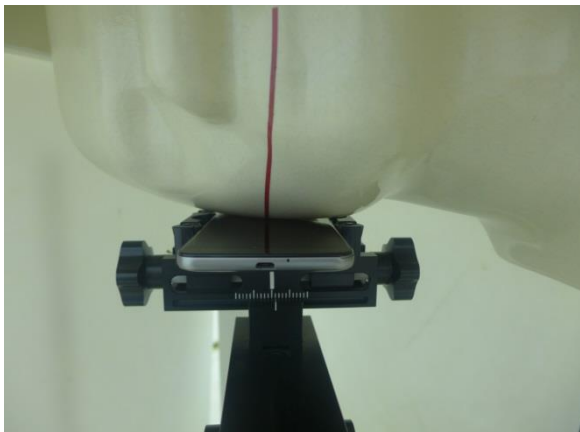
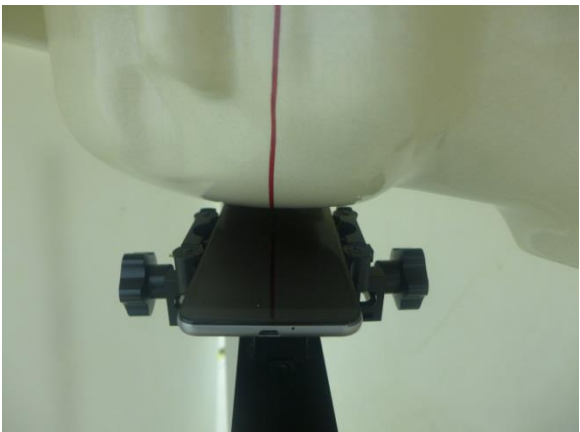
Photo 11: Left touch cheek	Photo 12: Left tilted
	
Photo 13: Right touch cheek	Photo 14: Right tilted
	
Photo 15: Front side 15mm	Photo 16: Back side 15mm
	



Photo 17: Front side 10mm	Photo 18: Back side 10mm
	
Photo 19: Left side 10mm	Photo 20: Right side 10mm
	
Photo 21: Top side 10mm	Photo 22: Bottom side 10mm
	

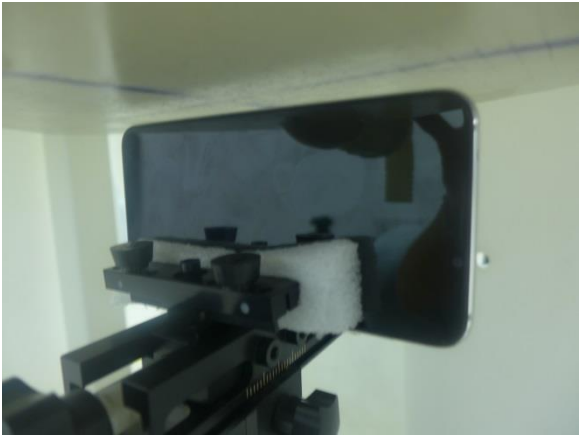

4. EUT Constructional Details

Photo 23: Front View	Photo 24: Back View
	