

LABELING

Original Freigabeformular in TR archiviert.
Original form stored in the technical writing department.

Label position: inside of the device

FA. Nr. ##### - ##

SN

YYMMCE####

Removing this label causes loss of warranty.
10000020594 03

MAX. IRRIGATION RATE2.0 l/min

MAX. PUMPING PRESSURE150 mmHg

MAINS VOLTAGE RANGEAC 100-240 V~

SUPPLY FREQUENCY50/60 Hz

POWER CONSUMPTIONAC 100 V ~ 0.85 A
AC 240 V ~ 0.50 A

WEIGHT6.3 kg

WARNING! Risk of fire. Replace fuse as marked.

RX
ONLY

IP 21

YYYY-MM-DD

99

2019

GYN-Pump

W.O.M. WORLD OF MEDICINE GmbH
Salzufer 8, 10587 Berlin, Germany
Phone: +49 30 39981-550

CE 0197

TYPE

PH304

SN / REF

YYMMCE#### / REF


Contains FCC ID: 2A55K-TSHW42
Contains IC ID:25004-TSHW42A
HVIN: 1430

GS1 EAN
DataMatrix
DB:
01/11/21


Issuing Agency:
GSI

(01)#####(11)YYMMDD(21)YYMMCE####

Rear of device

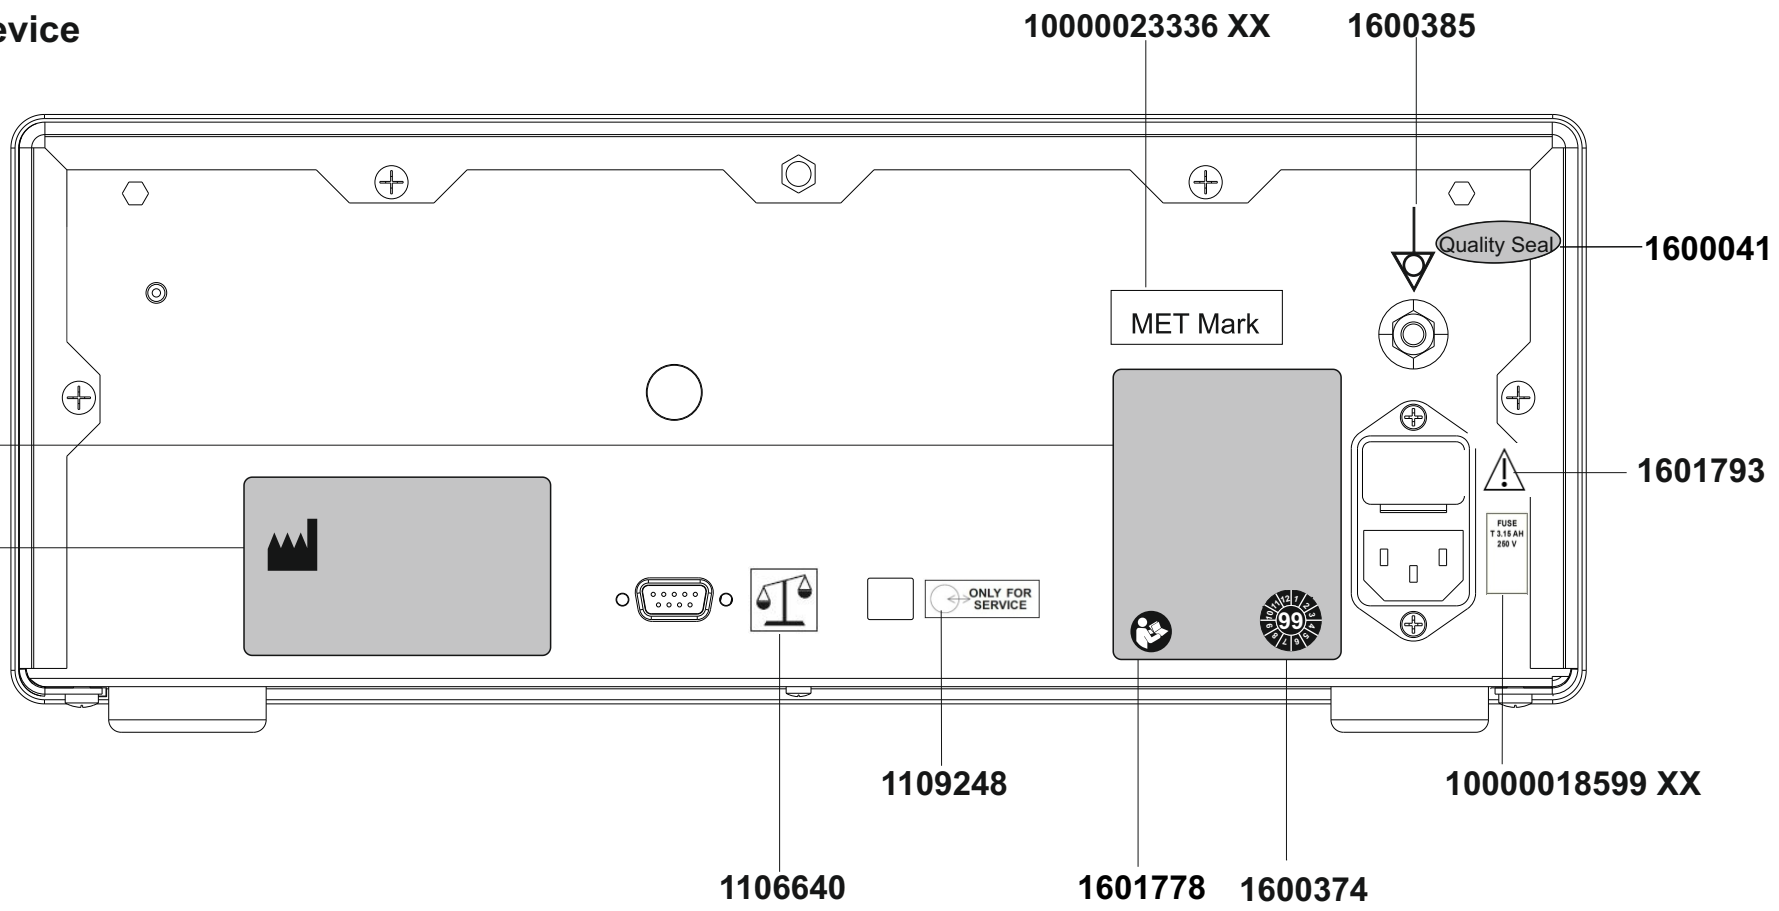

Box

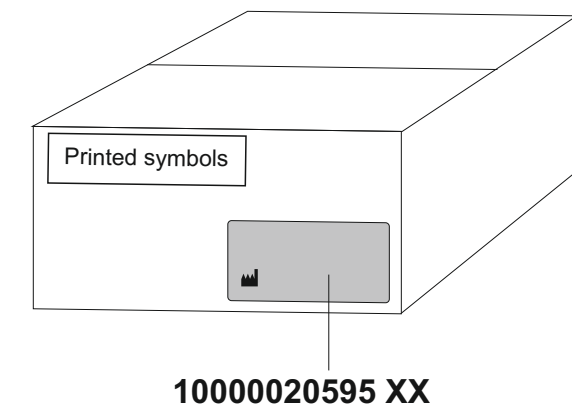

Revision history		
Legend: Change request(s) Internal updates		
Rev. WOM	ECR	Change
01	2017 613	MAX. PUMPING PRESSURE: 150 mmHg; added: symbol: RX only, WEIGHT removed: FUSE (data label)
02	2018 245	added: MET label, 1601778 above scale connection
03	2019 109	added: FCC ID, IC ID number, HVIN; symbols: Non-ionizing radiation; changed: position of quality seal label 1600041; moved symbols; removed: Technical data in German, 1x label 1601778 „Follow instructions for use“

Product Management / Customer	Project Management (R&D)	Regulatory Affairs	WORLD OF MEDICINE / Approval		
Overview device labels PH304 WOM			W.O.M. Item number	File FMT	File CDR
			10000020594 03	10000020594 03.fmt	10000020594 03.cdr
				Name	Date
				Berndt	26.03.2019