



RADIO REPORT FCC 47 CFR Part 15C ISED Canada RSS-210 ISED Canada RSS-Gen Operation within the 13.110 – 14.010 MHz band	
Report Reference No	G0M-1903-8084-TFC225RI-V02
Testing Laboratory	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	    DAkks - Registration number : D-PL-12092-01-03 (ISED) ISED Testing Laboratory site: 3470A-2 DAkks - Registration number : D-PL-12092-01-04 (FCC) FCC Filed Test Laboratory, Reg.-No.: 96970
Applicant	W.O.M. WORLD OF MEDICINE GmbH
Address	Salzufer 8 10587 Berlin GERMANY
Test Specification	According to FCC/ISED rules
Standard	FCC 47 CFR Part 15C ISED RSS-210, Issue 9, 2016-08 ISED RSS-Gen, Issue 5, Amendment 1, 2019-03
Non-Standard Test Method	None
Equipment under Test (EUT):	
Product Description	Irrigation Pump for HYS/LAP with Fluid Monitoring Module
Model(s)	PH304
Additional Model(s)	None
Brand Name(s)	GYN-Pump
Hardware Version(s)	03/2019
Software Version(s)	0.0.6.5
Contains FCC-ID	2AS5K-TSHW42
Contains IC	25004-TSHW42A
Test Result	PASSED

Possible test case verdicts:		
required by standard but not tested	N/T	
not required by standard	N/R	
not applicable to EUT	N/A	
test object does meet the requirement	P(PASS)	
test object does not meet the requirement	F(FAIL)	
Testing:		
Test Lab Temperature	20 - 23 °C	
Test Lab Humidity	32 – 38 %	
Date of receipt of test item	2019-04-01	
Report:		
Compiled by	Wilfried Treffke	
Tested by (+ signature) (Responsible for Test)	Wilfried Treffke	
Approved by (+ signature) (Head of Lab)	Christian Weber	
Date of Issue	2019-08-22	
Total number of pages	33	
General Remarks:		
The test results presented in this report relate only to the object tested. The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report. This report shall not be reproduced, except in full, without the written approval of the Issuing testing laboratory.		
Additional Comments:		

VERSION HISTORY

Version History			
Version	Issue Date	Remarks	Revised By
01	2019-05-09	Initial Release	
02	2019-08-22	Replaced document G0M-1903-8084-TFC225RI-V01 Replaced by G0M-1903-8084-TFC225RI-V02 Reason – Radiated sample corrected and radiated measurement results replaced – Serial numbers added – Conducted spurious emission results clarified – Editorial corrections	W. Treffke

ABBREVIATIONS AND ACRONYMS

Acronyms	
Acronym	Description
EUT	Equipment Under Test
FCC	Federal Communications Commission
ISED	Innovation, Science and Economic Development Canada
RBW	Resolution bandwidth
RFID	Radio Frequency Identification
RMS	Root mean square
VBW	Video bandwidth
V _{NOM}	Nominal supply voltage

REPORT INDEX


1	Equipment (Test Item) Under Test.....	6
1.1	Photos – Equipment External	7
1.2	Photos – Equipment Internal	9
1.3	Photos – Test Setup.....	11
1.4	Support Equipment.....	13
1.5	Test Modes	14
1.6	Test Frequencies.....	15
1.7	Sample emission level calculation.....	16
2	Result Summary.....	17
3	Test Conditions and Results.....	18
3.1	Test Conditions and Results - Occupied bandwidth.....	18
3.2	Test Conditions and Results - Fundamental in-band field strength emissions	20
3.3	Test Conditions and Results - Emissions radiated outside the specified frequency band	22
3.4	Test Conditions and Results - AC powerline conducted emissions.....	24
ANNEX A	Transmitter in-band emissions	29
ANNEX B	Transmitter radiated spurious emissions.....	30

1 Equipment (Test Item) Under Test

Description	Irrigation Pump for HYS/LAP with Fluid Monitoring Module	
Model	PH304	
Additional Model(s)	None	
Brand Name(s)	GYN-Pump	
Serial Number(s)	1709VG0797 (Radiated sample)	
Hardware Version(s)	03/2019	
Software Version(s)	0.0.6.5	
PMN	TS-HW42	
HVIN	1430	
FVIN	-/-	
HMN	PH304	
Contains FCC-ID	2AS5K-TSHW42	
Contains IC	25004-TSHW42A	
Equipment type	End Product	
Radio type	Transceiver	
Assigned frequency bands	13.110 - 14.010 MHz	
Radio technology	RFID	
Modulation	ASK	
Antenna	Type	External dedicated
	Model	TS-AH20
	Manufacturer	GiS GmbH
	Gain	N/A
Supply Voltage	V _{NOM}	120 VAC
Operating Temperature	T _{NOM}	25 °C
AC/DC-Adaptor	Model	N/A
	Vendor	N/A
	Input	N/A
	Output	N/A
Manufacturer	W.O.M. WORLD OF MEDICINE GmbH Salzufer 8 10587 Berlin GERMANY	

1.1 Photos – Equipment External


EUT Front View (radiated sample)

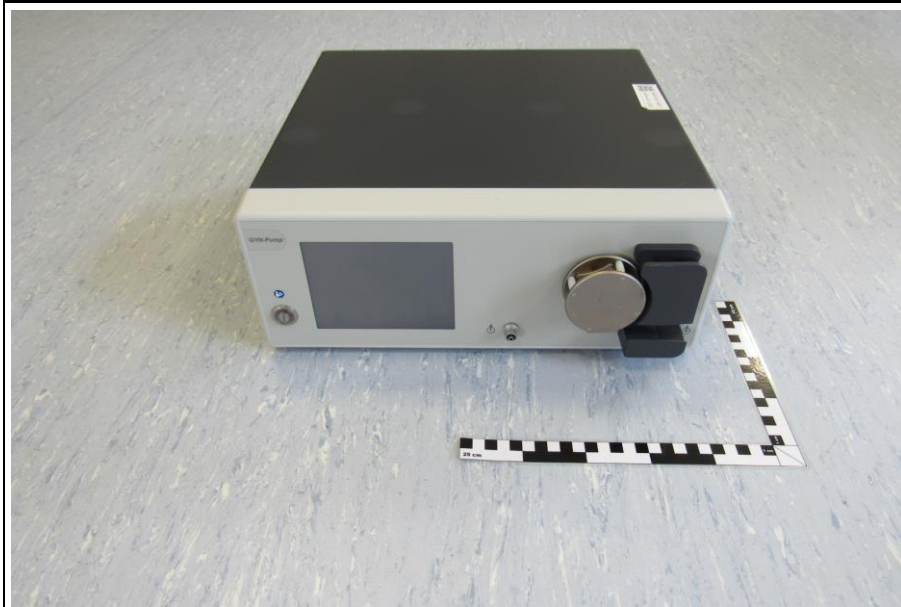



EUT Rear View (radiated sample)



EUR Top View (radiated sample)

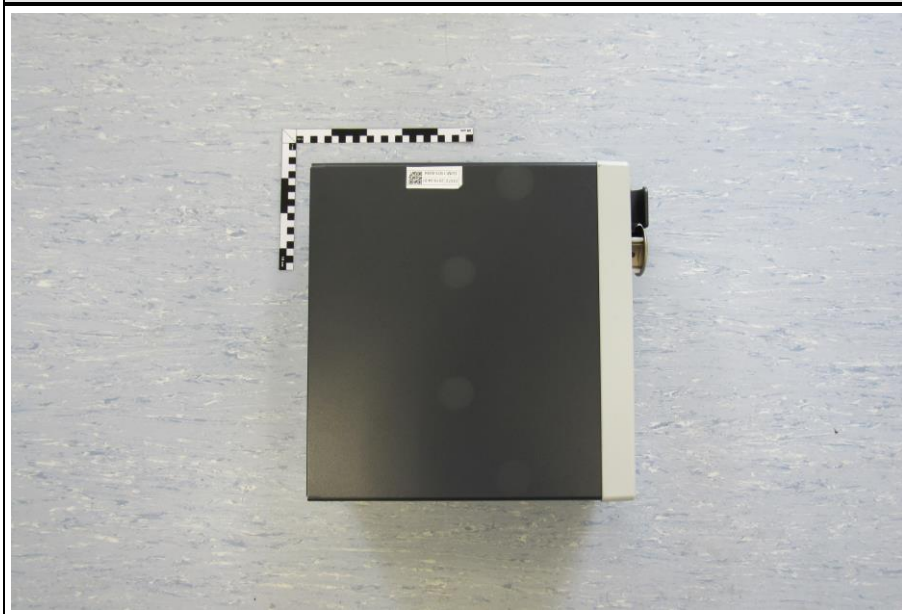



1.2 Photos – Equipment Internal

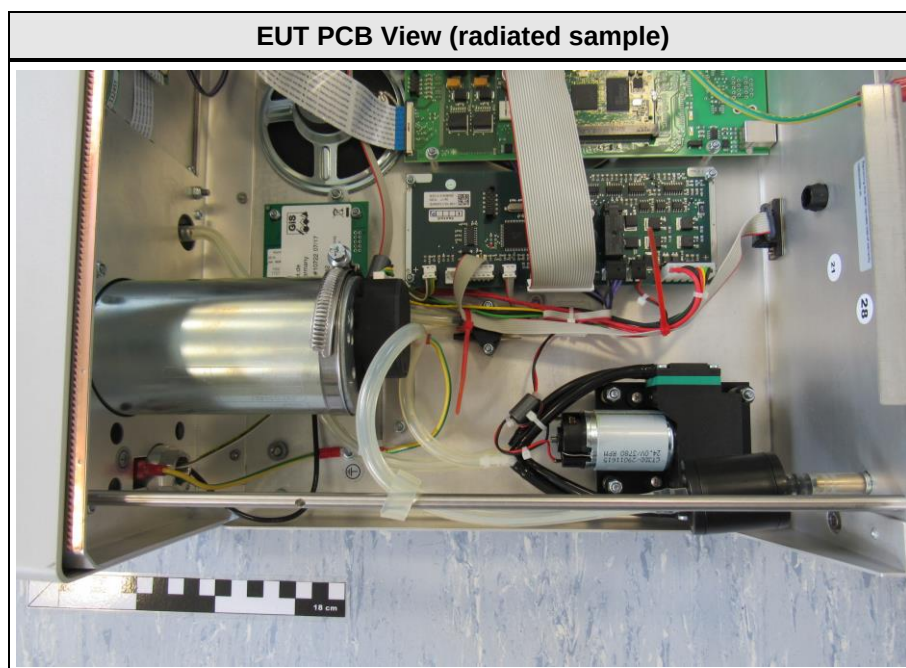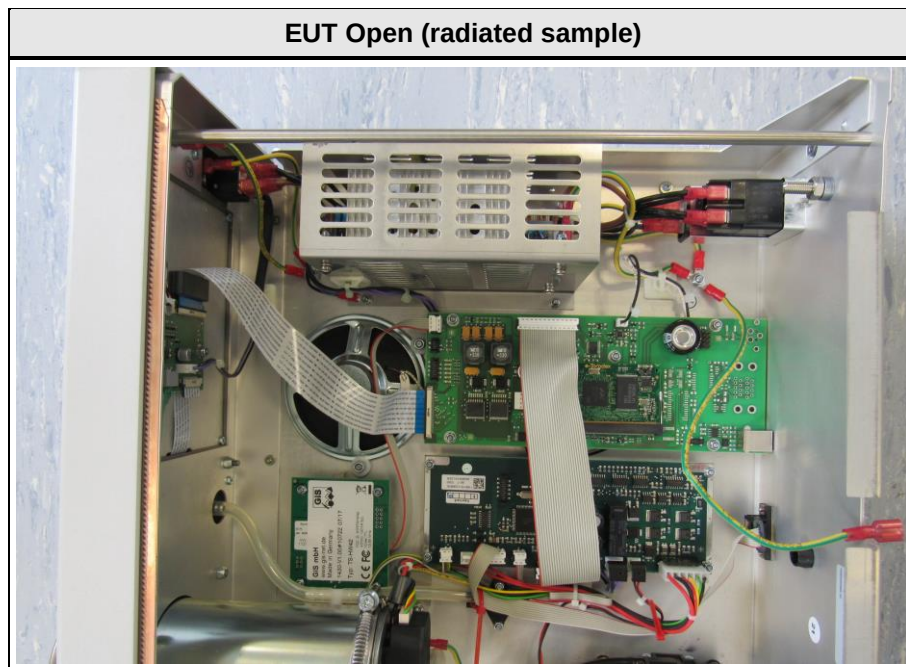


EUT RF-Module View (radiated sample)



1.3 Photos – Test Setup

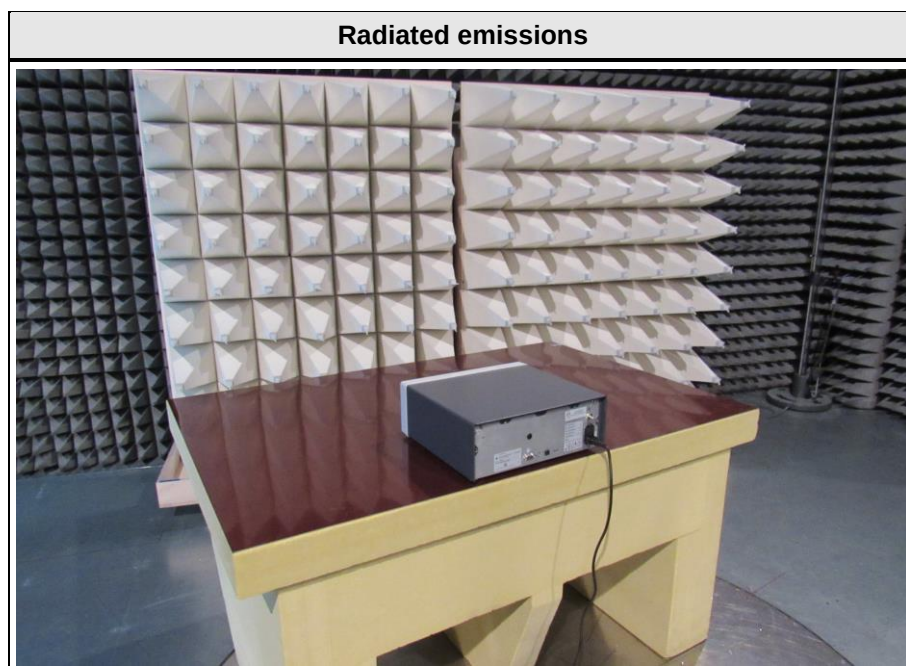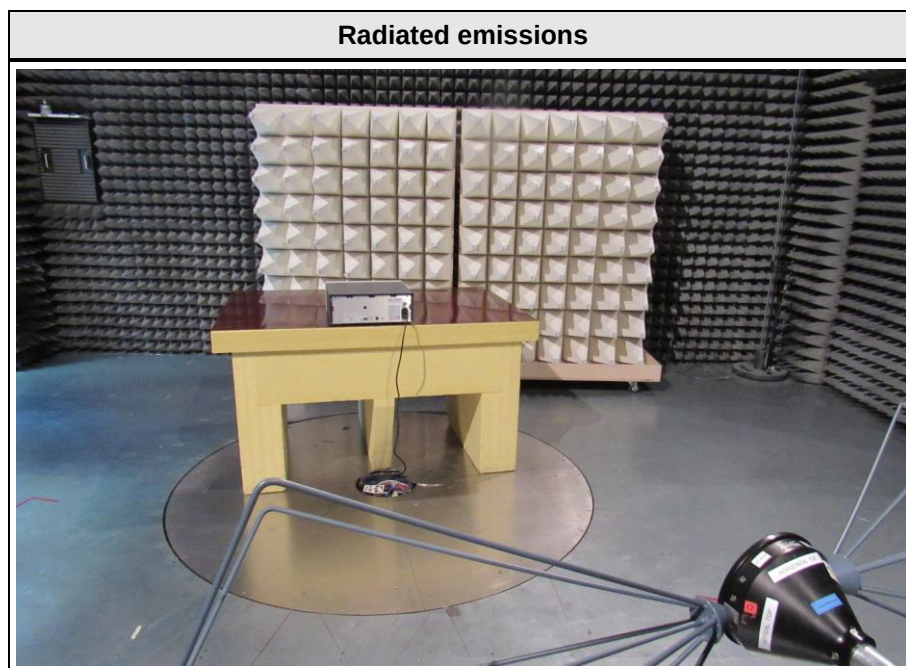

AC power line conducted emissions

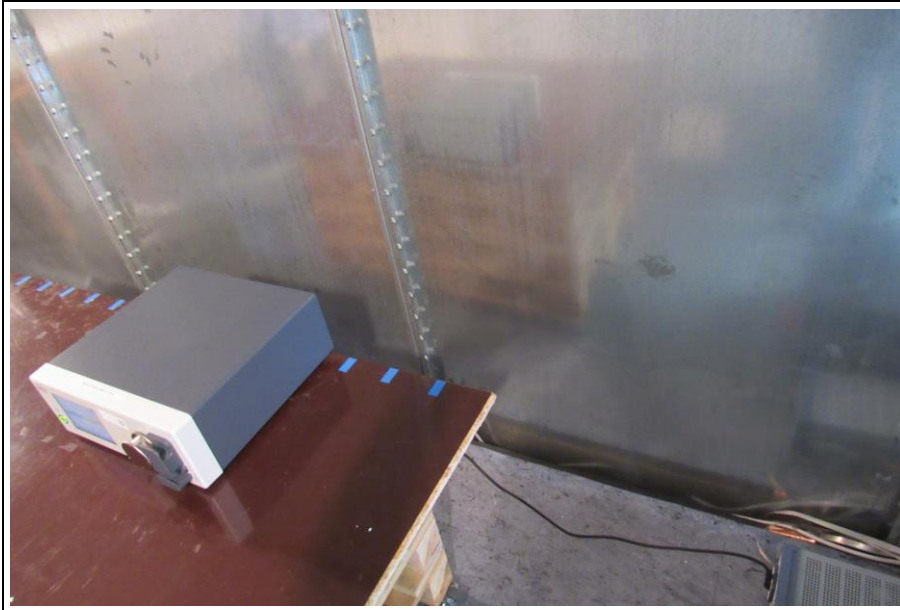

1.4 Support Equipment

Product Type	Device	Manufacturer	Model	Comment
None				
Description:				
AE	Auxiliary Equipment			
SIM	Simulator			
CBL	Connecting Cable			
SFT	Software			
Comment:				

1.5 Test Modes

Mode	Description
Transmit/Receive	Mode = Transmit Modulation = ASK
Comment:	

1.6 Test Frequencies

Designator	Mode	Channel	Frequency [MHz]
F1	Tx / Rx	0	13.5609

1.7 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyzer in dB μ V. Any external preamplifiers used are taken into account through internal analyzer settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyzer. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyzer (dB}\mu\text{V)} + \text{A.F. (dB/m)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dB μ V/m). The FCC limits are given in units of μ V/m. The following formula is used to convert the units of μ V/m to dB μ V/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 \cdot \log(\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

Reading + AF	= Net Reading	:	Net reading - FCC limit	= Margin
+21.5 dB μ V + 26 dB/m	= 47.5 dB μ V/m	:	47.5 dB μ V/m - 57.0 dB μ V/m	= -9.5 dB

2 Result Summary

FCC 47 CFR Part 15C, ISSED RSS-210; ISSED RSS GEN				
Product Standard Reference	Requirement	Reference Method	Result	Remarks
ISSED RSS-Gen 6.7	Occupied Bandwidth	ANSI C63.10-2013	N/R	Informational only
FCC 47 CFR 15.225(a-c) ISSED RSS-210 B.6(a)	Fundamental in-band field strength emissions	ANSI C63.10-2013	PASS	
FCC 47 CFR 15.225(d) FCC 47 CFR 15.209 ISSED RSS-210 B.6(d)	Emission radiated outside the specified frequency band	ANSI C63.10-2013	PASS	
FCC 47 CFR 15.225(e) ISSED RSS-210 B.6	Frequency stability	ANSI C63.10-2013	N/T	Module integration
ISSED RSS-Gen 4.10 ISSED RSS-Gen 7.1	Receiver radiated spurious emissions	ANSI C63.10-2013	N/R	Permanently co-located transmitter
FCC 47 CFR 15.207 ISSED RSS-Gen 8.8	AC power line conducted emissions	ANSI C63.10-2013	PASS	
Comment:				

Possible Test Case Verdicts	
PASS	Test object does meet the requirements
FAIL	Test object does not meet the requirements
N/T	Required by standard but not tested
N/R	Not required by standard for the test object

3 Test Conditions and Results

3.1 Test Conditions and Results - Occupied bandwidth


3.1.1 Information

Test Information	
Product Standard Reference	ISED RSS-Gen 6.7
Measurement Method	Conducted

3.1.2 Limits

Limits
None (Informational only)

3.1.3 Setup

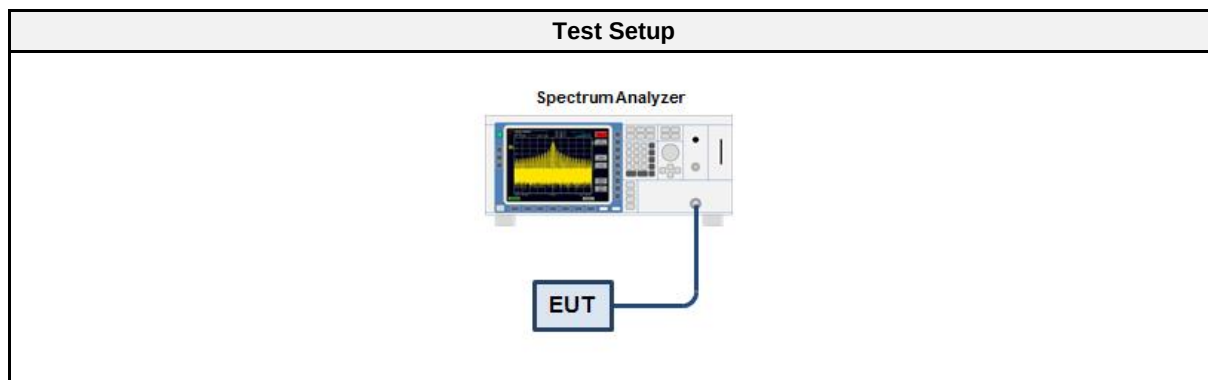

3.1.4 Equipment

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Spectrum Analyzer	R&S	FSU 26	EF01407	2018-12	2019-12

3.1.5 Procedure


Test Procedure
1. EUT set to test mode (Communication tester is used if needed) 2. Span set to at least twice the emission spectrum 3. Resolution bandwidth set between 1 % to 5 % of OBW 4. Occupied Bandwidth (99 %) measurement with spectrum analyzer built in measurement function

3.1.6 Results

Test Results	
Channel [MHz]	Bandwidth [kHz]
13.5609	145

Occupied Bandwidth

Project Number: G0M-1903-8084
 Applicant: W.O.M. WORLD OF MEDICINE GmbH
 Model Description: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
 Model: PH304
 Operator: Wilfried Treffke
 Test Site: Eurofins Product Service GmbH
 Test Date: 2019-05-06
 Operating Conditions: Tnom/Vnom
 Reference Standards: ANSI C63.10:2013, Section 6.9.3
 Mode: ASK, Channel: 13.5609 MHz
 Occupied Bandwidth [MHz]: 145 kHz

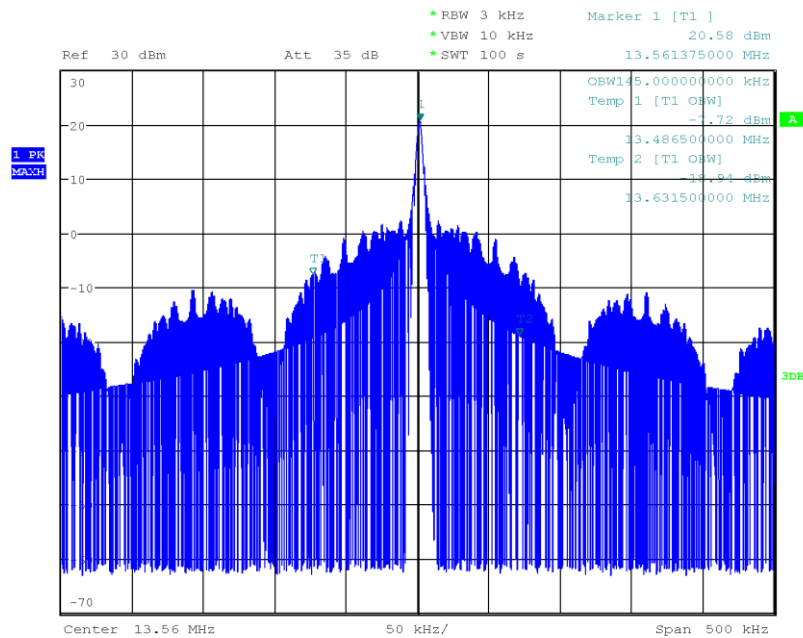

Date: 6.MAY.2019 08:59:32

3.2 Test Conditions and Results - Fundamental in-band field strength emissions


3.2.1 Information

Test Information	
Product Standard Reference	FCC 47 CFR 15.225(a-c) / ISSED RSS-210 B.6(a)
Measurement Method	Radiated
Operator	Christian Weber
Date	2019-06-06

3.2.2 Limits

Limits			
Frequency range [MHz]	Limit [$\mu\text{V/m}$]	Limit [$\text{dB}\mu\text{V/m}$]	Limit Distance [m]
13.553 - 13.567	15848	84	30
13.410 - 13.553 13.567 - 13.710	334	50.5	30
13.110 - 13.410 13.710 - 14.010	106	40.5	30

3.2.3 Setup

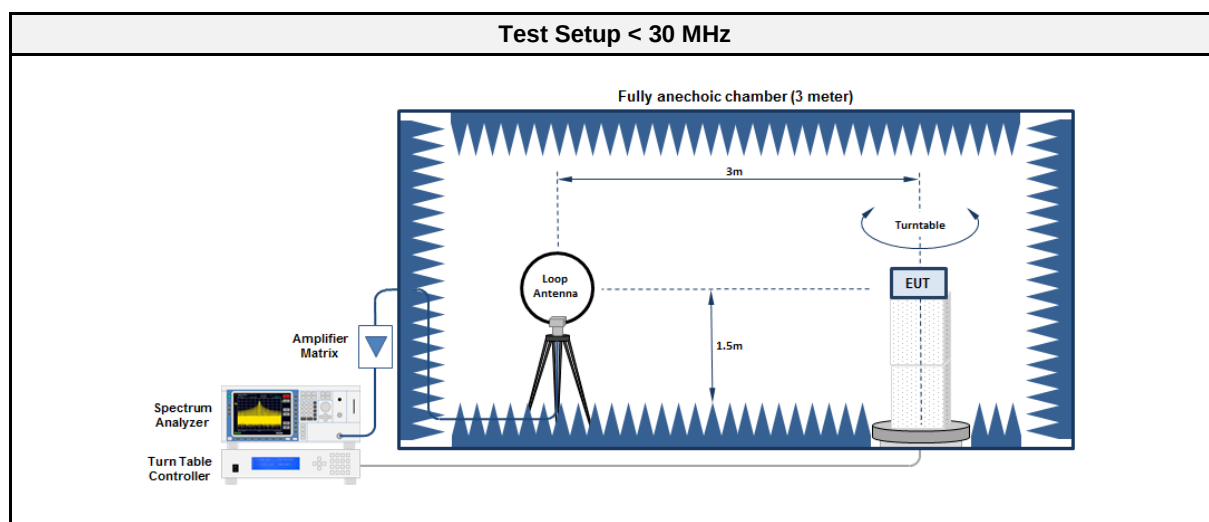

3.2.4 Equipment

Test Software			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	RadiMation	2015.2.4

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Semi-Anechoic Chamber	Frankonia	AC2	EF00196	-	-
Spectrum Analyzer	R&S	FSU 3	EF00241	2017-07	2019-07
Antenna	R&S	HFH2-Z2	EF00184	2017-12	2019-12

3.2.5 Procedure

Test Procedure	
1.	EUT set to test mode
2.	Span it set according to measurement range
3.	Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector
4.	Below 30MHz an extrapolation according ANSI 63.10; 6.4.4.2 is used.

3.2.6 Results

Test Results						
Channel [MHz]	Emission [MHz]	Level @ 30 m [dBμV/m]	Detector	Polarization	Limit @ 30 m [dBμV/m]	Margin
13.5609	13.56	13	pk	ver	84	-71.00

3.3 Test Conditions and Results - Emissions radiated outside the specified frequency band


3.3.1 Information


Test Information	
Product Standard Reference	FCC 47 CFR 15.225(d) / ISED RSS-210 B.6(d)
Measurement Method	Radiated
Operator	Christian Weber
Date	2019-06-06

3.3.2 Limits

Limits				
Frequency range [MHz]	Detector	Limit [$\mu\text{V/m}$]	Limit [$\text{dB}\mu\text{V/m}$]	Limit Distance [m]
0.009 - 0.490	Quasi-Peak	2400/F[kHz]	48.5 - 13.8	300
0.490 - 1.705	Quasi-Peak	2400/F[kHz]	13.8 - 2.97	30
1.705 - 30	Quasi-Peak	30	29.5	30
30 - 88	Quasi-Peak	100	40	3
88 - 216	Quasi-Peak	150	43.5	3

3.3.3 Setup

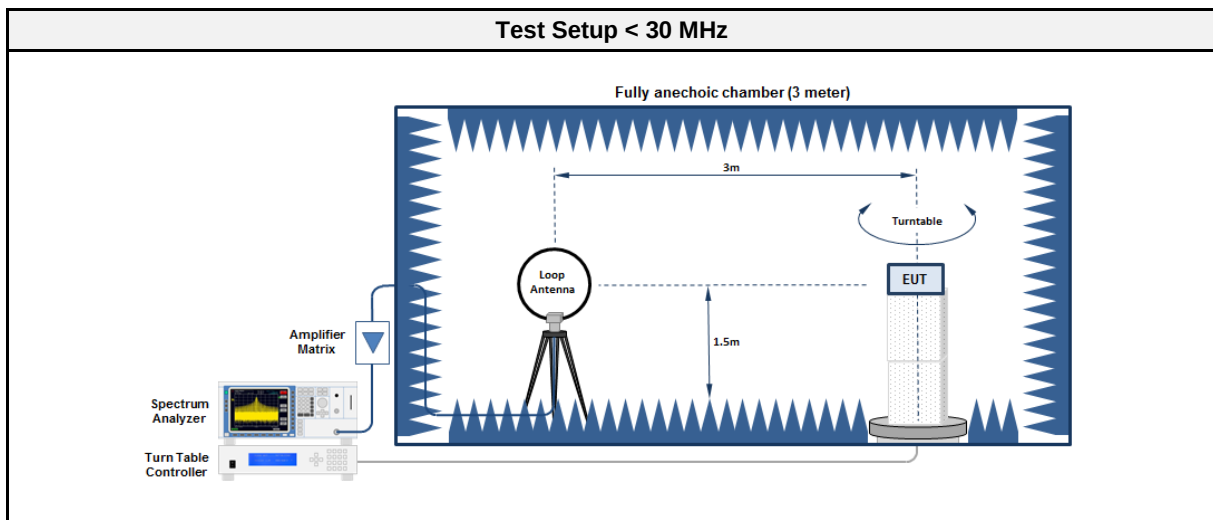

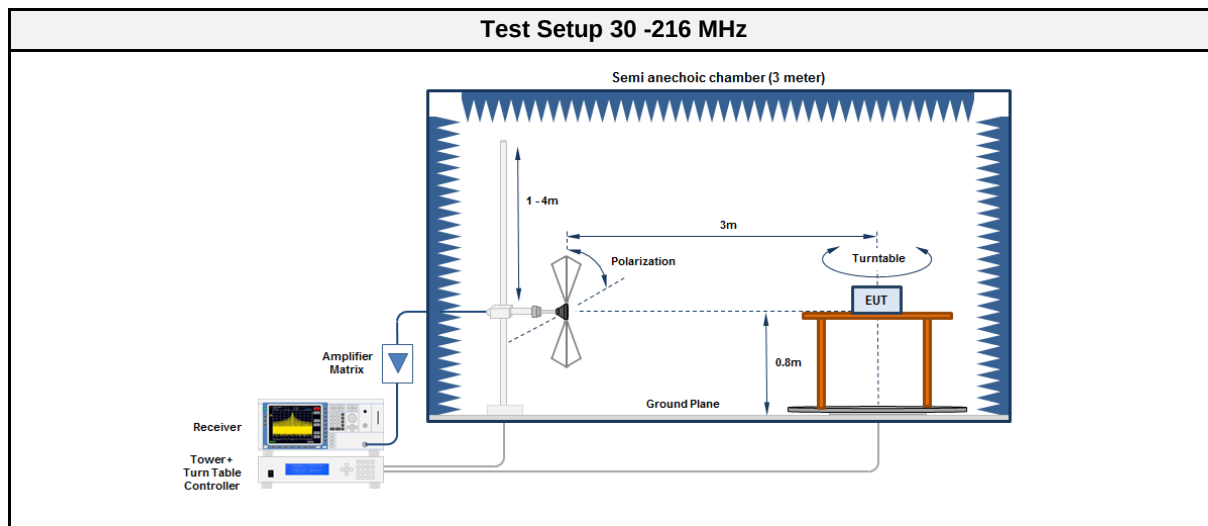

3.3.4 Equipment

Test Software			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	RadiMation	2015.2.4

Test Equipment < 30 MHz					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic Chamber	Frankonia	AC2	EF00196	-	-
Loop Antenna	R&S	HFH2-Z2	EF00184	2017-12	2019-12
Spectrum Analyzer	R&S	FSU 3	EF00241	2017-07	2019-07

Test Equipment 30 - 216 MHz					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic Chamber	Frankonia	AC1	EF00062	2018-07	2021-07
Measurement Receiver	R&S	N9038A-526/WXP	EF01070	2018-08	2019-08
Antenna	R&S	HK116	EF00186	2018-03	2020-03

3.3.5 Procedure

Test Procedure	
1. EUT set to test mode 2. Span it set according to measurement range 3. Resolution bandwidth below 1 GHz is set according to CISPR 16 with peak/quasi-peak detector and RBW of 1 MHz with peak/average detector is used above 1 GHz 4. Below 30MHz an extrapolation according ANSI 63.10; 6.4.4.2 is used. 5. Markers are set to maximum emission levels	

3.3.6 Results

Test Results						
Channel [MHz]	Emission [MHz]	Level [dBμV/m]	Detector	Polarization	Limit [dBμV/m]	Margin [dB]
13.5609	No significant spurious emissions					

3.4 Test Conditions and Results - AC powerline conducted emissions

3.4.1 Information


Test Information	
Reference	FCC 47 CFR 15.207; ISSED RSS-Gen, Issue 5
Measurement Method	ANSI C63.10 6.2
Operator	Mr. Weber
Date	2019-05-03

3.4.2 Limits

Limits		
Frequency [MHz]	Quasi-Peak [dBμV]	Average [dBμV]
0.15 - 0.5	66 - 56*	56 - 46*
0.5 - 5	56	46
5 - 30	60	50

* Limit decreases linearly with the logarithm of the frequency

3.4.3 Setup

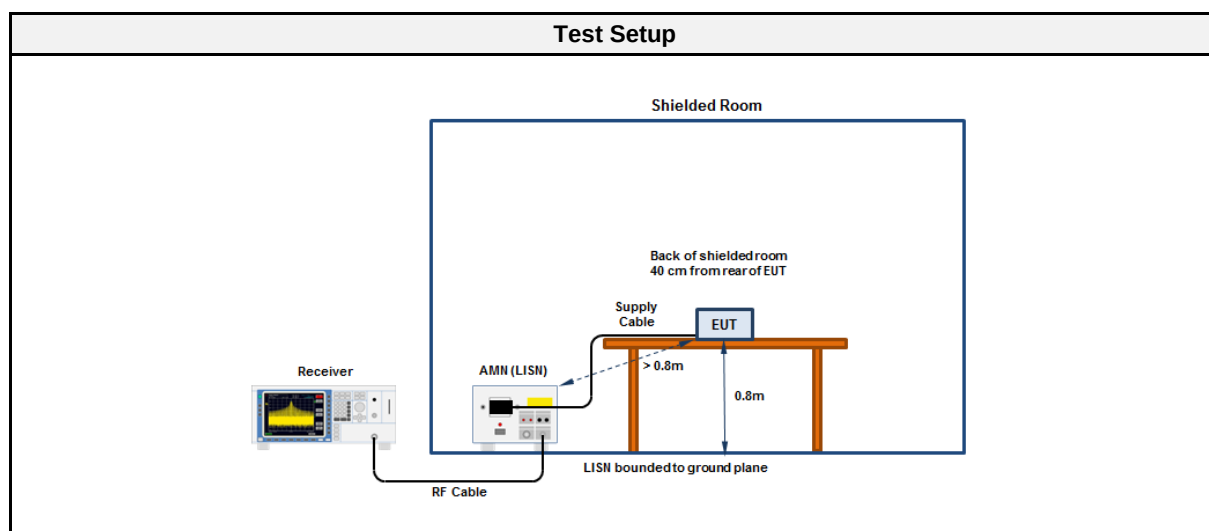

3.4.4 Equipment

Test Software			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	RadiMation	2016.1.10


Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
EMI Receiver	R&S	ESU 26	EF00241	2017-07	2019-07
LISN	R&S	ESH3-Z5	EF00036	2017-01	2019-07

EMI voltage test in the ac-mains according to FCC 47 CFR 15.207, ISSED RSS-GEN

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
 EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
 Model: PH304
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Weber
 Test Conditions: Tnom: 26°C, Unom: 120 VAC
 LISN: ESH3-Z5 (N)
 Mode: Transmit
 Test Date: 2019-05-03
 Note:

Index 8

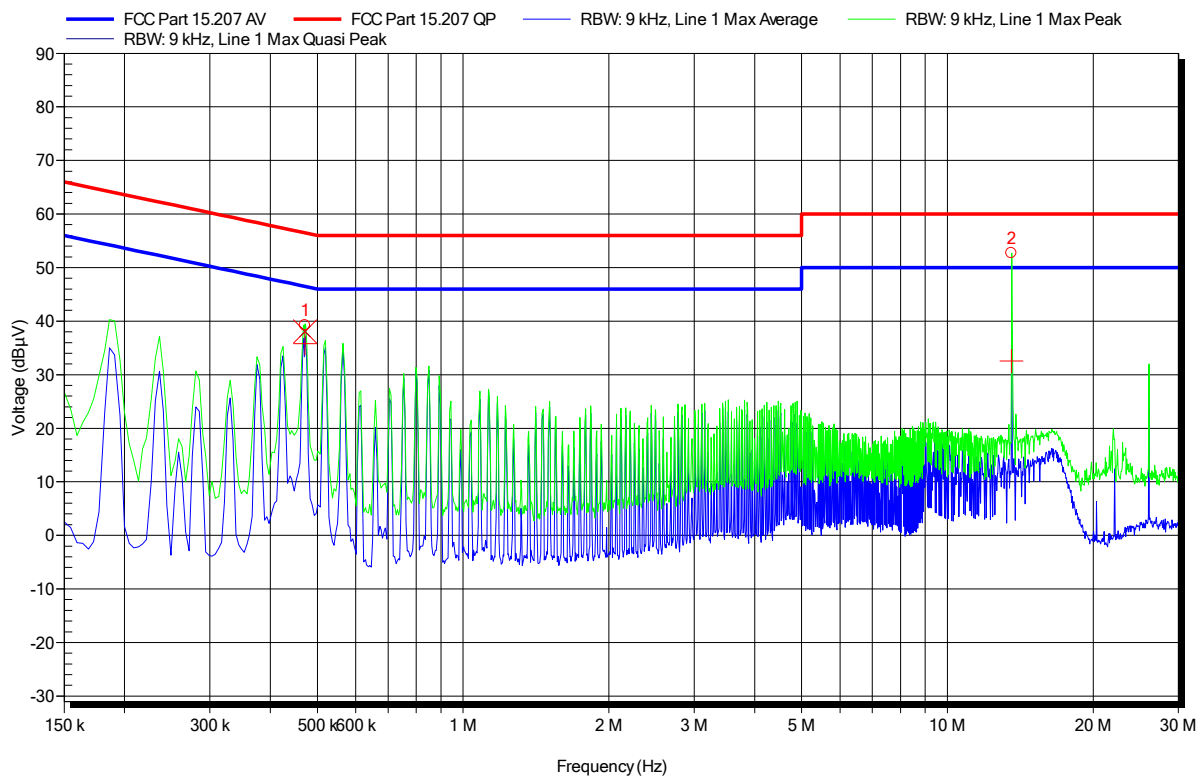

Peak Number	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
1	471.75 kHz	38.09 dBμV	56.48 dBμV	-18.39 dB	Pass
2	13.565 MHz	52.68 dBμV	60 dBμV	-07.32 dB	Pass


Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status
1	471.75 kHz	35.8 dBμV	46.48 dBμV	-10.68 dB	Pass
2	13.565 MHz	32.56 dBμV	50 dBμV	-17.44 dB	Pass

EMI voltage test in the ac-mains according to FCC 47 CFR 15.207, ISSED RSS-GEN

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
 EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
 Model: PH304
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Weber
 Test Conditions: Tnom: 26°C, Unom: 120 VAC
 LISN: ESH3-Z5 (L)
 Mode: Transmit
 Test Date: 2019-05-03
 Note:

Index 9

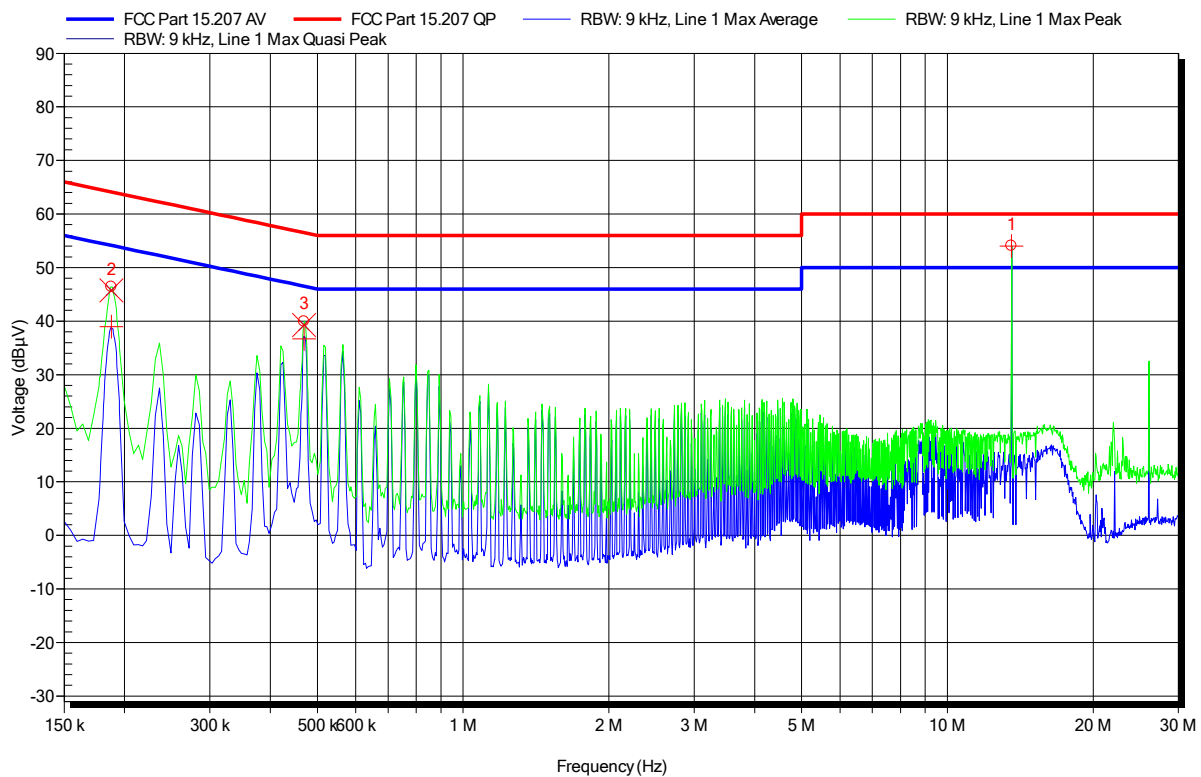

Peak Number	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
1	13.56 MHz				
2	187.8 kHz	45.77 dBµV	64.13 dBµV	-18.36 dB	Pass
3	469.5 kHz	39.24 dBµV	56.52 dBµV	-17.28 dB	Pass

Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status
1	13.56 MHz	54.03 dBµV	50 dBµV	4.03 dB	Fail*
2	187.8 kHz	38.97 dBµV	54.13 dBµV	-15.16 dB	Pass
3	469.5 kHz	36.71 dBµV	46.52 dBµV	-9.82 dB	Pass


* Note: According to FCC KDB 174176 D01 v01r01, emissions from the intentional radiator can exceed the limit in transmit mode with antenna connected as long as the emissions are below the limit with the antenna disconnected and the antenna port terminated by 50 Ohm load. This measurement is shown in the following two plots.

EMI voltage test in the ac-mains according to FCC 47 CFR 15.207, ISED RSS-GEN

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
Model: PH304
Test Site: Eurofins Product Service GmbH
Operator: Mr. Weber
Test Conditions: Tnom: 26°C, Unom: 120 VAC
LISN: ESH3-Z5 (N)
Mode: Transmit, Antenna port terminated
Test Date: 2019-05-03
Note:

Index 10

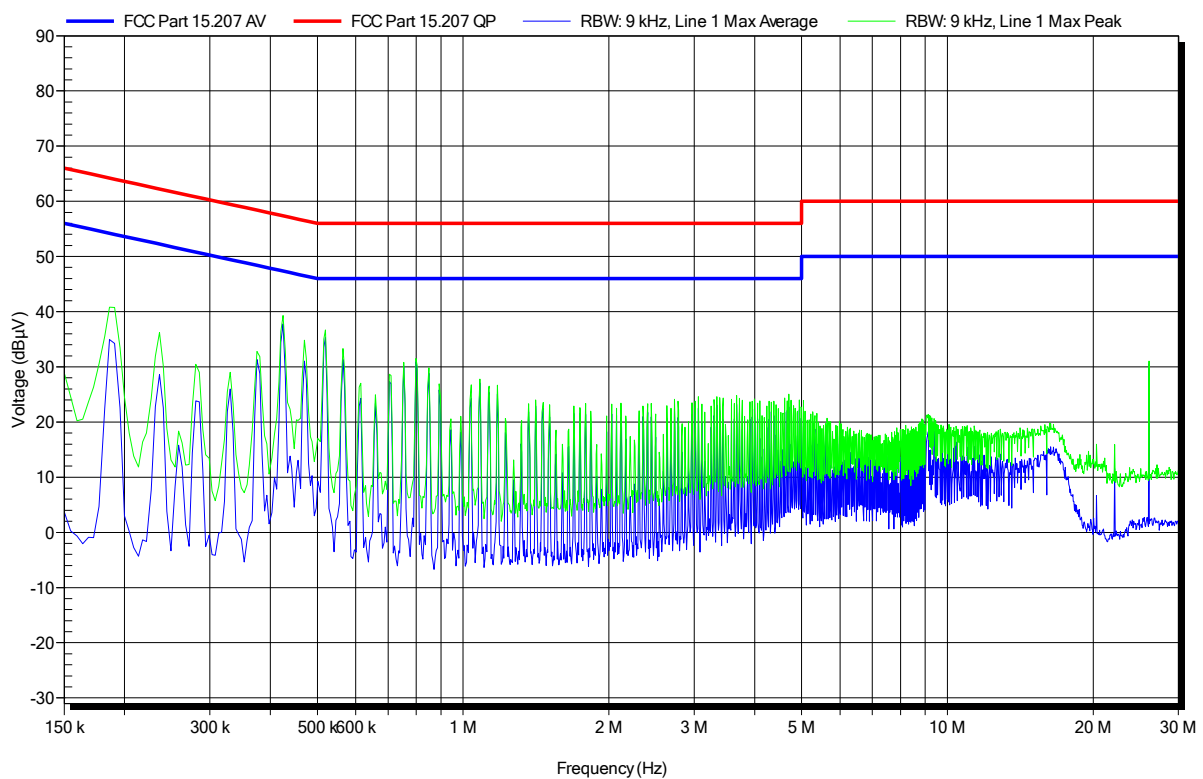


EMI voltage test in the ac-mains according to FCC 47 CFR 15.207, ISED RSS-GEN

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
Model: PH304
Test Site: Eurofins Product Service GmbH
Operator: Mr. Weber
Test Conditions: Tnom: 26°C, Unom: 120 VAC
LISN: ESH3-Z5 (L)
Mode: Transmit, Antenna port terminated
Test Date: 2019-05-03
Note:

Index 11

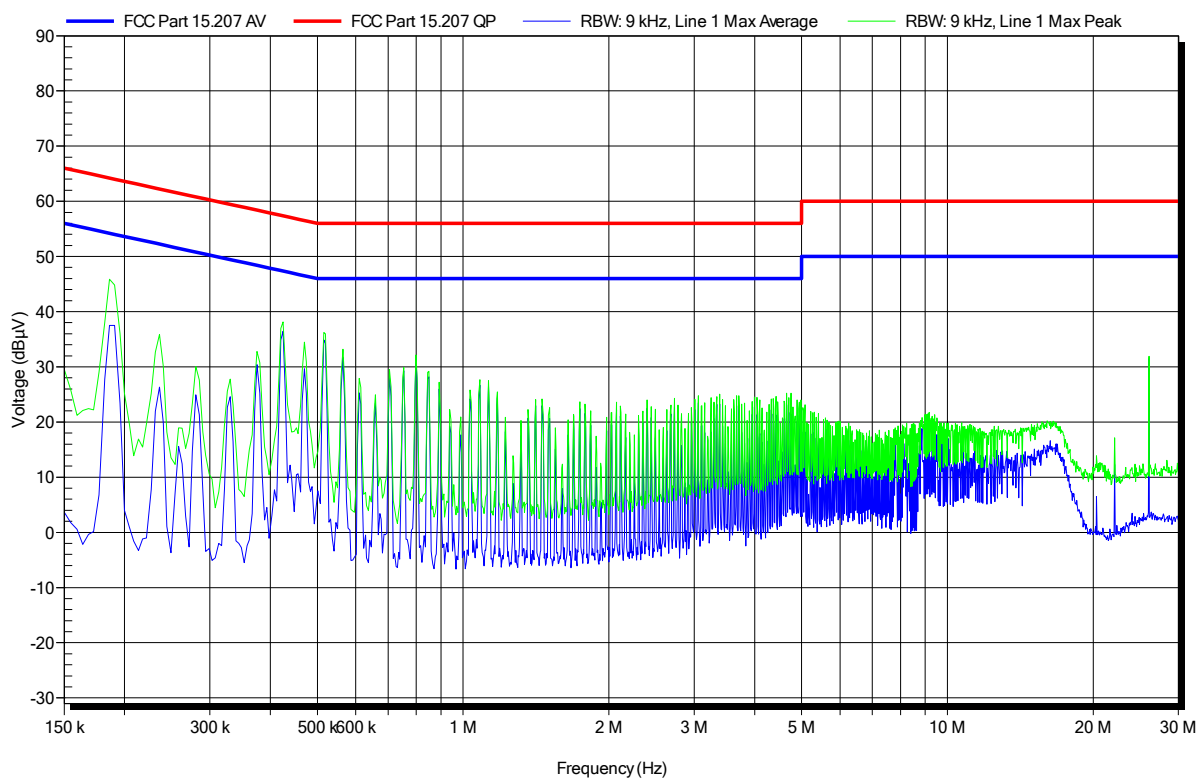


ANNEX A Transmitter in-band emissions

Radiated H-Field according to FCC 47 CFR 15.225; ISED RSS-210

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
Model: PH304
Test Site: Eurofins Product Service GmbH
Operator: Mr. Weber
Test Conditions: Tnom: 26°C, Vnom: 120 VAC
Antenna: Rohde & Schwarz HFH 2-Z2
Measurement distance: 3 m converted to 30 m
Mode: TX; Tx
Test Date: 2019-06-06
Note: EUT vertical, measured without Tag continuously reading

Index 12

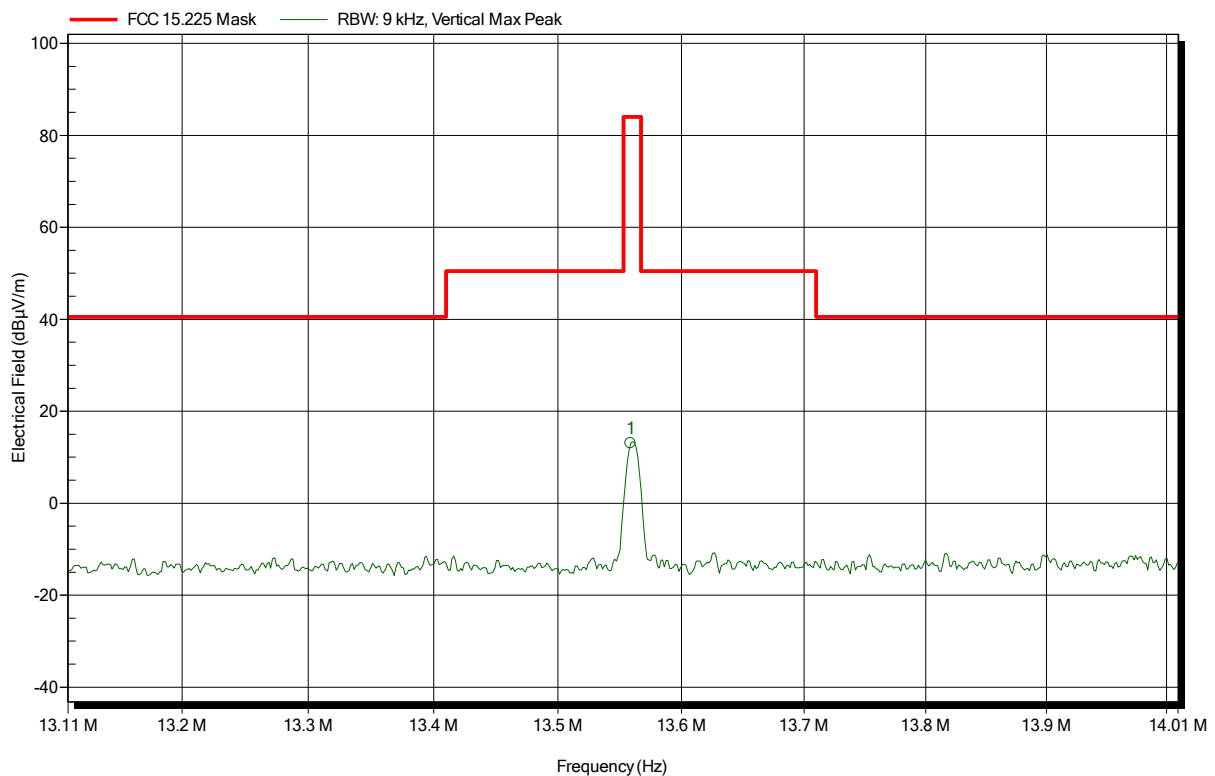

Frequency
13.559 MHz

Peak
13 dBµV/m


ANNEX B Transmitter radiated spurious emissions

Spurious emissions according to FCC 47 CFR 15.225, ISED RSS-210

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
Model: PH304
Test Site: Eurofins Product Service GmbH
Operator: Mr. Weber
Test Conditions: Tnom: 24°C, Vnom: 120 VAC
Antenna: Rohde & Schwarz HFH 2-Z2
Measurement distance: 3 m converted to 300 m
Mode: TX; Tx
Test Date: 2019-06-06
Note:

Index 13

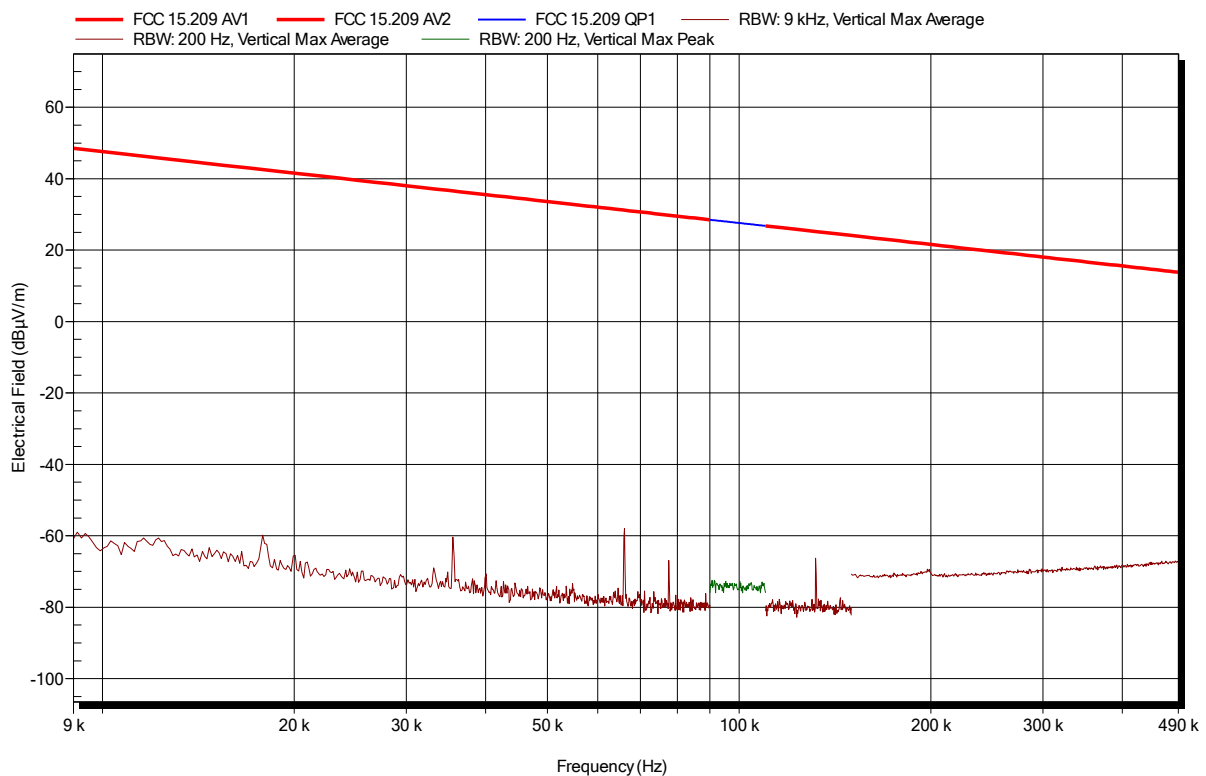


Spurious emissions according to FCC 47 CFR 15.225, ISED RSS-210

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
Model: PH304
Test Site: Eurofins Product Service GmbH
Operator: Mr. Weber
Test Conditions: Tnom: 24°C, Vnom: 120 VAC
Antenna: Rohde & Schwarz HFH 2-Z2
Measurement distance: 3 m converted to 30 m
Mode: TX; Tx
Test Date: 2019-06-06
Note: EUT vertical, measured without Tag continuously reading

Index 14

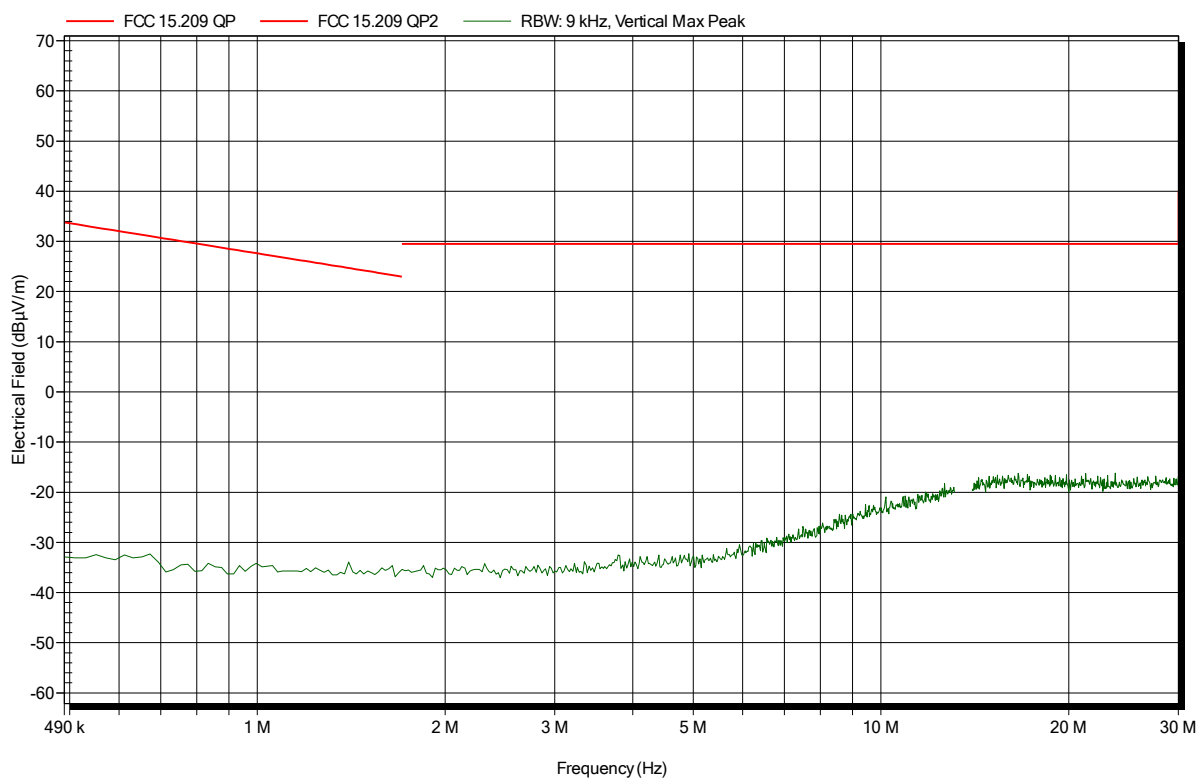


Spurious emissions according to FCC 47 CFR 15.225, ISED RSS-210

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
Model: PH304
Test Site: Eurofins Product Service GmbH
Operator: Florian Voigt (supervised)
Test Conditions: Tnom: 24°C, Vnom: 120 VAC
Antenna: HK116, Vertical
Measurement distance: 3 m
Mode: TX; Tx
Test Date: 2019-06-06
Note:

Index 15

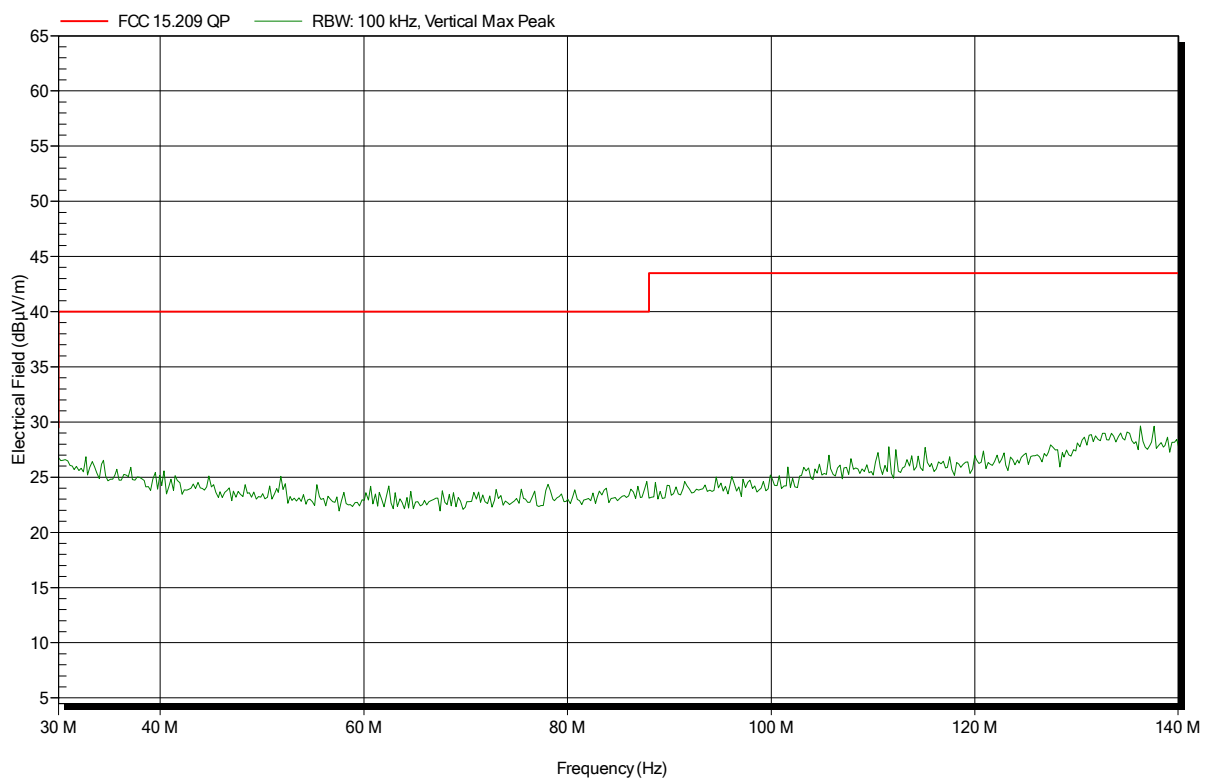

Spurious emissions according to FCC 47 CFR 15.225, ISED RSS-210

Project number: G0M-1903-8084

Applicant: W.O.M. WORLD OF MEDICINE GmbH
EUT Name: Irrigation Pump for HYS/LAP with Fluid Monitoring Module
Model: PH304
Test Site: Eurofins Product Service GmbH
Operator: Florian Voigt (supervised)
Test Conditions: Tnom: 24°C, Vnom: 120 VAC
Antenna: HK116, Horizontal
Measurement distance: 3 m
Mode: TX; Tx
Test Date: 2019-06-06
Note:

Index 16

