

## EMC TEST REPORT

### FCC 47 CFR Part 15B, ISED ICES-003 Issue 6

<b>Report Reference No</b>	G0M-1806-7459-EF0115B-V01
<b>Testing Laboratory</b>	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	     DAkkS - Registration number : D-PL-12092-01-03 (ISED) ISED Testing Laboratory site: 3470A-3 DAkkS - Registration number : D-PL-12092-01-04 (FCC) FCC Filed Test Laboratory, Reg.-No.: 96970
<b>Applicant</b>	W.O.M. WORLD OF MEDICINE GmbH
Address	Salzufer 8 10587 Berlin GERMANY
<b>Test Specification</b>	
Standard	FCC 47 CFR Part 15 Subpart B ISED ICES-003 Issue 6 ANSI C63.4:2014
Non-Standard Test Method	None
<b>Equipment under Test (EUT):</b>	
Product Description	The device PP120 is a pump providing irrigation and suction function for laparoscopy
Model(s)	PP120
Additional Model(s)	None
Brand Name(s)	LAP-Pump
Hardware Version(s)	04/15
Software Version(s)	01.01
Contains FCC-ID	2AS5K-TSHW42
Contains IC	25004-TSHW42A
<b>Test Result</b>	<b>PASSED</b>

<b>Possible test case verdicts:</b>		
required by standard but not tested	N/T	
not required by standard	N/R	
required by standard but not appl. to test object	N/A	
test object does meet the requirement	P(PASS)	
test object does not meet the requirement	F(FAIL)	
<b>Testing:</b>		
Date of receipt of test item	2019-03-21	
<b>Report:</b>		
Compiled by	Ruslan Colbasiuc	
Tested by (+ signature) (Responsible for Test)	Ruslan Colbasiuc	
Approved by (+ signature) (Deputy Head of Lab)	Jens Marquardt	
Date of Issue	2019-07-09	
Total number of pages	30	
<b>General Remarks:</b>		
<p><b>The test results presented in this report relate only to the object tested.</b></p> <p><b>The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.</b></p> <p>This report shall not be reproduced, except in full, without the written approval of the issuing testing laboratory.</p>		
<b>Additional Comments:</b>		

**ABBREVIATIONS AND ACRONYMS**

<b>Acronyms</b>	
Acronym	Description
EUT	Equipment Under Test
FCC	Federal Communications Commission
ISED	Innovation, Science and Economic Development Canada
$T_{NOM}$	Nominal operating temperature
$V_{NOM}$	Nominal supply voltage

**VERSION HISTORY**

<b>Version History</b>			
Version	Issue Date	Remarks	Revised By
01	2019-07-09	Initial Release	

**REPORT INDEX**

<b>1</b>	<b>Equipment (Test Item) Under Test.....</b>	<b>6</b>
1.1	Equipment Ports.....	7
1.2	Equipment Photos – Internal.....	8
1.3	Equipment Photos - External.....	12
1.4	Support Equipment.....	15
1.5	Operational Modes.....	16
1.6	EUT Configuration.....	17
1.7	Sample emission level calculation.....	18
<b>2</b>	<b>Result Summary.....</b>	<b>19</b>
2.1	Test Conditions and Results - Radiated emissions acc. to ANSI C63.4.....	20
2.2	Test Conditions and Results - Conducted emissions acc. to ANSI C63.4.....	26



## 1 Equipment (Test Item) Under Test



Description	The device PP120 is a pump providing irrigation and suction function for laparoscopy	
Model	PP120	
Additional Model(s)	None	
Brand Name(s)	None	
Serial Number(s)	1504PT0001	
Hardware Version(s)	04/15	
Software Version(s)	01.01	
Contains FCC-ID	2AS5K-TSHW42	
Contains IC	25004-TSHW42A	
Class	Class B	
Equipment type	Table top	
Highest internal frequency [MHz]	16	
Radio Module	Type	RFID Module
	Model	TS-HW42
	Manufacturer	GiS mbH
	FCC-ID	2AS5K-TSHW42
	IC	25004-TSHW42A
Supply Voltage	V <sub>NOM</sub>	120 VDC / 60 Hz
Manufacturer	W.O.M. WORLD OF MEDICINE GmbH Salzufer 8 10587 Berlin GERMANY	



### 1.1 Equipment Ports


Name	Type	Attributes	Comment
Mains	AC	Count: 1 Direction: IO Service only: No	
RS-232	IO	Count: 1 Direction: IO Service only: Yes	
Potential Equalization (PE)	AC	Count: 1 Direction: Out Service only: No	
Description:			
AC	AC mains power input/output port		
DC	DC power input/output port		
IO	Input/Output port		
TP	Telecommunication port		
NE	Non-electrical port		

## 1.2 Equipment Photos – Internal

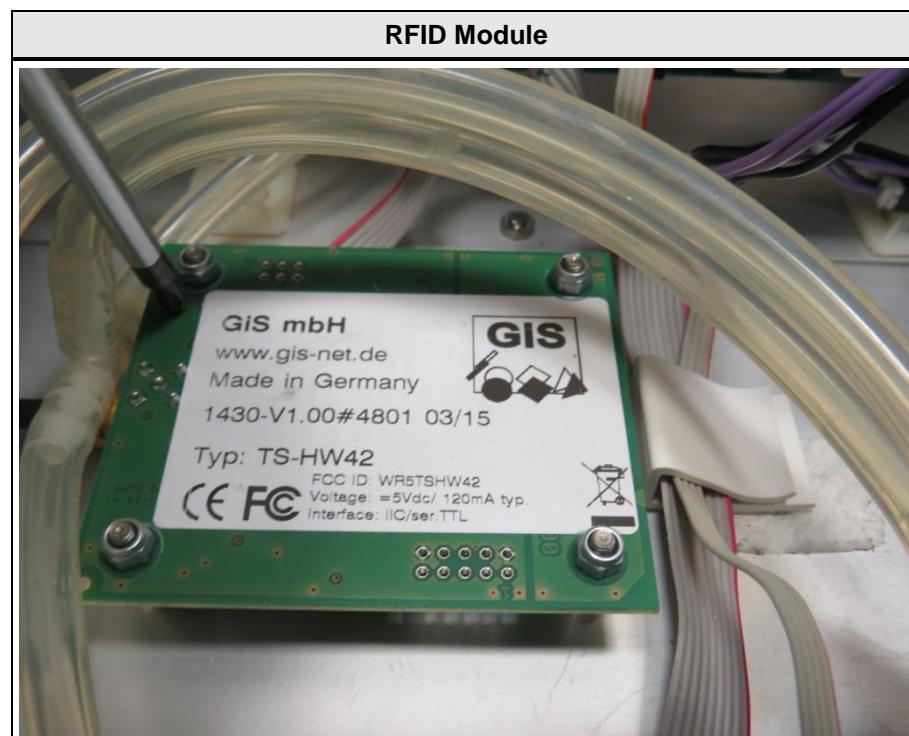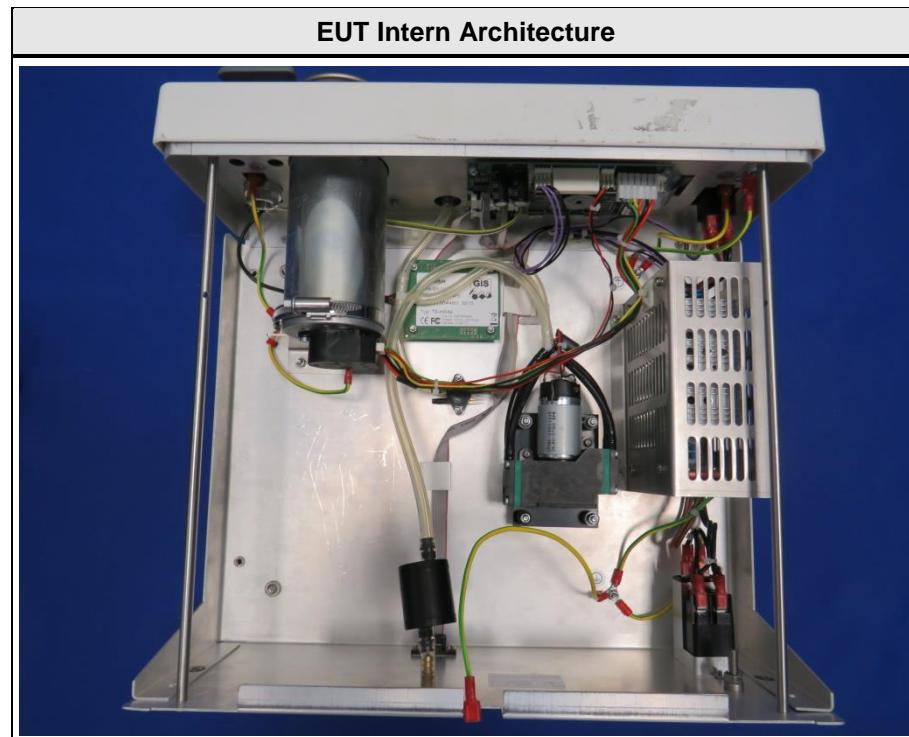

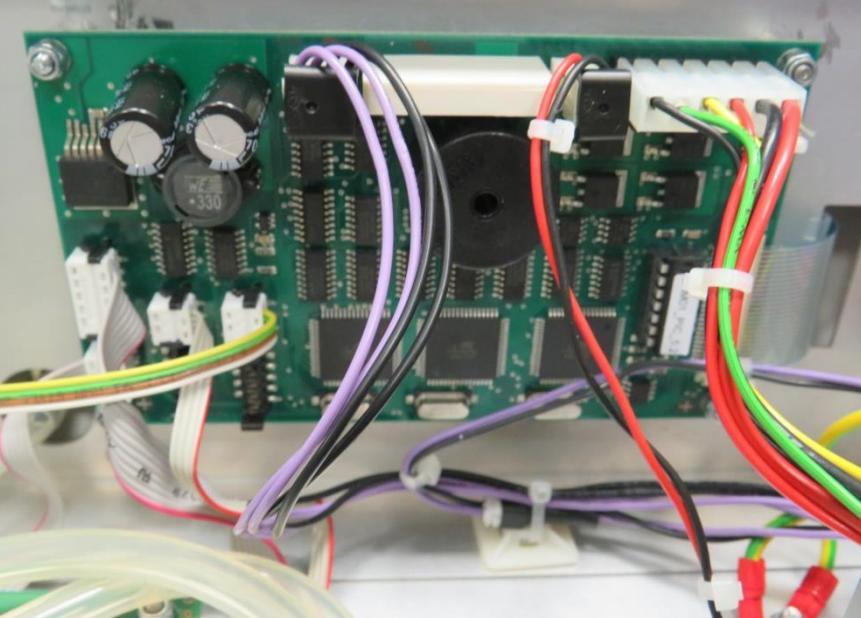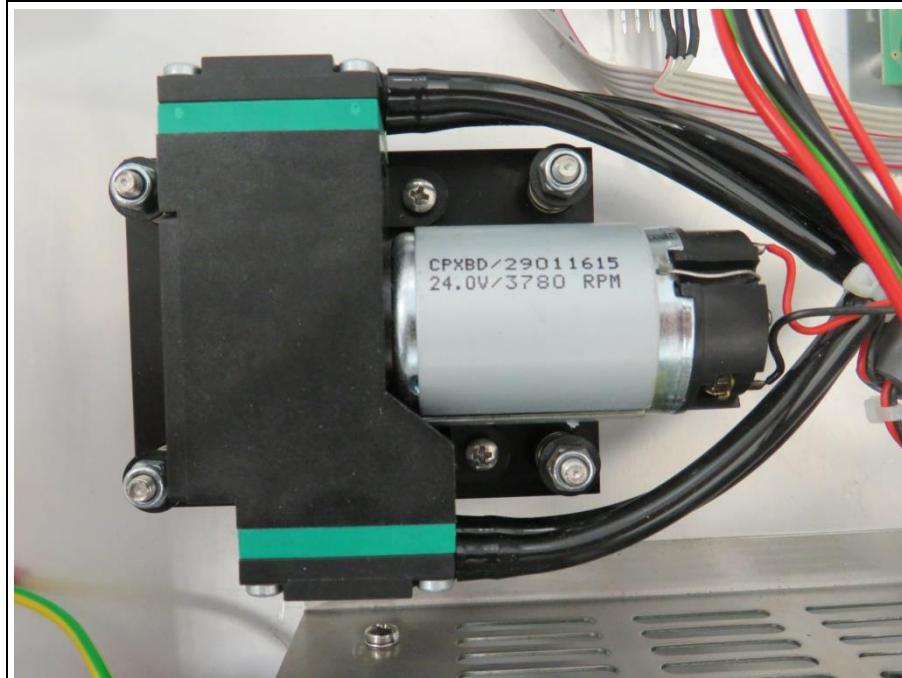**Main Board****Vacuum Pump**

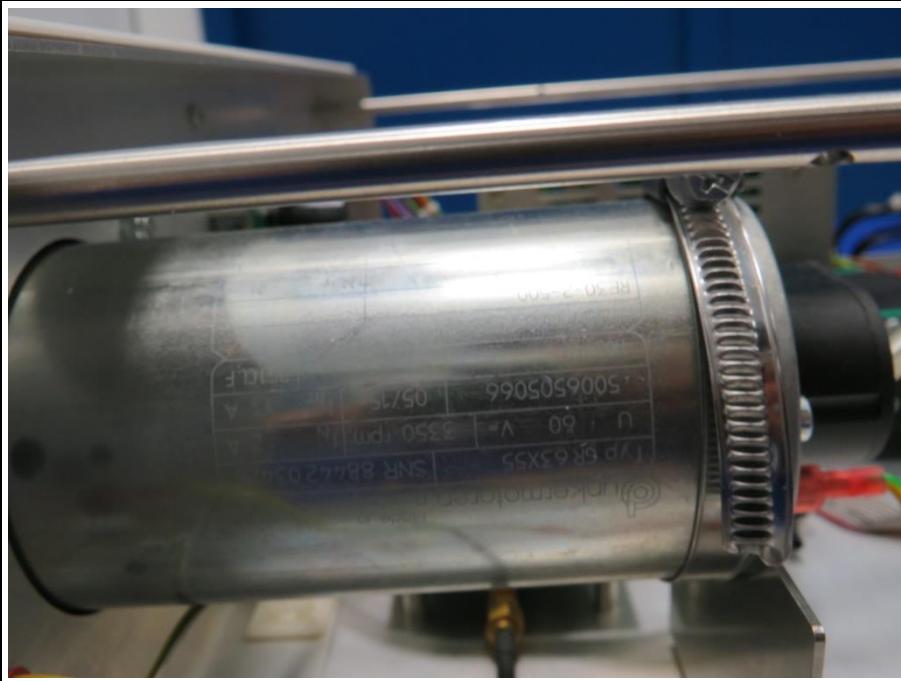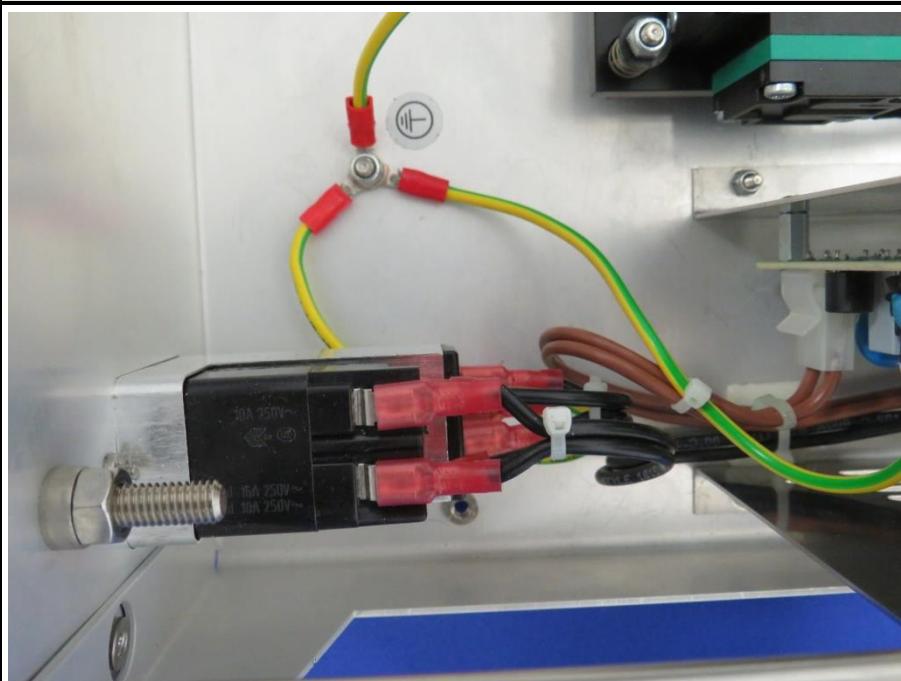
**Fluid Pump****Mains Filter**

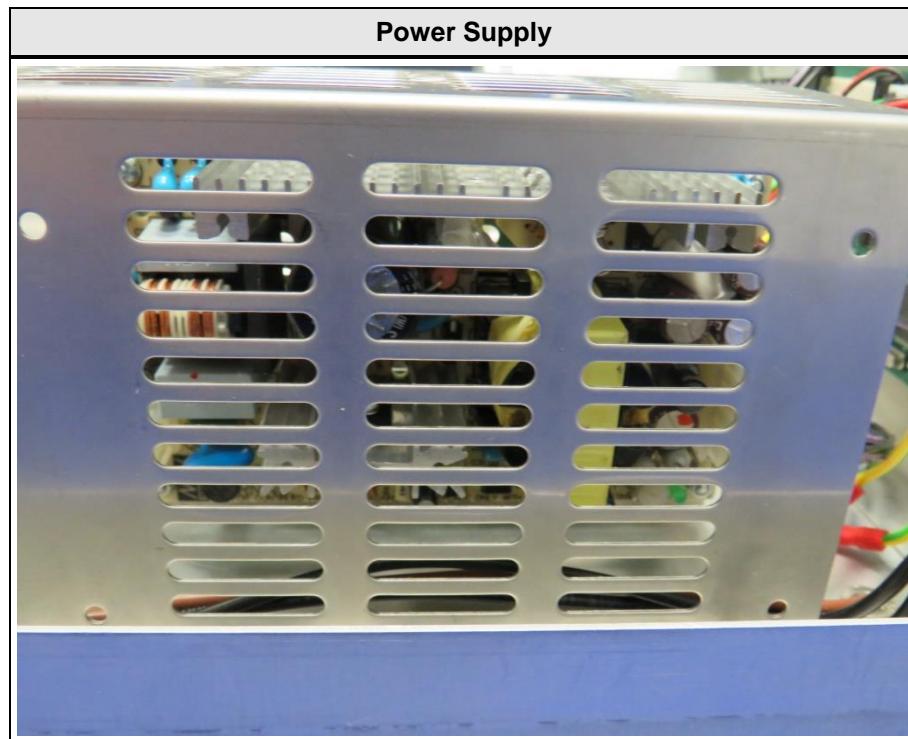

### 1.3 Equipment Photos - External



**EUT Right Side****EUT Back Side and Labels**

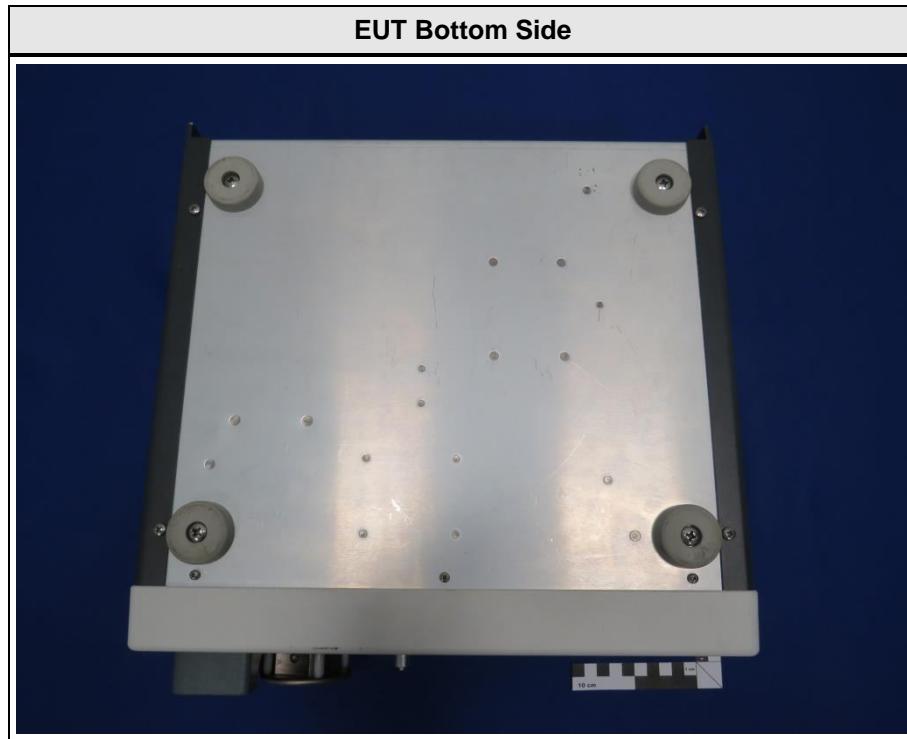

#### 1.4 Support Equipment

Product Type	Device	Manufacturer	Model	Comment
AE	Irrigation tubeset with multiuse RFID transponder	W.O.M. World of Medicine GmbH	T0505-01	
AE	Vacuum tubeset	W.O.M. World of Medicine GmbH	T0504-01	
AE	Mechanical Pressure gauge	Brannan	EN 837-1	
AE	Mechanical Pressure gauge	Sika	EN 837-1	
SIM	EMV Test Stand	W.O.M. World of Medicine GmbH	TestDummy I	Test stand including cavity, vacuum canister and pressure observation by mechanical pressure sensors
Description:				
AE	Auxiliary Equipment			
SIM	Simulator			
MON	Monitoring Equipment			
CBL	Connecting Cable			
Comment:				

## 1.5 Operational Modes

Mode #	Description
1	<p>Device Operation</p> <p>The device must be in operation, which can be achieved by pressing irrigation START/STOP key and suction START/STOP key respectively. Irrigation and suction pressure values can be observed on mechanical pressure gauges. The device has only one operation mode, which can be used for all kinds of testing.</p>
Comment:	

## 1.6 EUT Configuration

Configuration #	Description
1	<p>Connections</p> <ul style="list-style-type: none"><li>- Irrigation tube set inserted and connected to EMC test bench (pressure dummy)</li><li>- Vacuum tube set connected to EMC test bench (vacuum container with small leakiness / utilization of a Veress needle)</li></ul> <p>Device powered up with 120 V AC / 60 Hz.</p>
Comment:	

## 1.7 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyser in dB $\mu$ V. Any external preamplifiers used are taken into account through internal analyser settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyser. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyser (dB}\mu\text{V)} + \text{A.F. (dB/m)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dB $\mu$ V/m). The FCC limits are given in units of  $\mu$ V/m. The following formula is used to convert the units of  $\mu$ V/m to dB $\mu$ V/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 * \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

Reading + AF +21.5 dB $\mu$ V + 26 dB/m	= Net Reading = 47.5 dB $\mu$ V/m	:	Net reading - FCC limit 47.5 dB $\mu$ V/m - 57.0 dB $\mu$ V/m	= Margin = -9.5 dB
--	--------------------------------------	---	--	-----------------------

## 2 Result Summary

FCC 47 CFR Part 15B, ISED ICES-003 Issue 6				
Reference	Requirement	Reference Method	Result	Remarks
Emission				
FCC 47 CFR 15.109 ISED ICES-003, 8, 6.1	Radiated emissions	ANSI C63.4:2014	PASS	
FCC 47 CFR 15.107 ISED ICES-003, 8, 6.2	AC power line conducted emissions	ANSI C63.4:2014	PASS	
Comment:				



Possible Test Case Verdicts	
PASS	Test object does meet the requirements
FAIL	Test object does not meet the requirements
N/T	Required by standard but not tested
N/R	Not required by standard for the test object



## 2.1 Test Conditions and Results - Radiated emissions acc. to ANSI C63.4

### 2.1.1 Information

Test Information	
Reference	FCC 47 CFR 15.109, ISED ICES-003, 8, 6.1
Reference method	ANSI C63.4:2014 Section 8
Equipment class	Class B
Equipment type	Table top
Highest internal frequency [MHz]	16
Measurement range	30 MHz to 1 GHz
Temperature [°C]	26 °C
Humidity [%]	40 %
Operator	Ruslan Colbasiuc
Date	2019-06-27

### 2.1.2 Setup

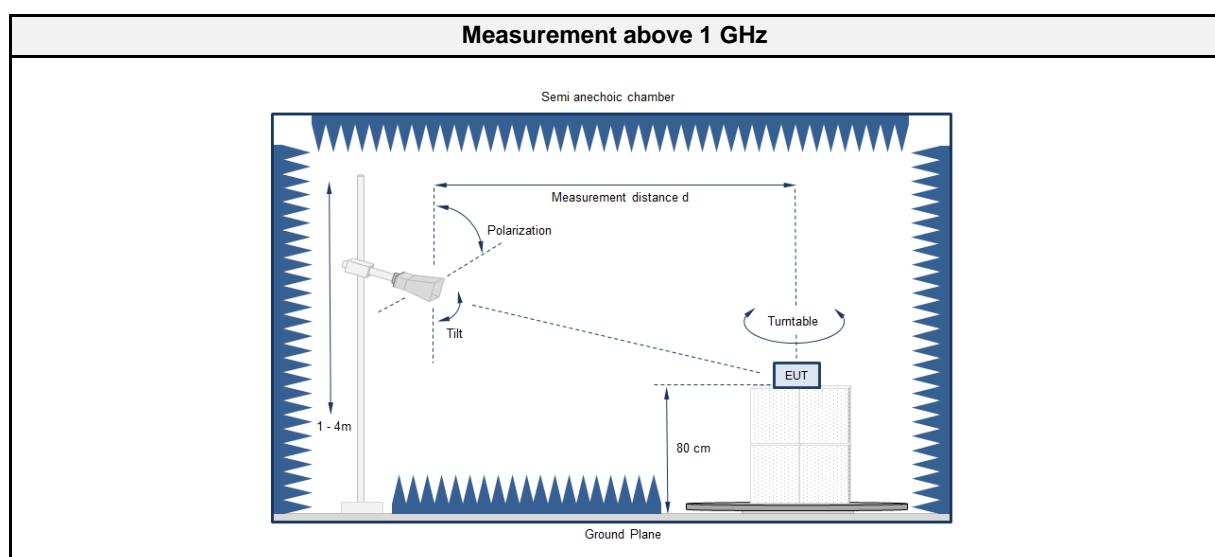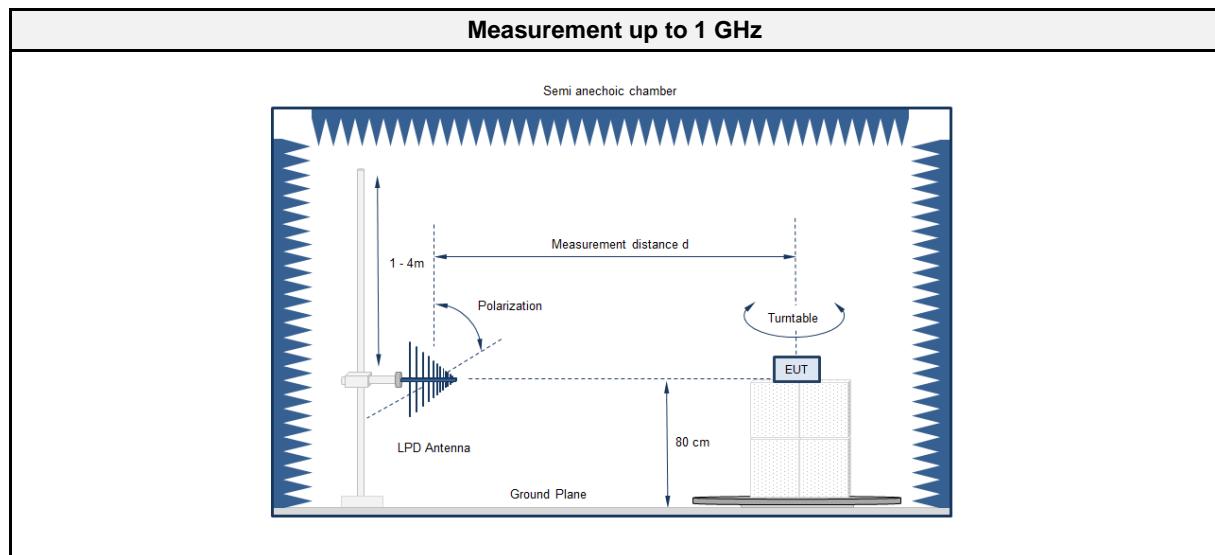

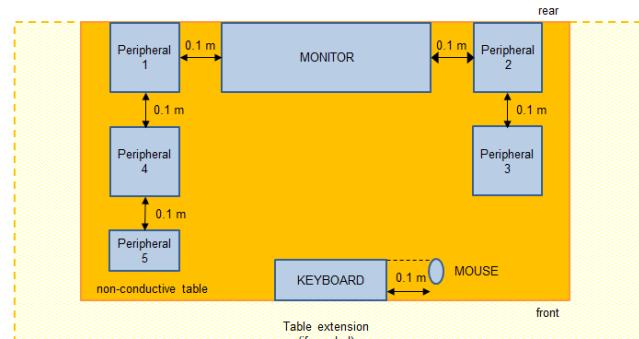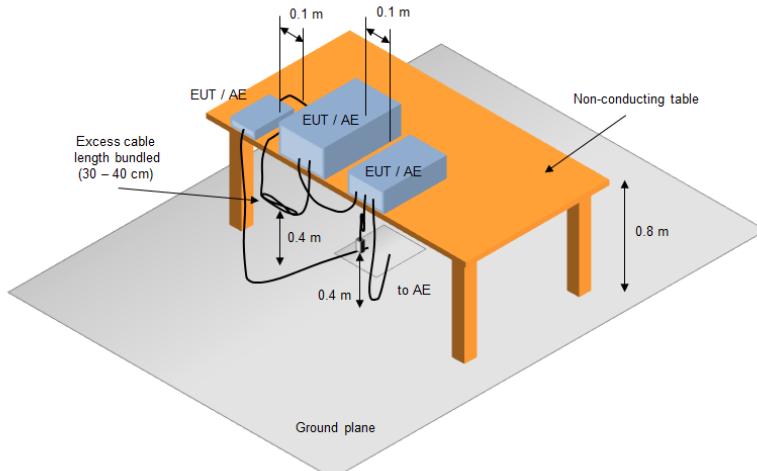**Equipment placement - Table top**

**Test Setup**

**2.1.3 Equipment**
**Test Software**

Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	Radimation	2016.1.10

**Test Equipment**

Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic chamber	Frankonia	AC6	EF00910	2017-03	2020-03
TRILOG Broadband Antenna	Schwarzbeck	VULB 9162 (30MHz - 7GHz, 100W)	EF00978	2016-11	2019-11
EMI Test Receiver	Rohde & Schwarz Vertriebs GmbH	ESU26	EF00887	2018-08	2019-08

#### 2.1.4 Procedure

<b>Exploratory measurement</b>
<ol style="list-style-type: none"> <li>1. The EUT was placed on a non-conductive table at a height of 0.8m.</li> <li>2. The EUT and support equipment, if needed, were set up to simulate typical usage.</li> <li>3. Cables, of type and length specified by the manufacturer, were connected to at least one port of each type and were terminated by a device or simulating load of actual usage.</li> <li>4. The antenna was placed at a distance of 3 or 10 m.</li> <li>5. The received signal was monitored at the measurement receiver.</li> <li>6. This procedure has to be performed in both antenna polarizations, horizontal and vertical.</li> <li>7. The arrangement of the equipment with the maximum emission level is shown on the setup picture at item 1.3</li> </ol>

<b>Final measurement</b>
<ol style="list-style-type: none"> <li>1. The EUT was placed on a 0.8 m non-conductive table at a 3 m distance from the receive antenna. The antenna output was connected to the measurement receiver.</li> <li>2. A biconical antenna was used for the frequency range 30 – 200 MHz, a logarithmic periodical antenna was used for the frequency range from 200 – 1000 MHz. Above one 1 GHz a Double Ridged Broadband Horn antenna was used. The antenna was placed on an adjustable height antenna mast.</li> <li>3. The EUT and cable arrangement were based on the exploratory measurement results.</li> <li>4. Emissions were maximized at each frequency by rotating the EUT and adjusting the receive antenna height and polarization. The maximum values were recorded.</li> <li>5. The test data of the worst-case conditions were recorded and shown on the next pages.</li> </ol>

#### 2.1.5 Limits



<b>Class B @ 3 m</b>		
Frequency [MHz]	Detector	Limit [dB $\mu$ V/m]
30 - 88	Quasi-peak	40
88 - 216	Quasi-peak	43.5
216 - 960	Quasi-peak	46
960 - 1000	Quasi-peak	54
> 1000	Peak Average	74 54

<b>Class A @ 10 m</b>		
Frequency [MHz]	Detector	Limit [dB $\mu$ V/m]
30 - 88	Quasi-peak	39
88 - 216	Quasi-peak	43.5
216 - 960	Quasi-peak	46.5
960 - 1000	Quasi-peak	49.5
> 1000	Peak Average	69.5 49.5

#### 2.1.6 Results

<b>Test Results</b>			
Operational mode	EUT Configuration	Verdict	Remark
1	1	PASS	

## 2.1.7 Setup Photos

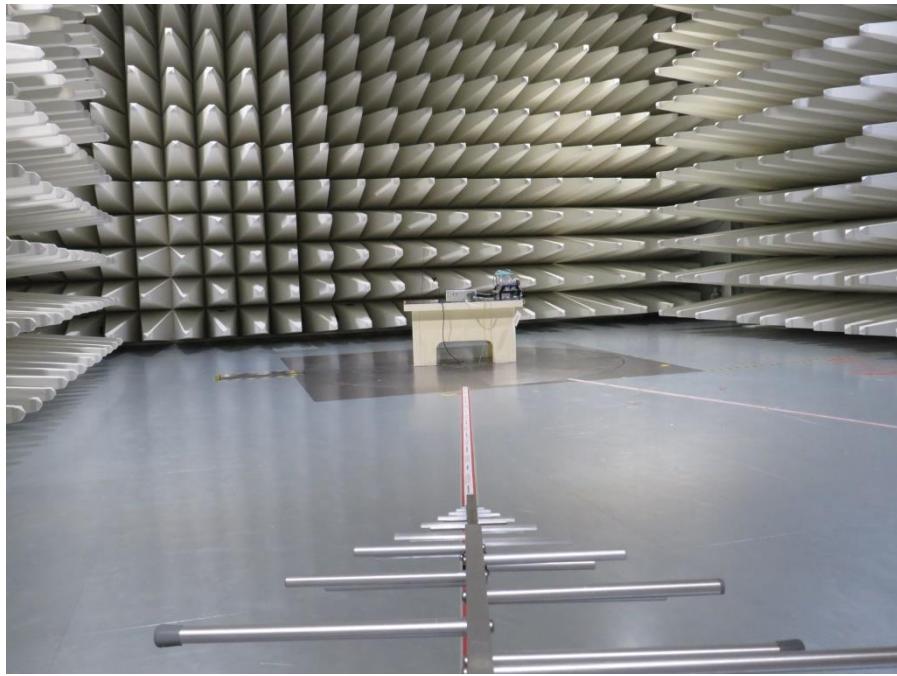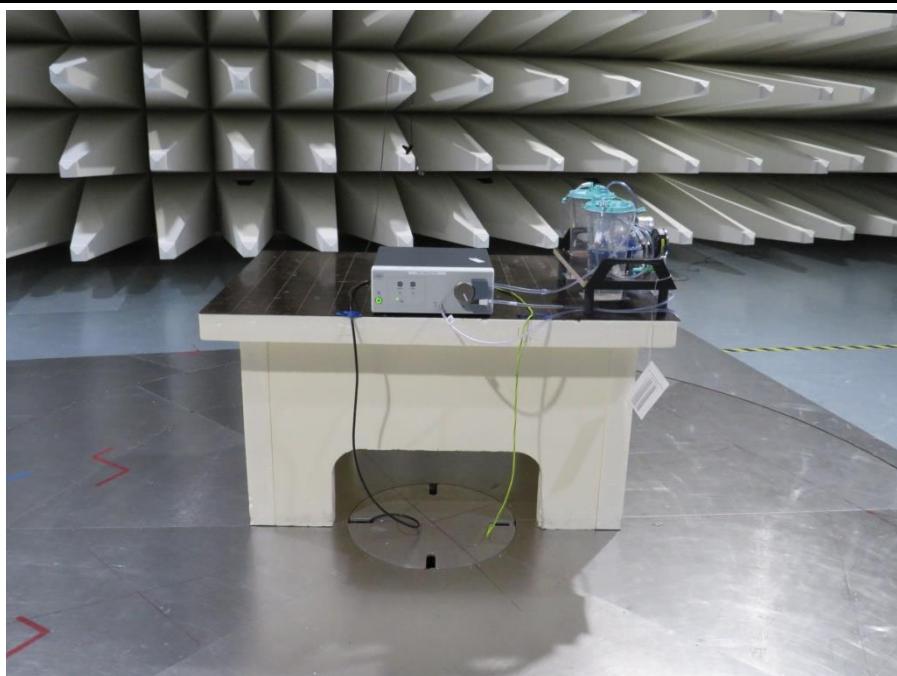**Test Setup Picture 1****Test Setup Picture 2**


## 2.1.8 Records

### Radiated emissions according to FCC 47 CFR 15 Subpart B

Project number: G0M-1806-7459

Applicant: W.O.M. WORLD OF MEDICINE GmbH  
 EUT Name: The device PP120 is a pump providing irrigation and suction function for laparoscopy  
 Model: PP120  
 Test Site: Eurofins Product Service GmbH  
 Operator: Mr. Colbasiuc  
 Test Conditions: Tnom: 26°C, Unom: 120 VAC / 60 Hz  
 Antenna: Schwarzbeck VULB 9162, Vertical  
 Measurement distance: 10 m converted to 3 m  
 Mode: 1  
 Test Date: 2019-06-27  
 Note:

Index 1

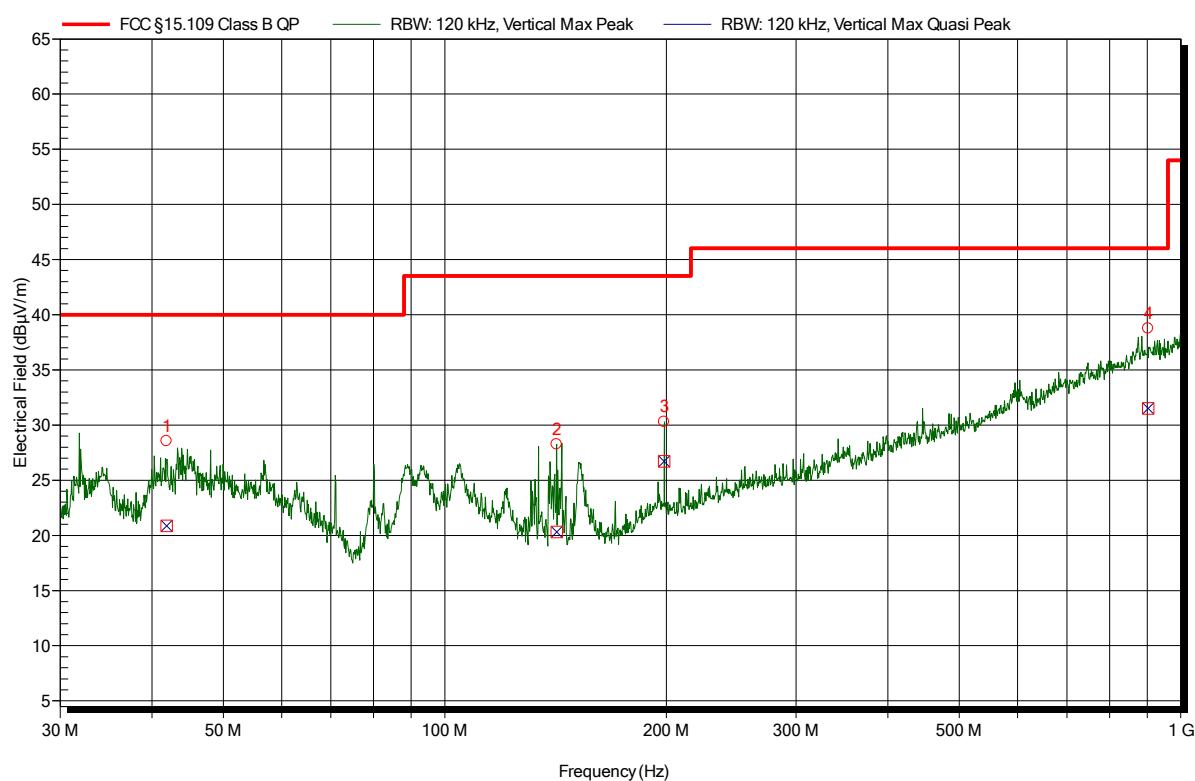


Peak Number	Frequency	Quasi-Peak	Quasi-Peak	Quasi-Peak	Quasi-Peak	Angle	Height
		Limit	Difference	Status			
1	41.88 MHz	20.9 dB $\mu$ V/m	40 dB $\mu$ V/m	-19.1 dB	Pass	0 Degree	1 m
2	141.87 MHz	20.3 dB $\mu$ V/m	43.5 dB $\mu$ V/m	-23.2 dB	Pass	0 Degree	1 m
3	198.63 MHz	26.7 dB $\mu$ V/m	43.5 dB $\mu$ V/m	-16.8 dB	Pass	0 Degree	1 m
4	902.88 MHz	31.5 dB $\mu$ V/m	46 dB $\mu$ V/m	-14.5 dB	Pass	0 Degree	1 m

**Radiated emissions according to FCC 47 CFR 15 Subpart B**

Project number: G0M-1806-7459

Applicant: W.O.M. WORLD OF MEDICINE GmbH  
 EUT Name: The device PP120 is a pump providing irrigation and suction function for laparoscopy  
 Model: PP120  
 Test Site: Eurofins Product Service GmbH  
 Operator: Mr. Colbasieuc  
 Test Conditions: Tnom: 26°C, Unom: 120 VAC / 60 Hz  
 Antenna: Schwarzbeck VULB 9162, Horizontal  
 Measurement distance: 10 m converted to 3 m  
 Mode: 1  
 Test Date: 2019-06-27  
 Note:

Index 2

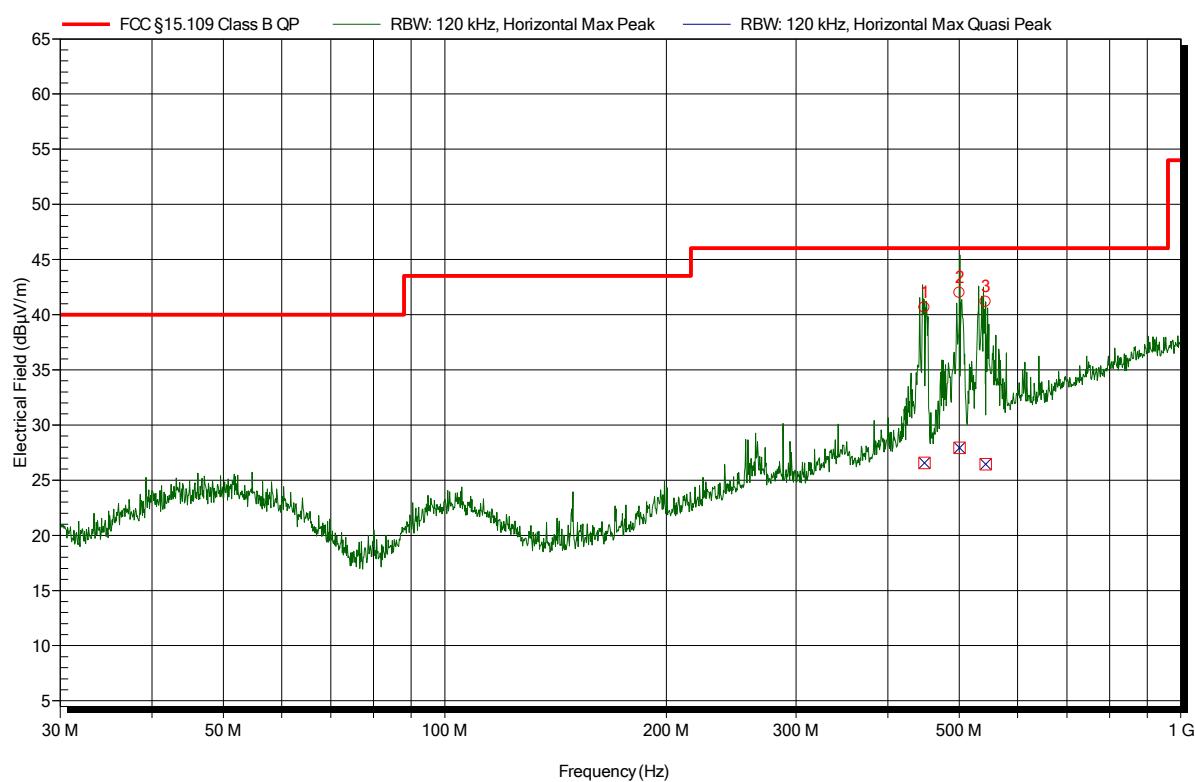



Peak Number	Frequency	Quasi-Peak	Quasi-Peak	Quasi-Peak	Quasi-Peak	Angle	Height
		Limit	Difference	Status			
1	448.542 MHz	26.6 dB $\mu$ V/m	46 dB $\mu$ V/m	-19.5 dB	Pass	160 Degree	1 m
2	500.49 MHz	27.9 dB $\mu$ V/m	46 dB $\mu$ V/m	-18.1 dB	Pass	160 Degree	1 m
3	542.724 MHz	26.5 dB $\mu$ V/m	46 dB $\mu$ V/m	-19.6 dB	Pass	160 Degree	1 m

## 2.2 Test Conditions and Results - Conducted emissions acc. to ANSI C63.4

### 2.2.1 Information

Test Information	
Reference	FCC 47 CFR 15.107, ISED ICES-003, 8, 6.2
Reference method	ANSI C63.4:2014 Section 12
Measurement range	150 kHz to 30 MHz
Equipment class	Class B
Equipment type	Table top
Temperature [°C]	25 °C
Humidity [%]	40 %
Operator	Ruslan Colbasiuc
Date	2019-06-27

### 2.2.2 Setup

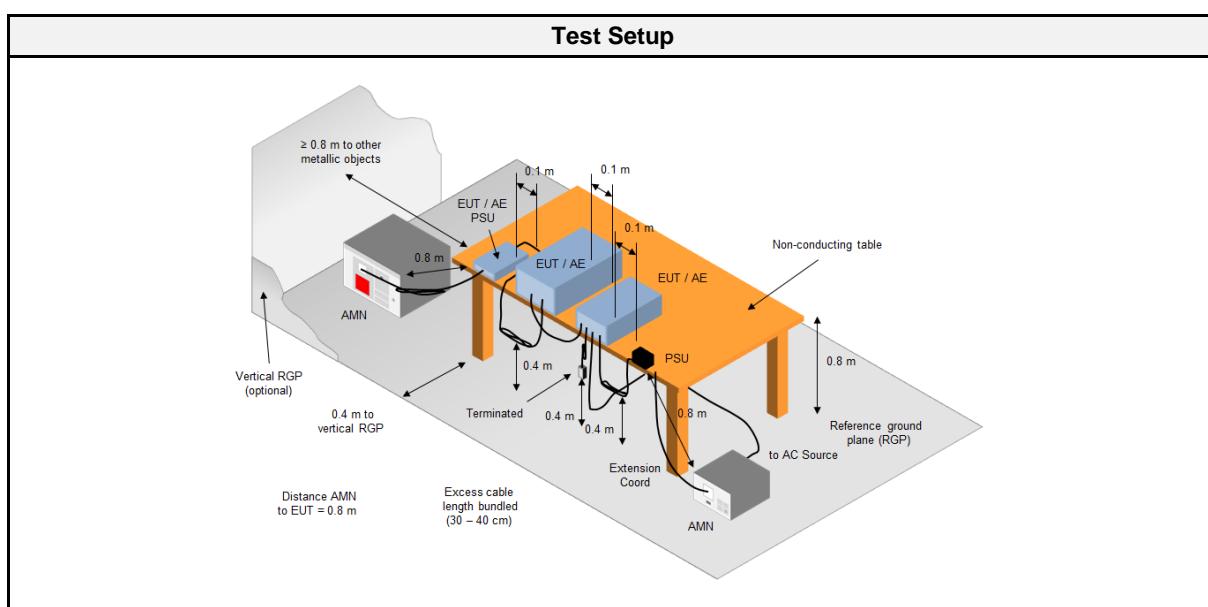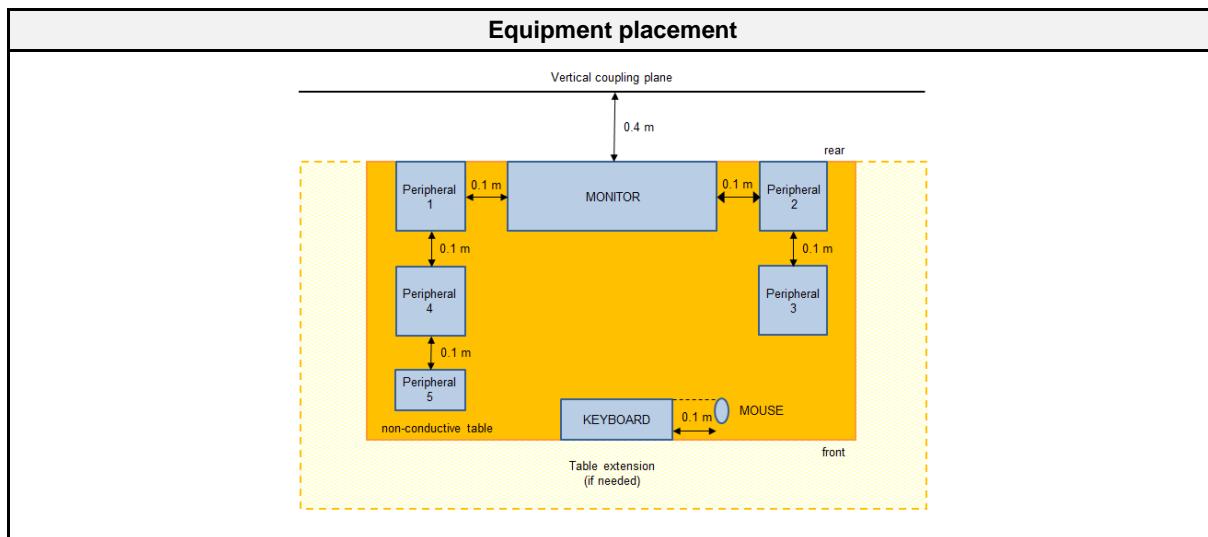

### 2.2.3 Equipment

<b>Test Software</b>			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	Radimation	2016.1.10

<b>Test Equipment</b>					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
AMN	Schwarzbeck	NSLK 8128	EF00975	2017-07	2019-07
Pulse Limiter	R&S	ESH3-Z2	EF01063	2018-07	2019-07
EMI Test Receiver	R&S	ESU26	EF00887	2018-08	2019-08

### 2.2.4 Procedure

<b>Exploratory measurement</b>
<ol style="list-style-type: none"> <li>1. The EUT was placed on a non conductive table 0.8 m above the reference ground plane and 0.4 m away from the vertical conducting plane (ANSI C63.4: 2014 item 7.3.1)</li> <li>2. The power cord that is normally supplied or recommended by the manufacturer was connected to the LISN.</li> <li>3. The distance between the outer edge of the EUT and the LISN shall be set to 0.8 m. A longer power cord shall be bundled to this length (bundling shall not exceed 40 cm in length).</li> <li>4. The LISN measurement port was connected to a measurement receiver</li> <li>5. I/O cables were bundled not longer than 0.4 m</li> <li>6. Measurement was performed in the frequency range 0.15 – 30MHz on each current-carrying conductor</li> <li>7. To maximize the emissions the cable positions were manipulated</li> <li>8. The worst configuration of EUT and cables is shown on a test setup picture at item 1.3</li> </ol>

<b>Final measurement</b>
<ol style="list-style-type: none"> <li>1. The EUT was placed on a non conductive table 0.8 m above the reference ground plane and 0.4 m away from the vertical conducting plane (ANSI C63.4: 2014 item 7.3.1)</li> <li>2. The power cord that is normally supplied or recommended by the manufacturer was connected to the LISN.</li> <li>3. The distance between the outer edge of the EUT and the LISN shall be set to 0.8 m. A longer power cord shall be bundled to this length (bundling shall not exceed 40 cm in length).</li> <li>4. The LISN measurement port was connected to a measurement receiver</li> <li>5. The EUT and cable arrangement were based on the exploratory measurement results</li> <li>6. The test data of the worst-case conditions were recorded and shown on the next pages</li> </ol>

### 2.2.5 Limits

<b>Class B</b>		
Frequency [MHz]	Quasi-peak Limit [dB $\mu$ V]	Average Limit [dB $\mu$ V]
0.15 - 0.5	66 - 56 *	56 - 46 *
0.5 - 5	56	46
5 - 30	60	50


\* Decreases with the logarithm of the frequency

### 2.2.6 Results

<b>AC power line conducted emissions</b>					
Port	Coupling	Operational mode	EUT Configuration	Verdict	Remark
Mains	AMN	1	1	PASS	

Test Report No.: G0M-1806-7459-EF0115B-V01

### 2.2.7 Setup Photos

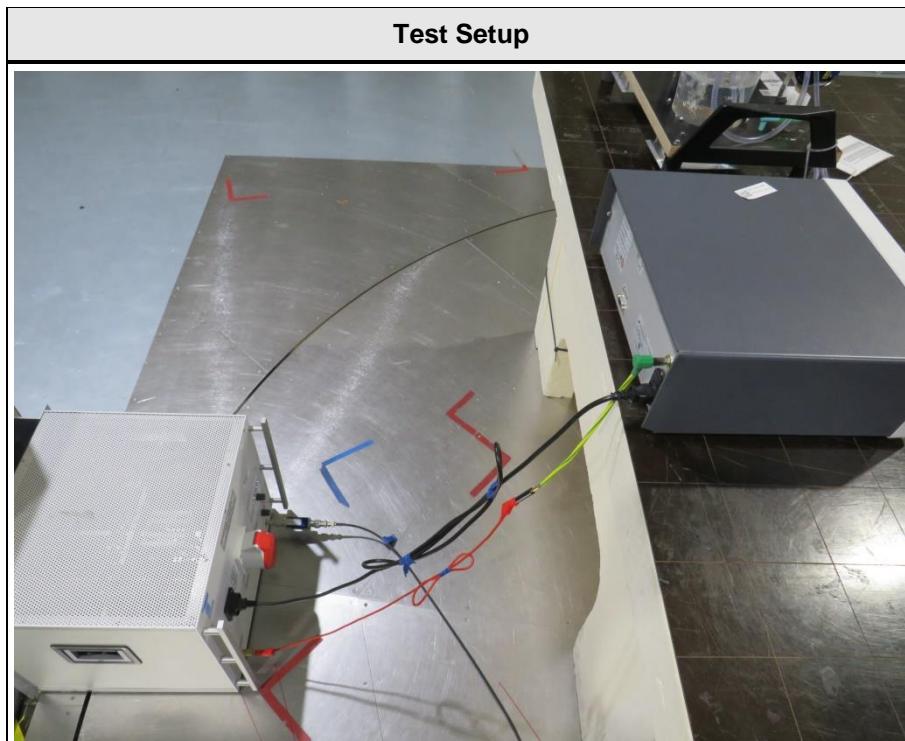


## 2.2.8 Records

### Conducted emissions according to FCC 47 CFR 15 Subpart B

Project number: G0M-1806-7459

Applicant: W.O.M. WORLD OF MEDICINE GmbH  
 EUT Name: The device PP120 is a pump providing irrigation and suction function for laparoscopy  
 Model: PP120  
 Test Site: Eurofins Product Service GmbH  
 Operator: Mr. Colbasiuc  
 Test Conditions: Tnom: 26°C, Unom: 120 VAC / 60 Hz  
 LISN: Schwarzbeck NSLK 8128 (N)  
 Mode: 1  
 Test Date: 2019-06-27  
 Note:

Index 3

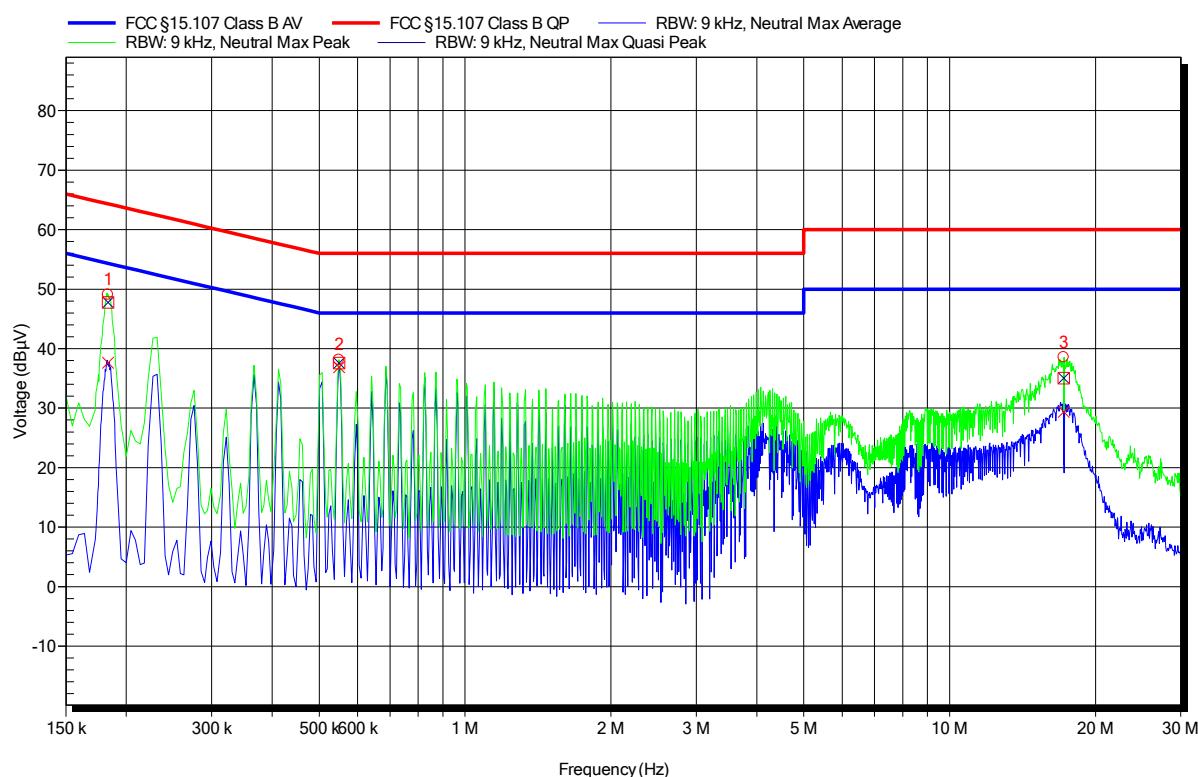

Peak Number	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
1	183.3 kHz	47.8 dB $\mu$ V	64.3 dB $\mu$ V	-16.6 dB	Pass
2	549.15 kHz	37.6 dB $\mu$ V	56 dB $\mu$ V	-18.4 dB	Pass
3	17.206 MHz	35 dB $\mu$ V	60 dB $\mu$ V	-25.0 dB	Pass


Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status
1	183.3 kHz	37.6 dB $\mu$ V	54.3 dB $\mu$ V	-16.7 dB	Pass
2	549.15 kHz	36.9 dB $\mu$ V	46 dB $\mu$ V	-9.1 dB	Pass
3	17.206 MHz	29.4 dB $\mu$ V	50 dB $\mu$ V	-20.6 dB	Pass

**Conducted emissions according to FCC 47 CFR 15 Subpart B**

Project number: G0M-1806-7459

Applicant: W.O.M. WORLD OF MEDICINE GmbH  
 EUT Name: The device PP120 is a pump providing irrigation and suction function for laparoscopy  
 Model: PP120  
 Test Site: Eurofins Product Service GmbH  
 Operator: Mr. Colbasiuc  
 Test Conditions: Tnom: 26°C, Unom: 120 VAC / 60 Hz  
 LISN: Schwarzbeck NSLK 8128 (L)  
 Mode: 1  
 Test Date: 2019-06-27  
 Note:

Index 4

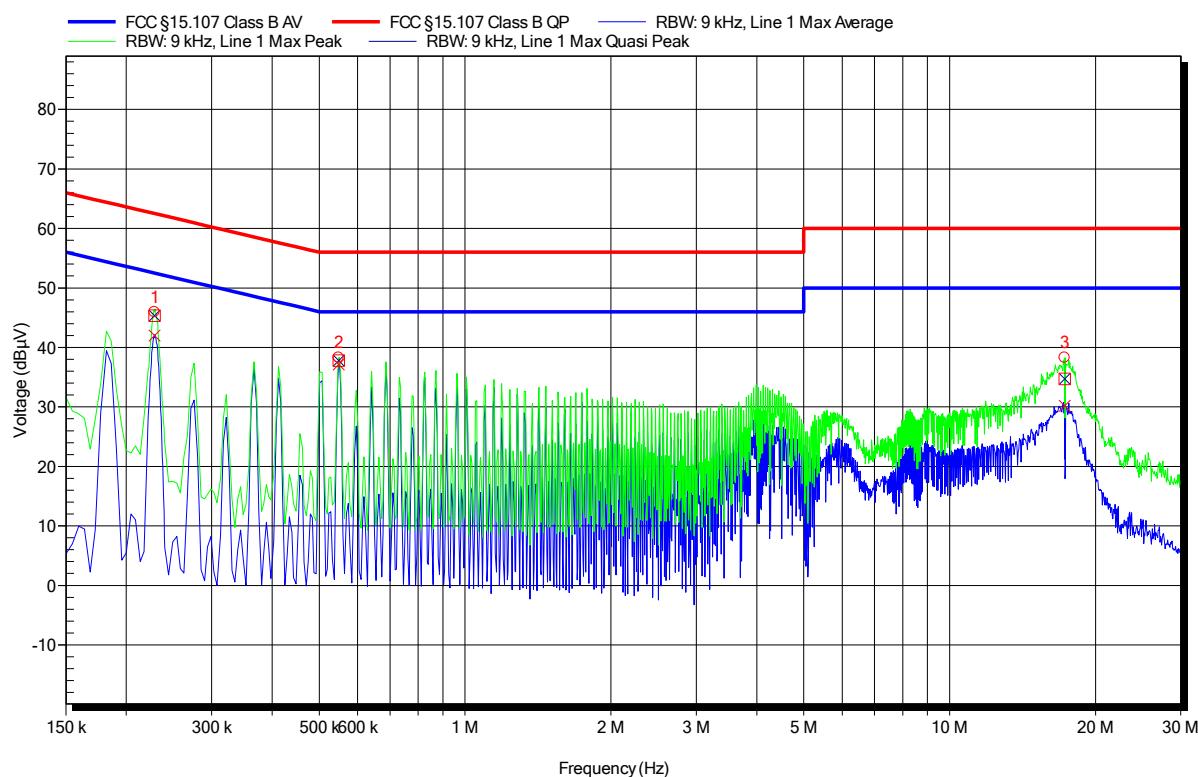

Peak Number	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status
1	228.75 kHz	45.3 dB $\mu$ V	62.5 dB $\mu$ V	-17.2 dB	Pass
2	548.7 kHz	37.8 dB $\mu$ V	56 dB $\mu$ V	-18.2 dB	Pass
3	17.287 MHz	34.7 dB $\mu$ V	60 dB $\mu$ V	-25.3 dB	Pass

Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status
1	228.75 kHz	42 dB $\mu$ V	52.5 dB $\mu$ V	-10.5 dB	Pass
2	548.7 kHz	37.1 dB $\mu$ V	46 dB $\mu$ V	-8.9 dB	Pass
3	17.287 MHz	30.2 dB $\mu$ V	50 dB $\mu$ V	-19.8 dB	Pass