

LABELING

Original Freigabeformular in TR archiviert.
Original form stored in the technical writing department.

Label sticks inside of the device

FA. Nr. ##### - ##

SN YYMMCE####

Removing this label causes loss of warranty.
10000017567 03

MAX. IRRIGATION RATE3.0 l/min

MAX. PUMPING PRESSURE450 mmHg (EU)

MAINS VOLTAGE RANGEAC 100-240 V

SUPPLY FREQUENCY50/60 Hz

POWER CONSUMPTIONAC 100 V~ 0.61 A
AC 240 V~ 0.31 A

FUSE2x T 3.15 AH
250 V, UL-recognized

YYYY-MM-DD

IP 41

LAP-Pump

W.O.M. WORLD OF MEDICINE GmbH
Salzufer 8, 10587 Berlin, Germany
Phone: +49 30 39981-550

Contains FCC ID: 2AS5K-TSHW42
Contains IC: 25004-TSHW42A
HVIN: 1430

CE 0197

TYPEPP110




SN / REFYYMMCE#### / #####

E114346
Complies with
AAMI ES60601-1
us CSA-C22.2 No. 60601-1

GS1 EAN
Datamatrix
01 / 11 / 21

(01)#####
(11)YYMMDD
(21)YYMMCE####

Issuing Agency:
GS1

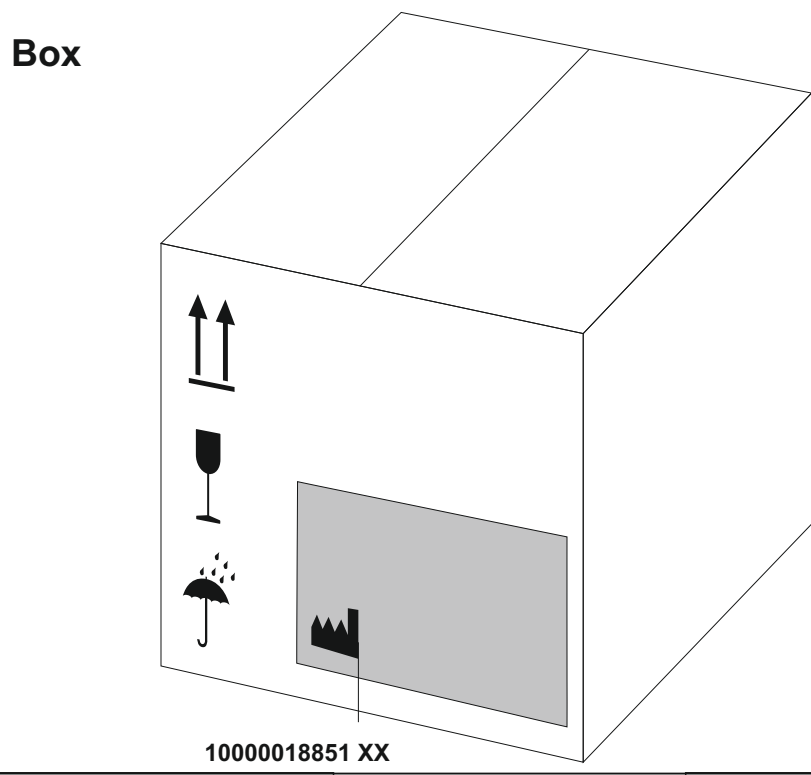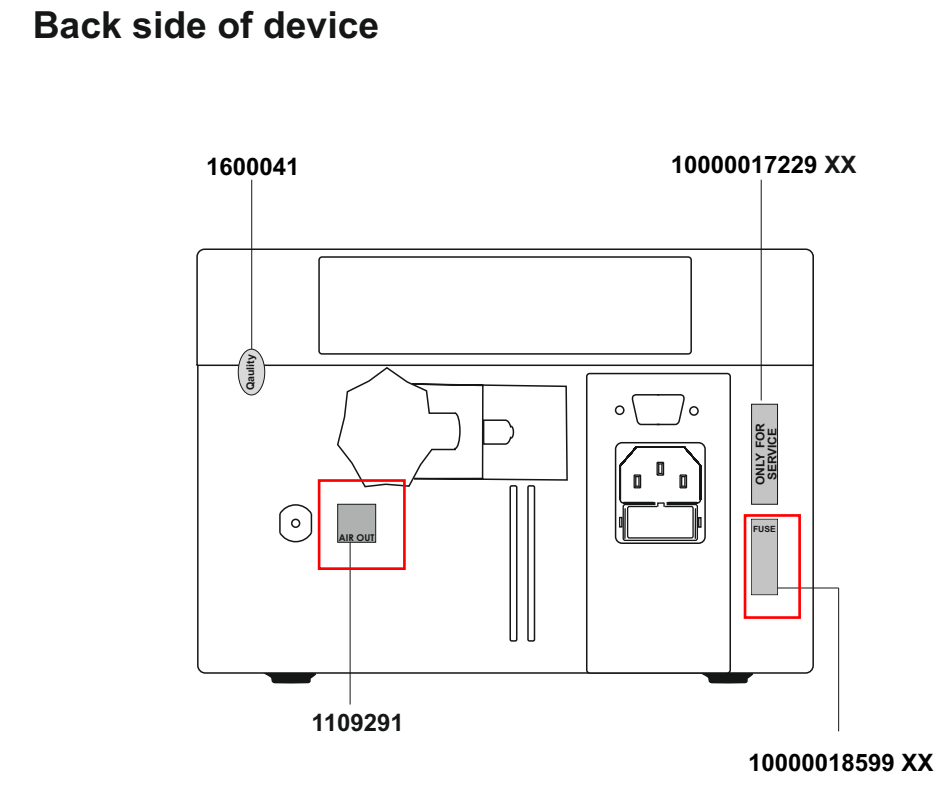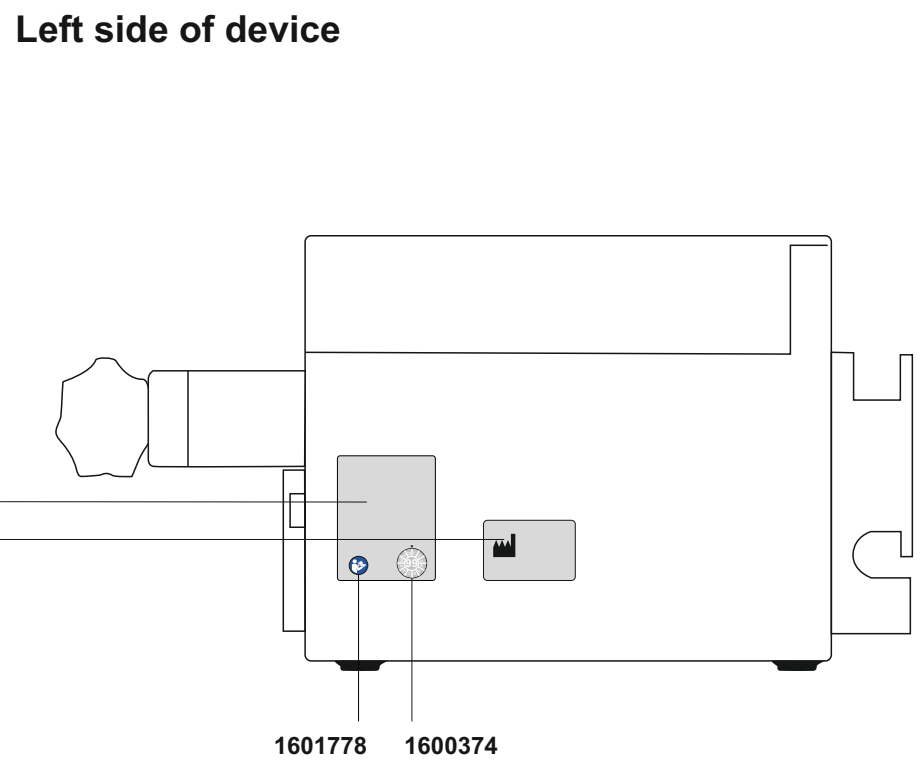

Revision history

Legend: Main Change Request(s) Technical Writing Change Request(s)		
Rev. WOM	ECR	Change
01	2017114	Position label on left side of device; added: MET symbol on device and packaging label
02	2017701	Added: MET number on device
03	2018894	Added: Label Air/Out, Fuse, RFID info on type label, symbol „NON- IONIZING RADIATION” Removed: Risk of fire, aligned with Technical Writing Dpt. templates

Product Management / Customer	Project Management (R&D)	Regulatory Affairs	WORLD OF MEDICINE / Approval		
Overview device labels PP110			W.O.M. Item number	File FMT	File CDR
			10000017567 03	10000017567 03.002.fmt	10000017567 03.002.cdr
				Name	Date
				TR	03.02.2020