

EMC TEST REPORT

FCC 47 CFR Part 15B, ISED ICES-003 Issue 6

Report Reference No	G0M-2010-9360-EF0115B-V01
Testing Laboratory	Eurofins Product Service GmbH
Address	Storkower Str. 38c 15526 Reichenwalde Germany
Accreditation	    DAkkS - Registration number : D-PL-12092-01-03 (ISED) ISED Testing Laboratory site: 3470A-3 DAkkS - Registration number : D-PL-12092-01-04 (FCC) FCC Filed Test Laboratory, Reg.-No.: 96970
Applicant	W.O.M. WORLD OF MEDICINE GmbH
Address	Salzufer 8 10587 Berlin GERMANY
Test Specification Standard(s)	47 CFR Part 15 Subpart B ISED ICES-003 Issue 6 ANSI C63.4:2014+A1:2017
Non-Standard Test Method	None
Equipment under Test (EUT):	
Product Description	Insufflator for Laparoscopy, Vessel Harvesting, Colorectal and Cardiac Procedures
Model(s)	FM300
Additional Model(s)	None
Brand Name(s)	PNEUMOCLEAR™
Hardware Version(s)	Hardware traceability is constituted by serial number of device (assembled with processor board Toradex IMX6) SN: 1902CE0537
Software Version(s)	1.1.1
Contains FCC-ID	2AS5K-TSHW42
Contains IC	25004-TSHW42A
Test Result	PASSED

Possible test case verdicts:		
required by standard but not tested	N/T	
not required by standard	N/R	
required by standard but not appl. to test object	N/A	
test object does meet the requirement	P(PASS)	
test object does not meet the requirement	F(FAIL)	
Testing:		
Date of receipt of test item	2020-09-30	
Report:		
Compiled by	Ruslan Colbasiuc	
Tested by (+ signature) (Responsible for Test)	Ruslan Colbasiuc	
Approved by (+ signature) (Deputy Head of Lab)	Jens Marquardt	
Date of Issue	2020-12-14	
Total number of pages	44	
General Remarks:		
<p>The test results presented in this report relate only to the object tested.</p> <p>The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.</p> <p>This report shall not be reproduced, except in full, without the written approval of the issuing testing laboratory.</p>		
Additional Comments:		

ABBREVIATIONS AND ACRONYMS

Acronyms	
Acronym	Description
EUT	Equipment Under Test
FCC	Federal Communications Commission
ISED	Innovation, Science and Economic Development Canada
T _{NOM}	Nominal operating temperature
V _{NOM}	Nominal supply voltage

VERSION HISTORY

Version History			
Version	Issue Date	Remarks	Revised By
01	2020-12-14	Initial Release	-

REPORT INDEX

1	Equipment (Test Item) Under Test.....	6
1.1	Equipment Ports.....	7
1.2	Equipment Photos - Internal.....	8
1.3	Equipment Photos - External.....	17
1.4	Support Equipment.....	23
1.5	Operational Modes.....	24
1.6	EUT Configuration.....	25
1.7	Sample emission level calculation.....	26
2	Result Summary.....	27
2.1	Test Conditions and Results - Radiated emissions acc. to ANSI C63.4.....	28
2.2	Test Conditions and Results - Conducted emissions acc. to ANSI C63.4.....	37



1 Equipment (Test Item) Under Test


Description	Insufflator for Laparoscopy, Vessel Harvesting, Colorectal and Cardiac Procedures	
Model	FM300	
Additional Model(s)	None	
Brand Name(s)	PNEUMOCLEAR™	
Serial Number(s)	1902CE0537/ÄV2018-143	
Hardware Version(s)	Hardware traceability is constituted by serial number of device (assembled with processor board Toradex IMX6) SN: 1902CE0537	
Software Version(s)	1.1.1	
Contains FCC-ID	2AS5K-TSHW42	
Contains IC	25004-TSHW42A	
Class	Class B	
Equipment type	Table top	
Highest internal frequency [MHz]	806	
Dimension (cm)	31.8 X 14.9 X 42.9	
Radio Module	Type	RFID Module
	Model	TS-HW42
	Manufacturer	GiS mbH
	FCC-ID	2AS5K-TSHW42
	IC	25004-TSHW42A
Supply Voltage	V _{NOM}	120 VAC / 60 Hz
Manufacturer	W.O.M. WORLD OF MEDICINE GmbH Salzufer 8 10587 Berlin GERMANY	



1.1 Equipment Ports



Name	Type	Attributes	Comment
Mains Connection	AC	Count: 1 Direction: In Service only: No	
SIDNE	IO	Count: 1 Direction: IO Service only: No	USB Type B
USB	IO	Count: 2 Direction: IO Service only: Yes	USB Type A USB Type Mini B
Tube Heater	DC;IO	Count: 1 Direction: IO Service only: No	
Gas Connection	NE	Count: 1 Direction: In Service only: No	
Potential Equalization Plug	PE	Count: 1 Direction: Out Service only: No	
Description:			
AC	AC mains power input/output port		
DC	DC power input/output port		
BAT	DC power input port connected to external battery		
IO	Input/Output port		
TP	Telecommunication port		
NE	Non-electrical port		
PE	Potential Equalization Port		


1.2 Equipment Photos - Internal

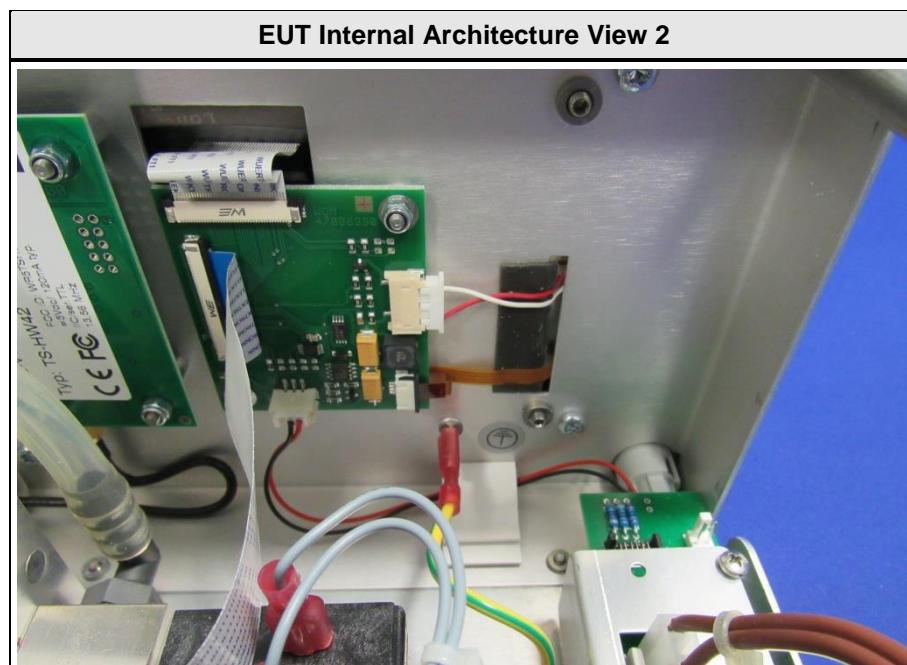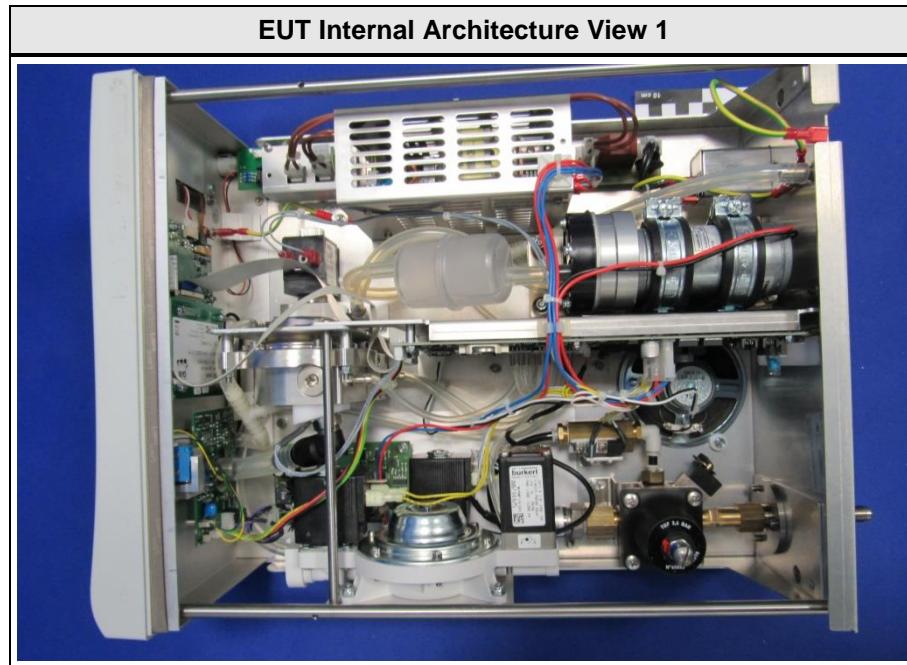


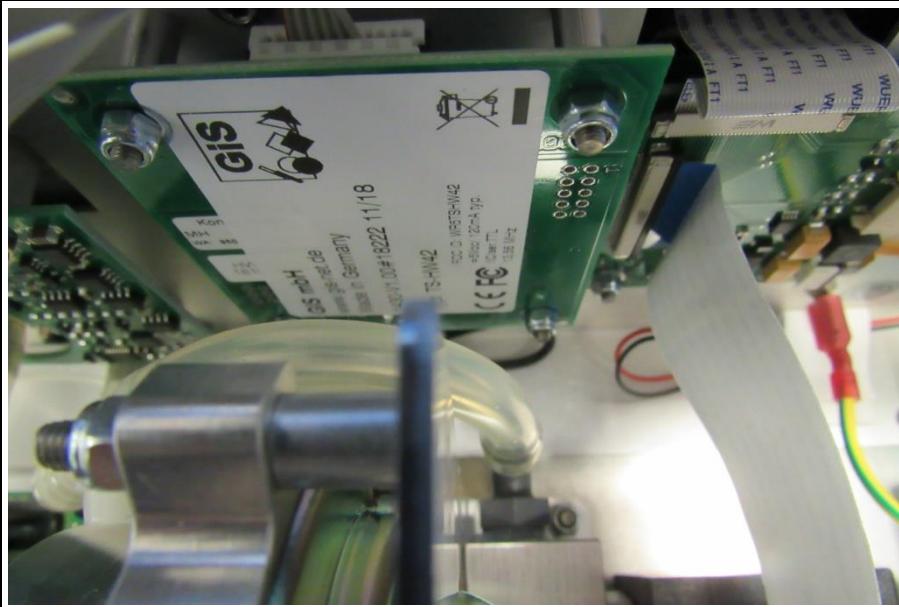EUT Internal Architecture View 3**EUT Internal Architecture View 4**

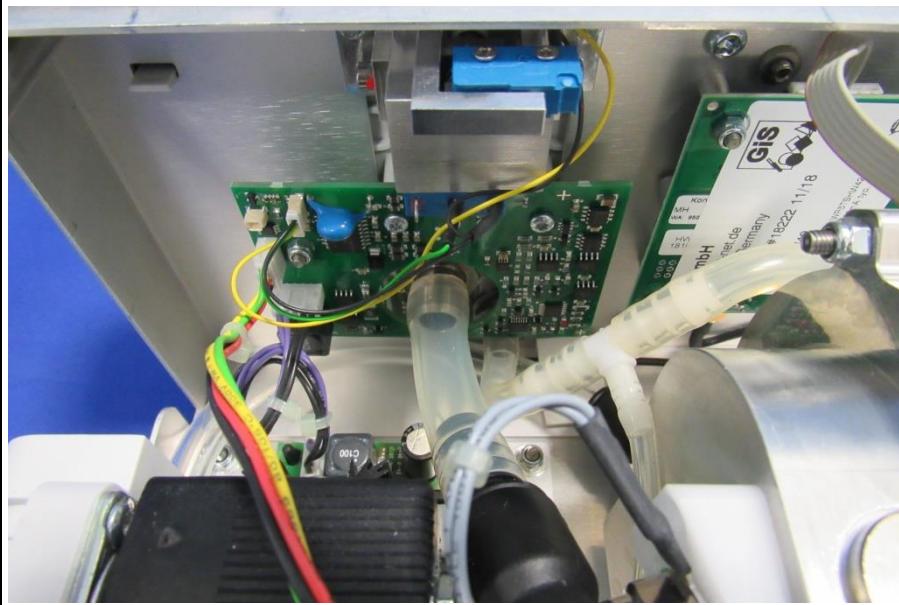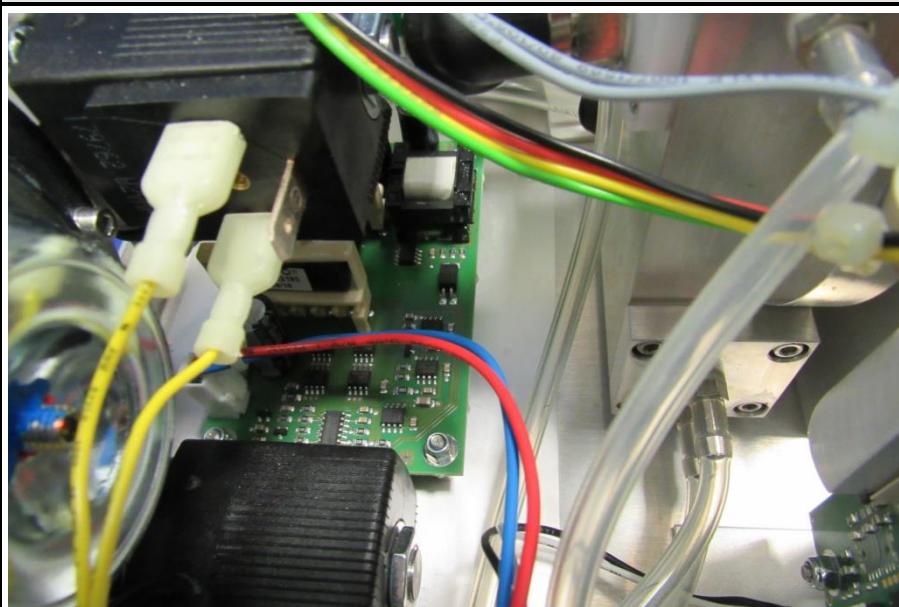
EUT Internal Architecture View 5**EUT Internal Architecture View 6**

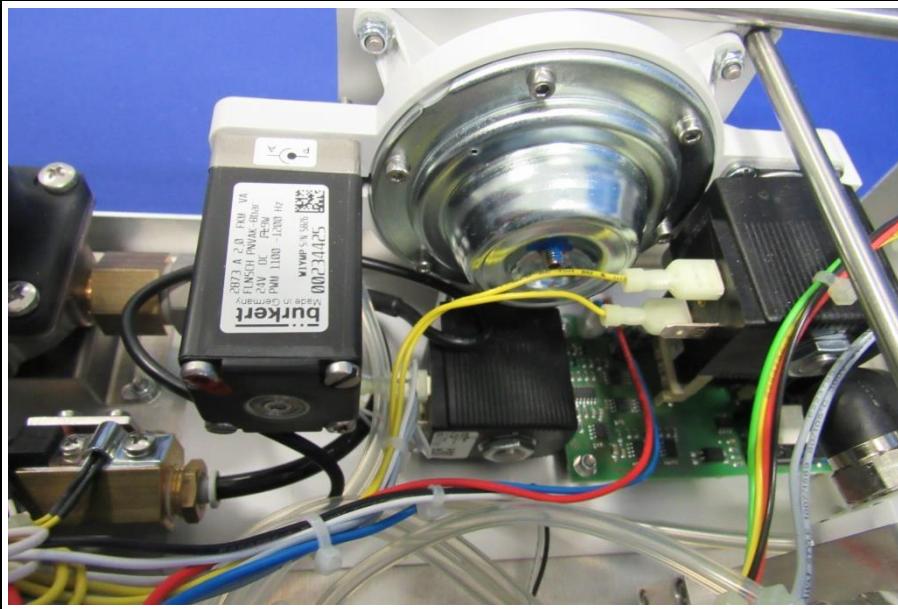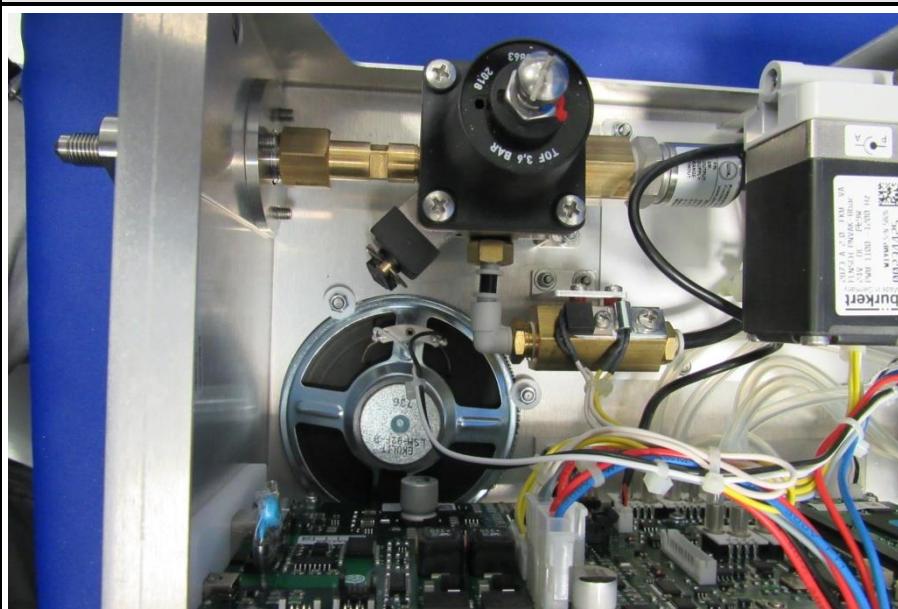EUT Internal Architecture View 7**EUT Internal Architecture View 8**

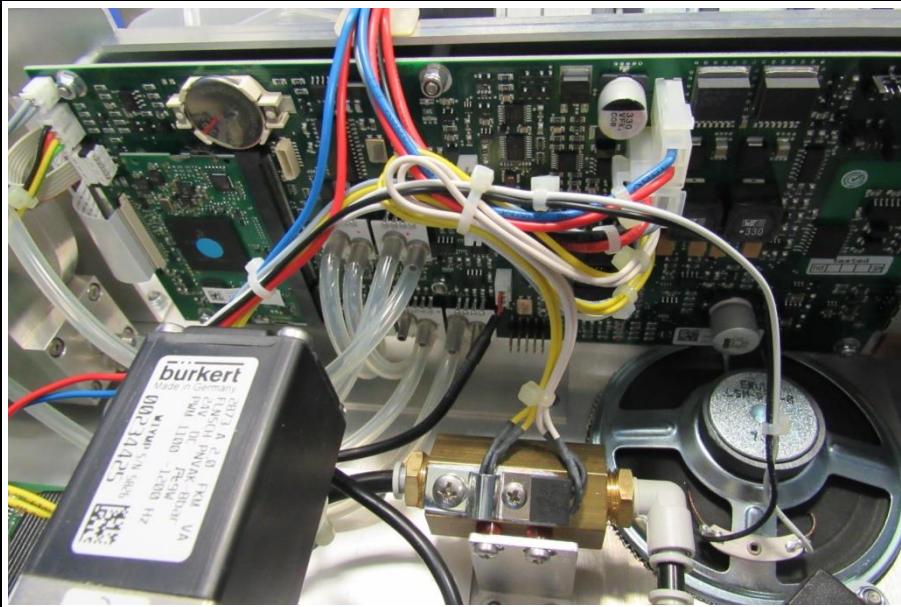
EUT Internal Architecture View 9**EUT Internal Architecture View 10**

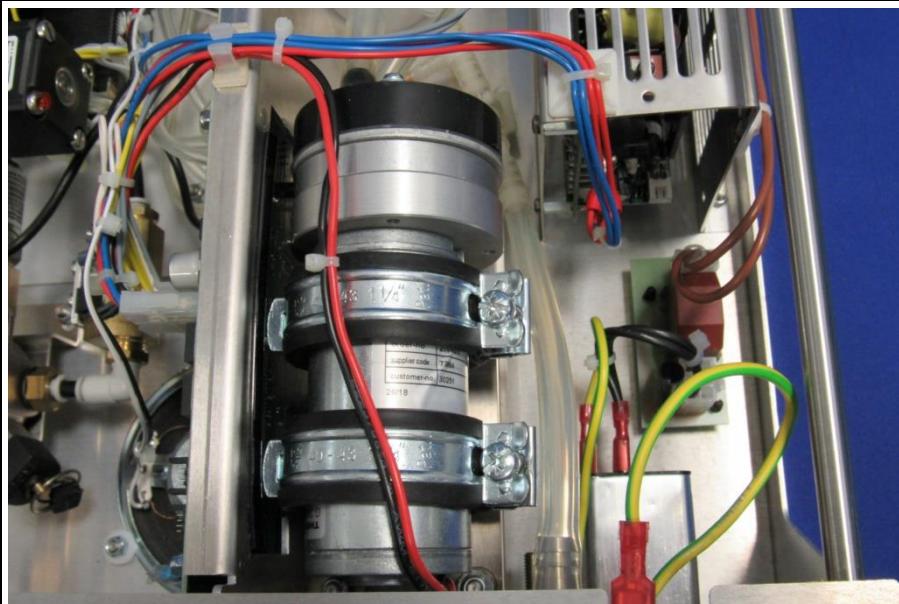EUT Internal Architecture View 11**EUT Internal Architecture View 12**

EUT Internal Architecture View 13


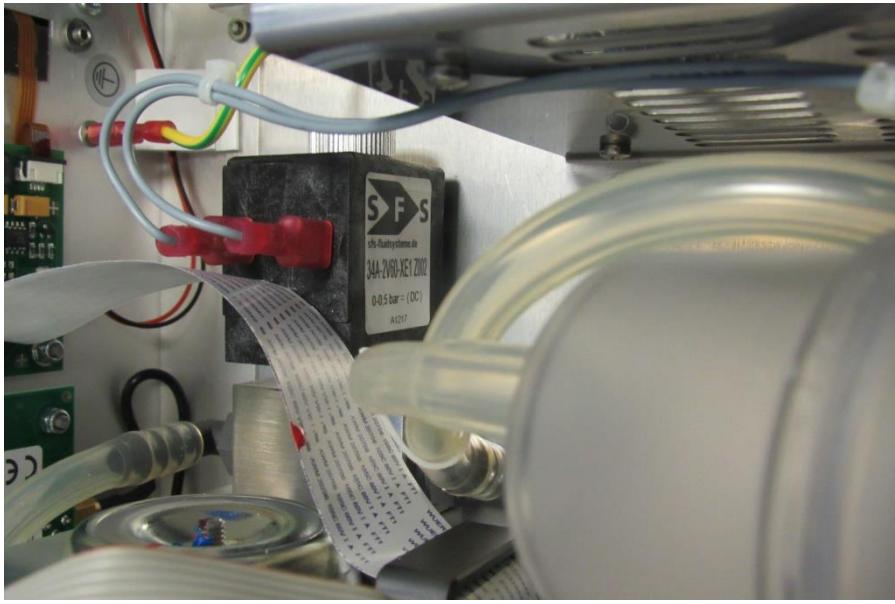




EUT Internal Architecture View 14

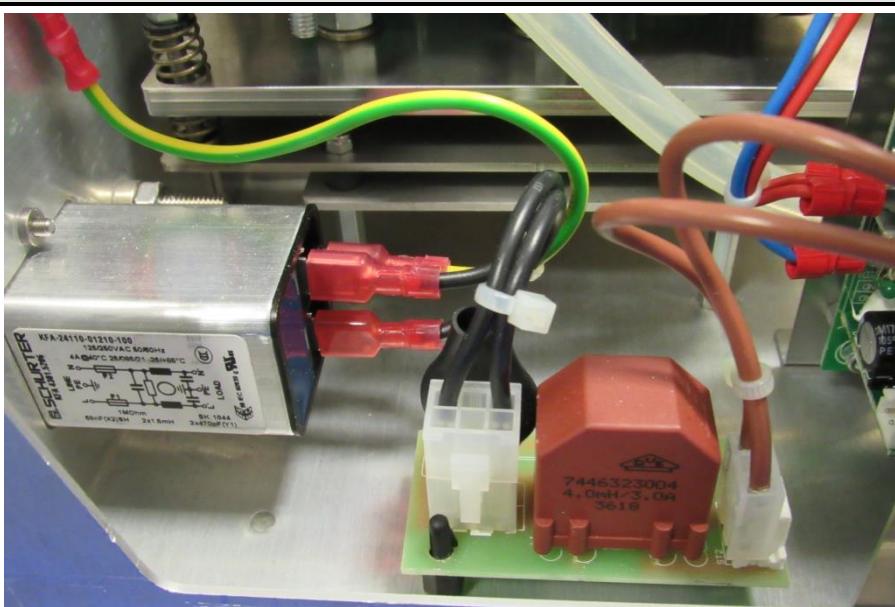


Test Report No.: G0M-2010-9360-EF0115B-V01

Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

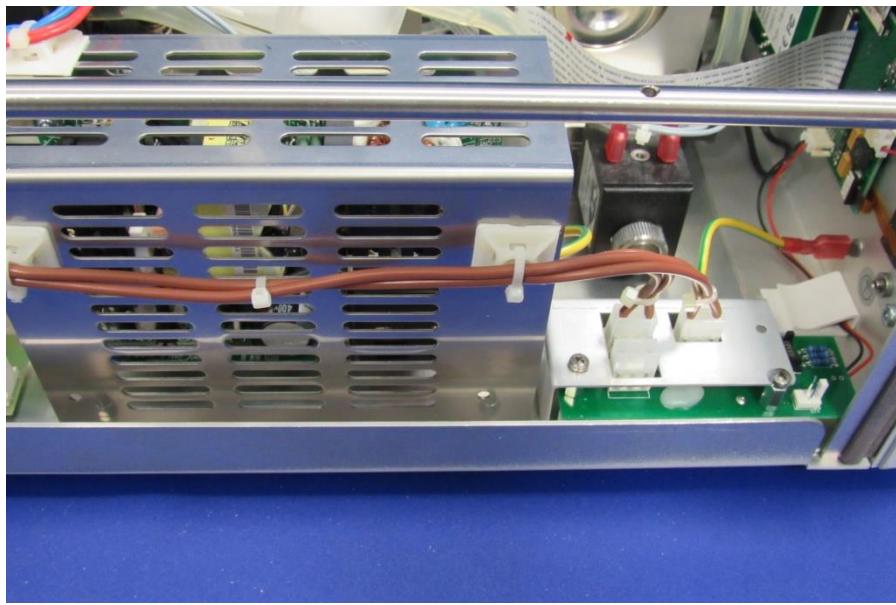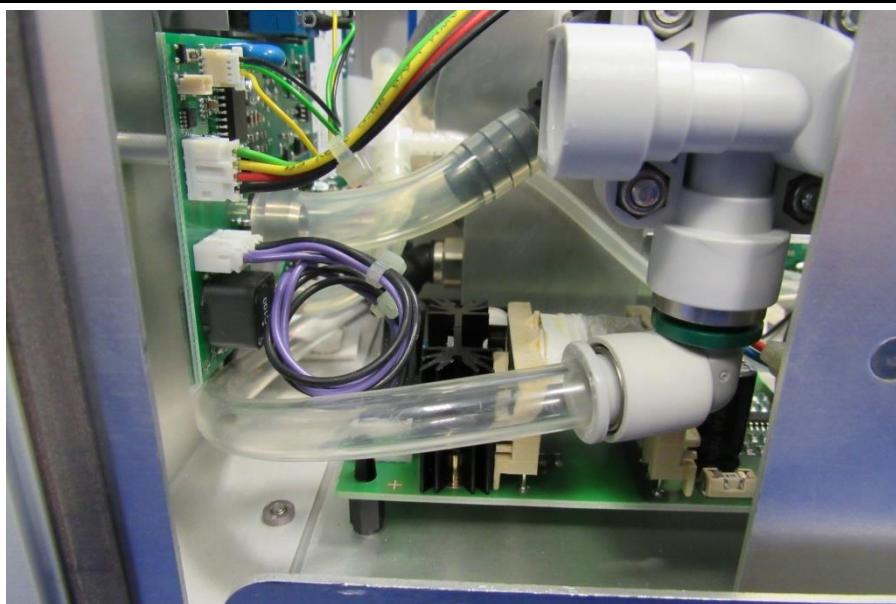EUT Internal Architecture View 15**EUT Internal Architecture View 16**

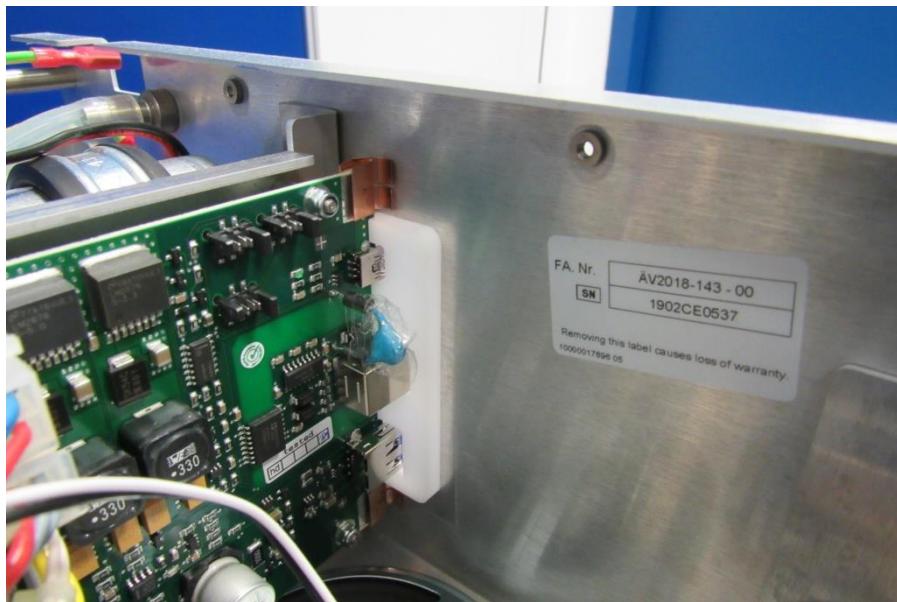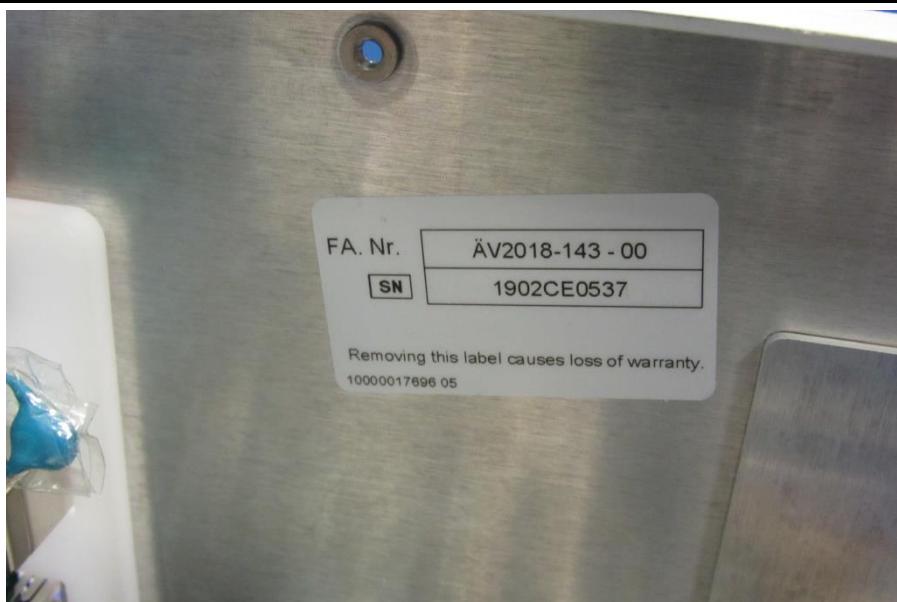EUT Internal Architecture View 17**EUT Internal Architecture View 18**


1.3 Equipment Photos - External

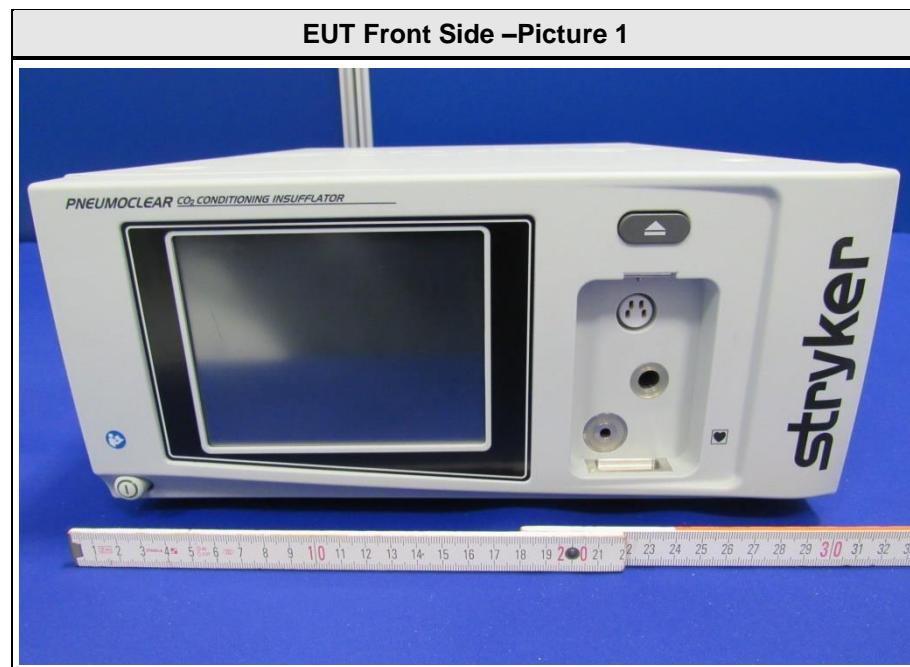


EUT Top Side View




EUT Left Side View

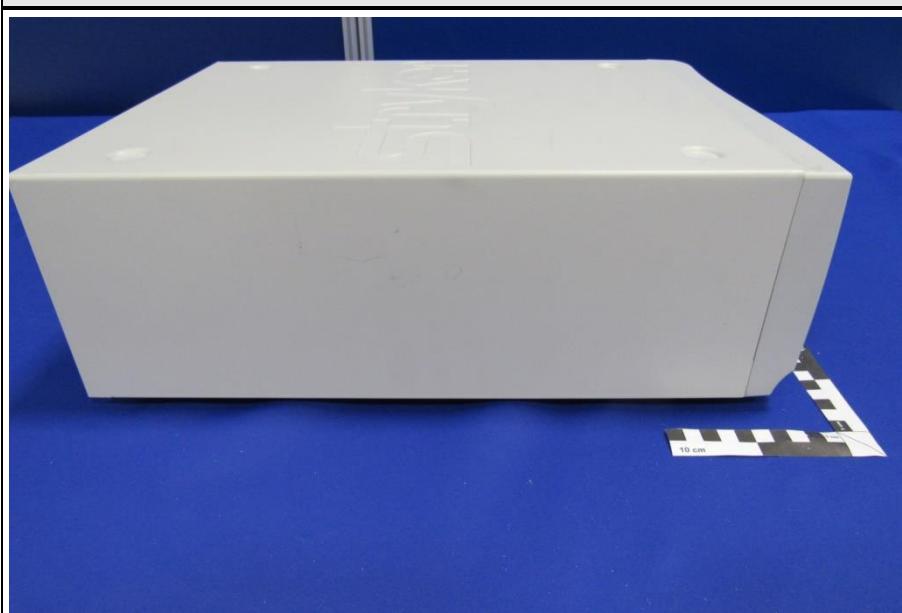


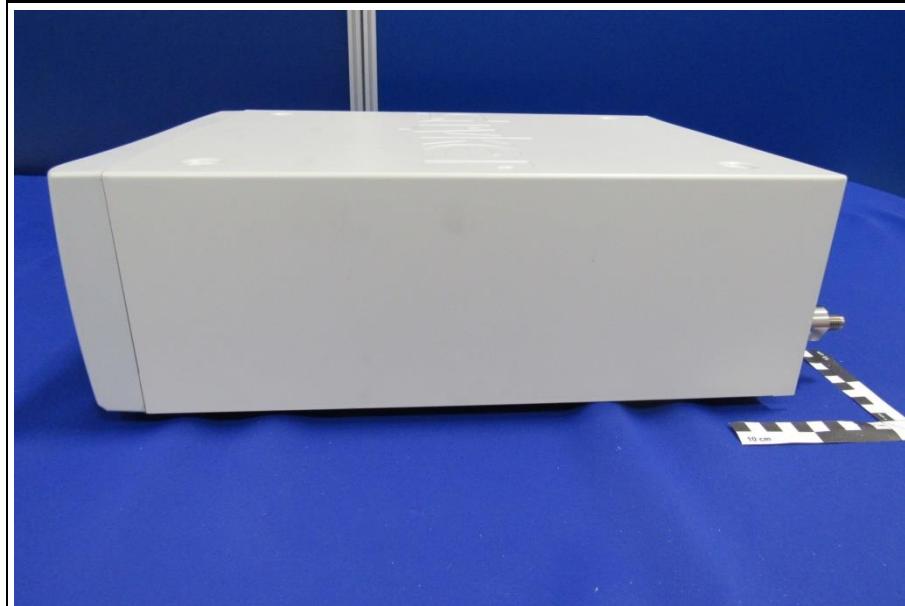
EUT Back Side View**EUT Right Side View**

Test Report No.: GOM-2010-9360-EF0115B-V01

Eurofins Product Service GmbH
Storkower Str. 38c, D-15526 Reichenwalde, Germany

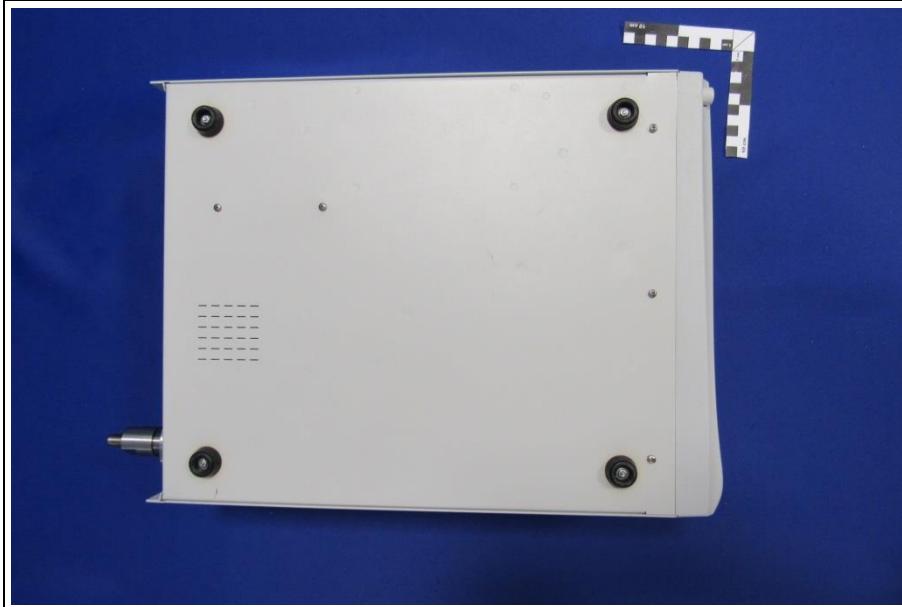EUT Bottom View**EUT Label**

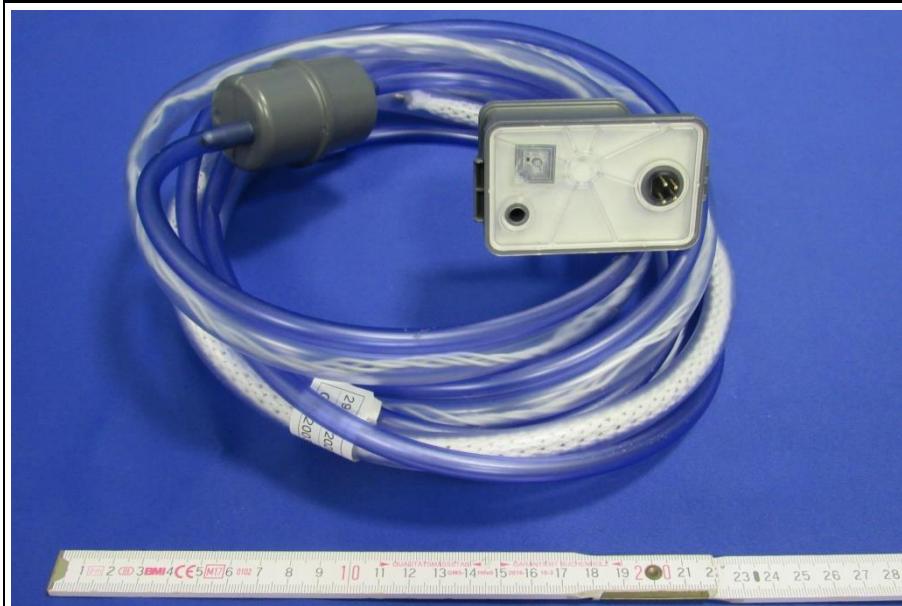Humidified / heated / smoke evacuation tube – View 1**Humidified / heated / smoke evacuation tube – View 2**

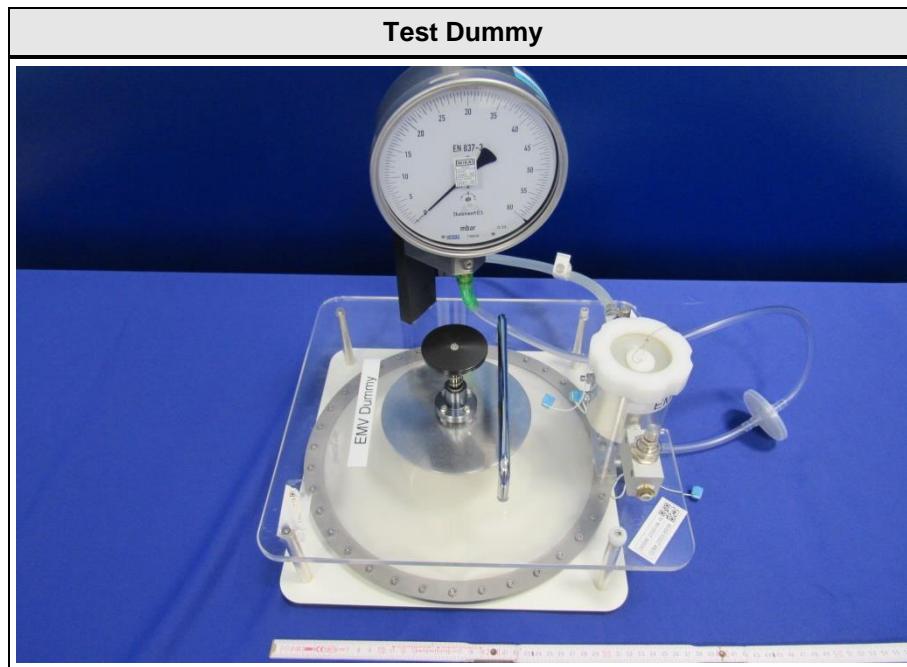

1.4 Support Equipment

Product Type	Device	Manufacturer	Model	Comment
CBL	EU power cord 2m	HAWA	1102131	
CBL	US power cord 2.5m	KCC	1102134	
AE	Humidified / heated / smoke evacuation tube	W.O.M. World of Medicine GmbH	ST298	
SIM	Dummy LAP Adul Plus	W.O.M. World of Medicine GmbH	2205477	
AE	CO2 gas tank	-	-	Food compatible
AE	High pressure tube	W.O.M. World of Medicine GmbH	ST216	
SIM	SIDNE Device Control	STRYKER	SDC3	SN: 16D001594
CBL	USB Cable	-	-	shielded
CBL	PE Cable	-	-	
Description:				
AE	Auxiliary Equipment			
SIM	Simulator			
MON	Monitoring Equipment			
CBL	Connecting Cable			
Comment:				

1.5 Operational Modes


Mode #	Description
1	<p>Standard Mode: Set Pressure : 15 mmHg Set Flow: 20 mmHg Smoke Evacuation: Level 4 (max)</p> <p>Comment:</p> <p>Standard Mode Settings:</p> 

1.6 EUT Configuration

Configuration #	Description
1	Insufflator connected with gas bottle and gas tube with heater system and RFID Tag. Gas tube connected to the test dummy with mechanical pressure sensor. USB connection with the SYDNE System established. Device powered up with 120 V / 60 Hz. See below Setup for operating mode 1

Comment:

Setup for operating mode 1

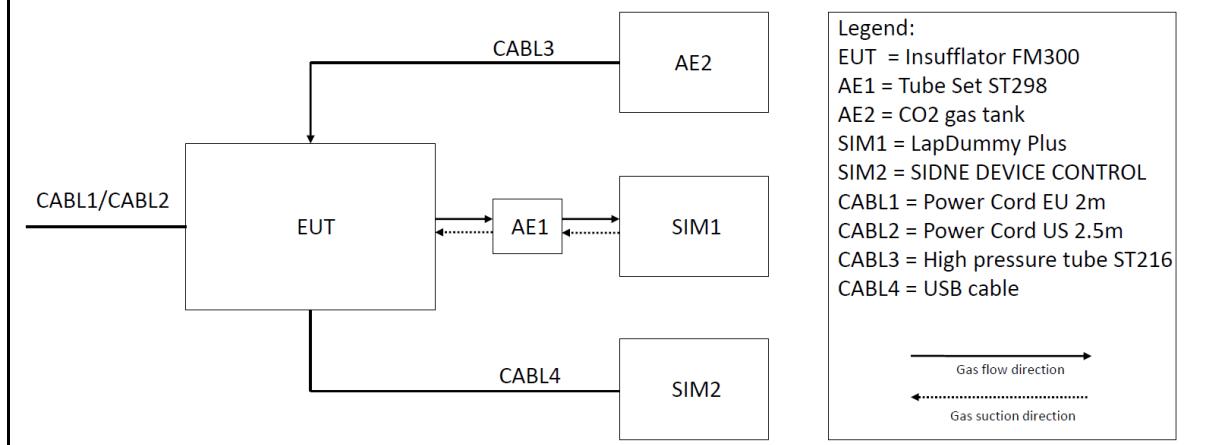

1.7 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyser in dB μ V. Any external preamplifiers used are taken into account through internal analyser settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyser. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyser (dB}\mu\text{V)} + \text{A.F. (dB/m)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dB μ V/m). The FCC limits are given in units of μ V/m. The following formula is used to convert the units of μ V/m to dB μ V/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 * \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

Reading + AF	= Net Reading	:	Net reading - FCC limit	= Margin
+21.5 dB μ V + 26 dB/m	= 47.5 dB μ V/m	:	47.5 dB μ V/m - 57.0 dB μ V/m	= -9.5 dB

2 Result Summary

FCC 47 CFR Part 15B, ISED ICES-003 Issue 6				
Reference	Requirement	Reference Method	Result	Remarks
Emission				
FCC 15.109 ICES-003, 6.2	Radiated emissions	ANSI C63.4:2014 +A1:2017	PASS	
FCC 15.107 ICES-003, 6.1	AC power line conducted emissions	ANSI C63.4:2014 +A1:2017	PASS	
Comment:				



Possible Test Case Verdicts	
PASS	Test object does meet the requirements
FAIL	Test object does not meet the requirements
N/T	Required by standard but not tested
N/R	Not required by standard for the test object



2.1 Test Conditions and Results - Radiated emissions acc. to ANSI C63.4

2.1.1 Information

Test Information	
Reference	FCC 15.109, ICES-003, 6.2
Reference method	ANSI C63.4:2014+A1:2017 Section 8
Equipment class	Class B
Equipment type	Table top
Highest internal frequency [MHz]	806
Measurement range	30 MHz to 5 GHz
Temperature [°C]	22 to 24
Humidity [%]	41
Operator	Ruslan Colbasiuc
Date	2020-10-28 to 2020-10-29

2.1.2 Setup

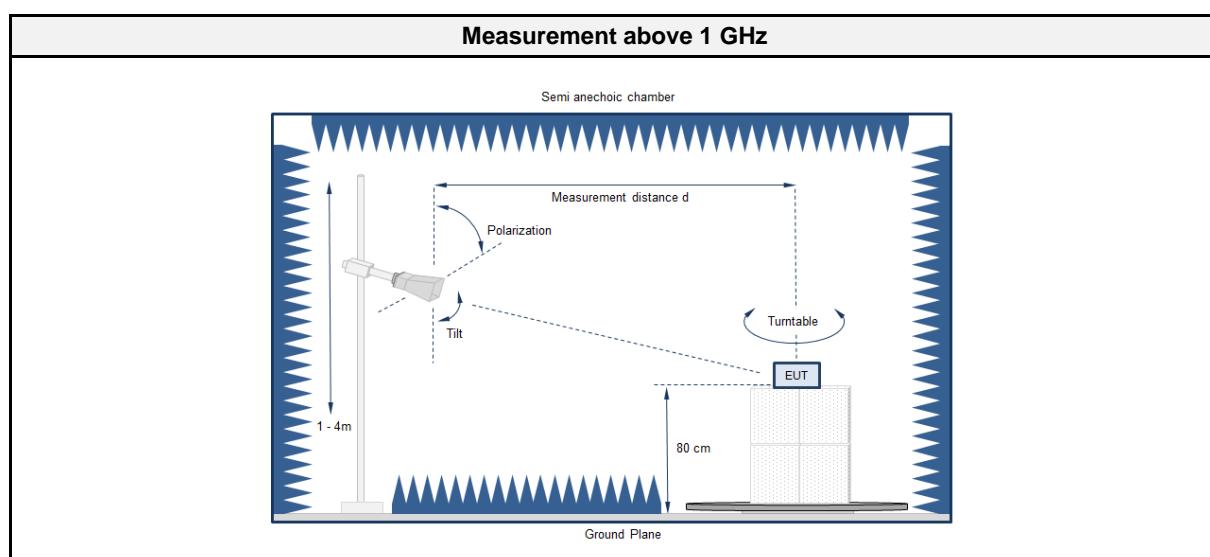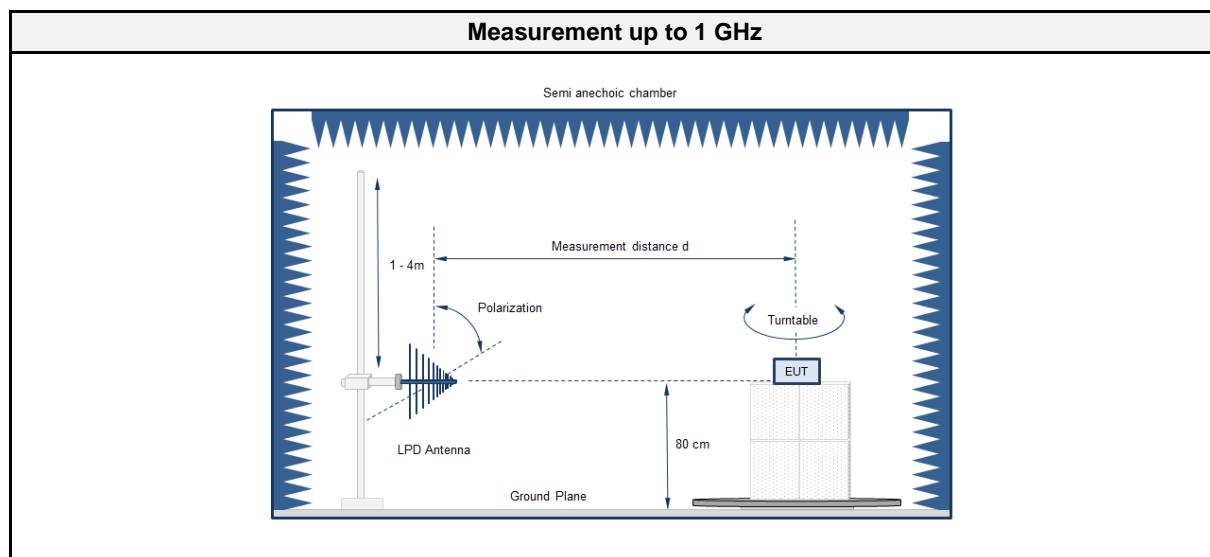

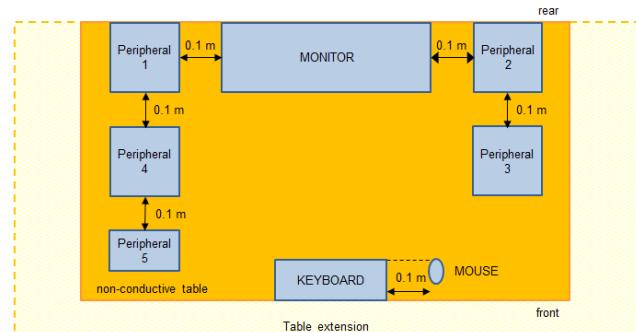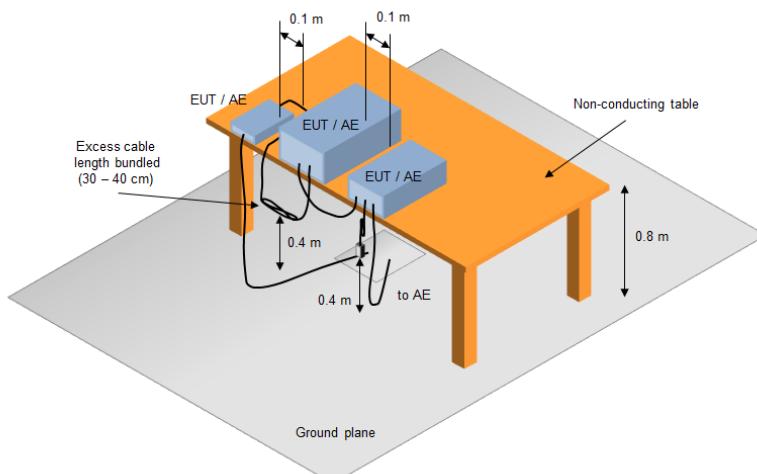Equipment placement - Table top

Test Setup

2.1.3 Equipment
Test Software

Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	Radimation	2016.1.10

Test Equipment

Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
Anechoic chamber	Frankonia	AC6	EF00910	2020-02	2023-02
EMI Test Receiver	R&S	ESU26	EF00887	2020-07	2021-07
TRILOG Broadband Antenna	Schwarzbeck	VULB 9162	EF00978	2019-10	2022-10
Horn Antenna	ETS-Lindgren	3117	EF00976	2019-03	2022-03
Climatic Sensor	Embedded Data Systems, LLC.	9A00100000254 77E	EF01124	2020-03	2021-03

2.1.4 Procedure

Exploratory measurement
<ol style="list-style-type: none"> 1. The EUT was placed on a non-conductive table at a height of 0.8m. 2. The EUT and support equipment, if needed, were set up to simulate typical usage. 3. Cables, of type and length specified by the manufacturer, were connected to at least one port of each type and were terminated by a device or simulating load of actual usage. 4. The antenna was placed at a distance of 3 or 10 m. 5. The received signal was monitored at the measurement receiver. 6. This procedure has to be performed in both antenna polarizations, horizontal and vertical. 7. The arrangement of the equipment with the maximum emission level is shown on the setup picture at item 1.3

Final measurement
<ol style="list-style-type: none"> 1. The EUT was placed on a 0.8 m non-conductive table at a 3 m distance from the receive antenna. The antenna output was connected to the measurement receiver. 2. A biconical antenna was used for the frequency range 30 – 200 MHz, a logarithmic periodical antenna was used for the frequency range from 200 – 1000 MHz. Above one 1 GHz a Double Ridged Broadband Horn antenna was used. The antenna was placed on an adjustable height antenna mast. 3. The EUT and cable arrangement were based on the exploratory measurement results. 4. Emissions were maximized at each frequency by rotating the EUT and adjusting the receive antenna height and polarization. The maximum values were recorded. 5. The test data of the worst-case conditions were recorded and shown on the next pages.



2.1.5 Limits



Class B @ 3 m		
Frequency [MHz]	Detector	Limit [dB μ V/m]
30 - 88	Quasi-peak	40
88 - 216	Quasi-peak	43.5
216 - 960	Quasi-peak	46
960 - 1000	Quasi-peak	54
> 1000	Peak Average	74 54

2.1.6 Results

Test Results			
Operational mode	EUT Configuration	Verdict	Remark
1	1	PASS	-

2.1.7 Setup Photos

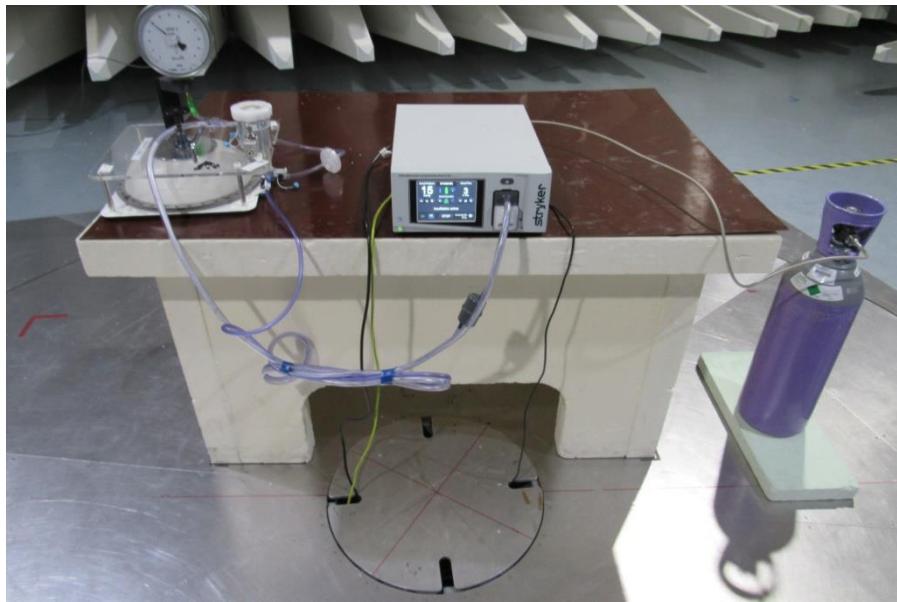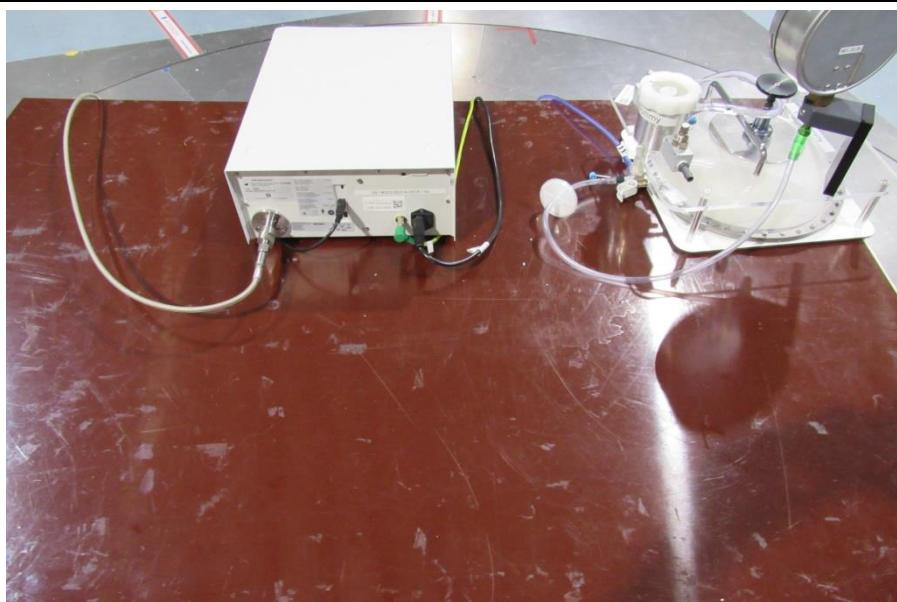Radiated Emission Test Setup View 1**Radiated Emission Test Setup View 2**

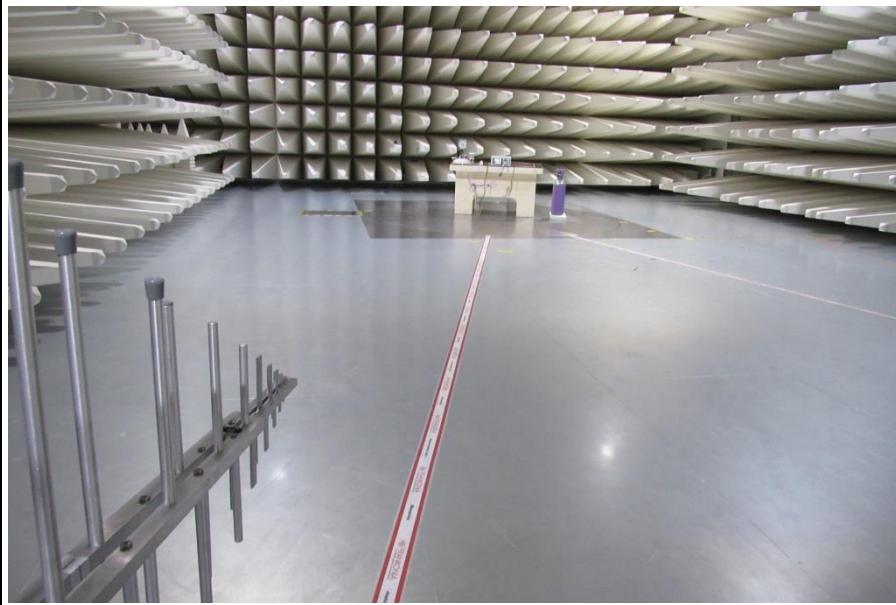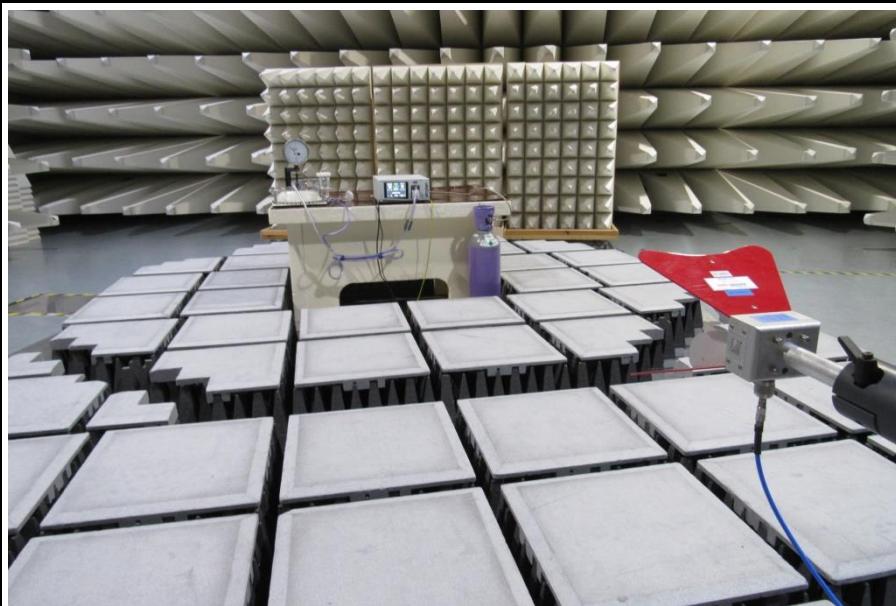Radiated Emission Test Setup TRILOG Broadband Antenna View**Radiated Emission Test Setup Horn Antenna View**


2.1.8 Records

Radiated emissions according to FCC 15B

Project Number: G0M-2010-9360
 Applicant: W.O.M. WORLD OF MEDICINE GmbH
 Model Description: Insufflator for Laparoscopy, Vessel Harvesting, Colorectal and Cardiac Procedures
 Model: FM300
 Test Sample ID: 31468
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Colbasiuc
 Test Date: 2020-10-28
 Operating Conditions: ambient temperature: 24°C
 power input: 120 VAC / 60 Hz
 Antenna: Schwarzbeck VULB 9162, Vertical
 Measurement Distance: 10 m corrected to 3 m
 Operational Mode & Configuration: Mode 1
 EUT Configuration: Configuration 1

Note 1:

Index 1

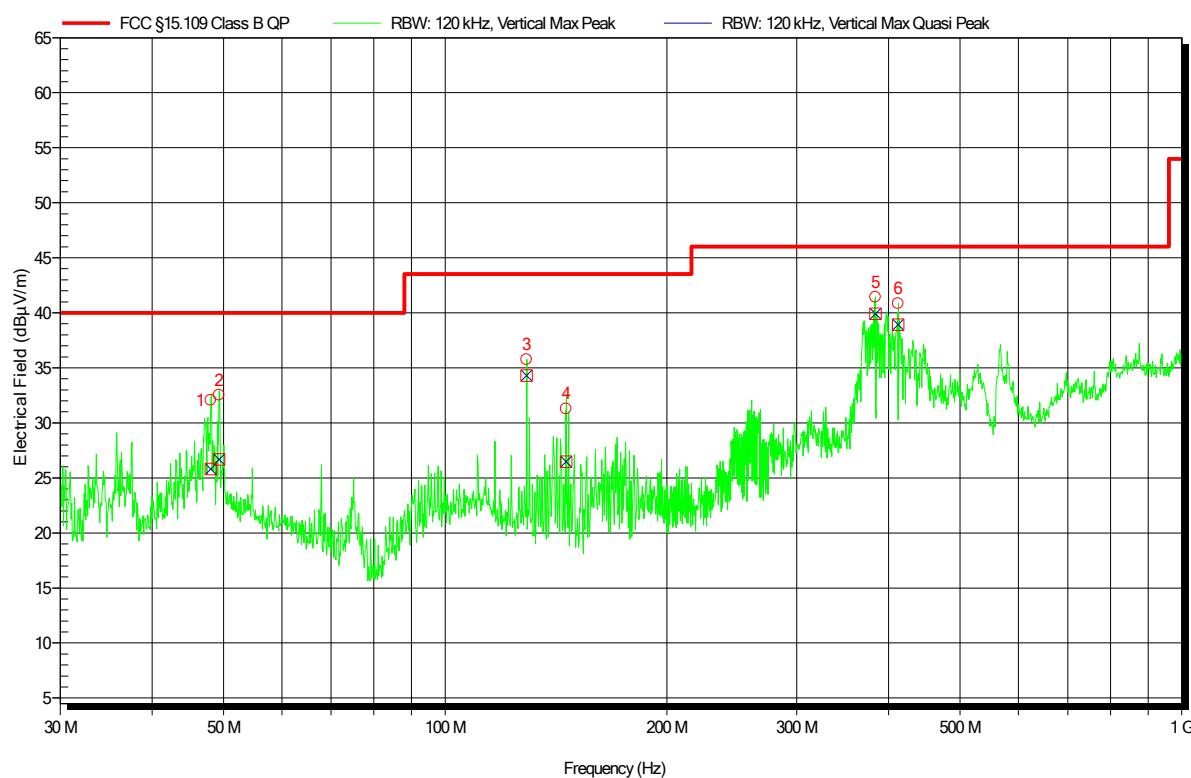

Peak Number	Frequency	Quasi-Peak	Quasi-Peak	Quasi-Peak	Quasi-Peak	Angle	Height
			Limit	Difference	Status		
1	48.054 MHz	25.8 dB μ V/m	40 dB μ V/m	-14.2 dB	Pass	-30 Degree	1 m
2	49.308 MHz	26.7 dB μ V/m	40 dB μ V/m	-13.3 dB	Pass	-30 Degree	1 m
3	129 MHz	34.3 dB μ V/m	43.5 dB μ V/m	-9.2 dB	Pass	-30 Degree	1 m
4	145.944 MHz	26.5 dB μ V/m	43.5 dB μ V/m	-17.0 dB	Pass	-30 Degree	1 m
5	383.743 MHz	39.9 dB μ V/m	46 dB μ V/m	-6.1 dB	Pass	180 Degree	1 m
6	412.045 MHz	38.9 dB μ V/m	46 dB μ V/m	-7.1 dB	Pass	180 Degree	1 m

Test Report No.: G0M-2010-9360-EF0115B-V01


 Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated emissions according to FCC 15B

Project Number: G0M-2010-9360
 Applicant: W.O.M. WORLD OF MEDICINE GmbH
 Model Description: Insufflator for Laparoscopy, Vessel Harvesting, Colorectal and Cardiac Procedures
 Model: FM300
 Test Sample ID: 31468
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Colbasici
 Test Date: 2020-10-28
 Operating Conditions: ambient temperature: 24°C
 power input: 120 VAC / 60 Hz
 Antenna: Schwarzbeck VULB 9162, Horizontal
 Measurement Distance: 10 m corrected to 3 m
 Operational Mode & EUT Configuration: Mode 1
 Configuration 1

Note 1:

Index 2

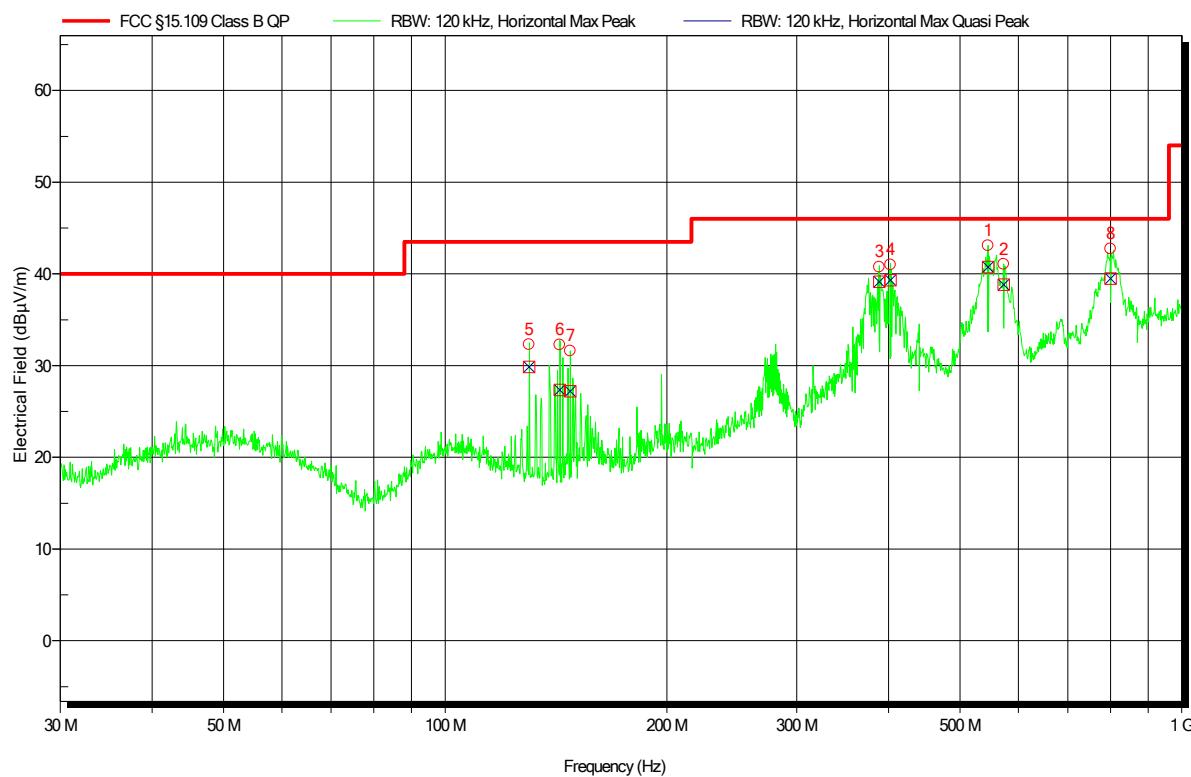

Peak Number	Frequency	Quasi-Peak	Quasi-Peak	Quasi-Peak	Quasi-Peak	Angle	Height
1	545.574 MHz	40.8 dB μ V/m	46 dB μ V/m	-5.3 dB	Pass	135 Degree	1.55 m
2	572.844 MHz	38.8 dB μ V/m	46 dB μ V/m	-7.2 dB	Pass	135 Degree	1.55 m
3	388.479 MHz	39.2 dB μ V/m	46 dB μ V/m	-6.9 dB	Pass	135 Degree	2.55 m
4	402.105 MHz	39.3 dB μ V/m	46 dB μ V/m	-6.7 dB	Pass	135 Degree	2.55 m
5	130.006 MHz	29.8 dB μ V/m	43.5 dB μ V/m	-13.7 dB	Pass	135 Degree	4 m
6	143.062 MHz	27.3 dB μ V/m	43.5 dB μ V/m	-16.2 dB	Pass	135 Degree	4 m
7	147.88 MHz	27.2 dB μ V/m	43.5 dB μ V/m	-16.3 dB	Pass	135 Degree	4 m
8	799.866 MHz	39.5 dB μ V/m	46 dB μ V/m	-6.5 dB	Pass	20 Degree	1 m

Test Report No.: G0M-2010-9360-EF0115B-V01


Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Radiated emissions according to FCC 15B

Project Number: G0M-2010-9360
 Applicant: W.O.M. WORLD OF MEDICINE GmbH
 Model Description: Insufflator for Laparoscopy, Vessel Harvesting, Colorectal and Cardiac Procedures
 Model: FM300
 Test Sample ID: 31468
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Colbasici
 Test Date: 2020-10-29
 Operating Conditions: ambient temperature: 24°C
 power input: 120 VAC / 60 Hz
 Antenna: ETS-Lindgren 3117, Horizontal
 Measurement Distance: 3 m
 Operational Mode & Configuration: Mode 1
 EUT Configuration: Configuration 1

Note 1:

Index 3

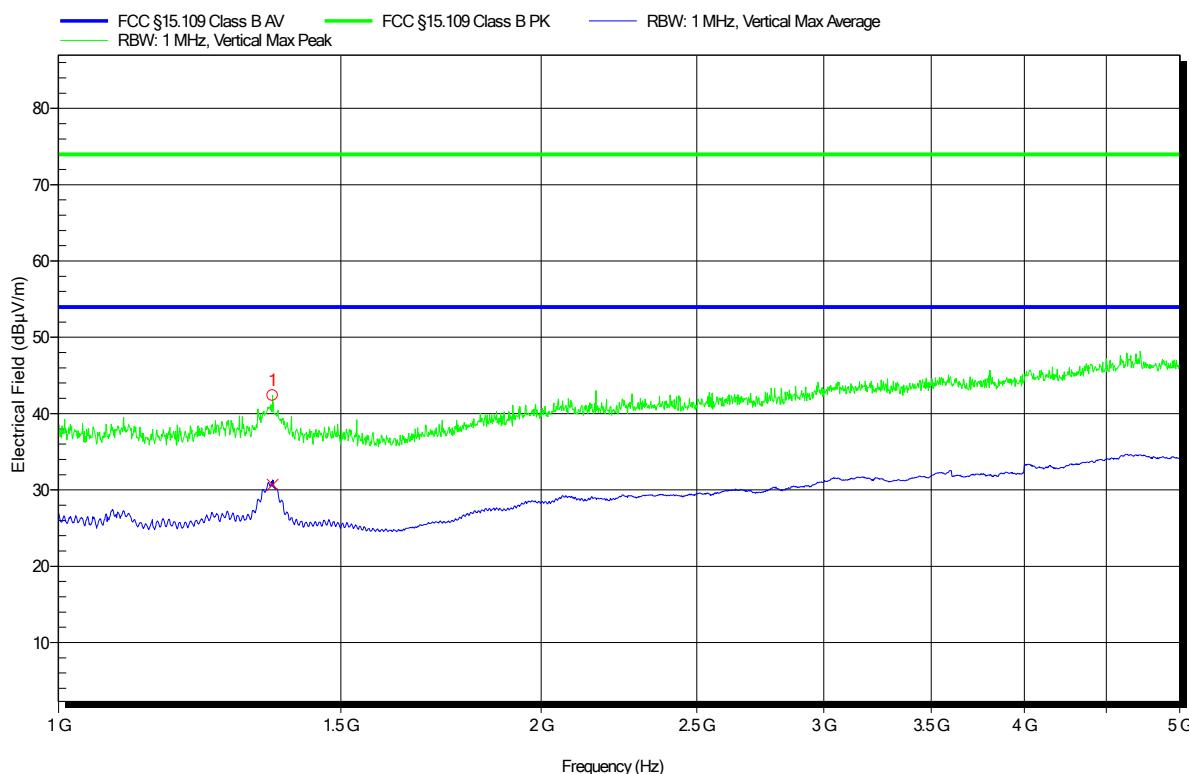


Peak Number	Frequency	Peak	Peak Limit	Peak Difference	Peak Status	Angle	Height
1	1.361 GHz	42.4 dB μ V/m	74 dB μ V/m	-31.6 dB	Pass	35 Degree	1 m
Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status	Angle	Height
1	1.361 GHz	30.7 dB μ V/m	54 dB μ V/m	-23.3 dB	Pass	35 Degree	1 m

Radiated emissions according to FCC 15B

Project Number: G0M-2010-9360
 Applicant: W.O.M. WORLD OF MEDICINE GmbH
 Model Description: Insufflator for Laparoscopy, Vessel Harvesting, Colorectal and Cardiac Procedures
 Model: FM300
 Test Sample ID: 31468
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Colbasiciu
 Test Date: 2020-10-29
 Operating Conditions: ambient temperature: 24°C
 power input: 120 VAC / 60 Hz
 Antenna: ETS-Lindgren 3117, Horizontal
 Measurement Distance: 3 m
 Operational Mode & EUT Configuration: Mode 1
 Configuration 1

Note 1:

Index 4

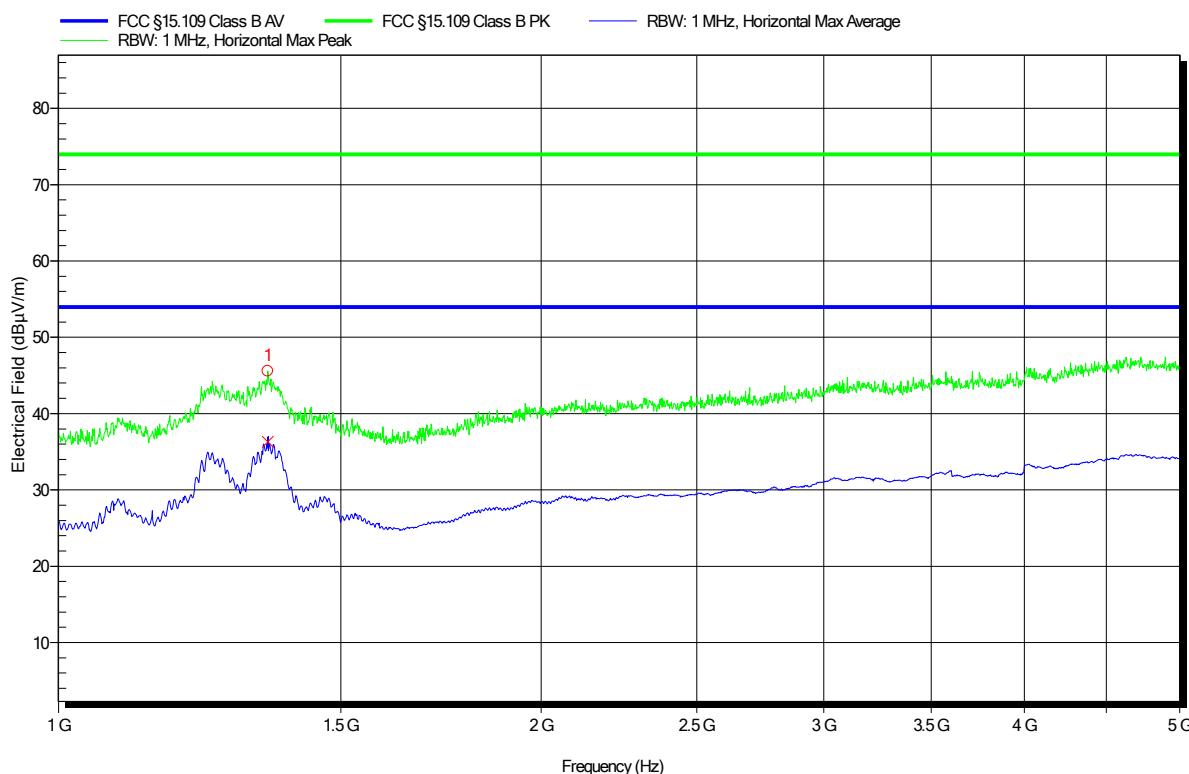



Peak Number	Frequency	Peak	Peak Limit	Peak Difference	Peak Status	Angle	Height
1	1.351 GHz	45.6 dB μ V/m	74 dB μ V/m	-28.4 dB	Pass	140 Degree	1 m
Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status	Angle	Height
1	1.351 GHz	36.3 dB μ V/m	54 dB μ V/m	-17.7 dB	Pass	0140Degree	1 m

2.2 Test Conditions and Results - Conducted emissions acc. to ANSI C63.4

2.2.1 Information

Test Information	
Reference	FCC 15.107, ICES-003, 6.1
Reference method	ANSI C63.4:2014+A1:2017 Section 12
Measurement range	150 kHz to 30 MHz
Equipment class	Class B
Equipment type	Table top
Temperature [°C]	23
Humidity [%]	41
Operator	Ruslan Colbasiuc
Date	2020-10-29

2.2.2 Setup

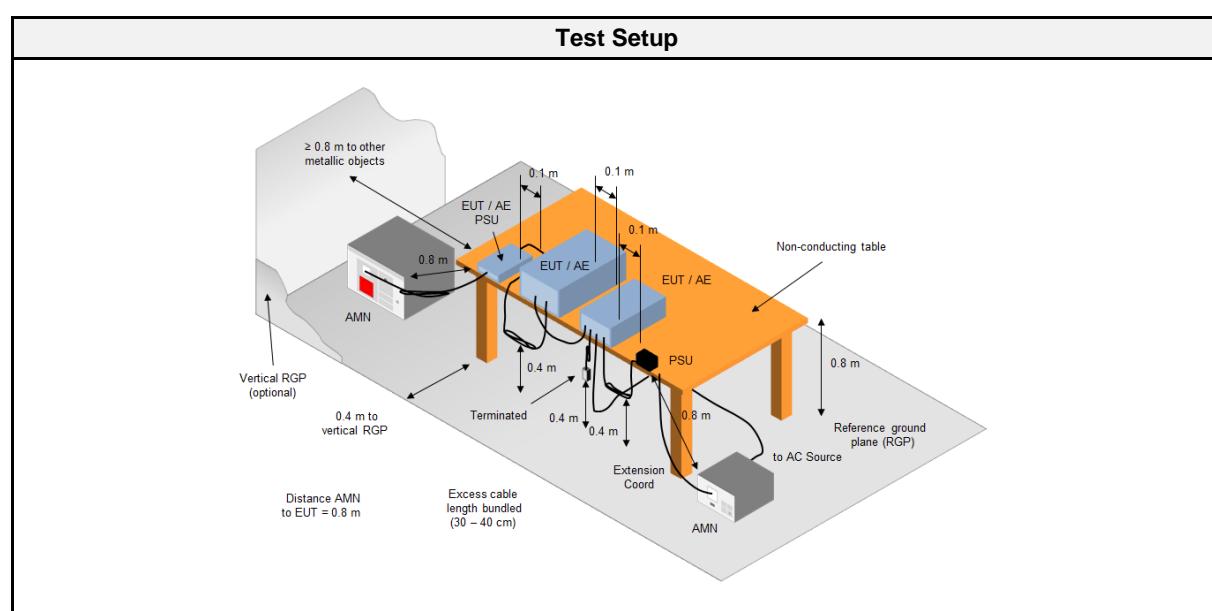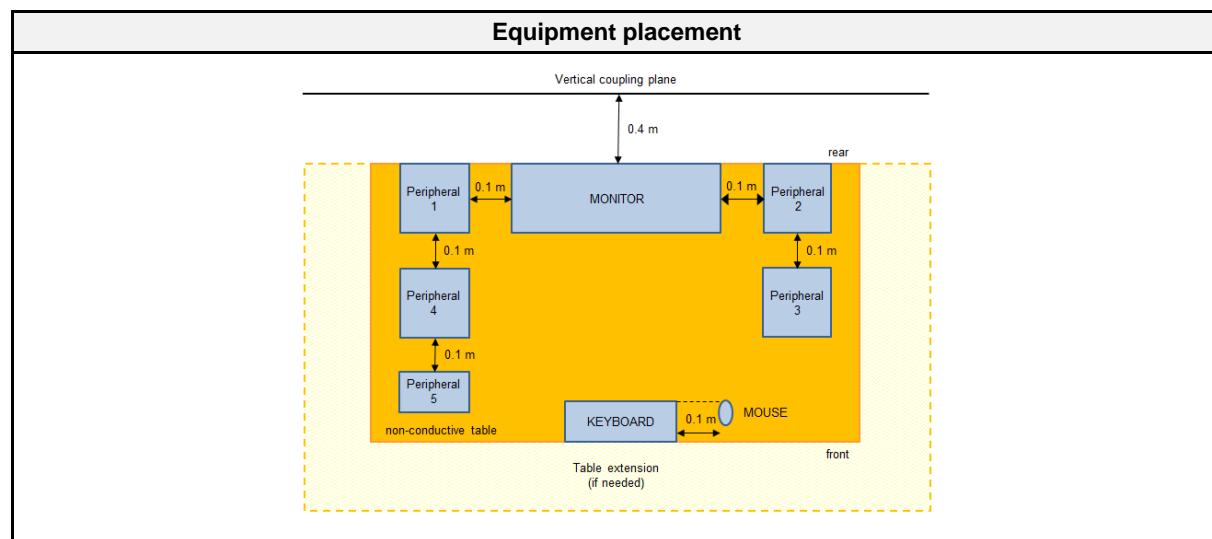

2.2.3 Equipment

Test Software			
Description	Manufacturer	Name	Version
EMC Software	DARE Instruments	Radimation	2016.1.10

Test Equipment					
Description	Manufacturer	Model	Identifier	Cal. Date	Cal. Due
AMN	Schwarzbeck	NSLK 8128	EF00975	2019-07	2021-07
Pulse Limiter	R&S	ESH3-Z2	EF01063	2020-07	2021-07
EMI Test Receiver	R&S	ESU26	EF00887	2020-07	2021-07
Climatic Sensor	Embedded Data Systems, LLC.	9A00100000254 77E	EF01124	2020-03	2021-03

2.2.4 Procedure

Exploratory measurement
<ol style="list-style-type: none"> 1. The EUT was placed on a non conductive table 0.8 m above the reference ground plane and 0.4 m away from the vertical conducting plane (ANSI C63.4: 2014 item 7.3.1) 2. The power cord that is normally supplied or recommended by the manufacturer was connected to the LISN. 3. The distance between the outer edge of the EUT and the LISN shall be set to 0.8 m. A longer power cord shall be bundled to this length (bundling shall not exceed 40 cm in length). 4. The LISN measurement port was connected to a measurement receiver 5. I/O cables were bundled not longer than 0.4 m 6. Measurement was performed in the frequency range 0.15 – 30MHz on each current-carrying conductor 7. To maximize the emissions the cable positions were manipulated 8. The worst configuration of EUT and cables is shown on a test setup picture at item 1.3

Final measurement
<ol style="list-style-type: none"> 1. The EUT was placed on a non conductive table 0.8 m above the reference ground plane and 0.4 m away from the vertical conducting plane (ANSI C63.4: 2014 item 7.3.1) 2. The power cord that is normally supplied or recommended by the manufacturer was connected to the LISN. 3. The distance between the outer edge of the EUT and the LISN shall be set to 0.8 m. A longer power cord shall be bundled to this length (bundling shall not exceed 40 cm in length). 4. The LISN measurement port was connected to a measurement receiver 5. The EUT and cable arrangement were based on the exploratory measurement results 6. The test data of the worst-case conditions were recorded and shown on the next pages

2.2.5 Limits



Class B		
Frequency [MHz]	Quasi-peak Limit [dB μ V]	Average Limit [dB μ V]
0.15 - 0.5	66 - 56 *	56 - 46 *
0.5 - 5	56	46
5 - 30	60	50

* Decreases with the logarithm of the frequency

2.2.6 Results

AC power line conducted emissions					
Port	Coupling	Operational mode	EUT Configuration	Verdict	Remark
Mains Connection	AMN	1	1	PASS	-

2.2.7 Setup Photos

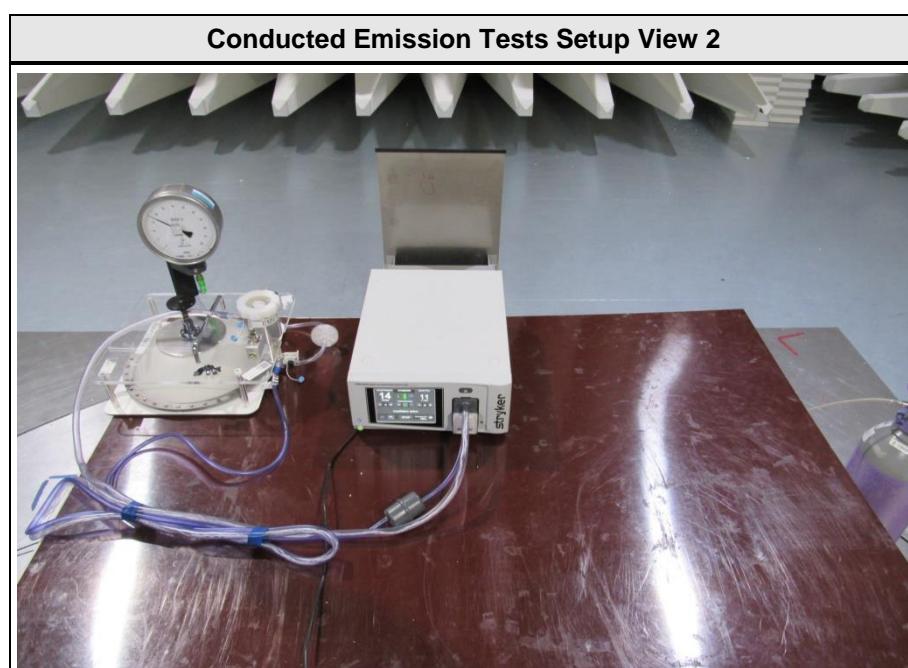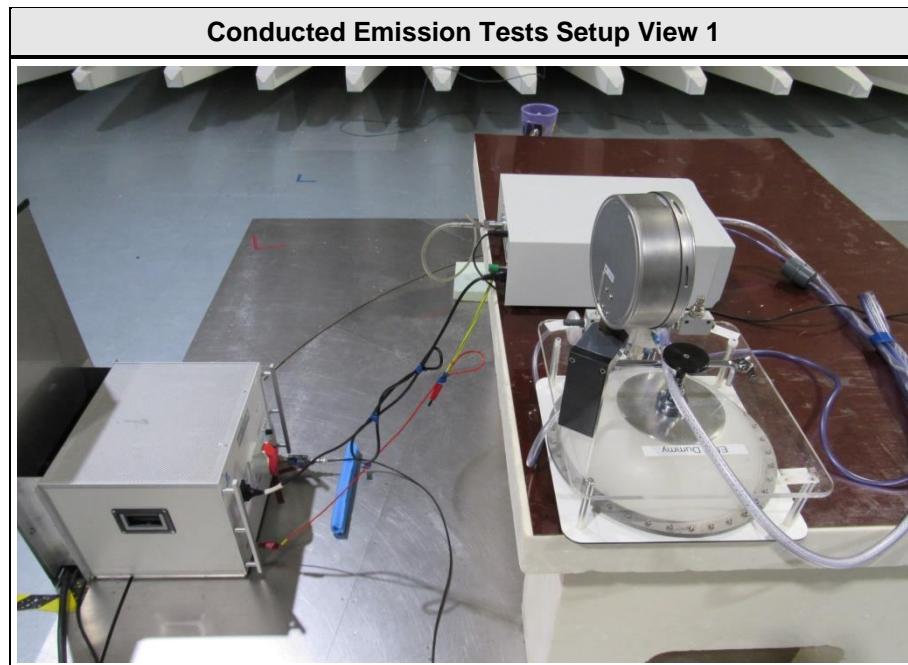


2.2.8 Records

Conducted emissions at the mains power port according to FCC 15B

Project Number: G0M-2010-9360
 Applicant: W.O.M. WORLD OF MEDICINE GmbH
 Model Description: Insufflator for Laparoscopy, Vessel Harvesting, Colorectal and Cardiac Procedures
 Model: FM300
 Test Sample ID: 31468
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Colbasiuc
 Test Date: 2020-10-29
 Operating Conditions: ambient temperature: 23°C
 power input: 120 VAC / 60 Hz
 LISN: Schwarzbeck NSLK 8128 (N)
 Operational Mode & Mode 1
 EUT Configuration: Configuration 1
 Applied to Port: Mains Connection
 Note 1:

Index 5

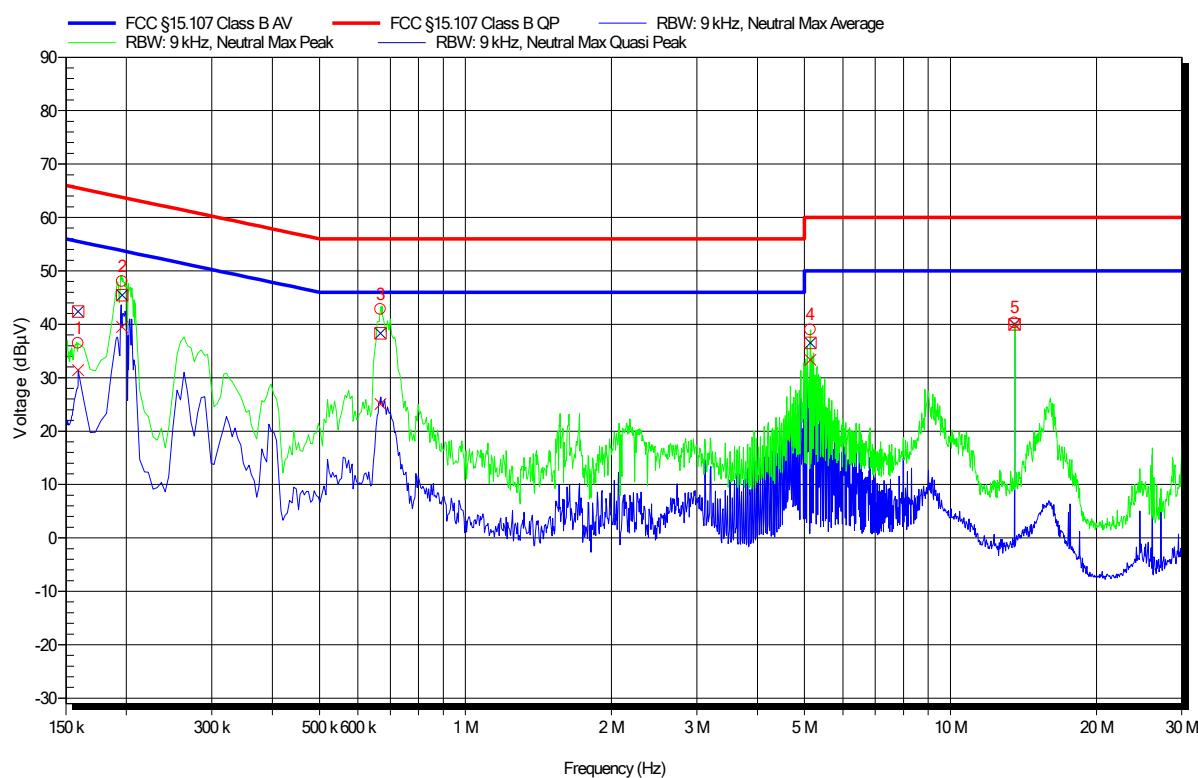

Peak Number	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status	LISN
1	159 kHz	42.4 dB μ V	65.5 dB μ V	-23.1 dB	Pass	Neutral
2	195.9 kHz	45.5 dB μ V	63.8 dB μ V	-18.3 dB	Pass	Neutral
3	668.4 kHz	38.3 dB μ V	56 dB μ V	-17.7 dB	Pass	Neutral
4	5.143 MHz	36.5 dB μ V	60 dB μ V	-23.5 dB	Pass	Neutral
5	13.56 MHz	40 dB μ V	60 dB μ V	-20.0 dB	Pass	Neutral

Test Report No.: G0M-2010-9360-EF0115B-V01


 Eurofins Product Service GmbH
 Storkower Str. 38c, D-15526 Reichenwalde, Germany

Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status	LISN
1	159 kHz	31.4 dB μ V	55.5 dB μ V	-24.1 dB	Pass	Neutral
2	195.9 kHz	39.5 dB μ V	53.8 dB μ V	-14.3 dB	Pass	Neutral
3	668.4 kHz	25.1 dB μ V	46 dB μ V	-20.9 dB	Pass	Neutral
4	5.143 MHz	33.3 dB μ V	50 dB μ V	-16.7 dB	Pass	Neutral
5	13.56 MHz	39.9 dB μ V	50 dB μ V	-10.1 dB	Pass	Neutral

Conducted emissions at the mains power port according to FCC 15B

Project Number: G0M-2010-9360
 Applicant: W.O.M. WORLD OF MEDICINE GmbH
 Model Description: Insufflator for Laparoscopy, Vessel Harvesting, Colorectal and Cardiac Procedures
 Model: FM300
 Test Sample ID: 31468
 Test Site: Eurofins Product Service GmbH
 Operator: Mr. Colbasiuc
 Test Date: 2020-10-29
 Operating Conditions: ambient temperature: 23°C
 power input: 120 VAC / 60 Hz
 LISN: Schwarzbeck NSLK 8128 (L)
 Operational Mode & Configuration: Mode 1
 Applied to Port: Mains Connection
 Note 1:

Index 6

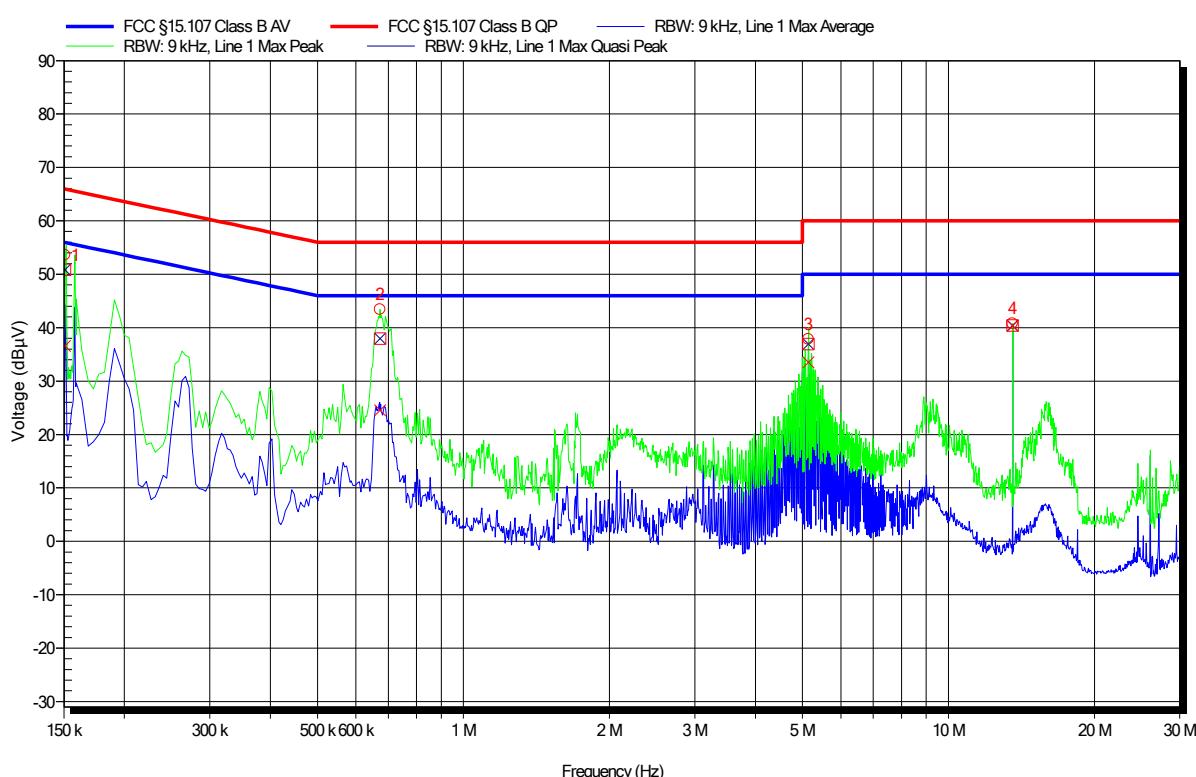

Peak Number	Frequency	Quasi-Peak	Quasi-Peak Limit	Quasi-Peak Difference	Quasi-Peak Status	LISN
1	150.9 kHz	50.8 dBµV	66 dBµV	-15.1 dB	Pass	Line 1
2	672.9 kHz	37.9 dBµV	56 dBµV	-18.1 dB	Pass	Line 1
3	5.145 MHz	36.9 dBµV	60 dBµV	-23.1 dB	Pass	Line 1
4	13.56 MHz	40.4 dBµV	60 dBµV	-19.6 dB	Pass	Line 1

Peak Number	Frequency	Average	Average Limit	Average Difference	Average Status	LISN
1	150.9 kHz	36.6 dB μ V	56 dB μ V	-19.4 dB	Pass	Line 1
2	672.9 kHz	24.5 dB μ V	46 dB μ V	-21.5 dB	Pass	Line 1
3	5.145 MHz	33.5 dB μ V	50 dB μ V	-16.5 dB	Pass	Line 1
4	13.56 MHz	40.3 dB μ V	50 dB μ V	-9.7 dB	Pass	Line 1

End of the test report