

LABELING

Original Freigabeformular in TR archiviert.
Original form stored in the technical writing department.

Label sticks inside of the device

FA. Nr. ##### - ##
SN YMMCE###

Removing this label causes loss of warranty.
10000012654 03

MAX. IRRIGATION RATE* 0.5 / 2.5 / 3.5 l/min
MAX. SPÜLEISTUNG*
MAX. PUMPING PRESSURE* 90 / 150 / 200 / 500 mmHg
MAX. PUMPENDRUCK*
MAINS VOLTAGE RANGE AC 100 - 240 V~
NETZSPANNUNGSBEREICH
SUPPLY FREQUENCY 50/60 Hz
VERSORGUNGSFREQUENZ
POWER CONSUMPTION 125 VA
LEISTUNGS-AUFNAHME
*Depending on operation mode
*Je nach Betriebsart

IP 41

Contains FCC ID: 2AS5K-TSHW42
Contains IC: 25004-TSHW42A
HVIN: 1430

AESCULAP®
Aesculap AG
Am Aesculap-Platz
78532 Tuttlingen/Germany

CE 0123

TYPE MultiFlow / PG130
SN / REF YMMCE### / PG130

GTIN #####


AESCULAP®
Aesculap AG
Am Aesculap-Platz
78532 Tuttlingen/Germany

CE 0123


TYPE MultiFlow / PG130
SN / REF YMMCE### / PG130
100-240 V~ 50/60 Hz

GTIN #####


Rear of device

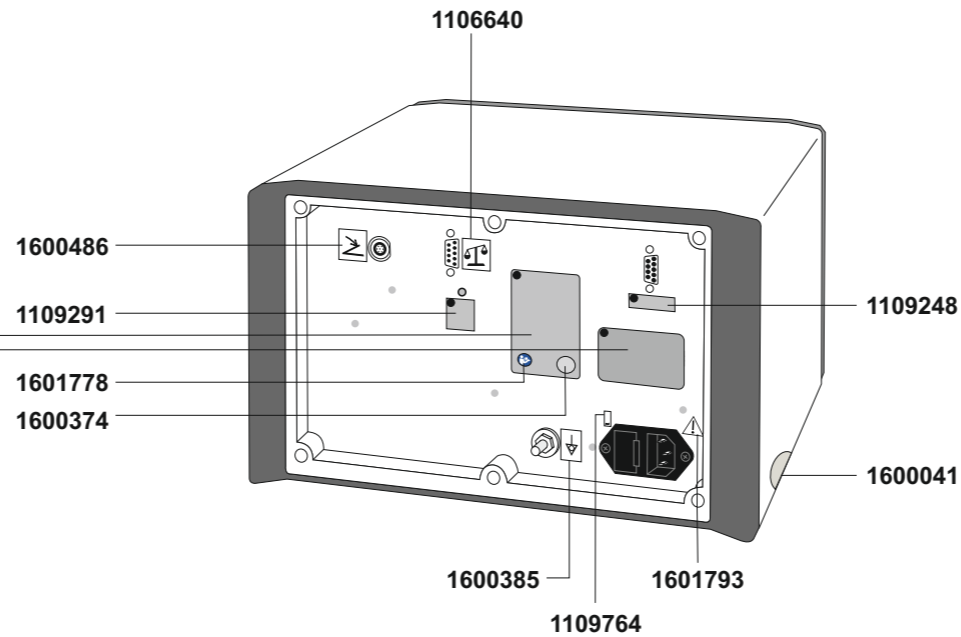

Front / side / top of device

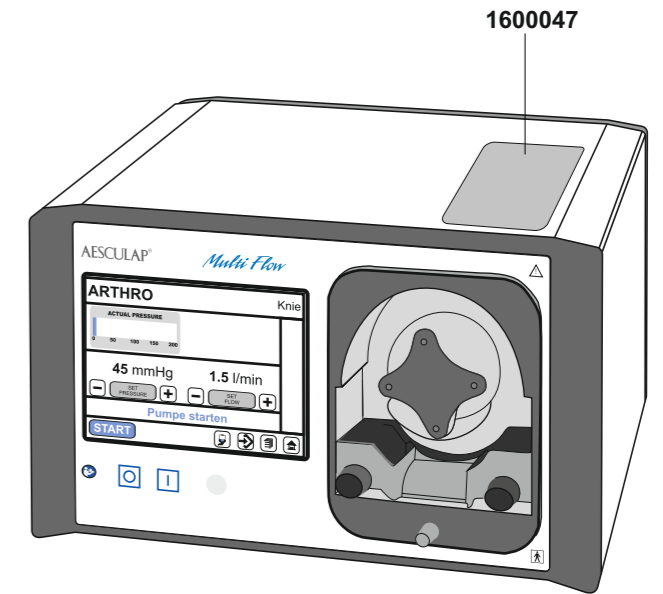

Box

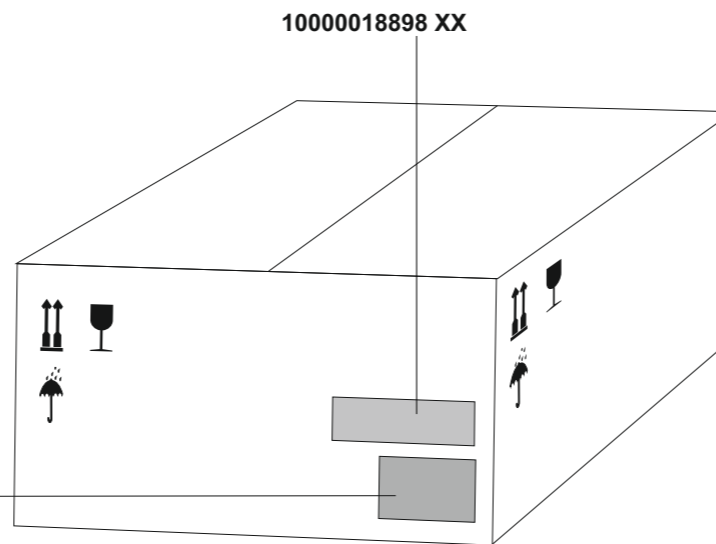

Revision history

Rev. WOM	ÄV-Nr.	Change
		Legend: Main Change request(s) Technical Writing Change Request(s)
01	2015287	IEC 3.1, listing of technical data; Added: GS1 EAN Data Matrix; symbol: manufactured (with date); symbol: quantity (with text); label storage and transport conditions; 10000018599 XX, 10000012512 XX; Removed: declaration voltage range, supply frequency (type label); barcode with serial number (internal label); declaration of standards (data label), FUSE (technical data)
02	2018059	supply frequency at data and packing label, Removed: WARNING! Risk of fire, Add AIR OUT symbol and 90 mmHg at max pumping pressure; ADDITIONAL: Change document number to material number, actualisation of the front
03	2020065	Added: symbol "Non-ionizing radiation", test numbers on the device label: "Contains FCC ID: 2AS5K-TSHW42", "Contains IC: 25004-TSHW42A", "HVIN: 1430"; Removed: symbol descriptions

Product Management / Customer

Project Management (R&D)

Regulatory Affairs

WORLD OF MEDICINE Freigabe / Approval



Overview device labels APUH100 PG130 Aesculap

W.O.M. Item number

10000012654 03

FMT File
10000012654 03.FMT

CDR File
10000012654 03.CDR

Name
TR

Date
11.11.2020