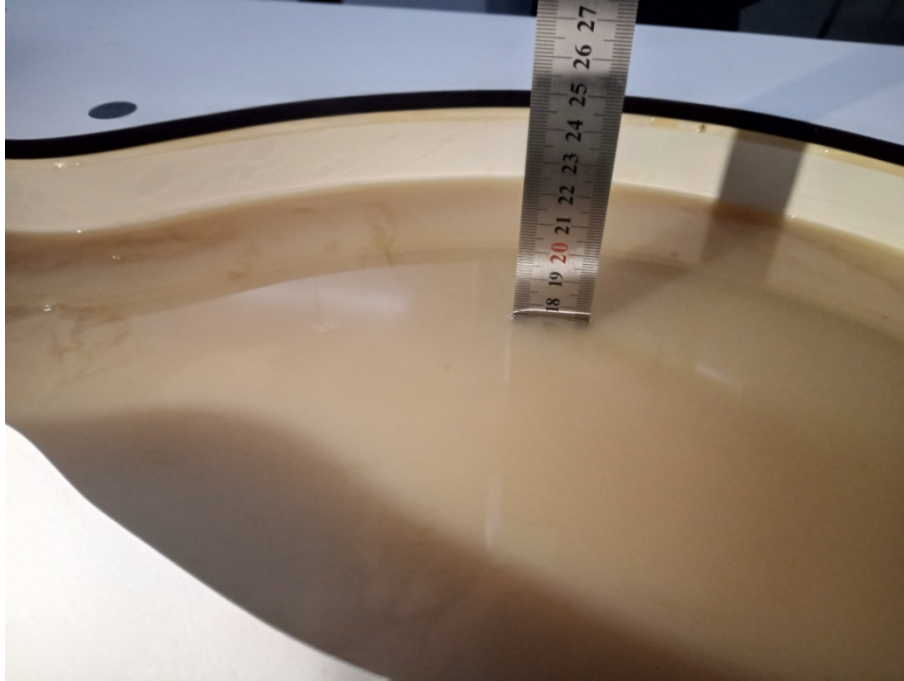
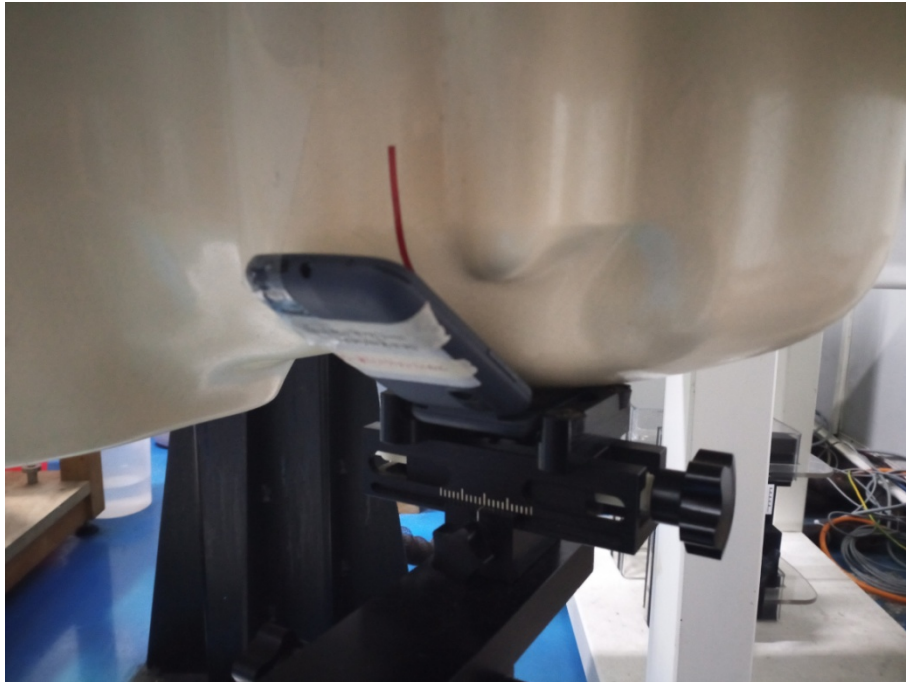

APPENDIX B EUT TEST POSITION PHOTOS

Liquid depth $\geq 15\text{cm}$

Phantom: SAM (30deg probe tilt) with CRP v5.0_20150321; Type: QD000P40CD; Serial: TP:1874



Head Left Cheek Setup Photo (0mm)



Head Left Tilt Setup Photo (0mm)



Head Right Cheek Setup Photo (0mm)



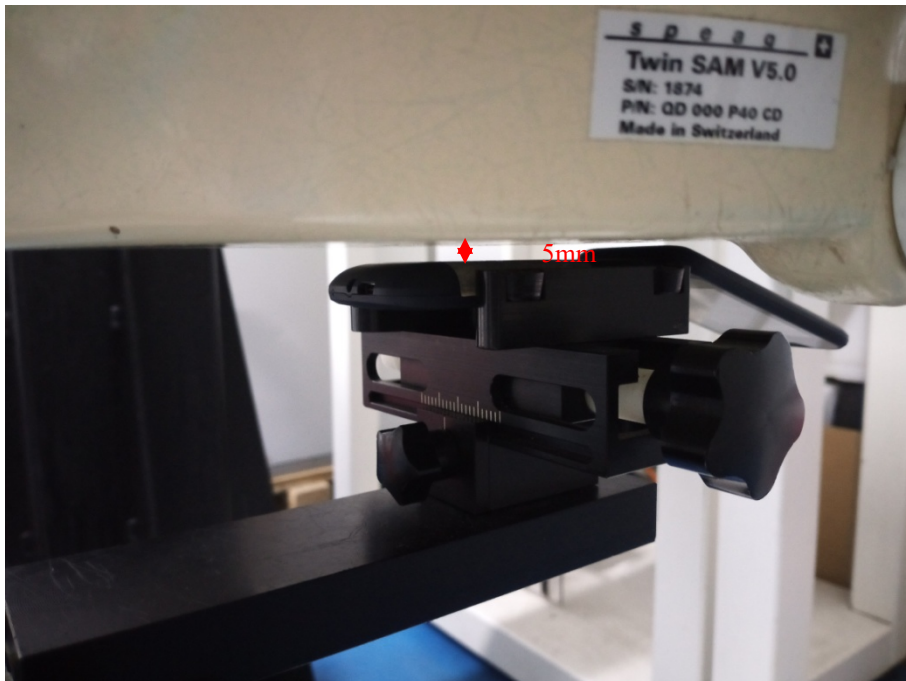
Head Right Tilt Setup Photo (0mm)



Body(Worn) Front Unfold Setup Photo (5mm)



Body(Worn) Unfold Setup Photo (5mm)



Body Front Fold Setup Photo (5mm)



Body Back Fold Setup Photo (5mm)

