


## LIST OF COMPONENTS



- ① User Guide
- ② **Basic Buddy®+ add-on kit.**  
Requires 2 "AAA" batteries (not included).  
3.0V  $\equiv$  205mA (Using two Alkaline 1.5V Batteries)

- ③ Lung Bag with Sensor Holder

Additional instructions  
packaged with the manikin.

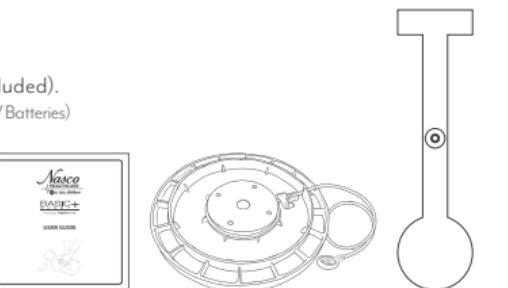


## DOWNLOAD APPS

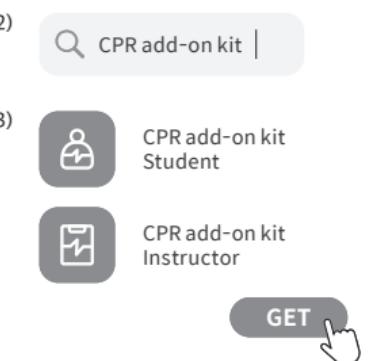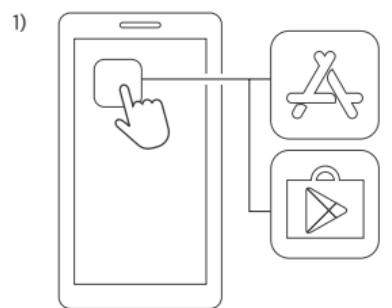


Student and instructor apps run on Apple® iPhone® devices. Apple® iPad® version apps will be available February 2019.  
Android™ version apps will be available in the first half of 2019. (iPad®, Android™, and Apple® tablet/phone not included).

## HOW TO INSTALL


1

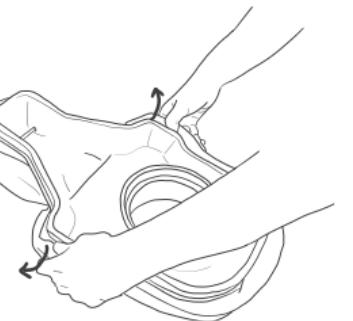

2

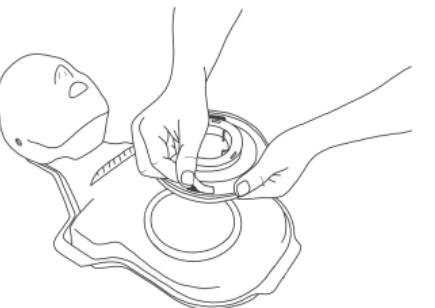


3

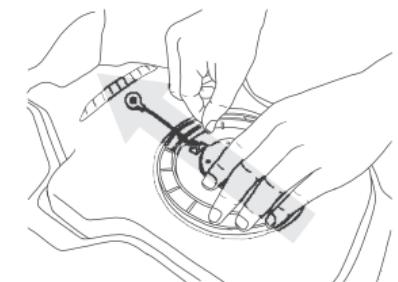

4



5

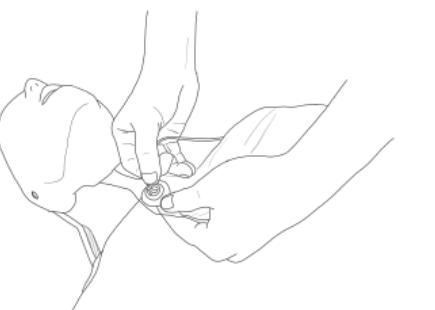

6



Actual product may vary slightly from photo.

Nasco reserves the right to change product color, materials, supplies, or function as needed.

## WARRANTY

1. Manufacturer offers a LIMITED WARRANTY against any defects in workmanship or materials under normal use for one (1) year from the date of purchase. Any component of the **Basic Buddy®+** add-on kit which proves defective within the warranty period will be repaired, free of charge. The customer is responsible for shipping and handling fees to the place which manufacturer designates.
2. Customer must provide proof of the date of purchase, place of purchase and the purchase price in order to obtain service under this limited warranty. No agent, representative, dealer of Manufacturer has the authority to alter the obligations or limitations of this limited warranty.
3. CUSTOMER'S SOLE AND EXCLUSIVE REMEDY AGAINST MANUFACTURE SHALL BE FOR THE REPAIR OR REPLACEMENT OF DEFECTIVE GOODS AS PROVIDED HEREIN. Repair of any component of any **Basic Buddy®+** add-on kit does not extend this limited warranty or begin a new limited warranty period.
4. Manufacturer reserves the right to refuse warranty service or replacement when product failure is due to abrasion, abnormal use, misuse, mishandling, misapplication, accident, neglect, improper installation, modification, use of unauthorized parts or attachments, adjustments or repair performed by anyone other than manufacturer or its authorized agent, or any causes other than defective workmanship or material. This limited warranty does not cover failure or damage resulting from unsuitable operating environments or storing environments or natural disasters or acts of God. MANUFACTURER SHALL NOT BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES ARISING OUT OF THE USE OF THE **Basic Buddy®+** add-on kit OR THE BREACH OF THIS OR ANY OTHER EXPRESSED OR IMPLIED WARRANTY.

## PRODUCT INFORMATION

<b>Product Name</b>	CPR add-on Kit (for <b>Basic Buddy®+</b> )
<b>Model</b>	AK1G BB
<b>Developer</b>	I.M. LAB Inc.
<b>Manufacturer Info.</b>	I.M. LAB Inc. / 7F, 165, Yeoksam-ro, Gangnam, Seoul, Korea
<b>Authorization Code</b>	FCC. / CE.
<b>Class B Device</b>	

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

### ⚠ CAUTION

- Keep the used batteries out of reach of children and dispose separately.
- If you do not use HeartiSense for a long period of time remove and store the batteries.
- Do not use a new battery and an old battery together.



ONLINE [NascoHealthcare.com](http://NascoHealthcare.com)  
EMAIL [lifeform@enasco.com](mailto:lifeform@enasco.com)  
PHONE 1.800.431.4310  
ADDRESS 901 Janesville Ave.  
Fort Atkinson, WI 53538

Copyright © 2019 HCI9000IINMI



**BASIC+**  
BUDDY

Powered by **heartisense™**

## USER GUIDE




## LIST OF COMPONENTS



- ① User Guide
- ② **Basic Buddy®+** add-on kit.  
Requires 2 "AAA" batteries (not included).  
3.0V  $\equiv$  205mA (Using two Alkaline 1.5V Batteries)

- ③ Lung Bag with Sensor Holder

Additional instructions  
packaged with the manikin.

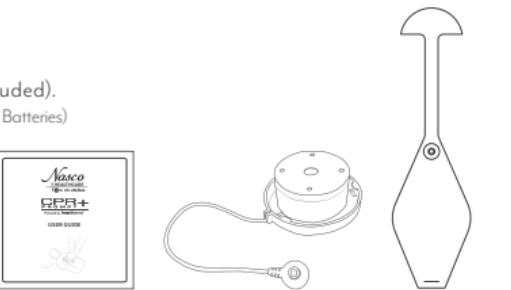


## DOWNLOAD APPS

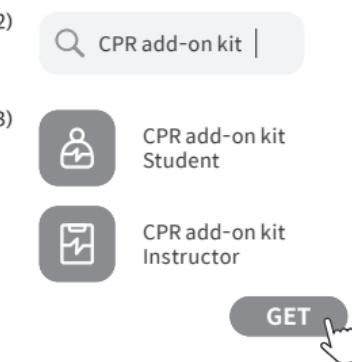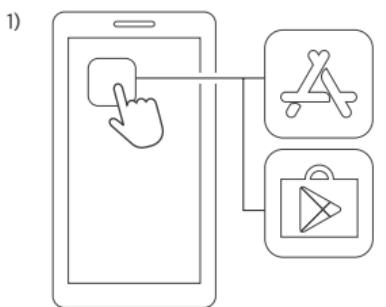


Student and instructor apps run on Apple® iPhone® devices. Apple® iPad® version apps will be available February 2019.  
Android™ version apps will be available in the first half of 2019. (iPad®, Android™, and Apple® tablet/phone not included).

## HOW TO INSTALL

1

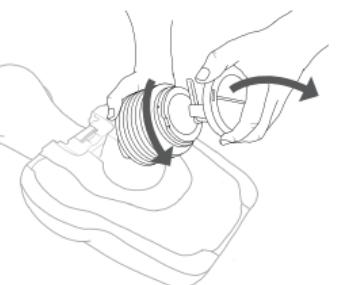


2

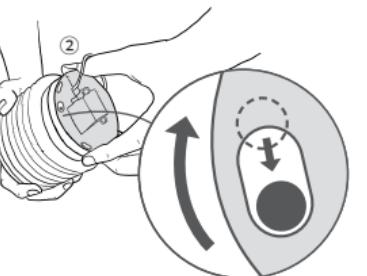

3



4

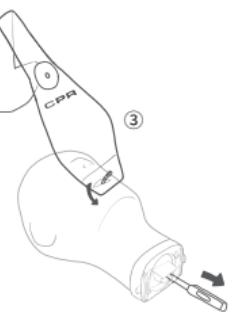

5



6



Actual product may vary slightly from photo.  
Nasco reserves the right to change product color, materials, supplies, or function as needed.

## WARRANTY

1. Manufacturer offers a LIMITED WARRANTY against any defects in workmanship or materials under normal use for one (1) year from the date of purchase. Any component of the **CPR Prompt®+** add-on kit which proves defective within the warranty period will be repaired, free of charge. The customer is responsible for shipping and handling fees to the place which manufacturer designates.
2. Customer must provide proof of the date of purchase, place of purchase and the purchase price in order to obtain service under this limited warranty. No agent, representative, dealer of Manufacturer has the authority to alter the obligations or limitations of this limited warranty.
3. CUSTOMER'S SOLE AND EXCLUSIVE REMEDY AGAINST MANUFACTURE SHALL BE FOR THE REPAIR OR REPLACEMENT OF DEFECTIVE GOODS AS PROVIDED HEREIN. Repair of any component of any **CPR Prompt®+** add-on kit does not extend this limited warranty or begin a new limited warranty period.
4. Manufacturer reserves the right to refuse warranty service or replacement when product failure is due to abrasion, abnormal use, misuse, mishandling, misapplication, accident, neglect, improper installation, modification, use of unauthorized parts or attachments, adjustments or repair performed by anyone other than manufacturer or its authorized agent, or any causes other than defective workmanship or material. This limited warranty does not cover failure or damage resulting from unsuitable operating environments or storing environments or natural disasters or acts of God. MANUFACTURER SHALL NOT BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES ARISING OUT OF THE USE OF THE **CPR Prompt®+** add-on kit OR THE BREACH OF THIS OR ANY OTHER EXPRESSED OR IMPLIED WARRANTY.

## PRODUCT INFORMATION

<b>Product Name</b>	CPR add-on Kit (for <b>CPR Prompt®+</b> )
<b>Model</b>	AK1G PT
<b>Developer</b>	I.M. LAB Inc.
<b>Manufacturer Info.</b>	I.M. LAB Inc. / 7F, 165, Yeoksam-ro, Gangnam, Seoul, Korea
<b>Authorization Code</b>	FCC. / CE.
<b>Class B Device</b>	

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

### ⚠ CAUTION

- Keep the used batteries out of reach of children and dispose separately.
- If you do not use HeartiSense for a long period of time remove and store the batteries.
- Do not use a new battery and an old battery together.



ONLINE [NascoHealthcare.com](http://NascoHealthcare.com)  
EMAIL [lifeform@enasco.com](mailto:lifeform@enasco.com)  
PHONE 1.800.431.4310  
ADDRESS 901 Janesville Ave.  
Fort Atkinson, WI 53538

Copyright © 2019 HCI9000IINM12



**CPR+**  
P R O M P T

Powered by **heartisense™**

## USER GUIDE

