

vitls



FW

1.11



2022-06-21

LOT

1110

REF

VT-F-010-V2

FCC




FCC ID: 2ASYD-VT-F-010-V2



P_X
ONLY





IP27



Vitls Inc.
2450 Holcombe Blvd
Houston, TX 77021
hello@vitlsinc.com



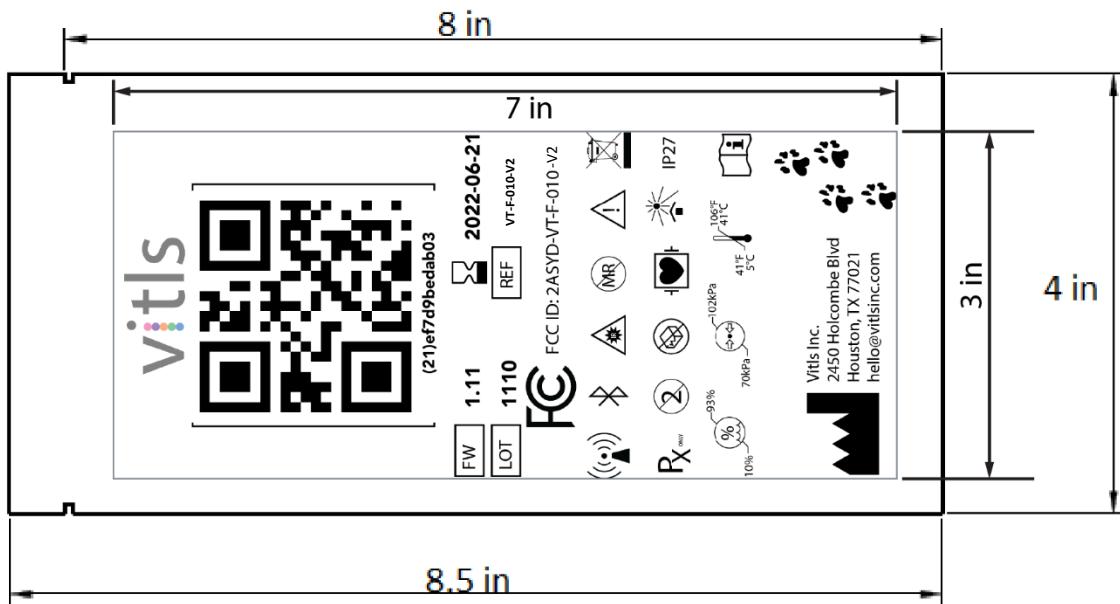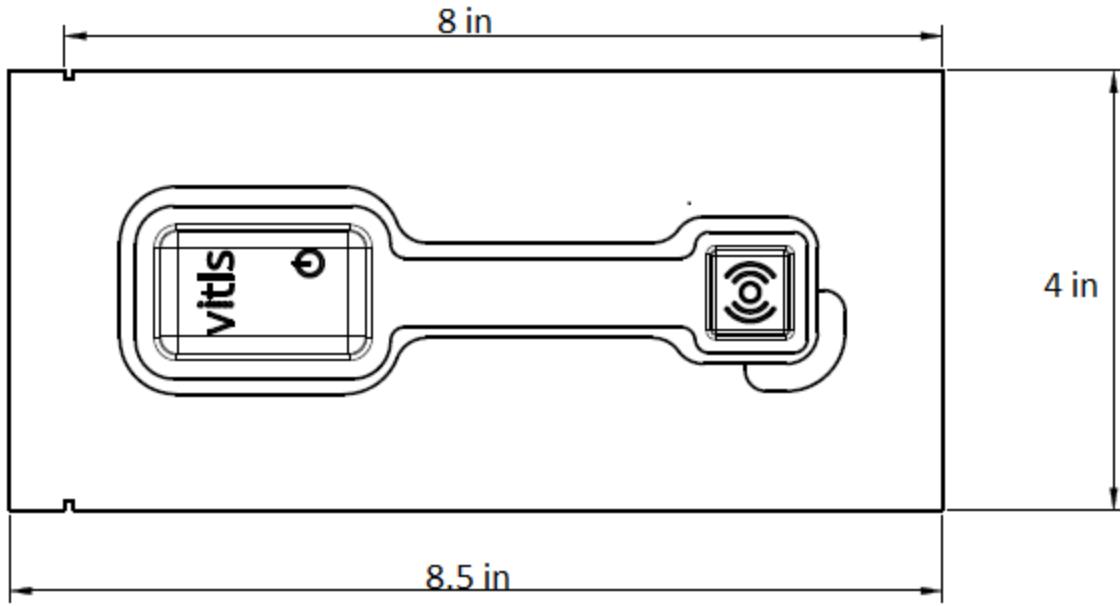

Label will be printed on a medical grade FDA approved adhesive material and adhered to the dissipative bags used for containing the VT-F-010-V2 during shipping and storage.

External labeling is not practical for the following reasons:

- 1) Product dimensionally is too small to apply a label.
- 2) Product foam material will not bond well with an external label.
- 3) Medical usage of the product will result in labeling potentially falling off.

The FCC has provided in KDB 784784 D01, Section 3, that instead of placing labels on a device externally, a grantee may elect to place the FCC ID labeling in an alternate location in such scenarios.

The labeling of the product will be placed on the exterior of the product packaging and the FCC ID of the product will also be noted in the product's Instructions for Use (IFU).