



Canada

## **Exhibit: Test Setup Photos**

Report File #: 7169006356RC-000

© TÜV SÜD Canada Inc. This test report shall not be reproduced except in full, without written approval of TÜV SÜD Canada Inc

Client	<b>Innovere Medical Inc.</b>	
Product	<b>IVID0608</b>	
Standard(s)	FCC 15.407 (b) & RSS-247 Clause 6.2.1.2	



Figure 1 – Radiated Emissions Setup – Photo 1

Client	<b>Innovere Medical Inc.</b>	
Product	<b>IVID0608</b>	
Standard(s)	FCC 15.407 (b) & RSS-247 Clause 6.2.1.2	



Figure 2 – Radiated Emissions Setup – Photo 2

Client	<b>Innovere Medical Inc.</b>	
Product	<b>IVID0608</b>	
Standard(s)	FCC 15.407 (b) & RSS-247 Clause 6.2.1.2	

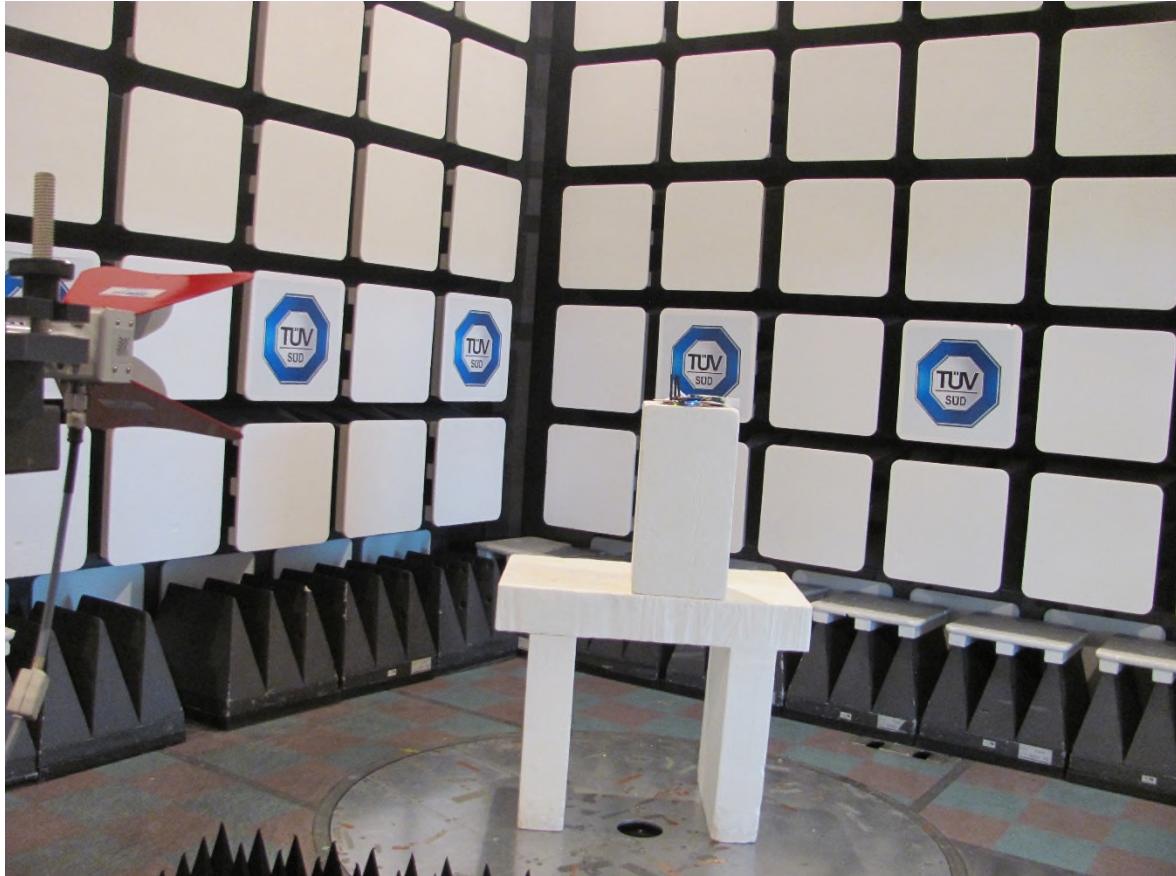


Figure 3 – Radiated Emissions Setup – Photo 3

Note: As per ANSI C63.10-2013 Clause 6.3.1, below 1GHz, the height of the EUT was set to 80cm. Above 1GHz, the height was raised to 1.5m.

Client	<b>Innovere Medical Inc.</b>	
Product	<b>IVID0608</b>	
Standard(s)	FCC 15.407 (b) & RSS-247 Clause 6.2.1.2	

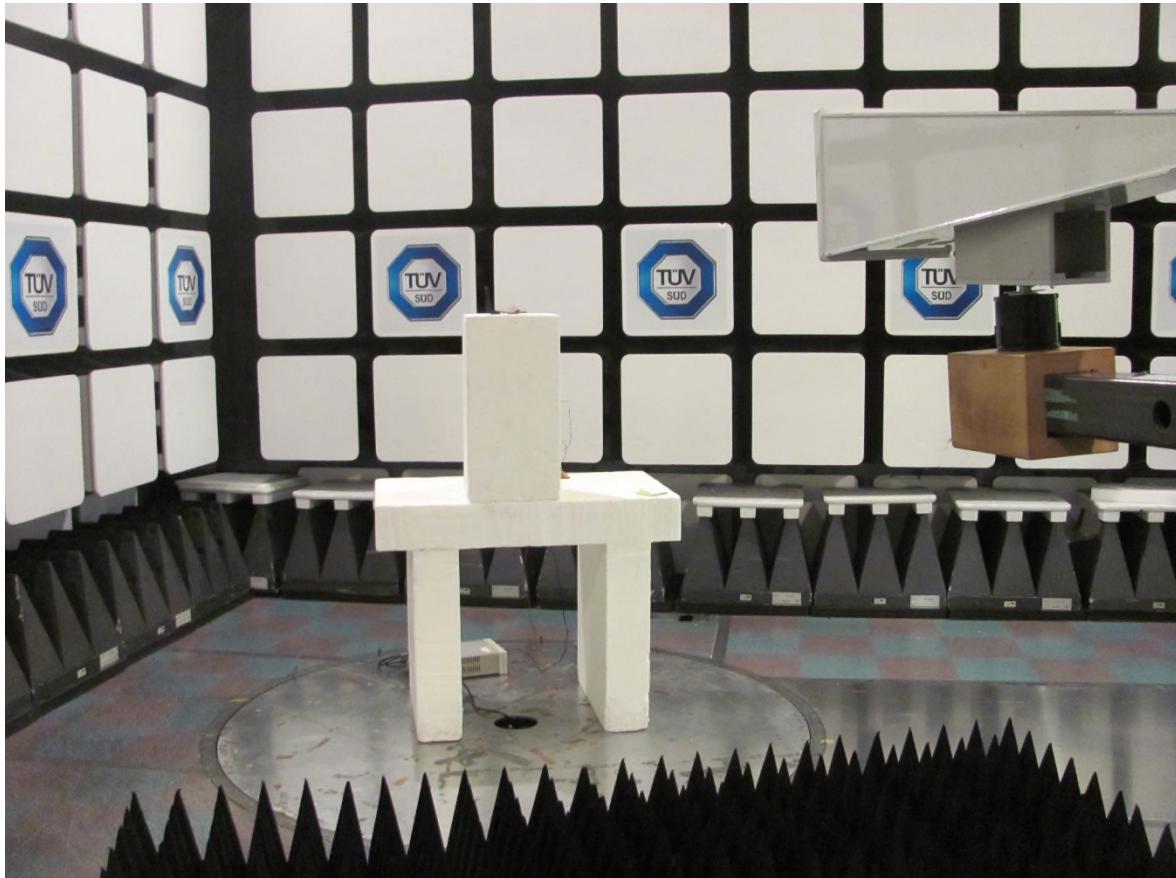


Figure 4 – Radiated Emissions Setup – Photo 4

Note: As per ANSI C63.10-2013 Clause 6.3.1, below 1GHz, the height of the EUT was set to 80cm. Above 1GHz, the height was raised to 1.5m.

Client	<b>Innovere Medical Inc.</b>	
Product	<b>IVID0608</b>	
Standard(s)	FCC 15.407 (b) & RSS-247 Clause 6.2.1.2	

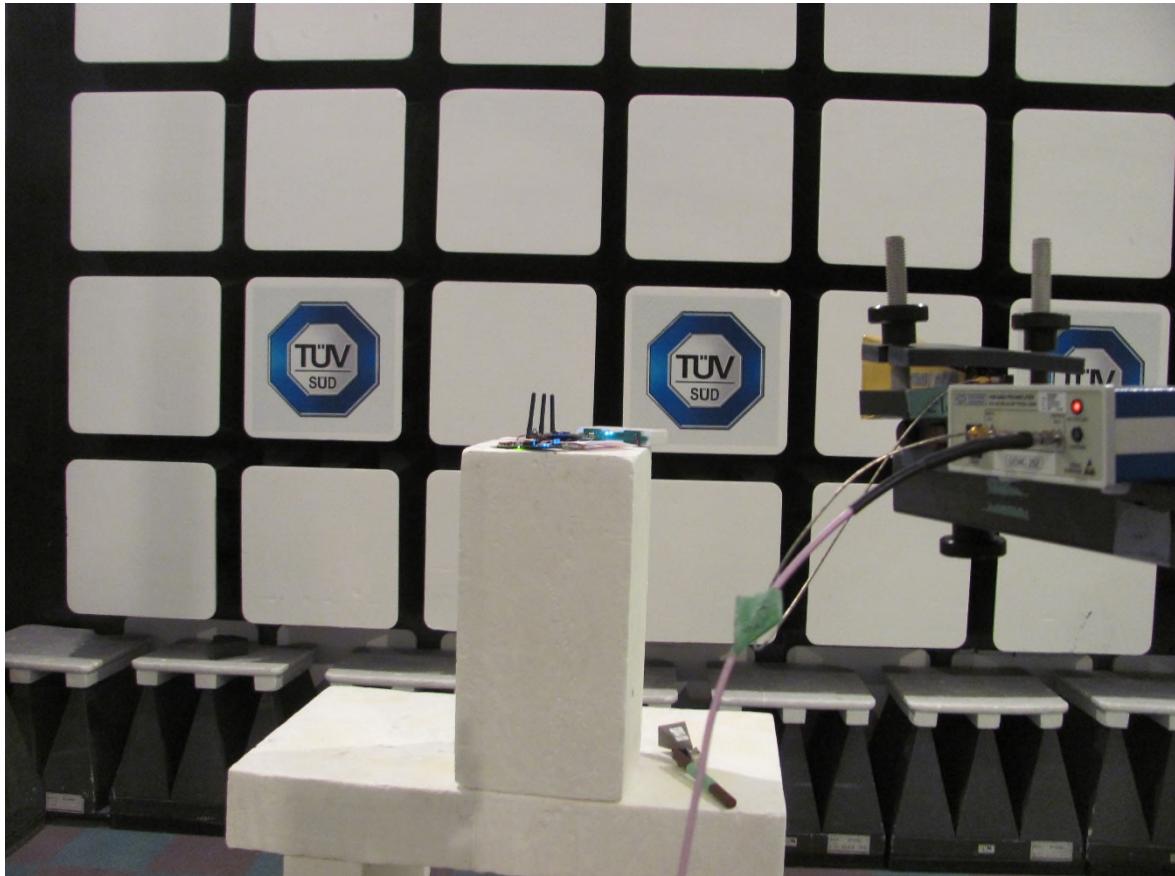


Figure 5 – Radiated Emissions Setup – Photo 5

Note: As per ANSI C63.10-2013 Clause 6.3.1, below 1GHz, the height of the EUT was set to 80cm. Above 1GHz, the height was raised to 1.5m.