

Annex D

Photo documentation

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid Head 600-6000MHz


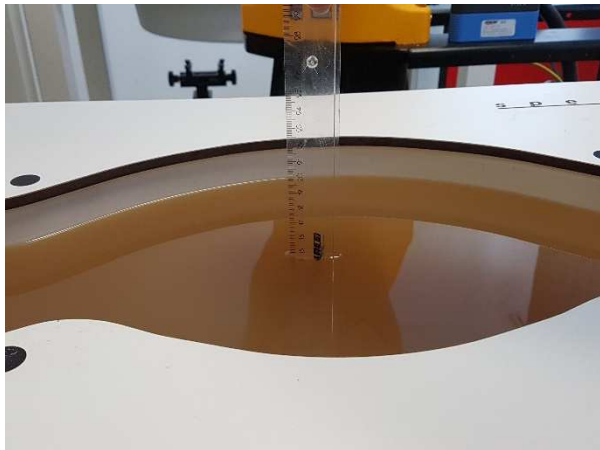


Photo 2: Tissue Simulant Liquid Head 600-6000MHz

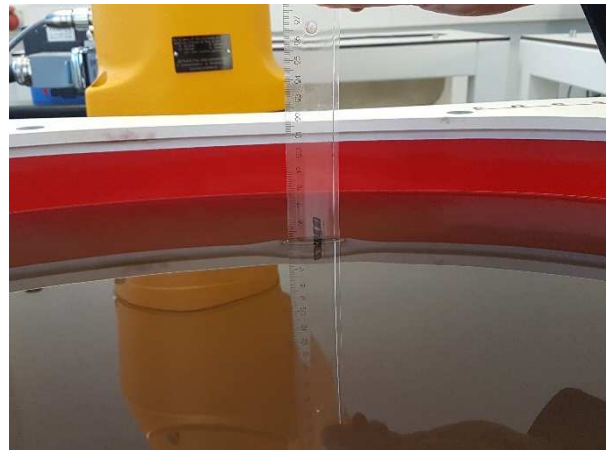

3. Photographs of EUT test position

Photo 1: Front side (DPM) 0mm



Photo 2: Back side (DPM) 0mm



Photo 3: Left side (DPM) 0mm



Photo 4: Right side (DPM) 0mm



Photo 5: Top side (DPM) 0mm



Photo 6: Top side (SPG) 0mm



Photo 7: Top side (DFT) 0mm



4. EUT Constructional Details

Photo 1: Front View



Photo 2: Back View



Photo 3: Front View (DPM) 0mm



Photo 4: Back view (DPM) 0mm



Photo 5: Front View (DFT) 0mm



Photo 6: Back View (DFT) 0mm



Photo 7: Front View (SPG) 0mm

Photo 8: Front View (SPG) 0mm