

**EMC TEST REPORT****FCC 47 CFR Part 15B, ISED ICES-003 Issue 6**

|  |  |
|--|--|
| <b>Report Reference No</b>               | G0M-2003-8888-EF0115B-V01  |
| <b>Testing Laboratory</b>                | Eurofins Product Service GmbH  |
| Address                                  | Storkower Str. 38c<br>15526 Reichenwalde<br>Germany  |
| Accreditation                            |    <br>DAkkS - Registration number : D-PL-12092-01-03 (ISED)<br>ISED Testing Laboratory site: 3470A-2<br>DAkkS - Registration number : D-PL-12092-01-04 (FCC)<br>FCC Filed Test Laboratory, Reg.-No.: 96970 |
| <b>Applicant</b>                         | GWA Hygiene GmbH   |
| Address                                  | Heinrich-Mann-Str. 11<br>18435 Stralsund<br>GERMANY  |
| <b>Test Specification</b><br>Standard(s) | 47 CFR Part 15 Subpart B<br>ISED ICES-003 Issue 6<br>ANSI C63.4:2014+A1:2017   |
| Non-Standard Test Method                 | None   |
| <b>Equipment under Test (EUT):</b>       |  |
| Product Description                      | Hygiene-Monitoring-System  |
| Model(s)                                 | NosoEx Point of Care / Drucksensor   |
| Additional Model(s)                      | None   |
| Brand Name(s)                            | None   |
| Hardware Version(s)                      | 1.7.1  |
| Software Version(s)                      | 2.17   |
| FCC-ID                                   | 2AU27NOSOEX002   |
| IC                                       | n/a  |
| <b>Test Result</b>                       | <b>PASSED</b>  |

| <b>Possible test case verdicts:</b>  |                  |   |
|--|------------------|---|
| required by standard but not tested  | N/T              |   |
| not required by standard   | N/R              |   |
| required by standard but not appl. to test object  | N/A              |   |
| test object does meet the requirement  | P(PASS)          |   |
| test object does not meet the requirement  | F(FAIL)          |   |
| <b>Testing:</b>  |                  |   |
| Date of receipt of test item   | 2020-03-27       |   |
| <b>Report:</b>   |                  |   |
| Compiled by  | Matthias Handrik |   |
| Tested by (+ signature)<br>(Responsible for Test)  | Matthias Handrik |    |
| Approved by (+ signature)<br>(Deputy Head of Lab)  | Jens Marquardt   |  |
| Date of Issue  | 2020-04-29       |   |
| Total number of pages  | 26               |   |
| <b>General Remarks:</b>  |                  |   |
| <p><b>The test results presented in this report relate only to the object tested.</b></p> <p><b>The results contained in this report reflect the results for this particular model and serial number. It is the responsibility of the manufacturer to ensure that all production models meet the intent of the requirements detailed within this report.</b></p> <p>This report shall not be reproduced, except in full, without the written approval of the issuing testing laboratory.</p> |                  |   |
| <b>Additional Comments:</b>  |                  |   |
|  |                  |   |

**ABBREVIATIONS AND ACRONYMS**

| <b>Acronyms</b> |   |
|-----------------|---|
| Acronym         | Description   |
| EUT             | Equipment Under Test                                |
| FCC             | Federal Communications Commission                   |
| ISED            | Innovation, Science and Economic Development Canada |
| $T_{NOM}$       | Nominal operating temperature                       |
| $V_{NOM}$       | Nominal supply voltage                              |

**VERSION HISTORY**

| <b>Version History</b> |            |                 |            |
|------------------------|------------|-----------------|------------|
| Version                | Issue Date | Remarks         | Revised By |
| 01                     | 2020-04-29 | Initial Release | -          |

**REPORT INDEX**

|          |  |           |
|----------|--|-----------|
| <b>1</b> | <b>Equipment (Test Item) Under Test.....</b>                             | <b>6</b>  |
| 1.1      | Equipment Ports.....   | 7         |
| 1.2      | Equipment Photos - Internal.....   | 8         |
| 1.3      | Equipment Photos - External.....   | 9         |
| 1.4      | Support Equipment.....   | 11        |
| 1.5      | Operational Modes.....   | 12        |
| 1.6      | EUT Configuration.....   | 13        |
| 1.7      | Sample emission level calculation.....                                   | 14        |
| <b>2</b> | <b>Result Summary.....</b>   | <b>15</b> |
| 2.1      | Test Conditions and Results - Radiated emissions acc. to ANSI C63.4..... | 16        |

## 1 Equipment (Test Item) Under Test


|                                  |   |  |
|----------------------------------|---|--|
| Description                      | Hygiene-Monitoring-System   |  |
| Model                            | NosoEx Point of Care / Drucksensor                                      |  |
| Additional Model(s)              | None  |  |
| Brand Name(s)                    | None  |  |
| Serial Number(s)                 | 2019030000000004  |  |
| Hardware Version(s)              | 1.7.1   |  |
| Software Version(s)              | 2.17  |  |
| Dimension[cm]                    | 6.7 x 6.7 x 2.1   |  |
| FCC-ID                           | 2AU27NOSOEX002  |  |
| IC                               | n/a   |  |
| Class                            | Class B   |  |
| Equipment type                   | Table top   |  |
| Highest internal frequency [MHz] | 48; 2480 (Bluetooth Low Energy carrier)                                 |  |
| Radio Module                     | Type  | Bluetooth Low Energy module                |
|                                  | Model   | Unspecified                                |
|                                  | Manufacturer  | Unspecified                                |
|                                  | FCC-ID  | Unspecified                                |
|                                  | IC  | Unspecified                                |
| Supply Voltage                   | V <sub>NOM</sub>  | 3 VDC (2x1.5V DC non rechargeable battery) |
| AC/DC-Adaptor                    | None  |  |
| Manufacturer                     | GWA Hygiene GmbH<br>Heinrich-Mann-Str. 11<br>18435 Stralsund<br>GERMANY |  |

## 1.1 Equipment Ports


| Name         | Type  | Attributes | Comment |  |
|--------------|---|------------|---------|--|
|              |   | None       |         |  |
| Description: |   |            |         |  |
| AC           | AC mains power input/output port                  |            |         |  |
| DC           | DC power input/output port                        |            |         |  |
| BAT          | DC power input port connected to external battery |            |         |  |
| IO           | Input/Output port                                 |            |         |  |
| TP           | Telecommunication port                            |            |         |  |
| NE           | Non-electrical port                               |            |         |  |

## 1.2 Equipment Photos - Internal


EUT PCB TOP

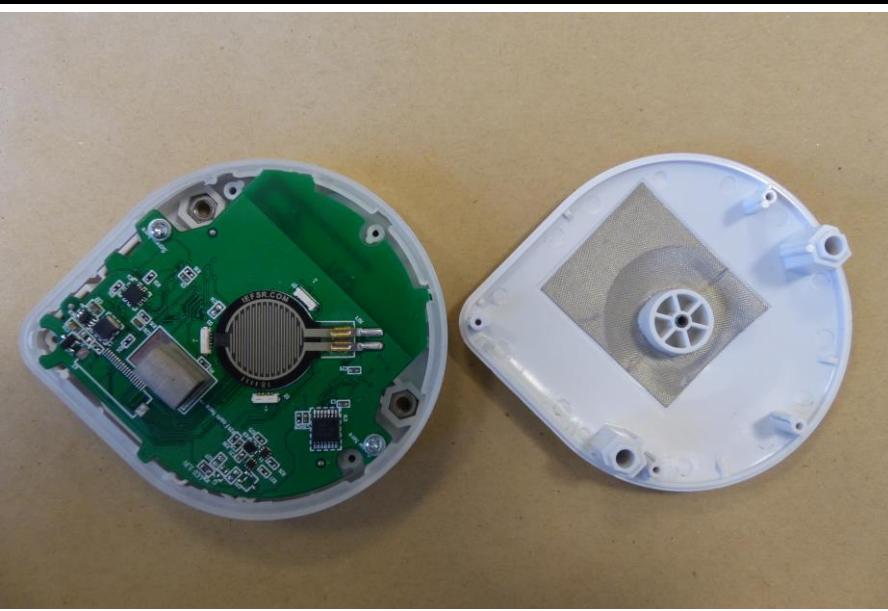


EUT PCB BOTTOM

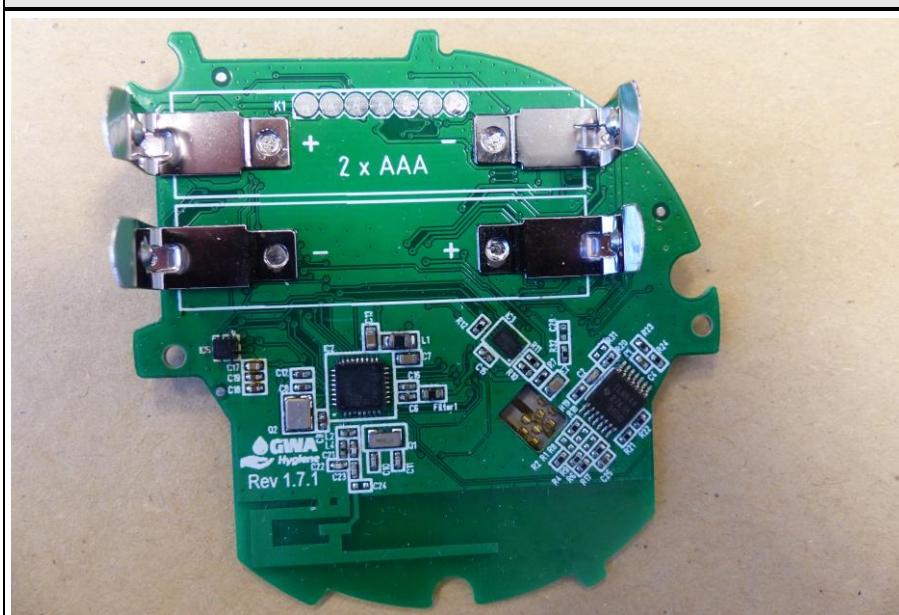

### 1.3 Equipment Photos - External

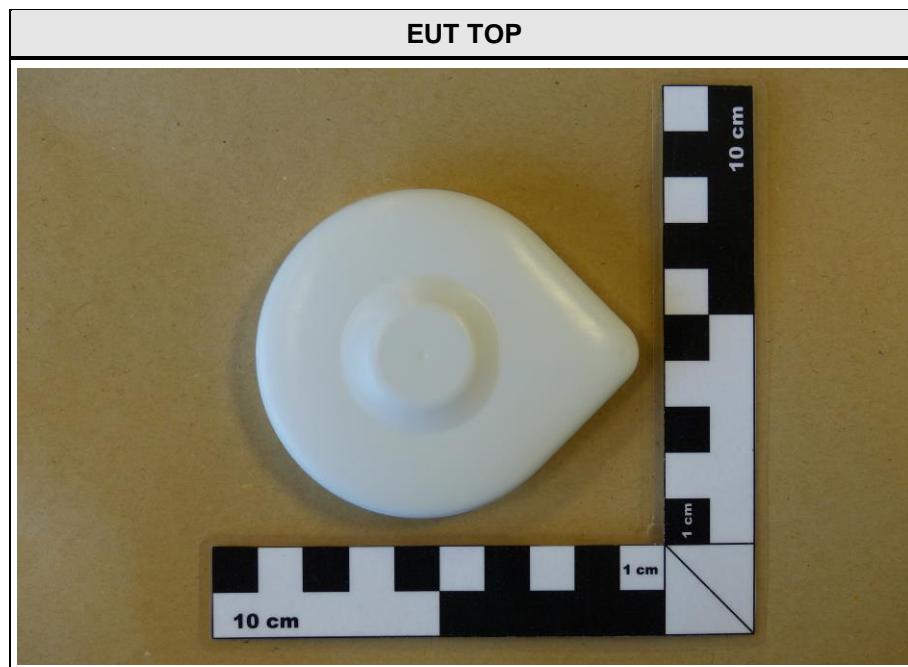

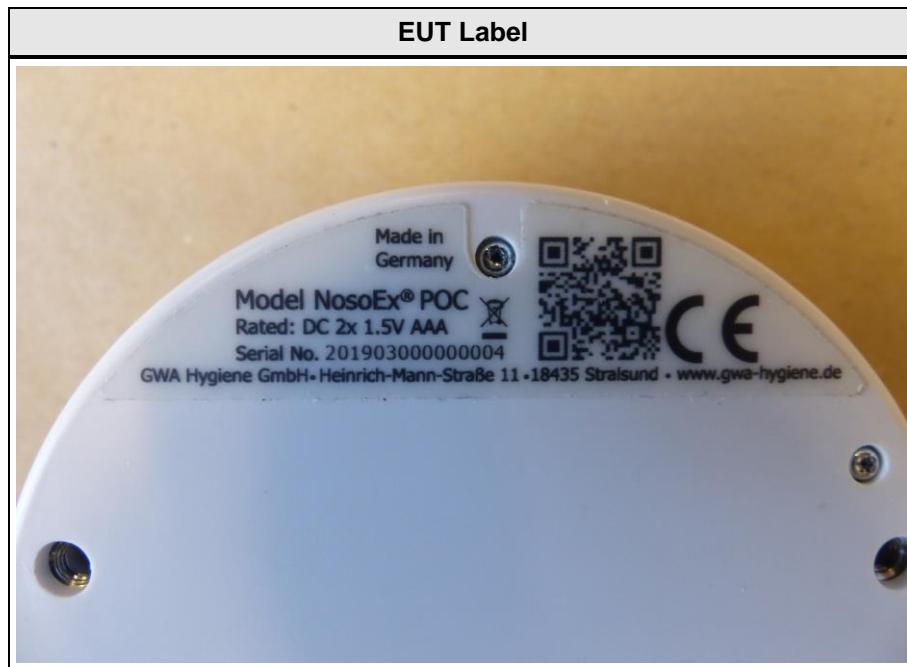

#### 1.4 Support Equipment

| Product Type | Device               | Manufacturer | Model   | Comment                       |
|--------------|----------------------|--------------|---------|-------------------------------|
| AE           | Tablet               | Samsung      | SM-T589 | Ser.: R52KA1PVAHL<br>Customer |
| AE           | Software application | GWA Hygiene  | 1.7.3   | Customer                      |
| Description: |                      |              |         |                               |
| AE           | Auxiliary Equipment  |              |         |                               |
| SIM          | Simulator            |              |         |                               |
| MON          | Monitoring Equipment |              |         |                               |
| CBL          | Connecting Cable     |              |         |                               |
| Comment:     |                      |              |         |                               |

### 1.5 Operational Modes

| Mode #   | Description   |
|----------|---|
| 1        | Bluetooth Low Energy connection to tablet.<br>Wait for activation by pushing on the top dome. |
| Comment: |   |

## 1.6 EUT Configuration

| Configuration # | Description  |
|-----------------|--|
| 1               | NosoEx POC detects activation by pushing on the top dome.<br>It will scan for BLE Devices like the Android tablet with activated app and will form a link to it and transmit sensor data.<br>Tablet is placed in the corner of the measurement chamber.<br>Software application counts activities of disinfections.. |
| Comment:        |  |

## 1.7 Sample emission level calculation

The following is a description of terms and a sample calculation, as appears in the radiated emissions data table. The numbers used in the calculation are for example only. There is no direct correlation to the specific data taken for the product described in this document:

Reading:

This is the reading obtained on the spectrum analyser in dB $\mu$ V. Any external preamplifiers used are taken into account through internal analyser settings.

A.F.:

This is the antenna factor for the receiving antenna. It is a conversion factor, which converts electric fields strengths to voltages, which can be measured directly on the spectrum analyser. It is treated as a loss in dB. Cable losses have been included with the A.F. to simplify the calculations. The antenna factor is used in calculations as follows:

$$\text{Reading on Analyser (dB}\mu\text{V)} + \text{A.F. (dB/m)} = \text{Net field strength (dB}\mu\text{V/m)}$$

Net:

This is the net field strength measurement (as shown above).

Limit:

This is the FCC Class B radiated emission limit (in units of dB $\mu$ V/m). The FCC limits are given in units of  $\mu$ V/m. The following formula is used to convert the units of  $\mu$ V/m to dB $\mu$ V/m:

$$\text{Limit (dB}\mu\text{V/m)} = 20 * \log (\mu\text{V/m})$$

Margin:

This is the margin of compliance below the FCC limit. The units are given in dB. A negative margin indicates the emission was below the limit. A positive margin indicates that the emission exceeds the limit.

Example only:

|                            |                     |   |                                       |           |
|----------------------------|---------------------|---|---------------------------------------|-----------|
| Reading + AF               | = Net Reading       | : | Net reading - FCC limit               | = Margin  |
| +21.5 dB $\mu$ V + 26 dB/m | = 47.5 dB $\mu$ V/m | : | 47.5 dB $\mu$ V/m - 57.0 dB $\mu$ V/m | = -9.5 dB |

## 2 Result Summary

| FCC 47 CFR Part 15B, ISED ICES-003 Issue 6 |                                   |                             |        |                  |
|--|-----------------------------------|-----------------------------|--------|------------------|
| Reference                                  | Requirement                       | Reference Method            | Result | Remarks          |
| Emission                                   |                                   |                             |        |                  |
| FCC 15.109<br>ICES-003, 6.2                | Radiated emissions                | ANSI C63.4:2014<br>+A1:2017 | PASS   | -                |
| FCC 15.107<br>ICES-003, 6.1                | AC power line conducted emissions | ANSI C63.4:2014<br>+A1:2017 | N/R    | No relevant port |
| Comment:                                   |                                   |                             |        |                  |



| Possible Test Case Verdicts |  |
|-----------------------------|--|
| PASS                        | Test object does meet the requirements       |
| FAIL                        | Test object does not meet the requirements   |
| N/T                         | Required by standard but not tested          |
| N/R                         | Not required by standard for the test object |



## 2.1 Test Conditions and Results - Radiated emissions acc. to ANSI C63.4

### 2.1.1 Information

| Test Information                 |                                   |
|----------------------------------|-----------------------------------|
| Reference                        | FCC 15.109, ICES-003, 6.2         |
| Reference method                 | ANSI C63.4:2014+A1:2017 Section 8 |
| Equipment class                  | Class B                           |
| Equipment type                   | Table top                         |
| Highest internal frequency [MHz] | 2480                              |
| Measurement range                | 30 MHz to 12400 MHz               |
| Temperature [°C]                 | 23                                |
| Humidity [%]                     | 23                                |
| Operator                         | Matthias Handrik                  |
| Date                             | 2020-04-20                        |

### 2.1.2 Setup

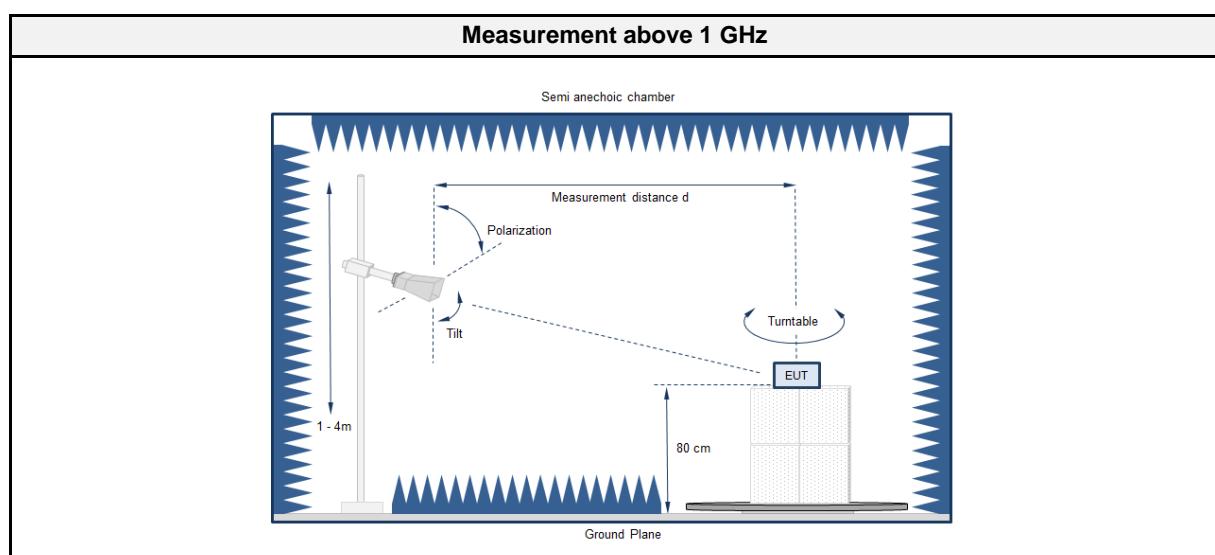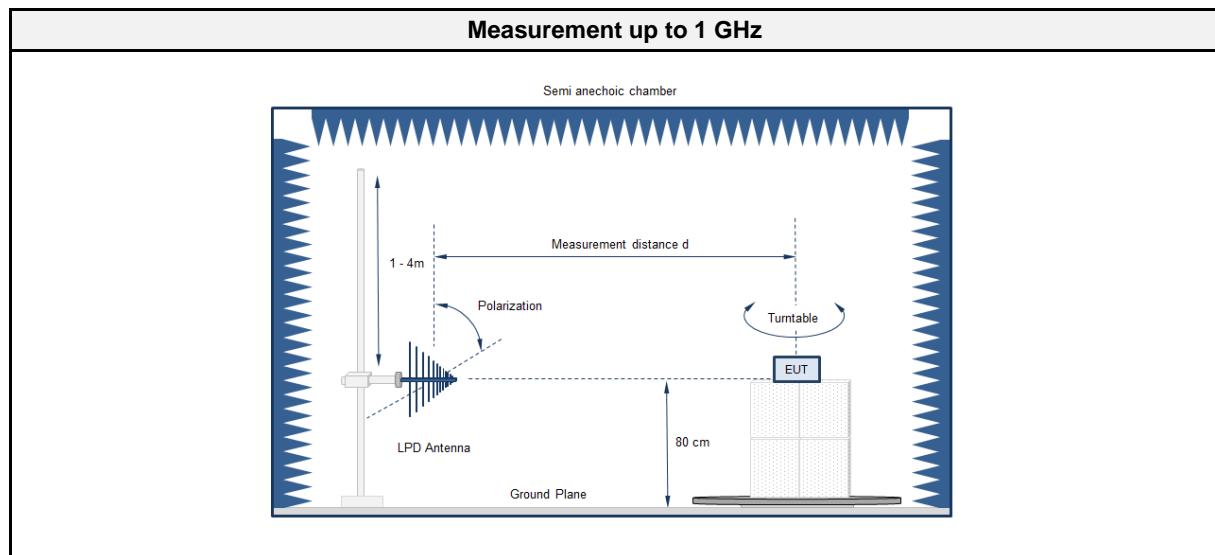

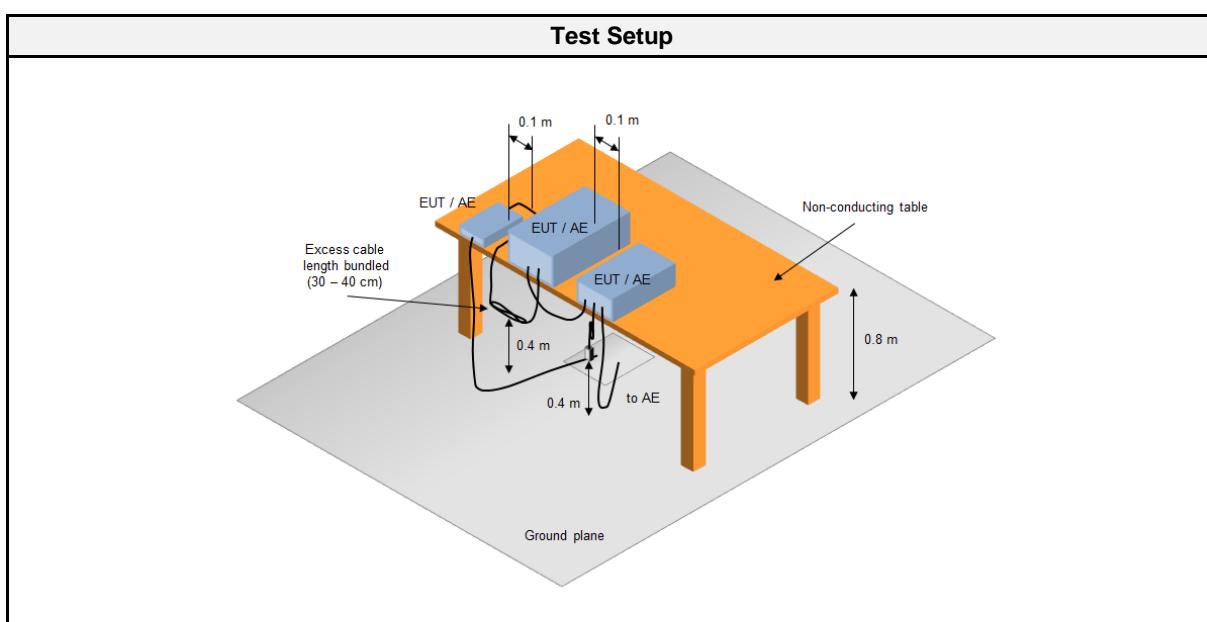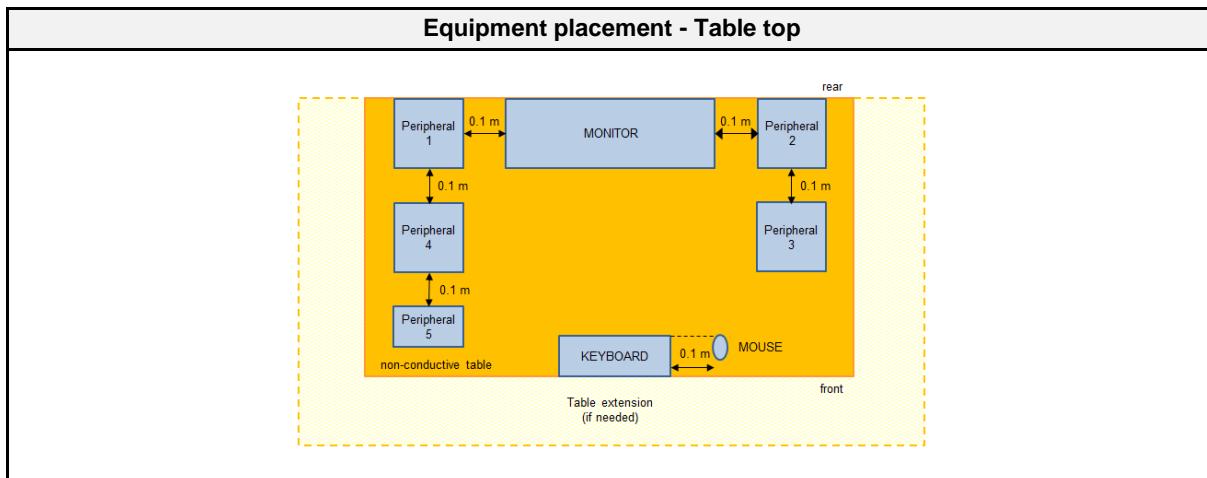

### 2.1.3 Equipment

| Test Software |                  |            |           |  |  |
|---------------|------------------|------------|-----------|--|--|
| Description   | Manufacturer     | Name       | Version   |  |  |
| EMC Software  | DARE Instruments | Radimation | 2016.1.10 |  |  |

| Test Equipment    |                             |                      |            |           |          |
|-------------------|-----------------------------|----------------------|------------|-----------|----------|
| Description       | Manufacturer                | Model                | Identifier | Cal. Date | Cal. Due |
| Anechoic chamber  | Frankonia                   | AC1                  | EF00062    | 2018-07   | 2021-07  |
| EMI Test Receiver | Keysight                    | N9038A-526/WXP       | EF01070    | 2019-09   | 2020-09  |
| Biconical Antenna | R&S                         | HK 116               | EF00030    | 2019-04   | 2022-04  |
| LPD Antenna       | R&S                         | HL 223               | EF00187    | 2019-05   | 2022-05  |
| Horn antenna      | Schwarzbeck                 | BBHA 9120D (1-18GHz) | EF00018    | 2019-10   | 2022-10  |
| Climatic Sensor   | Embedded Data Systems, LLC. | 2800100000254 17E    | EF01054    | 2019-05   | 2020-05  |
| Climatic Sensor   | Embedded Data Systems, LLC. | 0200100000253 77E    | EF01336    | 2019-05   | 2020-05  |

Test Report No.: G0M-2003-8888-EF0115B-V01

Eurofins Product Service GmbH  
Storkower Str. 38c, D-15526 Reichenwalde, Germany

#### 2.1.4 Procedure

| <b>Exploratory measurement</b>   |
|--|
| <ol style="list-style-type: none"> <li>1. The EUT was placed on a non-conductive table at a height of 0.8m.</li> <li>2. The EUT and support equipment, if needed, were set up to simulate typical usage.</li> <li>3. Cables, of type and length specified by the manufacturer, were connected to at least one port of each type and were terminated by a device or simulating load of actual usage.</li> <li>4. The antenna was placed at a distance of 3 or 10 m.</li> <li>5. The received signal was monitored at the measurement receiver.</li> <li>6. This procedure has to be performed in both antenna polarizations, horizontal and vertical.</li> <li>7. The arrangement of the equipment with the maximum emission level is shown on the setup picture at item 1.3</li> </ol> |

| <b>Final measurement</b>   |
|--|
| <ol style="list-style-type: none"> <li>1. The EUT was placed on a 0.8 m non-conductive table at a 3 m distance from the receive antenna. The antenna output was connected to the measurement receiver.</li> <li>2. A biconical antenna was used for the frequency range 30 – 200 MHz, a logarithmic periodical antenna was used for the frequency range from 200 – 1000 MHz. Above one 1 GHz a Double Ridged Broadband Horn antenna was used. The antenna was placed on an adjustable height antenna mast.</li> <li>3. The EUT and cable arrangement were based on the exploratory measurement results.</li> <li>4. Emissions were maximized at each frequency by rotating the EUT and adjusting the receive antenna height and polarization. The maximum values were recorded.</li> <li>5. The test data of the worst-case conditions were recorded and shown on the next pages.</li> </ol> |



#### 2.1.5 Limits



| <b>Class B @ 3 m</b> |                 |                         |
|----------------------|-----------------|-------------------------|
| Frequency<br>[MHz]   | Detector        | Limit<br>[dB $\mu$ V/m] |
| 30 - 88              | Quasi-peak      | 40                      |
| 88 - 216             | Quasi-peak      | 43.5                    |
| 216 - 960            | Quasi-peak      | 46                      |
| 960 - 1000           | Quasi-peak      | 54                      |
| > 1000               | Peak<br>Average | 74<br>54                |

#### 2.1.6 Results

| <b>Test Results</b> |                   |         |        |
|---------------------|-------------------|---------|--------|
| Operational mode    | EUT Configuration | Verdict | Remark |
| 1                   | 1                 | PASS    | -      |

2.1.7 Setup Photos

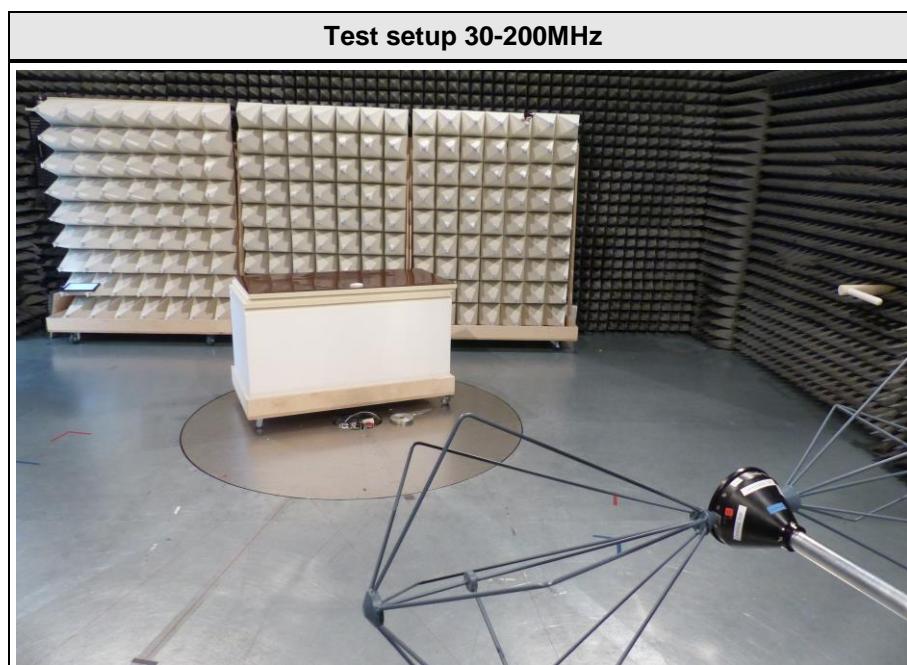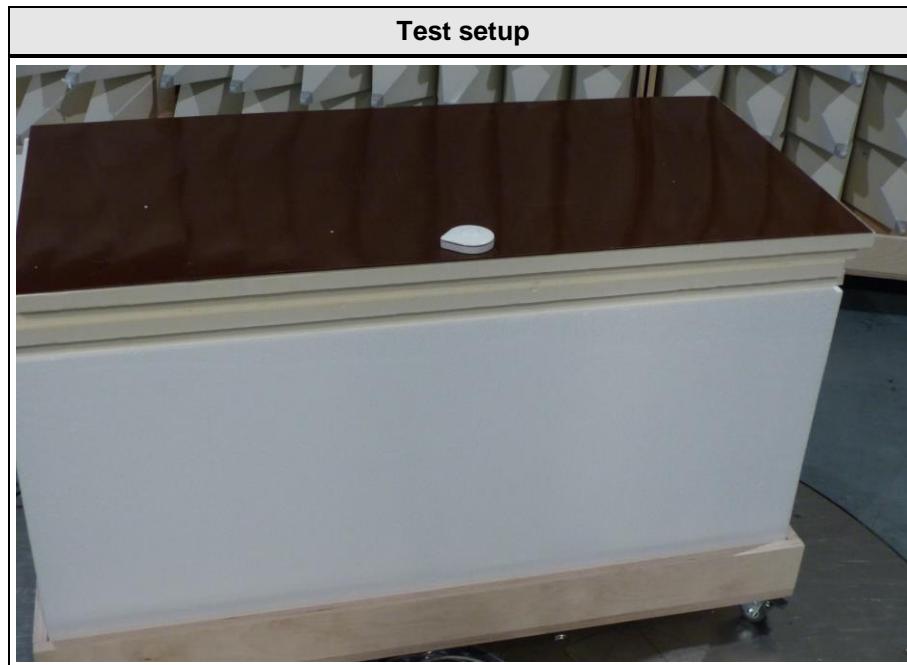

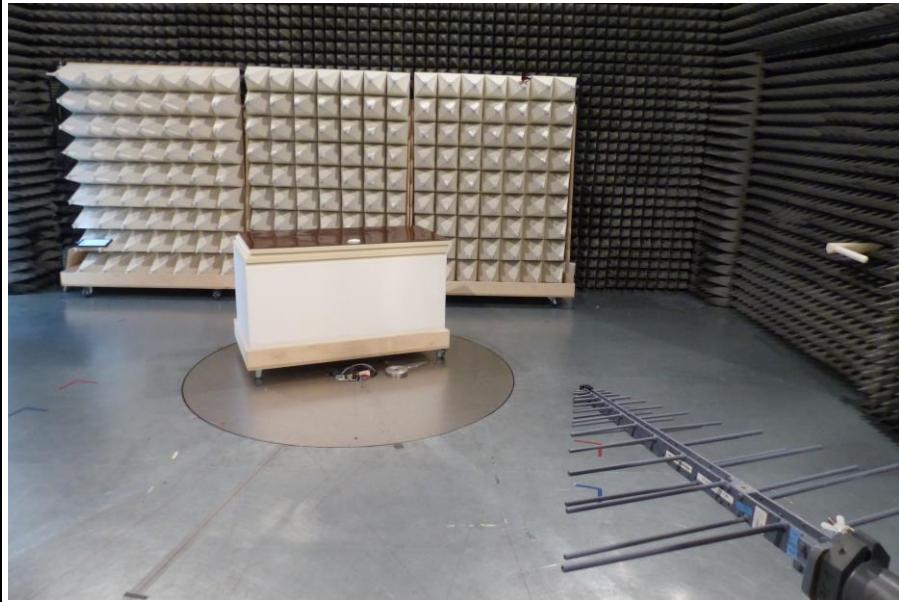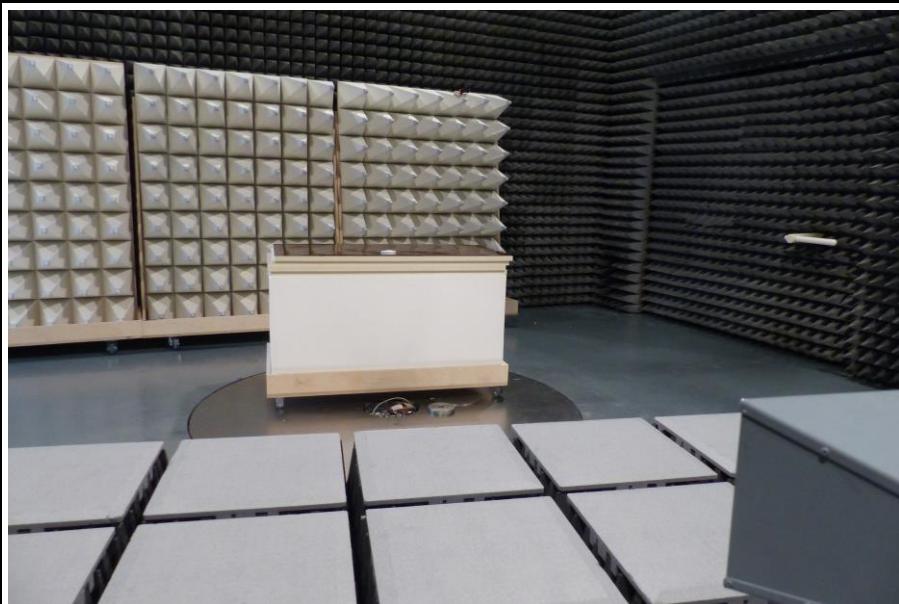
**Test setup 200-1000MHz****Test setup 1-13GHz**

## 2.1.8 Records

### Radiated emissions according to FCC part 15B

Project Number: G0M-2003-8888  
Applicant: GWA Hygiene GmbH  
Model Description: Hygiene-Monitoring-System  
Model: NosoEx Point of Care / Drucksensor  
Test Sample ID: 28705  
Test Site: Eurofins Product Service GmbH  
Operator: Mr. Handrik  
Test Date: 2020-04-20  
Operating Conditions: ambient temperature: 23°C  
Operating Conditions: power input: 2x1.5V DC (non rechargeable battery)  
Antenna: Rohde & Schwarz HK 116, Vertical  
Measurement Distance: 3m  
Mode: 1  
Note 1:


Index 53

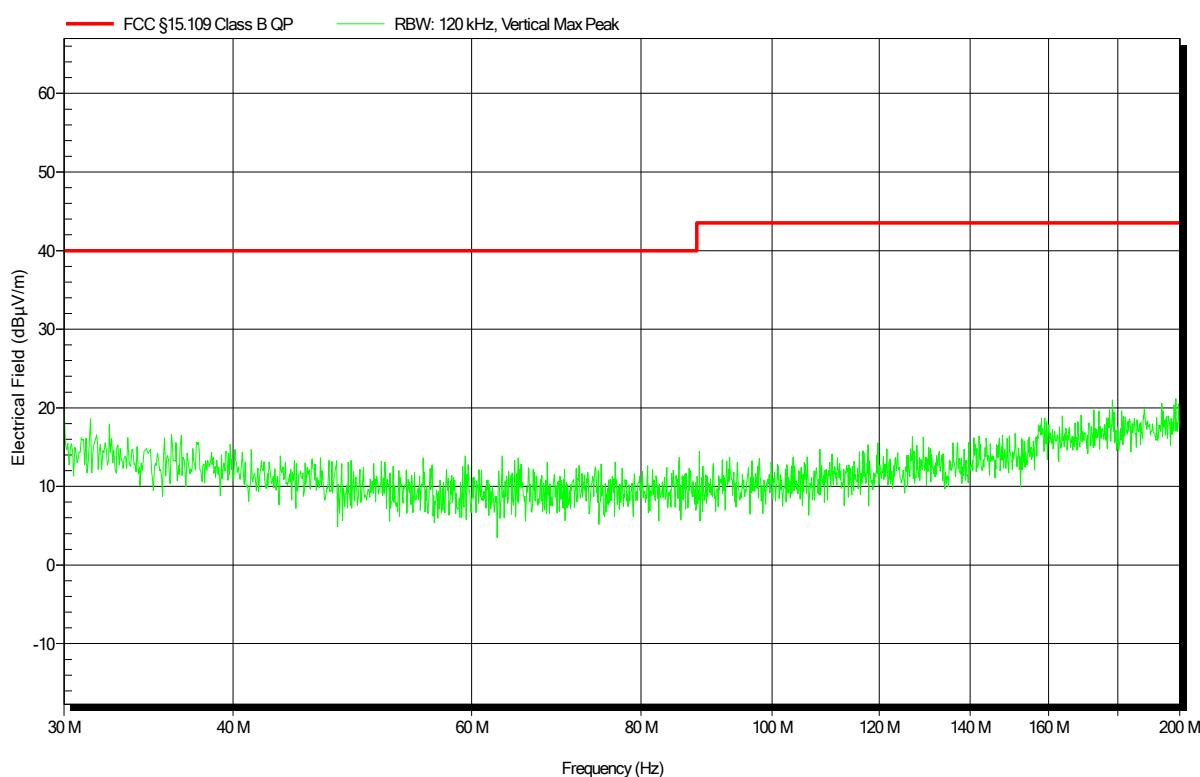

## Radiated emissions according to FCC part 15B

Project Number: G0M-2003-8888  
Applicant: GWA Hygiene GmbH  
Model Description: Hygiene-Monitoring-System  
Model: NosoEx Point of Care / Drucksensor  
Test Sample ID: 28705  
Test Site: Eurofins Product Service GmbH  
Operator: Mr. Handrik  
Test Date: 2020-04-20  
Operating Conditions: ambient temperature: 23°C  
power input: 2x1.5V DC (non rechargeable battery)  
Antenna: Rohde & Schwarz HK 116, Horizontal  
Measurement Distance: 3m  
Mode: 1  
Note 1:


Index 54

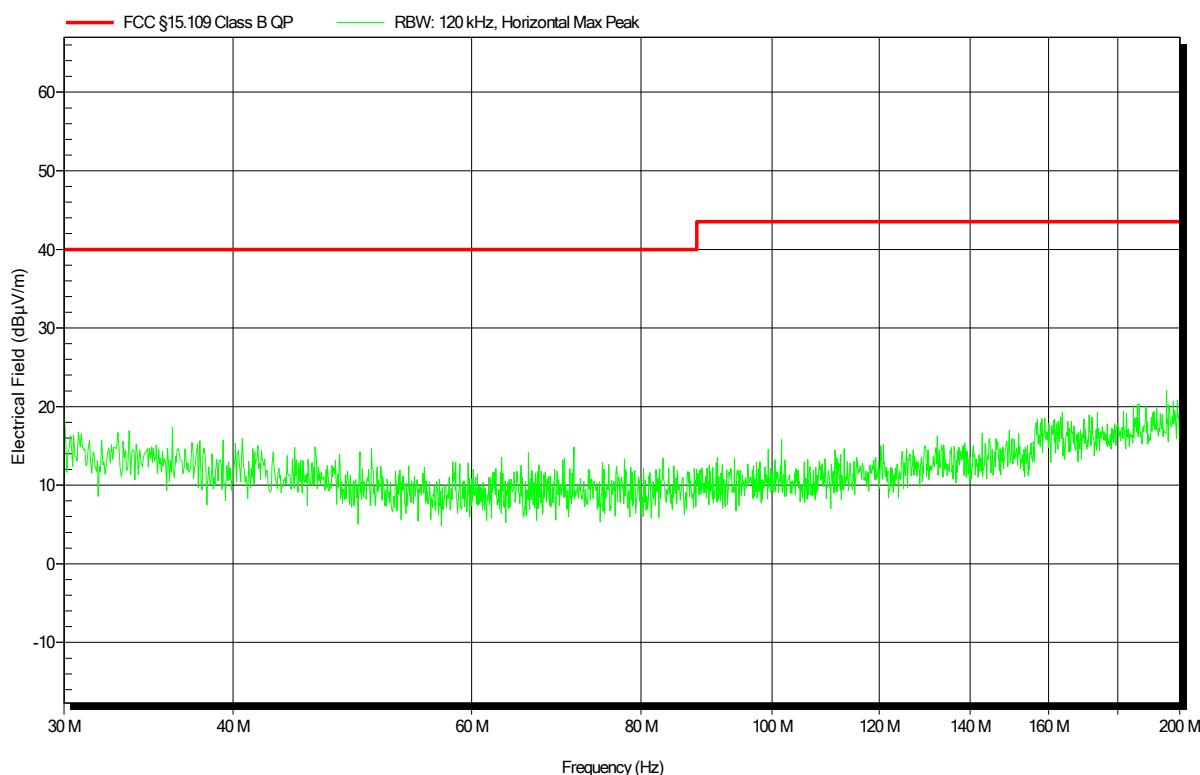

## Radiated emissions according to FCC part 15B

Project Number: G0M-2003-8888  
Applicant: GWA Hygiene GmbH  
Model Description: Hygiene-Monitoring-System  
Model: NosoEx Point of Care / Drucksensor  
Test Sample ID: 28705  
Test Site: Eurofins Product Service GmbH  
Operator: Mr. Handrik  
Test Date: 2020-04-20  
Operating Conditions: ambient temperature: 23°C  
power input: 2x1.5V DC (non rechargeable battery)  
Antenna: Rohde & Schwarz HL 223, Vertical  
Measurement Distance: 3m  
Mode: 1  
Note 1:


Index 55

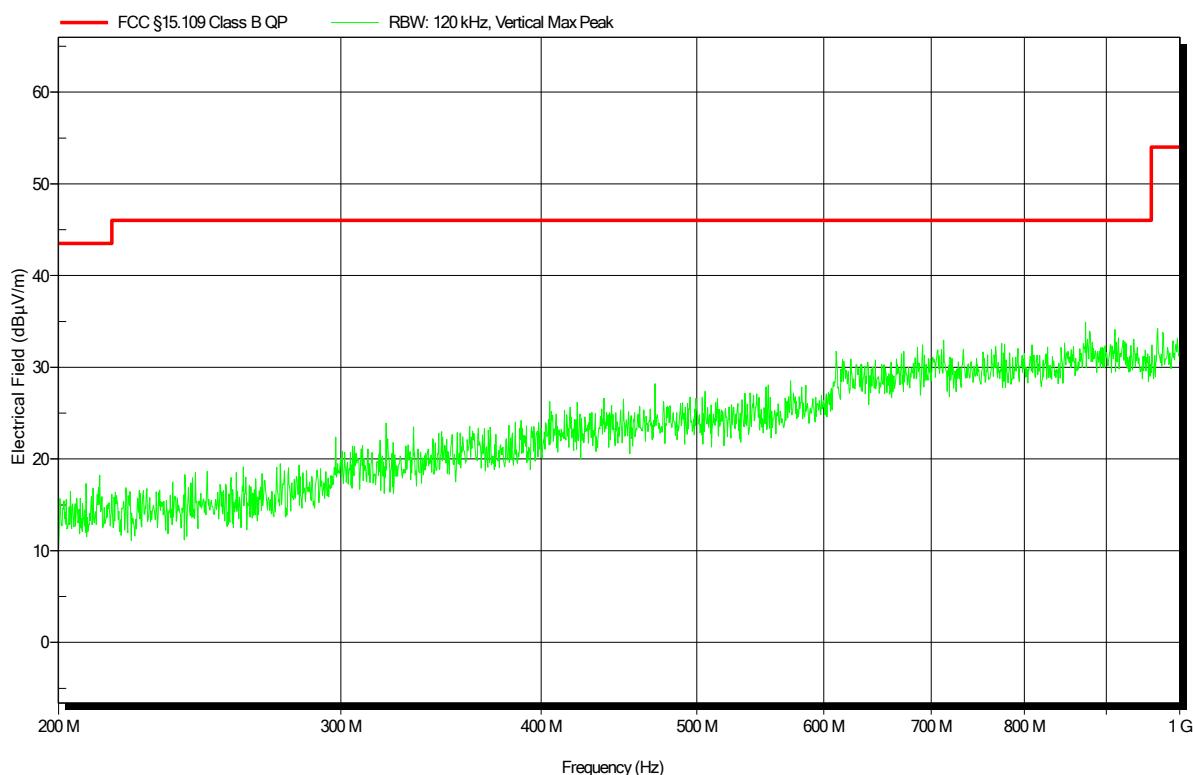

## Radiated emissions according to FCC part 15B

Project Number: G0M-2003-8888  
Applicant: GWA Hygiene GmbH  
Model Description: Hygiene-Monitoring-System  
Model: NosoEx Point of Care / Drucksensor  
Test Sample ID: 28705  
Test Site: Eurofins Product Service GmbH  
Operator: Mr. Handrik  
Test Date: 2020-04-20  
Operating Conditions: ambient temperature: 23°C  
power input: 2x1.5V DC (non rechargeable battery)  
Antenna: Rohde & Schwarz HL 223, Horizontal  
Measurement Distance: 3m  
Mode: 1  
Note 1:


Index 56

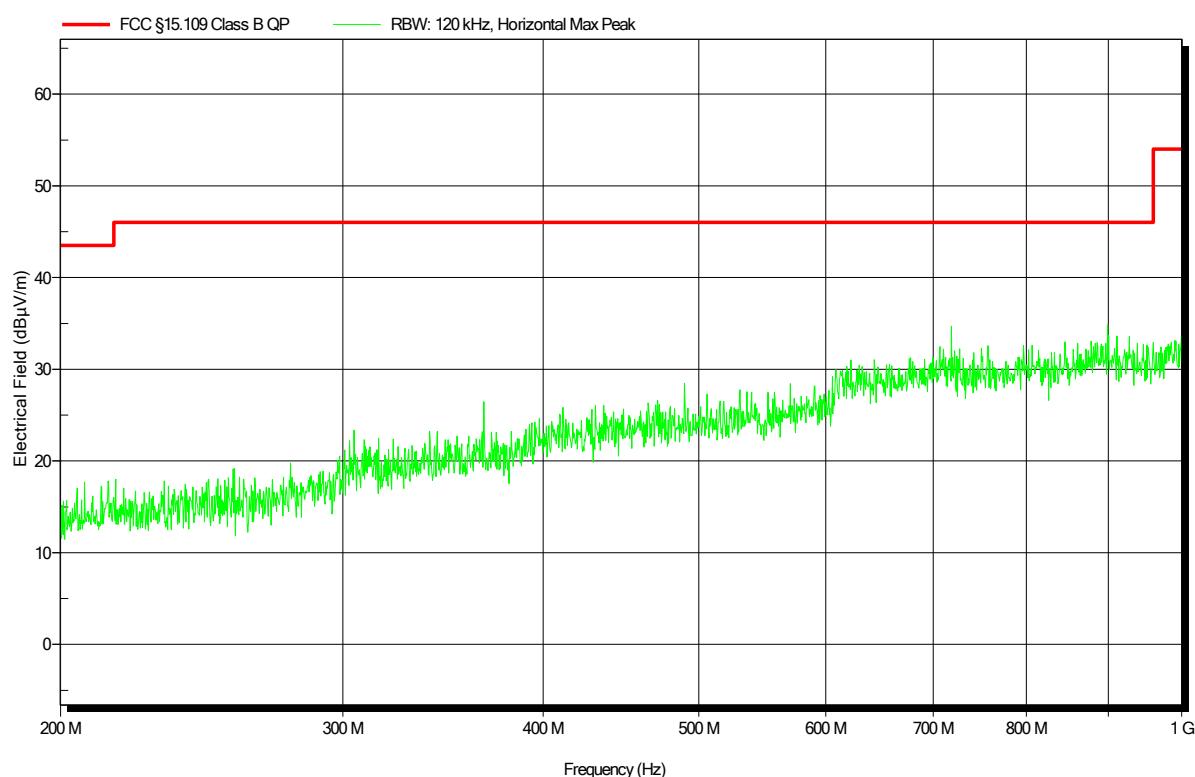

**Radiated emissions  
according to FCC part 15B**

Project Number: G0M-2003-8888  
 Applicant: GWA Hygiene GmbH  
 Model Description: Hygiene-Monitoring-System  
 Model: NosoEx Point of Care / Drucksensor  
 Test Sample ID: 28705  
 Test Site: Eurofins Product Service GmbH  
 Operator: Mr. Handrik  
 Test Date: 2020-04-20  
 Operating Conditions: ambient temperature: 23°C  
 power input: 2x1.5V DC (non rechargeable battery)  
 Antenna: Schwarzbeck BBHA 9120D, Vertical  
 Measurement Distance: 3m  
 Mode: 1  
 Note 1:

Index 57

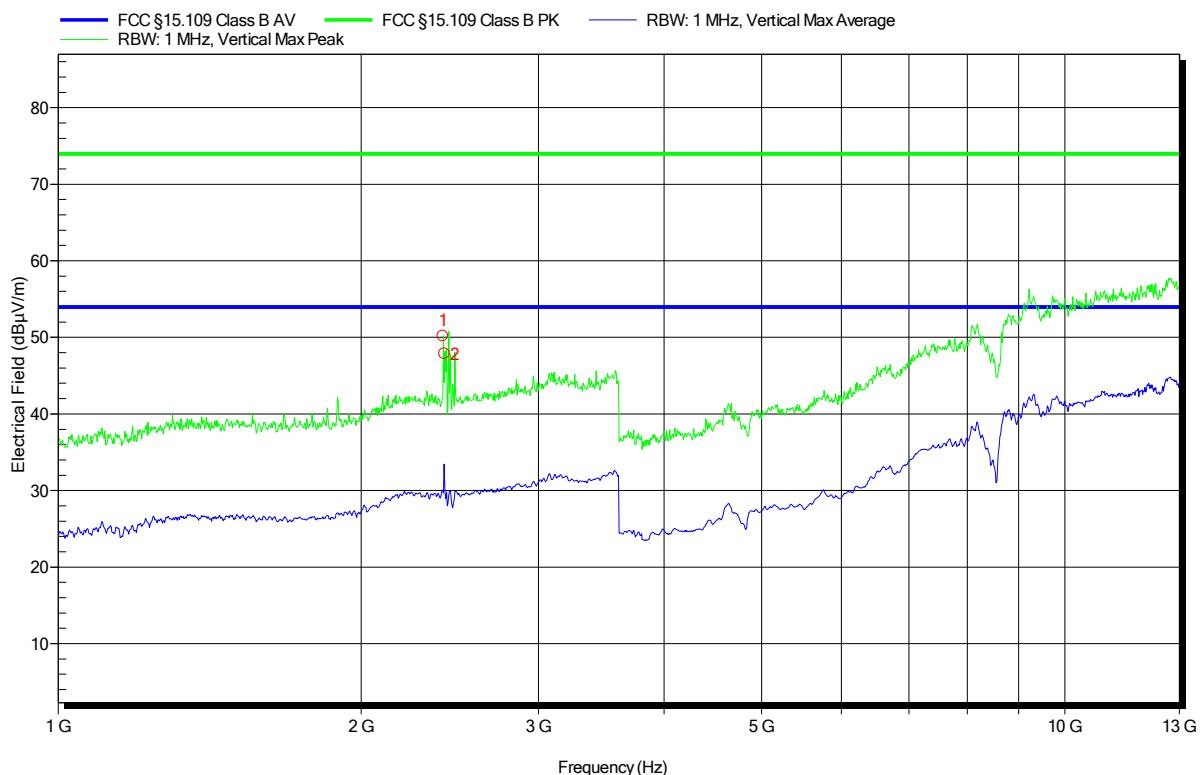


| Peak Number | Frequency |            |
|-------------|-----------|------------|
| 1           | 2.41 GHz  | BT carrier |
| 2           | 2.419 GHz | BT carrier |

**Radiated emissions  
according to FCC part 15B**

Project Number: G0M-2003-8888  
 Applicant: GWA Hygiene GmbH  
 Model Description: Hygiene-Monitoring-System  
 Model: NosoEx Point of Care / Drucksensor  
 Test Sample ID: 28705  
 Test Site: Eurofins Product Service GmbH  
 Operator: Mr. Handrik  
 Test Date: 2020-04-20  
 Operating Conditions: ambient temperature: 23°C  
 power input: 2x1.5V DC (non rechargeable battery)  
 Antenna: Schwarzbeck BBHA 9120D, Horizontal  
 Measurement Distance: 3m  
 Mode: 1  
 Note 1:

Index 58

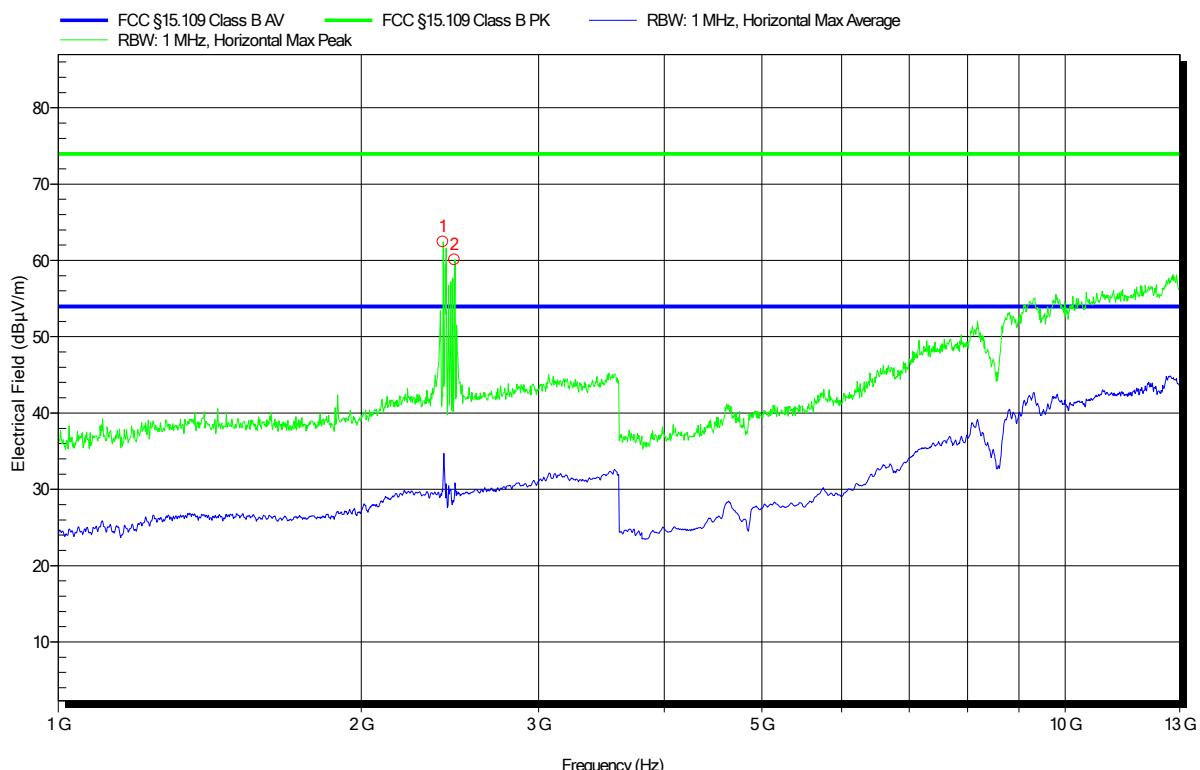

| Peak Number | Frequency | Type       |
|-------------|-----------|------------|
| 1           | 2.41 GHz  | BT carrier |
| 2           | 2.476 GHz | BT carrier |