


Appendix D

Photographs


1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

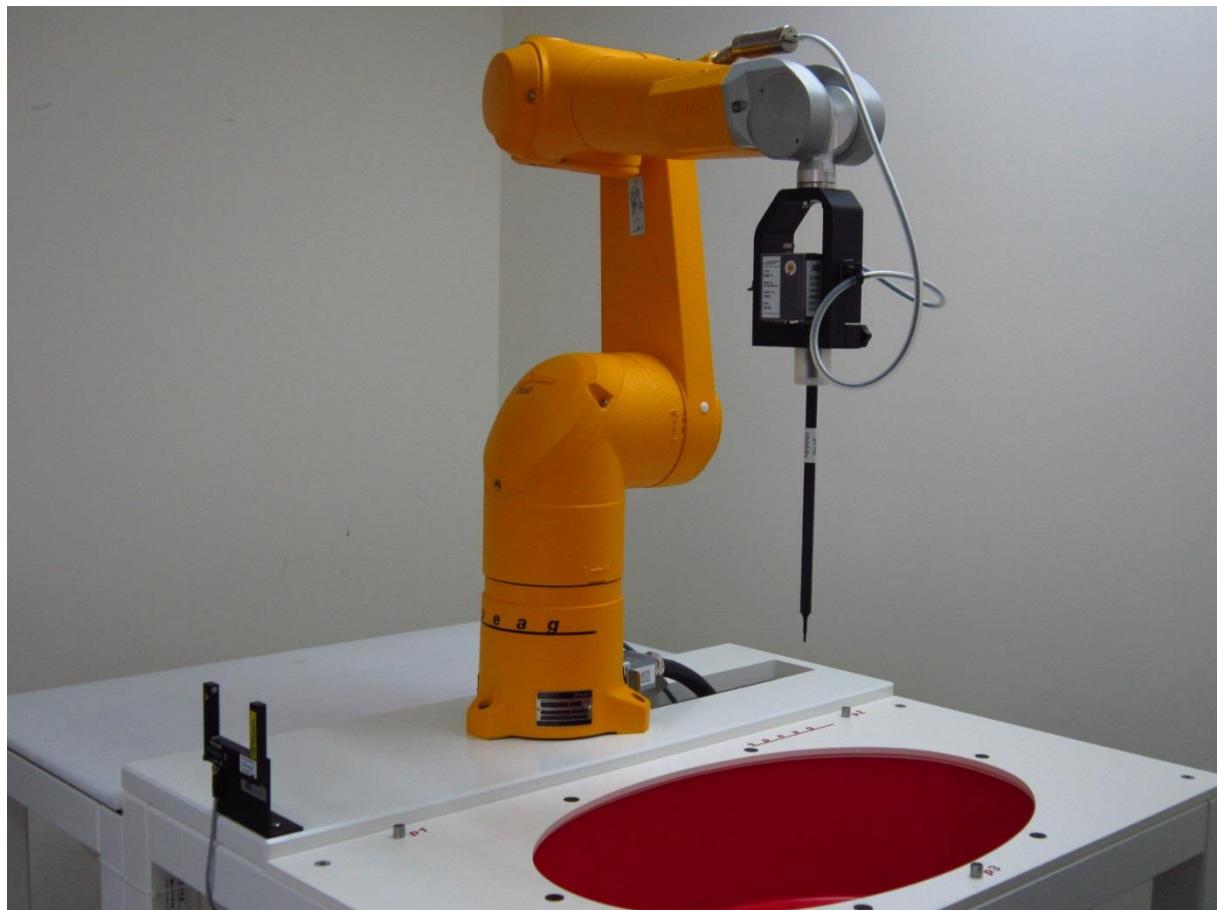

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2600

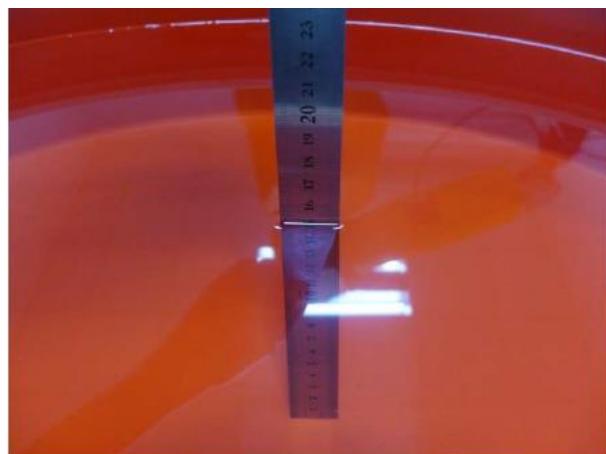

3. Photographs of EUT test position

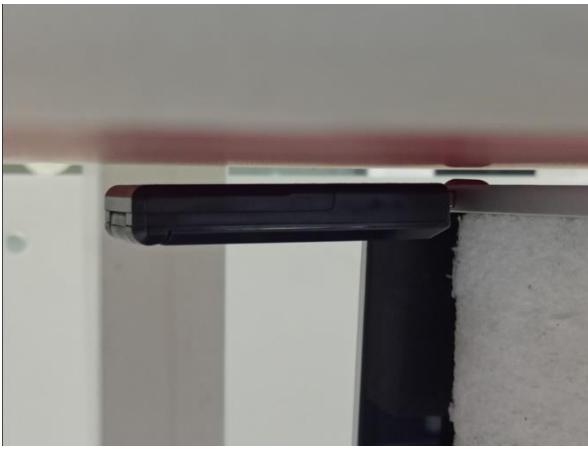
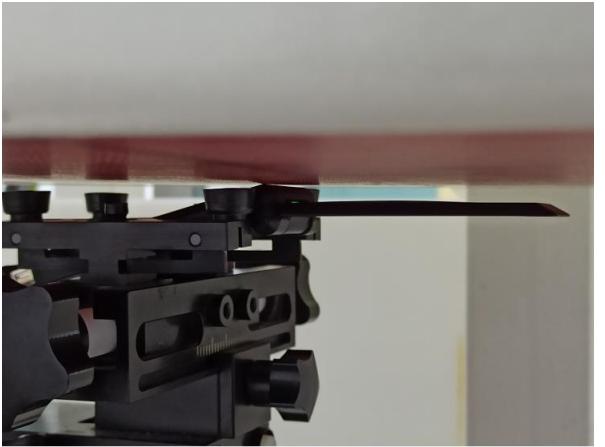
Photo 2: Horizontal Down 5mm	Photo 3: Horizontal up 5mm
	
Photo 4: Vertical Front 5mm	Photo 5: Vertical Back 5mm
	
Photo 6: Tip mode 5mm	Photo 7: Bottom side 5mm
	

Photo 8: Horizontal Down 90° 5mm	Photo 9: Horizontal Down 180° 5mm
 A photograph showing a black mechanical device, likely a test fixture, positioned under a wooden ceiling. A black line points from the text label to a specific part of the device. The background shows a room with glass walls and some equipment.	 A photograph showing a close-up view of the black mechanical device from a different angle, focusing on its internal components and structure. The background is a plain wall.

4. EUT Constructional Details

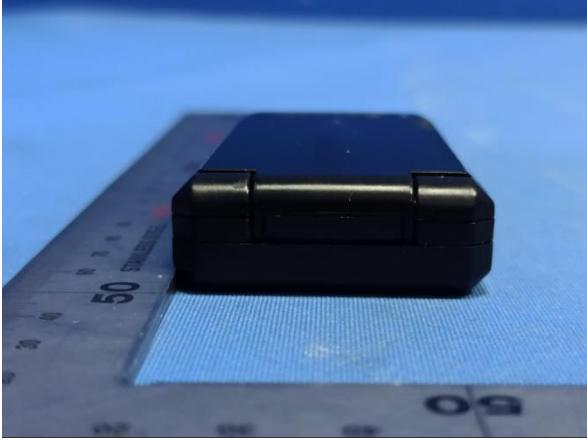
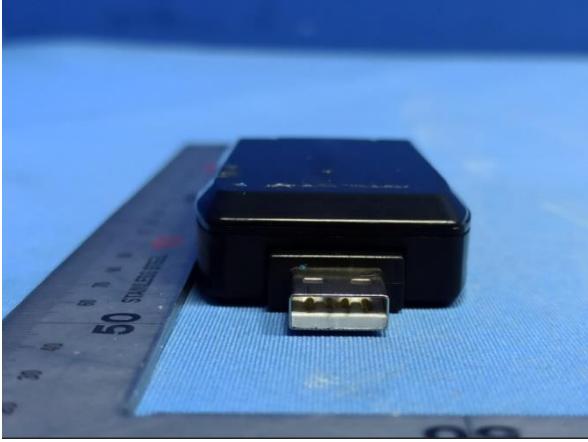
Photo 10: Front View	Photo 11: Back View
	
Photo 12: Left View	Photo 13: Right View
	
Photo 14: Top View	Photo 15: Bottom View
	

Photo 16: Front view with cover open	Photo 17: Left view with cover open with 90°
	
Photo 18: Left view with cover open with 180°	
	