


Appendix D

Photographs


1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

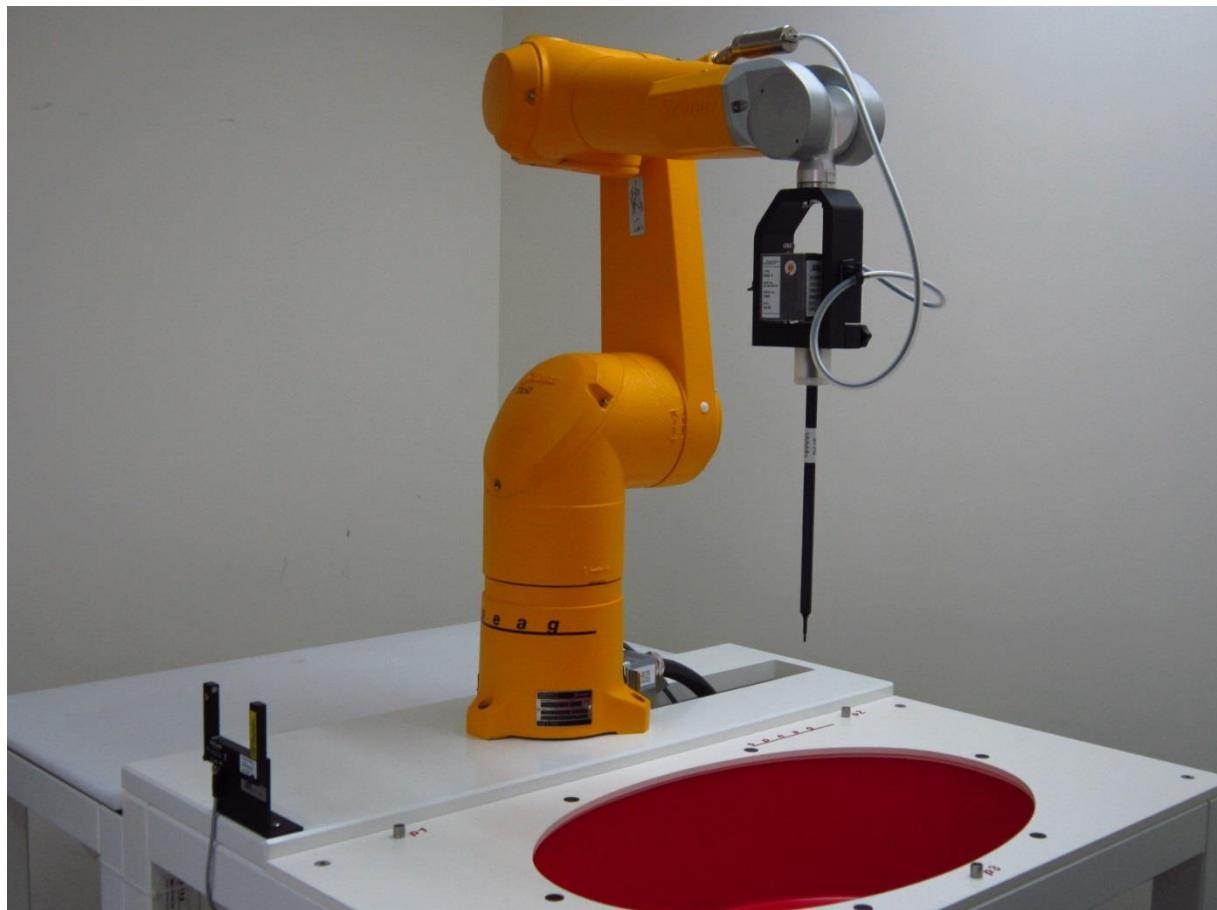

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 2600

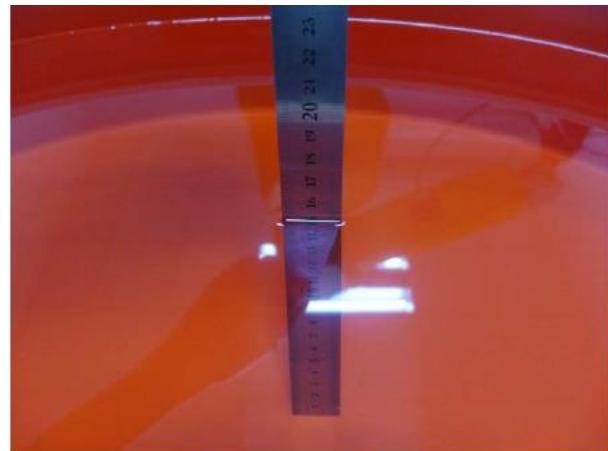

3. Photographs of EUT test position

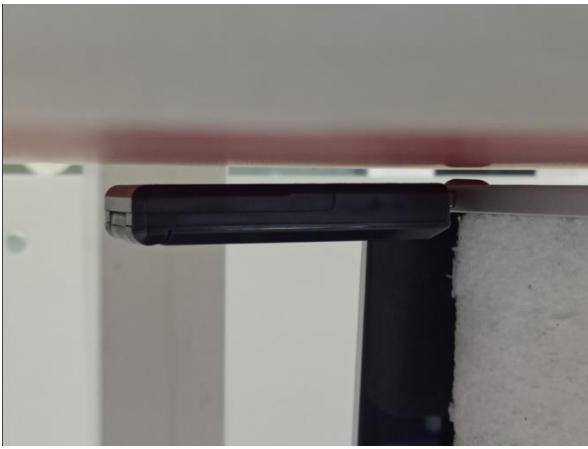
Photo 2: Horizontal Down 5mm	Photo 3: Horizontal up 5mm
	
Photo 4: Vertical Front 5mm	Photo 5: Vertical Back 5mm
	
Photo 6: Tip mode 5mm	Photo 7: Bottom side 5mm
	

Photo 8: Horizontal Down 90° 5mm	Photo 9: Horizontal Down 180° 5mm
	
Photo 10: Horizontal up 180° 5mm	
	

4. EUT Constructional Details

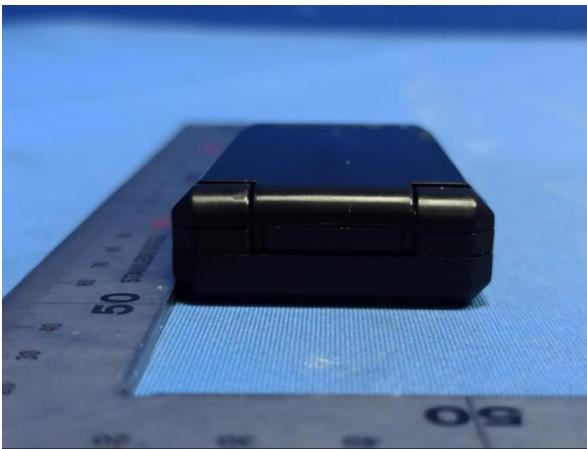
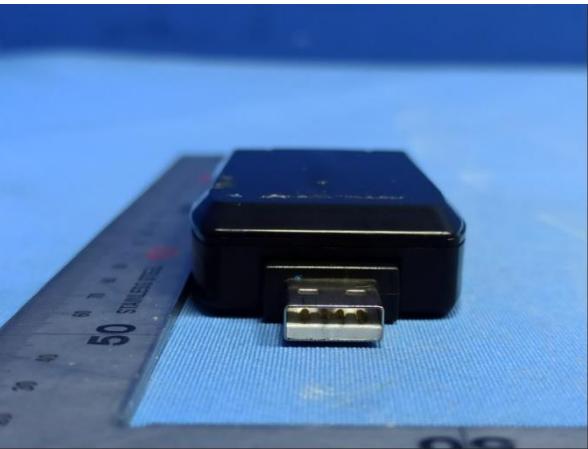
Photo 11: Front View	Photo 12: Back View
	
Photo 13: Left View	Photo 14: Right View
	
Photo 15: Top View	Photo 16: Bottom View
	

Photo 17: Front view with cover open	Photo 18: Left view with cover open with 90°
	
Photo 19: Left view with cover open with 180°	
	