

SID5000-6000



## SAR Reference Waveguide Calibration Report

Ref : ACR.256.12.15.SATU.A

### SHENZHEN TONGCE TESTING LAB

2101&2201, ZHENCHANG FACTORY, RENSHAN INDUSTRIAL  
ZONE, FUHAI SUBDISTRICT, BAOAN DISTRICT, SHENZHEN,  
GUANGDONG, 518103, PEOPLES REPUBLIC OF CHINA

### MVG COMOSAR REFERENCE WAVEGUIDE

FREQUENCY: 5000-6000 MHZ

SERIAL NO.: SN 13/14 WGA32

### Calibrated at MVG US

2105 Barrett Park Dr. - Kennesaw, GA 30144



Calibration Date: 05/15/2024

### Summary:

This document presents the method and results from an accredited SAR reference waveguide calibration performed in MVG USA using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



## SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.256.12.15.SATU.A

|                      | <i>Name</i>   | <i>Function</i> | <i>Date</i> | <i>Signature</i> |
|----------------------|---------------|-----------------|-------------|------------------|
| <i>Prepared by :</i> | Jérôme LUC    | Product Manager | 5/15/2024   |                  |
| <i>Checked by :</i>  | Jérôme LUC    | Product Manager | 5/15/2024   |                  |
| <i>Approved by :</i> | Kim RUTKOWSKI | Quality Manager | 5/15/2024   |                  |

|                       | <i>Customer Name</i>           |
|-----------------------|--------------------------------|
| <i>Distribution :</i> | SHENZHEN TONGCE<br>TESTING LAB |

| <i>Issue</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|----------------------|
| A            | 5/15/2024   | Initial release      |
|              |             |                      |
|              |             |                      |
|              |             |                      |



## TABLE OF CONTENTS

|     |                                       |    |
|-----|---------------------------------------|----|
| 1   | Introduction.....                     | 4  |
| 2   | Device Under Test .....               | 4  |
| 3   | Product Description .....             | 4  |
| 3.1 | General Information .....             | 4  |
| 4   | Measurement Method .....              | 4  |
| 4.1 | Return Loss Requirements .....        | 4  |
| 4.2 | Mechanical Requirements .....         | 4  |
| 5   | Measurement Uncertainty .....         | 5  |
| 5.1 | Return Loss .....                     | 5  |
| 5.2 | Dimension Measurement .....           | 5  |
| 5.3 | Validation Measurement .....          | 5  |
| 6   | Calibration Measurement Results ..... | 5  |
| 6.1 | Return Loss .....                     | 5  |
| 6.2 | Mechanical Dimensions .....           | 6  |
| 7   | Validation measurement .....          | 6  |
| 7.1 | Head Liquid Measurement .....         | 7  |
| 7.2 | Measurement Result .....              | 7  |
| 7.3 | Body Measurement Result .....         | 10 |
| 8   | List of Equipment .....               | 13 |



## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEEE 1528 and CEI/IEC 62209 standards for reference waveguides used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                           |
|--------------------------------|-------------------------------------------|
| Device Type                    | COMOSAR 5000-6000 MHz REFERENCE WAVEGUIDE |
| Manufacturer                   | MVG                                       |
| Model                          | SWG5500                                   |
| Serial Number                  | SN 13/14 WGA32                            |
| Product Condition (new / used) | New                                       |

A yearly calibration interval is recommended.

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Waveguides are built in accordance to the IEEE 1528 and CEI/IEC 62209 standards.

## 4 MEASUREMENT METHOD

The IEEE 1528 and CEI/IEC 62209 standards provide requirements for reference waveguides used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The waveguide used for SAR system validation measurements and checks must have a return loss of -8 dB or better. The return loss measurement shall be performed with matching layer placed in the open end of the waveguide, with the waveguide and matching layer in direct contact with the phantom shell as outlined in the fore mentioned standards.

### 4.2 MECHANICAL REQUIREMENTS

The IEEE 1528 and CEI/IEC 62209 standards specify the mechanical dimensions of the validation waveguide, the specified dimensions are as shown in Section 6.2. Figure 1 shows how the dimensions relate to the physical construction of the waveguide.

Page: 4/13

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.  
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*

Page 83 of 94



## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of  $k=2$ , traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.1 dB                              |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 3 - 300     | 0.05 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEEE 1528 and CEI/IEC 62209 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 20.3 %               |
| 10 g        | 20.1 %               |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS IN HEAD LIQUID

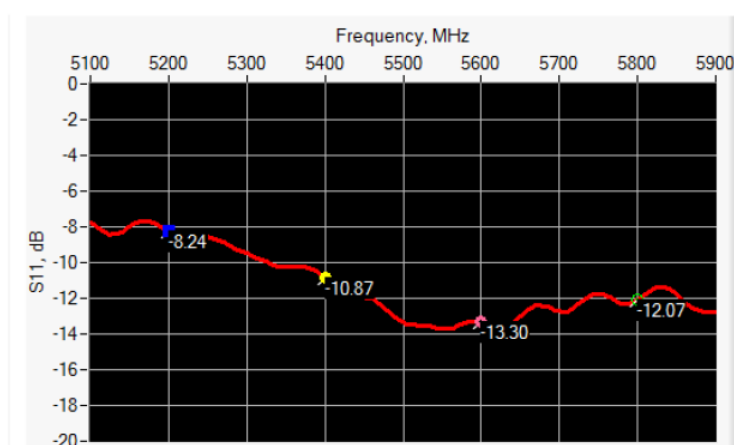

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) |
|-----------------|------------------|------------------|
| 5000-6000       | < -8.24          | -8               |

## 6.2 RETURN LOSS IN BODY LIQUID

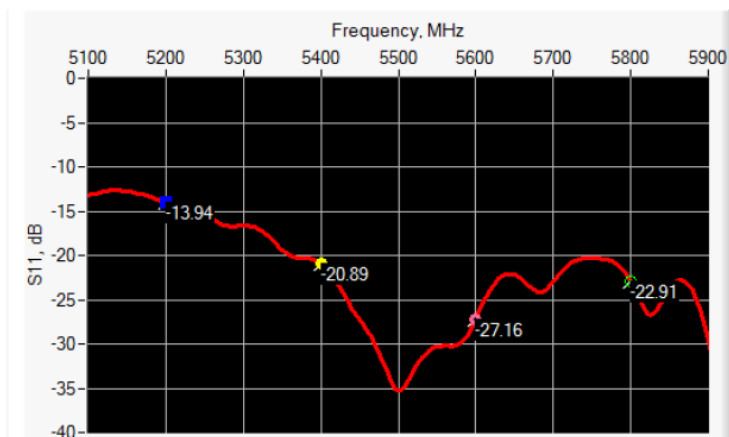

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) |
|-----------------|------------------|------------------|
| 5000-6000       | < -13.94         | -8               |

## 6.3 MECHANICAL DIMENSIONS

| Frequency (MHz) | L (mm)       |          | W (mm)       |          | L <sub>f</sub> (mm) |          | W <sub>f</sub> (mm) |          | T (mm)      |          |
|-----------------|--------------|----------|--------------|----------|---------------------|----------|---------------------|----------|-------------|----------|
|                 | Requirement  | Measured | Requirement  | Measured | Requirement         | Measured | Requirement         | Measured | Requirement | Measured |
| 5200            | 40.39 ± 0.13 | PASS     | 20.19 ± 0.13 | PASS     | 81.03 ± 0.13        | PASS     | 61.98 ± 0.13        | PASS     | 5.3*        | PASS     |
| 5800            | 40.39 ± 0.13 | PASS     | 20.19 ± 0.13 | PASS     | 81.03 ± 0.13        | PASS     | 61.98 ± 0.13        | PASS     | 4.3*        | PASS     |

\* The tolerance for the matching layer is included in the return loss measurement.

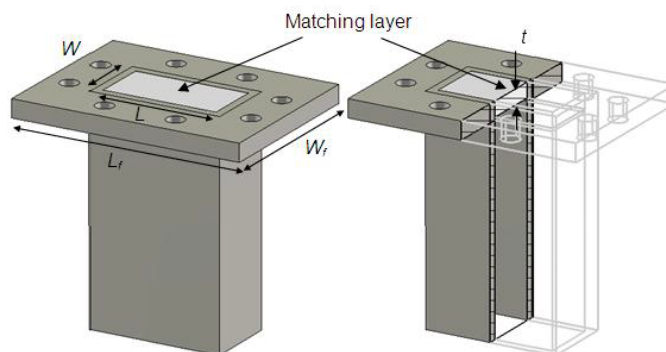


Figure 1: Validation Waveguide Dimensions

## 7 VALIDATION MEASUREMENT

The IEEE Std. 1528 and CEI/IEC 62209 standards state that the system validation measurements must be performed using a reference waveguide meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed with the matching layer placed in the open end of the waveguide, with the waveguide and matching layer in direct contact with the phantom shell.

Page: 6/13

*This document shall not be reproduced, except in full or in part, without the written approval of MVG. The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*



## 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 5000             | 36.2 $\pm$ 10 %                         |          | 4.45 $\pm$ 10 %               |          |
| 5100             | 36.1 $\pm$ 10 %                         |          | 4.56 $\pm$ 10 %               |          |
| 5200             | 36.0 $\pm$ 10 %                         | PASS     | 4.66 $\pm$ 10 %               | PASS     |
| 5300             | 35.9 $\pm$ 10 %                         |          | 4.76 $\pm$ 10 %               |          |
| 5400             | 35.8 $\pm$ 10 %                         | PASS     | 4.86 $\pm$ 10 %               | PASS     |
| 5500             | 35.6 $\pm$ 10 %                         |          | 4.97 $\pm$ 10 %               |          |
| 5600             | 35.5 $\pm$ 10 %                         | PASS     | 5.07 $\pm$ 10 %               | PASS     |
| 5700             | 35.4 $\pm$ 10 %                         |          | 5.17 $\pm$ 10 %               |          |
| 5800             | 35.3 $\pm$ 10 %                         | PASS     | 5.27 $\pm$ 10 %               | PASS     |
| 5900             | 35.2 $\pm$ 10 %                         |          | 5.38 $\pm$ 10 %               |          |
| 6000             | 35.1 $\pm$ 10 %                         |          | 5.48 $\pm$ 10 %               |          |

## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

At those frequencies, the target SAR value can not be generic. Hereunder is the target SAR value defined by MVG, within the uncertainty for the system validation. All SAR values are normalized to 1 W net power. In bracket, the measured SAR is given with the used input power.

|                                              |                                                                                                                                                                                                                                                                      |
|----------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Software                                     | OPENSAR V4                                                                                                                                                                                                                                                           |
| Phantom                                      | SN 20/09 SAM71                                                                                                                                                                                                                                                       |
| Probe                                        | SN 18/11 EPG122                                                                                                                                                                                                                                                      |
| Liquid                                       | Head Liquid Values 5200 MHz: $\epsilon_r'$ :36.62 sigma : 4.93<br>Head Liquid Values 5400 MHz: $\epsilon_r'$ :35.95 sigma : 5.18<br>Head Liquid Values 5600 MHz: $\epsilon_r'$ :36.08 sigma : 5.60<br>Head Liquid Values 5800 MHz: $\epsilon_r'$ :34.73 sigma : 5.74 |
| Distance between dipole waveguide and liquid | 0 mm                                                                                                                                                                                                                                                                 |
| Area scan resolution                         | $dx=8mm/dy=8mm$                                                                                                                                                                                                                                                      |
| Zoon Scan Resolution                         | $dx=4mm/dy=4m/dz=2mm$                                                                                                                                                                                                                                                |
| Frequency                                    | 5200 MHz<br>5400 MHz<br>5600 MHz<br>5800 MHz                                                                                                                                                                                                                         |
| Input power                                  | 20 dBm                                                                                                                                                                                                                                                               |
| Liquid Temperature                           | 21 °C                                                                                                                                                                                                                                                                |
| Lab Temperature                              | 21 °C                                                                                                                                                                                                                                                                |
| Lab Humidity                                 | 45 %                                                                                                                                                                                                                                                                 |




## SAR REFERENCE WAVEGUIDE CALIBRATION REPORT


Ref: ACR.256.12.15.SATU.A

| Frequency (MHz) | 1 g SAR (W/kg) |                | 10 g SAR (W/kg) |              |
|-----------------|----------------|----------------|-----------------|--------------|
|                 | required       | measured       | required        | measured     |
| 5200            | 159.00         | 163.88 (16.39) | 56.90           | 57.29 (5.73) |
| 5400            | 166.40         | 172.23 (17.22) | 58.43           | 59.16 (5.92) |
| 5600            | 173.80         | 181.28 (18.13) | 59.97           | 61.57 (6.16) |
| 5800            | 181.20         | 188.95 (18.90) | 61.50           | 63.45 (6.35) |

### SAR MEASUREMENT PLOTS @ 5200 MHz

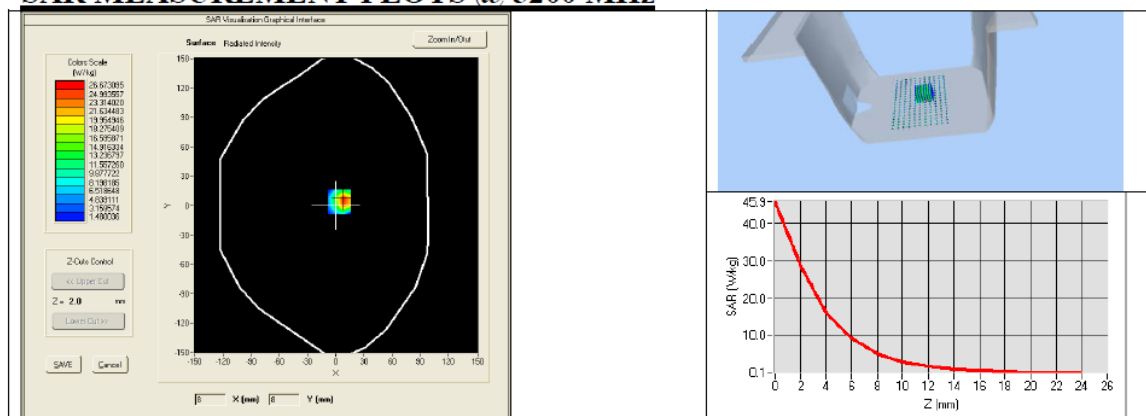

### SAR MEASUREMENT PLOTS @ 5400 MHz

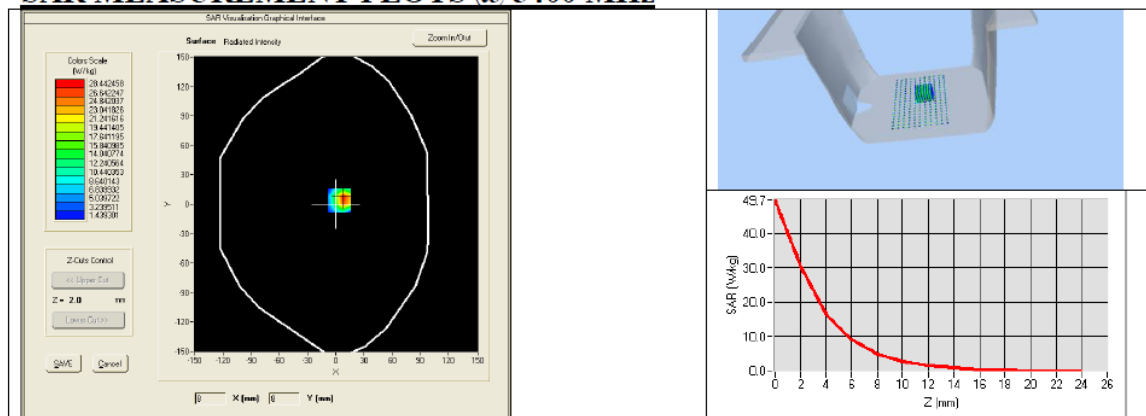





## SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.256.12.15.SATU.A

### SAR MEASUREMENT PLOTS @ 5600 MHz

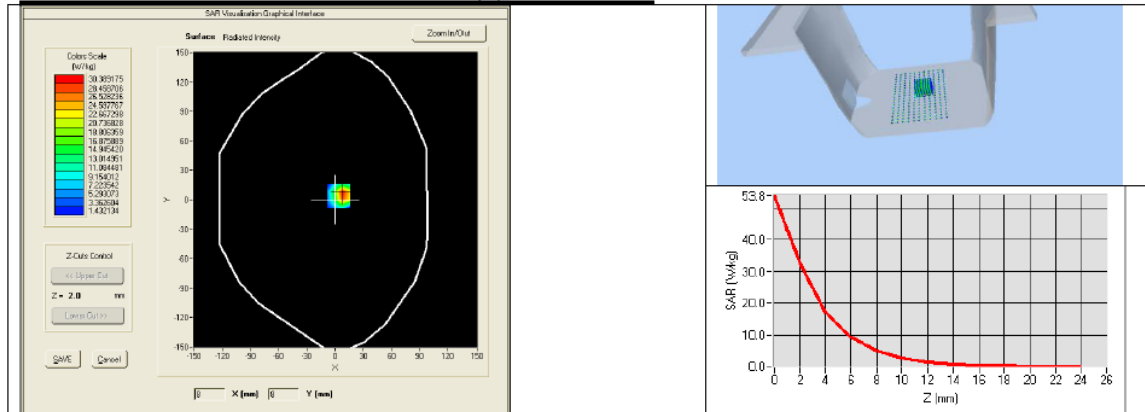

### SAR MEASUREMENT PLOTS @ 5800 MHz

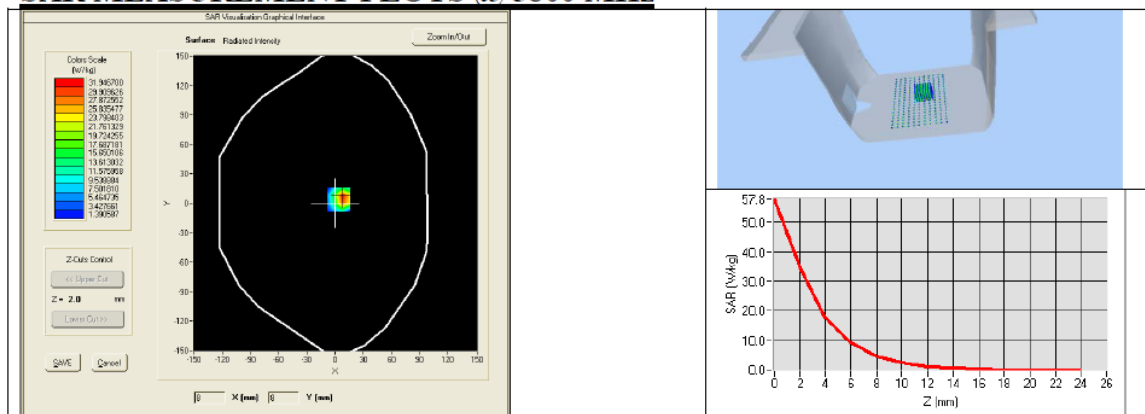



## 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 5200             | 49.0 $\pm$ 10 %                         | PASS     | 5.30 $\pm$ 10 %               | PASS     |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         | PASS     | 5.53 $\pm$ 10 %               | PASS     |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         | PASS     | 5.77 $\pm$ 10 %               | PASS     |
| 5800             | 48.2 $\pm$ 10 %                         | PASS     | 6.00 $\pm$ 10 %               | PASS     |

## 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                              |                                                                                                                                                                                                                                                                      |
|----------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Software                                     | OPENSAR V4                                                                                                                                                                                                                                                           |
| Phantom                                      | SN 20/09 SAM71                                                                                                                                                                                                                                                       |
| Probe                                        | SN 18/11 EPG122                                                                                                                                                                                                                                                      |
| Liquid                                       | Body Liquid Values 5200 MHz: $\epsilon_r'$ :50.69 sigma : 4.98<br>Body Liquid Values 5400 MHz: $\epsilon_r'$ :48.45 sigma : 5.82<br>Body Liquid Values 5600 MHz: $\epsilon_r'$ :50.57 sigma : 6.37<br>Body Liquid Values 5800 MHz: $\epsilon_r'$ :48.19 sigma : 6.45 |
| Distance between dipole waveguide and liquid | 0 mm                                                                                                                                                                                                                                                                 |
| Area scan resolution                         | dx=8mm/dy=8mm                                                                                                                                                                                                                                                        |
| Zoon Scan Resolution                         | dx=4mm/dy=4m/dz=2mm                                                                                                                                                                                                                                                  |
| Frequency                                    | 5200 MHz<br>5400 MHz<br>5600 MHz<br>5800 MHz                                                                                                                                                                                                                         |
| Input power                                  | 20 dBm                                                                                                                                                                                                                                                               |
| Liquid Temperature                           | 21 °C                                                                                                                                                                                                                                                                |
| Lab Temperature                              | 21 °C                                                                                                                                                                                                                                                                |
| Lab Humidity                                 | 45 %                                                                                                                                                                                                                                                                 |


| Frequency (MHz) | 1 g SAR (W/kg) | 10 g SAR (W/kg) |
|-----------------|----------------|-----------------|
|                 | measured       | measured        |
| 5200            | 158.49 (15.85) | 55.40 (5.54)    |
| 5400            | 167.20 (16.72) | 57.39 (5.74)    |
| 5600            | 175.65 (17.57) | 59.48 (5.95)    |
| 5800            | 183.06 (18.31) | 61.62 (6.16)    |




## SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.256.12.15.SATU.A


### BODY SAR MEASUREMENT PLOTS @ 5200 MHz

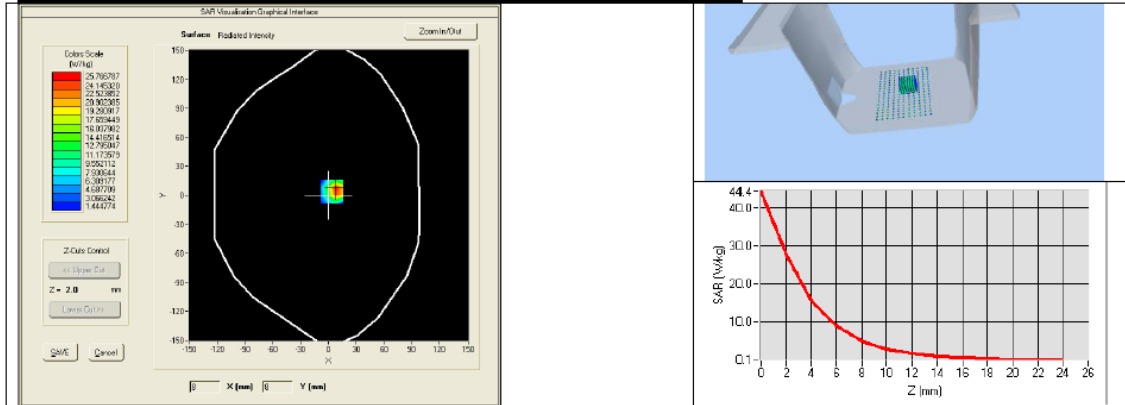

### BODY SAR MEASUREMENT PLOTS @ 5400 MHz

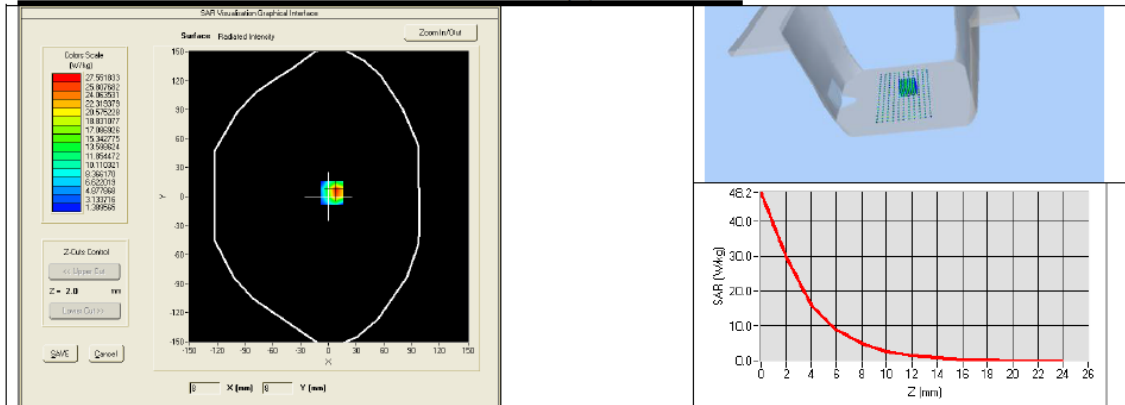

### BODY SAR MEASUREMENT PLOTS @ 5600 MHz

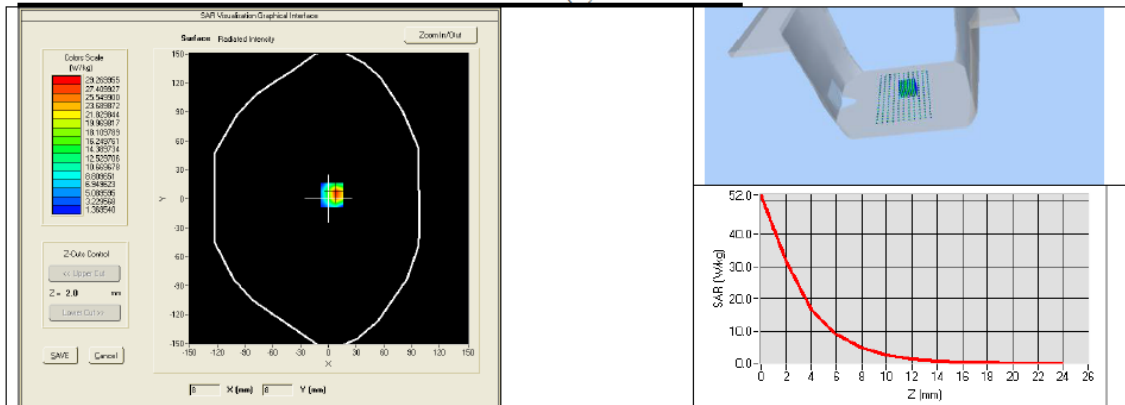




## SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.256.12.15.SATU.A

### BODY SAR MEASUREMENT PLOTS @ 5800 MHz

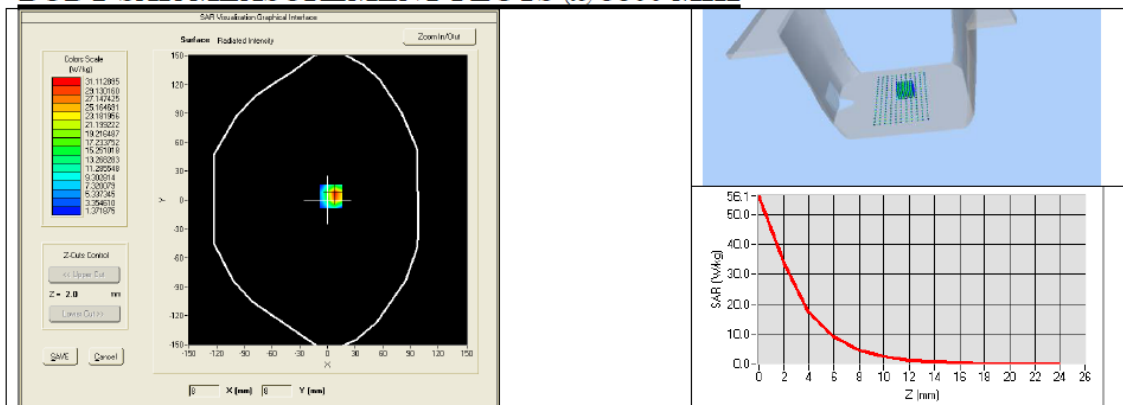



## SAR REFERENCE WAVEGUIDE CALIBRATION REPORT

Ref: ACR.256.12.15.SATU.A

### 8 LIST OF EQUIPMENT

| Equipment Summary Sheet         |                      |                    |                                               |                                               |
|---------------------------------|----------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description           | Manufacturer / Model | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| Flat Phantom                    | MVG                  | SN-20/09-SAM71     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench              | Version 3            | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                | Rhode & Schwarz ZVA  | SN100132           | 02/2024                                       | 02/2025                                       |
| Calipers                        | Carrera              | CALIPER-01         | 01/2024                                       | 01/2025                                       |
| Reference Probe                 | MVG                  | EPG122 SN 18/11    | 10/2023                                       | 10/2024                                       |
| Multimeter                      | Keithley 2000        | 1188656            | 01/2024                                       | 01/2025                                       |
| Signal Generator                | Agilent E4438C       | MY49070581         | 01/2024                                       | 01/2025                                       |
| Amplifier                       | Aethercomm           | SN 046             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                     | HP E4418A            | US38261498         | 01/2024                                       | 01/2025                                       |
| Power Sensor                    | HP ECP-E26A          | US37181460         | 01/2024                                       | 01/2025                                       |
| Directional Coupler             | Narda 4216-20        | 01386              | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature and Humidity Sensor | Control Company      | 150798832          | 10/2023                                       | 10/2024                                       |

Page: 13/13

*This document shall not be reproduced, except in full or in part, without the written approval of MVG.  
The information contained herein is to be used only for the purpose for which it is submitted and is not to be released in whole or part without written approval of MVG.*

Page 92 of 94

## Appendix E: SAR SYSTEM VALIDATION

Per FCC KDB 865664 D02v01, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the required tissue- equivalent media for system validation, according to the procedures outlined in FCC KDB 865664 D01 v01 and IEEE 1528-2013. Since SAR probe calibrations are frequency dependent, each probe calibration point was validated at a frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probes and tissue dielectric parameters has been included.

**SAR System Validation Summary**

| Date       | Freq. [MHz] | Probe S/N         | Tissue type | COND. PERM.  | COND. PERM.      | CW Validation |                 |                | Mod. Validation |             |                             |
|------------|-------------|-------------------|-------------|--------------|------------------|---------------|-----------------|----------------|-----------------|-------------|-----------------------------|
|            |             |                   |             | ( $\sigma$ ) | ( $\epsilon_r$ ) | sensitivity   | Probe linearity | Probe isotropy | Mod. type       | Duty factor | Peak to average power ratio |
| 08/18/2023 | 2450        | SN 25/22 EPGO 375 | Body        | 2.37         | 52.10            | PASS          | PASS            | PASS           | GMSK            | PASS        | N/A                         |
| 08/18/2023 | 5G          | SN 25/22 EPGO3 75 | Body        | 48.94        | 1.92~5.95        | PASS          | PASS            | PASS           | OFDM            | PASS        | N/A                         |

NOTE: While the probes have been calibrated for both a CW and modulated signals, all measurements were performed using communication systems calibrated for CW signals only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01v01 for scenarios when CW probe calibrations are used with other signal types. SAR systems were validated for modulated signals with a periodic duty cycle, such as OFDM according to KDB 865664.

## Appendix F: The Check Data of Impedance and Return Loss

The information are included in the SAR report to qualify for the three-year extended calibration interval;

| Impedance in body liquid |           |                        |        |                            |                        |        | Date: 08/18/2023           |
|--------------------------|-----------|------------------------|--------|----------------------------|------------------------|--------|----------------------------|
| Freq. (MHz)              | Temp (°C) | Dipole Impedance Re(z) |        |                            | Dipole Impedance Im(z) |        |                            |
|                          |           | measured               | Target | $\Delta$ ( $\pm 5\Omega$ ) | measured               | Target | $\Delta$ ( $\pm 5\Omega$ ) |
| 2450                     | 22        | 45.90                  | 46.50  | -0.60                      | -0.36                  | -0.20  | -0.16                      |
| 5G                       | 22        | 49.02                  | 50.01  | -0.99                      | 5.52                   | 5.70   | -0.18                      |

| Return loss in body liquid |           |                 |        |                         | Date: 08/18/2023 |
|----------------------------|-----------|-----------------|--------|-------------------------|------------------|
| Freq. (MHz)                | Temp (°C) | Return loss(dB) |        |                         |                  |
|                            |           | measured        | Target | $\Delta$ ( $\pm 20\%$ ) |                  |
| 2450                       | 22        | -34.65          | -32.86 | 5.45                    |                  |
| 5G                         | 22        | -32.66          | -34.56 | 1.90                    |                  |

| liquid | Freq. (MHz) | Temp (°C) | $\epsilon_r$ / relative permittivity |        |                        | $\sigma$ (s/m) / conductivity |        |                        | $\rho$ (kg/m <sup>3</sup> ) |
|--------|-------------|-----------|--------------------------------------|--------|------------------------|-------------------------------|--------|------------------------|-----------------------------|
|        |             |           | measured                             | Target | $\Delta$ ( $\pm 5\%$ ) | measured                      | Target | $\Delta$ ( $\pm 5\%$ ) |                             |
| Body   | 2450        | 22        | 45.90                                | 46.50  | -0.60                  | -0.36                         | -0.20  | -0.16                  | 1000                        |
|        | 5G          | 22        | 49.02                                | 50.01  | -0.99                  | 5.52                          | 5.70   | -0.18                  | 1000                        |

| Test Equipment                | Manufacturer    | Model           | Serial Number | Calibration              |                         |
|-------------------------------|-----------------|-----------------|---------------|--------------------------|-------------------------|
|                               |                 |                 |               | Calibration Date (D.M.Y) | Calibration Due (D.M.Y) |
| Signal Generator              | Angilent        | N5182A          | MY47070282    | Jun. 27, 2024            | Jun. 26, 2025           |
| Multimeter                    | Keithley        | Multimeter 2000 | 4078275       | Jun. 27, 2024            | Jun. 26, 2025           |
| Network Analyzer              | Agilent         | 8753E           | US38432457    | Jun. 27, 2024            | Jun. 26, 2025           |
| Power Meter                   | Agilent         | E4418B          | GB43312526    | Jun. 27, 2024            | Jun. 26, 2025           |
| Power Sensor                  | Agilent         | E9301A          | MY41497725    | Jun. 27, 2024            | Jun. 26, 2025           |
| Power Amplifier               | PE              | PE15A4019       | 112342        | N/A                      | N/A                     |
| Temperature / Humidity Sensor | Control company | TH101B          | 152470214     | Jun. 27, 2024            | Jun. 26, 2025           |

\*\*\*\*\*END OF REPORT\*\*\*\*\*