

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
	NA

3. Photographs of EUT test position

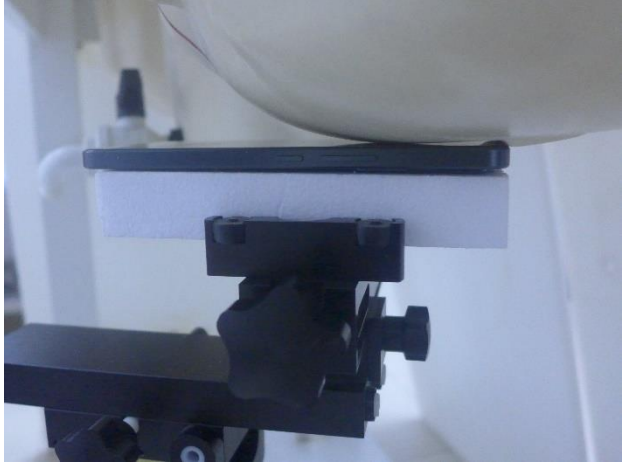
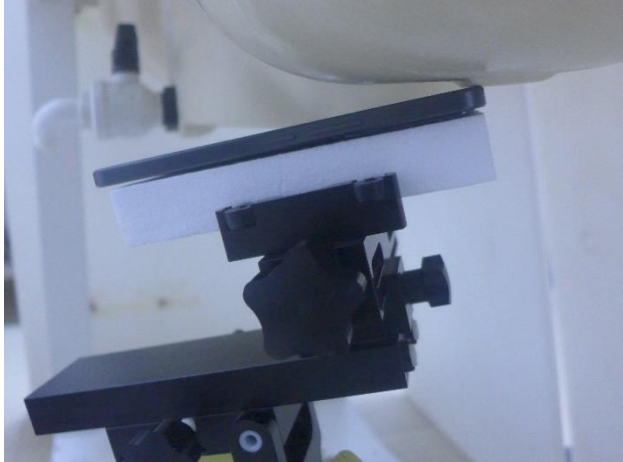
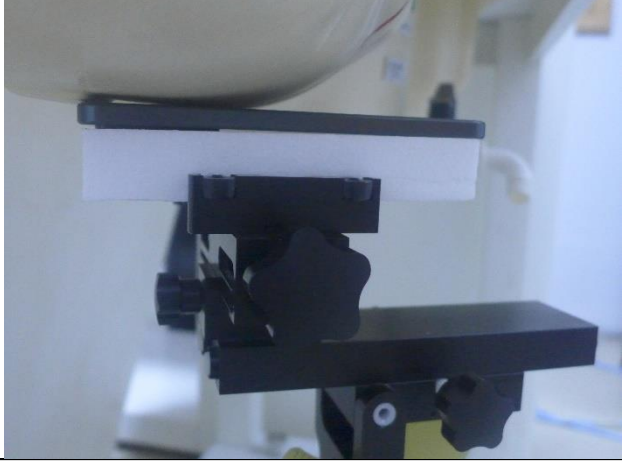
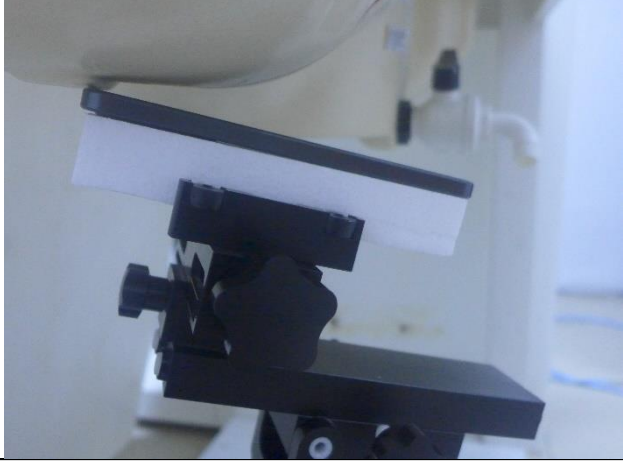
Photo 2: Left cheek	Photo 3: Left tilted
	
Photo 4: Right cheek	Photo 5: Right tilted
	
Photo 6: Front side 15mm	Photo 7: Back side 15mm
	

Photo 8: Back side 12mm	Photo 9: Top side 11mm
	
Photo 10: Left side 11mm	Photo 11: Front side 10mm
	
Photo 12: Back side 10mm	Photo 13: Left side 10mm
	

Photo 14: Right side 10mm

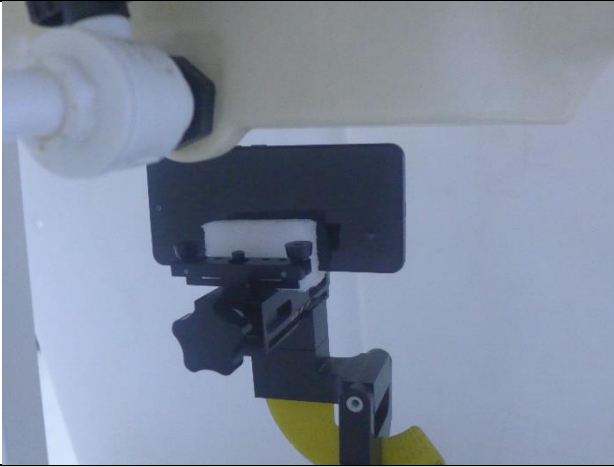


Photo 15: Top side 10mm



Photo 16: Bottom side 10mm



Photo 17: Front side 0mm



Photo 18: Back side 0mm



Photo 19: Left side 0mm



Photo 20: Right side 0mm

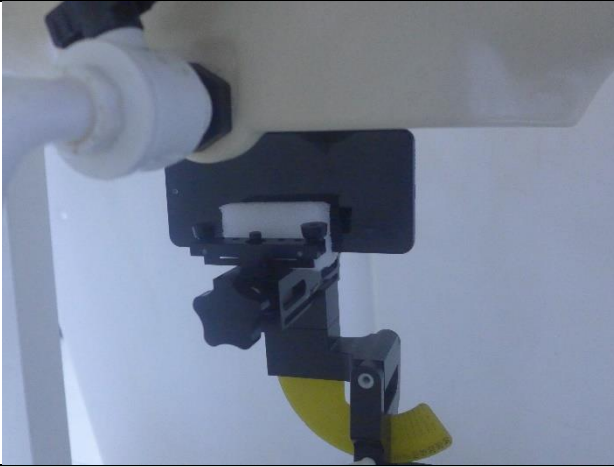


Photo 21: Top side 0mm



Photo 22: Bottom side 0mm



4. EUT Constructional Details

