

Part 1_Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
	NA

3. Photographs of EUT test position

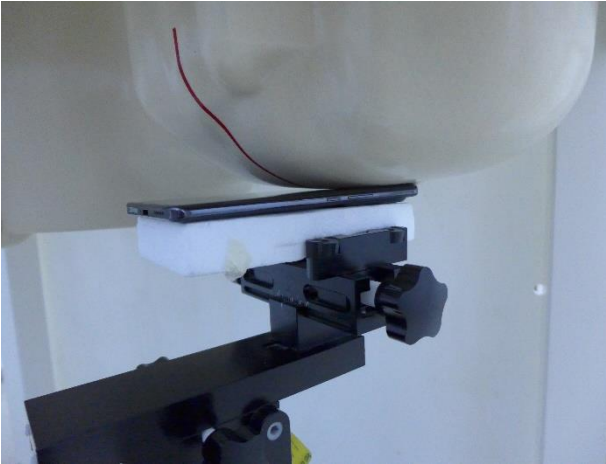
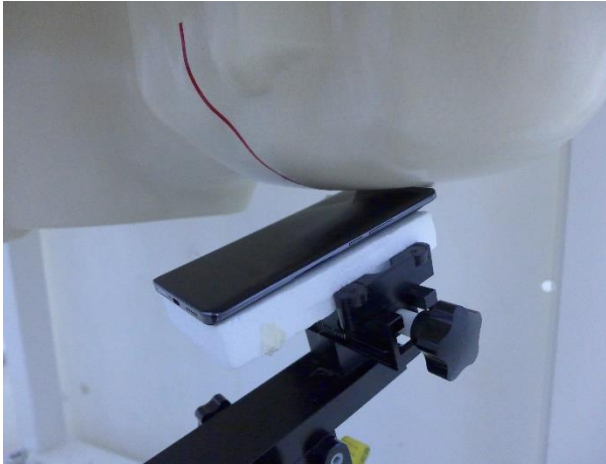
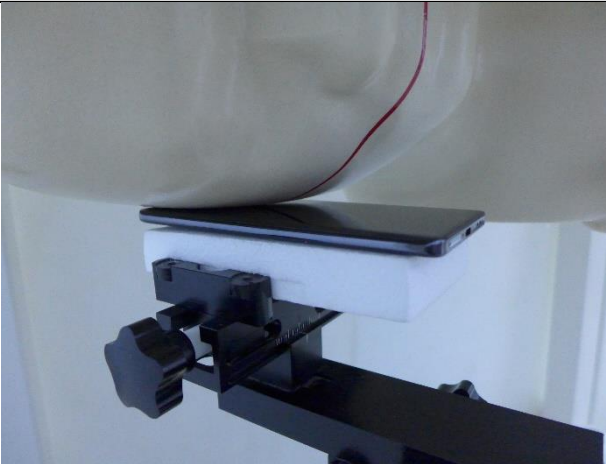
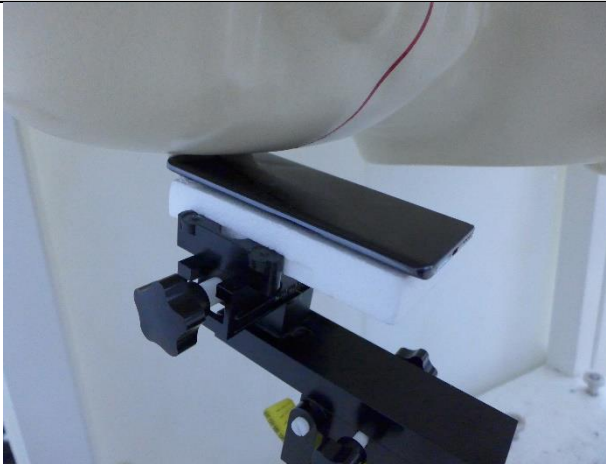
Photo 2: Left cheek 	Photo 3: Left tilted 
Photo 4: Right cheek 	Photo 5: Right tilted 
Photo 6: Front side 15mm 	Photo 7: Back side 15mm 

Photo 8: Back side 11mm 	Photo 9: Top side 11mm 
Photo 10: Left side 12mm 	Photo 11: Front side 10mm 
Photo 12: Back side 10mm 	Photo 13: Left side 10mm 

Photo 14: Right side 10mm



Photo 15: Top side 10mm



Photo 16: Bottom side 10mm



Photo 17: Front side 0mm



Photo 18: Back side 0mm



Photo 19: Left side 0mm



Photo 20: Right side 0mm



Photo 21: Top side 0mm



4. EUT Constructional Details

