

Date: 2025/7/11

System Check_750MHz**DUT:D750V3-SN:1099**

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.881$ S/m; $\epsilon_r = 43.8$

Ambient Temperature: 23.2°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(9.81, 8.75, 9.26); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (42.0 mm x 210.0 mm): Measurement Grid: 7.0 mm x 15.0 mm
mmSAR (1g) = 2.27 W/kg; SAR (10g) = 1.50 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = -0.01 dB

SAR (1g) = 2.15 W/kg; SAR (10g) = 1.35 W/kg

Smallest distance from peaks to all points 3 dB below = 21.3 mm

Ratio of SAR at M2 to SAR at M1 = 87.3 %

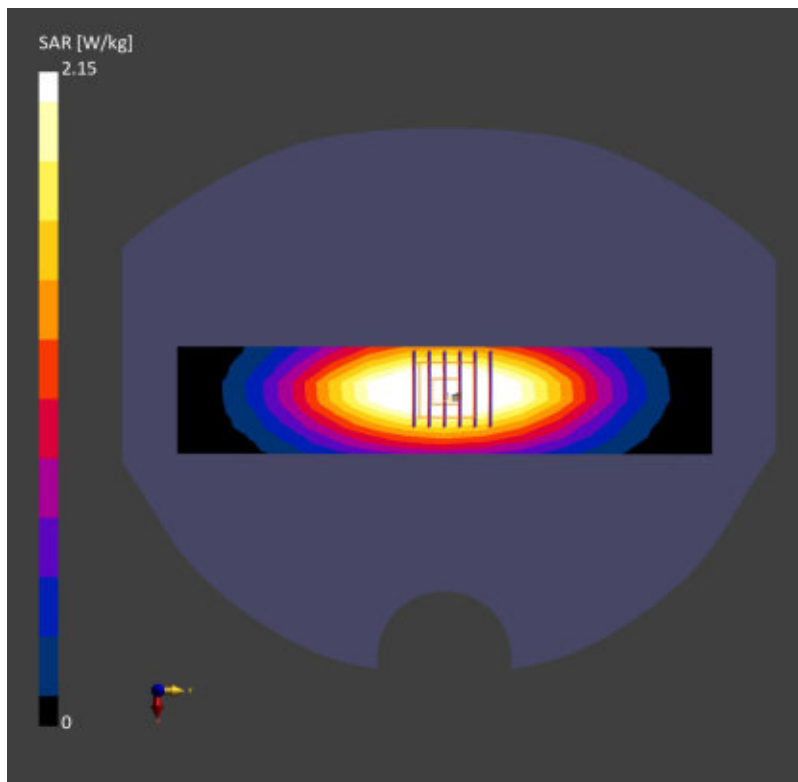

Date: 2025/7/26

System Check_750MHz**DUT:D750V3-SN:1099**

Communication System: CW; Frequency: 750.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 750.0$ MHz; $\sigma = 0.883$ S/m; $\epsilon_r = 43.9$

Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(9.81, 8.75, 9.26); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (42.0 mm x 210.0 mm): Measurement Grid: 7.0 mm x 15.0 mm
mmSAR (1g) = 2.25 W/kg; SAR (10g) = 1.50 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.20 W/kg; SAR (10g) = 1.42 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 89.1 %

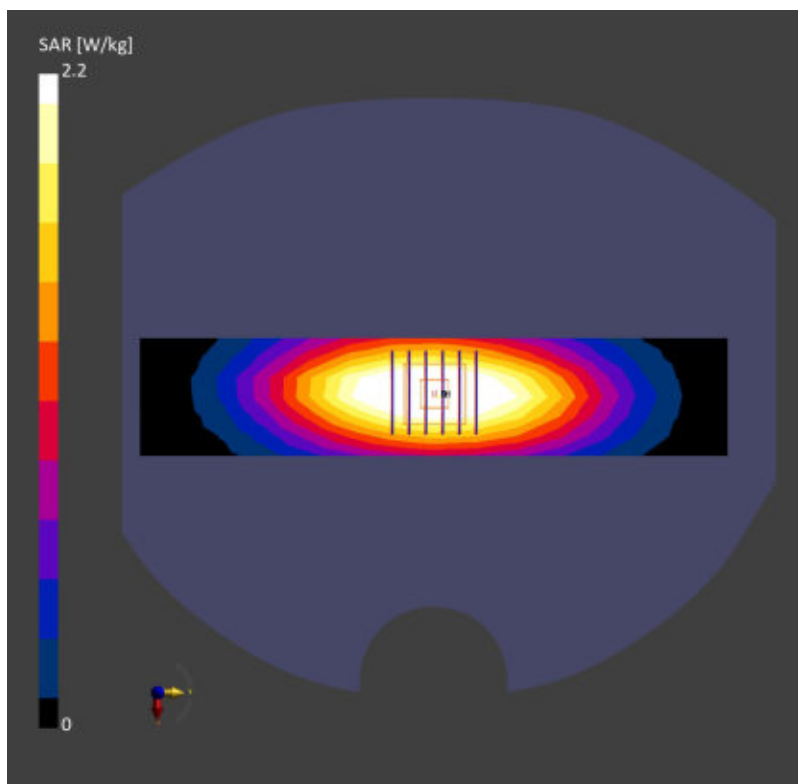

Date: 2025/7/11

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.911$ S/m; $\epsilon_r = 43.5$


Ambient Temperature: 23.1°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(9.4, 8.38, 8.87); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (42.0 mm x 210.0 mm): Measurement Grid: 7.0 mm x 15.0 mm
mmSAR (1g) = 2.55 W/kg; SAR (10g) = 1.67 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 2.40 W/kg; SAR (10g) = 1.53 W/kg
Smallest distance from peaks to all points 3 dB below = 18.4 mm
Ratio of SAR at M2 to SAR at M1 = 87.7 %

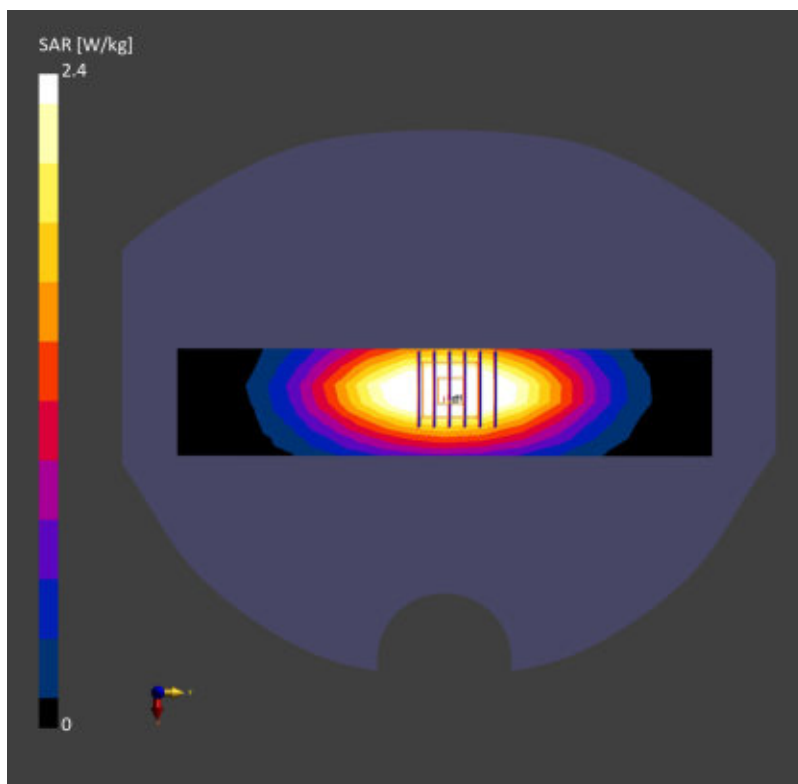

Date: 2025/8/3

System Check_835MHz**DUT:D835V2-SN:4d162**

Communication System: CW; Frequency: 835.0 MHz; Duty Cycle: 1:1

Medium: HSL Medium parameters used: $f = 835.0$ MHz; $\sigma = 0.919$ S/m; $\epsilon_r = 43.4$

Ambient Temperature: 23.4°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(9.4, 8.38, 8.87); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (42.0 mm x 210.0 mm): Measurement Grid: 7.0 mm x 15.0 mm
mmSAR (1g) = 2.53 W/kg; SAR (10g) = 1.65 W/kg;


Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm

Power Drift = 0.00 dB

SAR (1g) = 2.37 W/kg; SAR (10g) = 1.51 W/kg

Smallest distance from peaks to all points 3 dB below = 20.5 mm

Ratio of SAR at M2 to SAR at M1 = 88.5 %

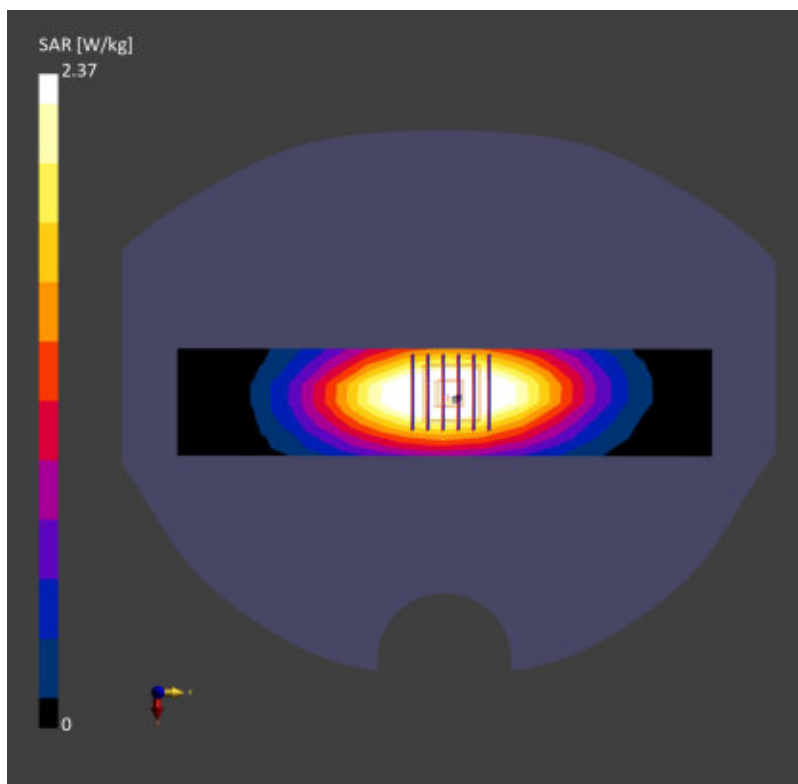

Date: 2025/7/12

System Check_1750MHz**DUT:D1750V2-SN:1137**


Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.31$ S/m; $\epsilon_r = 41.5$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.94, 7.08, 7.5); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
mmSAR (1g) = 8.85 W/kg; SAR (10g) = 4.80 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 8.76 W/kg; SAR (10g) = 4.71 W/kg
Smallest distance from peaks to all points 3 dB below = 9.9 mm
Ratio of SAR at M2 to SAR at M1 = 83.1 %

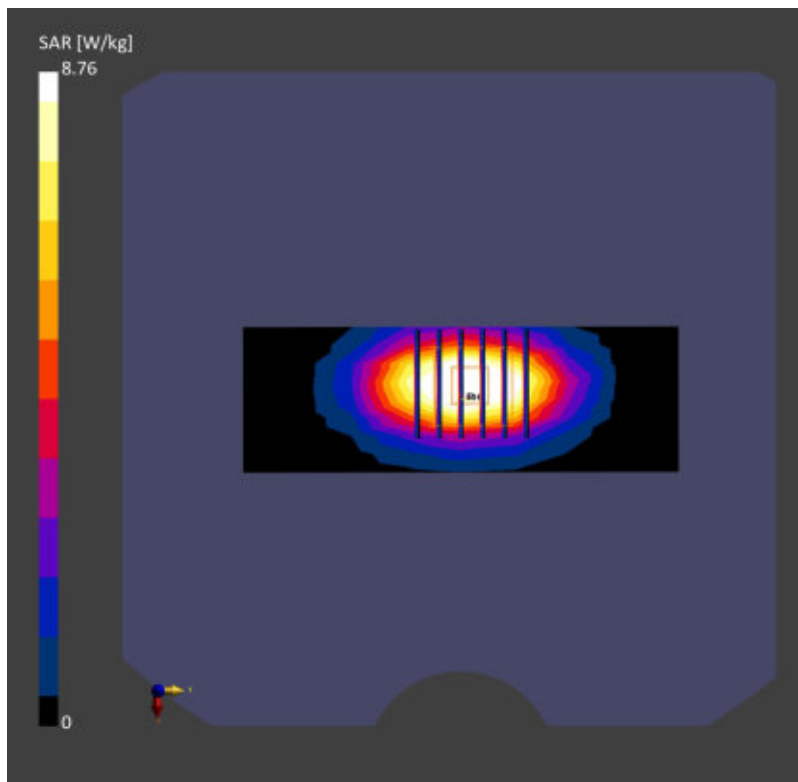

Date: 2025/8/2

System Check_1750MHz**DUT:D1750V2-SN:1137**


Communication System: CW; Frequency: 1750.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1750.0$ MHz; $\sigma = 1.35$ S/m; $\epsilon_r = 41.7$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.94, 7.08, 7.5); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
mmSAR (1g) = 8.82 W/kg; SAR (10g) = 4.75 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 8.62 W/kg; SAR (10g) = 4.59 W/kg
Smallest distance from peaks to all points 3 dB below = 10.8 mm
Ratio of SAR at M2 to SAR at M1 = 82.8 %

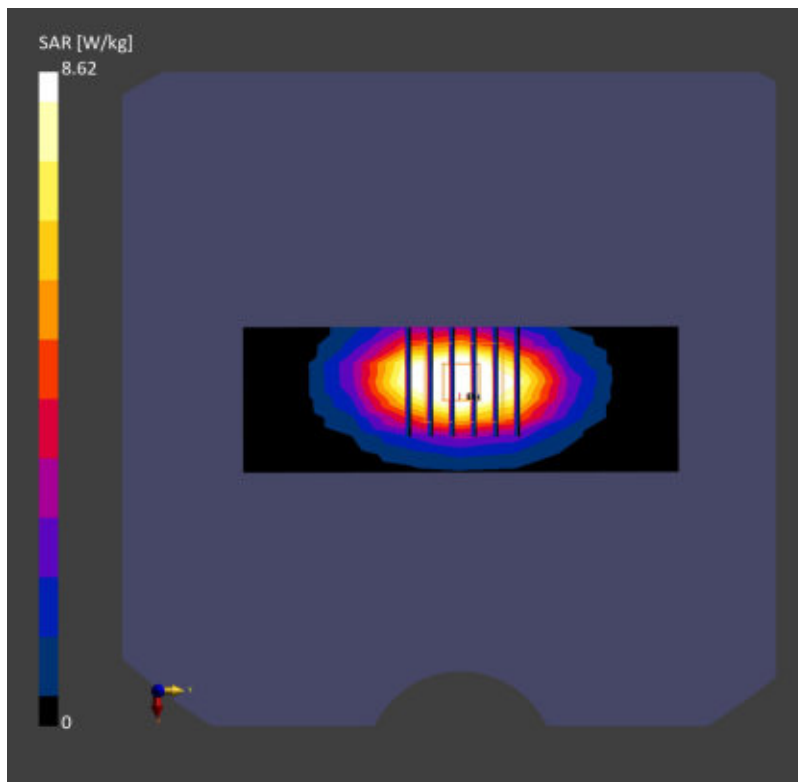

Date: 2025/7/12

System Check_1900MHz**DUT:D1900V2-SN:5d182**


Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.45$ S/m; $\epsilon_r = 41.3$
Ambient Temperature: 23.4°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.95, 7.09, 7.51); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
mmSAR (1g) = 9.93 W/kg; SAR (10g) = 5.22 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.01 dB
SAR (1g) = 9.83 W/kg; SAR (10g) = 5.11 W/kg
Smallest distance from peaks to all points 3 dB below = 9.7 mm
Ratio of SAR at M2 to SAR at M1 = 82.2 %

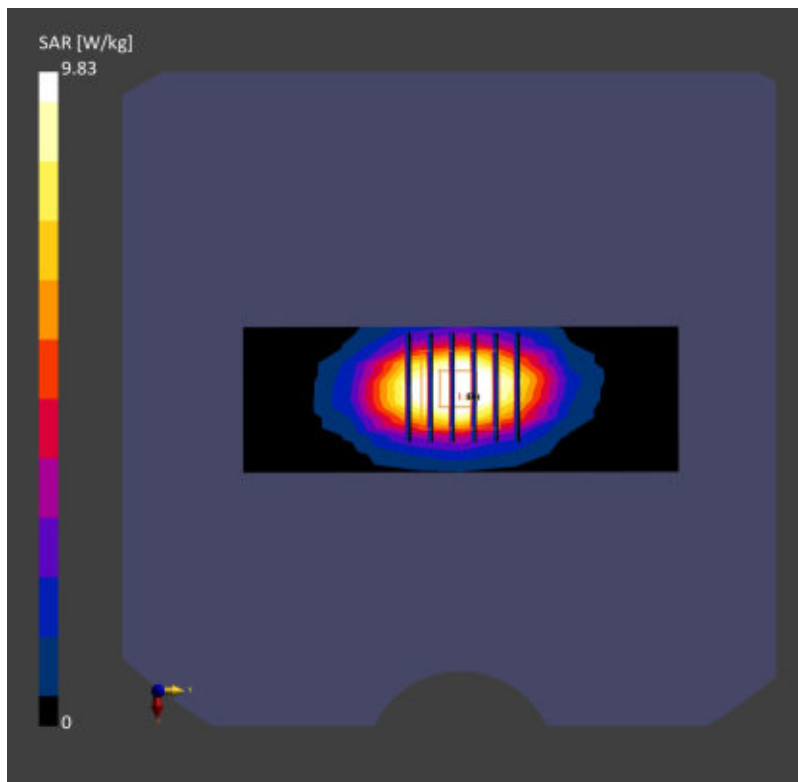

Date: 2025/7/25

System Check_1900MHz**DUT:D1900V2-SN:5d182**


Communication System: CW; Frequency: 1900.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 1900.0$ MHz; $\sigma = 1.42$ S/m; $\epsilon_r = 41.1$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.95, 7.09, 7.51); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 120.0 mm): Measurement Grid: 5.0 mm x 15.0 mm
mmSAR (1g) = 9.85 W/kg; SAR (10g) = 5.19 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 6.0 mm x 6.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 9.73 W/kg; SAR (10g) = 5.01 W/kg
Smallest distance from peaks to all points 3 dB below = 10.3 mm
Ratio of SAR at M2 to SAR at M1 = 81.2 %

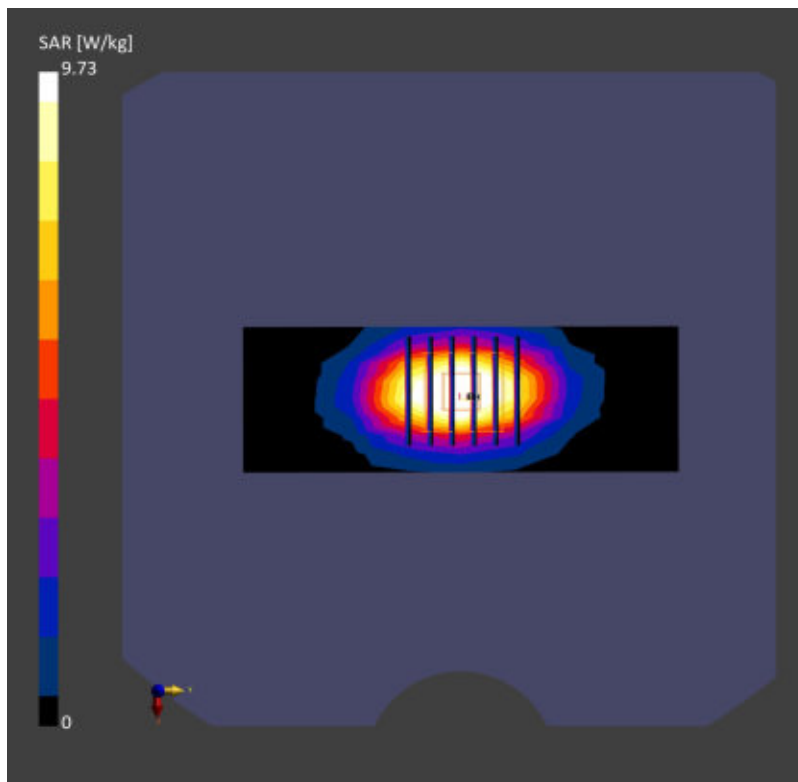

Date: 2025/7/19

System Check_2450MHz**DUT:D2450V2-SN:924**


Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 40.6$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.82, 6.98, 7.39); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 12.7 W/kg; SAR (10g) = 5.99 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.00 dB
SAR (1g) = 12.4 W/kg; SAR (10g) = 5.71 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 79.4 %

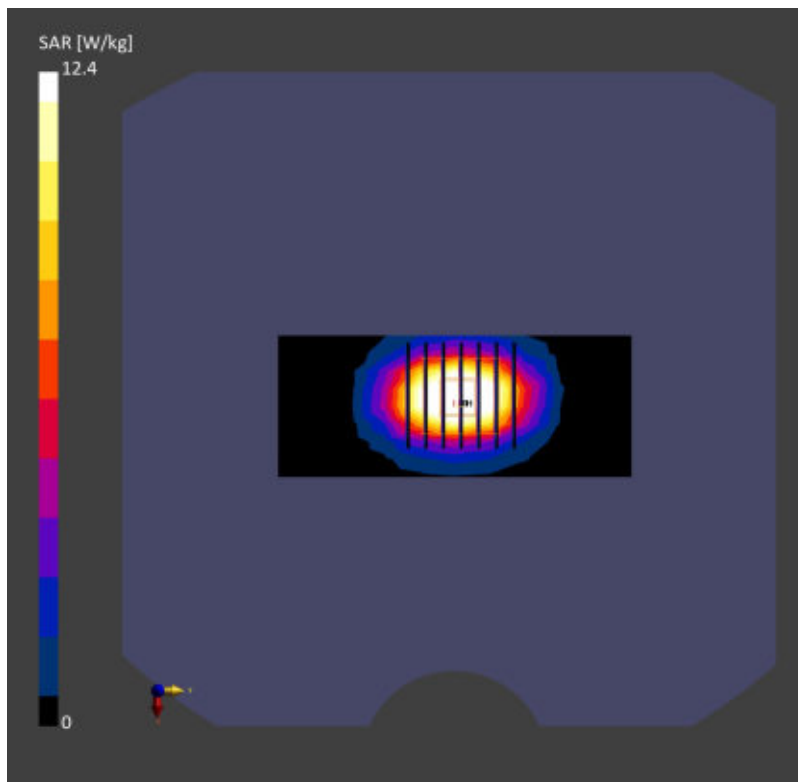

Date: 2025/8/4

System Check_2450MHz**DUT:D2450V2-SN:924**


Communication System: CW; Frequency: 2450.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2450.0$ MHz; $\sigma = 1.81$ S/m; $\epsilon_r = 40.4$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.6°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.82, 6.98, 7.39); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 100.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 13.2 W/kg; SAR (10g) = 6.25 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = 0.01 dB
SAR (1g) = 13.0 W/kg; SAR (10g) = 6.02 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 80.0 %

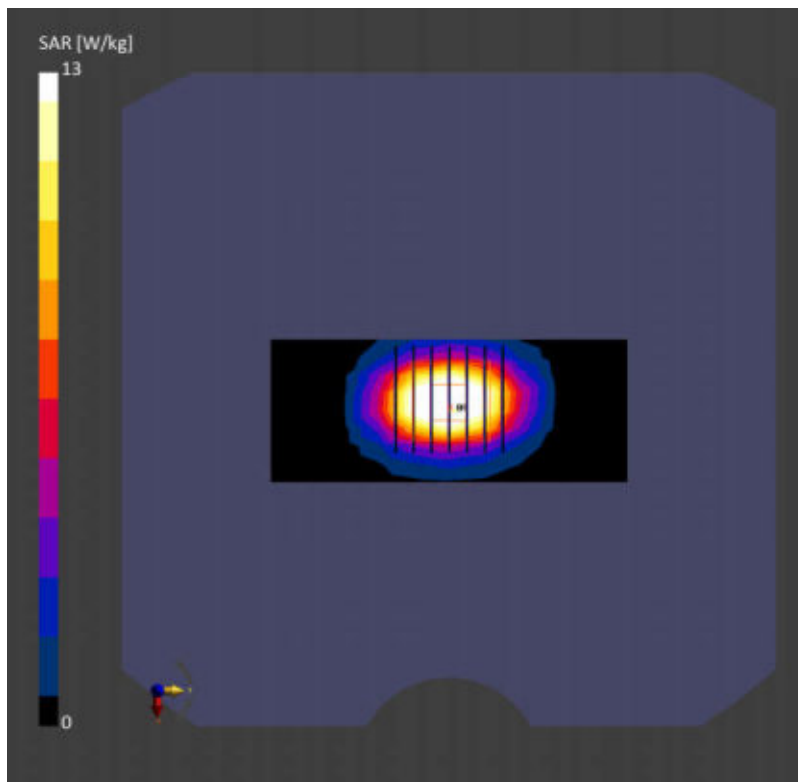

Date: 2025/7/17

System Check_2600MHz**DUT:D2600V2-SN:1070**


Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.97$ S/m; $\epsilon_r = 40.7$
Ambient Temperature: 23.1°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.68, 6.85, 7.26); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 13.5 W/kg; SAR (10g) = 6.16 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 13.1 W/kg; SAR (10g) = 6.06 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 77.5 %

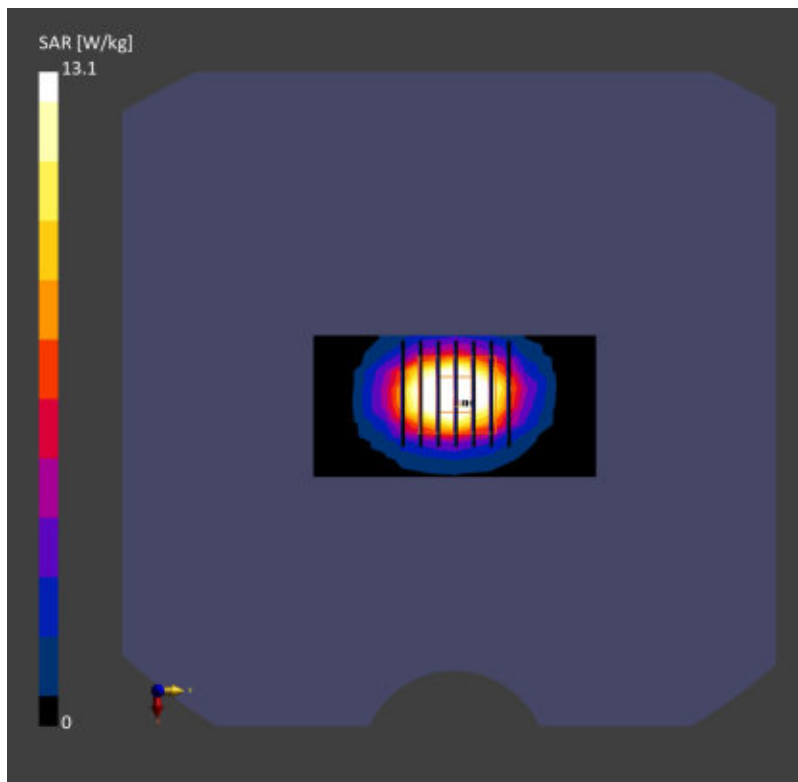

Date: 2025/7/30

System Check_2600MHz**DUT:D2600V2-SN:1070**


Communication System: CW; Frequency: 2600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 2600.0$ MHz; $\sigma = 1.94$ S/m; $\epsilon_r = 40.5$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.4°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(7.68, 6.85, 7.26); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=250mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 13.8 W/kg; SAR (10g) = 6.24 W/kg;

Pin=250mW/Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm
Power Drift = -0.00 dB
SAR (1g) = 13.6 W/kg; SAR (10g) = 6.05 W/kg
Smallest distance from peaks to all points 3 dB below = 9.0 mm
Ratio of SAR at M2 to SAR at M1 = 77.4 %

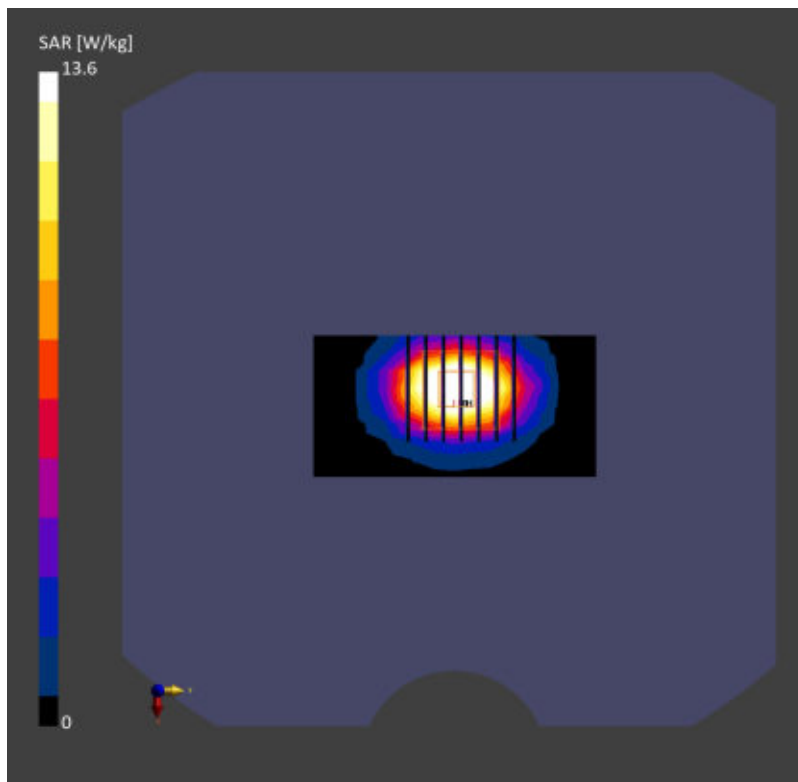

Date: 2025/7/13

System Check_3500MHz**DUT:D3500V2-SN:1037**


Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.79$ S/m; $\epsilon_r = 39.1$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.91, 6.16, 6.52); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 6.47 W/kg; SAR (10g) = 2.51 W/kg;

Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.00 dB
SAR (1g) = 6.43 W/kg; SAR (10g) = 2.41 W/kg
Smallest distance from peaks to all points 3 dB below = 8.1 mm
Ratio of SAR at M2 to SAR at M1 = 75.9 %

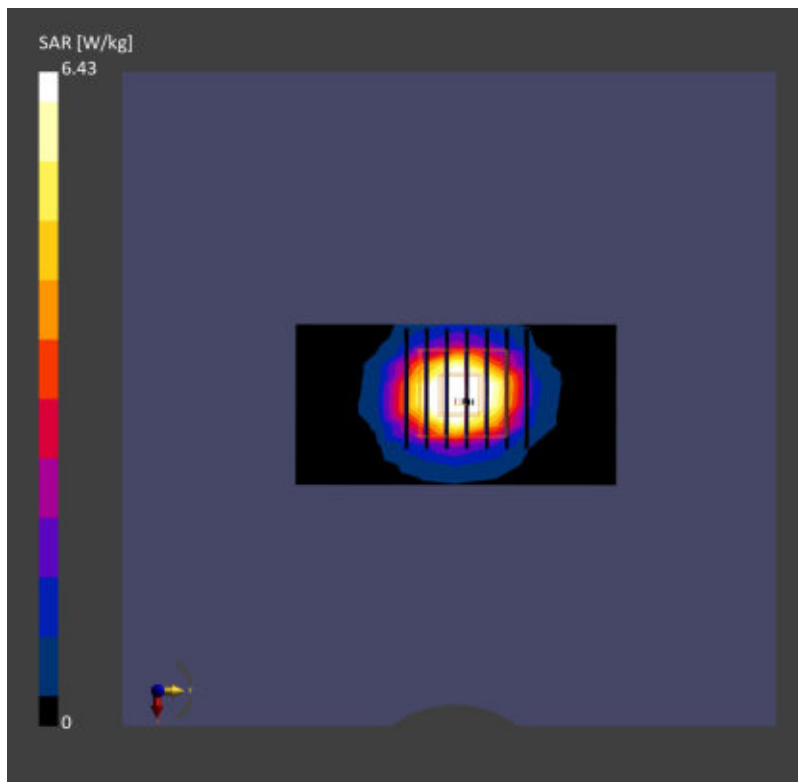

Date: 2025/8/6

System Check_3500MHz**DUT:D3500V2-SN:1037**


Communication System: CW; Frequency: 3500.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 3500.0$ MHz; $\sigma = 2.83$ S/m; $\epsilon_r = 38.9$
Ambient Temperature: 23.5°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.91, 6.16, 6.52); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 5.97 W/kg; SAR (10g) = 2.31 W/kg;

Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.03 dB
SAR (1g) = 6.12 W/kg; SAR (10g) = 2.29 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 77.7 %

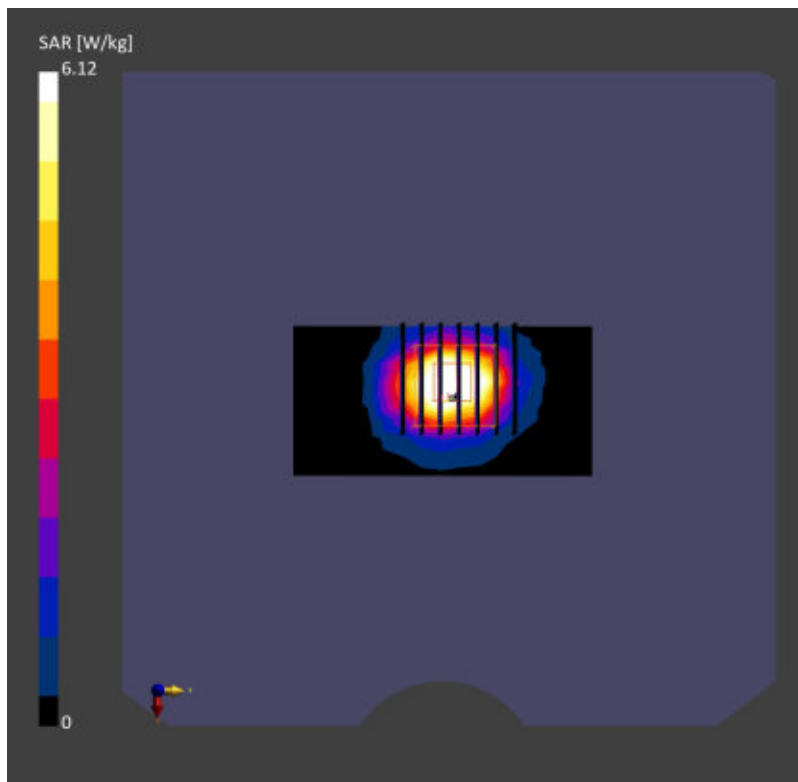

Date: 2025/7/14

System Check_3700MHz**DUT:D3700V2-SN:1008**


Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.13$ S/m; $\epsilon_r = 38.6$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.92, 6.17, 6.53); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 6.65 W/kg; SAR (10g) = 2.50 W/kg;

Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = -0.00 dB
SAR (1g) = 6.59 W/kg; SAR (10g) = 2.40 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 74.2 %

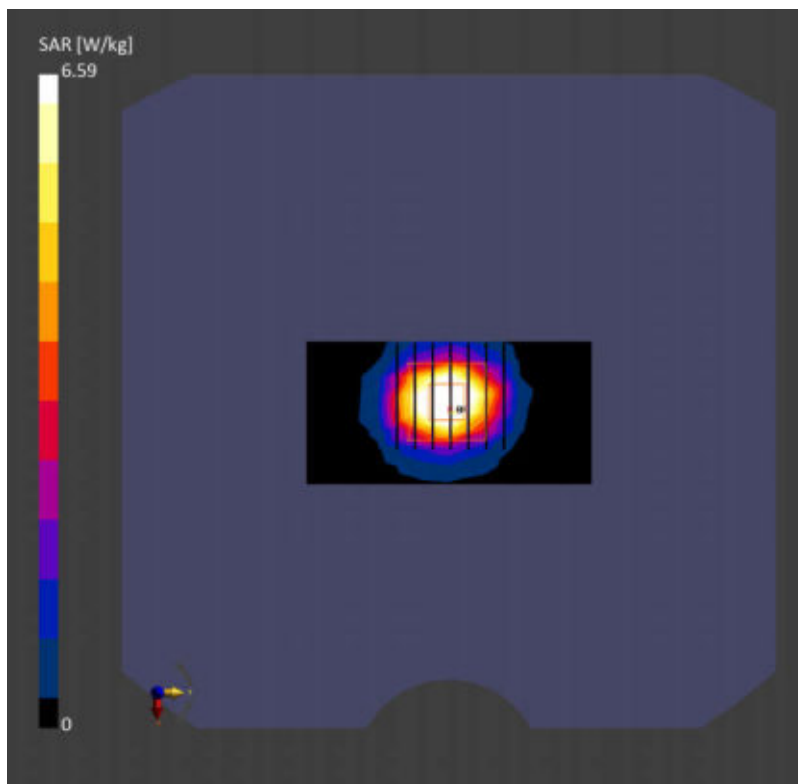

Date: 2025/7/24

System Check_3700MHz**DUT:D3700V2-SN:1008**


Communication System: CW; Frequency: 3700.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 3700.0$ MHz; $\sigma = 3.15$ S/m; $\epsilon_r = 39.0$
Ambient Temperature: 23.7°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.92, 6.17, 6.53); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 6.96 W/kg; SAR (10g) = 2.64 W/kg;

Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 7.03 W/kg; SAR (10g) = 2.63 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 76.6 %

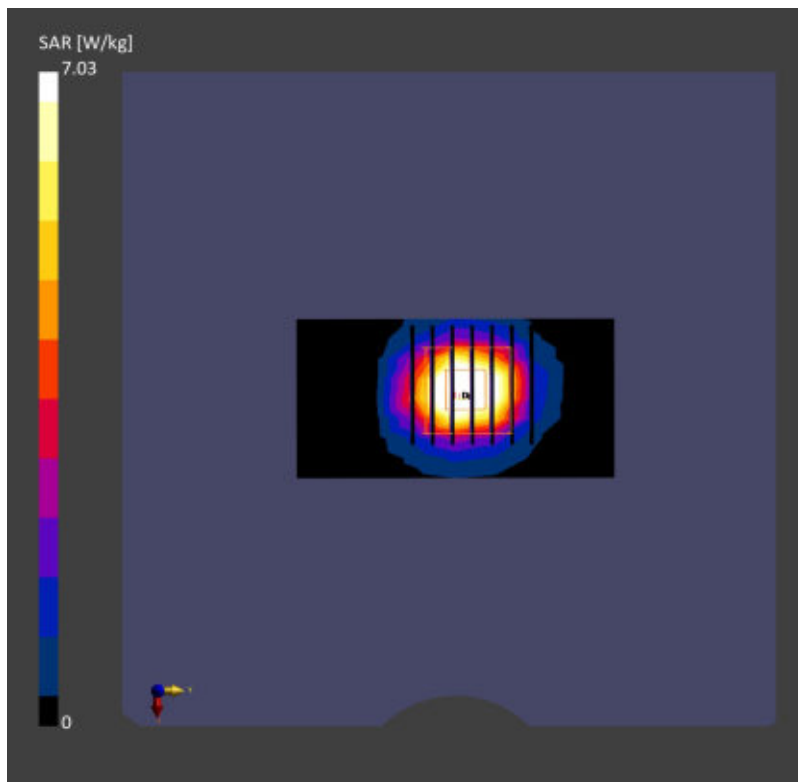

Date: 2025/7/14

System Check_3900MHz**DUT:D3900V2-SN:1022**


Communication System: CW; Frequency: 3900.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 3900.0$ MHz; $\sigma = 3.26$ S/m; $\epsilon_r = 38.3$
Ambient Temperature: 23.1°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.83, 6.09, 6.45); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 6.54 W/kg; SAR (10g) = 2.33 W/kg;

Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.00 dB
SAR (1g) = 6.45 W/kg; SAR (10g) = 2.25 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 75.3 %

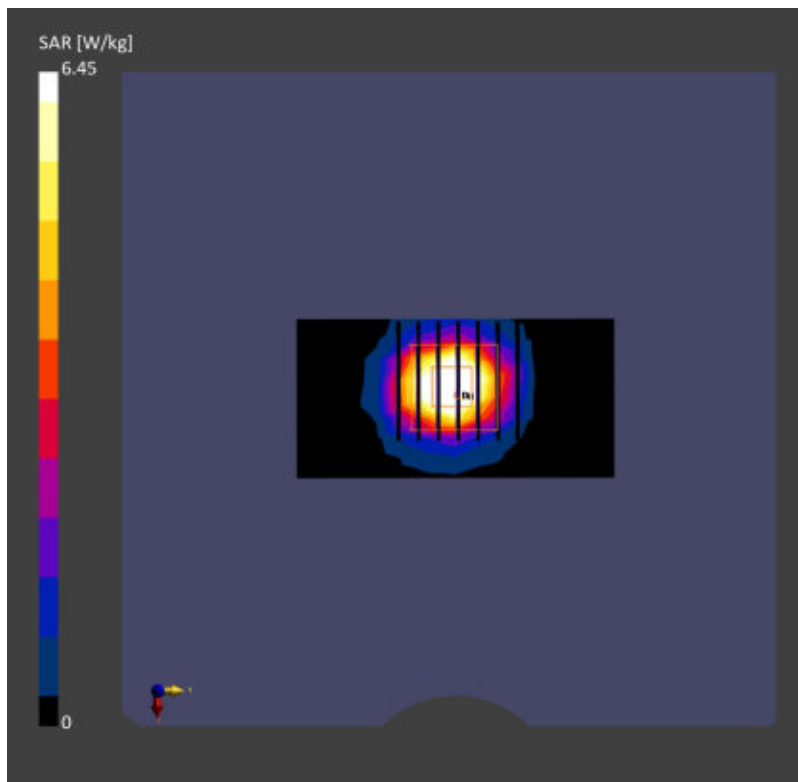

Date: 2025/8/6

System Check_3900MHz**DUT:D3900V2-SN:1022**


Communication System: CW; Frequency: 3900.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 3900.0$ MHz; $\sigma = 3.23$ S/m; $\epsilon_r = 38.5$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(6.83, 6.09, 6.45); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 7.16 W/kg; SAR (10g) = 2.57 W/kg;

Pin=100mW/Zoom Scan (28.0 mm x 28.0 mm x 28.0 mm): Measurement Grid: 5.0 mm x 5.0 mm x 1.4 mm
Power Drift = 0.03 dB
SAR (1g) = 7.12 W/kg; SAR (10g) = 2.47 W/kg
Smallest distance from peaks to all points 3 dB below = 8.0 mm
Ratio of SAR at M2 to SAR at M1 = 75.8 %

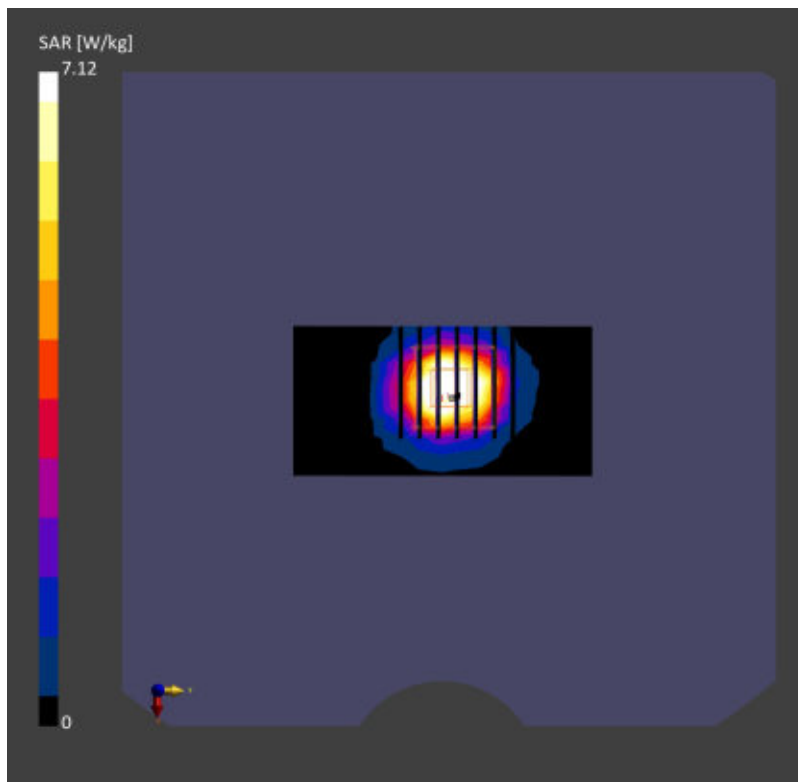

Date: 2025/7/18

System Check_5250MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.55$ S/m; $\epsilon_r = 36.5$
Ambient Temperature: 23.6°C; Liquid Temperature: 22.2°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(5.59, 4.99, 5.28); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 7.62 W/kg; SAR (10g) = 2.20 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 7.97 W/kg; SAR (10g) = 2.28 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 65.2 %

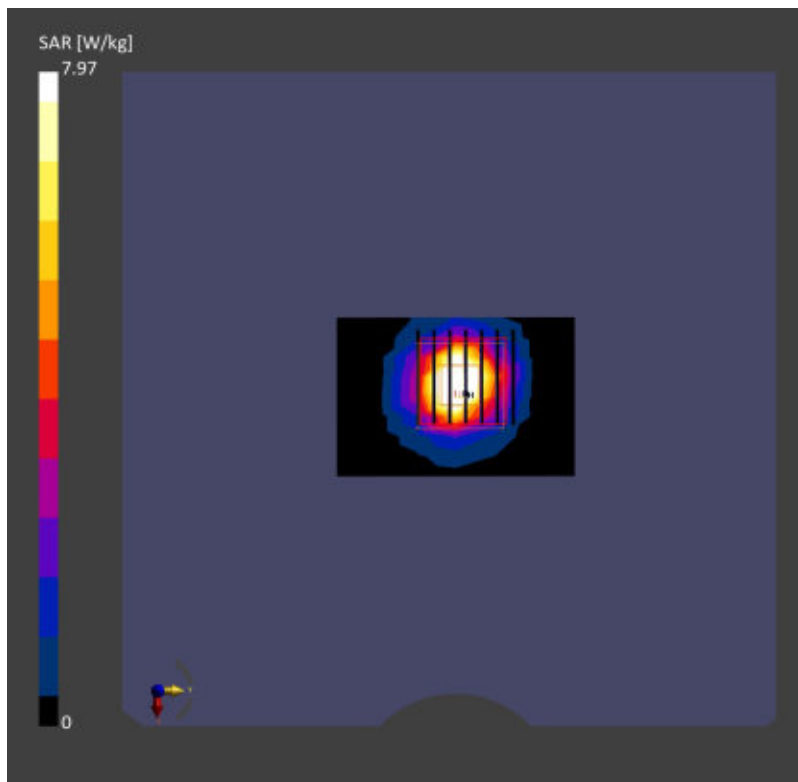

Date: 2025/8/7

System Check_5250MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5250.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5250.0$ MHz; $\sigma = 4.62$ S/m; $\epsilon_r = 36.3$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.1°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(5.59, 4.99, 5.28); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 7.73 W/kg; SAR (10g) = 2.22 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.08 dB
SAR (1g) = 8.14 W/kg; SAR (10g) = 2.33 W/kg
Smallest distance from peaks to all points 3 dB below = 7.2 mm
Ratio of SAR at M2 to SAR at M1 = 64.3 %

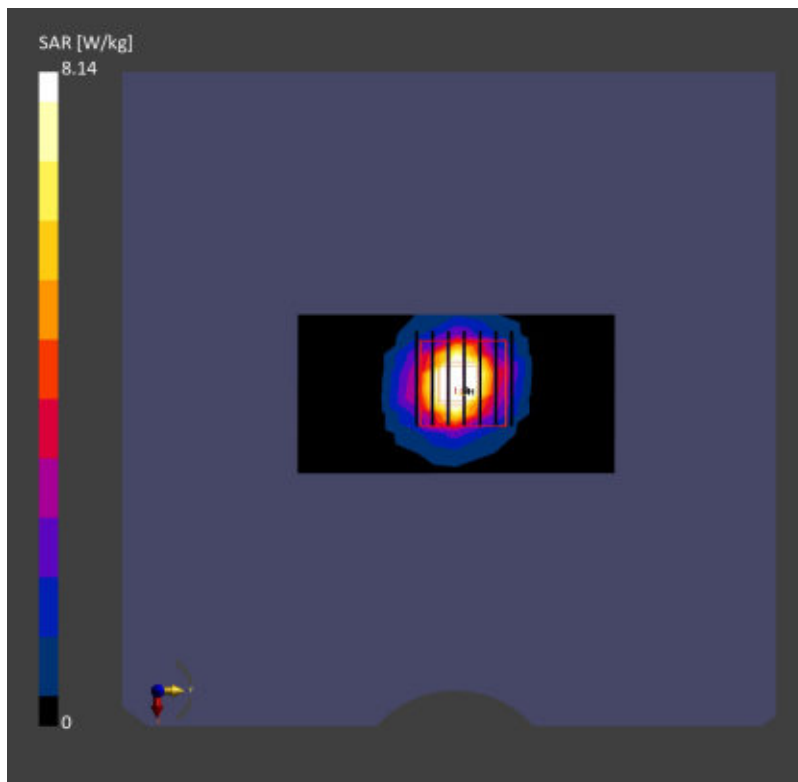

Date: 2025/7/20

System Check_5600MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 5.05$ S/m; $\epsilon_r = 35.3$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(5.26, 4.69, 4.97); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 7.78 W/kg; SAR (10g) = 2.26 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.00 dB
SAR (1g) = 8.22 W/kg; SAR (10g) = 2.34 W/kg
Smallest distance from peaks to all points 3 dB below = 7.4 mm
Ratio of SAR at M2 to SAR at M1 = 62.4 %

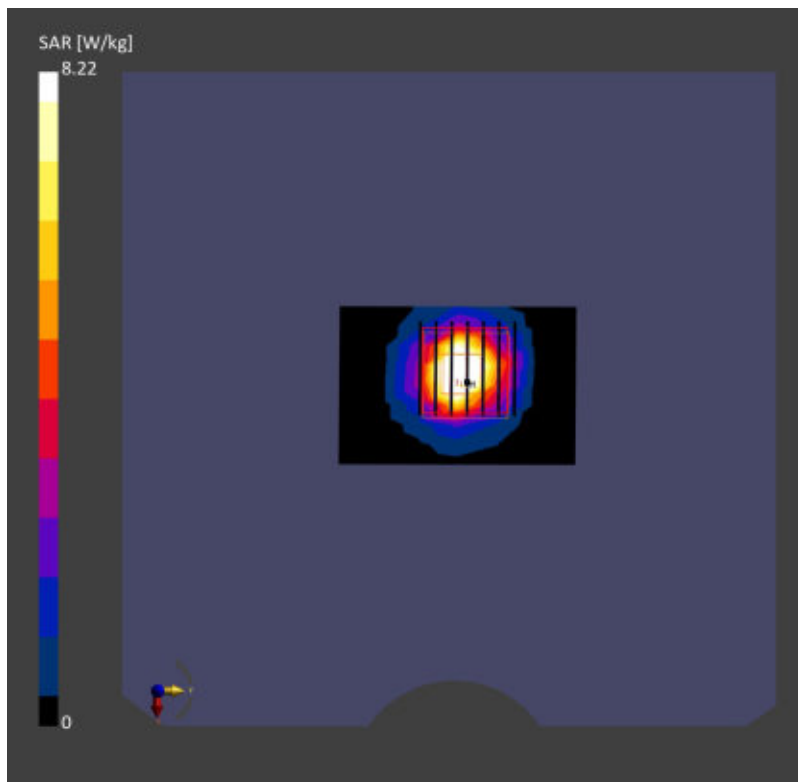

Date: 2025/7/28

System Check_5600MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5600.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5600.0$ MHz; $\sigma = 5.01$ S/m; $\epsilon_r = 35.6$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.5°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(5.26, 4.69, 4.97); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 7.63 W/kg; SAR (10g) = 2.17 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.02 dB
SAR (1g) = 8.80 W/kg; SAR (10g) = 2.49 W/kg
Smallest distance from peaks to all points 3 dB below = 7.4 mm
Ratio of SAR at M2 to SAR at M1 = 60.8 %

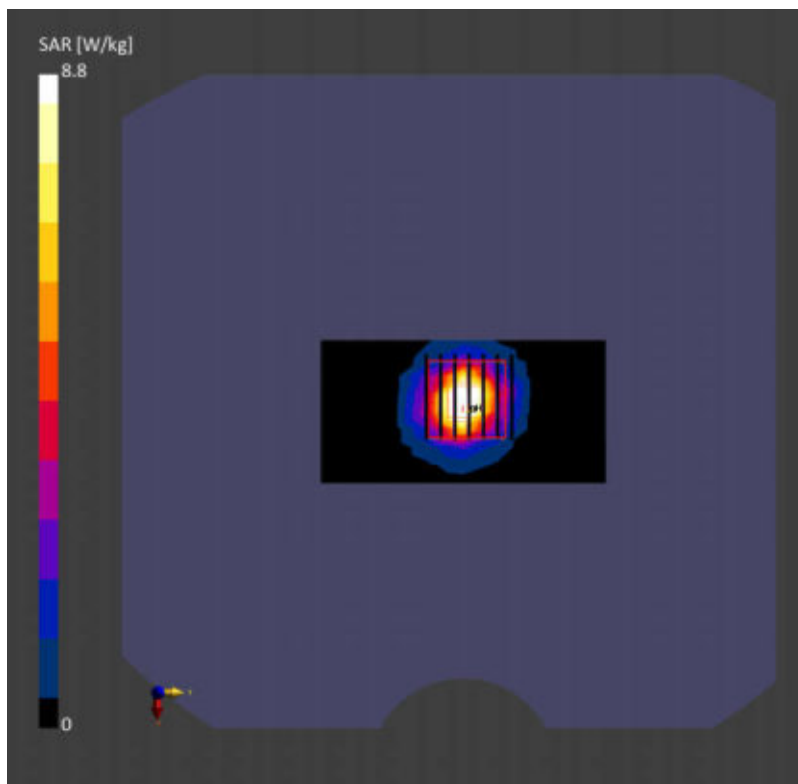

Date: 2025/7/21

System Check_5800MHz**DUT:D5GHzV2-SN:1341**


Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.19$ S/m; $\epsilon_r = 35.1$
Ambient Temperature: 23.3°C; Liquid Temperature: 22.3°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(5.17, 4.61, 4.89); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 60.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 7.87 W/kg; SAR (10g) = 2.26 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = 0.01 dB
SAR (1g) = 8.17 W/kg; SAR (10g) = 2.31 W/kg
Smallest distance from peaks to all points 3 dB below = 7.4 mm
Ratio of SAR at M2 to SAR at M1 = 62.5 %

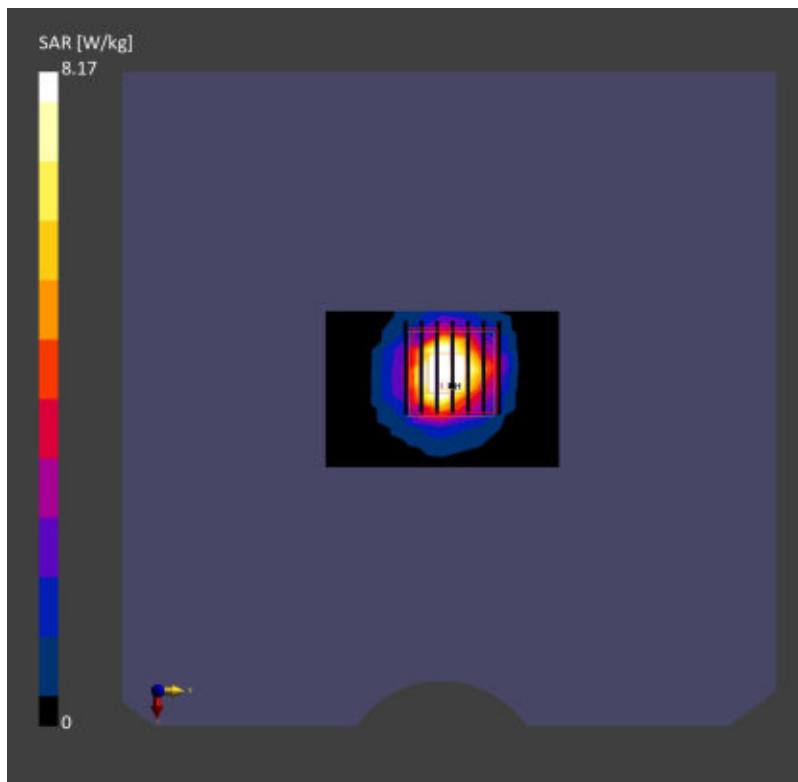

Date: 2025/8/10

System Check_5800MHz**DUT:D5GHzV2-SN:1341**

Communication System: CW; Frequency: 5800.0 MHz; Duty Cycle: 1:1
Medium: HSL Medium parameters used: $f = 5800.0$ MHz; $\sigma = 5.15$ S/m; $\epsilon_r = 35.4$
Ambient Temperature: 23.2°C; Liquid Temperature: 22.7°C

DASY6 Configuration:

- Probe: EX3DV4 - SN3819; ConvF(5.17, 4.61, 4.89); Calibrated: 2024/8/22
- Sensor-Surface: 1.4 mm
- Electronics: DAE4 Sn1386; Calibrated: 2024/8/30
- Phantom: Twin-SAM V5.0 (30deg probe tilt); Serial: 1670; Section: Flat
- Measurement Software: 16.2.2.1588
- UID: CW, 0--

Pin=100mW/Area Scan (40.0 mm x 80.0 mm): Measurement Grid: 5.0 mm x 10.0 mm
mmSAR (1g) = 7.94 W/kg; SAR (10g) = 2.27 W/kg;

Pin=100mW/Zoom Scan (22.0 mm x 22.0 mm x 22.0 mm): Measurement Grid: 4.0 mm x 4.0 mm x 1.4 mm
Power Drift = -0.02 dB
SAR (1g) = 8.45 W/kg; SAR (10g) = 2.39 W/kg
Smallest distance from peaks to all points 3 dB below = 7.6 mm
Ratio of SAR at M2 to SAR at M1 = 60.0 %

