

Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the liquid level reaching approximately the 10 cm mark. The container has a blue outer rim and a white inner lining.	NA

3. Photographs of EUT test position

Photo 2: Left Cheek

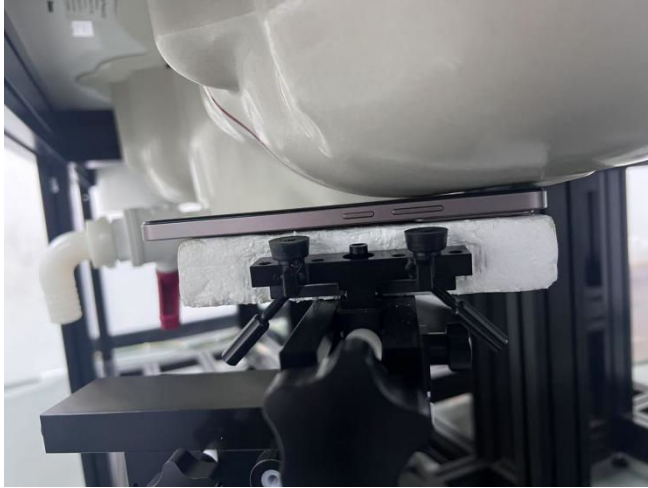


Photo 3: Left Tilted



Photo 4: Right Cheek

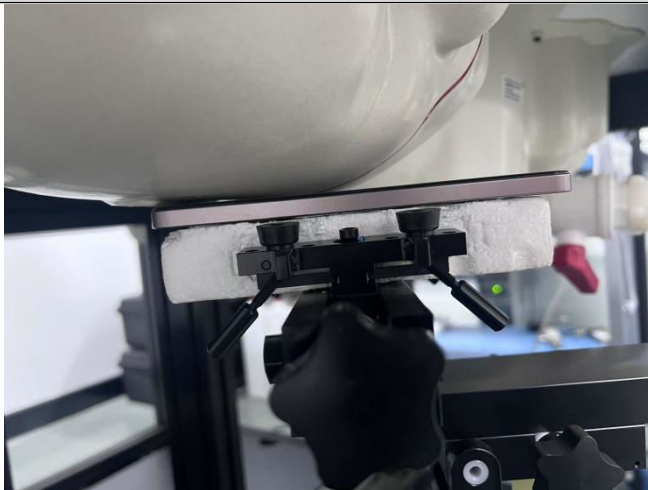


Photo 5: Right Tilted



Photo 6: Front side 15mm

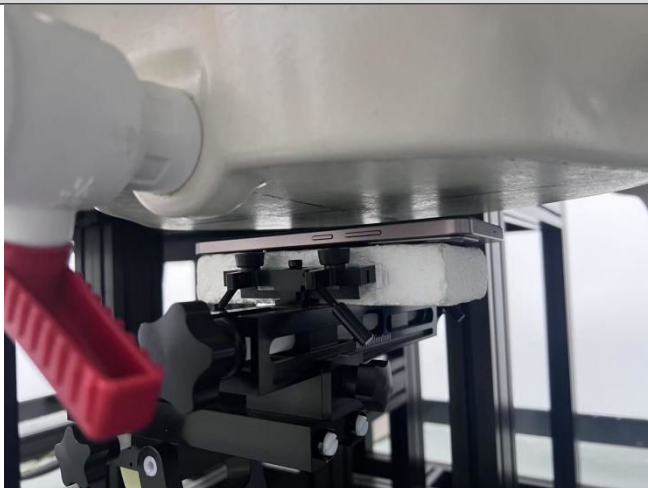


Photo 7: Back side 15mm



Photo 8: Front side 10mm



Photo 9: Back side 10mm



Photo 10: Left side 10mm



Photo 11: Right side 10mm



Photo 12: Top side 10mm

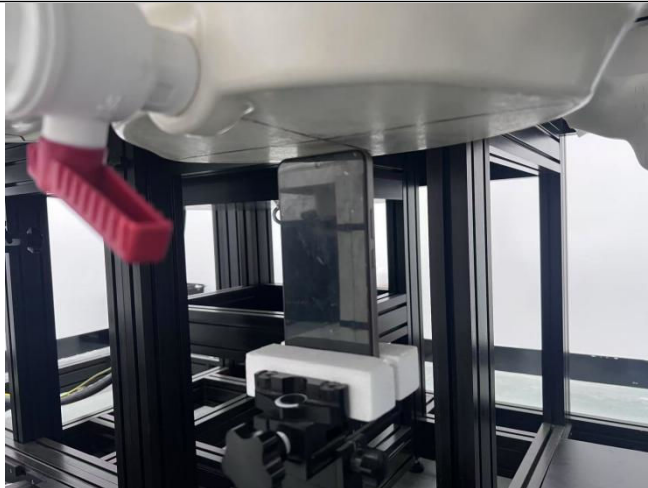


Photo 13: Bottom side 10mm

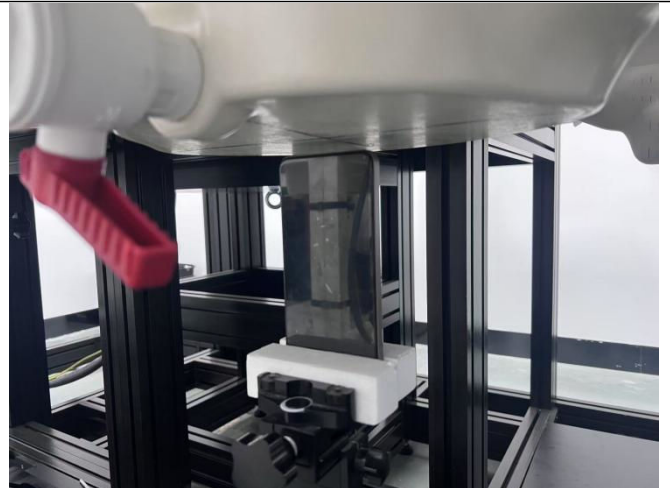


Photo 14: Front side 0mm



Photo 15: Back side 0mm



Photo 16: Left side 0mm



Photo 17: Right side 0mm



Photo 18: Top side 0mm

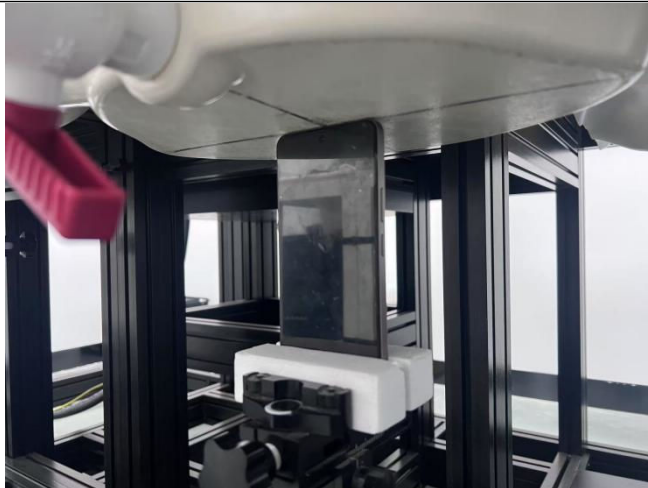


Photo 19: NFC Front side 0mm



Photo 20: NFC Back side 0mm



Photo 21: NFC Left side 0mm



Photo 22: NFC Right side 0mm



Photo 23: NFC Top side 0mm



Photo 24: NFC Bottom side 0mm



4. EUT Constructional Details

Photo 25: Front View

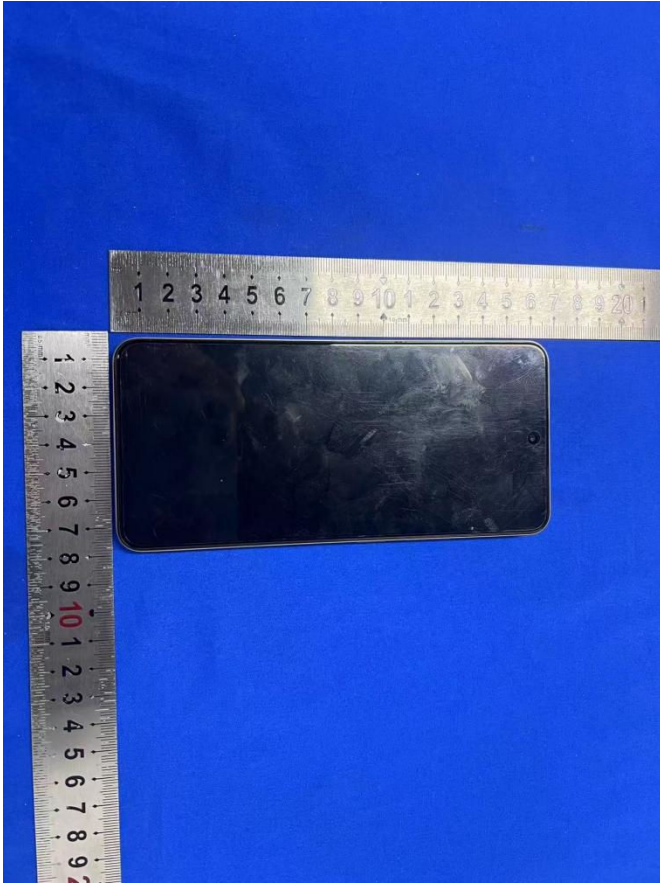


Photo 26: Back View

