



CERTIFICATION TEST REPORT

Report Number: R13105073-E1

Applicant : SONIQUENCE LLC
2477 GRAND AVE
BALDWIN, NY 11510-3556

Model : Soniquence Generator

FCC ID : 2AV4P-0270412

EUT Description : MEDICAL DEVICE WITH RFID RADIO

Test Standard(s) : FCC 47 CFR PART 15 SUBPART C
ISED CANADA RSS-210 ISSUE 10

Date Of Issue:

June 12, 2020

Prepared by:

UL LLC

12 Laboratory Dr.

Research Triangle Park, NC 27709 U.S.A.

TEL: (919) 549-1400



NVLAP Lab code: 200246-0

REPORT REVISION HISTORY

Rev.	Issue Date	Revisions	Revised By
V1	2020-05-29	Initial Issue	Cristian Melara
V2	2020-06-03	- Revised applicant address	Cristian Melara
V3	2020-06-12	- Revised model name - Revised test methodology and references	Cristian Melara

TABLE OF CONTENTS

REPORT REVISION HISTORY	2
TABLE OF CONTENTS	3
1. ATTESTATION OF TEST RESULTS.....	4
2. TEST METHODOLOGY	6
3. FACILITIES AND ACCREDITATION.....	6
4. CALIBRATION AND UNCERTAINTY	7
4.1. MEASURING INSTRUMENT CALIBRATION	7
4.2. SAMPLE CALCULATION.....	7
4.3. MEASUREMENT UNCERTAINTY	7
5. EQUIPMENT UNDER TEST	8
5.1. EUT DESCRIPTION.....	8
5.2. MAXIMUM FIELD STRENGTH.....	8
5.3. SOFTWARE AND FIRMWARE	8
5.4. WORST-CASE CONFIGURATION AND MODE.....	8
5.5. DESCRIPTION OF TEST SETUP.....	9
6. MEASUREMENT METHOD	10
7. TEST AND MEASUREMENT EQUIPMENT	11
8. OCCUPIED BANDWIDTH AND 20dB BANDWIDTH.....	13
8.1. 99% BANDWIDTH PLOT	14
8.2. 20dB BANDWIDTH PLOT	15
9. FREQUENCY STABILITY.....	16
10. RADIATED TEST RESULTS	17
10.1. LIMITS AND PROCEDURE	17
10.2. TRANSMISSION SPURIOUS EMISSIONS.....	19
10.2.1. TAG	20
10.2.2. WITHOUT TAG.....	26
11. AC POWER LINE CONDUCTED EMISSIONS.....	32
11.1. RFID	33
11.1.1. NORMAL OPERATION	33
11.1.2. ANTENNAS TERMINATED	35
12. SETUP PHOTOS.....	37

1. ATTESTATION OF TEST RESULTS

COMPANY NAME: SONIQUENCE LLC
2477 GRAND AVE
BALDWIN, NY 11510-3556

EUT DESCRIPTION: MEDICAL DEVICE WITH RFID RADIO

MODEL: Soniquence Generator

SERIAL NUMBER: 1S130008

DATE TESTED: 2020-03-05 to 2020-04-03

APPLICABLE STANDARDS	
STANDARD	TEST RESULTS
CFR 47 Part 15 Subpart C	Complies
ISED CANADA RSS-210 Issue 10, Annex B.6	Complies
ISED CANADA RSS-GEN Issue 5	Complies

UL LLC tested the above equipment in accordance with the requirements set forth in the above standards. The test results show that the equipment tested is capable of demonstrating compliance with the requirements as documented in this report.

The results documented in this report apply only to the tested sample, under the conditions and modes of operation as described herein. It is the manufacturer's responsibility to assure that additional production units of this model are manufactured with identical electrical and mechanical components. All samples tested were in good operating condition throughout the entire test program. Measurement Uncertainties are published for informational purposes only and were not taken into account unless noted otherwise.


This document may not be altered or revised in any way unless done so by UL LLC and all revisions are duly noted in the revisions section. Any alteration of this document not carried out by UL LLC will constitute fraud and shall nullify the document. This report must not be used by the client to claim product certification, approval, or endorsement by NVLAP, NIST, or any agency of the U.S. government.

Approved & Released For
UL LLC By:



Jeffrey Moser
Operations Leader
Consumer Technology Division
UL LLC

Prepared By:



Cristian Melara
Engineer
Consumer Technology Division
UL LLC

2. TEST METHODOLOGY

The tests documented in this report were performed in accordance with ANSI C63.10-2013, FCC CFR 47 Part 2, FCC CFR 47 Part 15, RSS-GEN Issue 5 and RSS-210 Issue 10 Annex B.6.

3. FACILITIES AND ACCREDITATION

The test sites and measurement facilities used to collect data are located at 12 Laboratory Drive, Research Triangle Park, North Carolina, USA and 2800 Perimeter Park Dr., Suite B, Morrisville, North Carolina, USA. The following table identifies which facilities were utilized for radiated emission measurements documented in this report. Specific facilities are also identified in the test results sections.

12 Laboratory Dr.		2800 Perimeter Park Dr.	
ISED Site Code: 2180C			
☐	Chamber A RTP	☐	North Chamber
☐	Chamber C RTP	☒	South Chamber

UL LLC (RTP) is accredited by NVLAP, Laboratory Code 200246-0

4. CALIBRATION AND UNCERTAINTY

4.1. MEASURING INSTRUMENT CALIBRATION

The measuring equipment utilized to perform the tests documented in this report has been calibrated in accordance with the manufacturer's recommendations, and is traceable to recognized national standards.

4.2. SAMPLE CALCULATION

RADIATED EMISSIONS

Where relevant, the following sample calculation is provided:

Field Strength (dBuV/m) = Measured Voltage (dBuV) + Antenna Factor (dB/m) + Cable Loss (dB) – Preamp Gain (dB)
 $36.5 \text{ dBuV} + 18.7 \text{ dB/m} + 0.6 \text{ dB} - 26.9 \text{ dB} = 28.9 \text{ dBuV/m}$

MAINS CONDUCTED EMISSIONS

Where relevant, the following sample calculation is provided:

Final Voltage (dBuV) = Measured Voltage (dBuV) + Cable Loss (dB) + Limiter Factor (dB) + LISN Insertion Loss.
 $36.5 \text{ dBuV} + 0 \text{ dB} + 10.1 \text{ dB} + 0 \text{ dB} = 46.6 \text{ dBuV}$

4.3. MEASUREMENT UNCERTAINTY

Where relevant, the following measurement uncertainty levels have been estimated for tests performed on the apparatus:

PARAMETER	UNCERTAINTY
Radio Frequency (Spectrum Analyzer)	141.2 Hz
Occupied Channel Bandwidth	2.00%
Unwanted Emissions, conducted	3.05 dB
All emissions, radiated	4.88 dB
Temperature	2.26°C
Humidity	6.79%
DC Supply voltages	1.70%
Time	3.39%

Uncertainty figures are valid to a confidence level of 95%.

5. EQUIPMENT UNDER TEST

5.1. EUT DESCRIPTION

The EUT, Soniquence Generator, is a medical device that generates high radiofrequency energy for surgical applications. The EUT employs a 13.56 MHz RFID radio for the detection of the type of tool connected to the instrument.

5.2. MAXIMUM FIELD STRENGTH

The maximum E-field reading with tag at 30m is 24.19 dBuV/m.

The maximum E-field reading without tag at 30m is -4.81 dBuV/m.

5.3. SOFTWARE AND FIRMWARE

The test utility software used during testing was V6-08.

5.4. WORST-CASE CONFIGURATION AND MODE

The EUT is intended to be installed in only one orientation therefore all radiated testing was performed in its intended orientation (X-Axis). The EUT was tested with both RFIDs transmitting simultaneously for worst case emissions.

Worst case emissions were found to be with the tags (tools) in place. Occupied bandwidth, frequency tolerance, and AC mains emissions testing were performed with tags.

5.5. DESCRIPTION OF TEST SETUP

SUPPORT EQUIPMENT

Support Equipment List				
Description	Manufacturer	Model	Serial Number	FCC ID
Triple footswitch	Soniquence	TF-FSCB	00014	N/A
3-Button Fingerswitch Handpiece	Soniquence	N/A	N/A	N/A
Resistor	N/A	N/A	N/A	N/A
Neutral Plate	Soniquence	N/A	N/A	N/A

I/O CABLES

I/O Cable List						
Cable No.	Port	# of Identical Ports	Connector Type	Cable Type	Cable Length (m)	Remarks
1	AC power	1	C14	AC	0.2 m	
2	Monopolar	1	3-pin	I/O	0.3 m	Cable integrated with 3-Button Fingerswitch Handpiece
3	Bipolar	1	2-pin	I/O	0.3 m	Connected to resistor
4	Neutral	1	3-pin	I/O	0.3 m	Cable integrated with neutral plate
5	Footswitch	1	Multi pin	I/O	4 m	Cable integrate with footswitch

TEST SETUP

The EUT is installed as a standalone device.

SETUP DIAGRAMS

Please refer to R13105073-EP1 for setup diagram.

6. MEASUREMENT METHOD

Occupied BW (20dB): ANSI C63.10-2013 Section 6.9.2

Occupied BW (99%): ANSI C63.10-2013 Section 6.9.3

Frequency Stability : ANSI C63.10-2013 Clause 6.8

General Radiated emissions: ANSI C63.10 Section 6.3 to 6.5

AC Power Line Conducted Emissions: ANSI C63.10-2013, Section 6.2 and KDB 174176 D01
Line Conducted FAQ v01r01, Q5.

7. TEST AND MEASUREMENT EQUIPMENT

The following test and measurement equipment was utilized for the tests documented in this report:

Test Equipment Used - Radiated Disturbance Emissions Test Equipment (Morrisville - South Chamber)

Equip. ID	Description	Manufacturer	Model Number	Last Cal.	Next Cal.
	0.009-30MHz	(Loop Ant.)			
AT0079	Active Loop Antenna	ETS-Lindgren	6502	2019-08-08	2020-08-08
	30-1000 MHz				
AT0074	Hybrid Broadband Antenna	Sunol Sciences Corp.	JB3	2019-07-16	2020-07-16
	Gain-Loss Chains				
S-SAC01	Gain-loss string: 0.009-30MHz	Various	Various	2019-05-02	2020-05-02
S-SAC02	Gain-loss string: 25-1000MHz	Various	Various	2019-05-02	2020-05-02
	Receiver & Software				
SA0027	Spectrum Analyzer	Agilent	N9030A	2019-05-15	2020-05-15
SOFTEMI	EMI Software	UL	Version 9.5 June 15, 2019	NA	NA
	Additional Equipment used				
s/n 181474409	Environmental Meter	Fisher Scientific	15-077-963	2018-07-27	2020-07-27

NOTES:

1. For equipment listed above that was calibrated during the testing period, please note the equipment was used for testing after calibration.
2. For equipment listed above that has a calibration due date during the testing period, the testing was completed before the equipment expiration date.

Test Equipment Used - Wireless Conducted Measurement Equipment

Equip. ID	Description	Manufacturer	Model Number	Last Cal.	Next Cal.
Conducted Room 2					
T177 (PRE0079253)	Spectrum Analyzer	Agilent Technologies	E4446A	2019-04-22	2020-04-22
76023 (EC0225)	Temp/Humid Chamber	Cincinnati Sub-Zero	ZPH-8-3.5-SCT/AC	2019-06-14	2020-06-14
SN 181474341	Environmental Meter	Fisher Scientific	15-077-963	2018-07-27	2020-07-27
76021	DC Regulated Power Supply	CircuitSpecialists.Com	CSI3005X5	N/A	N/A
SOFTEMI	EMC Software	UL	Version 2020.03.11	NA	NA
Additional Equipment used					
MM0167	Multi-Meter	Agilent	U1232A	2019-08-23	2020-08-23

NOTES:

1. For equipment listed above that was calibrated during the testing period, please note the equipment was used for testing after calibration.
2. For equipment listed above that has a calibration due date during the testing period, the testing was completed before the equipment expiration date.

Test Equipment Used - Line-Conducted Emissions – Voltage (Morrisville – Conducted 1)

Equip. ID	Description	Manufacturer	Model Number	Last Cal.	Next Cal.
CBL087	Coax cable, RG223, N-male to BNC-male, 20-ft.	Pasternack	PE3W06143-240	2019-05-29	2020-05-29
s/n 181562858	Environmental Meter	Fisher Scientific	14-650-118	2018-09-04	2020-09-04
LISN003	LISN, 50-ohm/50-uH, 2-conductor, 25A	Fischer Custom Com.	FCC-LISN-50-25-2-01-550V	2019-08-19	2020-08-19
75141 (PRE0101521)	EMI Test Receiver 9kHz-7GHz	Rohde & Schwarz	ESCI 7	2019-08-20	2020-08-20
TL001	Transient Limiter, 0.009-30MHz	Com-Power	LIT-930A	2019-05-29	2020-05-29
PS214	AC Power Source	Elgar	CW2501M (s/n 1523A02396)	NA	NA
SOFTEMI	EMI Software	UL	Version 9.5 June 15, 2019	NA	NA
Miscellaneous (if needed)					
LISN008	LISN, 50-ohm/50-uH, 2-conductor, 25A (For support gear only.)	Solar Electronics	8012-50-R-24-BNC	2019-07-10	2020-07-10

NOTES:

1. For equipment listed above that was calibrated during the testing period, please note the equipment was used for testing after calibration.
2. For equipment listed above that has a calibration due date during the testing period, the testing was completed before the equipment expiration date.

8. OCCUPIED BANDWIDTH AND 20dB BANDWIDTH

LIMITS

None; for reporting purposes only.


FCC §15.215 (c) and RSS-GEN, ANSI C63.10 Sections 6.9.2 and 6.9.3 were used for the measurement procedure.

RESULTS

99% and 20dB BW

Frequency (MHz)	99% Bandwidth (KHz)	20dB Bandwidth (KHz)
13.56	457.4669	54.17


8.1. 99% BANDWIDTH PLOT

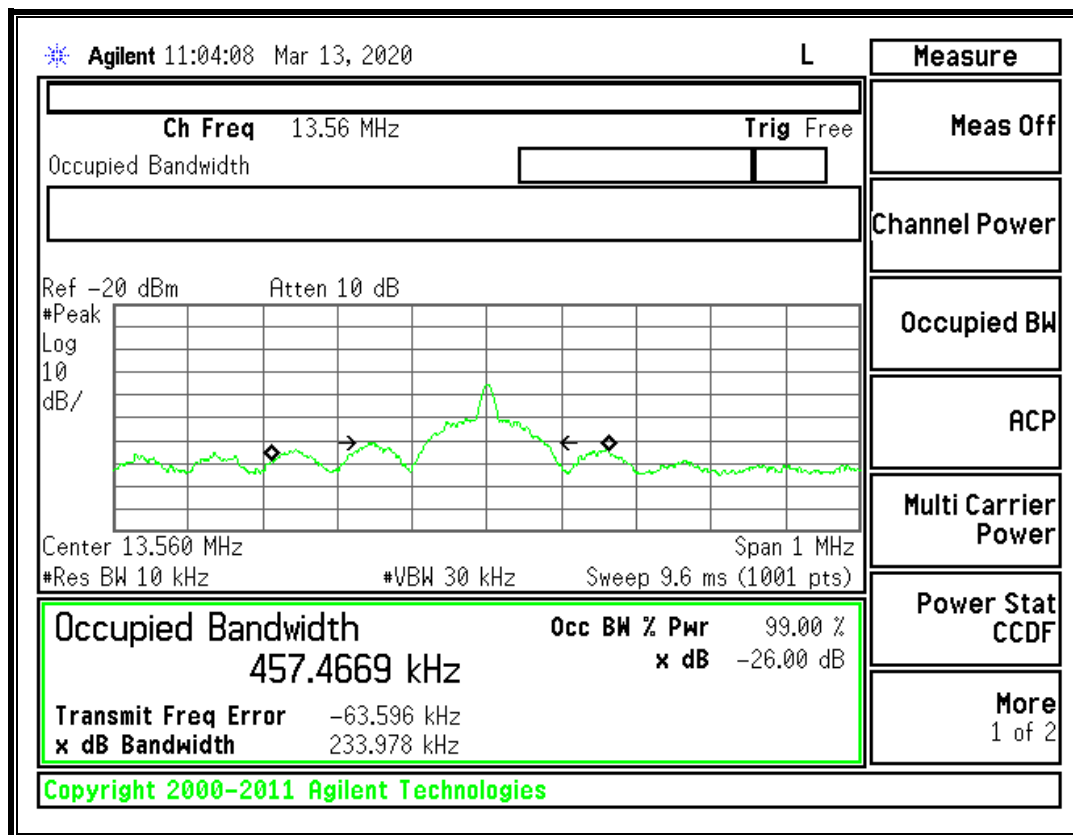

TEST INFORMATION

Test Date: 2020-03-13
Tested By: 40882

8.2. 20dB BANDWIDTH PLOT

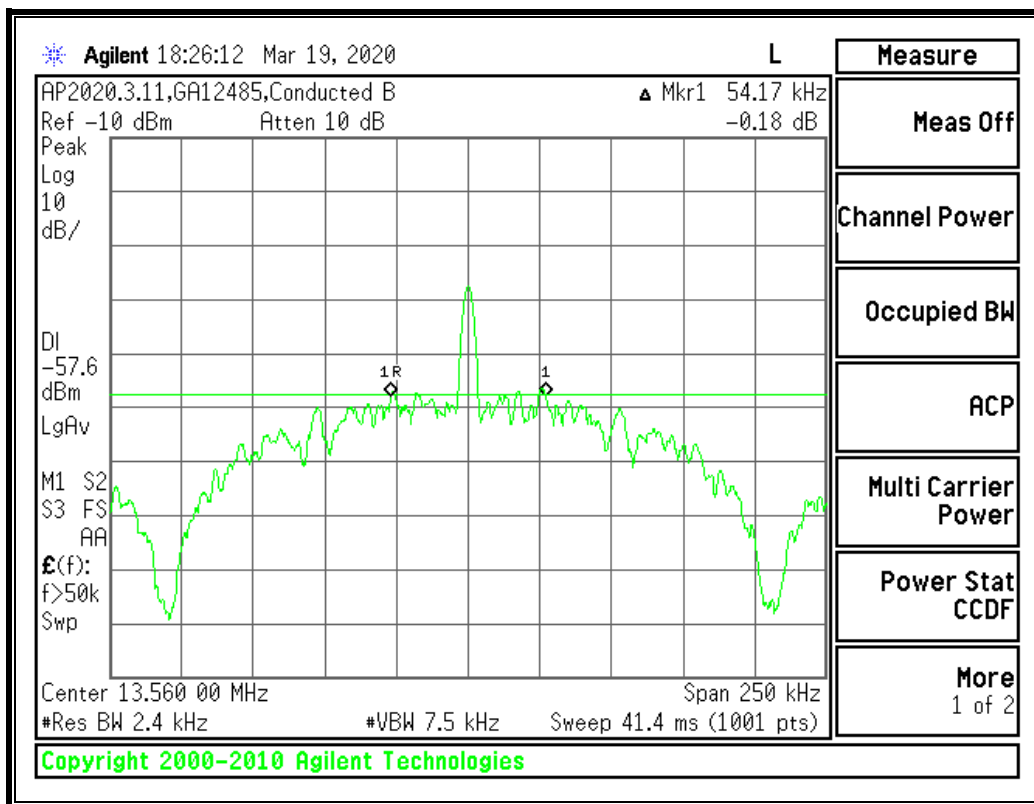

TEST INFORMATION

Test Date: 2020-03-13

Tested By: 40882

9. FREQUENCY STABILITY

LIMIT

§15.225 (e) The frequency tolerance of the carrier signal shall be maintained within $\pm 0.01\%$ of the operating frequency, over a temperature variation of -20 degrees to +50 degrees C at normal supply voltage, and for a variation in the primary supply voltage from 85% to 115% of the rated supply voltage at a temperature of 20 degrees C. For battery operated equipment, the equipment tests shall be performed using a new battery.

IC RSS-210, Annex B.6

Carrier frequency stability shall be maintained to $\pm 0.01\%$ (± 100 ppm).

TEST PROCEDURE

ANSI C63.10-2013 Clause 6.8

RESULTS

No non-compliance noted.

Reference Frequency: EUT Channel 13.56 MHz @ 20°C Limit: ± 100 ppm = 1.356 kHz										
Power Supply	Envir. Temp	Frequency Deviation Measured with Time Elapse								
VDC	(°C)	Startup (MHz)	Delta (ppm)	@ 2 mins (MHz)	Delta (ppm)	@ 5 mins (MHz)	Delta (ppm)	@ 10 mins (MHz)	Delta (ppm)	Limit (ppm)
120.00	50	13.5598780	5.015	13.5598760	5.162	13.5598730	5.383	13.5598720	5.457	± 100
120.00	40	13.5598990	3.466	13.5598960	3.687	13.5598920	3.982	13.5598890	4.204	± 100
120.00	30	13.5599180	2.065	13.5599140	2.360	13.5599130	2.434	13.5599130	2.434	± 100
120.00	20	13.5599460	0.000	13.5599390	0.516	13.5599340	0.885	13.5599380	0.590	± 100
120.00	10	13.5599630	-1.254	13.5599630	-1.254	13.5599630	-1.254	13.5599610	-1.106	± 100
120.00	0	13.5599730	-1.991	13.5599730	-1.991	13.5599740	-2.065	13.5599740	-2.065	± 100
120.00	-10	13.5599690	-1.696	13.5599690	-1.696	13.5599690	-1.696	13.5599700	-1.770	± 100
120.00	-20	13.5599730	-1.991	13.5599720	-1.917	13.5599710	-1.844	13.5599700	-1.770	± 100
138.00	20	13.5598990	3.466	13.5599000	3.392	13.5599000	3.392	13.5599100	2.655	± 100
102.00	20	13.5599120	2.507	13.5599100	2.655	13.5599090	2.729	13.5599070	2.876	± 100

TEST INFORMATION

Date: 2020-03-13

Tester: 40882

10. RADIATED TEST RESULTS

10.1. LIMITS AND PROCEDURE

LIMIT

§15.225

IC RSS-210, Annex B.6

IC RSS-GEN, Section 8.9 (Transmitter)

(a) The field strength of any emissions within the band 13.553–13.567 MHz shall not exceed 15,848 microvolts/ meter at 30 meters.

(b) Within the bands 13.410–13.553 MHz and 13.567–13.710 MHz, the field strength of any emissions shall not exceed 334 microvolts/meter at 30 meters.

(c) Within the bands 13.110–13.410 MHz and 13.710–14.010 MHz the field strength of any emissions shall not exceed 106 microvolts/meter at 30 meters.

(d) The field strength of any emissions appearing outside of the 13.110– 14.010 MHz and shall not exceed the general radiated emission limits in § 15.209 as follows:

§15.209 (a) Except as provided elsewhere in this subpart, the emissions from an intentional radiator shall not exceed the field strength levels specified in the following table:

Limits for radiated disturbance of an intentional radiator		
Frequency range (MHz)	Limits (µV/m)	Measurement Distance (m)
0.009 – 0.490	2400 / F (kHz)	300
0.490 – 1.705	24000 / F (kHz)	30
1.705 – 30.0	30	30
30 – 88	100**	3
88 - 216	150**	3
216 – 960	200**	3
Above 960	500	3

** Except as provided in paragraph (g), fundamental emissions from intentional radiators operating under this section shall not be located in the frequency bands 54-72 MHz, 76-88 MHz, 174-216 MHz or 470-806 MHz. However, operation within these frequency bands is permitted under other sections of this part, e.g. §§ 15.231 and 15.241.

§15.209 (b) In the emission table above, the tighter limit applies at the band edges.

Formula for converting the field strength from µV/m to dBµV/m is:

Limit (dBµV/m) = 20 log limit (µV/m)

In addition:

§15.209 (d) The emission limits shown the above table are based on measurements employing a CISPR quasi-peak detector except for the frequency bands 9-90 kHz, 110-490 kHz and above 1000 MHz. Radiated emissions limits in these three bands are based on measurements employing an average detector.

§15.209 (d) The provisions in §§ 15.225, measuring emissions at distances other than the distances specified in the above table, determining the frequency range over which radiated emissions are to be measured, and limiting peak emissions apply to all devices operated under this part.

Base on FCC 15.31 (f) (2): measurements may be performed at a distance closer than that specified in the regulations; however, an attempt should be made to avoid making measurements in the near field.

KDB 414788 Open Field Site(OFS) and Chamber Correlation Justification

OFS and chamber correlation testing had been performed and chamber measured test result is the worst case test result.

TEST PROCEDURE

ANSI C63.10, 2013

The EUT is an intentional radiator that incorporates a digital device, the highest fundamental frequency generated or used in the device is 13.56 MHz; therefore, the frequency range was investigated from 0.15 MHz to the 10th harmonic of highest fundamental frequency or to 40 GHz, whichever is lower.

Since the EUT contains a digital device operating at 13.56 MHz, the frequency range was expanded to 1 GHz, as specified in the following table

Highest frequency generated or used in the device or on which the device operates or tunes (MHz)	Upper frequency of measurement range (MHz)
Below 1.705	30.
1.705-108	1000.
108-500	2000.
500-1000	5000.
Above 1000	5th harmonic of the highest frequency or 40 GHz, whichever is lower.


10.2. TRANSMISSION SPURIOUS EMISSIONS

Note for below 30 MHz scans: All measurements were made at a test distance of 3 m. The measured data was extrapolated from the test distance (3m) to the specification distance (300 m from 9-490 kHz and 30 m from 490 kHz – 30 MHz) to clearly show the relative levels of fundamental and spurious emissions and demonstrate compliance with the requirement that the level of any spurious emissions be below the level of the intentionally transmitted signal. The extrapolation factor for the limits were $40 \cdot \log(\text{test distance} / \text{specification distance})$.

The below 30 MHz limits in CFR 47, Part 15, Subpart C, paragraph 15.209 (a), are identical to those in RSS-GEN Section 8.9, Table 6, since the measurements are performed in terms of magnetic field strength and converted to electric field strength levels (as reported in the table) using the free space impedance of 377Ω . For example, the measurement frequency 9.5 KHz resulted in a level of -14.44 dBuV/m, which is equivalent to $-14.44 - 51.5 = -65.94$ dBuA/m, which has the same margin, -62.49 dB, to the corresponding RSS-GEN Table 6 limit as it has to be 15.209(a) limit.

10.2.1. TAG

SPURIOUS AND HARMONICS EMISSIONS 9 kHz TO 30 MHz

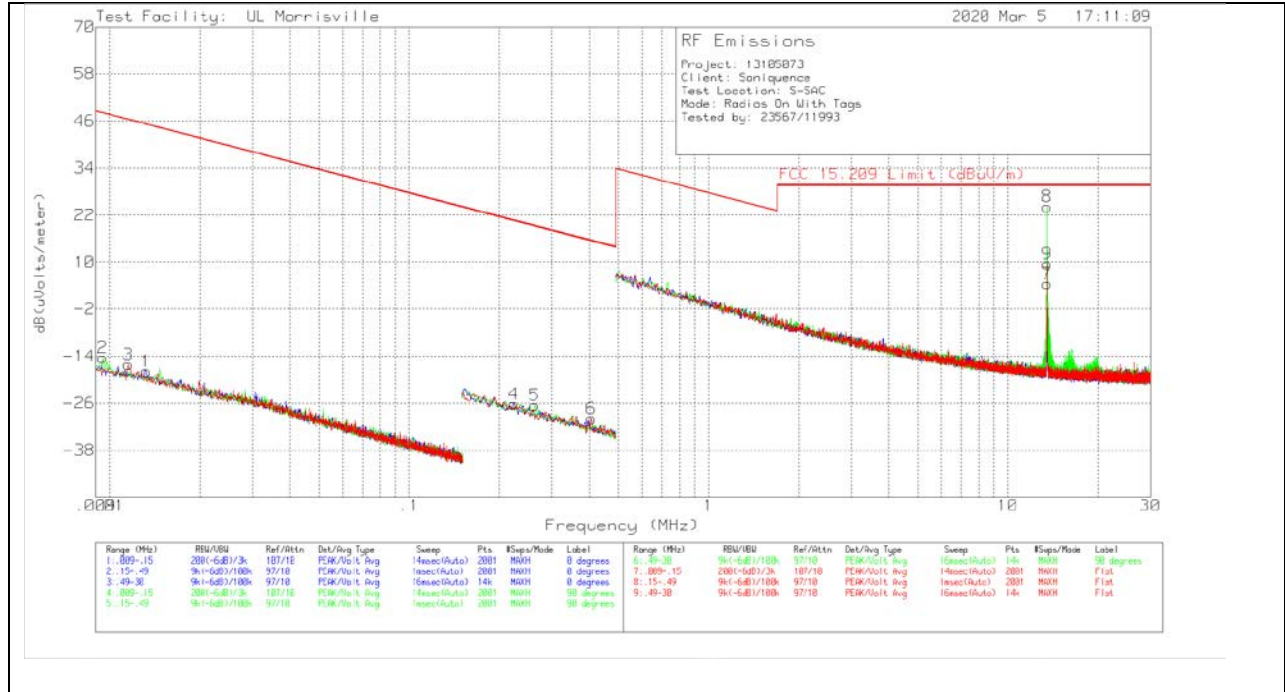


RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0079 AF (dB/m)	Cbl (dB)	Dist. Corr. Factor (dB)	Corrected Reading dB(uVolts/meter)	FCC 15.209 QP/AV Limit (dBuV/m)	FCC 15.209 PK Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)
2	.0095	46.86	Pk	18.6	.1	-80	-14.44	48.05	68.05	-62.49	0-360
3	.01156	46.2	Pk	17.5	.1	-80	-16.2	46.35	66.35	-62.55	0-360
1	.01326	45.13	Pk	16.8	.1	-80	-17.97	45.15	65.15	-63.12	0-360
4	.22429	42.71	Pk	11	.1	-80	-26.19	20.59	40.59	-46.78	0-360
5	.26339	42.36	Pk	11	.1	-80	-26.54	19.19	39.19	-45.73	0-360
6	.40568	38.94	Pk	11	.1	-80	-29.96	15.44	35.44	-45.4	0-360
7	13.5596	33.9	Pk	10	.6	-40	4.5	29.54	-	-25.04	0-360
8	13.5597	38.92	Qp	10	.6	-40	9.52	29.54	-	-20.02	230
9	13.5596	38.97	Pk	10	.6	-40	9.57	29.54	-	-19.97	0-360


Pk- Peak Detector

SPURIOUS AND HARMONIC EMISSIONS 30MHz to 1000MHz

VERTICAL RESULT

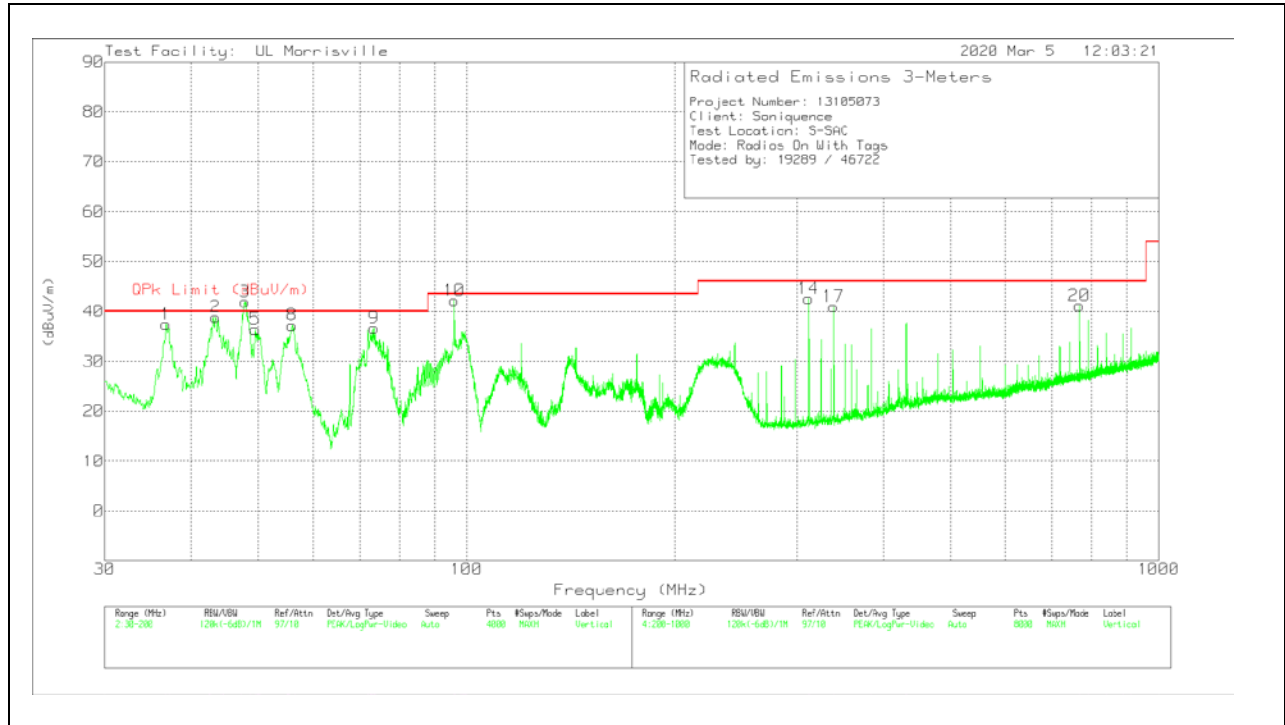

HORIZONTAL RESULT

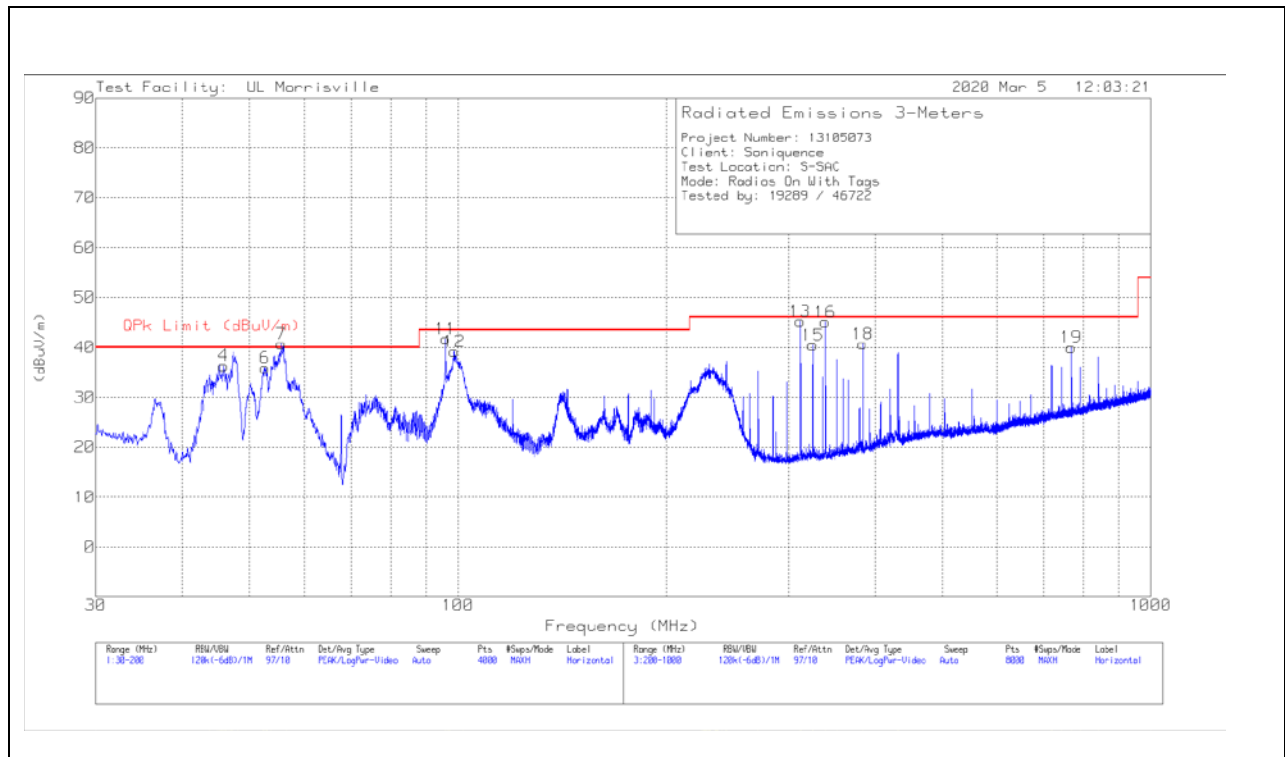


RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0074 AF (dB/m)	Cbl/Amp	Corrected Reading (dBuV/m)	QPk Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)	Height (cm)	Polarity
4	45.9621	47.25	Qp	15.7	-31.5	31.45	40	-8.55	155	374	H
6	52.8329	48.22	Qp	13.5	-31.5	30.22	40	-9.78	167	364	H
7	55.8371	53.3	Qp	13.4	-31.5	35.2	40	-4.8	172	386	H
11	95.9996	56.31	Qp	15.2	-31	40.51	43.52	-3.01	211	299	H
12	98.9178	50.52	Qp	16.1	-31	35.62	43.52	-7.9	194	294	H
13	311.882	54.49	Qp	19.8	-29.5	44.79	46.02	-1.23	149	101	H
15	325.4483	49.3	Qp	20	-29.5	39.8	46.02	-6.22	203	102	H
16	339.0039	54.05	Qp	20.1	-29.4	44.75	46.02	-1.27	134	101	H
18	384.0004	48.61	Qp	21.1	-29.3	40.41	46.02	-5.61	279	102	H
19	768.0016	41.97	Qp	27.1	-28.3	40.77	46.02	-5.25	17	125	H
1	36.8598	39.99	Qp	22.2	-31.7	30.49	40	-9.51	4	114	V
2	43.4457	47.68	Qp	17.3	-31.6	33.38	40	-6.62	163	117	V
3	47.9846	53.7	Qp	14.8	-31.5	37	40	-3	20	151	V
5	49.6775	48.25	Qp	14.1	-31.5	30.85	40	-9.15	325	127	V
8	55.9167	51.51	Qp	13.4	-31.5	33.41	40	-6.59	80	113	V
9	73.0442	45.98	Qp	14.1	-31.2	28.88	40	-11.12	308	157	V
10	96.0052	56.37	Qp	15.2	-31	40.57	43.52	-2.95	316	114	V
14	311.8852	52.11	Qp	19.8	-29.5	42.41	46.02	-3.61	277	163	V
17	338.9953	51.77	Qp	20.1	-29.4	42.47	46.02	-3.55	266	143	V
20	768.0023	41.33	Qp	27.1	-28.3	40.13	46.02	-5.89	126	102	V

Qp - Quasi-Peak detector

Fundamental 0 Degrees

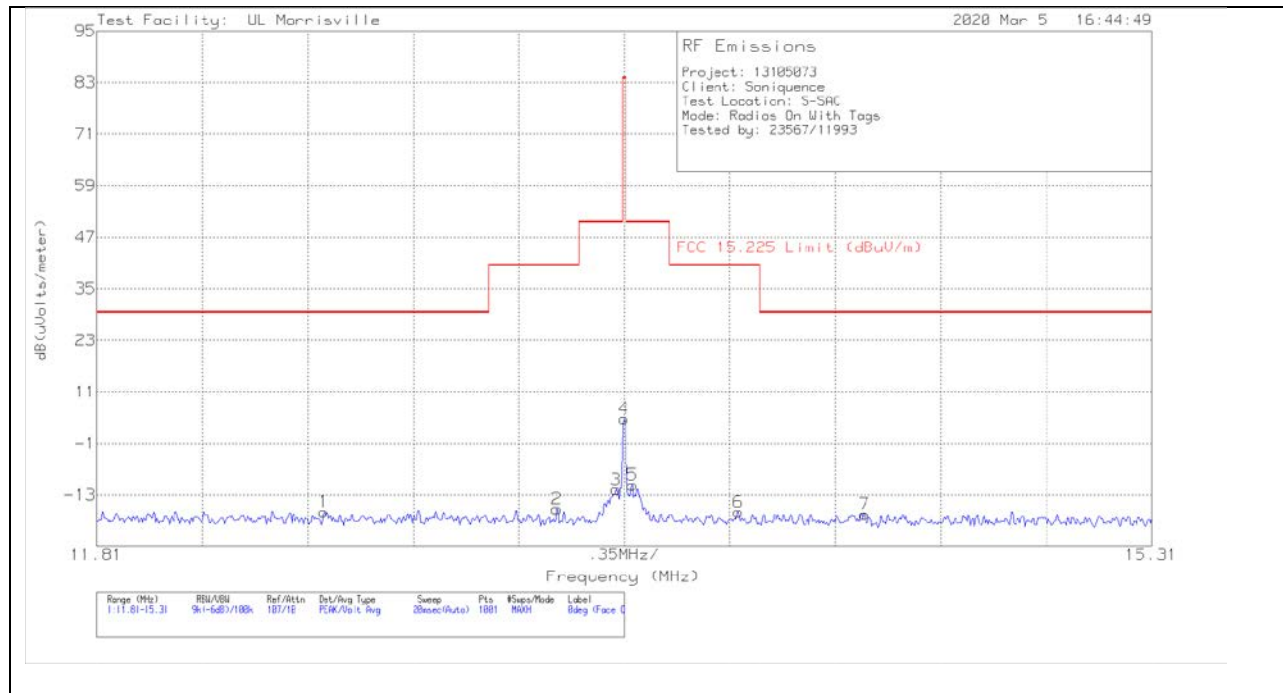

RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0079 AF (dB/m)	Cbl (dB)	Dist. Corr. Factor (dB)	Corrected Reading dB(uVolts/meter)	FCC 15.225 Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)
1	12.5625	12.4	Pk	10.1	.6	-40	-16.9	29.5	-46.4	239
2	13.336	13.12	Pk	10	.6	-40	-16.28	40.5	-56.78	239
3	13.532	17.66	Pk	10	.6	-40	-11.74	50.5	-62.24	239
4	13.56	34.15	Pk	10	.6	-40	4.75	84	-79.25	239
5	13.588	18.77	Pk	10	.6	-40	-10.63	50.5	-61.13	239
6	13.938	12.57	Pk	9.9	.6	-40	-16.93	40.5	-57.43	239
7	14.358	12.03	Pk	9.9	.6	-40	-17.47	29.5	-46.97	239

Pk - Peak detector

Test Facility: UL Morrisville

2020 Mar 5 16:52:11

RF Emissions

Project: 13105073

Client: Sonique

Test Location: S-SAC

Mode: Radios On With Tags

Tested by: 23567/11993

FCC 15.225 Limit (dBuV/m)

dB(μVolts/meter)


Frequency (MHz)

Range (MHz)	Ref/Att	Ref/Att	Det/Avrg Type	Sweep	Pls	#Sps/Mode	Label
1.1-15.3	96-165/100	10/10	Peak/Avg	20000/Hz	1001	1001	Strong/Face 1

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0079 AF (dB/m)	Cbl (dB)	Dist. Corr. Factor (dB)	Corrected Reading dB(uVolts/meter)	FCC 15.225 Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)
1	13.0805	15.61	Pk	10	.6	-40	-13.79	29.5	-43.29	185
2	13.399	23.95	Pk	10	.6	-40	-5.45	40.5	-45.95	185
3	13.532	35.77	Pk	10	.6	-40	6.37	50.5	-44.13	185
4	13.56	53.59	Pk	10	.6	-40	24.19	84	-59.81	185
5	13.588	36.46	Pk	10	.6	-40	7.06	50.5	-43.44	185
6	13.826	20.99	Pk	9.9	.6	-40	-8.51	40.5	-49.01	185
7	14.1445	15.73	Pk	9.9	.6	-40	-13.77	29.5	-43.27	185

Page 24 of 37

Fundamental Parallel to GRP

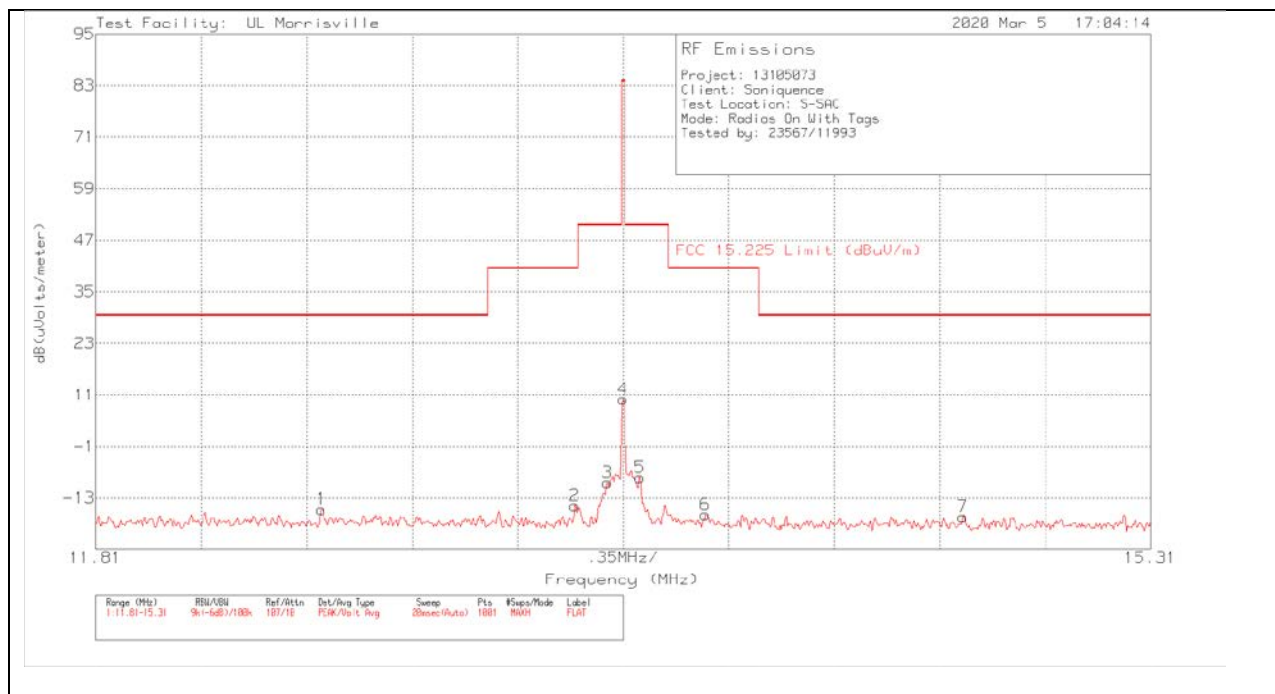


RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0079 AF (dB/m)	Cbl (dB)	Dist. Corr. Factor (dB)	Corrected Reading dB(uVolts/meter)	FCC 15.225 Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)
1	12.559	13.7	Pk	10.1	.6	-40	-15.6	29.5	-45.1	227
2	13.399	14.65	Pk	10	.6	-40	-14.75	40.5	-55.25	227
3	13.5075	20.01	Pk	10	.6	-40	-9.39	50.5	-59.89	227
4	13.56	39.43	Pk	10	.6	-40	10.03	84	-73.97	227
5	13.616	21.27	Pk	9.9	.6	-40	-8.23	50.5	-58.73	227
6	13.833	12.63	Pk	9.9	.6	-40	-16.87	40.5	-57.37	227
7	14.687	12.25	Pk	9.8	.6	-40	-17.35	29.5	-46.85	227

Pk - Peak detector

10.2.2. WITHOUT TAG

SPURIOUS AND HARMONICS EMISSIONS .09MHZ TO 30 MHZ

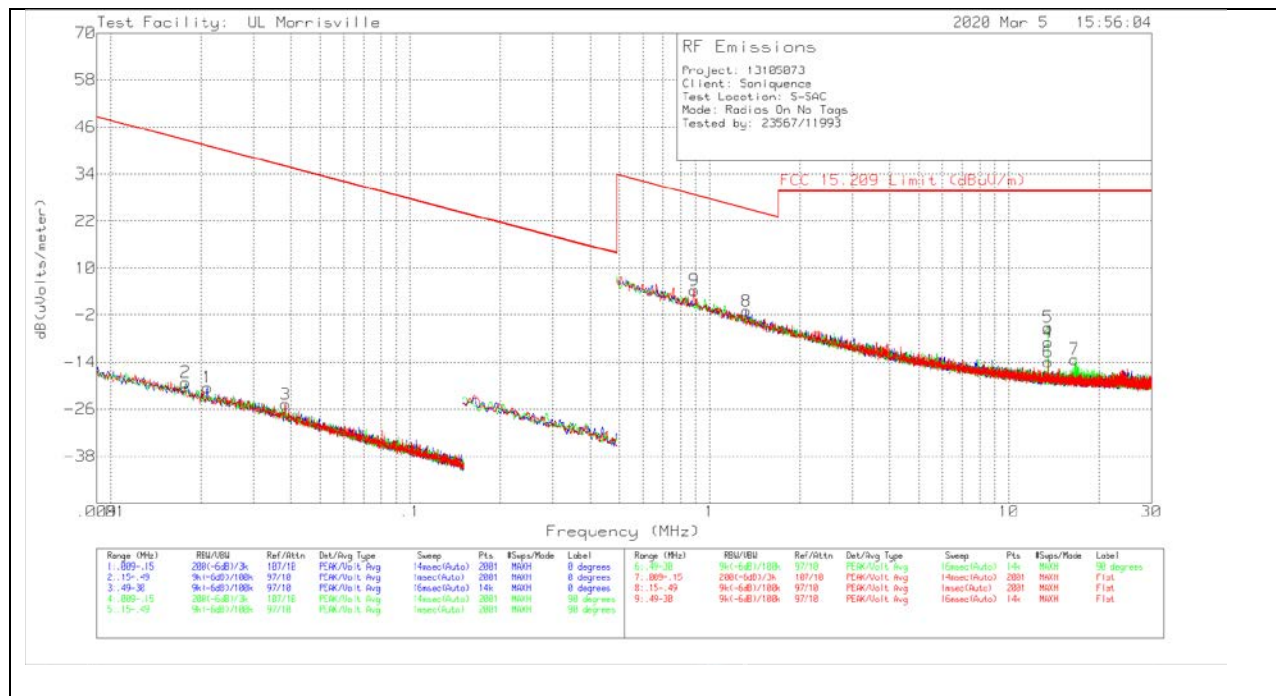


RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0079 AF (dB/m)	Cbl (dB)	Dist. Corr. Factor (dB)	Corrected Reading dB(uVolts/meter)	FCC 15.209 QP/AV Limit (dBuV/m)	FCC 15.209 PK Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)
2	.0178	45.86	Pk	14.9	.1	-80	-19.14	42.59	62.59	-61.73	0-360
1	.02107	45.54	Pk	13.9	.1	-80	-20.46	41.13	61.13	-61.59	0-360
3	.03832	42.59	Pk	12.5	.1	-80	-24.81	35.94	55.94	-60.75	0-360
9	.89052	33.23	Pk	11	.1	-40	4.33	28.61	-	-24.28	0-360
8	1.32898	27.74	Pk	11.1	.2	-40	-.96	25.13	-	-26.09	0-360
4	13.5596	20.48	Pk	10	.6	-40	-8.92	29.54	-	-38.46	0-360
6	13.5596	15.46	Pk	10	.6	-40	-13.94	29.54	-	-43.48	0-360
5	13.56171	24.3	Pk	10	.6	-40	-5.1	29.54	-	-34.64	0-360
7	16.59301	16.3	Pk	9.7	.7	-40	-13.3	29.54	-	-42.84	0-360


Pk- Peak Detector

SPURIOUS AND HARMONIC EMISSIONS 30MHz to 1000MHz

VERTICAL RESULT

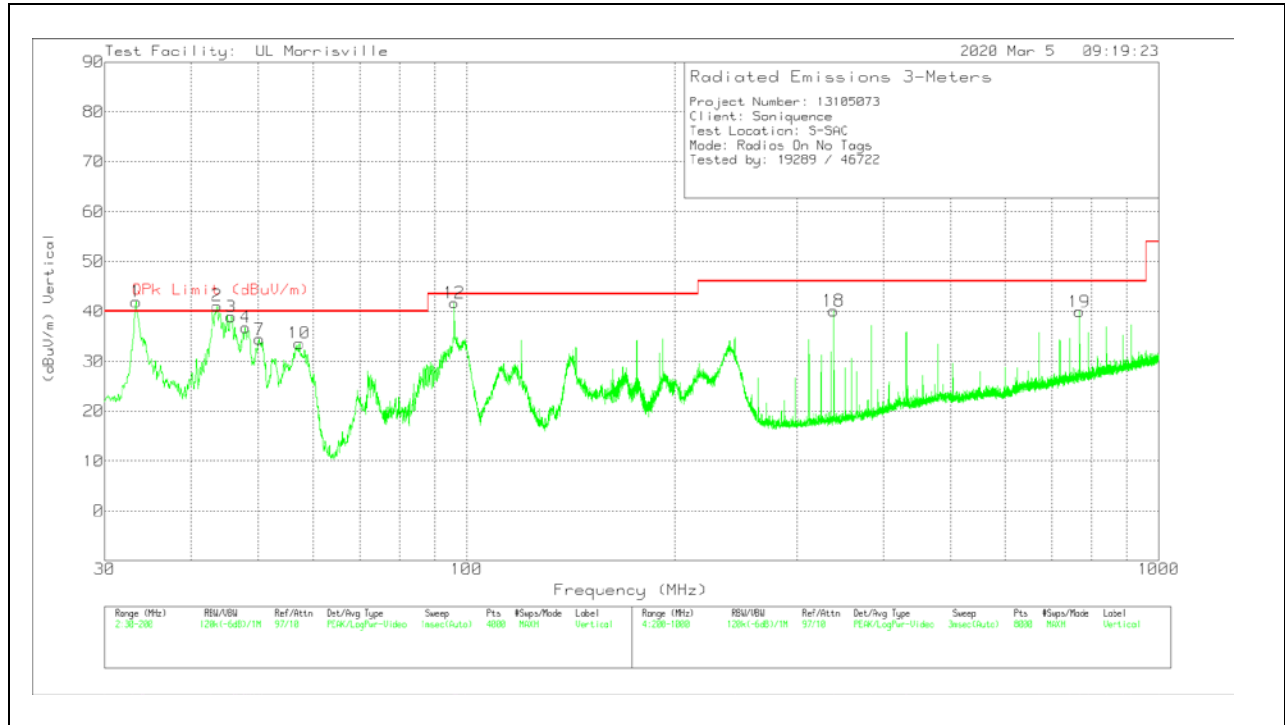

HORIZONTAL RESULT

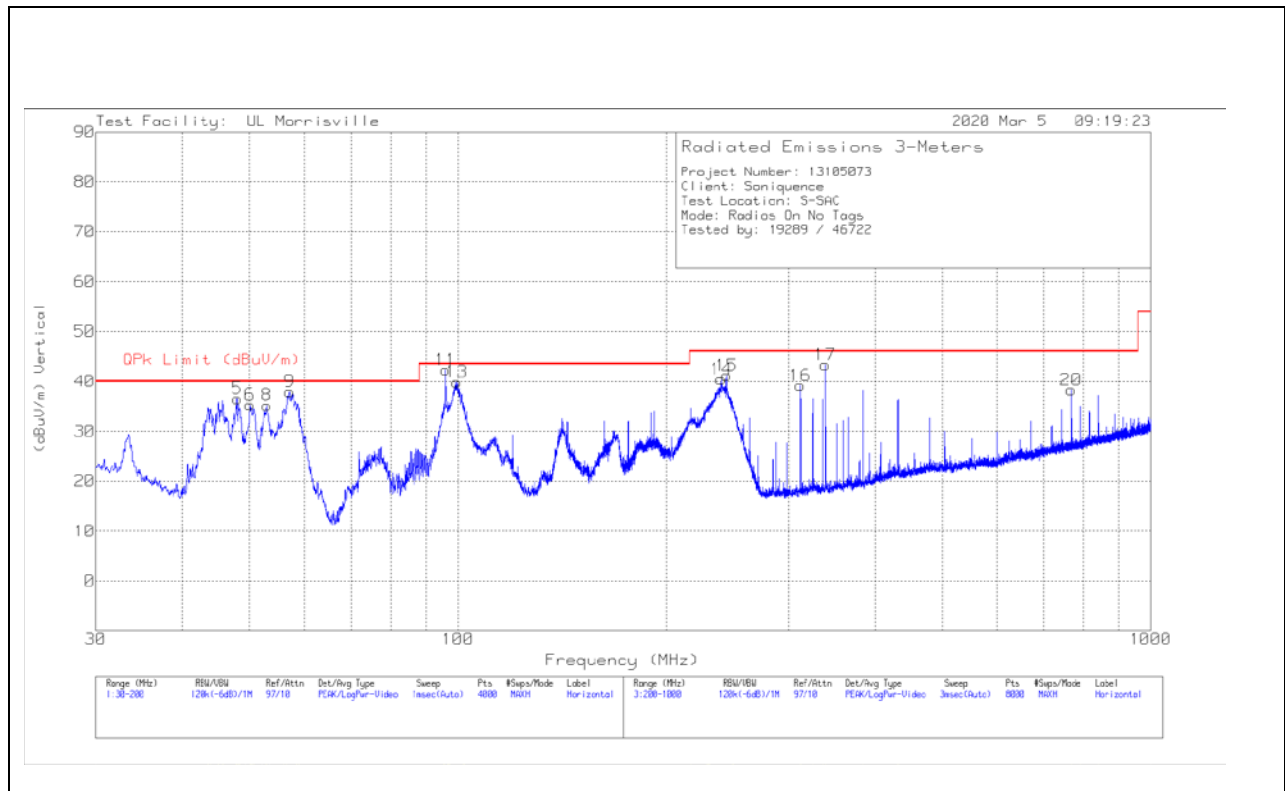


RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0074 AF (dB/m)	Cbl/Amp	Corrected Reading (dBuV/m)	QPk Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)	Height (cm)	Polarity
5	48.0057	49.18	Qp	14.8	-31.5	32.48	40	-7.52	355	393	H
6	50.2277	48.8	Qp	14	-31.5	31.3	40	-8.7	355	392	H
8	52.4625	48.77	Qp	13.6	-31.5	30.87	40	-9.13	351	394	H
9	57.8445	50.32	Qp	13.5	-31.4	32.42	40	-7.58	341	374	H
11	95.9846	56.9	Qp	15.2	-31	41.1	43.52	-2.42	10	311	H
13	99.566	50.53	Qp	16.3	-31	35.83	43.52	-7.69	170	299	H
14	240.0032	51.41	Qp	17.7	-30	39.11	46.02	-6.91	303	126	H
15	244.0757	52.79	Qp	17.7	-29.9	40.59	46.02	-5.43	303	133	H
16	311.9916	47.49	Qp	19.8	-29.5	37.79	46.02	-8.23	225	102	H
17	338.9995	52.55	Qp	20.1	-29.4	43.25	46.02	-2.77	268	102	H
20	768.0064	39.85	Qp	27.1	-28.3	38.65	46.02	-7.37	23	117	H
1	33.4359	41.15	Qp	24.5	-31.7	33.95	40	-6.05	38	144	V
2	43.5855	50.74	Qp	17.2	-31.6	36.34	40	-3.66	137	114	V
3	45.2428	51.25	Qp	16.2	-31.6	35.85	40	-4.15	319	120	V
4	47.9451	49.35	Qp	14.8	-31.5	32.65	40	-7.35	340	106	V
7	50.1942	49.28	Qp	14	-31.5	31.78	40	-8.22	250	105	V
10	57.5821	44.58	Qp	13.5	-31.4	26.68	40	-13.32	232	113	V
12	96.0071	56.43	Qp	15.2	-31	40.63	43.52	-2.89	328	107	V
18	339	50.43	Qp	20.1	-29.4	41.13	46.02	-4.89	252	156	V
19	767.9913	40.17	Qp	27.1	-28.3	38.97	46.02	-7.05	129	103	V

Qp - Quasi-Peak detector

Fundamental 0 Degrees

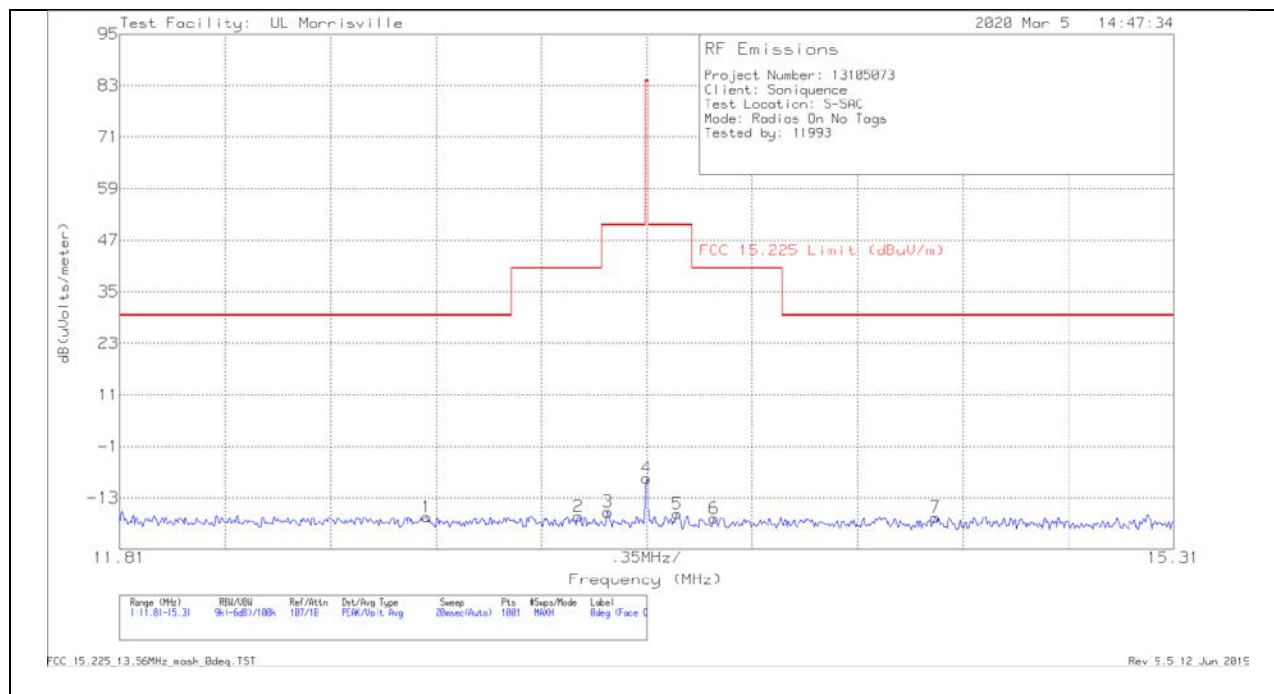


RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0079 AF (dB/m)	Cbl (dB)	Dist. Corr. Factor (dB)	Corrected Reading dB(uVolts/meter)	FCC 15.225 Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)
1	12.8285	12.03	Pk	10	.6	-40	-17.37	29.5	-46.87	68
2	13.3325	12.12	Pk	10	.6	-40	-17.28	40.5	-57.78	68
3	13.4305	13.21	Pk	10	.6	-40	-16.19	50.5	-66.69	68
4	13.56	21.05	Pk	10	.6	-40	-8.35	84	-92.35	68
5	13.6615	12.8	Pk	9.9	.6	-40	-16.7	50.5	-67.2	68
6	13.784	11.81	Pk	9.9	.6	-40	-17.69	40.5	-58.19	68
7	14.519	12.02	Pk	9.9	.6	-40	-17.48	29.5	-46.98	68

Pk - Peak detector

Fundamental 90 Degrees

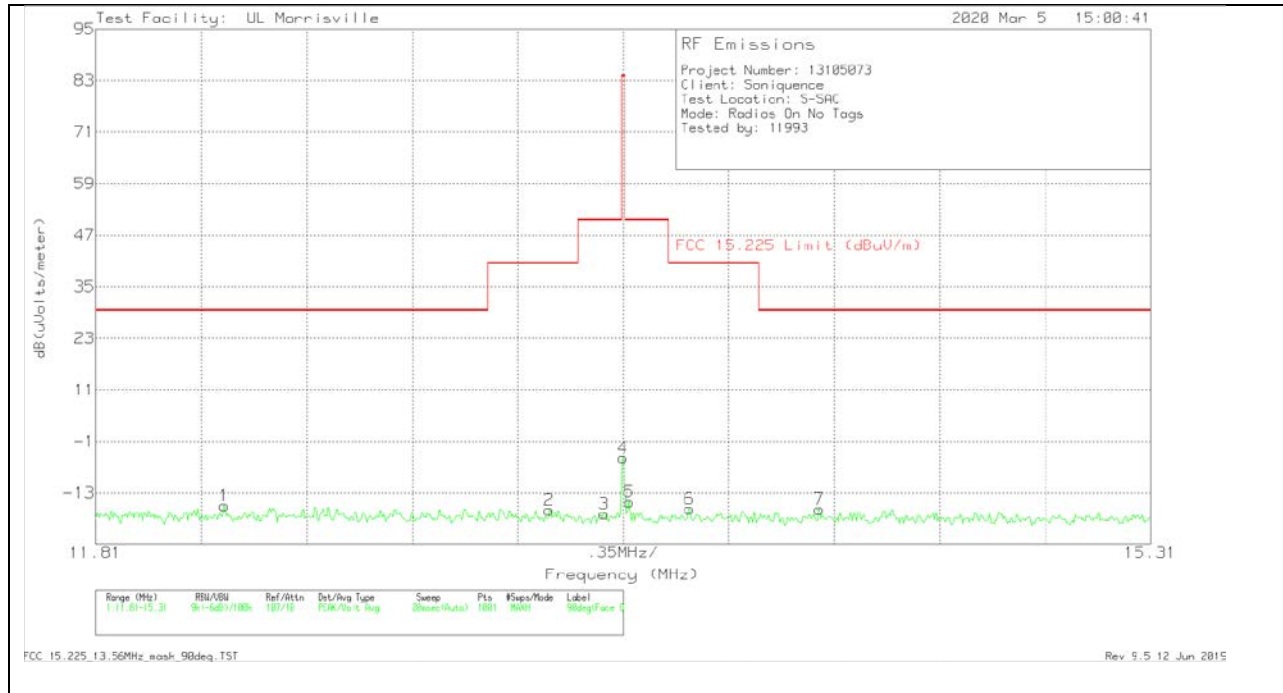


RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0079 AF (dB/m)	Cbl (dB)	Dist. Corr. Factor (dB)	Corrected Reading dB(uVolts/meter)	FCC 15.225 Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)
1	12.237	13.35	Pk	10.1	.6	-40	-15.95	29.5	-45.45	205
2	13.315	12.41	Pk	10	.6	-40	-16.99	40.5	-57.49	205
3	13.497	11.52	Pk	10	.6	-40	-17.88	50.5	-68.38	205
4	13.56	24.59	Pk	10	.6	-40	-4.81	84	-88.81	205
5	13.581	14.35	Pk	10	.6	-40	-15.05	50.5	-65.55	205
6	13.7805	12.8	Pk	9.9	.6	-40	-16.7	40.5	-57.2	205
7	14.211	12.73	Pk	9.9	.6	-40	-16.77	29.5	-46.27	205

Pk - Peak detector

Fundamental Parallel to GRP

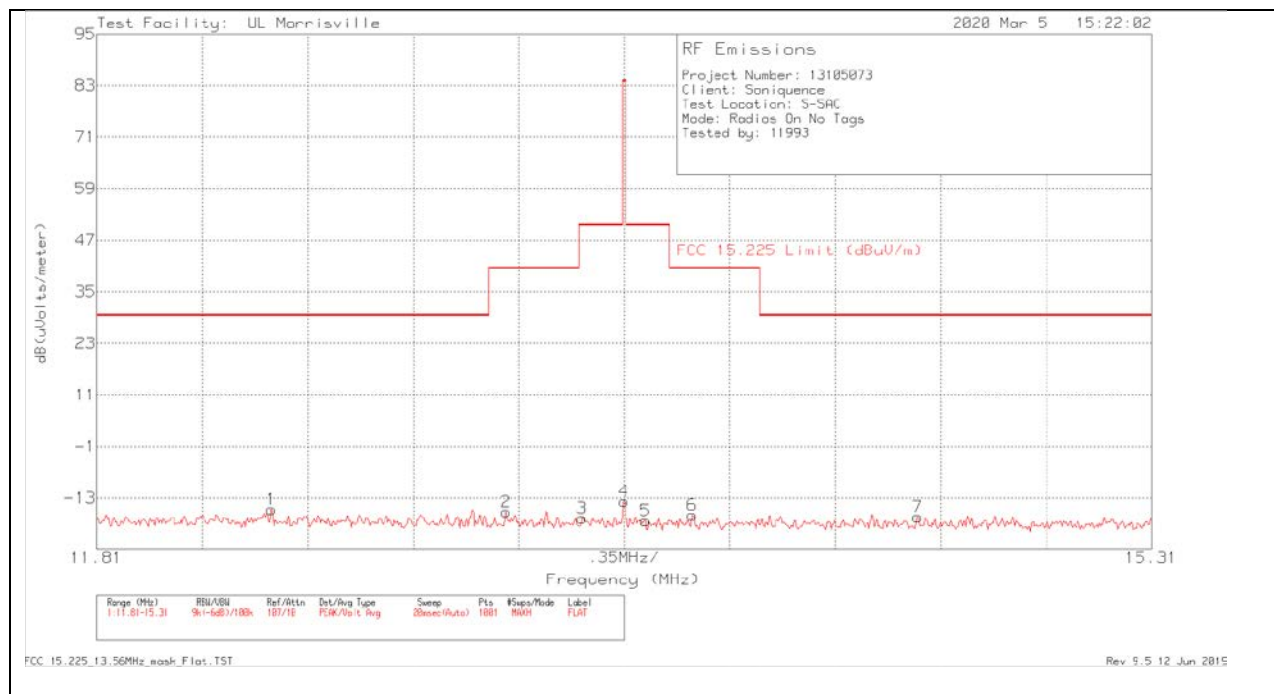

RADIATED EMISSIONS

Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	AT0079 AF (dB/m)	Cbl (dB)	Dist. Corr. Factor (dB)	Corrected Reading dB(uVolts/meter)	FCC 15.225 Limit (dBuV/m)	Margin (dB)	Azimuth (Degs)
1	12.391	13.62	Pk	10.1	.6	-40	-15.68	29.5	-45.18	63
2	13.168	13.16	Pk	10	.6	-40	-16.24	40.5	-56.74	63
3	13.42	11.69	Pk	10	.6	-40	-17.71	50.5	-68.21	63
4	13.56	15.6	Pk	10	.6	-40	-13.8	84	-97.8	63
5	13.63	11.22	Pk	9.9	.6	-40	-18.28	50.5	-68.78	63
6	13.7875	12.57	Pk	9.9	.6	-40	-16.93	40.5	-57.43	63
7	14.533	12.07	Pk	9.9	.6	-40	-17.43	29.5	-46.93	63

Pk - Peak detector

11. AC POWER LINE CONDUCTED EMISSIONS

§15.207

IC RSS-GEN, Section 8.8

(a) Except as shown in paragraphs (b) and (c) of this section, for an intentional radiator that is designed to be connected to the public utility (AC) power line, the radio frequency voltage that is conducted back onto the AC power line on any frequency or frequencies, within the band 150 kHz to 30 MHz, shall not exceed the limits in the following table, as measured using a 50 μ H/50 ohms line impedance stabilization network (LISN). Compliance with the provisions of this paragraph shall be based on the measurement of the radio frequency voltage between each power line and ground at the power terminal. The lower limit applies at the band edges.

Frequency range (MHz)	Limits (dB μ V)	
	Quasi-peak	Average
0.15 to 0.50	66 to 56	56 to 46
0.50 to 5	56	46
5 to 30	60	50
Notes: 1. The lower limit shall apply at the transition frequencies 2. The limit decreases linearly with the logarithm of the frequency in the range 0.15 MHz to 0.50 MHz.		

TEST PROCEDURE


ANSI C63.10:2013 and KDB 174176 D01 Line Conducted FAQ v01r01, Q5.

RESULTS

11.1. RFID

11.1.1. NORMAL OPERATION

LINE 1 RESULTS

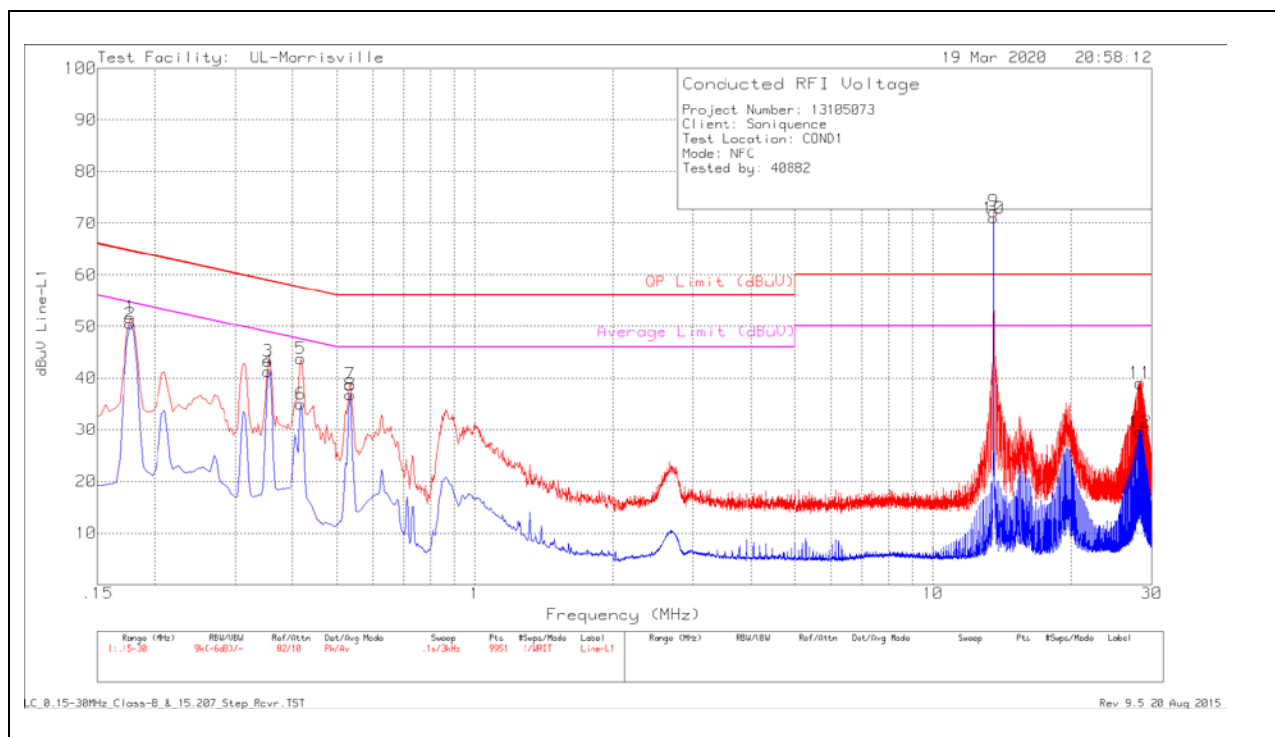

Range 1: Line-L1 .15 - 30MHz										
Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	LISN VCF (dB)	Cbl/Limiter (dB)	Corrected Reading dBuV	QP Limit (dBuV)	Margin (dB)	Average Limit (dBuV)	Margin (dB)
1	.177	41.61	Pk	.2	10	51.81	64.63	-12.82	-	-
2	.177	39.07	Av	.2	10	49.27	-	-	54.63	-5.36
3	.354	33.2	Pk	.1	10	43.3	58.87	-15.57	-	-
4	.354	31.2	Av	.1	10	41.3	-	-	48.87	-7.57
5	.417	33.68	Pk	.1	10	43.78	57.51	-13.73	-	-
6	.417	24.87	Av	.1	10	34.97	-	-	47.51	-12.54
7	.534	28.7	Pk	.1	10	38.8	56	-17.2	-	-
8	.534	26.69	Av	.1	10	36.79	-	-	46	-9.21
9	13.56	61.29	Qp	.1	10.4	71.79	60	11.79	-	-
10	13.56	60.68	Av	.1	10.4	71.18	-	-	50	21.18
11	28.359	28.04	Pk	.3	10.7	39.04	60	-20.96	-	-
12	28.359	18.57	Av	.3	10.7	29.57	-	-	50	-20.43


Note – Markers 9 and 10 are the fundamental. Refer to following terminated plots.

Pk - Peak detector

Qp - Quasi-Peak detector

Av - Average detection

LINE 2 RESULTS

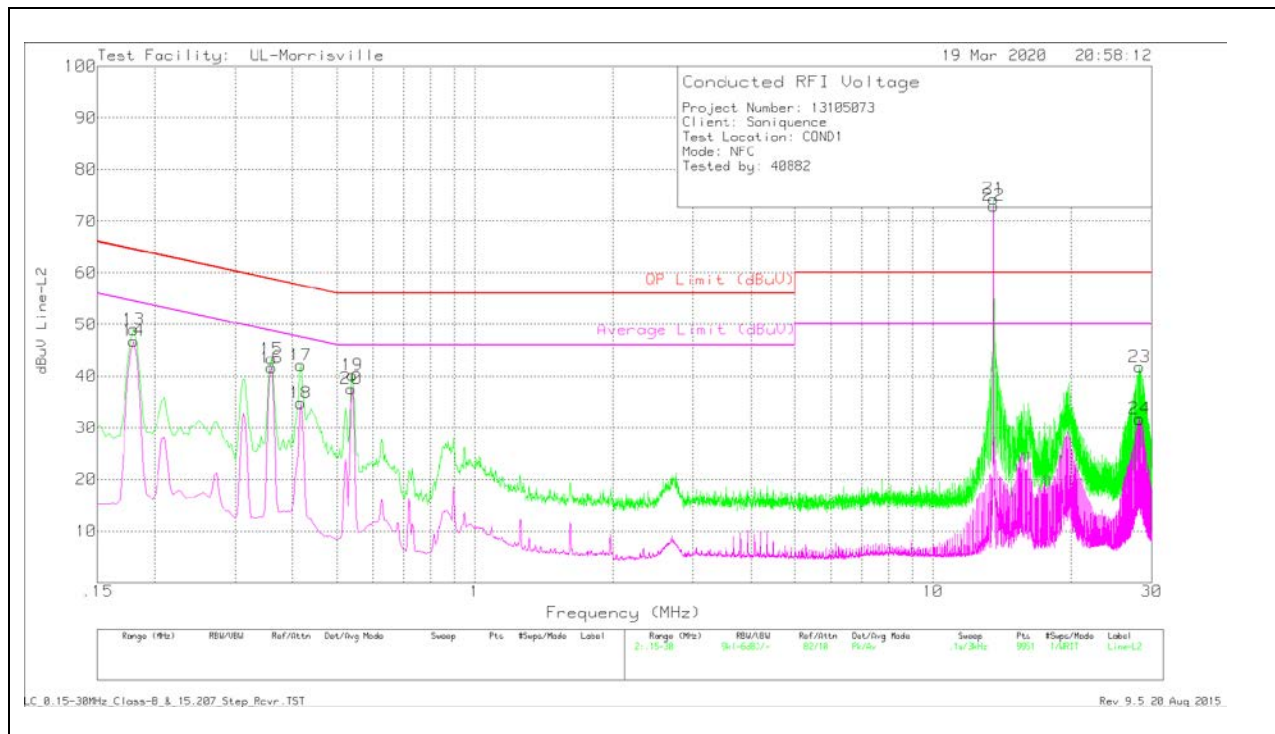


Range 2: Line-L2 .15 - 30MHz										
Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	LISN VCF (dB)	Cbl/Limiter (dB)	Corrected Reading dBuV	QP Limit (dBuV)	Margin (dB)	Average Limit (dBuV)	Margin (dB)
13	.18	38.83	Pk	.2	10	49.03	64.49	-15.46	-	-
14	.18	36.62	Av	.2	10	46.82	-	-	54.49	-7.67
15	.36	33.22	Pk	.1	10	43.32	58.73	-15.41	-	-
16	.36	31.55	Av	.1	10	41.65	-	-	48.73	-7.08
17	.417	31.99	Pk	.1	10	42.09	57.51	-15.42	-	-
18	.417	24.68	Av	.1	10	34.78	-	-	47.51	-12.73
19	.54	30.15	Pk	0	10	40.15	56	-15.85	-	-
20	.537	27.56	Av	0	10	37.56	-	-	46	-8.44
21	13.56	62.72	Qp	.1	10.4	73.22	60	13.22	-	-
22	13.56	62.04	Av	.1	10.4	72.54	-	-	50	22.54
23	28.251	30.78	Pk	.3	10.7	41.78	60	-18.22	-	-
24	28.251	20.74	Av	.3	10.7	31.74	-	-	50	-18.26

Note – Markers 21 and 22 are the fundamental. Refer to following terminated plots.

Pk - Peak detector
Qp - Quasi-Peak detector
Av - Average detection

11.1.2. ANTENNAS TERMINATED


LINE 1 RESULTS

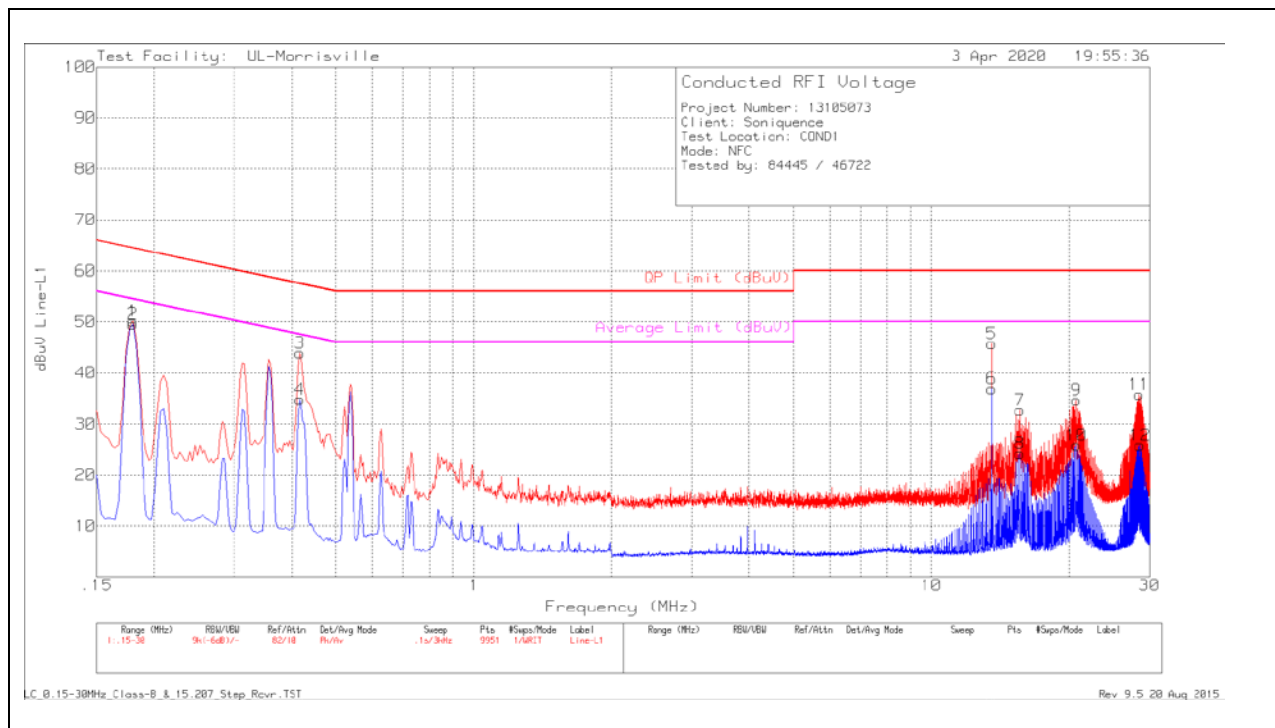

Range 1: Line-L1 .15 - 30MHz										
Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	LISN VCF (dB)	Cbl/Limiter (dB)	Corrected Reading (dBuV)	QP Limit (dBuV)	Margin (dB)	Average Limit (dBuV)	Margin (dB)
1	.18	40.26	Pk	.2	9.7	50.16	64.49	-14.33	-	-
2	.17939	40.22	Ca	.2	9.7	50.12	-	-	54.51	-4.39
3	.417	34.11	Pk	.1	9.7	43.91	57.51	-13.6	-	-
4	.417	25.01	Av	.1	9.7	34.81	-	-	47.51	-12.7
5	13.56	35.61	Pk	.1	10	45.71	60	-14.29	-	-
6	13.56	26.84	Av	.1	10	36.94	-	-	50	-13.06
7	15.624	22.49	Pk	.1	10.1	32.69	60	-27.31	-	-
8	15.627	14	Av	.1	10.1	24.2	-	-	50	-25.8
9	20.754	24.35	Pk	.2	10.1	34.65	60	-25.35	-	-
10	20.754	15.54	Av	.2	10.1	25.84	-	-	50	-24.16
11	28.467	25.3	Pk	.3	10.2	35.8	60	-24.2	-	-
12	28.572	15.33	Av	.3	10.2	25.83	-	-	50	-24.17

Pk - Peak detector
Ca - CISPR average detection
Av - Average detection

LINE 2 RESULTS

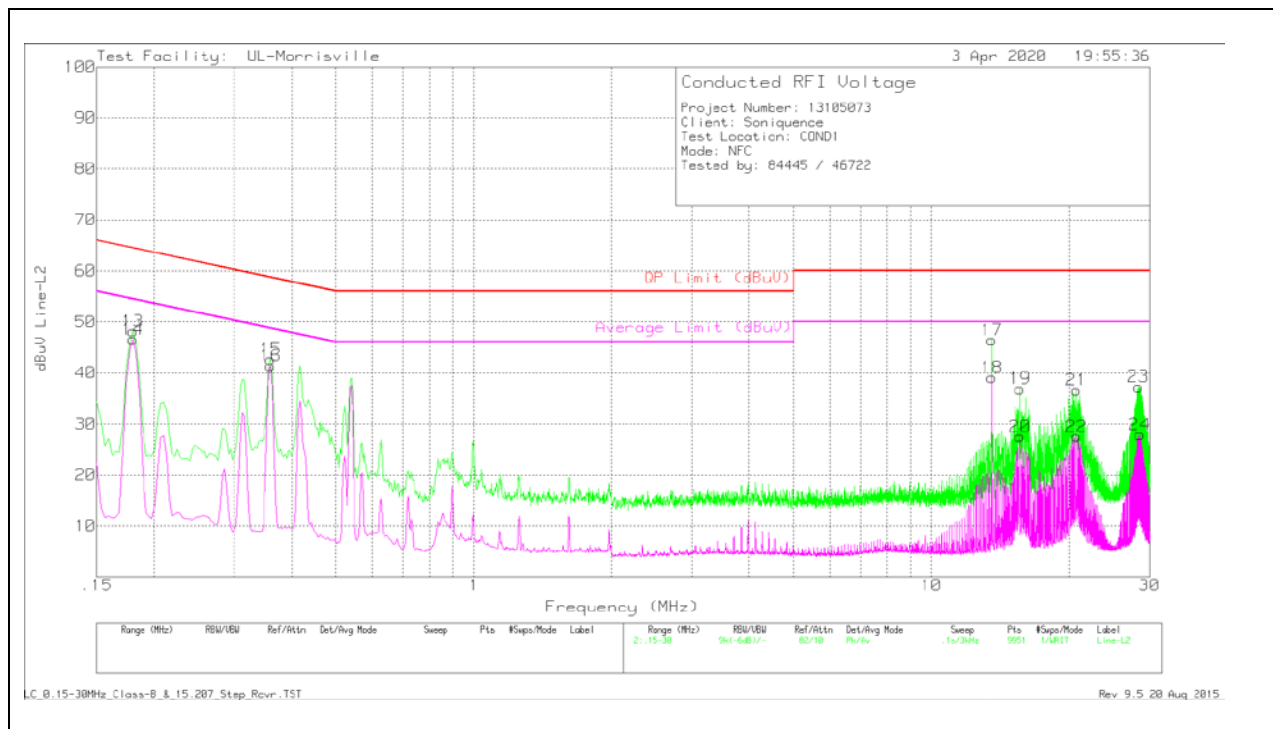

Range 2: Line-L2 .15 - 30MHz										
Marker	Frequency (MHz)	Meter Reading (dBuV)	Det	LISN VCF (dB)	Cbl/Limiter (dB)	Corrected Reading dBuV	QP Limit (dBuV)	Margin (dB)	Average Limit (dBuV)	Margin (dB)
13	.18	38.29	Pk	.2	9.7	48.19	64.49	-16.3	-	-
14	.18	36.73	Av	.2	9.7	46.63	-	-	54.49	-7.86
15	.36	32.88	Pk	.1	9.7	42.68	58.73	-16.05	-	-
16	.36	31.62	Av	.1	9.7	41.42	-	-	48.73	-7.31
17	13.56	36.35	Pk	.1	10	46.45	60	-13.55	-	-
18	13.56	29	Av	.1	10	39.1	-	-	50	-10.9
19	15.639	26.74	Pk	.1	10.1	36.94	60	-23.06	-	-
20	15.639	17.38	Av	.1	10.1	27.58	-	-	50	-22.42
21	20.748	26.38	Pk	.2	10.1	36.68	60	-23.32	-	-
22	20.754	17.22	Av	.2	10.1	27.52	-	-	50	-22.48
23	28.359	26.81	Pk	.3	10.2	37.31	60	-22.69	-	-
24	28.566	17.41	Av	.3	10.2	27.91	-	-	50	-22.09

Pk - Peak detector
Qp - Quasi-Peak detector
Av - Average detection

12. SETUP PHOTOS

Please refer to R13105073-EP1 for setup photos.

END OF TEST REPORT