

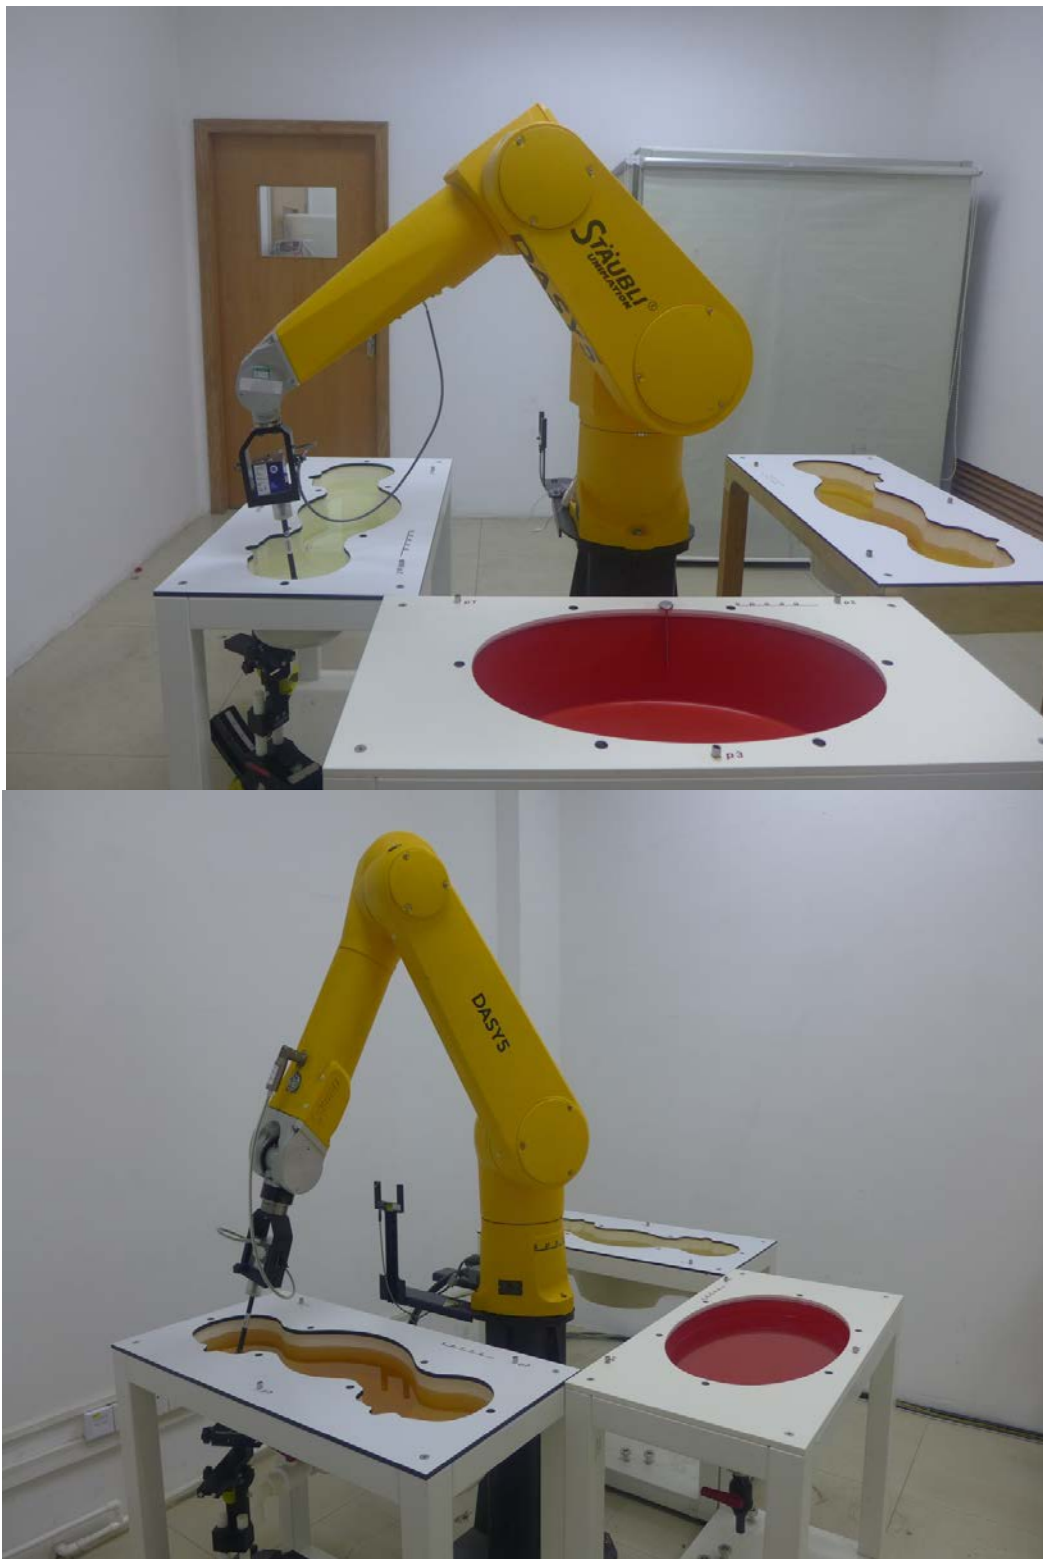


Appendix D

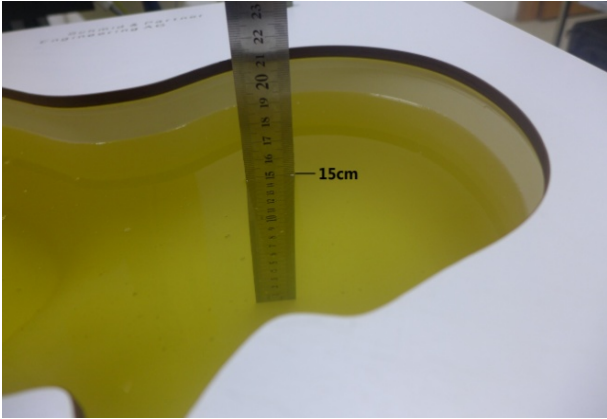
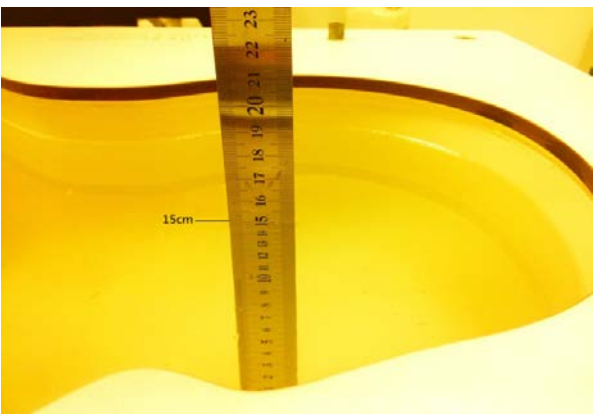
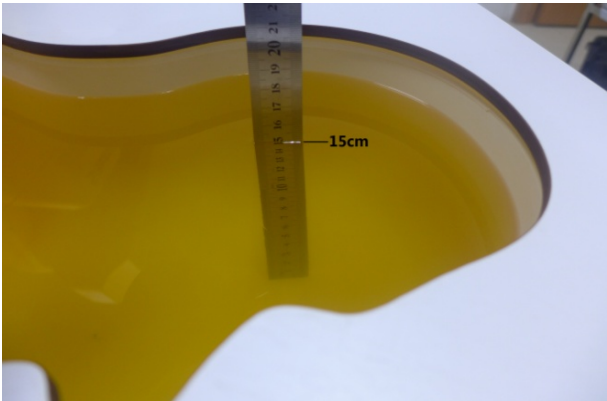
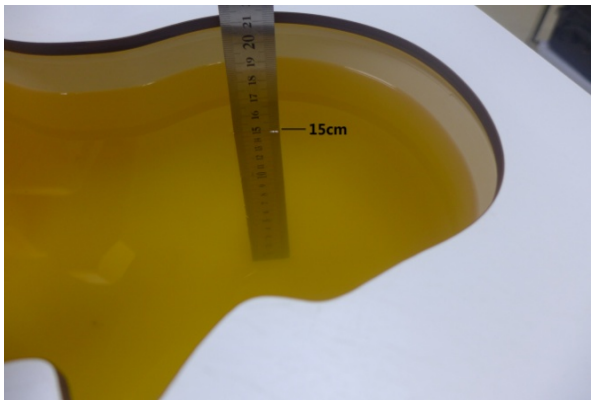
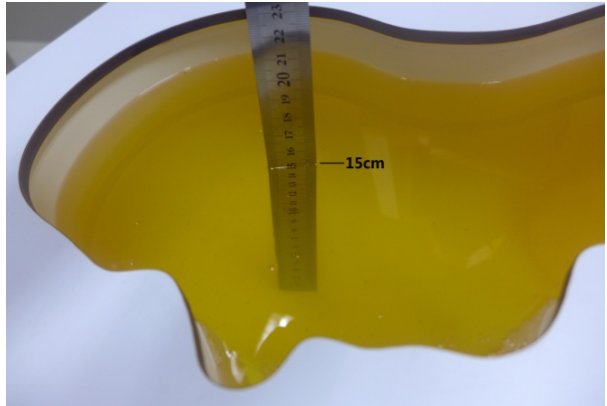
Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 750	Photo 2: Tissue Simulant Liquid for Head 835
	
Photo 3: Tissue Simulant Liquid for Head 1750	Photo 4: Tissue Simulant Liquid for Head 1900
	
Photo 5: Tissue Simulant Liquid for Head 2450	NA
	NA

3. Photographs of EUT test position

Photo 6: Front side 15mm	Photo 7: Back side 15mm
	
Photo 8: Front side 10mm	Photo 9: Back side 10mm
	
Photo 10: Left side 10mm	Photo 11: Right side 10mm
	



Photo 12: Top side 10mm	Photo 13: Bottom side 10mm
 A photograph showing the top side of a white, rectangular electronic device. The device is mounted on a black, adjustable stand. The device has a large, dark screen and a small, circular camera lens at the top. The background is a plain, light-colored wall.	 A photograph showing the bottom side of the same white, rectangular electronic device. The device is mounted on the same black stand. The bottom side features a small, circular camera lens and a small, rectangular port. The background is a plain, light-colored wall.

4. EUT Constructional Details

Photo 14: Front View	Photo 15: Back View
	