

Annex 3: External photographs 19-1-0137401T05a-C01-A3

Number of pages:	6	Date of Report:	2021-Jun-09
Testing company:	CETECOM GmbH Im Teelbruch 116 45219 Essen Germany Tel. + 49 (0) 20 54 / 95 19-0 Fax: + 49 (0) 20 54 / 95 19-150	Applicant:	Bosch Healthcare Solutions GmbH
Test Object / Tested Device(s):	System for quantitative measurement of fractional nitric oxide (FeNO) in human breath, Vivatmo pro (Base Station)		
FCC ID:	2AVQ9VMPBS1	IC:	25928-VMPBS1
Testing has been carried out in accordance with:	Title 47 CFR, Chapter I FCC Regulations, Subchapter A Subpart C: §15.247 (DTS) RSS-247, Issue 2 (DTS) RSS-Gen., Issue 5		



Table of Contents

1 External photographs of Main device under test (EUT/DUT)3

2 External photographs of Accessories.....5


1 External photographs of Main device under test (EUT/DUT)




Photograph 1: EUT 1_Top view



Photograph 2: EUT 1_under side view

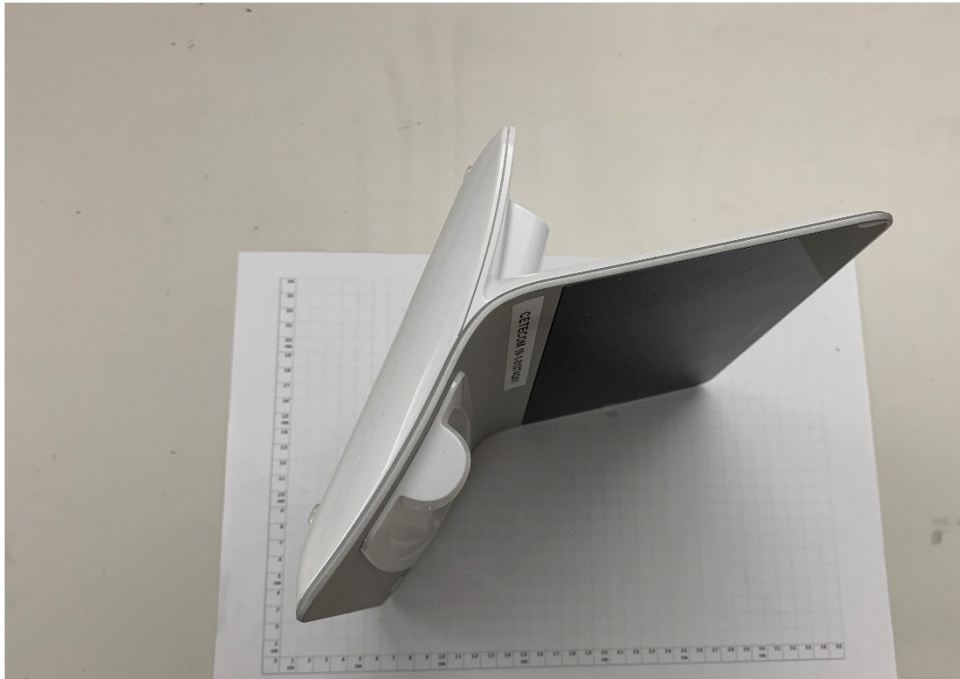

Photograph 3: EUT 1_Left side view

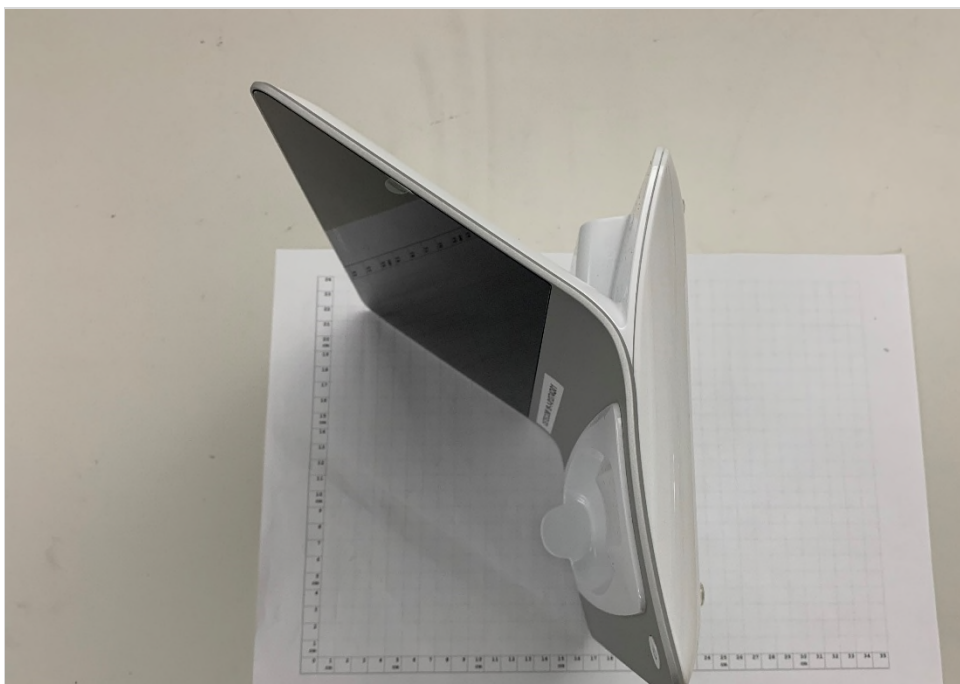

Photograph 4: EUT 1_Right side view


2 External photographs of Accessories



Photograph 1: Power Supply Vivatmo pro (AE1)



Photograph 2: AE4 and AE 5

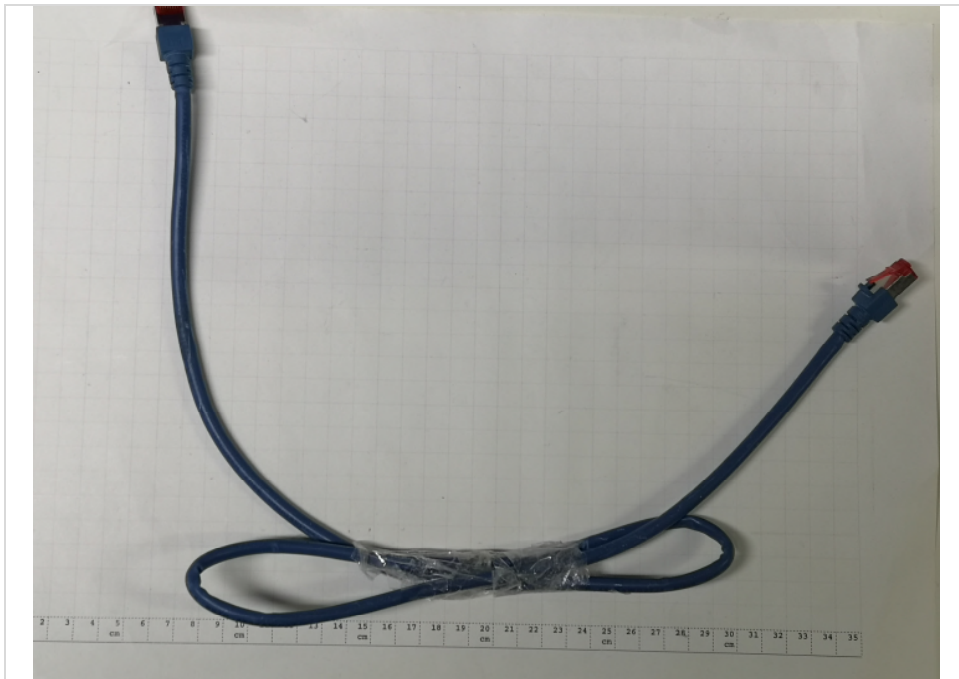

Photograph 3: AE 2

End Of Annex 3