

Annex 3: Test setup photographs to Test Report 19-1-0137401T01a-C01-A3



Number of pages:	5	Date of Report:	2021-Mai-03
Testing company:	CETECOM GmbH Im Teelbruch 116 45219 Essen Germany Tel. + 49 (0) 20 54 / 95 19-0 Fax: + 49 (0) 20 54 / 95 19-150	Applicant:	Bosch Healthcare Solutions GmbH
Test Object / Tested Device(s):	Vivatmo pro (Handheld), System for quantitative measurement of fractional nitric oxide (FeNO) in human breath		
Listing FCC ID:	2AVQ9VMPHH1	ISED:	25928-VMPPHH1
Testing has been carried out in accordance with:	Title 47 CFR, Chapter I FCC Regulations, Subchapter A §15.247 (DTS) ISED-Regulations RSS-Gen, Issue 5 RSS-210, Issue 10		


Table of contents

1	Test setup photographs	3
1.1	Measurements of magnetic fields in range 9 kHz to 30 MHz	3
1.2	Measurements of electric fields in range 30 MHz to 1GHz	4
1.3	Measurements of electric fields in range 1GHz to 18GHz.....	5

1 Test setup photographs

1.1 Measurements of magnetic fields in range 9 kHz to 30 MHz

Photograph 1: EUT Test Setup in the semi anechoic chamber, overall view

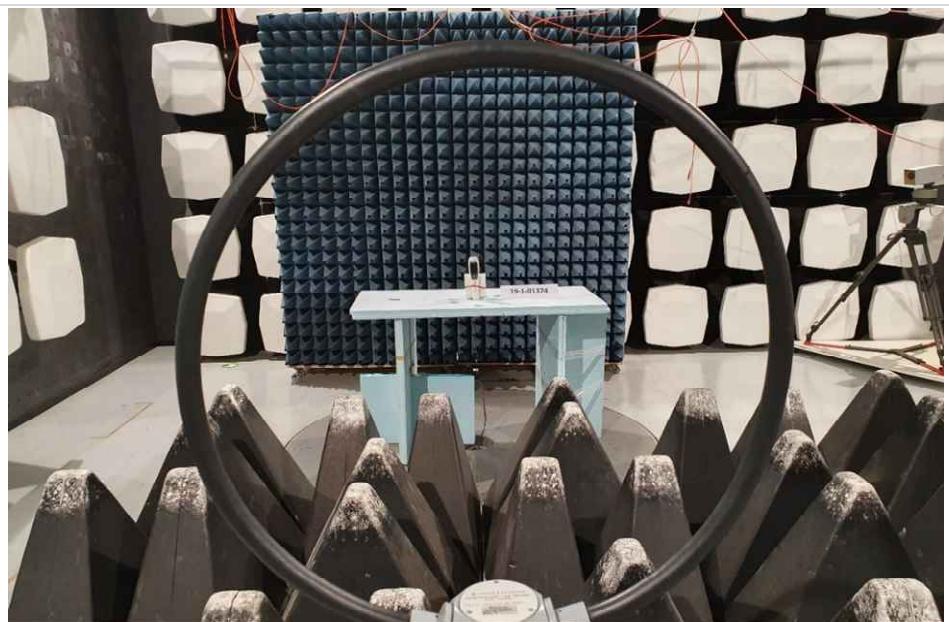

Photograph 2: EUT Test Setup in the semi anechoic chamber, close-up view



1.2 Measurements of electric fields in range 30 MHz to 1GHz

Photograph 3: EUT Test Setup in the semi anechoic chamber, overall view



Photograph 4: EUT Test Setup in the semi anechoic chamber, close-up view



1.3 Measurements of electric fields in range 1GHz to 18GHz

Photograph 5: EUT Test Setup in the fully anechoic chamber, overall view



Photograph 6: EUT Test Setup in the fully anechoic chamber, close-up view



End Of Annex 3