


# Owandy-RX DC

FCC ID: 2AVTNWDC0

## Device External Photos - overview

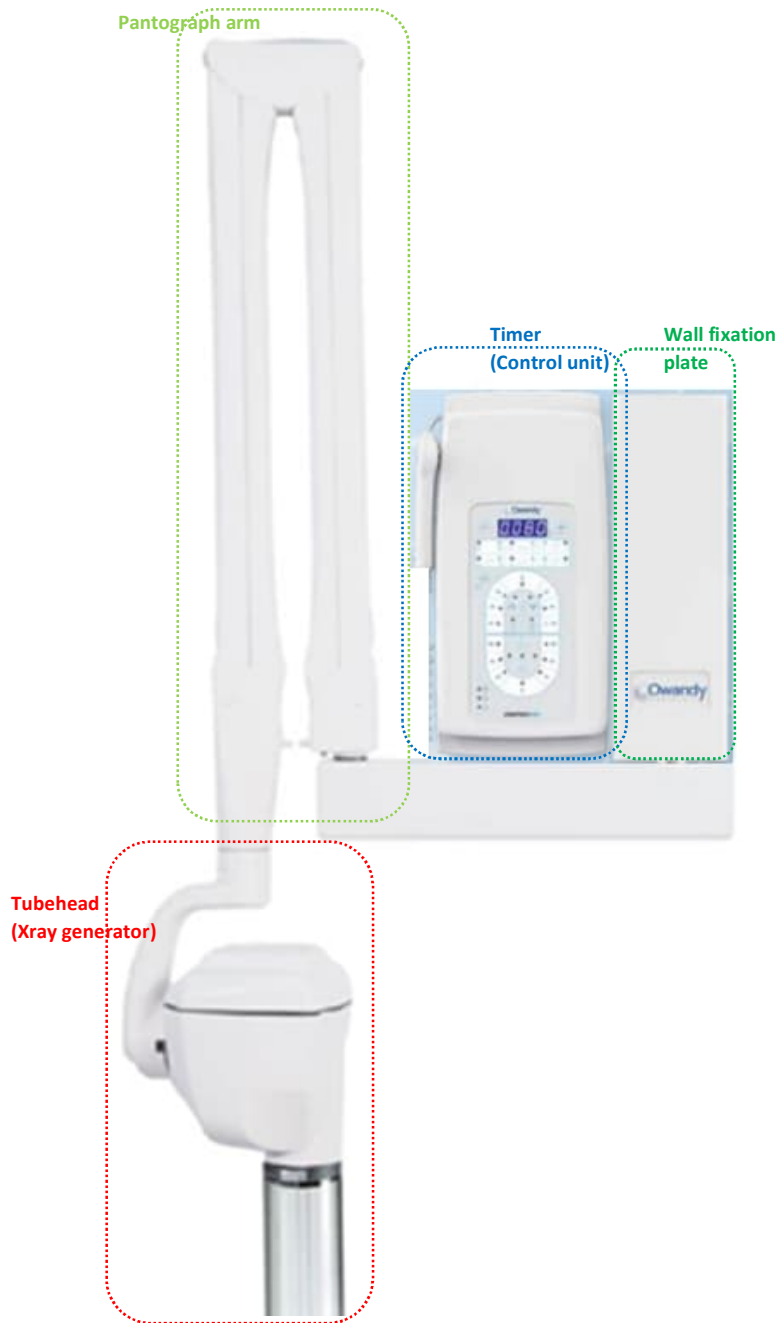

# Owandy-RX DC

FCC ID: 2AVTNWDC0

**Device External Photos – mains supply port (unique port present)**

The mains supply cable is not supplied with the medical device; in the picture below is only representative to show the port




# Owandy-RX DC

FCC ID: 2AVTNWDC0

Device External Photos – timer (control unit) and wall plate fixation details



FRONT Timer

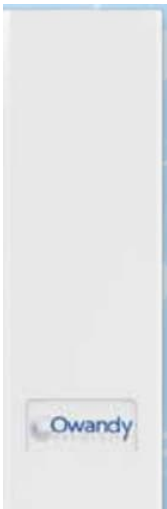

Wall fixation



BACK Timer



Wall fixation

# Owandy-RX DC

**FCC ID: 2AVTNWDC0**

**Device External Photos – tubehead (Xray generator) details**



# Owandy-RX DC

FCC ID: 2AVTNWDC0

Device External Photos – pantograph arm details



FRONT



TOP



BOTTOM

# Owandy-RX DC



BACK