



Canada

RF Test Report

As per

RSS-210 Annex B.6, Issue 10:2019

&

FCC Part 15 Subpart 15.225:2019

Low Power Licence Exempt Radio
Communication Devices
Intentional Radiators

on the

OmniCure S2000 Elite

Issued by:

TÜV SÜD Canada Inc.
11 Gordon Collins Dr,
Gormley, ON, L0H 1G0
Canada
Ph: (905) 883-7255

Testing produced for

EXCELITAS
TECHNOLOGIES®

Excelitas Canada Inc

See Appendix A for full client &
EUT details.

Prepared by:

Raymond Lee Au,
Project Engineer

Raymond Lee Au

Reviewed by:

Amir Emami,
Project Engineer

Amir Emami

 Innovation, Science and
Economic Development Canada

Registration #
6844A-3



Testing Laboratory
Certificate #2955.02



R-4023, G-506
C-4498, T-1246



Registration #
CA6844

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Table of Contents

Table of Contents	2
Report Scope.....	3
Summary	5
Test Results Summary	6
Notes, Justifications, or Deviations	7
Sample Calculation(s)	8
Applicable Standards, Specifications and Methods.....	9
Document Revision Status	10
Definitions and Acronyms	11
Testing Facility	12
Calibrations and Accreditations.....	12
Testing Environmental Conditions and Dates	13
Detailed Test Results Section	14
Radiated Emission Field Strength.....	15
Transmitter Spurious Radiated Emissions	26
Carrier Frequency Stability.....	37
Power Line Conducted Emissions	39
20dB and 99% Occupied Bandwidth	45
Appendix A – EUT Summary.....	49

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Report Scope

This report addresses the EMC verification testing and test results of the **OmniCure S2000 Elite** unit from **Excelitas Canada Inc.** This unit is herein referred to as EUT (Equipment Under Test). The EUT was tested for compliance against the following standards:

RSS-210 Annex B.6, Issue 10:2019,
FCC Part 15 Subpart C 15.225:2019

Test procedures, results, justifications, and engineering considerations, if any, follow later in this report.

This report does not imply product endorsement by any government, accreditation agency, or TÜV SÜD Canada Inc.

Opinions or interpretations expressed in this report, if any, are outside the scope of TÜV SÜD Canada Inc accreditations. Any opinions expressed do not necessarily reflect the opinions of TÜV SÜD Canada Inc, unless otherwise stated.

The tested sample is the OmniCure **S2000 Elite**. As per the client/manufacturer, this test report is also applicable to other similar models in the product family, the **S1500 Pro**, and the **S2000 Pro**. The tested sample is the most populated model in the product family, and the features of the other models are subsets of the tested unit. The following shows their differences:

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Model Variants' Differences

As provided by the client/manufacturer

The tested sample is the **S2000 Elite**



Beta Spec minus:

- No Shutter
- No Radiometer
- No CLF
- Limited PLC/StepCure
- Reduced Output

Beta Spec minus:

- No Shutter

Full Beta Spec

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Summary

The results contained in this report relate only to the item(s) tested.

EUT Model:	S2000 ELITE
EUT FCC Certification #, FCC ID:	2AXSI-SSERIES
ISED Certification #, IC:	26590-SSERIES
EUT passed all tests performed	Yes
Tests conducted by	Raymond Lee Au

For testing dates, see "Testing Environmental Conditions and Dates".

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Test Results Summary

Standard/Method	Description	Class/Limit	Result
FCC 15.203	Antenna Requirement	Unique	Pass ^a
FCC 15.225 (a), (b), (c) RSS-210 B.6 a. i, ii, iii.	Operation within the band 13.110-14.010 MHz (Field Strength)	Quasi-Peak Average	Pass
FCC 15.225 (d) FCC 15.209 RSS-210 B.6 a. iv RSS-GEN (Tables 5 & 6)	Transmitter Spurious Radiated Emissions	Quasi-Peak Average	Pass
FCC 15.225 (e) RSS-210 B.6 b. RSS-Gen 6.11	Operation within the band 13.110-14.010 MHz (Frequency Stability at Extreme Temperatures)	$\pm 0.01\%$ -20°C – +50°C	Pass
FCC 15.225 (e) RSS-210 B.6 b. RSS-Gen 6.11	Operation within the band 13.110-14.010 MHz (Frequency Stability at Extreme Voltages)	$\pm 0.01\%$ 85% – 115%	Pass
FCC 15.205 RSS-GEN (Table 7)	Restricted Bands for Intentional Operation	QuasiPeak Average	Pass ^a
FCC 15.207 RSS-GEN (Table 4)	Power Line Conducted Emissions	QuasiPeak Average	Pass
Overall Result			Pass

^a See Notes, Justifications, or Deviations section for more details.

If the product as tested or otherwise complies with the specification, the EUT is deemed to comply with the requirement and is deemed a 'PASS' grade. If not 'FAIL' grade will be issued. Note that 'PASS' / 'FAIL' grade is independent of any measurement uncertainties.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Notes, Justifications, or Deviations

The following notes, justifications for tests not performed or deviations from the above listed specifications apply:

The EUT is a spot UV curing system for precision adhesive curing with an integrated 13.56 MHz NFC card reader/writer.

For the antenna requirement specified in FCC 15.203, the NFC loop antenna is printed on the PCB which is sealed within the unit's enclosure. It is not meant to be replicable by the user, nor is it accessible.

The EUT is rated to be operated between 15°C – 40°C. However, the 13.56 MHz transmission is tested between -20°C to +50°C.

For the Restricted Bands of operation, the EUT is designed to only operate between 13.110-14.010 MHz.

The EUT's output is set to transmit continuously at 100% duty cycle at the maximum output power.

See separate RF Exposure Exhibit for this unit regarding the permissible RF exposure levels.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Sample Calculation(s)

Radiated Emission Test

E-Field Level = Received Signal + Antenna Factor + Cable Loss – Pre-Amp Gain

E-Field Level = $50\text{dB}\mu\text{V} + 10\text{dB/m} + 2\text{dB} - 20\text{dB}$

E-Field Level = $42\text{dB}\mu\text{V/m}$

Margin = Limit – E-Field Level

Margin = $50\text{dB}\mu\text{V/m} - 42\text{dB}\mu\text{V/m}$

Margin = 8.0 dB (pass)

Power Line Conducted Emission Test

E-Field Level = Received Signal + Attenuation Factor + Cable Loss + LISN Factor

E-Field Level = $50\text{dB}\mu\text{V} + 10\text{dB} + 2.5\text{dB} + 0.5\text{dB}$

E-Field Level = $63\text{dB}\mu\text{V}$

Margin = Limit – E-Field Level

Margin = $73\text{dB}\mu\text{V} - 63\text{dB}\mu\text{V}$

Margin = 10.0 dB (pass)

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Applicable Standards, Specifications and Methods

ANSI C63.4:2014 Methods of Measurement of Radio-Noise Emissions from Low-Voltage Electrical and Electronic Equipment in the Range of 9 kHz to 40 GHz

ANSI C63.10:2013 American National Standard For Testing Unlicensed Wireless Devices

CFR 47 FCC 15 Subpart C:2019 Code of Federal Regulations – Radio Frequency Devices, Intentional Radiators

RSS-Gen Issue 5 2019 General Requirements and Information for the Certification of Radio Apparatus

RSS 210:2019 Issue 10: Licence-Exempt Radio Apparatus: Category I Equipment

ISO 17025:2017 General Requirements for the Competence of Testing and Calibration Laboratories

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Document Revision Status

Revision 000

January 18, 2021

- Initial Release

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Definitions and Acronyms

The following definitions and acronyms are applicable in this report.
See also ANSI C63.14.

AE – Auxiliary Equipment. A digital accessory that feeds data into or receives data from another device (host) that in turn, controls its operation.

BW – Bandwidth. Unless otherwise stated, this is refers to the 6 dB bandwidth.

EMC – Electro-Magnetic Compatibility. The ability of an equipment or system to function satisfactorily in its electromagnetic environment without introducing intolerable electromagnetic disturbances to anything in that environment.

EMI – Electro-Magnetic Immunity. The ability to maintain a specified performance when the equipment is subjected to disturbance (unwanted) signals of specified levels.

EUT – Equipment Under Test. A device or system being evaluated for compliance that is representative of a product to be marketed.

ITE – Information Technology Equipment with a primary function(s) of entry, storage, display, retrieval, transmission, processing, switching, or control, of data.

LISN – Line Impedance Stabilization Network

NCR – No Calibration Required

RF – Radio Frequency

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Testing Facility

Testing for EMC on the EUT was carried out at TÜV SÜD Canada testing lab near Toronto, Ontario. The testing lab has calibrated 3m semi-anechoic chambers which allow measurements on a EUT that has a maximum width or length of up to 2m and a height of up to 3m. The testing lab also has a calibrated 10m Open Area Test Site (OATS). The chambers are equipped with a turntable that is capable of testing devices up to 5000lb in weight and are equipped with a mast that controls the polarization and height of the antenna. Control of the mast occurs in the control room adjoining the shielded chamber. This facility is capable of testing products that are rated for single phase or 3-phase AC input and DC capability is also available. Radiated emission measurements are performed using a BiLog antenna and a Horn antenna where applicable. Conducted emissions, unless otherwise stated, are performed using a LISN and using the vertical ground plane if applicable.

Calibrations and Accreditations

The 3m semi-anechoic chamber is registered with Federal Communications Commission (FCC, CA6844), Innovation, Science and Economic Development Canada (ISED, 6844A-3) and Voluntary Control Council for Interference (VCCI, R-14023, G-20072, C-14498, and T-20060). This chamber was calibrated for Normalized Site Attenuation (NSA) using test procedures outlined in ANSI C63.4 "Methods of Measurement of Radio-Noise Emissions from Low-Voltage Electrical and Electronic Equipment in the Range of 9 kHz to 40 GHz". The chamber is lined with ferrite tiles and absorption cones to minimize any undesired reflections. The NSA data is kept on file at TÜV SÜD Canada. For radiated susceptibility testing, a 16 point field calibration has been performed on the chamber. The field uniformity data is kept on file at TÜV SÜD Canada. TÜV SÜD Canada Inc. is accredited to ISO 17025 by A2LA with Testing Certificate #2955.02. The laboratory's current scope of accreditation listing can be found as listed on the A2LA website. All measuring equipment is calibrated on an annual or biennial basis as listed for each respective test.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Testing Environmental Conditions and Dates

Following environmental conditions were recorded in the facility during time of testing

Date	Test	Initials	Temperature (°C)	Humidity (%)	Pressure (kPa)
Nov. 16, 2020	Operation within the band 13.110-14.010 MHz (Field Strength)	RA	22.0	27.6	101.7
Nov. 11, 2020	Transmitter Spurious Radiated Emissions	RA	22.5	45.8	101.0
Nov. 16, 2020	20dB and 99% Occupied Bandwidth	RA	22.0	27.6	101.7
Nov. 25, 2020	Frequency Stability at Extreme Temperatures	RA	20.8 (Outside temperature chamber)	26.2	101.6
Nov. 25, 2020	Frequency Stability at Extreme Voltages	RA	20.8	26.2	101.6
Nov. 20, 2020	Power Line Conducted Emissions	RA	23.4	24.7	101.8

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Detailed Test Results Section

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Radiated Emission Field Strength

Purpose

The purpose of this test is to ensure that the RF energy unintentionally emitted from the EUT does not exceed the limits listed below as defined in the applicable test standard, as measured from a receiving antenna. This helps protect other devices which may be using the same spectrum allocations for similar or other purposes and also ensures the transmit range of the device is within the pre-determined suitable range. This also ensures public safety by not exceeding a level which has been deemed safe for human exposure.

Limits and Method

The method is as defined in ANSI C63.4.

The limits are defined in FCC Part 15.225 (a), (b), (c), and RSS-210 B.6.

The field strength of any emissions within the bands given in the table below shall not exceed the limits specified.

The testing is performed using a loop antenna.

Frequency Range (MHz)	Limit (uV/m) ¹ at 30m	Limit (dBuV/m) ¹ at 3m
< 13.110	Emission limits of FCC 15.209 apply. See <i>Transmitter Spurious Radiated Emissions</i> section	
13.110 – 13.410	106	80.5
13.410 – 13.553	334	90.5
13.553 – 13.567	15,848	124.0
13.567 – 13.710	334	90.5
13.710 – 14.010	106	80.5
> 14.010	Emission limits of FCC 15.209 apply. See <i>Transmitter Spurious Radiated Emissions</i> section	


¹ Limit is with a Quasi-Peak detector with bandwidths as defined in CISPR-16-1-1

Based on ANSI C63.4 Section 4.2, if the Peak detector measurements do not exceed the Quasi-Peak limits, where defined, then the EUT is deemed to have passed the requirements.

In accordance with FCC Part 15, section 15.31(f)(2), testing was performed at a 3 meter test distance and an extrapolation factor of 40 dB/decade was applied. For example, an extrapolation of 30m to 3m is $20\log(uV/m) + 40\log(30m/3m)$.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Typical Radiated Emissions Setup

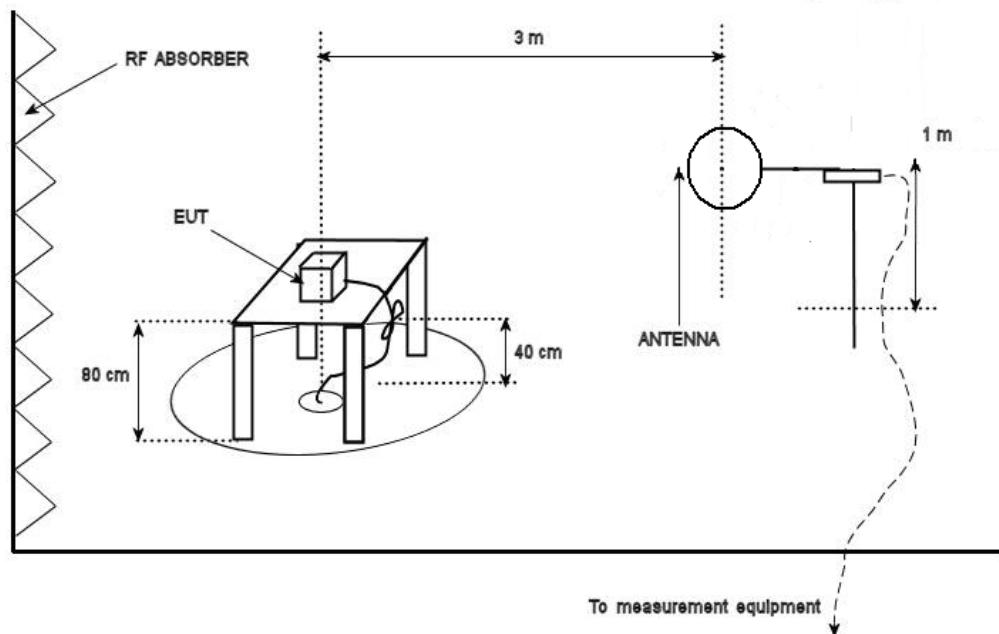

Measurement Uncertainty


The expanded measurement uncertainty is calculated in accordance with CISPR 16-4-2 and is $\pm 4.25\text{dB}$ for 30MHz – 1GHz and $\pm 4.93\text{dB}$ for 1GHz – 18GHz with a 'k=2' coverage factor and a 95% confidence level.

Preliminary Graphs

The graphs shown below are maximized peak measurement graphs over a full 0-360° rotation. The loop was orientated at 0 degrees and 90 degrees and a maximized reading is shown. The marker shows the value before factors are applied. See the *Final Measurements* section following for factor corrected values.


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Peak Emission
Max Fundamental Emission & Band Edges
13.553-13.567 MHz
3m test distance
 (Factors not incorporated. See *Final Measurements*.)
R5

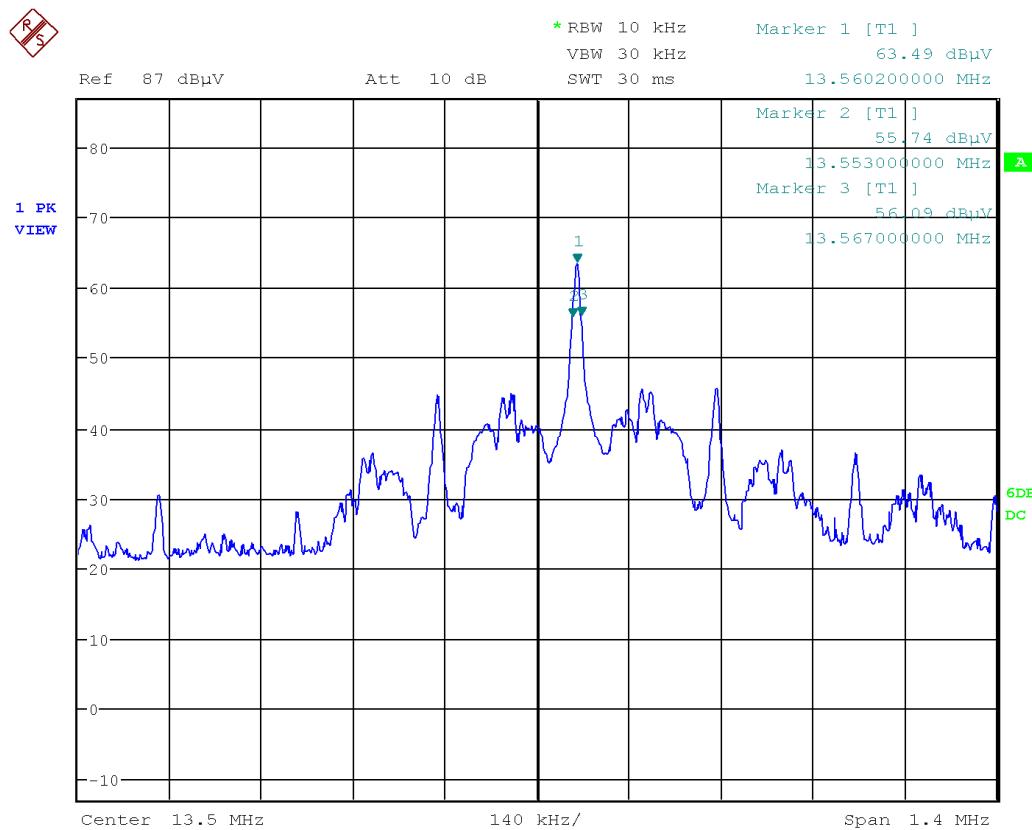


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Peak Emission
 Band Edges
 13.410-13.553 MHz
 3m test distance
 (Factors not incorporated. See *Final Measurements*.)

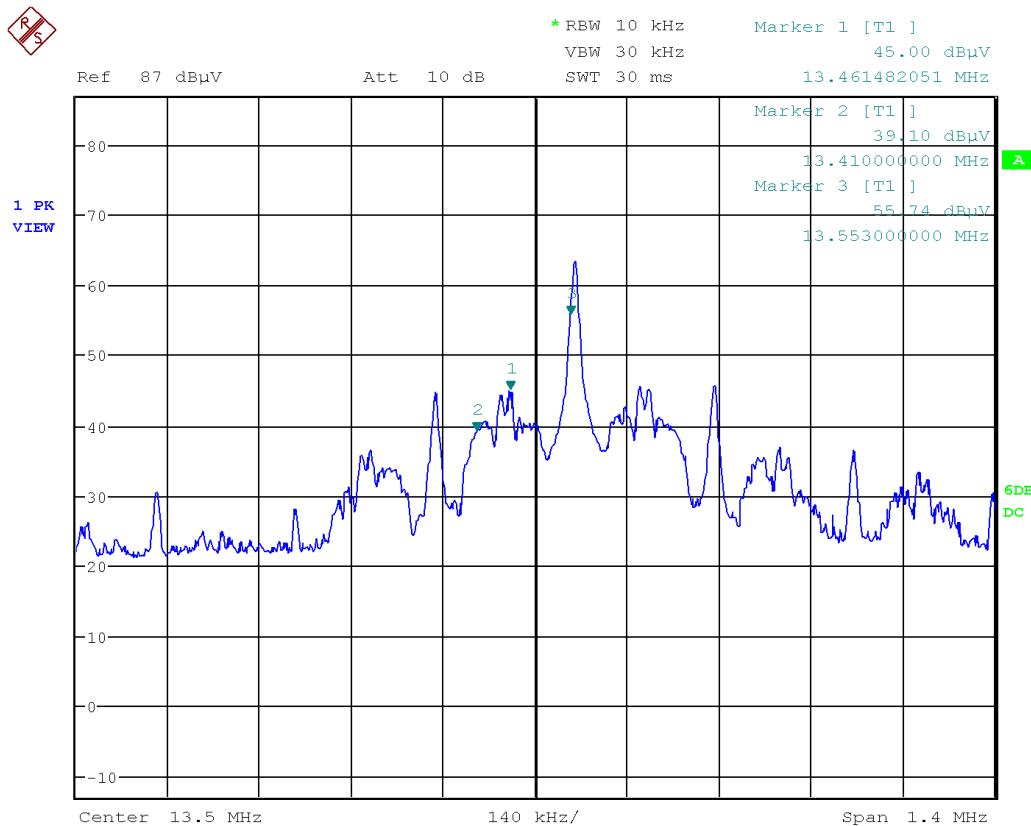

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	


Peak Emission
 Band Edges
 13.110-13.410 MHz
 3m test distance
 (Factors not incorporated. See *Final Measurements*.)

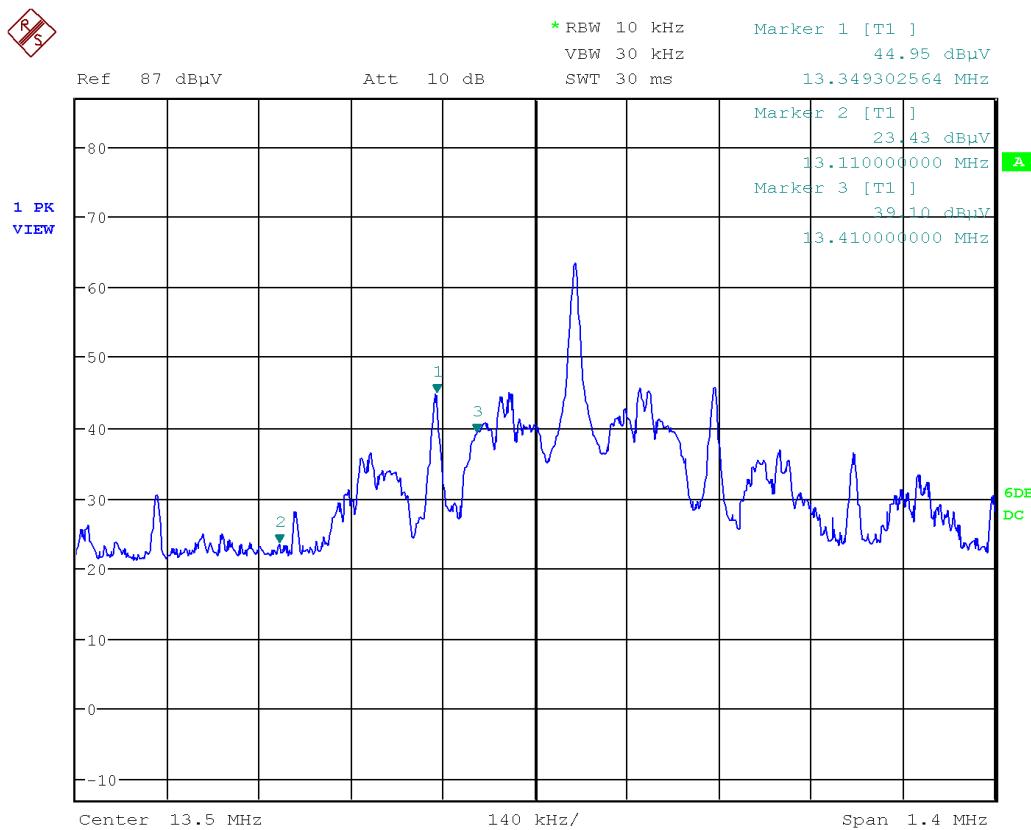

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	


Peak Emission
Band Edges
< 13.110 MHz
3m test distance

(Factors not incorporated. See *Final Measurements*.)

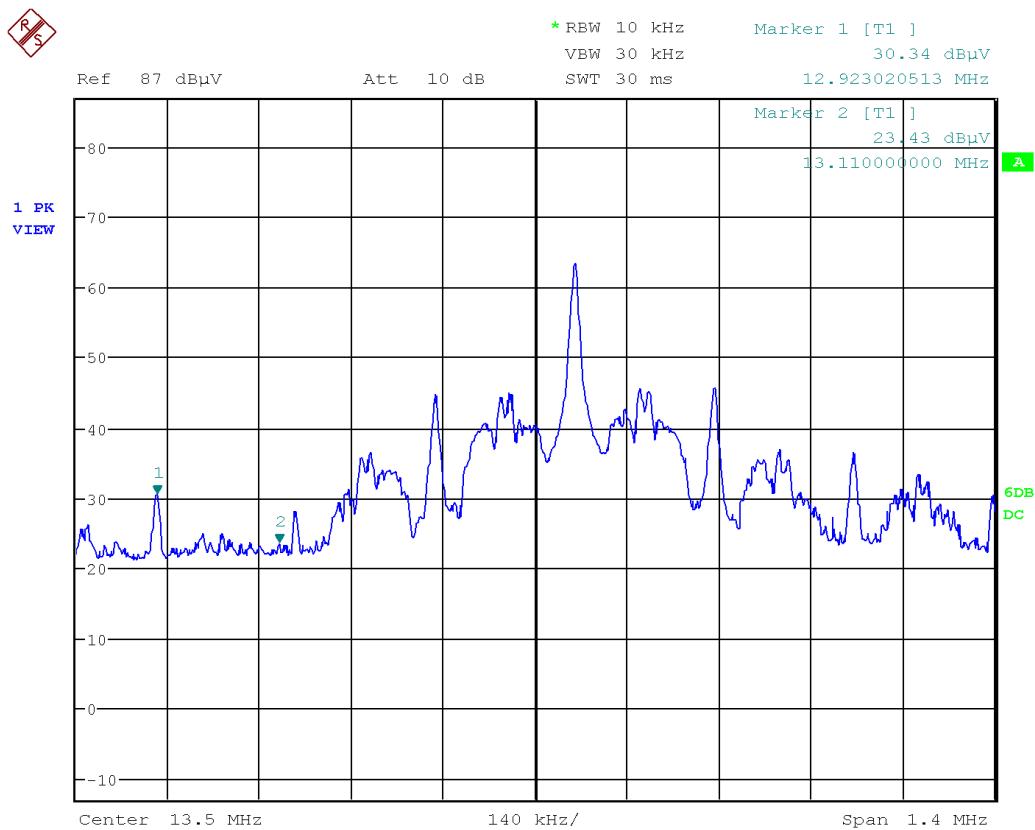


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Peak Emission
 Band Edges
 13.567-13.710 MHz
 3m test distance
 (Factors not incorporated. See *Final Measurements*.)

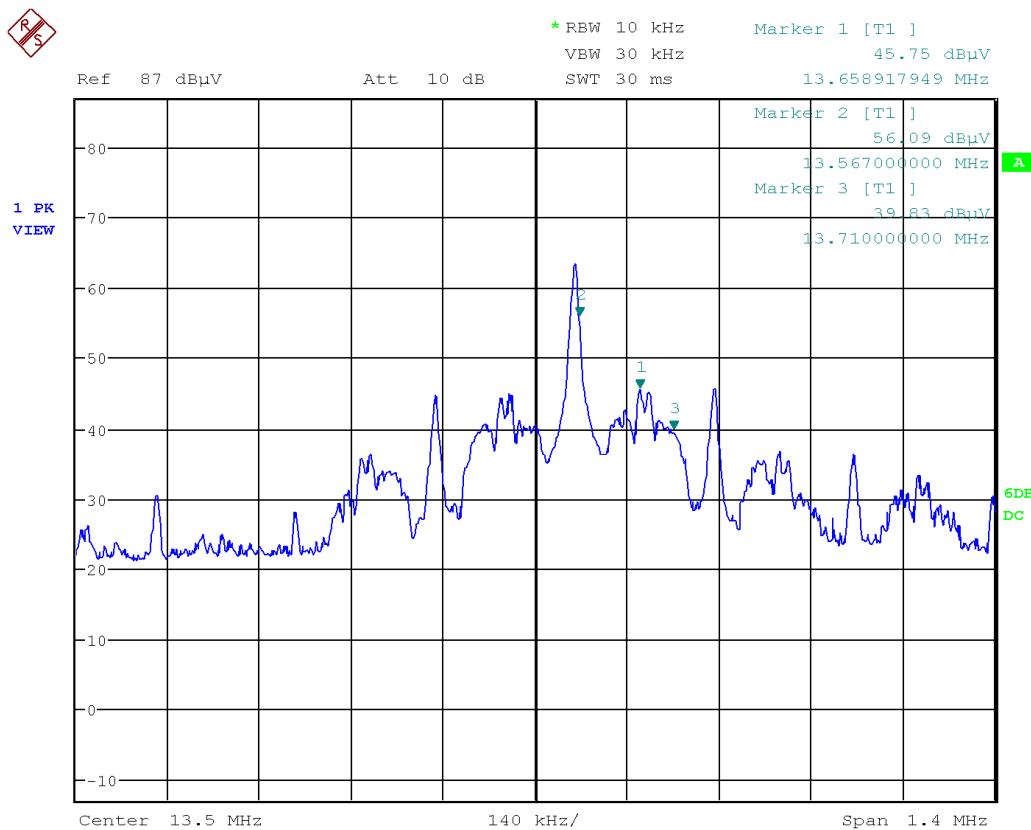

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	


Peak Emission
 Band Edges
 13.710-14.010 MHz
 3m test distance
 (Factors not incorporated. See *Final Measurements*.)

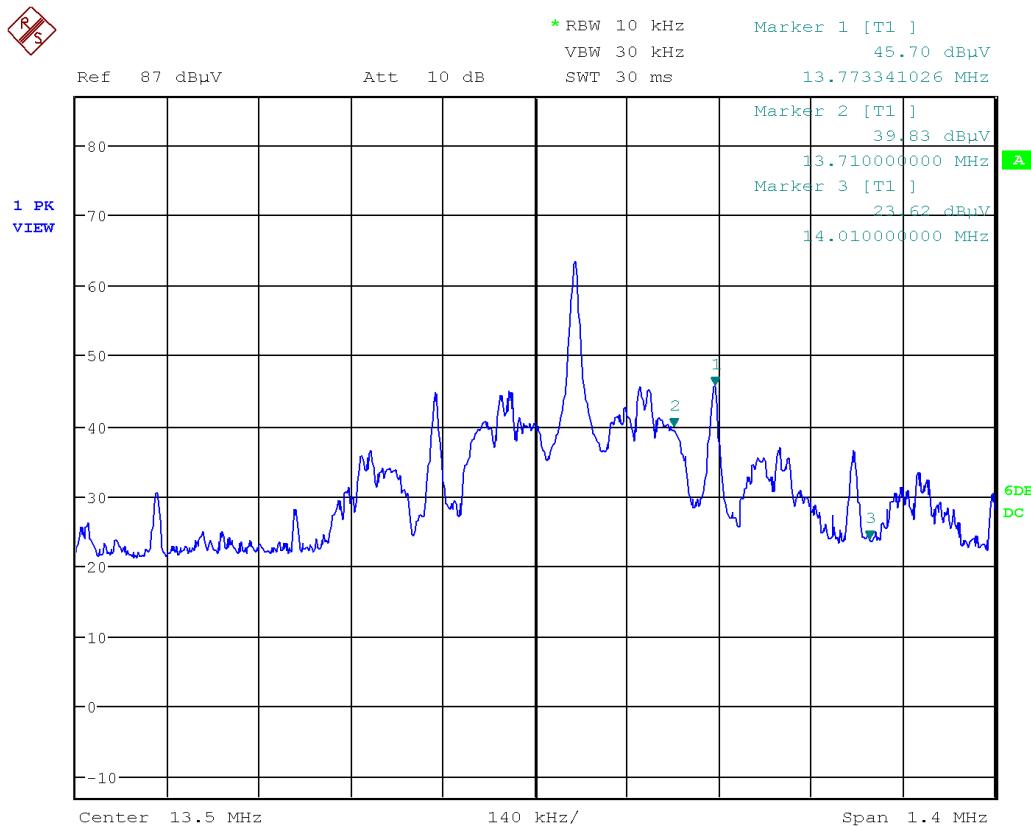

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Peak Emission
Band Edges
> 14.010 MHz
3m test distance

(Factors not incorporated. See *Final Measurements*.)

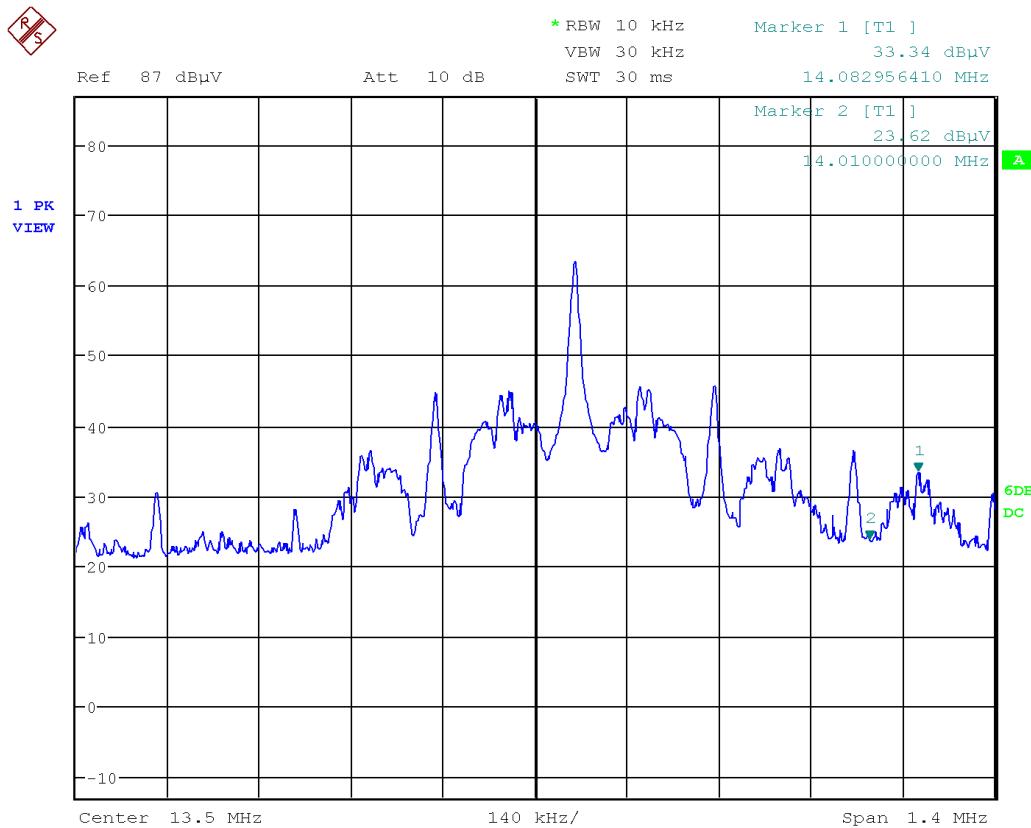

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Final Measurements

Radiated Emissions Table - 15.225
Fundamental

Test Frequency (MHz)	Detection mode	Raw signal (dB μ V)	Cable loss + Pre-selector (dB)	Antenna factor (dBS/m)	Current to voltage conversion factor (dB)	Pre-Amp Gain (dB)	Received signal (dB μ V/m)	Emission limit (dB μ V/m)	Margin (dB)	Result
13.560	Peak	63.49	0.3	-16.7	51.5	-33.7	64.87	123.9	59.03	Pass

Radiated Emissions Table - 15.225
Band Edges

Test Frequency (MHz)	Detection mode	Raw signal (dB μ V)	Cable loss + Pre-selector (dB)	Antenna factor (dBS/m)	Current to voltage conversion factor (dB)	Pre-Amp Gain (dB)	Received signal (dB μ V/m)	Emission limit (dB μ V/m)	Margin (dB)	Result
12.923	Peak	30.34	0.3	-16.8	51.5	-33.7	31.66	69.5	37.84	Pass
13.110	Peak	23.43	0.3	-16.8	51.5	-33.7	24.75	69.5	44.75	Pass
13.349	Peak	44.95	0.3	-16.8	51.5	-33.7	46.31	80.5	34.19	Pass
13.410	Peak	39.1	0.3	-16.8	51.5	-33.7	40.46	80.5	40.04	Pass
13.461	Peak	45.0	0.3	-16.8	51.5	-33.7	46.37	90.47	44.1	Pass
13.553	Peak	55.74	0.3	-16.8	51.5	-33.7	57.11	90.47	33.36	Pass
13.567	Peak	56.09	0.3	-16.7	51.5	-33.7	57.47	90.47	33.0	Pass
13.659	Peak	45.75	0.3	-16.7	51.5	-33.7	47.13	90.47	43.34	Pass
13.710	Peak	39.83	0.3	-16.7	51.5	-33.7	41.22	80.5	39.28	Pass
13.773	Peak	45.7	0.3	-16.7	51.5	-33.7	47.09	80.5	33.41	Pass
14.010	Peak	23.62	0.3	-16.7	51.5	-33.7	25.04	69.5	44.46	Pass
14.083	Peak	33.34	0.3	-16.7	51.5	-33.7	34.76	69.5	34.74	Pass

Notes:

See *Transmitter Spurious Radiated Emissions* section in this report for spurious emissions test results outside of the FCC 15.225 bands.

See photo exhibits for photos showing the test set-up.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	ESR 26	Rohde & Schwarz	Mar. 6, 2020	Mar. 6, 2022	GEMC 341
Loop Antenna 150 kHz – 30 MHz	EM 6872	Electro-Metrics	Feb 15, 2019	Feb 15, 2021	GEMC 71
Pre-Amp 9 kHz – 1 GHz	CPA9230	Chase	May 22, 2020	May 22, 2022	GEMC 301
RF Cable 10m	LMR-400-10M-50Ω-MN-MN	LexTec	NCR	NCR	GEMC 27
RF Cable 3m	HP305S	Semflex	NCR	NCR	GEMC 310

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Transmitter Spurious Radiated Emissions

Purpose

The purpose of this test is to ensure that the RF energy unintentionally emitted from the EUT does not exceed the limits listed below as defined in the applicable test standard, as measured from a receiving antenna. This helps protect broadcast radio services such as television, FM radio, pagers, cellular telephones, emergency services, and so on, from unwanted interference.

Limits and Method

The method is defined in ANSI C63.10.

The requirement is stated in FCC 15.225(d), and RSS-210 B.6 a. iv.

The limits are as defined in 47 CFR FCC Part 15.209 and RSS-Gen (Table 5 and Table 6).

The limits apply for emissions that fall outside the 13.110–14.010 MHz band.

These limits are as follows:

Frequency	Limit
0.009 MHz – 0.490 MHz	2400/F(kHz) uV/m at 300m ¹
0.490 MHz – 1.705 MHz	24000/F(kHz) uV/m at 30m ¹
1.705 MHz – 30 MHz	30 uV/m at 30m ¹
30 MHz – 88 MHz	100 uV/m (40.0 dBuV/m ¹) at 3m
88 MHz – 216 MHz	150 uV/m (43.5 dBuV/m ¹) at 3m
216 MHz – 960 MHz	200 uV/m (46.0 dBuV/m ¹) at 3m
Above 960 MHz	500 uV/m (54.0 dBuV/m ¹) at 3m
Above 1000 MHz	500 uV/m (54 dBuV/m ²) at 3m
Above 1000 MHz	500 uV/m (74 dBuV/m ³) at 3m

¹ Limit is with Quasi Peak detector with bandwidths as defined in CISPR-16-1-1


² Limit is with 1 MHz measurement bandwidth and using an Average detector

³ Limit is with 1 MHz measurement bandwidth and using a Peak detector

Based on ANSI C63.4 Section 4.2, if the Peak detector measurements do not exceed the Quasi-Peak limits, where defined, then the EUT is deemed to have passed the requirements.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Typical Radiated Emissions Setup

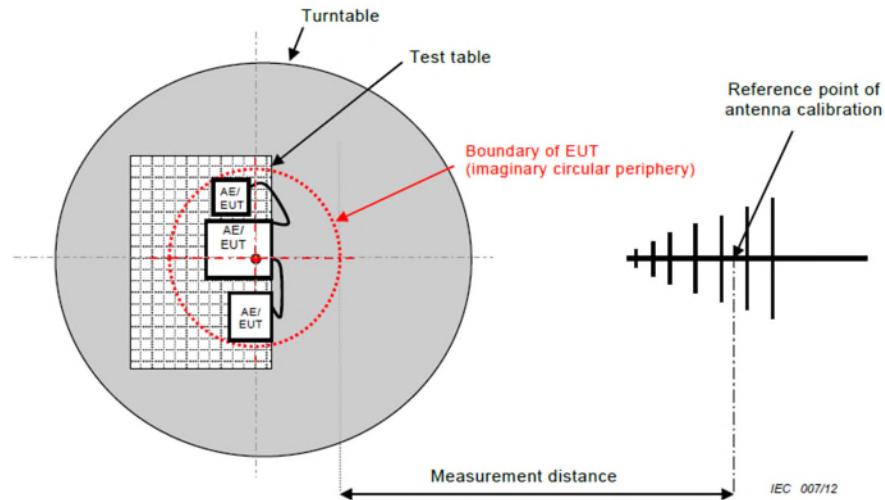

Measurement Uncertainty

The expanded measurement uncertainty is calculated in accordance with CISPR 16-4-2 and is $\pm 4.25\text{dB}$ for 30MHz – 1GHz and $\pm 4.93\text{dB}$ for 1GHz – 18GHz with a 'k=2' coverage factor and a 95% confidence level.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Preliminary Graphs

The graphs shown below are maximized peak measurement graphs measured with a resolution bandwidth greater than or equal to the final required detector over a full 0-360°. This peaking process is done as a worst case measurement and enables the detection of frequencies of concern for final measurement. For final measurements with the appropriate detector, where applicable, please refer to the tables under *Final Measurements*.

In accordance with FCC Part 15, Subpart A, Section 15.33, the device was scanned to the 10th harmonic.

Devices may be scanned at alternate test distances and in accordance with FCC Part 15, Subpart A, Section 15.31, an extrapolation factor of 20 dB/decade was used above 30 MHz and 40 dB/decade below 30 MHz.


All transmitters in the EUT are on and transmitting continuous modulated data at the maximum power setting used by the manufacturer.

Plots and measurements are made at a 3 meter distance.

See *Radiated Emission Field Strength* section for measurements at the band-edges.


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

9 kHz – 150 kHz
Peak Emission Graph

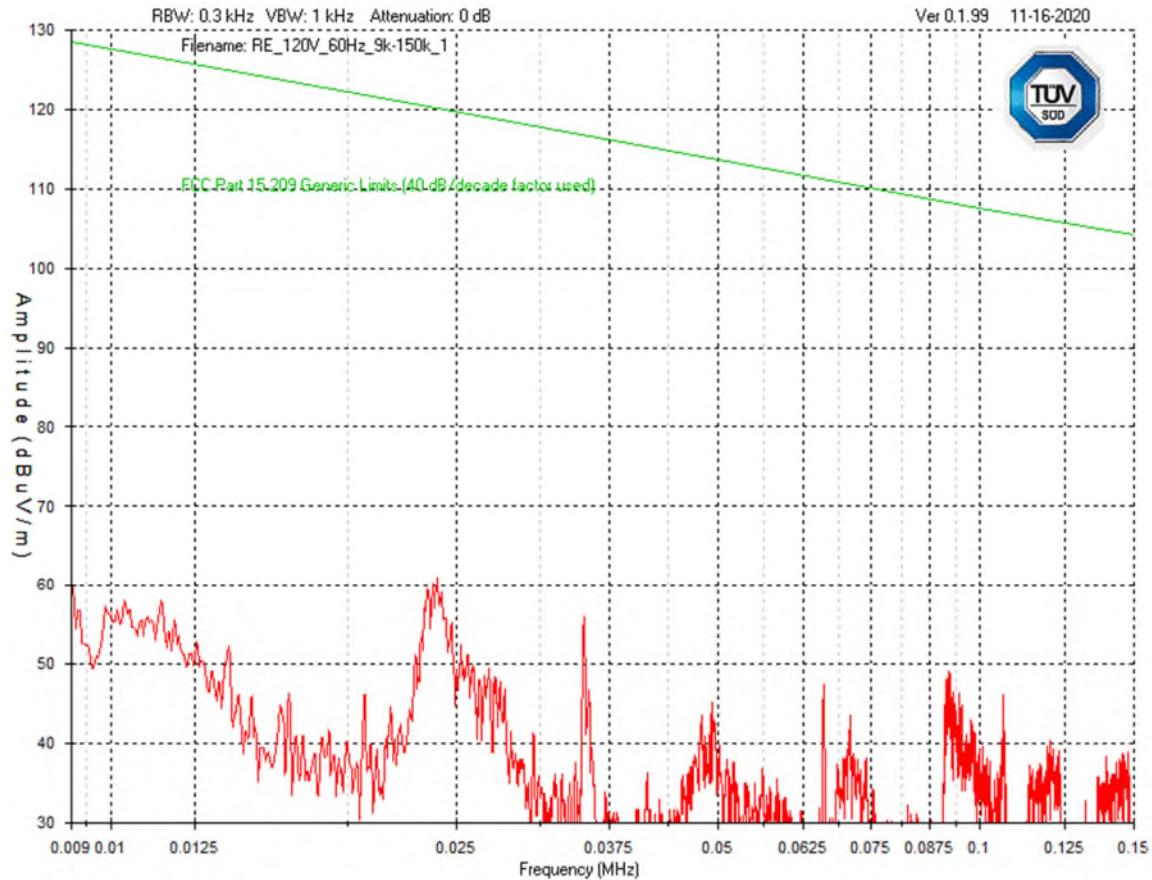


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

150 kHz – 30 MHz
Peak Emission Graph

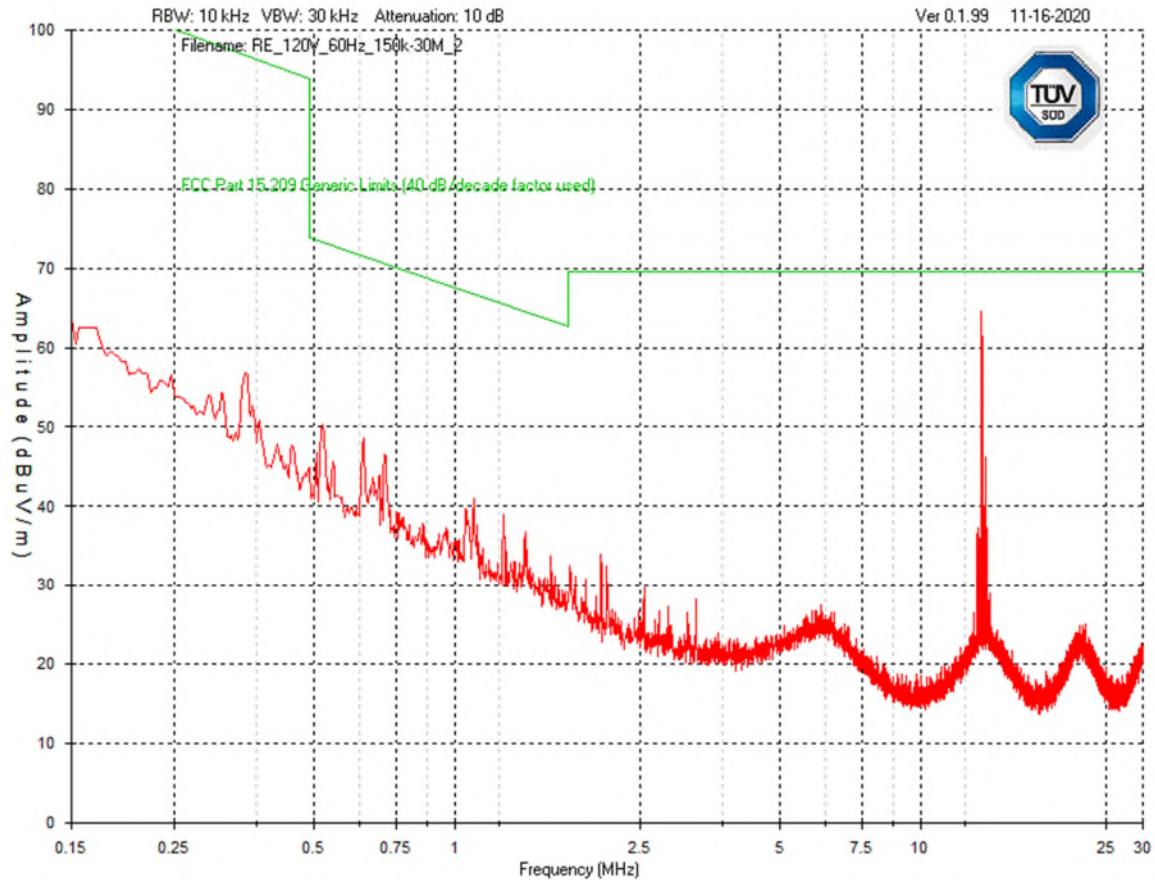


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

30 MHz – 1 GHz
Horizontal - Peak Emission Graph

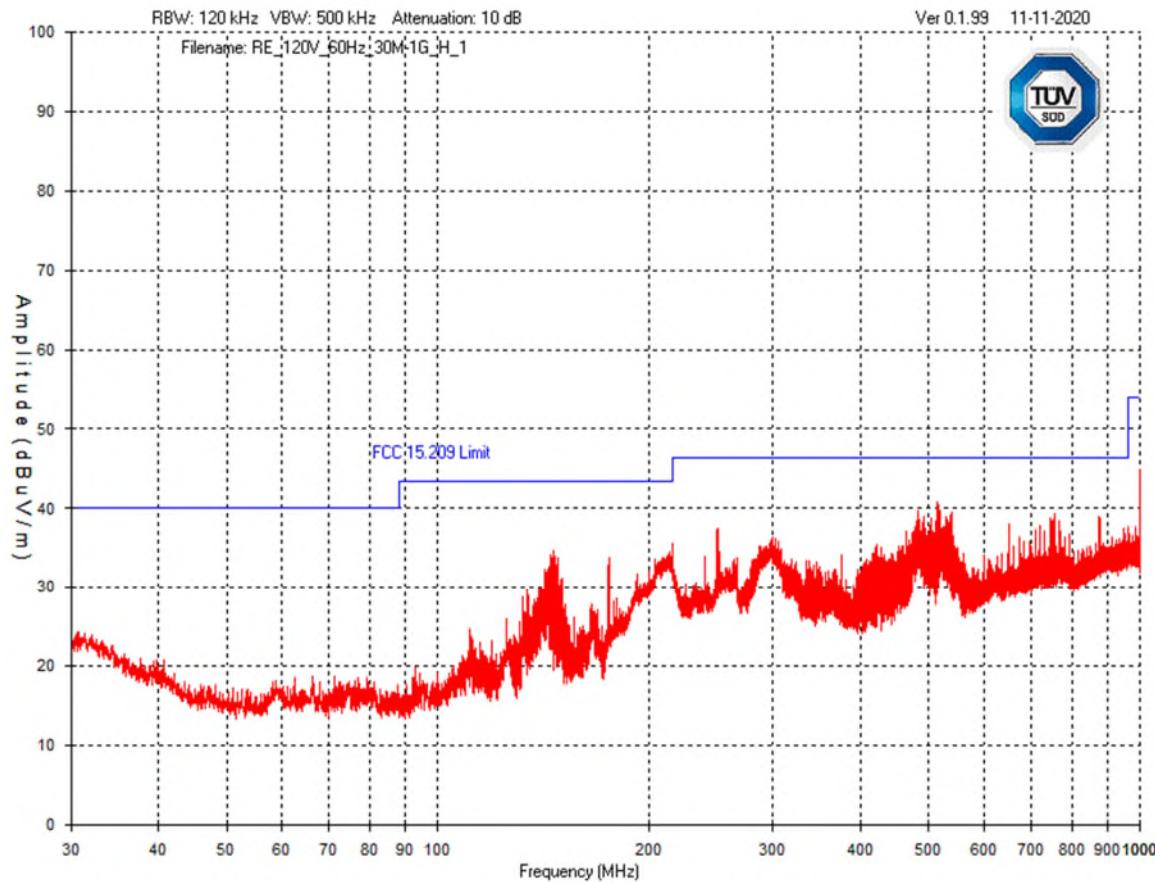


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

1GHz – 2GHz
Horizontal - Peak Emission Graph

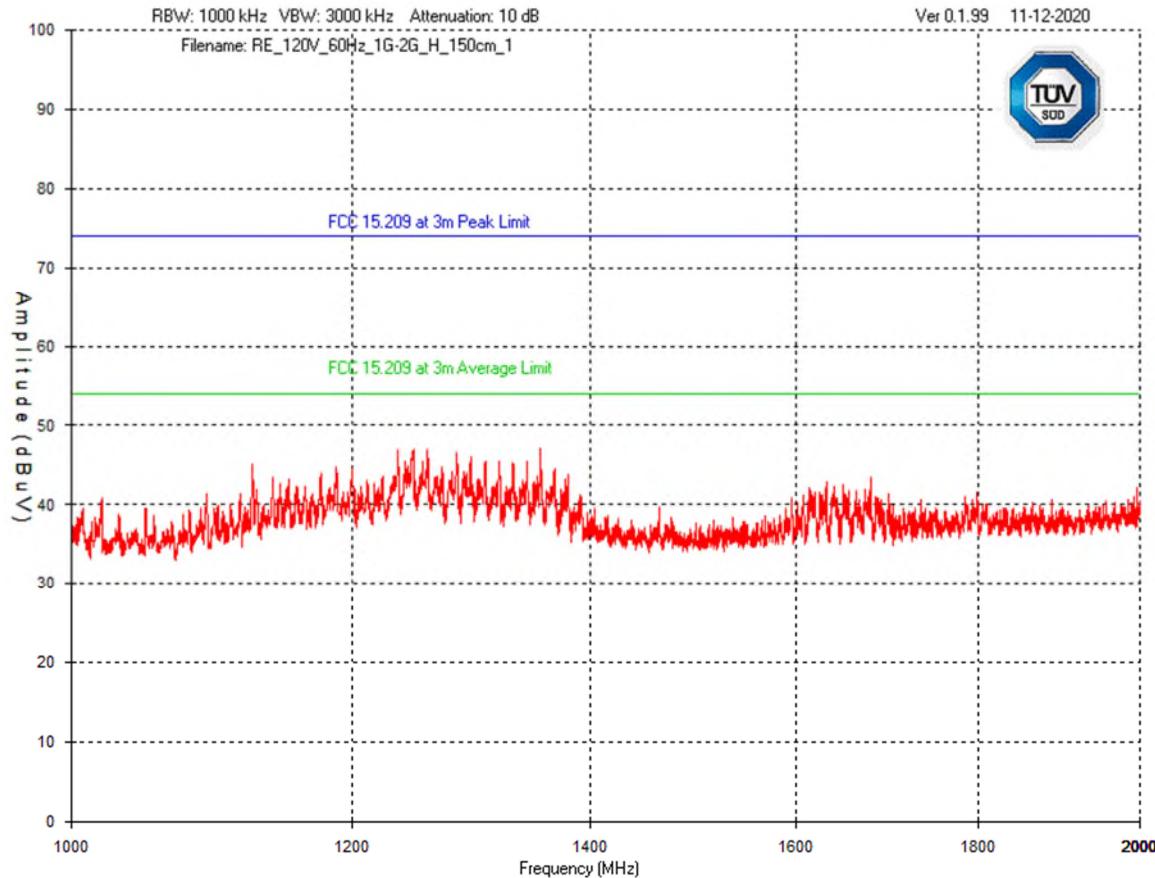


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

30 MHz – 1 GHz
Vertical - Peak Emission Graph

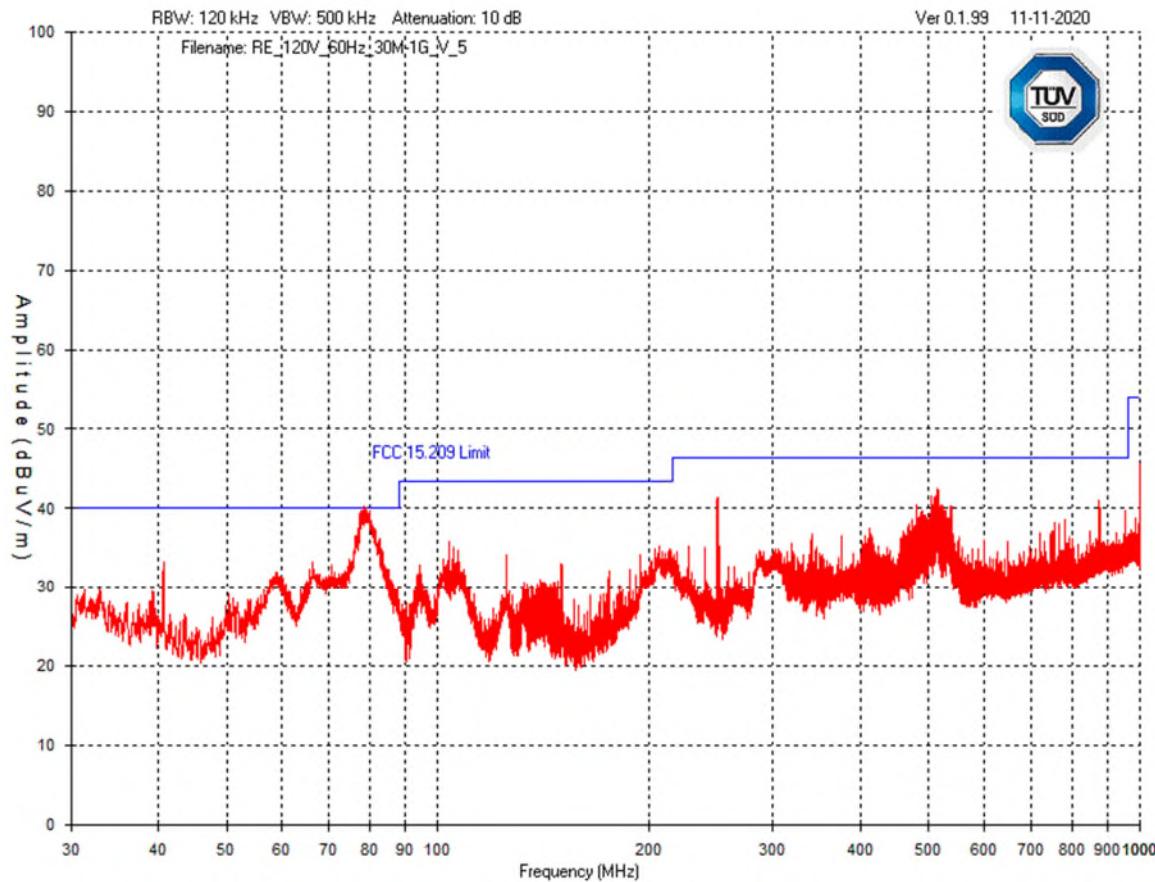

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

1 GHz – 2 GHz
Vertical - Peak Emission Graph

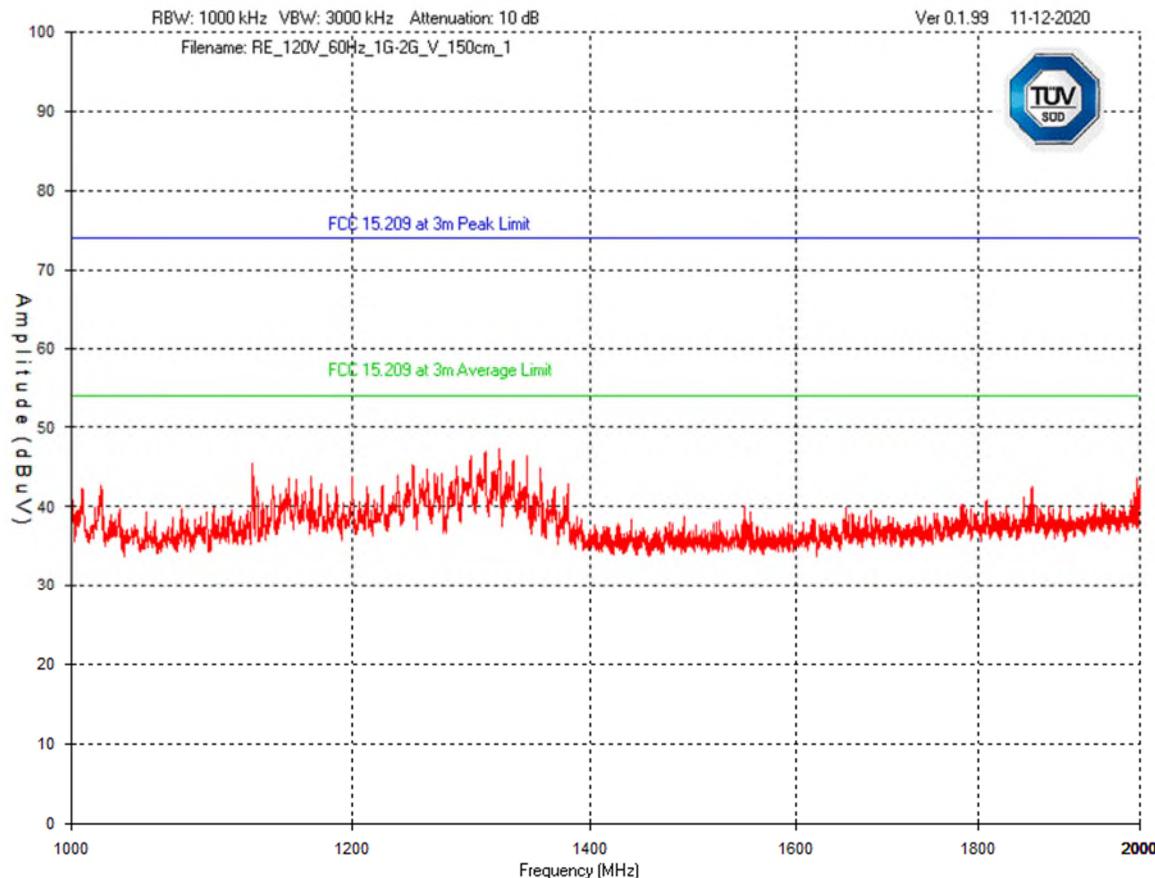

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Final Measurements and Results

The measurements were maximized by rotating the turn table over a full 0-360° rotation and the antenna height was varied from 1 m to 4 m.

Spurious Radiated Emissions Table

Frequency (MHz)	Detector	Received Signal (dB μ V)	Antenna Factor (dB/m)	Cable Factor (dB)	Pre-Amp (dB)	Level (dB μ V/m)	Limit (dB μ V/m)	Margin (dB)	Test Result
Horizontal Antenna Polarization									
513.84	PEAK	41.5	24.8	3.1	-28.7	40.7	46.4	5.7	Pass
481.77	PEAK	40.7	24.6	3.0	-28.6	39.7	46.4	6.7	Pass
517.60	PEAK	40.3	24.9	3.1	-28.7	39.6	46.4	6.8	Pass
755.97	PEAK	35.6	28.0	4.2	-28.5	39.3	46.4	7.1	Pass
875.01	PEAK	33.4	29.3	4.6	-28.4	38.9	46.4	7.5	Pass
650.00	PEAK	35.9	26.9	3.8	-28.6	38.0	46.4	8.4	Pass
Vertical Antenna Polarization									
78.44	QP	52.5	12.2	0.9	-28.5	37.1	40.0	2.9	Pass
514.92	QP	39.9	24.8	3.1	-28.7	39.1	46.4	7.3	Pass
515.82	PEAK	43.0	24.8	3.1	-28.7	42.2	46.4	4.2	Pass
512.98	PEAK	42.6	24.8	3.1	-28.7	41.8	46.4	4.6	Pass
513.99	PEAK	42.5	24.8	3.1	-28.7	41.7	46.4	4.7	Pass
504.21	PEAK	42.7	24.4	3.1	-28.7	41.5	46.4	4.9	Pass

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	ESU 40	Rohde & Schwarz	Jan. 15, 2020	Jan. 15, 2022	GEMC 233
Loop Antenna 9 – 150 kHz	EM 6871	Electro-Metrics	Feb 15, 2019	Feb 15, 2021	GEMC 70
Loop Antenna 150 kHz – 30 MHz	EM 6872	Electro-Metrics	Feb 15, 2019	Feb 15, 2021	GEMC 71
BiLog Antenna 30 MHz – 1 GHz	3142-C	ETS	Mar. 01, 2019	Mar. 01, 2021	GEMC 137
Pre-Amp 9 kHz – 1 GHz	LNA 6901	Teseq	Feb. 25, 2019	Feb. 25, 2021	GEMC 168
Attenuator 6 dB	612-6-1	Meca Electronics, Inc	NCR	NCR	GEMC 287
RF Cable 10m	LMR-400-10M-50Ω-MN-MN	LexTec	NCR	NCR	GEMC 274
RF Cable 2m	Sucoflex 104A	Huber+Suhner	NCR	NCR	GEMC 271
Emissions Software	0.1.99	TUV SUD Canada, Inc.	NCR	NCR	GEMC 58

FCC - 15.209 -Radiated Emissions_Rev1

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Carrier Frequency Stability

Purpose

The purpose of this test is to ensure that the frequency tolerance of the carrier signal is maintained within the required limits during extreme temperature and voltage variations. This helps protect radio broadcasts and receivers with spectrum nearby to the equipment under test from unwanted interference. This also helps ensure proper reception of the intended signal by ensuring the transmit frequency is correct over the expected temperature and voltage range.

Limits and Method

The limits are as defined in FCC Part 15, Section 15.225 (e). The frequency tolerance of the carrier signal shall be maintained within $\pm 0.01\%$ of the operating frequency (i.e. 13.558644 – 13.561356 MHz) over a temperature variation of -20°C to $+50^{\circ}\text{C}$ at normal supply voltage, and for a variation in the primary supply voltage from 85% to 115% of the rated supply voltage at a temperature of 20°C .

Results (Temperature Variation)

There is no deviation in the fundamental frequency during the tests which would cause it to be non-compliant with the requirements. The results are presented in the charts below.

The EUT is only rated to be used within 15°C - 40°C . However, the 13.56 MHz transmission is tested between -20°C to $+50^{\circ}\text{C}$.

Frequency Tolerance Table

Fundamental Frequency Recorded After EUT is Turned On (MHz)				
Temperature	Immediately	+2 mins	+5 mins	+10 mins
+50 °C	13.560435897	13.560435897	13.560435897	13.560435897
+40 °C	13.560435897	13.560432692	13.560432692	13.560435897
+30 °C	13.560439103	13.560432692	13.560432692	13.560435897
+20 °C	13.560432692	13.560439103	13.560435897	13.560435897
+15 °C	13.560438333	13.56045833	13.560458333	13.560451923
+10 °C	13.560455128	13.560458333	13.560461538	13.560461538
0 °C	13.560464744	13.560461538	13.560464744	13.560464744
-10 °C	13.560448718	13.560448718	13.560448718	13.560448718
-20 °C	13.560391026	13.560391026	13.560391026	13.560397436

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Results (Voltage Variation)

There is no deviation in the fundamental frequency during the tests which would cause it to be non-compliant with the requirements. The results are presented in the charts below.

The EUT is powered by mains. Its rated input voltage is 100-240V. The voltage is varied between 85% to 115% of the rated voltage at a temperature of 20 °C. The voltage is varied between 85V-276V, at 60Hz.

Voltage Variation Table

Voltage (V)	Fundamental Frequency (MHz)
85	13.560451923
102	13.560451923
120	13.560455128
138	13.560451923
276	13.560451923

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	ESL 6	Rohde & Schwarz	Feb. 25, 2019	Feb. 25, 2021	GEMC 160
Loop Antenna	EM 6872	Electro-Metrics	Feb 15, 2019	Feb 15, 2021	GEMC 71
Pre-Amp	CPA9230	Chase	May 22, 2020	May 22, 2022	GEMC 301
Temperature & Humidity Monitor	iTHX-SD	Omega	Feb. 28, 2019	Feb. 28, 2021	GEMC 225
Digital Multimeter	287	Fluke	Jul. 16, 2020	Jul. 16, 2021	CANE 00151

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Power Line Conducted Emissions

Purpose

The purpose of this test is to ensure that the RF energy unintentionally emitted from the EUT's power line does not exceed the limits listed below as defined in the applicable test standard, as measured from a LISN. This helps protect lower frequency radio services such as AM radio, shortwave radio, amateur radio operators, maritime radio, CB radio, and so on, from unwanted interference.

Limits and Method

The limits are defined in FCC 15.207 and RSS-Gen Table 4.

Method is as defined in ANSI C63.4.

Average Limits		Quasi-Peak Limits	
150 kHz – 500 kHz	56 to 46* dB μ V	150 kHz – 500 kHz	66 to 56* dB μ V
500 kHz – 5 MHz	46 dB μ V	500 kHz – 5 MHz	56 dB μ V
5 MHz – 30 MHz	50 dB μ V	5 MHz – 30 MHz	60 dB μ V


* Decreases linearly with the logarithm of the frequency

Both Quasi-Peak and Average limits are applicable and each is specified as being measured with a resolution bandwidth of 9 kHz. For Quasi-Peak, a video bandwidth at least three times greater than the resolution bandwidth is used.

Based on ANSI C63.4 Section 4.2, if the Peak or Quasi-Peak detector measurements do not exceed the Average limits, then the EUT is deemed to have passed the requirements.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Typical Setup Diagram

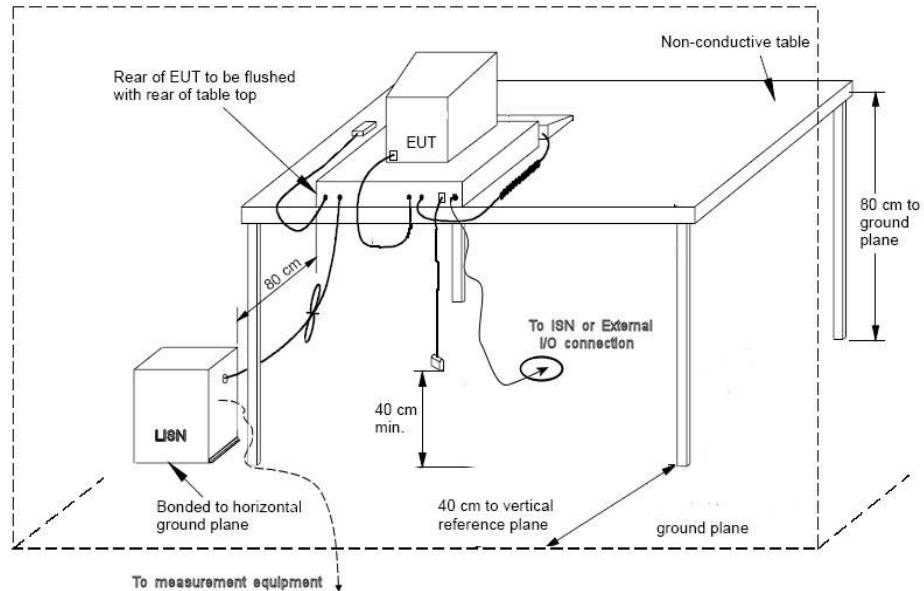

Measurement Uncertainty

The expanded measurement uncertainty is calculated in accordance with CISPR 16-4-2 and is $\pm 2.73\text{dB}$ with a 'k=2' coverage factor and a 95% confidence level.


Preliminary Graphs

The graphs shown below are maximized peak measurement graphs measured with a resolution bandwidth greater than or equal to the final required detector. This peaking process is done as a worst case measurement and enables the detection of frequencies of concern for final measurement. For final measurements with the appropriate detector, where applicable, please refer to the tables under Final Measurements.

Note: CISPR 11 Class B limits shown in the plots below (green limit lines) are equivalent to the limits of FCC 15.207 and RSS-Gen Table 4.


Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Line 1 (L1) – 120Vac 60Hz

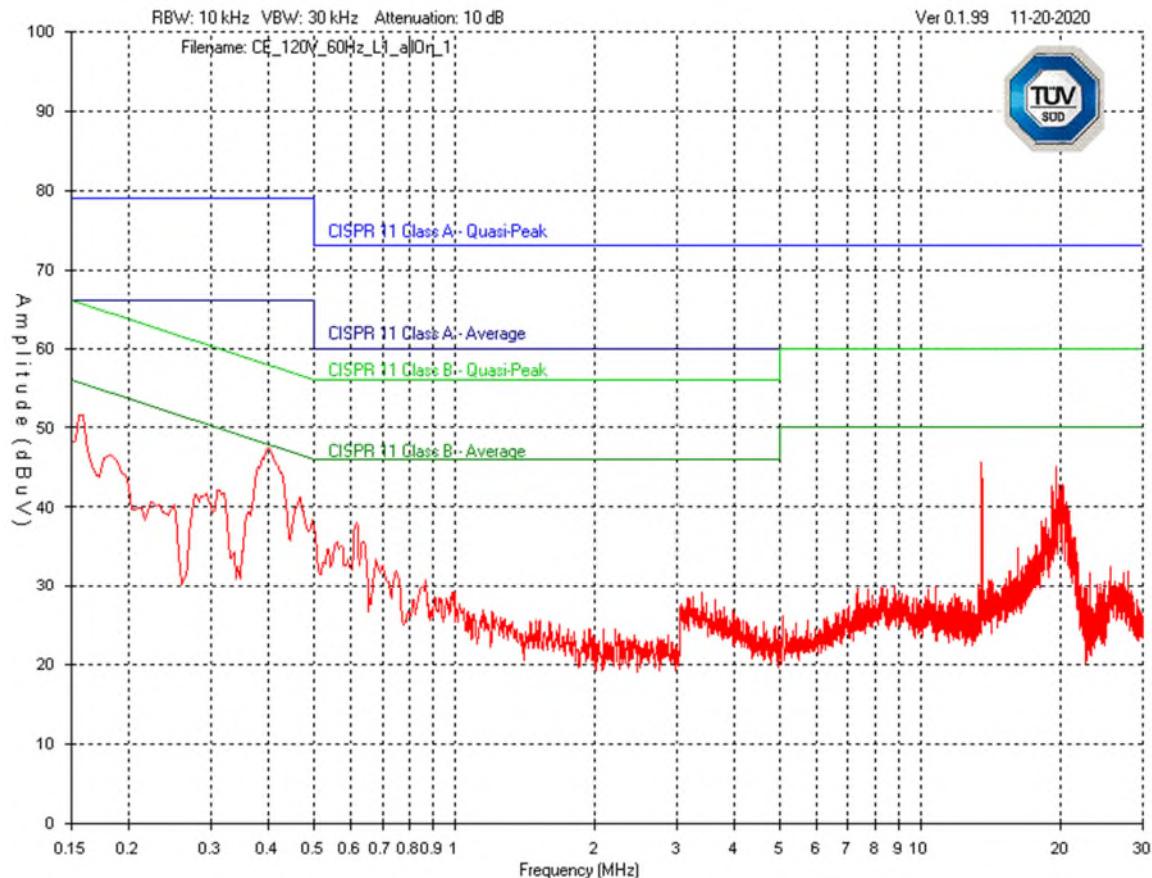

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Line 2 (L2) – 120Vac 60Hz

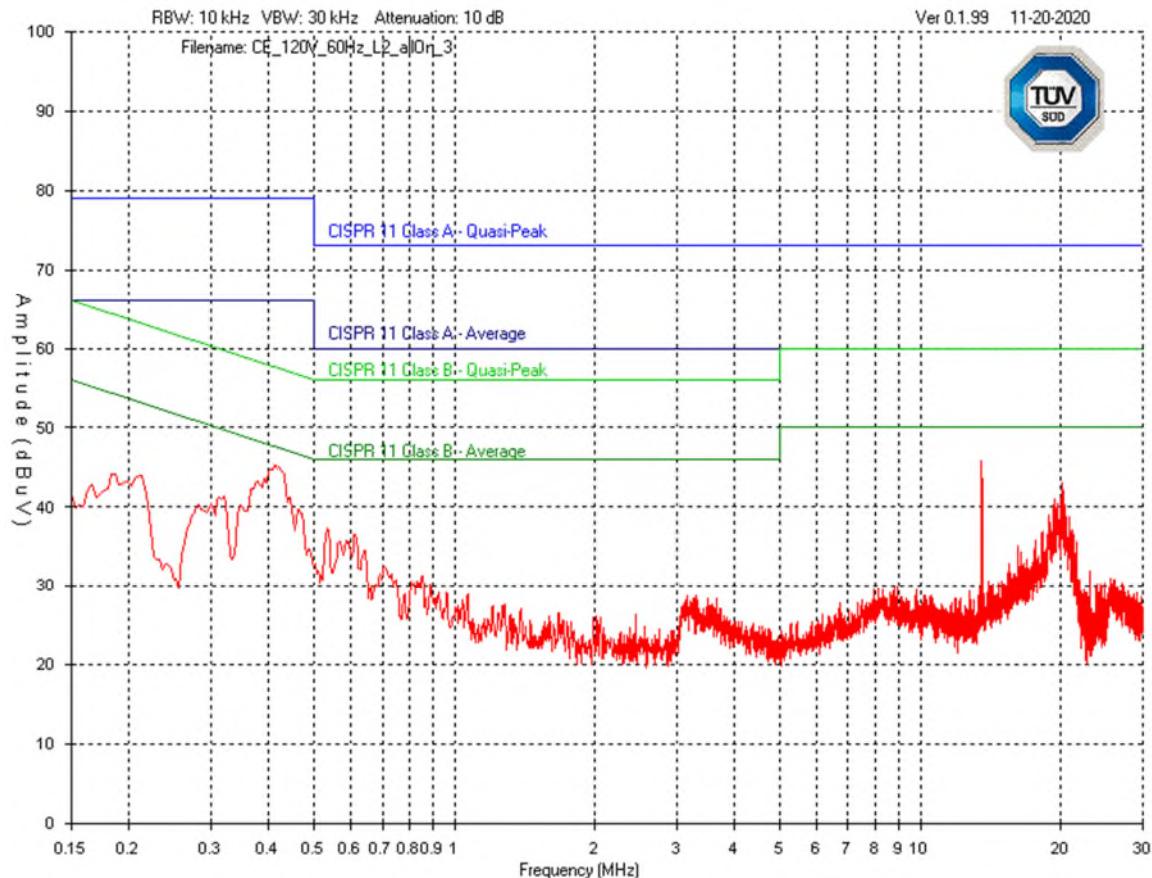

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Final Measurements

Power Line Conducted Emissions Table
120V, 60Hz

Frequency (MHz)	Detector	Received Signal (dB μ V)	Atten Factor (dB)	Cable Factor (dB)	LISN Factor (dB)	Level (dB μ V)	QP Limit (dB μ V)	AVG Limit (dB μ V)	QP Margin (dB)	AVG Margin (dB)	Test Result
Line											
0.399	PEAK	37.3	10	0.1	0.0	47.4	57.9	--	10.5	--	Pass
0.399	AVG	24.4	10	0.1	0.0	34.5	--	47.9	--	13.4	Pass
0.157	PEAK	41.5	10	0.0	0.1	51.6	65.6	--	14.0	--	Pass
0.157	AVG	24.8	10	0.0	0.1	34.9	--	55.6	--	20.7	Pass
13.560	PEAK	35.2	10	0.1	0.3	45.6	60.0	--	14.4	--	Pass
13.560	AVG	34.7	10	0.1	0.3	45.1	--	50.0	--	4.9	Pass
19.558	PEAK	34.4	10	0.1	0.7	45.2	60.0	--	14.8	--	Pass
19.558	AVG	19.7	10	0.1	0.7	30.5	--	50.0	--	19.5	Pass
0.313	PEAK	32.0	10	0.1	0.1	42.2	59.9	49.9	17.7	7.7	Pass
0.615	PEAK	27.9	10	0.1	0.0	38.0	56.0	46.0	18.0	8.0	Pass
Neutral											
0.409	PEAK	35.1	10	0.1	0.1	45.3	57.7	--	12.4	--	Pass
0.409	AVG	24.3	10	0.1	0.1	34.5	--	47.7	--	13.2	Pass
13.560	PEAK	35.4	10	0.1	0.3	45.8	60.0	--	14.2	--	Pass
13.560	AVG	34.9	10	0.1	0.3	45.3	--	50.0	--	4.7	Pass
20.163	PEAK	32.2	10	0.1	0.8	43.1	60.0	--	16.9	--	Pass
20.163	AVG	20.5	10	0.1	0.8	31.4	--	50.0	--	18.6	Pass
0.320	PEAK	31.3	10	0.1	0.1	41.5	59.7	49.7	18.2	8.2	Pass
0.532	PEAK	27.1	10	0.1	0.1	37.3	56.0	46.0	18.7	8.7	Pass
0.187	PEAK	34.1	10	0.0	0.1	44.2	64.2	54.2	20.0	10.0	Pass

Notes:

PEAK = Peak measurement

AVG = Average measurement

See photo exhibits for photos showing the test set-up.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration Date	Next Calibration Date	Asset #
Spectrum Analyzer	ESL 6	Rohde & Schwarz	Feb. 25, 2019	Feb. 25, 2021	GEMC 160
LISN	FCC-LISN-50/250-16-2-01	FCC	Feb. 27, 2019	Feb. 27, 2021	GEMC 303
RF Cable 3m	LMR-400-3M-50Ω-MN-MN	LexTec	NCR	NCR	GEMC 276
Attenuator 10 dB	6N10W-10	Inmet	NCR	NCR	GEMC 350
Emissions Software	0.1.99	TUV SUD Canada, Inc.	NCR	NCR	GEMC 58

FCC-ICES003_CE_Rev1'

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

20dB and 99% Occupied Bandwidth

Purpose

The purpose of this test is to find the 20 dB and 99% occupied bandwidths of the 13.56 MHz emission. This is the bandwidth which is attenuated 20 dB from the peak of the intentional transmission, and the bandwidth which contains 99% transmitted power, respectively.

Limits and Method

The method is as defined in ANSI C63.10.

There are no applicable limits for the 13.56 MHz emission. Its results are for informational purposes only.

Results


The 20dB BW measured is: 433 kHz

The 99% BW measured is: 742 kHz

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	


Graphs

20dB Bandwidth

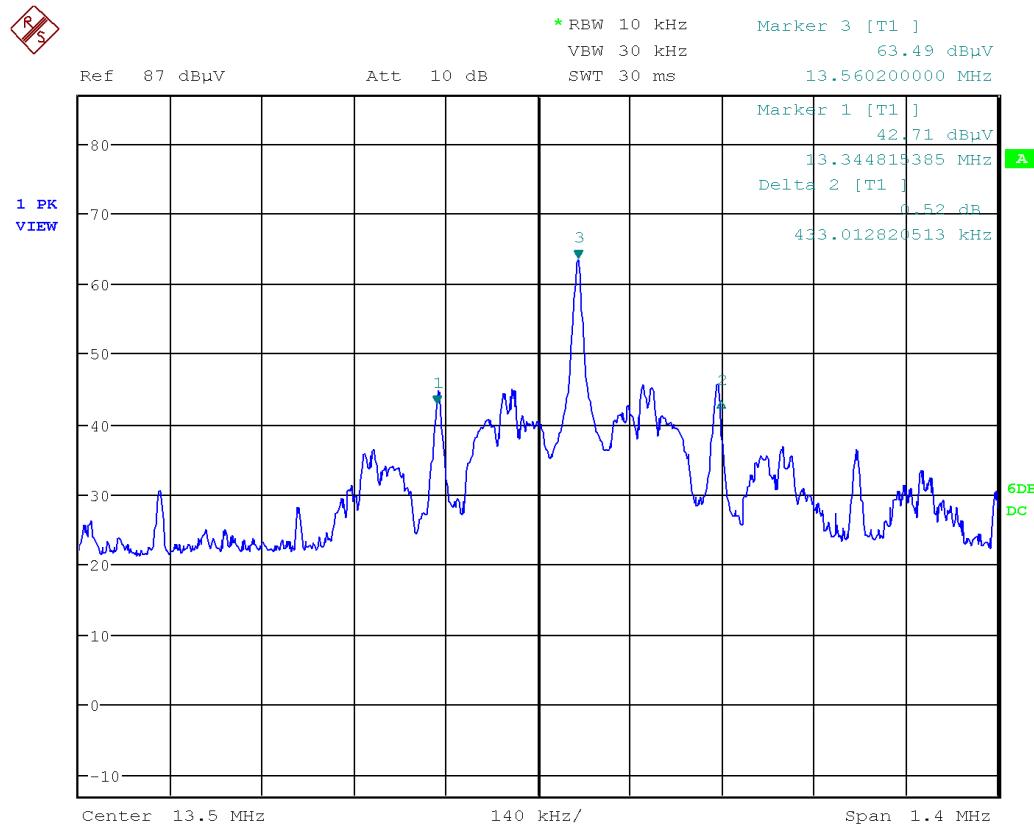

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

99% Bandwidth

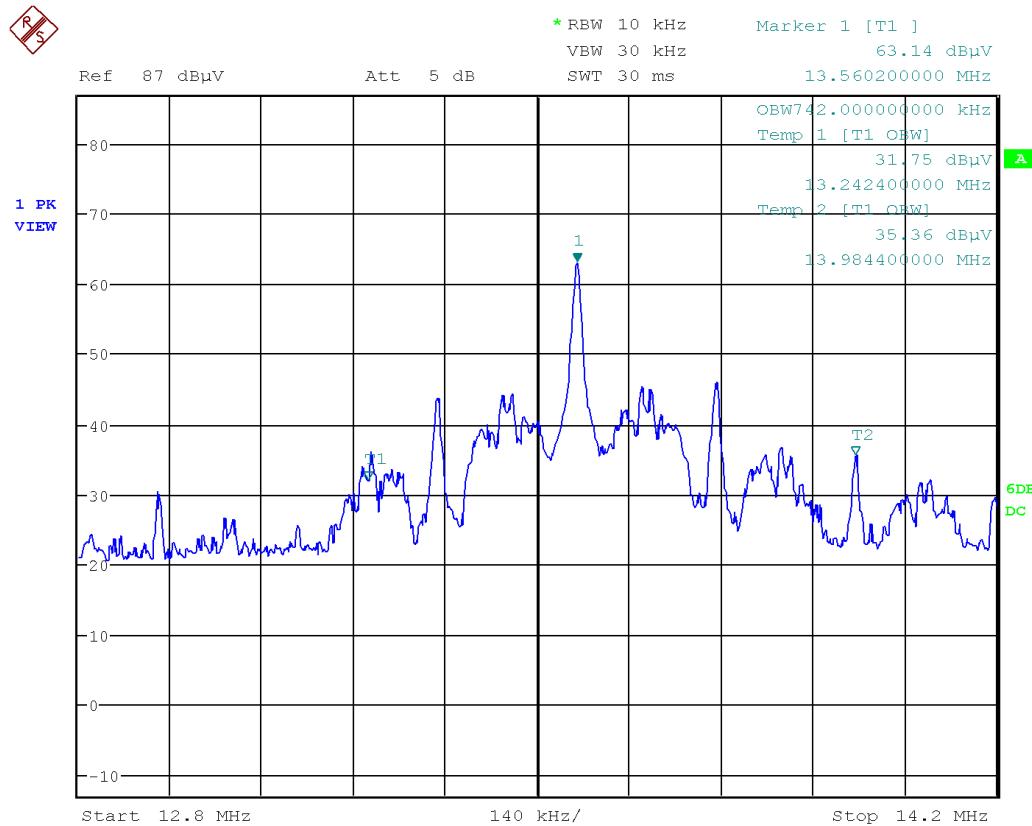

See photo exhibits for photos showing the test set-up.

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Test Equipment List

Equipment	Model No.	Manufacturer	Last Calibration / Verification Date	Next Calibration / Verification Date	Asset #
Spectrum Analyzer	ESR 26	Rohde & Schwarz	Mar. 6, 2020	Mar. 6, 2022	GEMC 341
Loop Antenna 150 kHz – 30 MHz	EM 6872	Electro-Metrics	Feb 15, 2019	Feb 15, 2021	GEMC 71
Pre-Amp 9 kHz – 1 GHz	CPA9230	Chase	May 22, 2020	May 22, 2022	GEMC 301
RF Cable 10m	LMR-400-10M-50Ω-MN-MN	LexTec	NCR	NCR	GEMC 27
RF Cable 3m	HP305S	Semflex	NCR	NCR	GEMC 310

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

Appendix A – EUT Summary

Client	Excelitas Canada Inc.	 Canada
Product	OmniCure S2000 Elite	
Standard(s)	RSS 210 Annex B.6, Issue 10:2019 FCC Part 15 Subpart 15.225:2019	

For further details for filing purposes, refer to filing package.

General EUT Description

Client Details	
Organization / Address	Excelitas Canada Inc. 2260 Argentia Road Mississauga, Ontario Canada, L5N 6H7
Contact	Daoud Attayi
Phone	1-905-821-3201
Email	daoud.attayi@excelitas.com
EUT (Equipment Under Test) Details	
EUT Name	Omnicure
EUT Model	S2000 Elite
EUT is powered using	Mains
Input voltage (V)	100-240 V, 50/60 Hz
Rated input current (A)	3.5/2.0 A
Frequency range(s)	NFC: 13.56 MHz
Transmits RF energy?	NFC transceiver
Basic EUT functionality description	Lamp Spot UV Curing System used for precision adhesive curing of medical devices, electronics and optoelectronics with an integrated NFC Card Reader/Writer and internal antenna.
Modes of operation	NFC: 13.56 MHz, ASK modulation.
Frequency of all clocks present in EUT	133 MHz, 24 MHz, 24 MHz, 50.0 MHz, 32.7680 kHz
I/O connectors & cable description	RJ45 Ethernet, USB Type B, Analog jack (footswitch), PLC Connector (15 pin), Light Guide Port, Radiometer Calibration Port
Peripherals required to exercise EUT	All provided by manufacturer: - Asus model X555Q notebook PC with Asus W15-065N1A AC adapter. - EXFO R2000 UV/Visible Radiometer.
Dimensions of product (approx.)	L: 29cm, W: 14cm, H: 27cm

Note the EUT is considered to have been received the date of the commencement of the first test, unless otherwise stated.

For close-up pictures of the EUT, see photo exhibits.