


# Appendix D

## Photographs

|                                          |
|------------------------------------------|
| 1. SAR measurement System                |
| 2. Photographs of Tissue Simulate Liquid |
| 3. Photographs of EUT test position      |
| 4. EUT Constructional Details            |

## 1. SAR measurement System

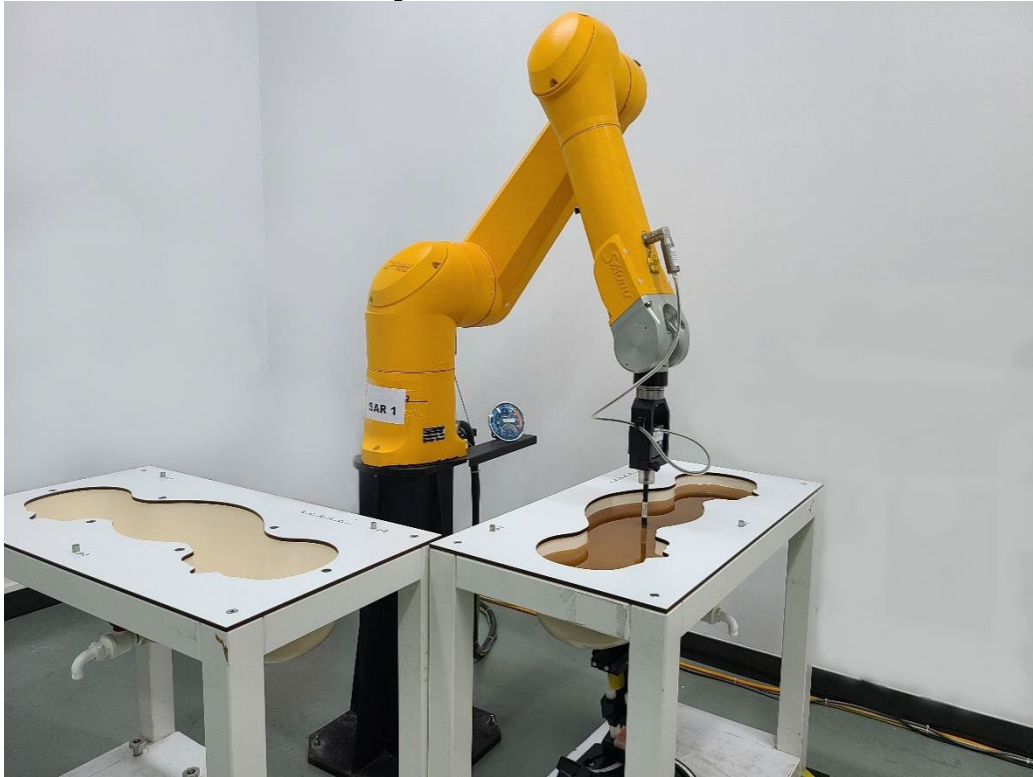

## 2. Photographs of Tissue Simulate Liquid

| Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz                                                                                                                                                                                                                                                                                                                                | NA |
|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----|
|  A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the 10 cm mark visible. The container has a blue outer rim and a white inner lining. The liquid level is approximately 8 cm high. | NA |

### 3. Photographs of EUT test position

Photo 2: Front Side 10mm



Photo 3: Back Side 10mm



Photo 4: Left Side 10mm




Photo 5: Right Side 10mm



Photo 6: Top Side 10mm



Photo 7: Bottom Side 10mm

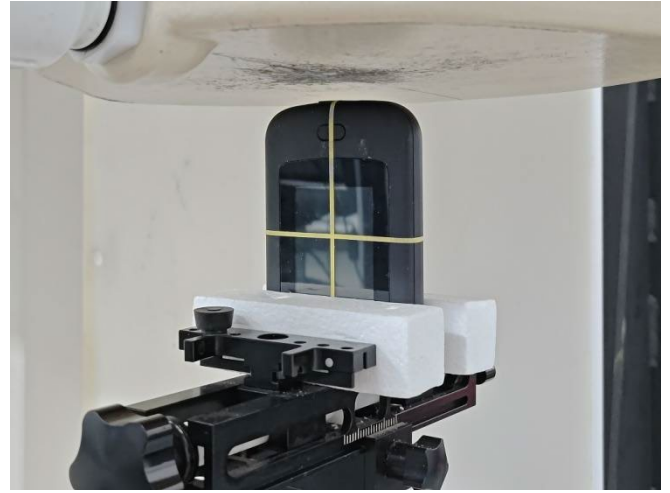

#### 4. EUT Constructional Details

