






Band4_20MHz_QPSK_20300_1RB#0

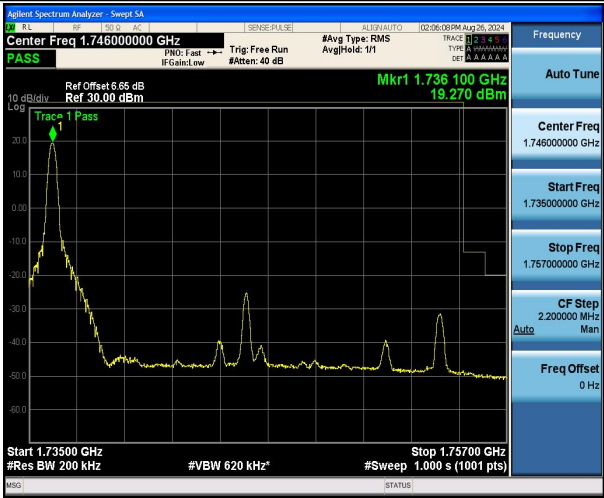

Band4_20MHz_16QAM_20300_1RB#0

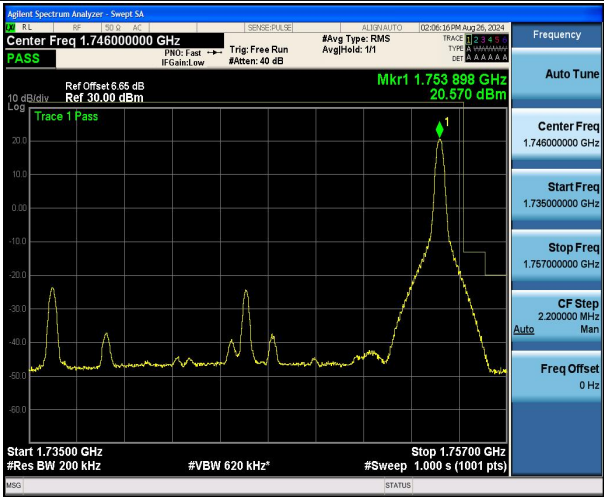

Band4_20MHz_QPSK_20300_1RB#99

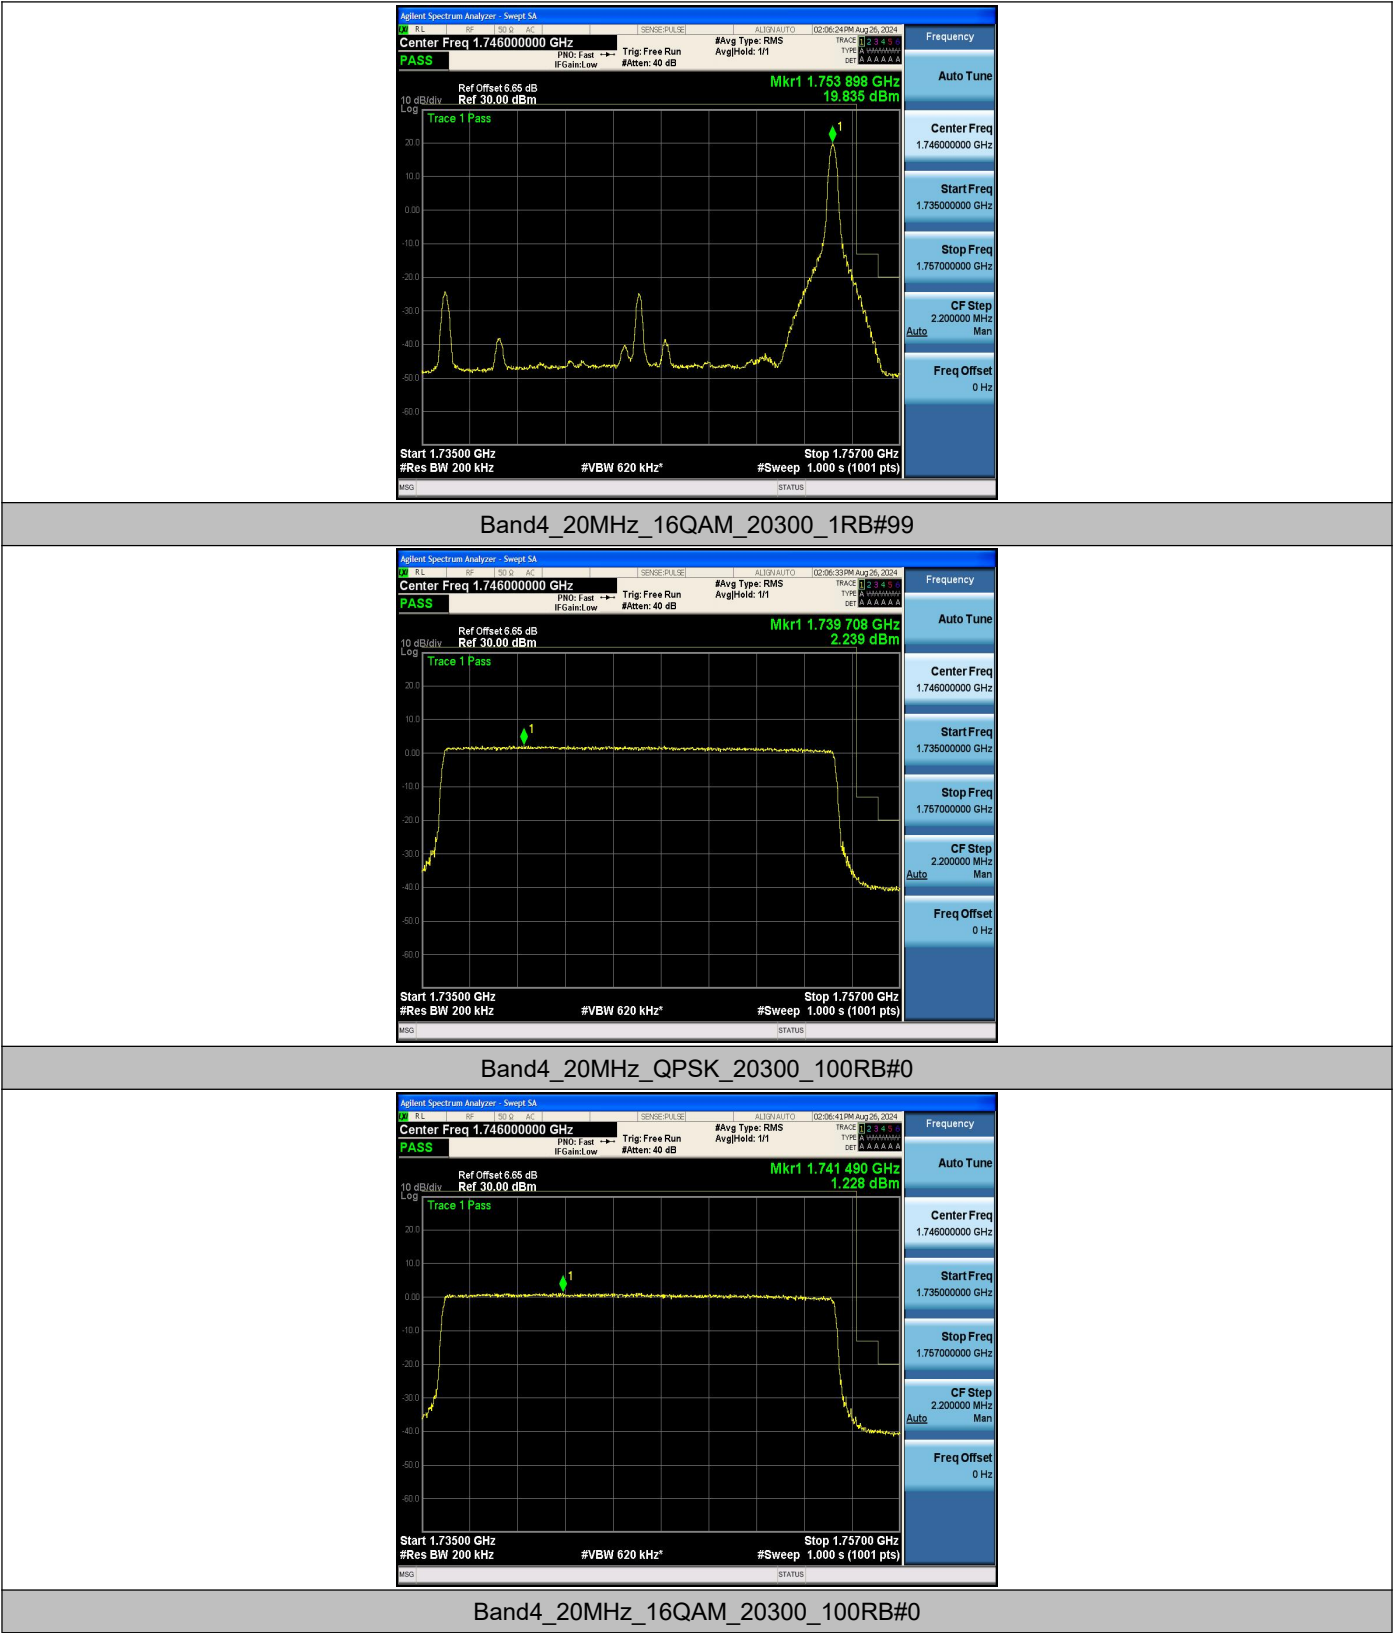

Agilent Spectrum Analyzer - Sweep SA

Center Freq 1.746000000 GHz

Ref Offset 6.65 dB

Ref 30.00 dBm

Trace 1 Pass

Start 1.73500 GHz

Stop 1.75700 GHz

Res BW 200 kHz

VBW 620 kHz

Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq

1.746000000 GHz

Start Freq

1.735000000 GHz

Stop Freq

1.757000000 GHz

CF Step

2.200000 MHz

Auto

Man

Freq Offset

0 Hz

10 dB/div

Log

Mkr1 1.741 490 GHz

1.228 dBm

MSG

STATUS

Band4_20MHz_16QAM_20300_100RB#0




Band5_1.4MHz_QPSK_20407_1RB#0



Band5_1.4MHz_16QAM_20407_1RB#0



Band5_1.4MHz_QPSK_20407_1RB#5

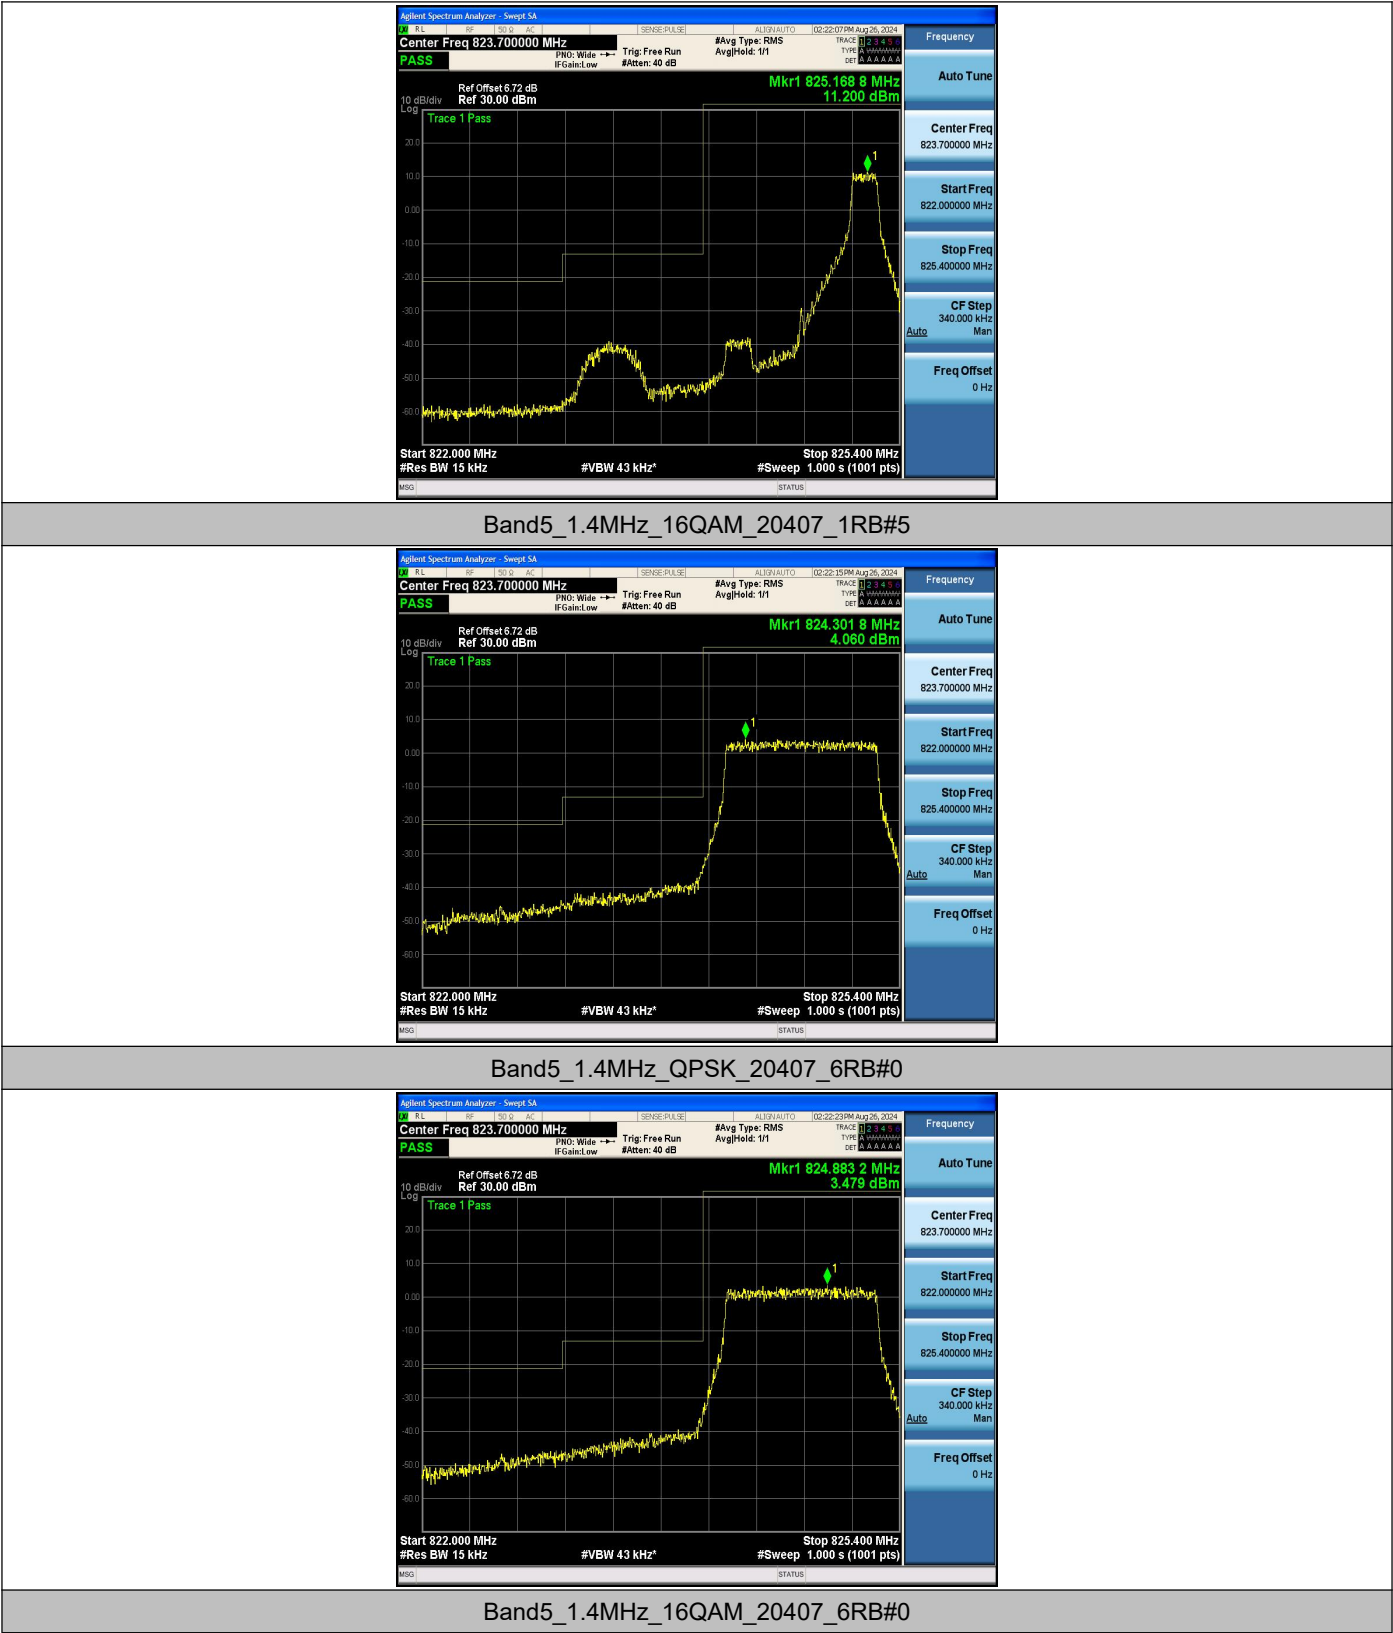

Agilent Spectrum Analyzer - Sweep SA

Center Freq 823.700000 MHz

PASS

Ref Offset 6.72 dB

Ref 30.00 dBm

Trace 1 Pass

Start 822.000 MHz

Res BW 15 kHz

VBW 43 kHz

Stop 825.400 MHz

Sweep 1.000 s (1001 pts)

Mkr1 824.883 2 MHz

3.479 dBm

Frequency

Auto Tune

Center Freq

823.700000 MHz

Start Freq

822.000000 MHz

Stop Freq

825.400000 MHz

CF Step

340.000 kHz


Auto

Man

Freq Offset

0 Hz

Band5_1.4MHz_16QAM_20407_6RB#0

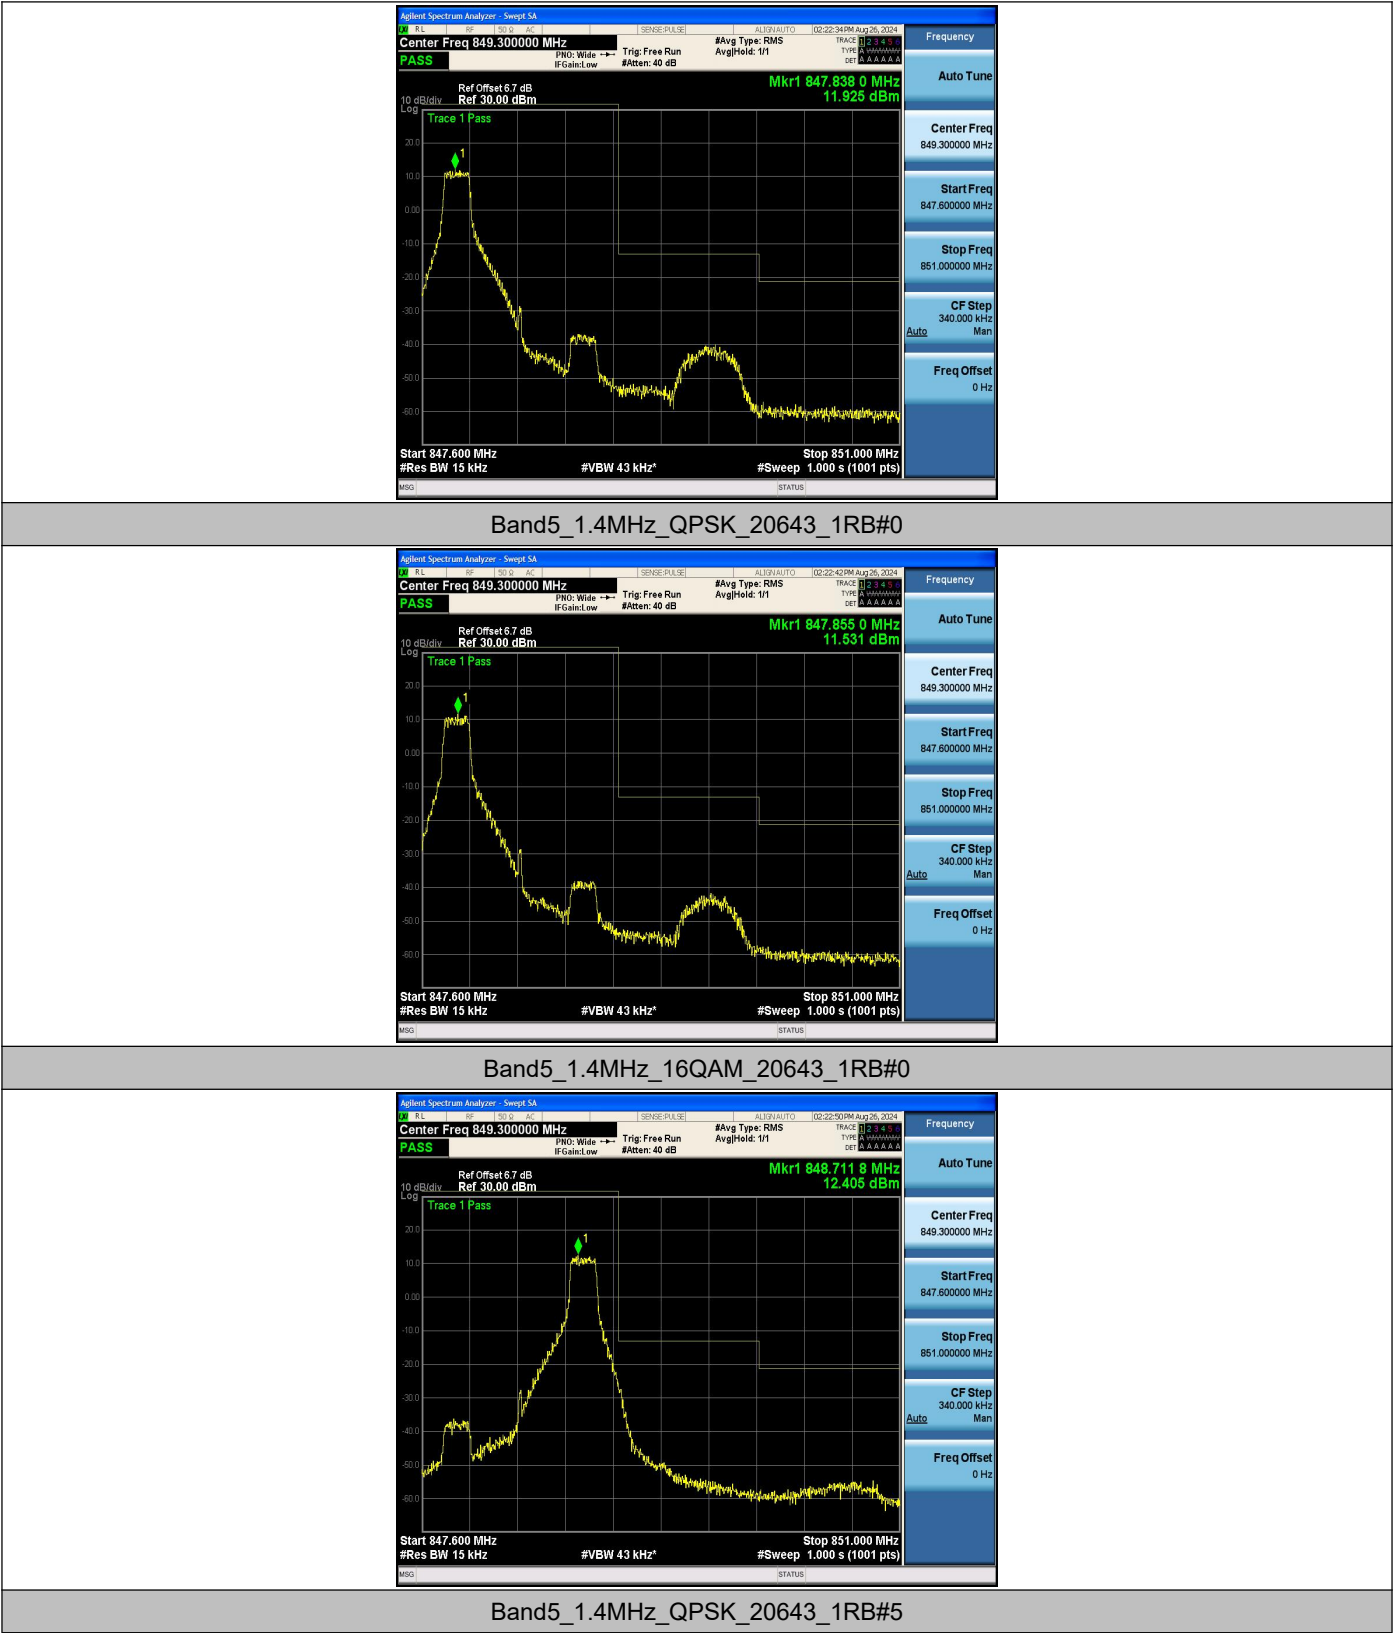

Band5_1.4MHz_16QAM_20643_1RB#0

Agilent Spectrum Analyzer - Swept SA

Center Freq 849.300000 MHz

PASS

Ref Offset 6.7 dB

Ref 30.00 dBm

Trace 1 Pass

Start 847.600 MHz

#Res BW 15 kHz

#VBW 43 kHz

Stop 851.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq

849.300000 MHz

Start Freq

847.600000 MHz

Stop Freq

851.000000 MHz

CF Step

340.000 kHz

Auto

Man


Freq Offset

0 Hz

Mkr1 848.711 8 MHz

12.405 dBm

Band5_1.4MHz_QPSK_20643_1RB#5

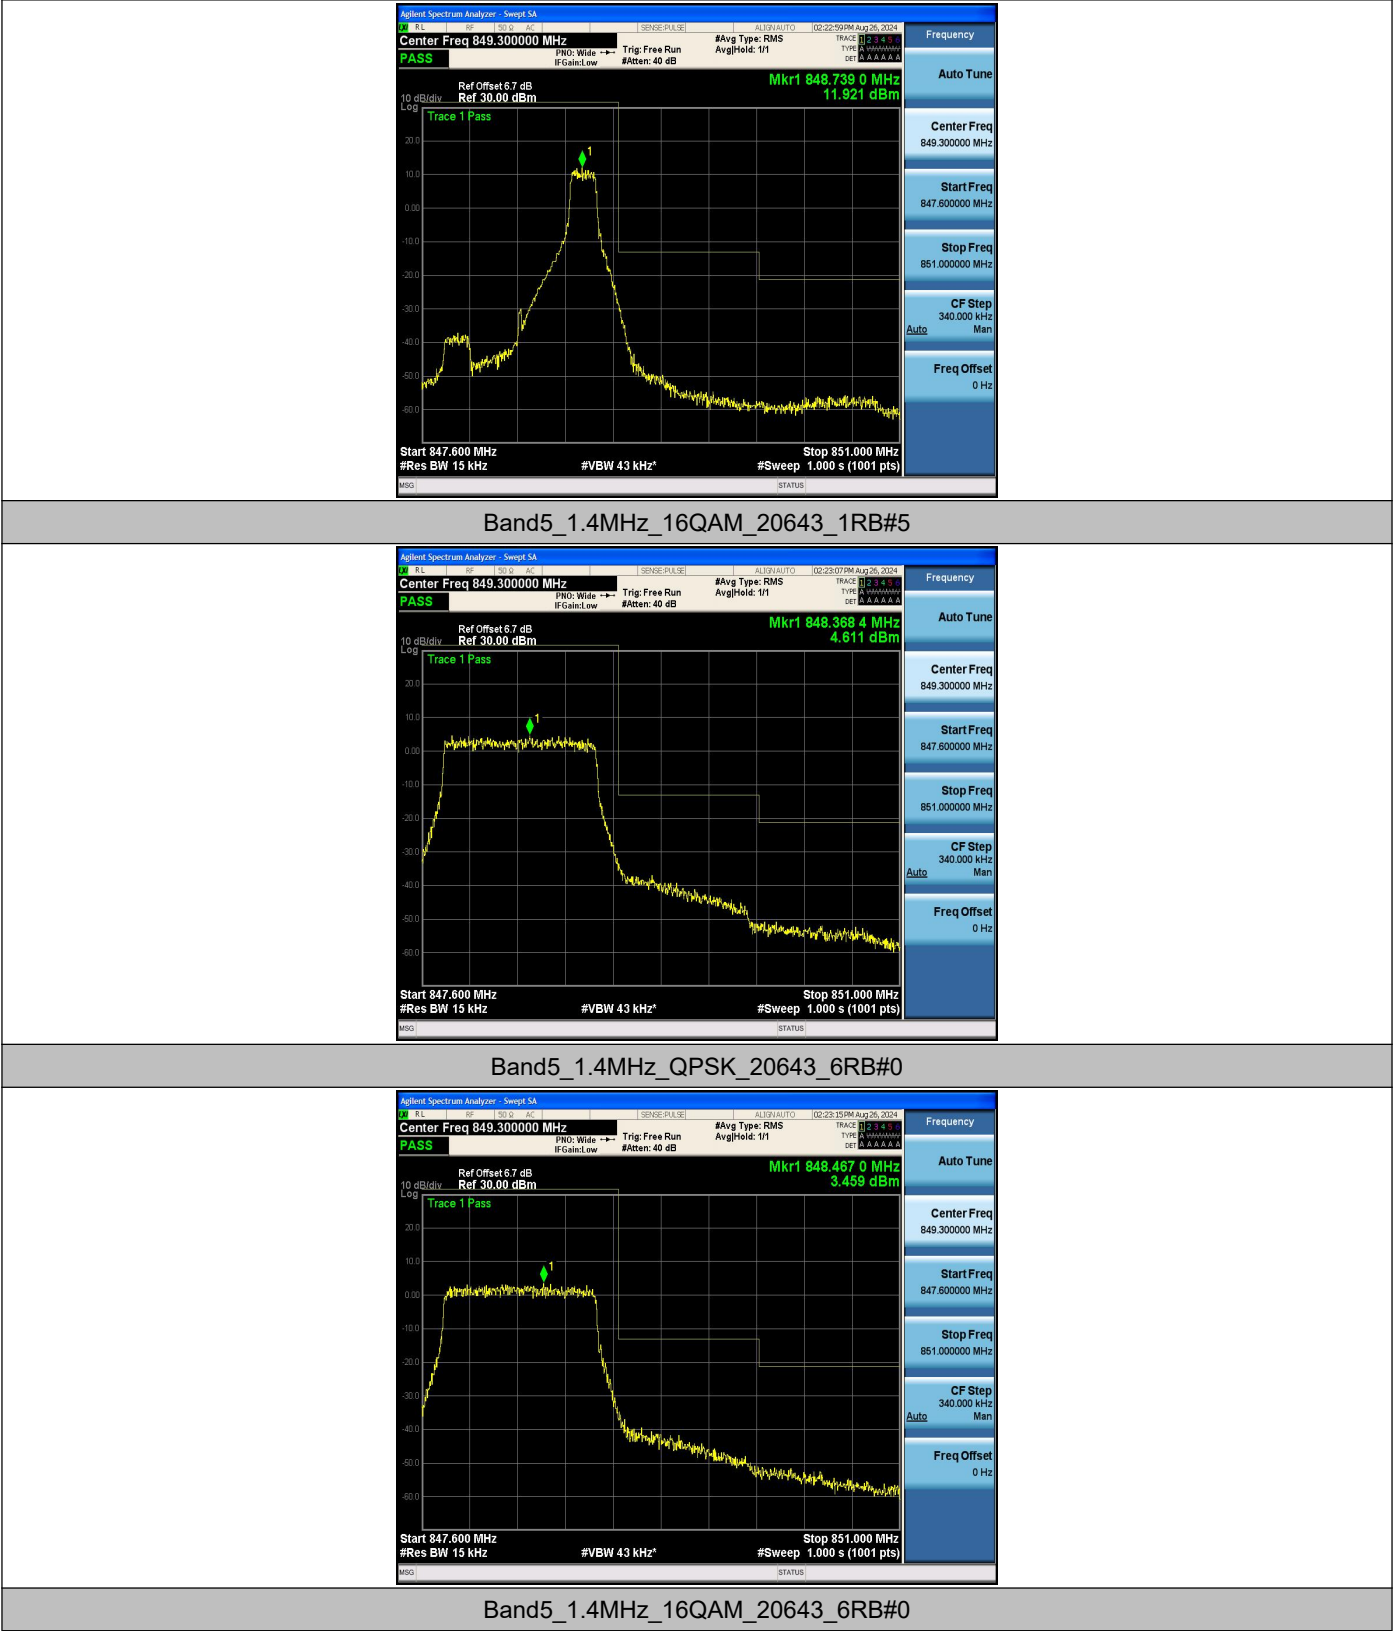

Agilent Spectrum Analyzer - Sweep SA

Center Freq 849.300000 MHz

PASS

Ref Offset 6.7 dB

Ref 30.00 dBm

Trace 1 Pass

Start 847.600 MHz

#Res BW 15 kHz

#VBW 43 kHz

Stop 851.000 MHz

#Sweep 1.000 s (1001 pts)

Mkr1 848.467 0 MHz

3.459 dBm

Frequency

Auto Tune

Center Freq

849.300000 MHz

Start Freq

847.600000 MHz

Stop Freq

851.000000 MHz

CF Step

340.000 kHz


Auto

Man


Freq Offset

0 Hz

Band5_1.4MHz_16QAM_20643_6RB#0

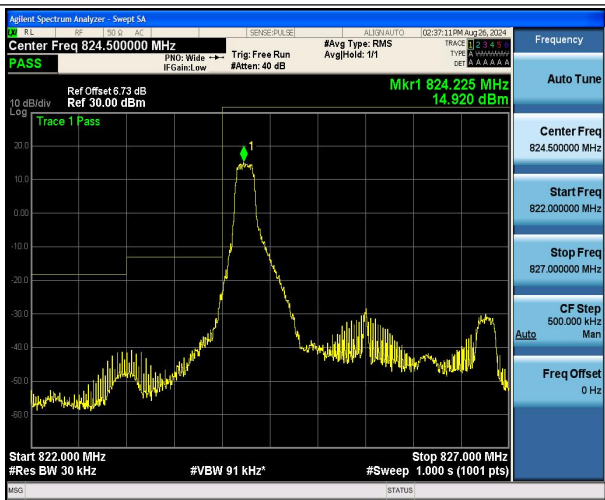

Band5_3MHz_QPSK_20415_1RB#0

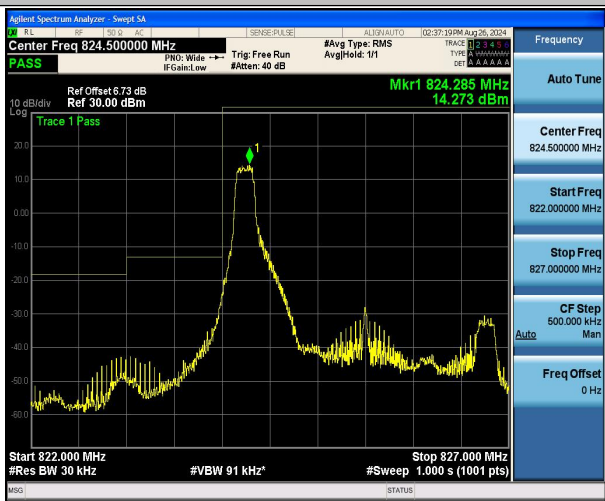


Band5_3MHz_16QAM_20415_1RB#0



Band5_3MHz_QPSK_20415_1RB#14




Band5_3MHz_16QAM_20415_1RB#14

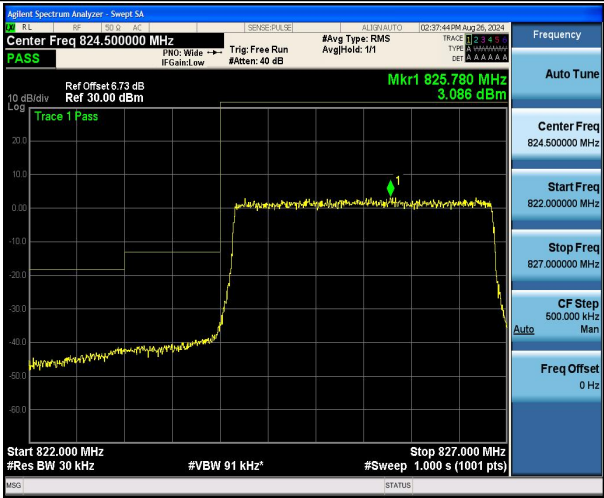

Band5_3MHz_QPSK_20415_15RB#0



Band5_3MHz_16QAM_20415_15RB#0

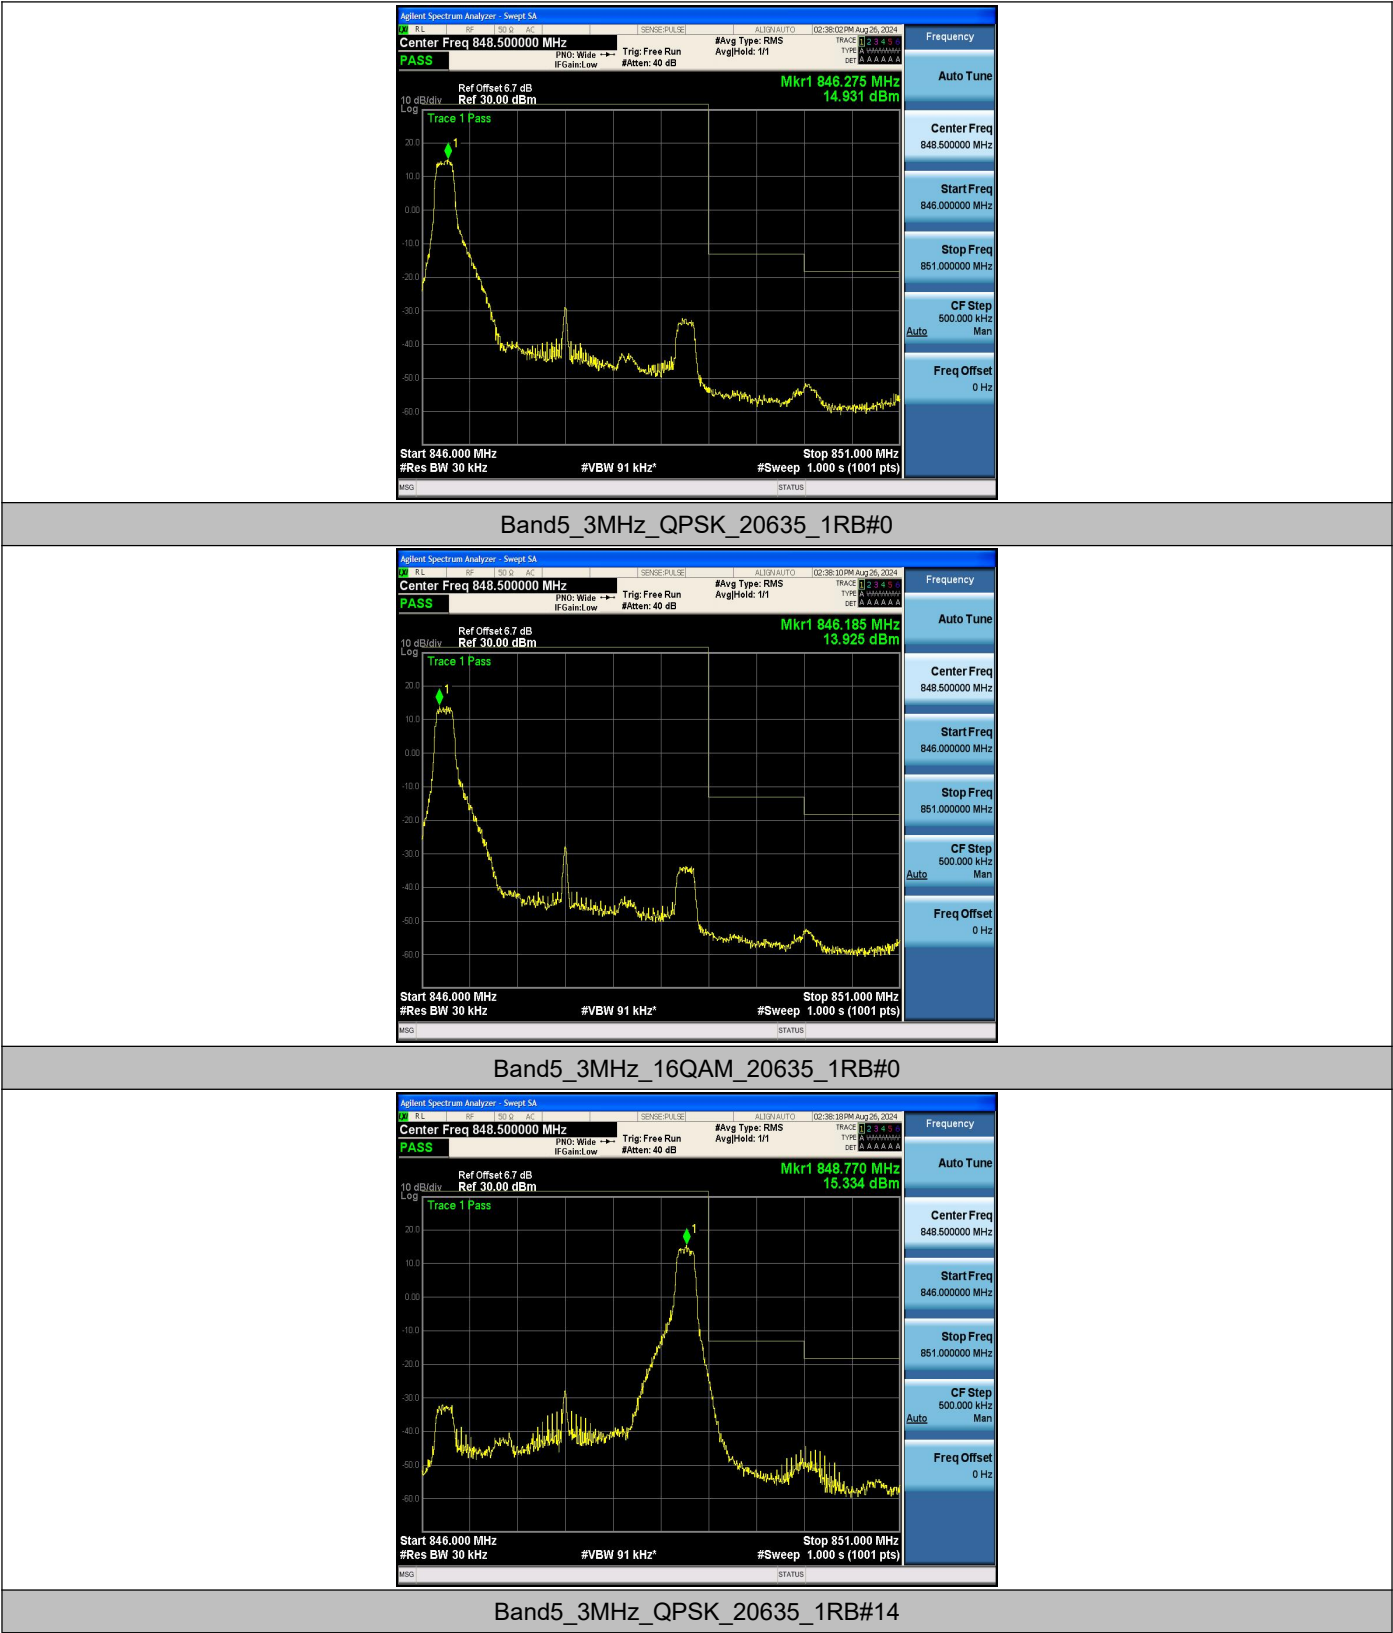

Band5_3MHz_16QAM_20635_1RB#0

Agilent Spectrum Analyzer - Sweep SA

Center Freq 848.500000 MHz

PASS

Ref Offset 6.7 dB

Ref 30.00 dBm

Trace 1 Pass

Start 846.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 851.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 848.500000 MHz

Start Freq 846.000000 MHz

Stop Freq 851.000000 MHz


CF Step 500.000 kHz

Auto

Freq Offset 0 Hz

Mkr1 848.770 MHz

15.334 dBm

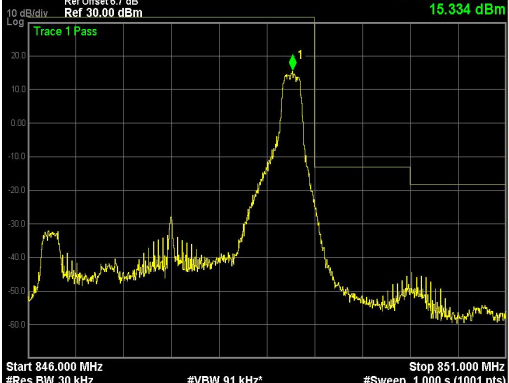

Band5_3MHz_QPSK_20635_1RB#14




Band5_3MHz_16QAM_20635_1RB#14



Band5_3MHz_QPSK_20635_15RB#0



Band5_3MHz_16QAM_20635_15RB#0

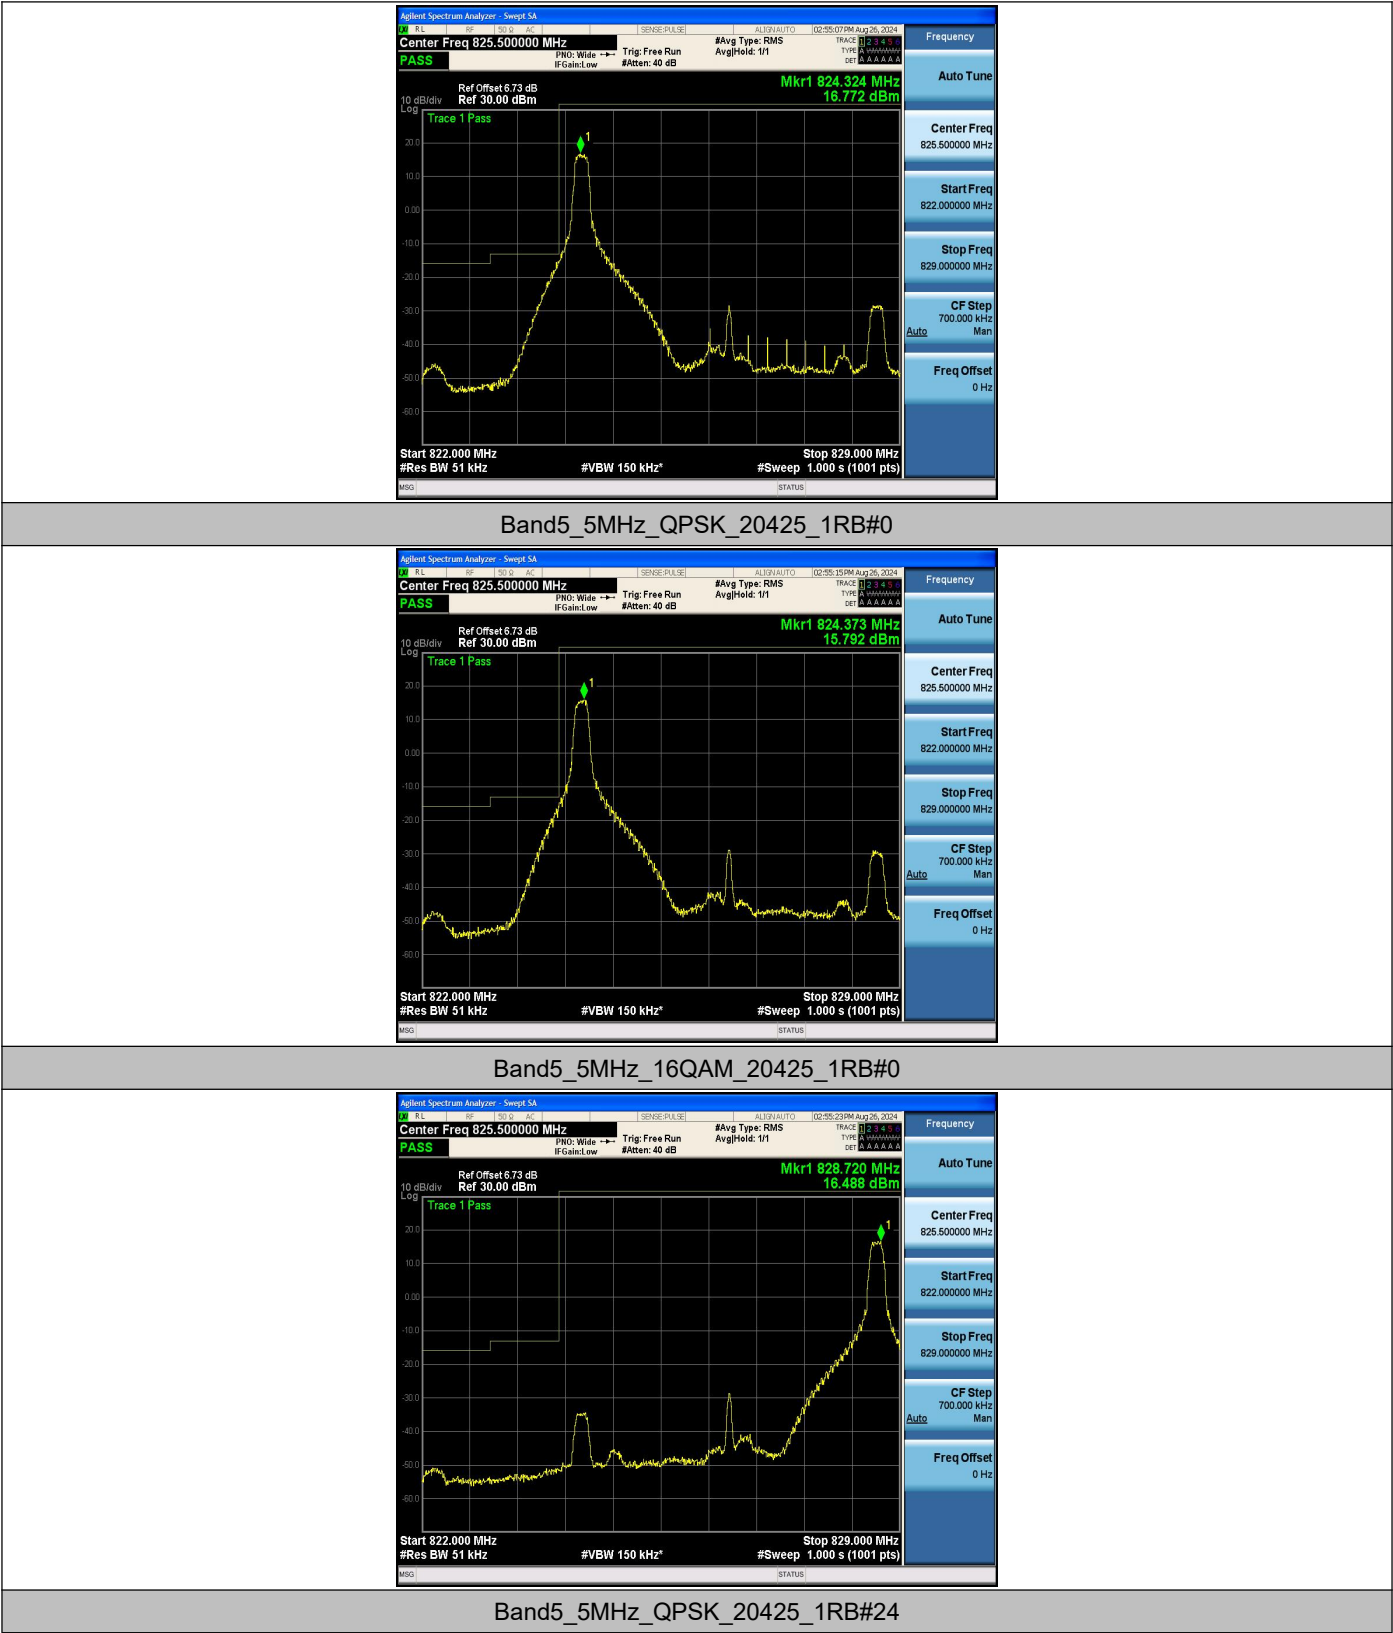



Band5_5MHz_16QAM_20425_1RB#24



Band5_5MHz_QPSK_20425_25RB#0



Band5_5MHz_16QAM_20425_25RB#0




Band5_5MHz_QPSK_20625_1RB#0



Band5_5MHz_16QAM_20625_1RB#0




Band5_5MHz_QPSK_20625_1RB#24

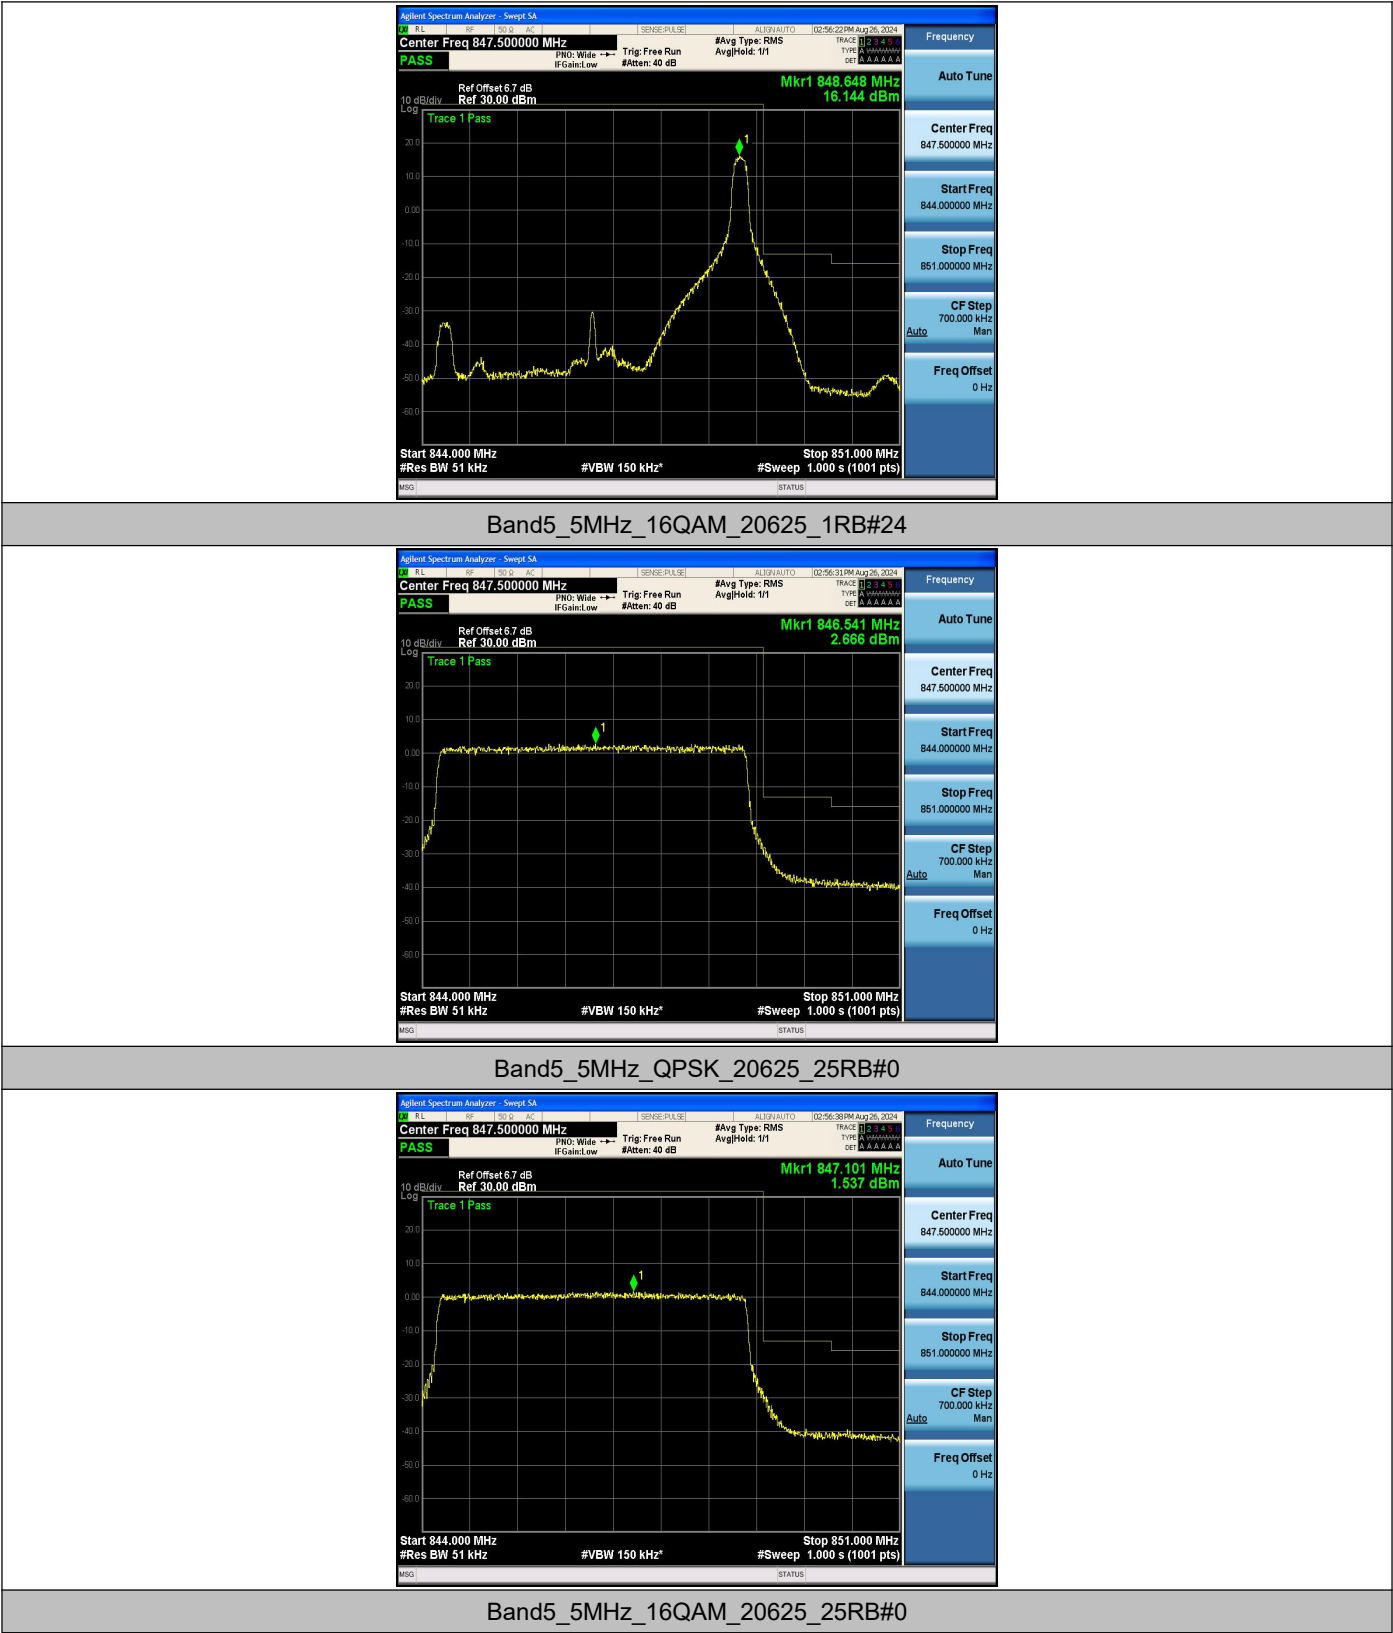



Band5_10MHz_QPSK_20450_1RB#0

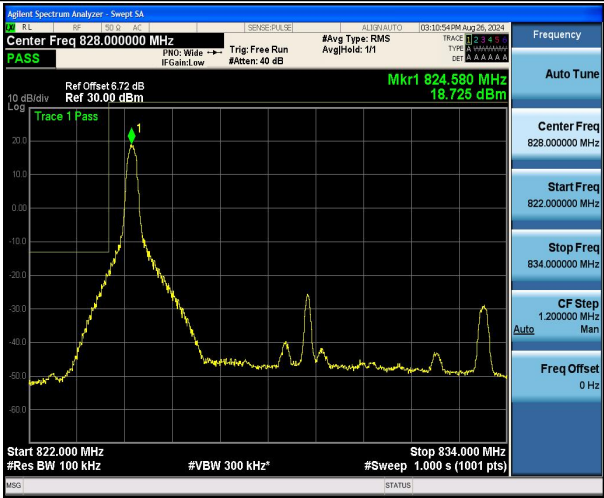

Band5_10MHz_16QAM_20450_1RB#0



Band5_10MHz_QPSK_20450_1RB#49