





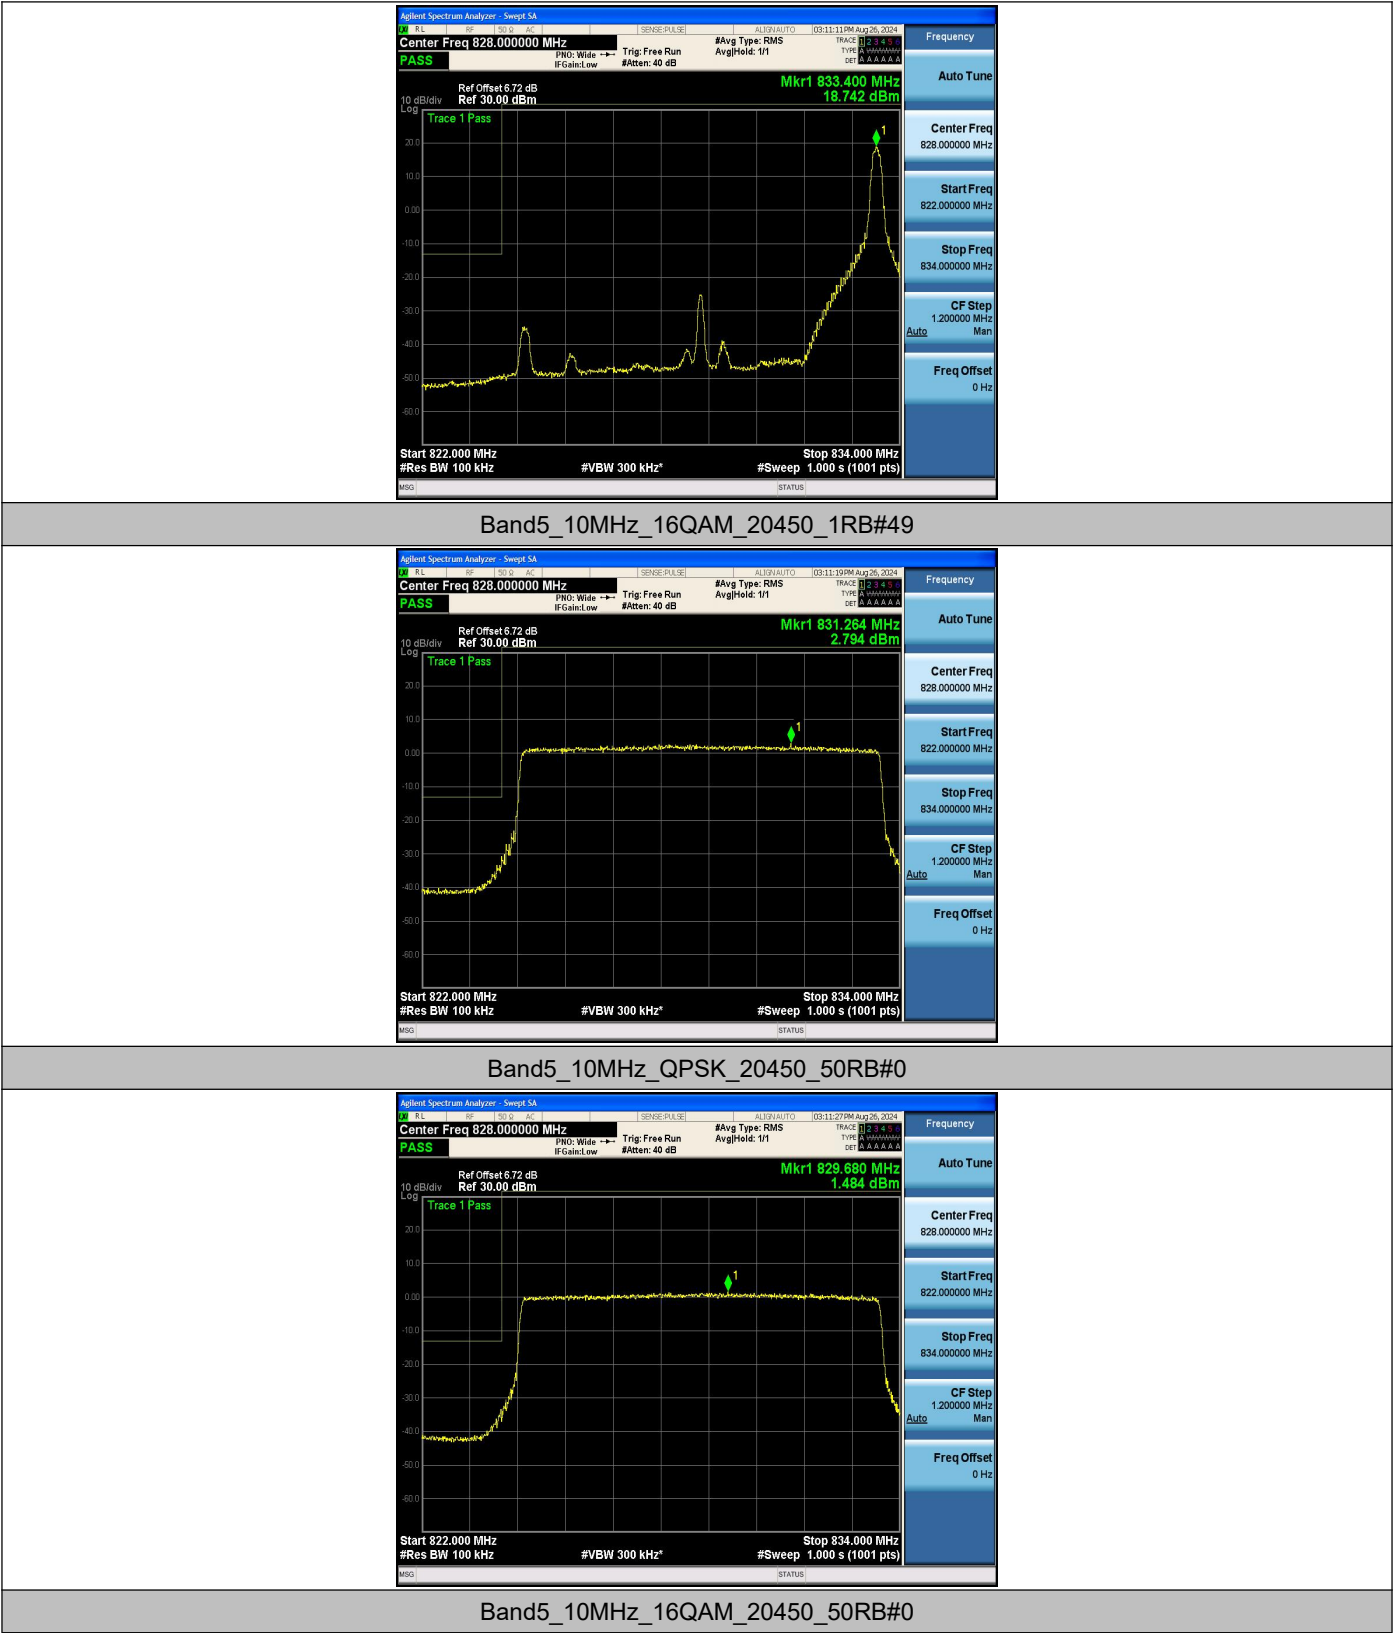


Band5_10MHz_QPSK_20600_1RB#0

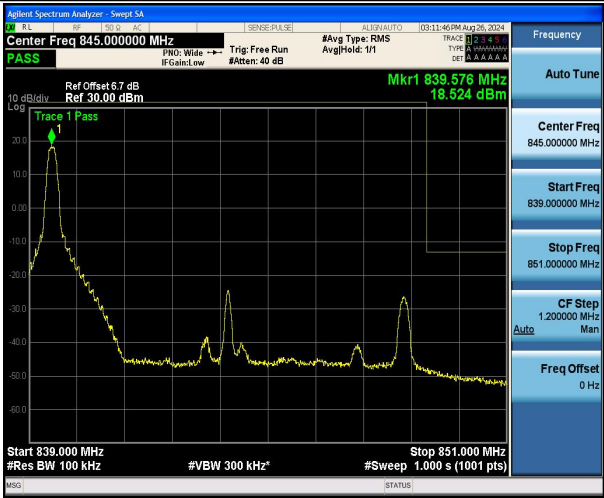

Band5_10MHz_16QAM_20600_1RB#0



Band5_10MHz_QPSK_20600_1RB#49

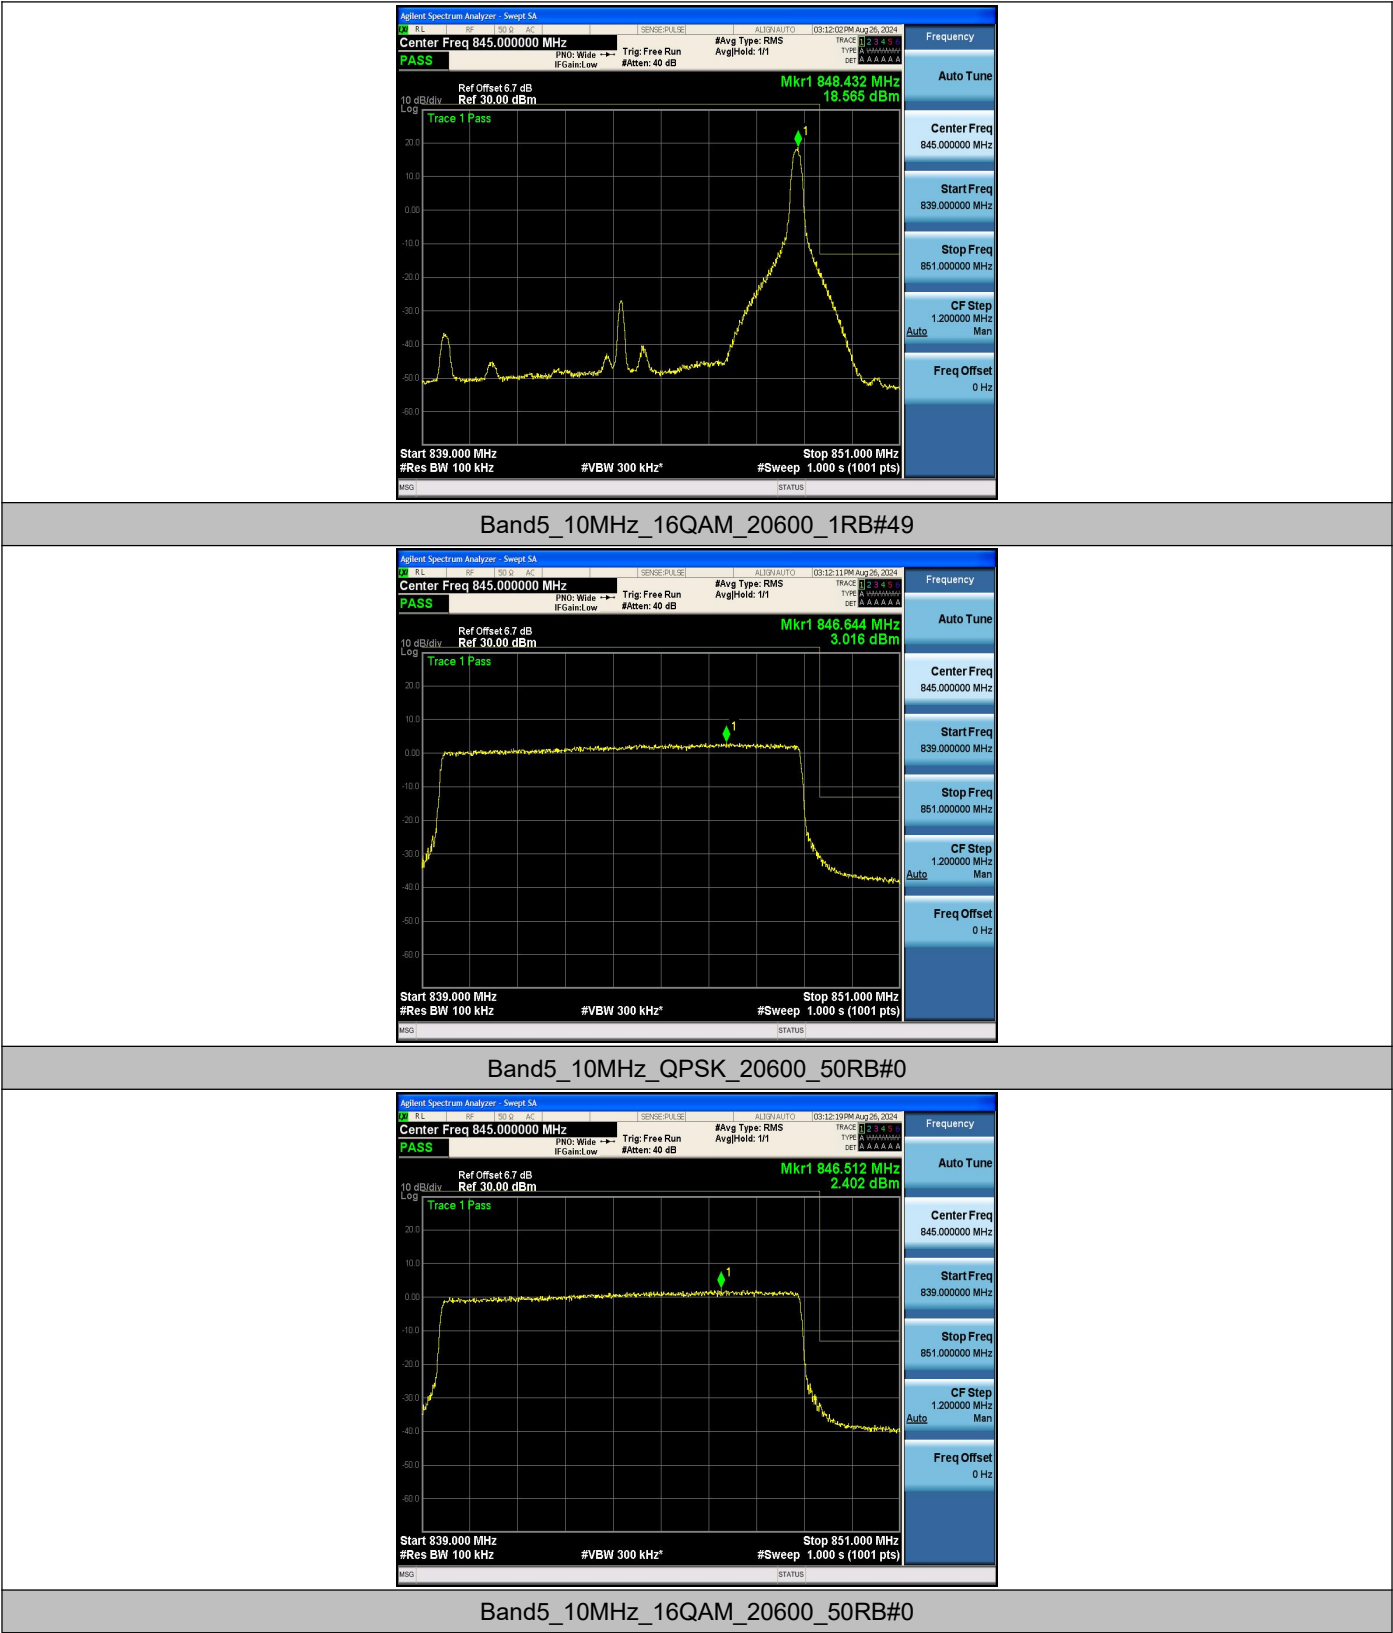

Agilent Spectrum Analyzer - Sweep SA

Center Freq 845.000000 MHz

PASS

Ref Offset 6.7 dB

Ref 30.00 dBm

Trace 1 Pass

Start 839.000 MHz

#Res BW 100 kHz

#VBW 300 kHz

#Sweep 1.000 s (1001 pts)

SENSE (PLA SE)

ALTO AUTO

03-12-10PM Aug 26, 2024

TRIG: Free Run

#Avg Type: RMS

Avg Hold: 1/1

TYPE A

DEF A

10 dB/div

Log

Mkr1 846.512 MHz

2.402 dBm

Auto Tune

Center Freq 845.000000 MHz

Start Freq 839.000000 MHz

Stop Freq 851.000000 MHz

CF Step 1.200000 MHz


Auto

Freq Offset 0 Hz

Band5_10MHz_16QAM_20600_50RB#0



Band7_5MHz_QPSK_20775_1RB#0

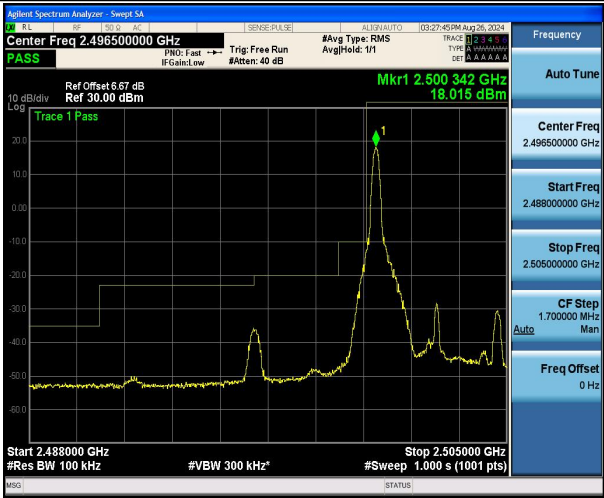

Band7_5MHz_16QAM_20775_1RB#0



Band7_5MHz_QPSK_20775_1RB#24




Band7_5MHz_16QAM_20775_1RB#24



Band7_5MHz_QPSK_20775_25RB#0



Band7_5MHz_16QAM_20775_25RB#0

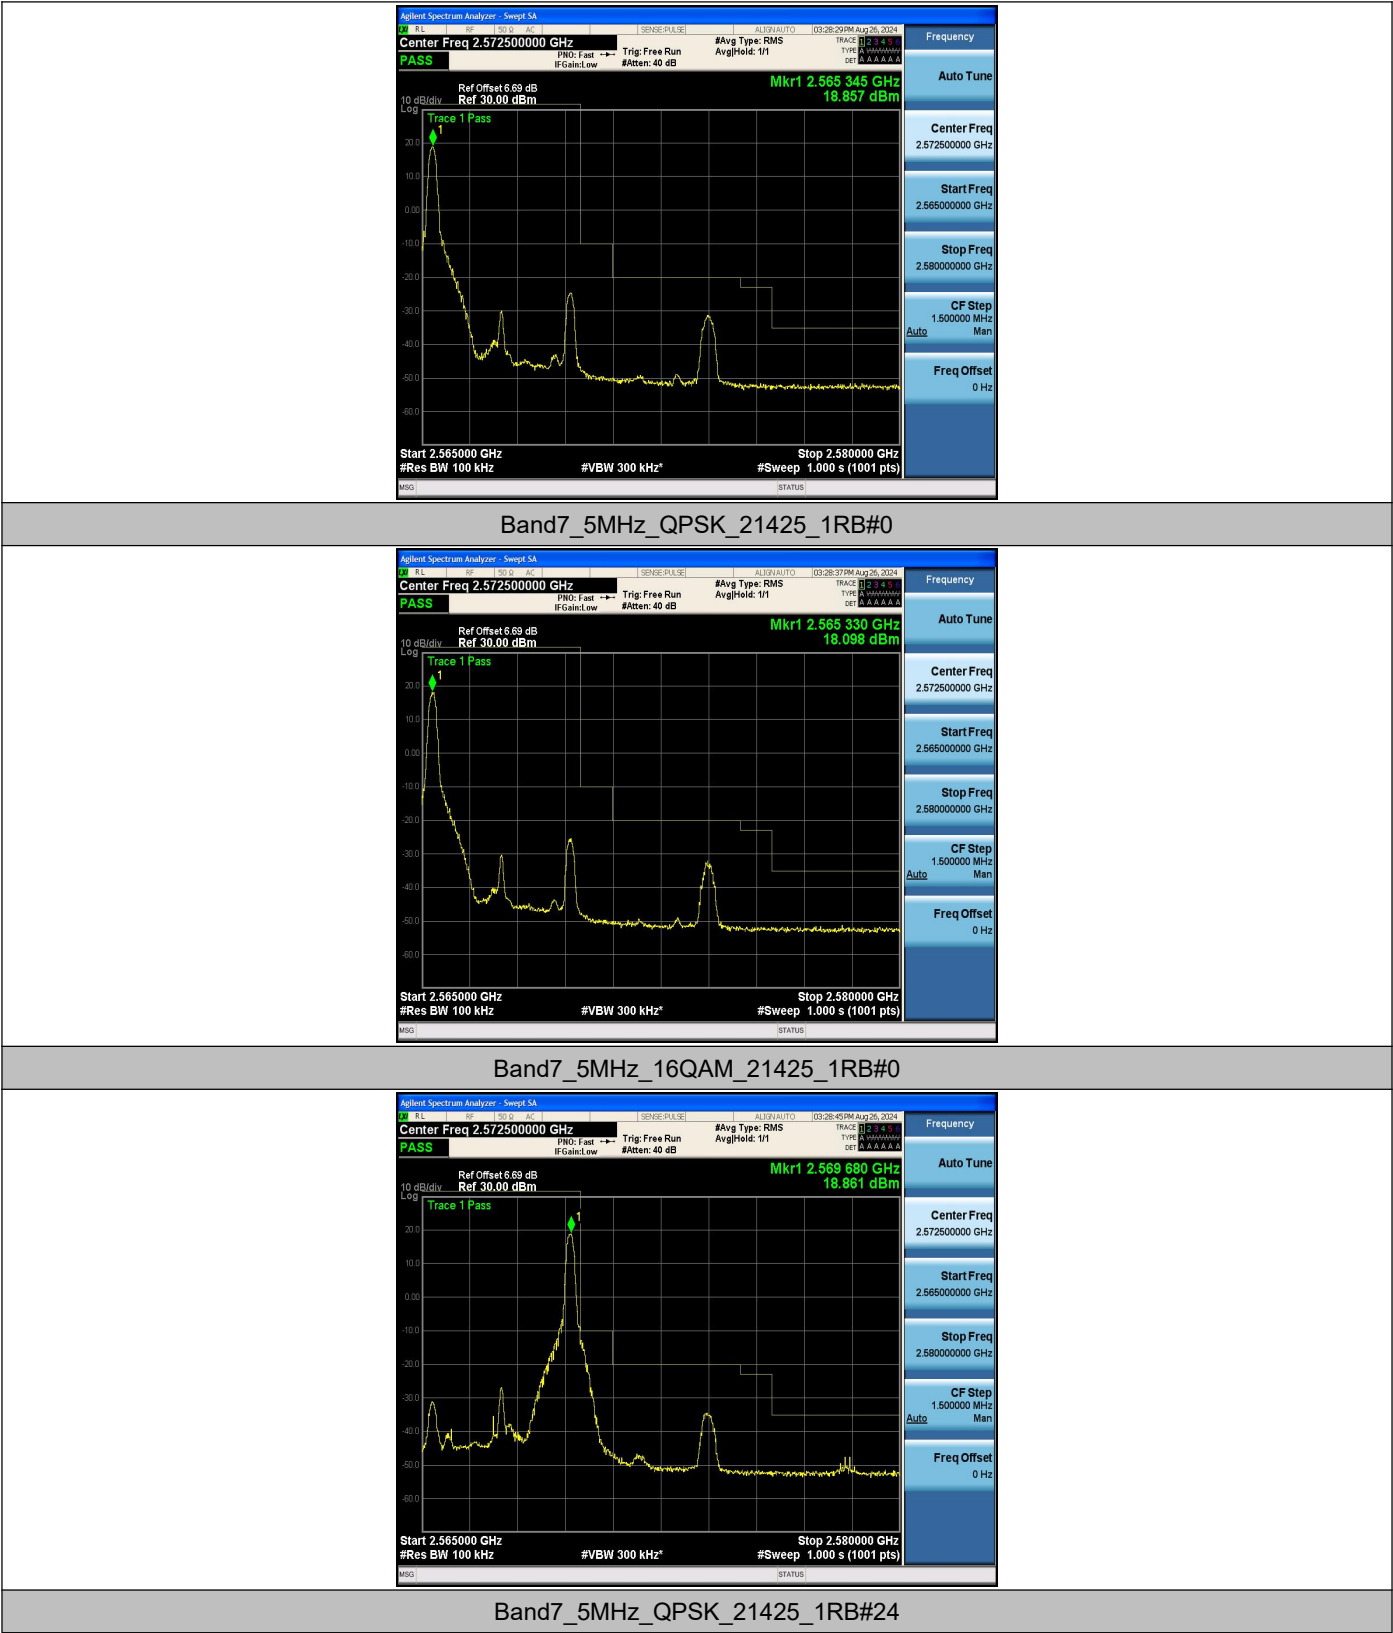

Band7_5MHz_16QAM_21425_1RB#0

Agilent Spectrum Analyzer - Sweep SA

Center Freq 2.572500000 GHz

PASS

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.565000 GHz

#Res BW 100 kHz

#VBW 300 kHz

Stop 2.580000 GHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq2.572500000 GHz

Start Freq2.565000000 GHz


Stop Freq2.580000000 GHz

CF Step1.500000 MHz

Auto

Freq Offset0 Hz

Band7_5MHz_QPSK_21425_1RB#24

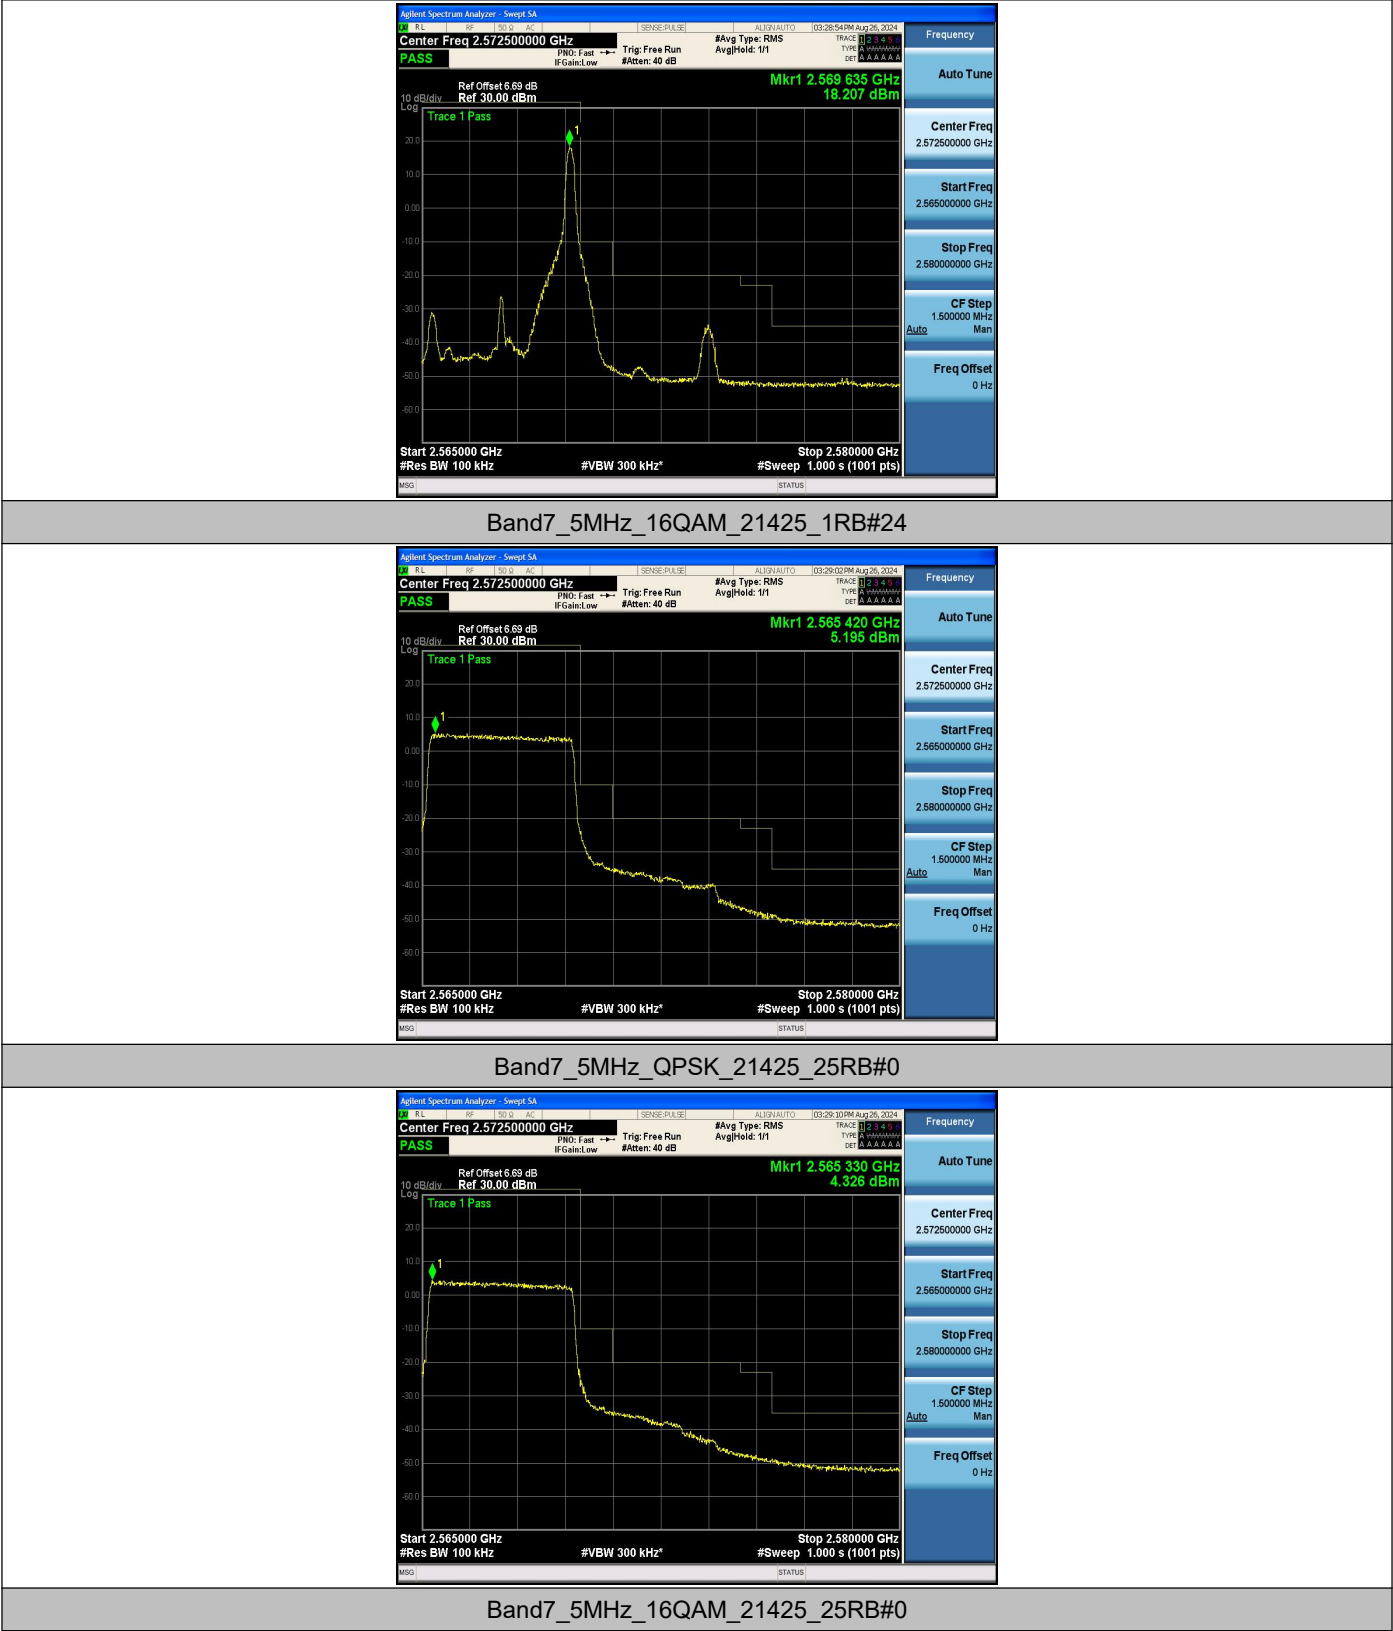

Agilent Spectrum Analyzer - Sweep SA

Center Freq 2.572500000 GHz

PASS

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.565000 GHz

#Res BW 100 kHz

#VBW 300 kHz

#Sweep 1.000 s (1001 pts)

SENSE (PLA SE)

ALTO AUTO

03-28-2024 Aug 26, 2024

TRACE 1 2 3 4 5

TYPE A W W W W W W W W

DET A A A A A A A A

Trig: Free Run

#Att: 40 dB

Avg Hold: 1/1

#Avg Type: RMS

Mkr1 2.565 330 GHz

4.326 dBm

Frequency

Auto Tune

Center Freq

2.572500000 GHz

Start Freq

2.565000000 GHz

Stop Freq

2.580000000 GHz

CF Step

1500000 MHz


Auto

Man


Freq Offset

0 Hz

Band7_5MHz_16QAM_21425_25RB#0

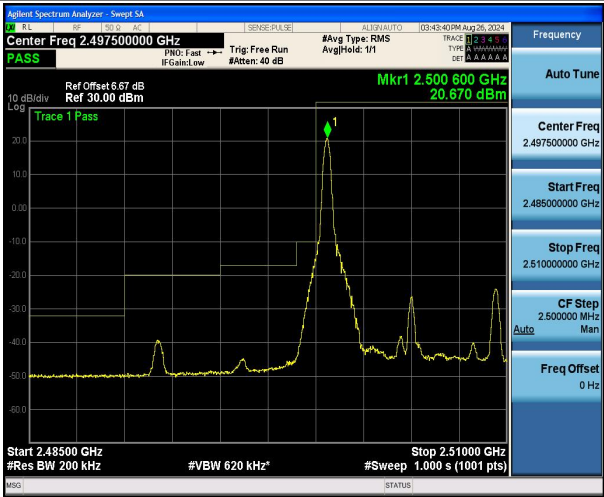


Band7_10MHz_QPSK_20800_1RB#0

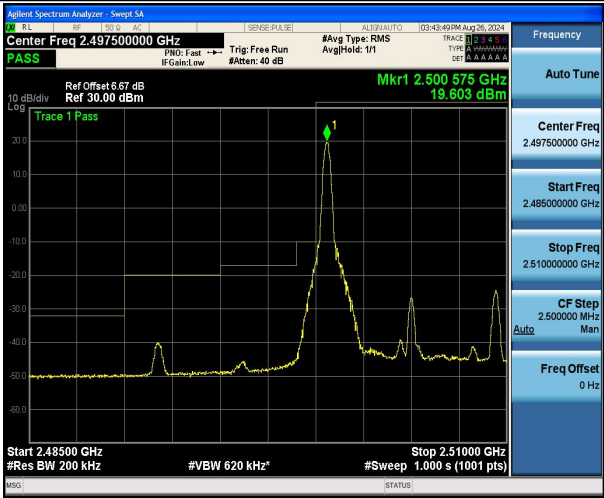



Band7_10MHz_16QAM_20800_1RB#0



Band7_10MHz_QPSK_20800_1RB#49

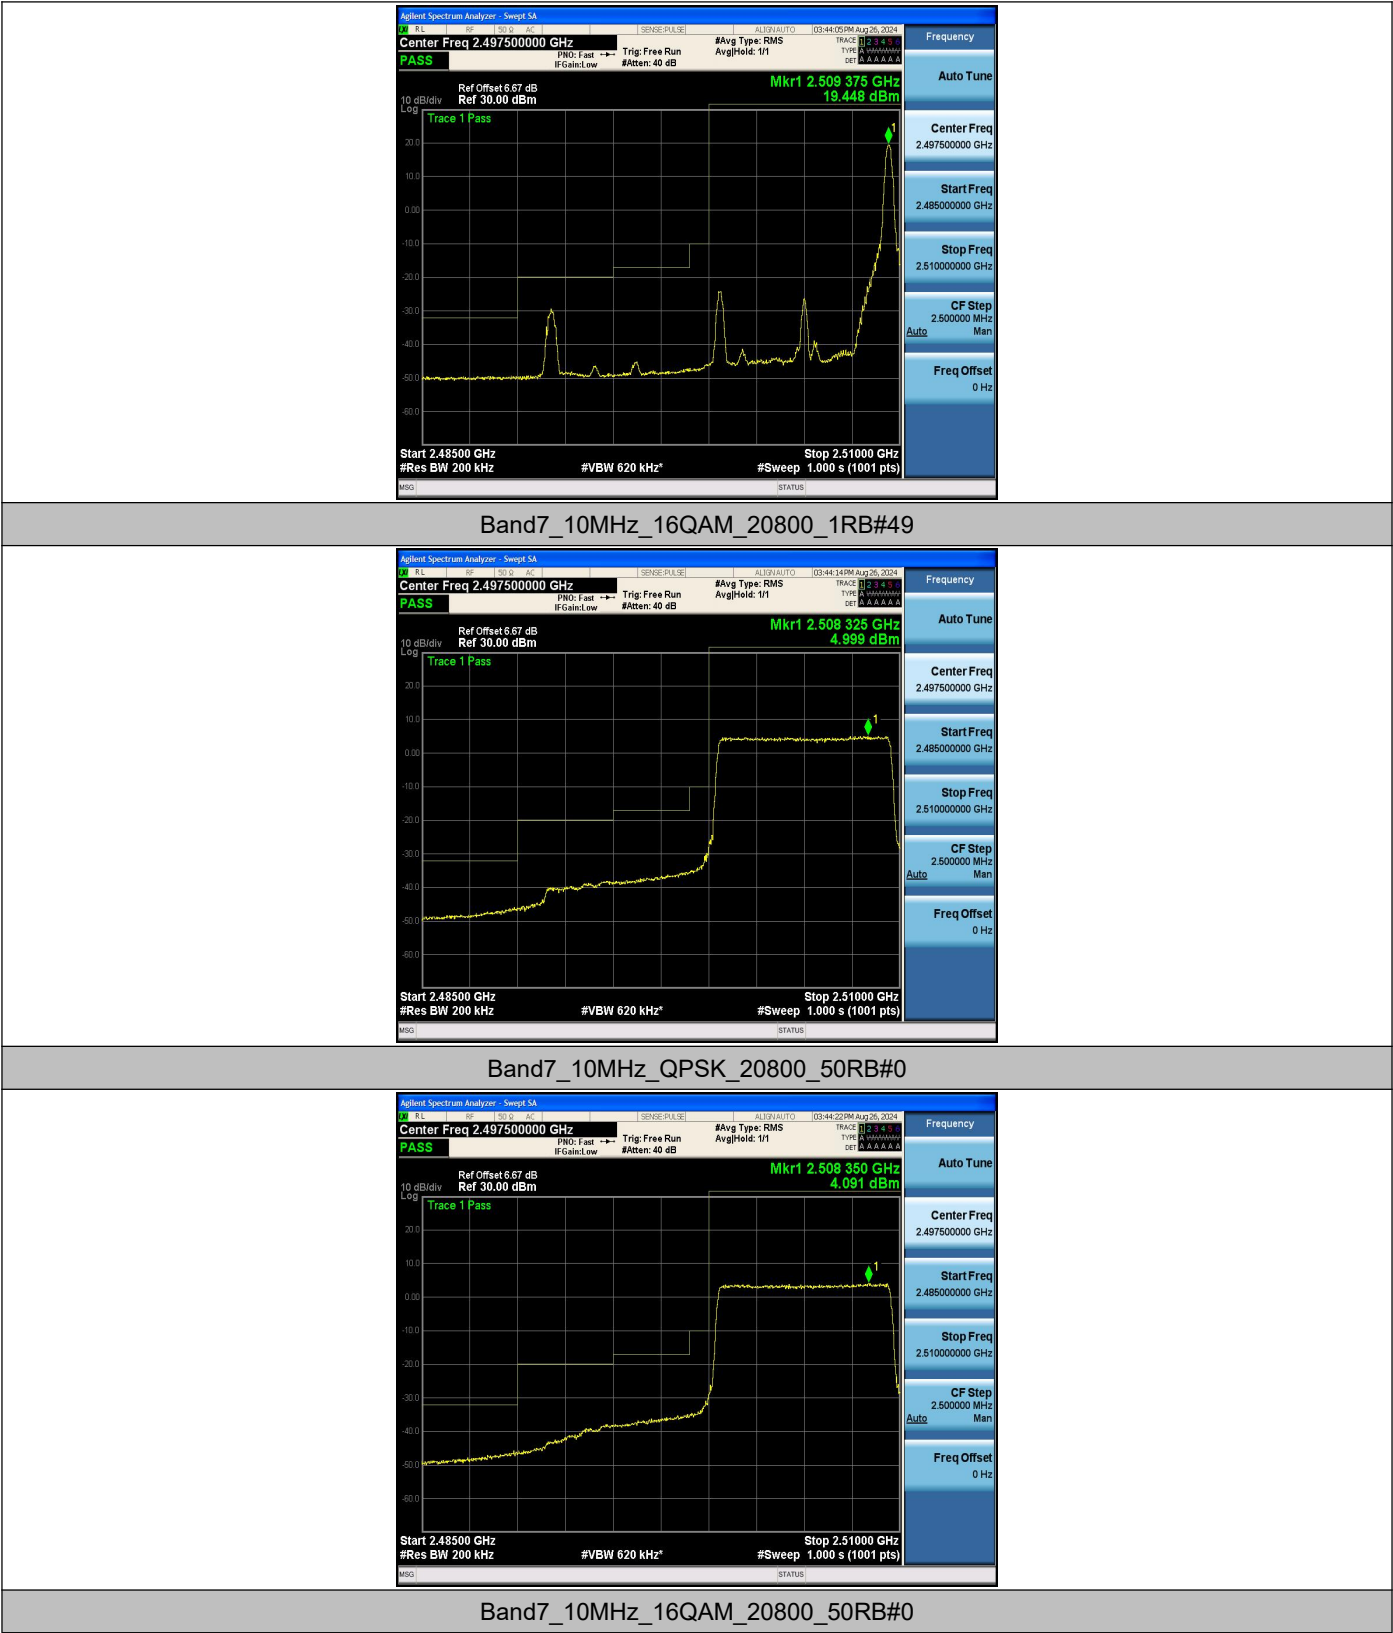

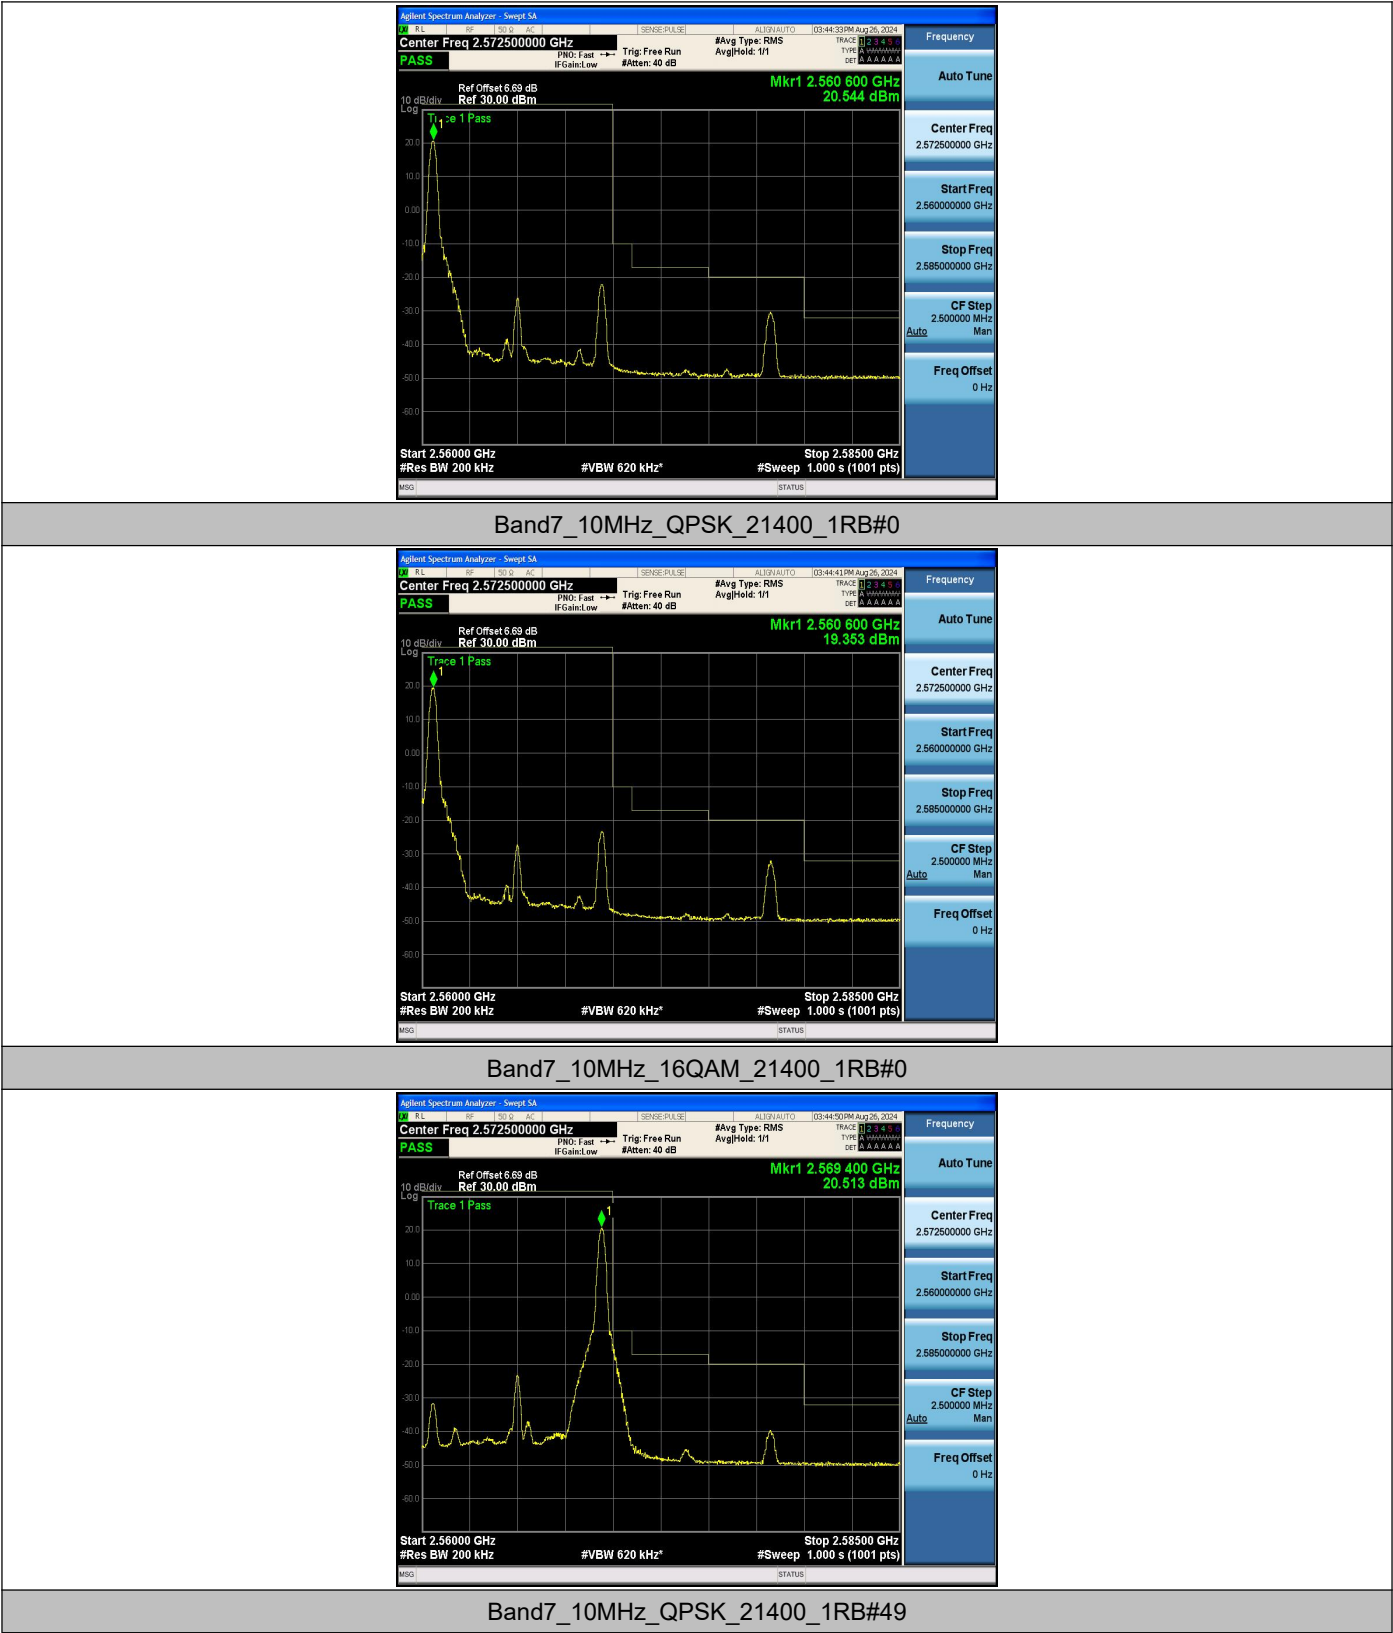

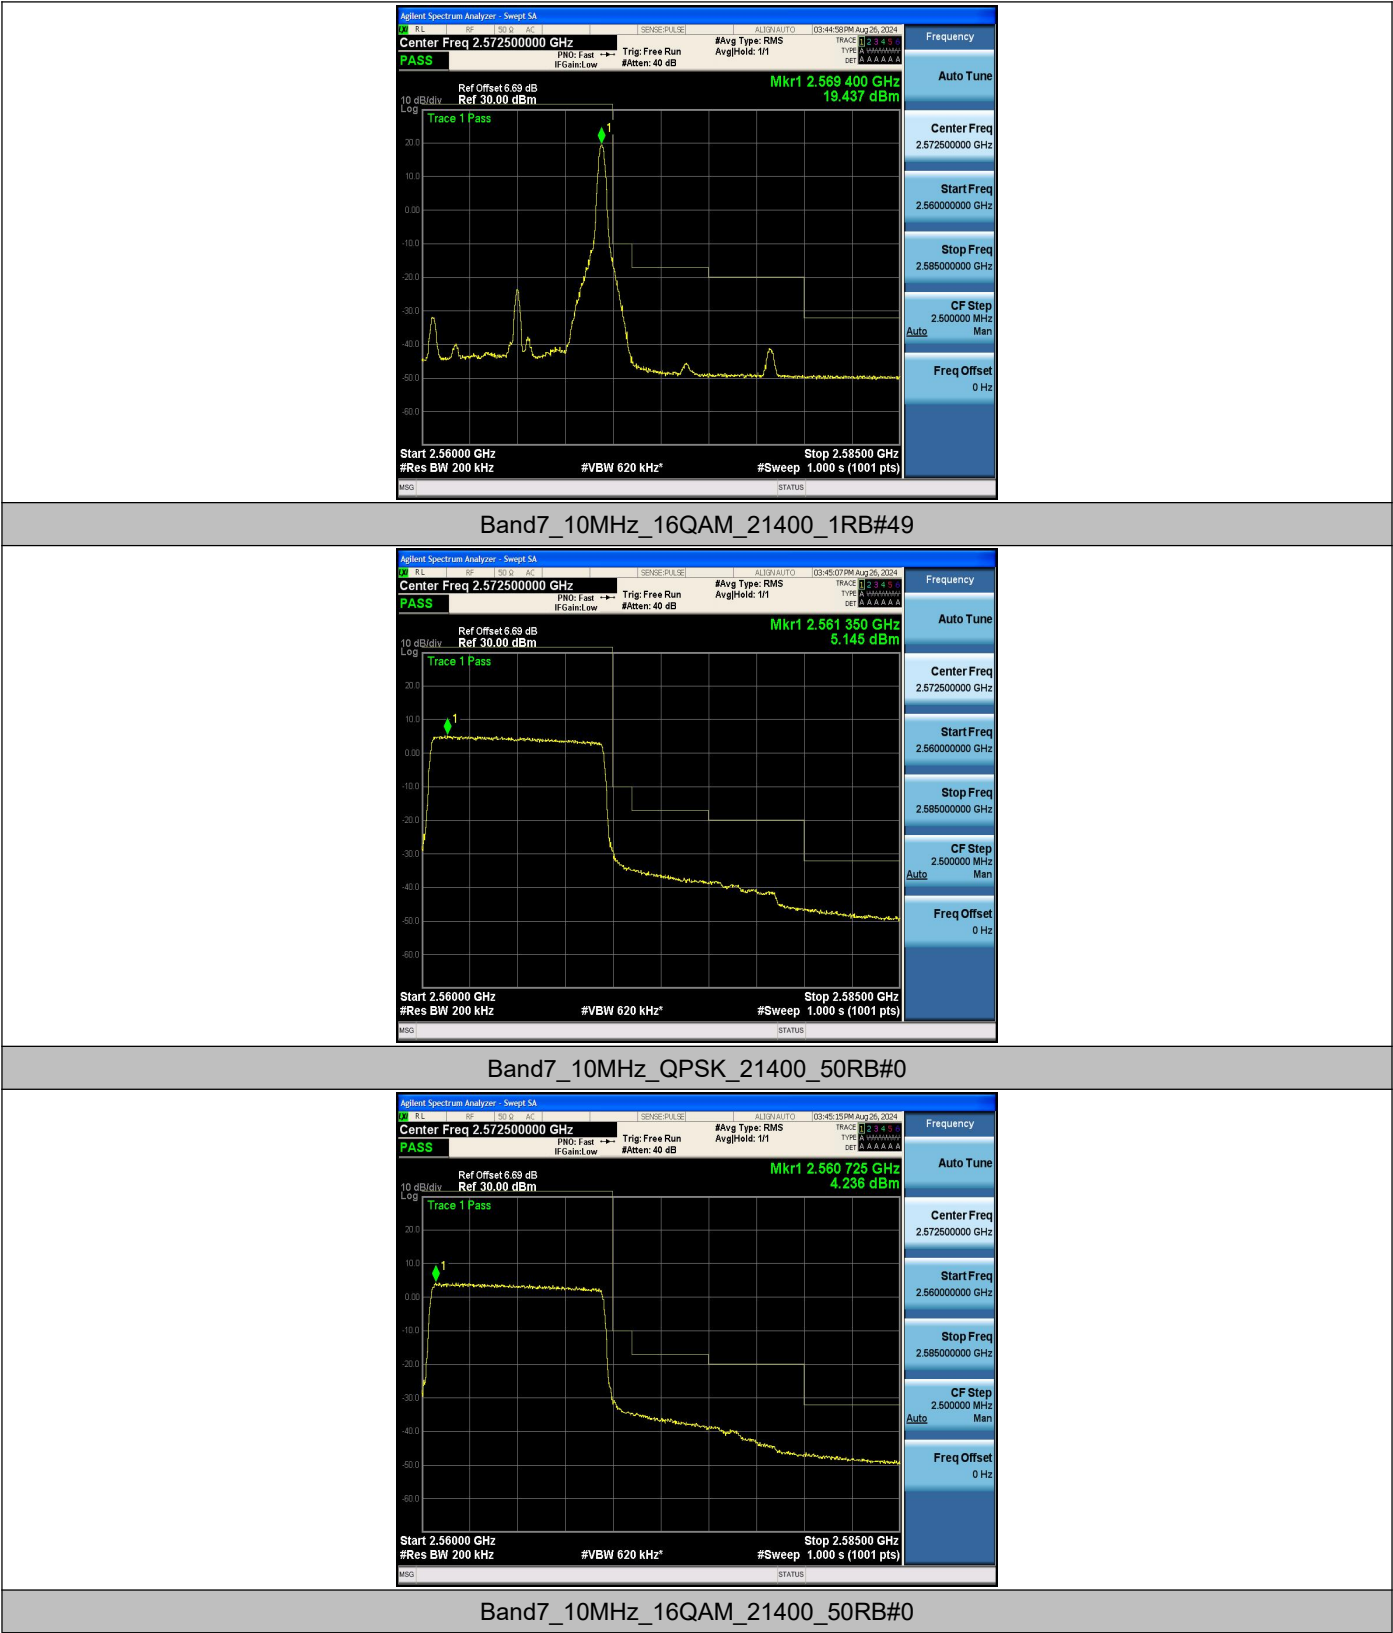

Agilent Spectrum Analyzer - Sweep SA

Center Freq 2.572500000 GHz

PASS

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.56000 GHz

Res BW 200 kHz

Stop 2.58500 GHz

Sweep 1.000 s (1001 pts)

Mkr1 2.560 725 GHz

4.236 dBm

Band7_10MHz_16QAM_21400_50RB#0

Frequency

Auto Tune

Center Freq

2.572500000 GHz

Start Freq

2.560000000 GHz

Stop Freq

2.585000000 GHz


CF Step

2.500000 MHz


Auto

Freq Offset


0 Hz

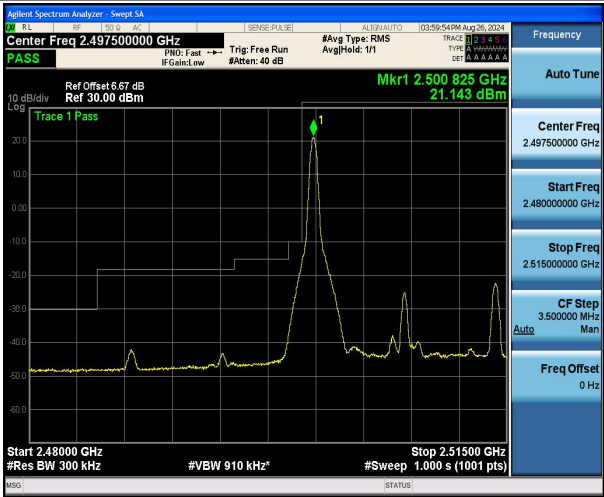

Band7_15MHz_QPSK_20825_1RB#0

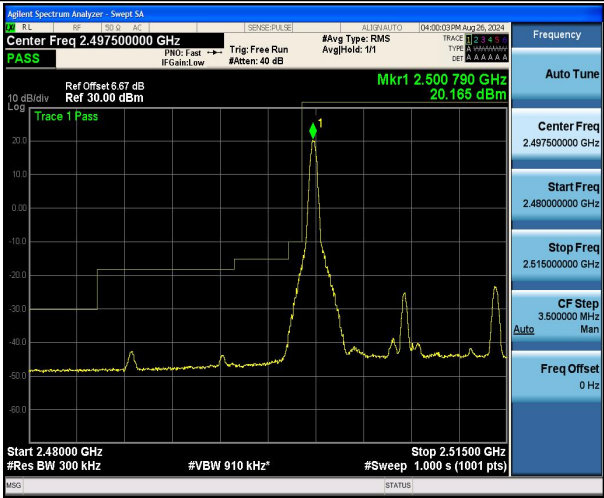

Band7_15MHz_16QAM_20825_1RB#0

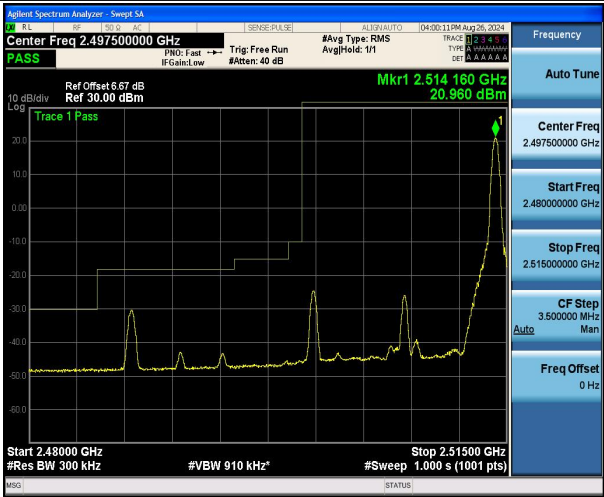

Band7_15MHz_QPSK_20825_1RB#74



