


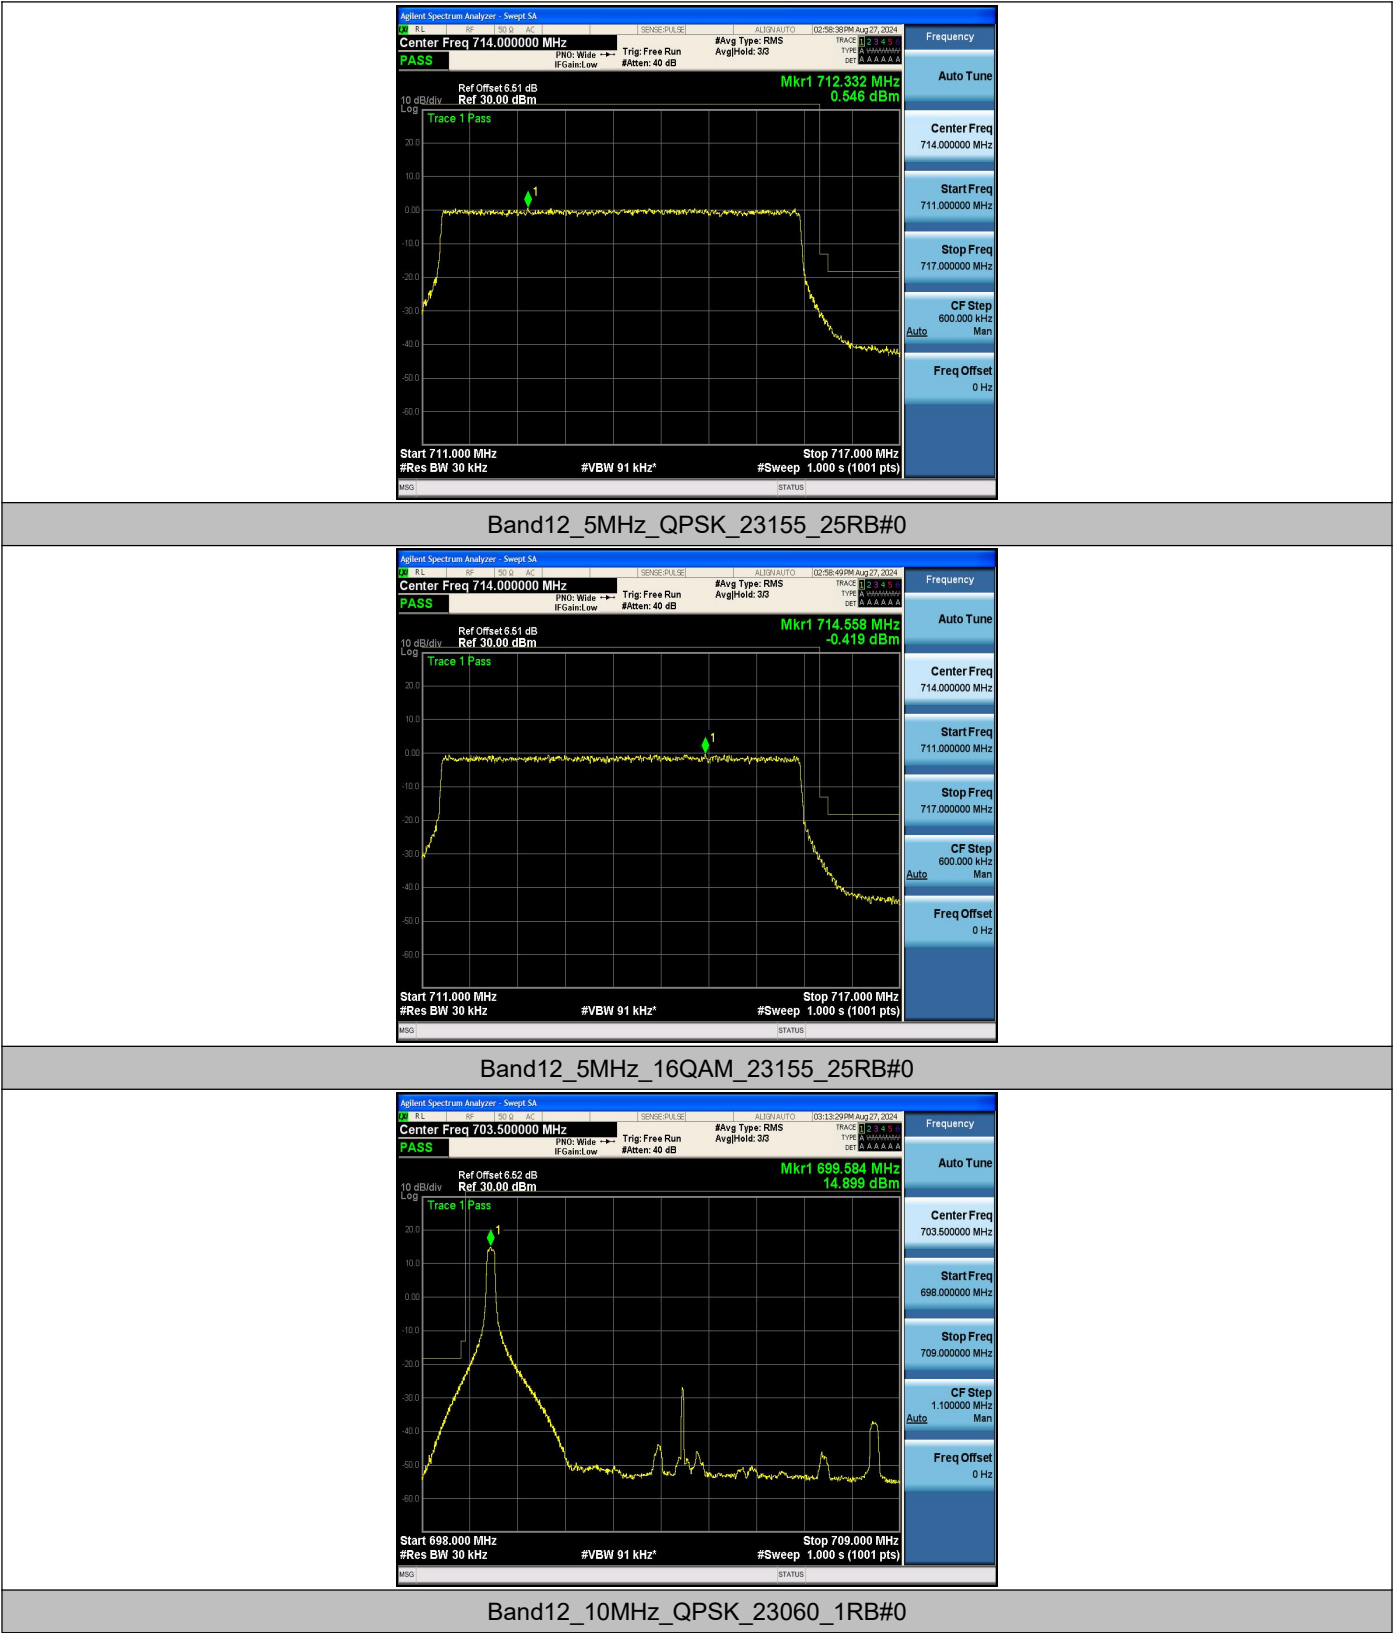

Agilent Spectrum Analyzer - Sweep SA

Center Freq 703.500000 MHz

PASS

Ref Offset 6.52 dB

Ref 30.00 dBm

Trace 1 Pass

Start 698.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 709.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 703.500000 MHz

Start Freq 698.000000 MHz

Stop Freq 709.000000 MHz

CF Step 1.100000 MHz


Auto

Freq Offset 0 Hz

Mkr1 699.584 MHz

14.899 dBm

Band12_10MHz_QPSK_23060_1RB#0

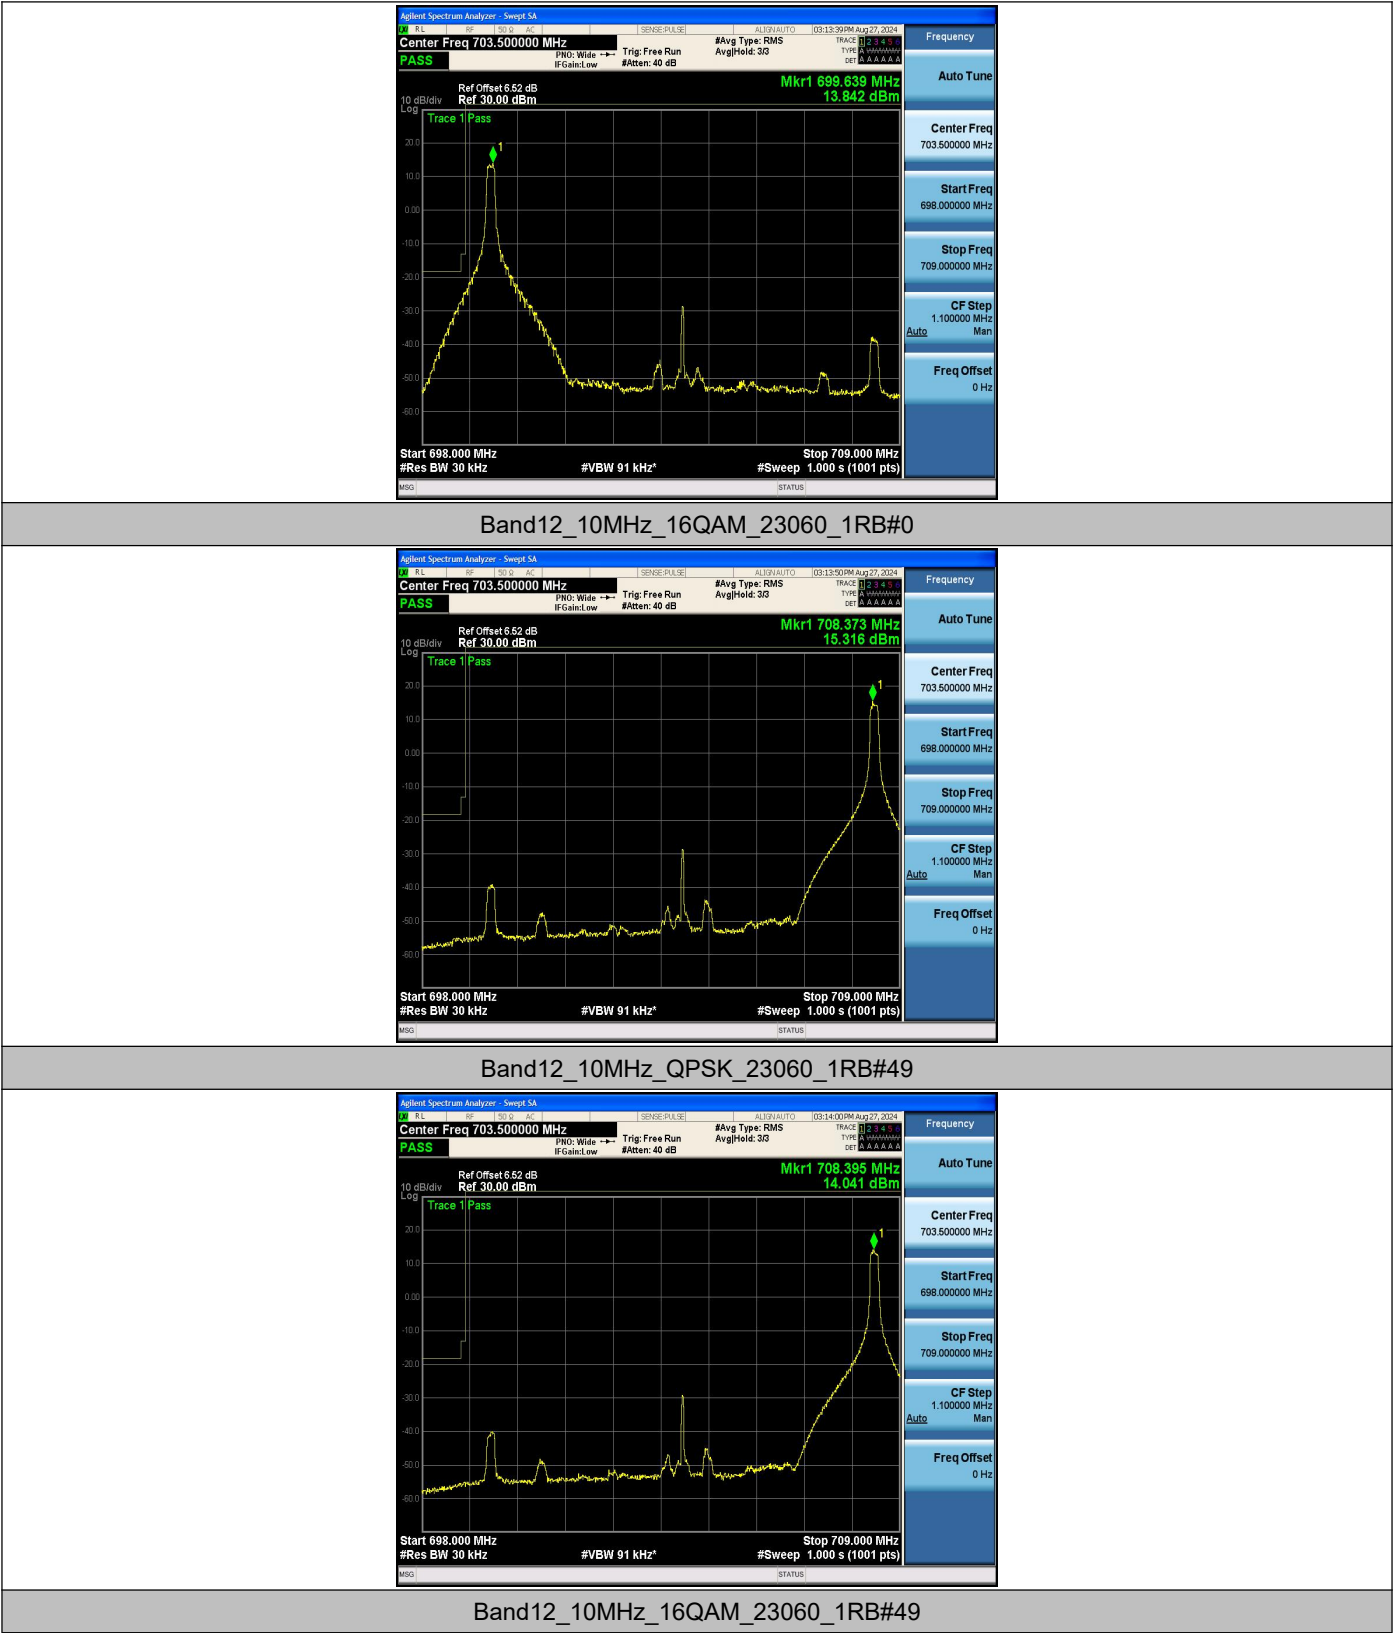

Agilent Spectrum Analyzer - Swept SA

Center Freq 703.500000 MHz

PASS

Ref Offset 6.52 dB

Ref 30.00 dBm

Trace 1 Pass

Start 698.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 703.500000 MHz

Start Freq 698.000000 MHz

Stop Freq 709.000000 MHz


CF Step 1.000000 MHz

Auto


Freq Offset 0 Hz

Mkr1 708.395 MHz

14.041 dBm

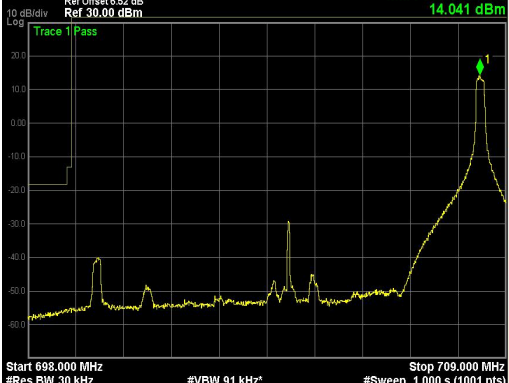

Band12_10MHz_16QAM_23060_1RB#49

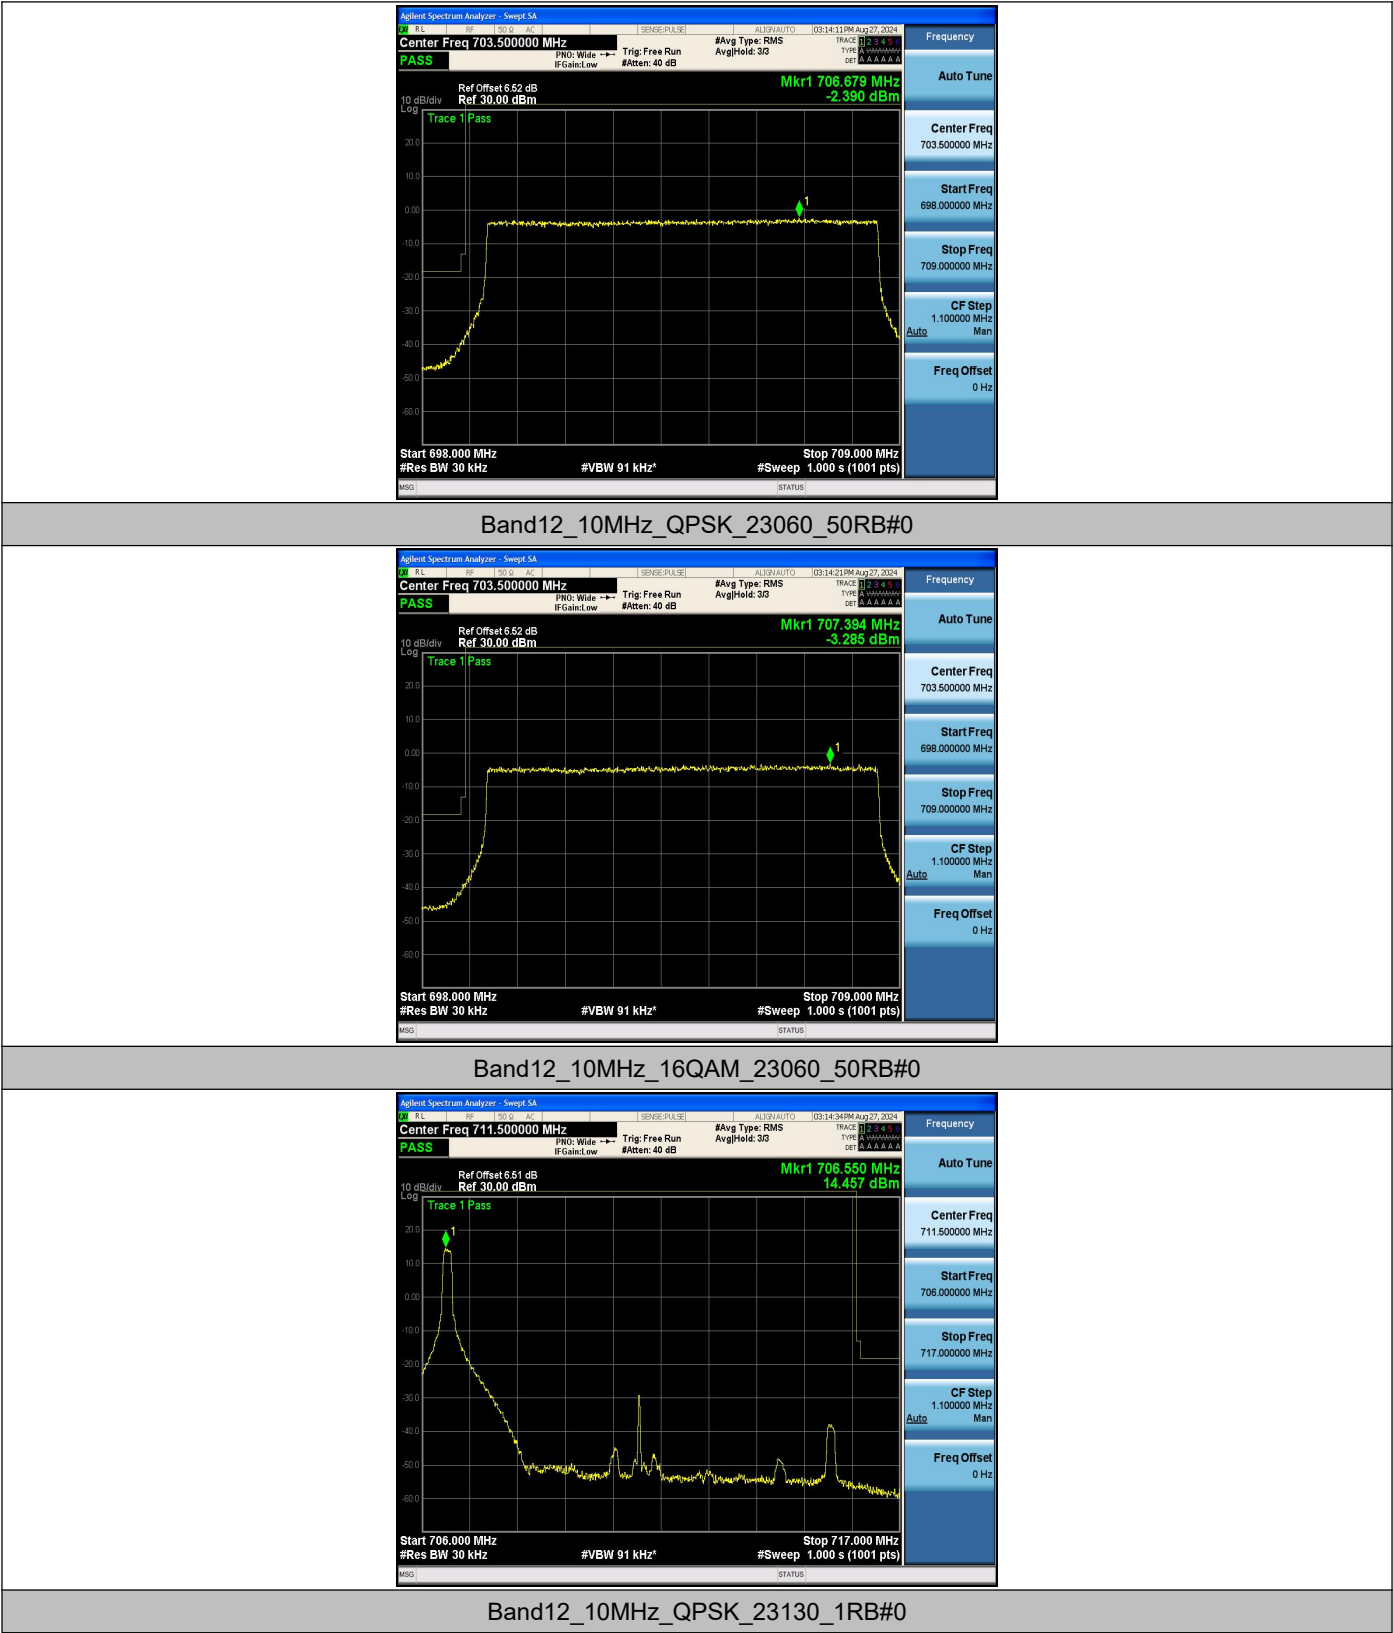

Agilent Spectrum Analyzer - Sweep SA

Center Freq 711.500000 MHz

PASS

Ref Offset 6.51 dB

Ref 30.00 dBm

Trace 1 Pass

Start 706.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 711.500000 MHz

Start Freq 706.000000 MHz

Stop Freq 717.000000 MHz

CF Step 1.100000 MHz


Auto


Freq Offset 0 Hz


Mkr1 706.550 MHz


14.457 dBm

Band12_10MHz_QPSK_23130_1RB#0

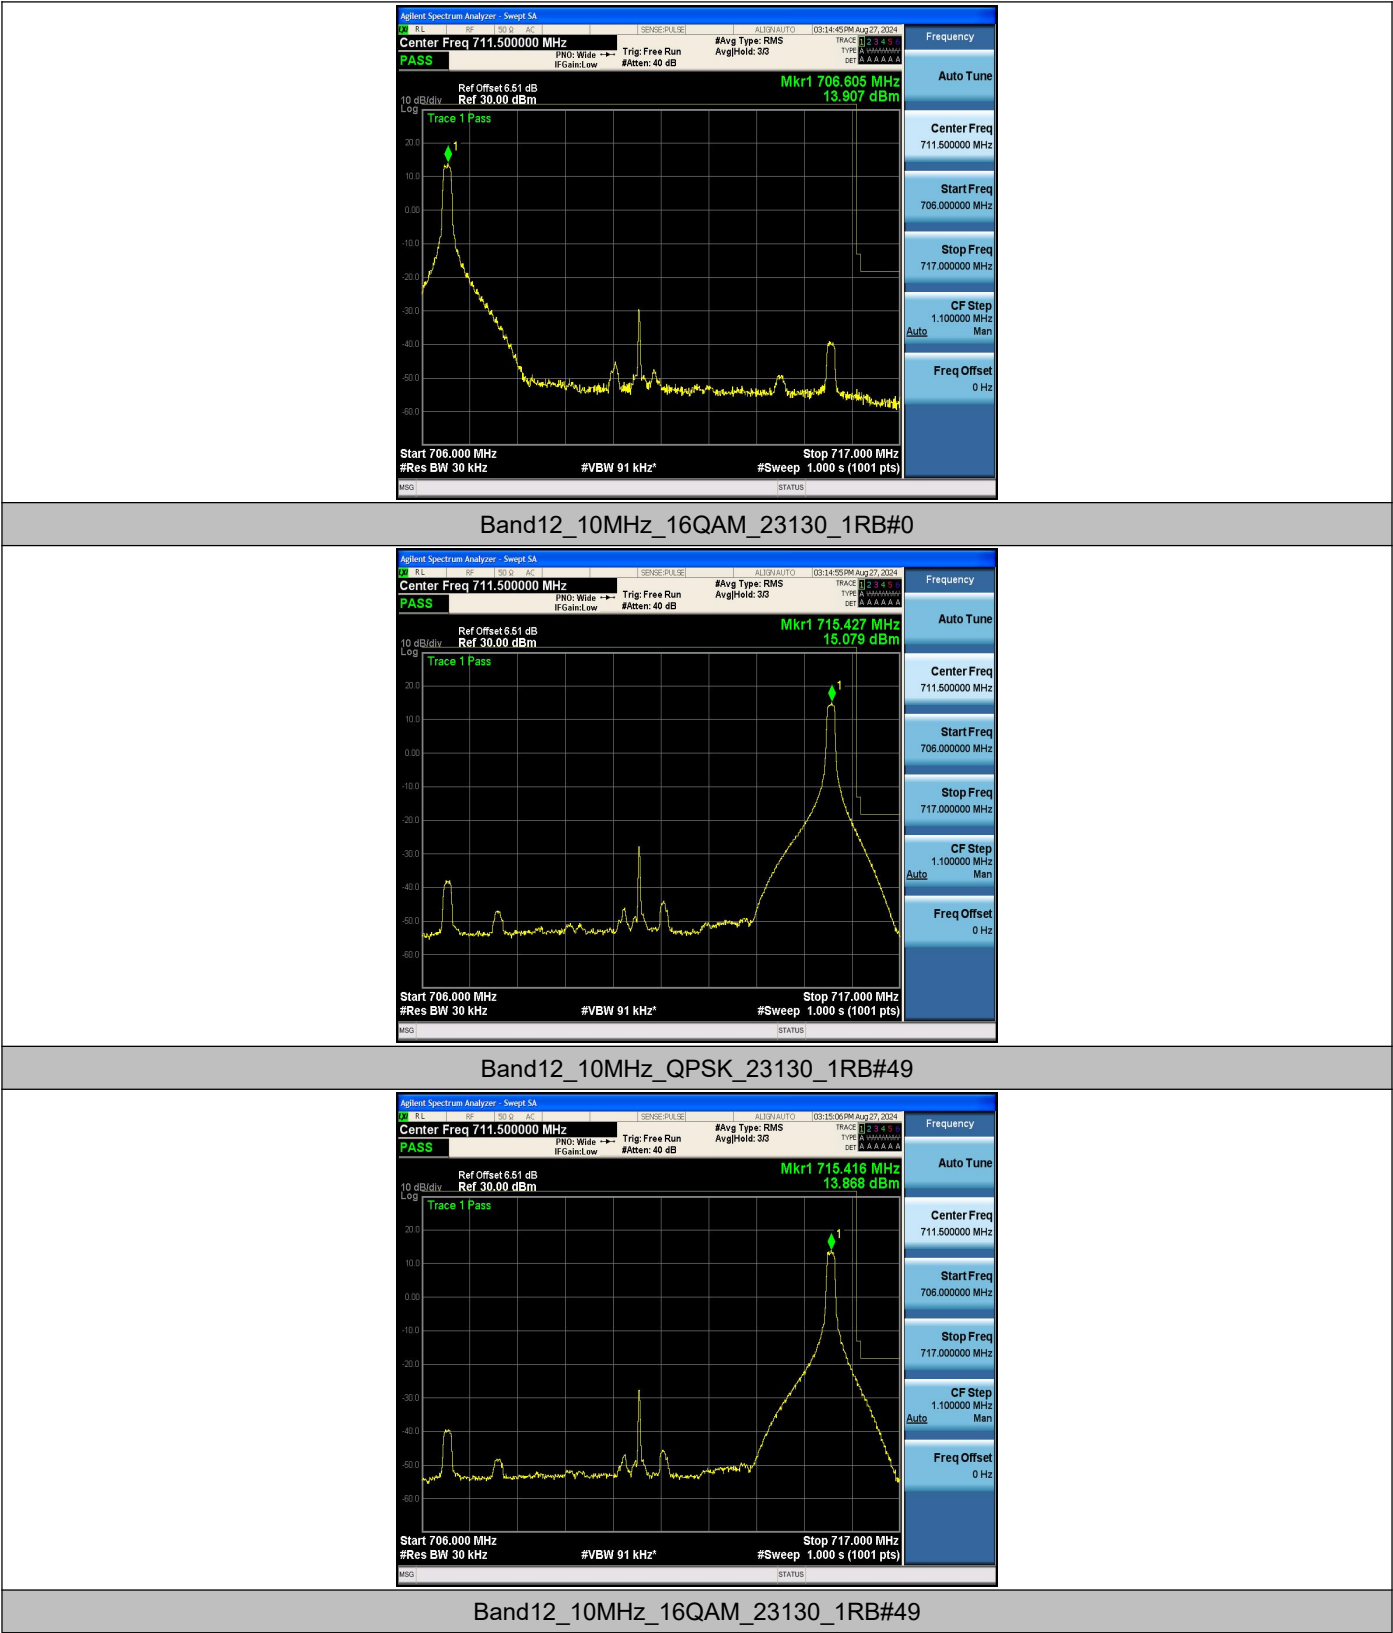


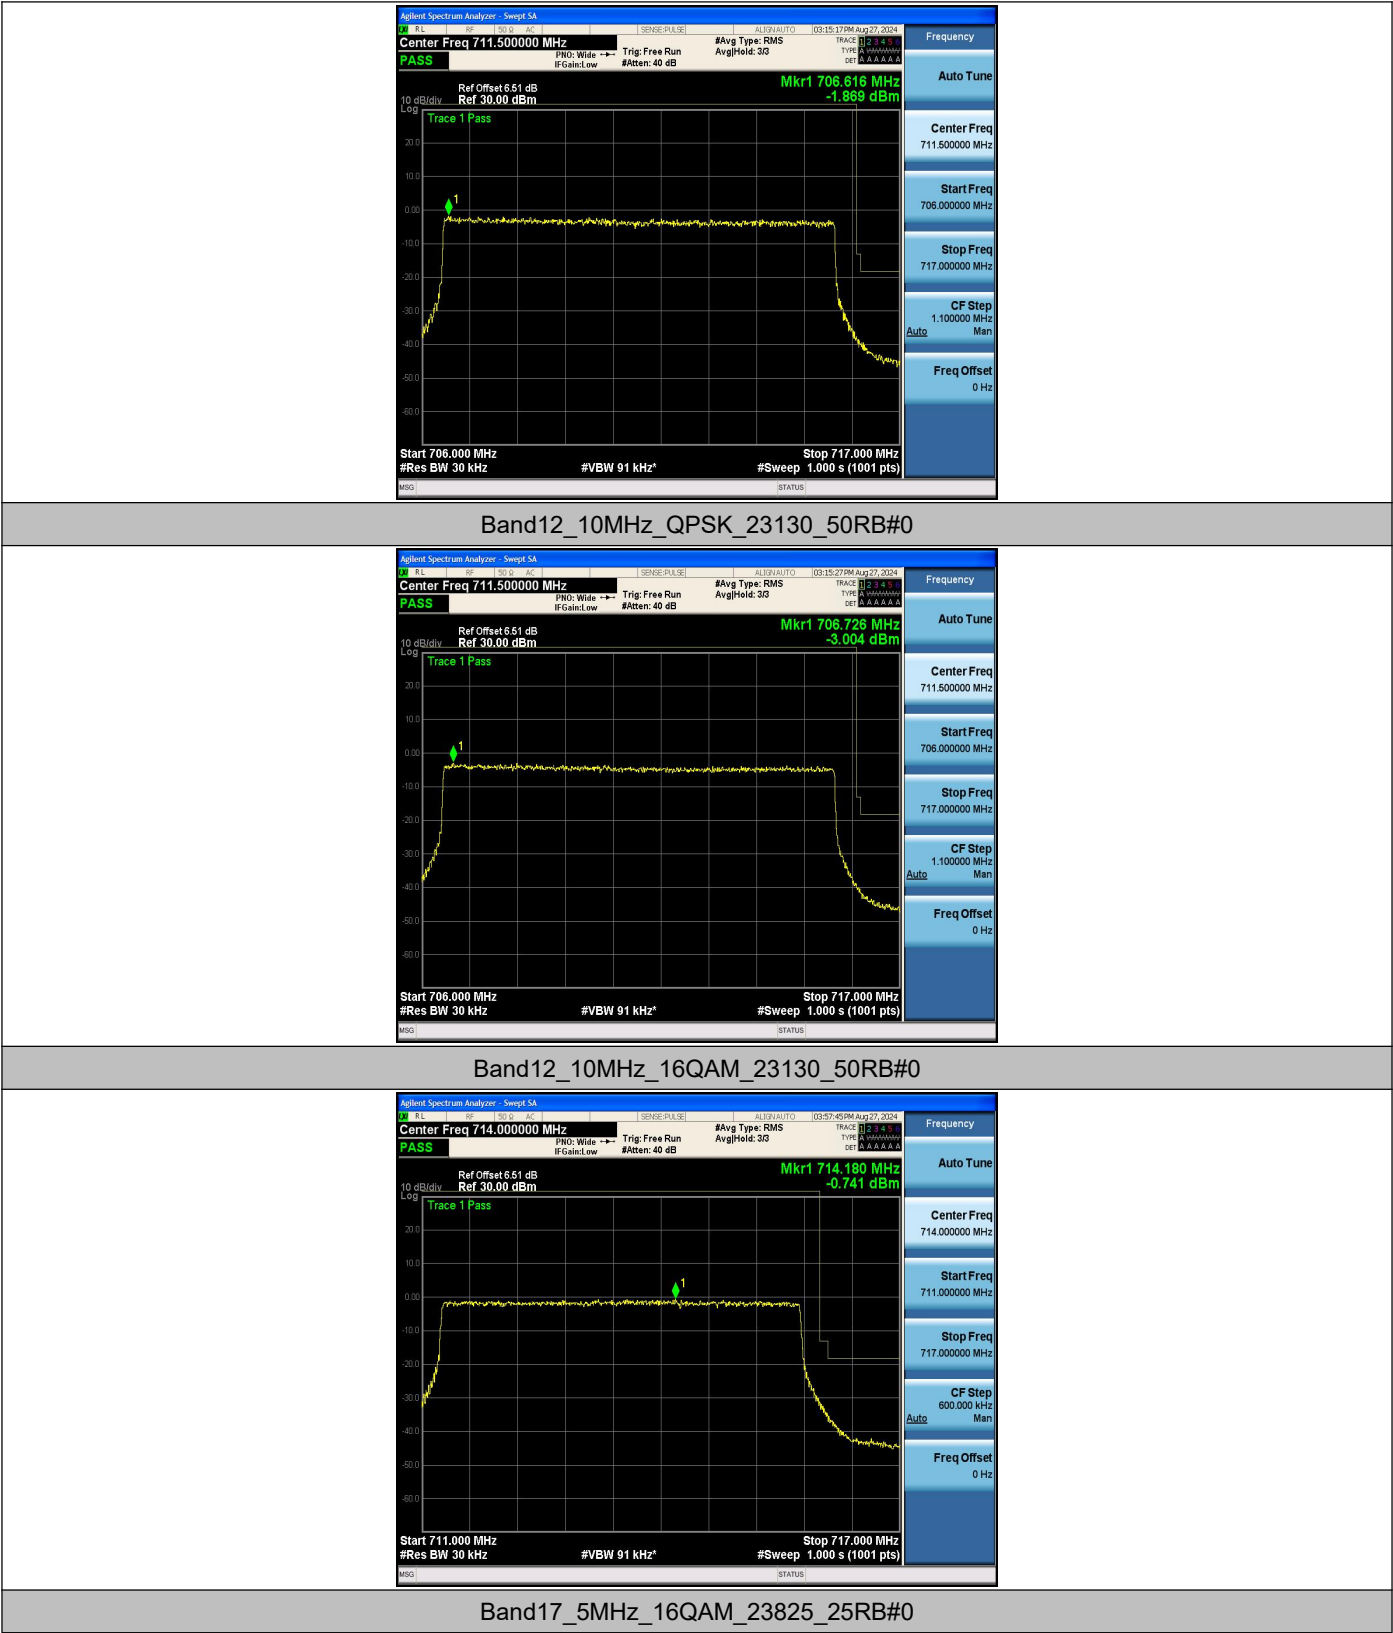

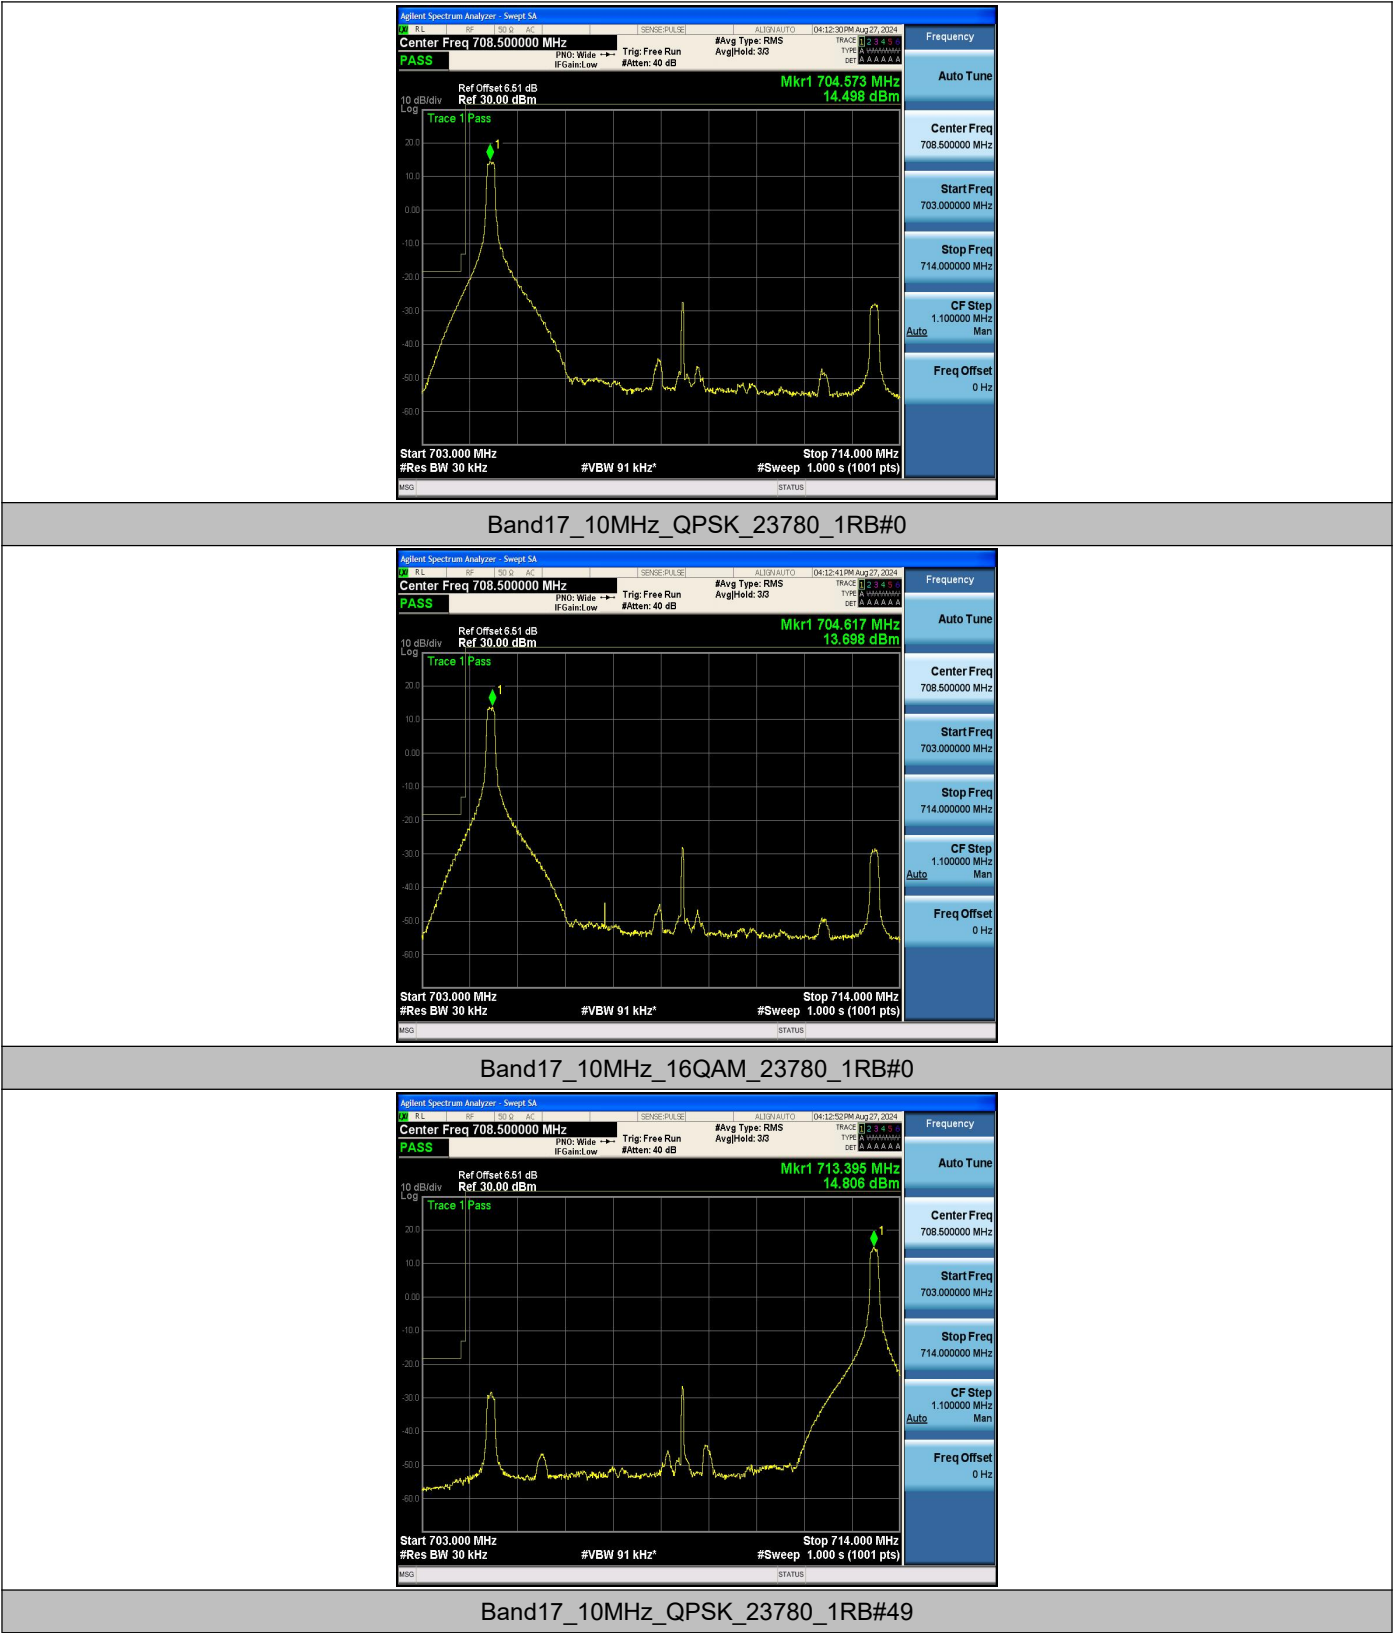

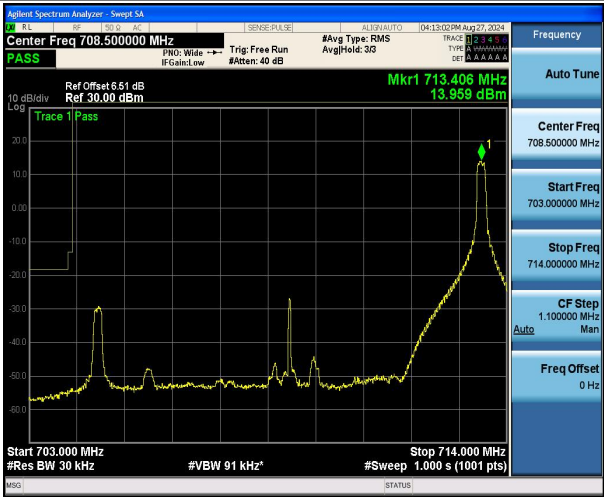


Band17_10MHz_16QAM_23780_1RB#49

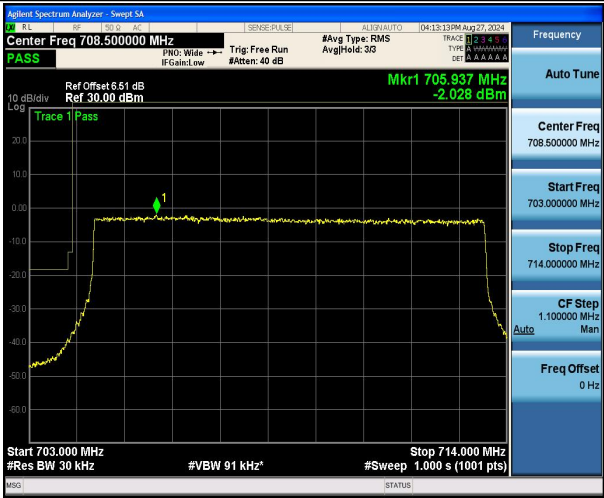


Band17_10MHz_QPSK_23780_50RB#0




Band17_10MHz_16QAM_23780_50RB#0

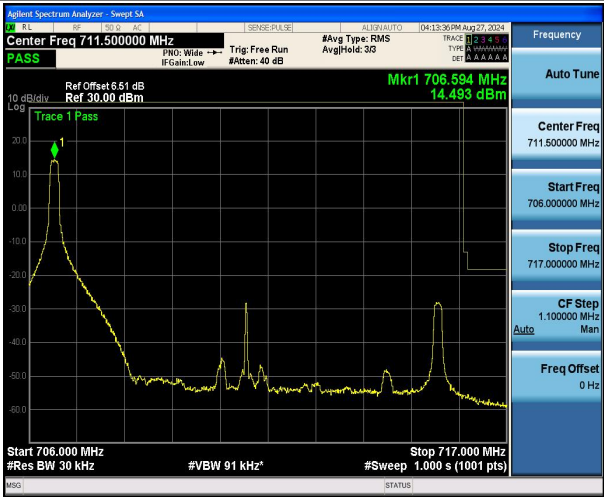


Band17_10MHz_QPSK_23800_1RB#0

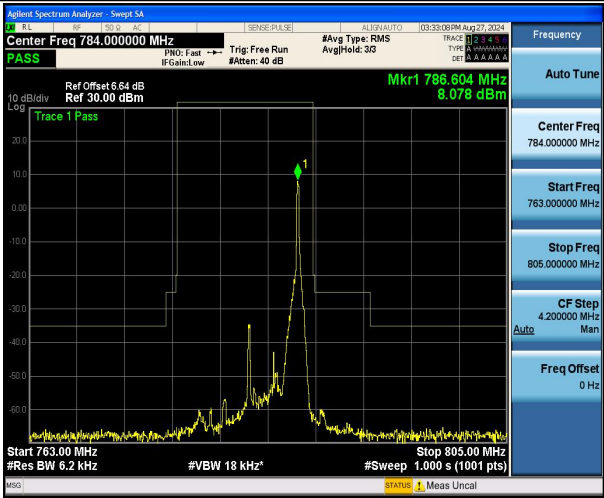


Band13_5MHz_QPSK_23255_1RB#24

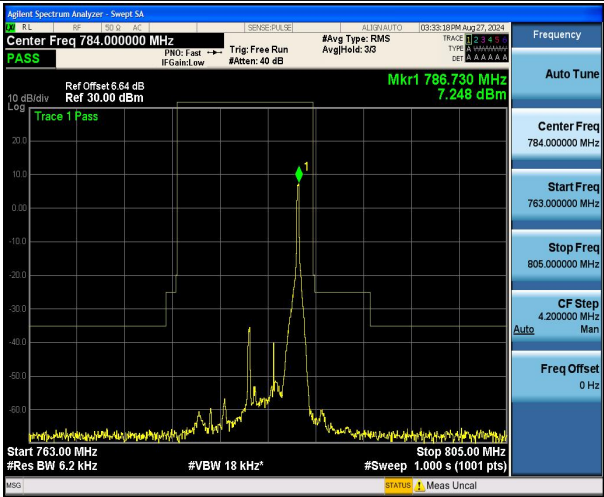

Band13_5MHz_16QAM_23255_1RB#24

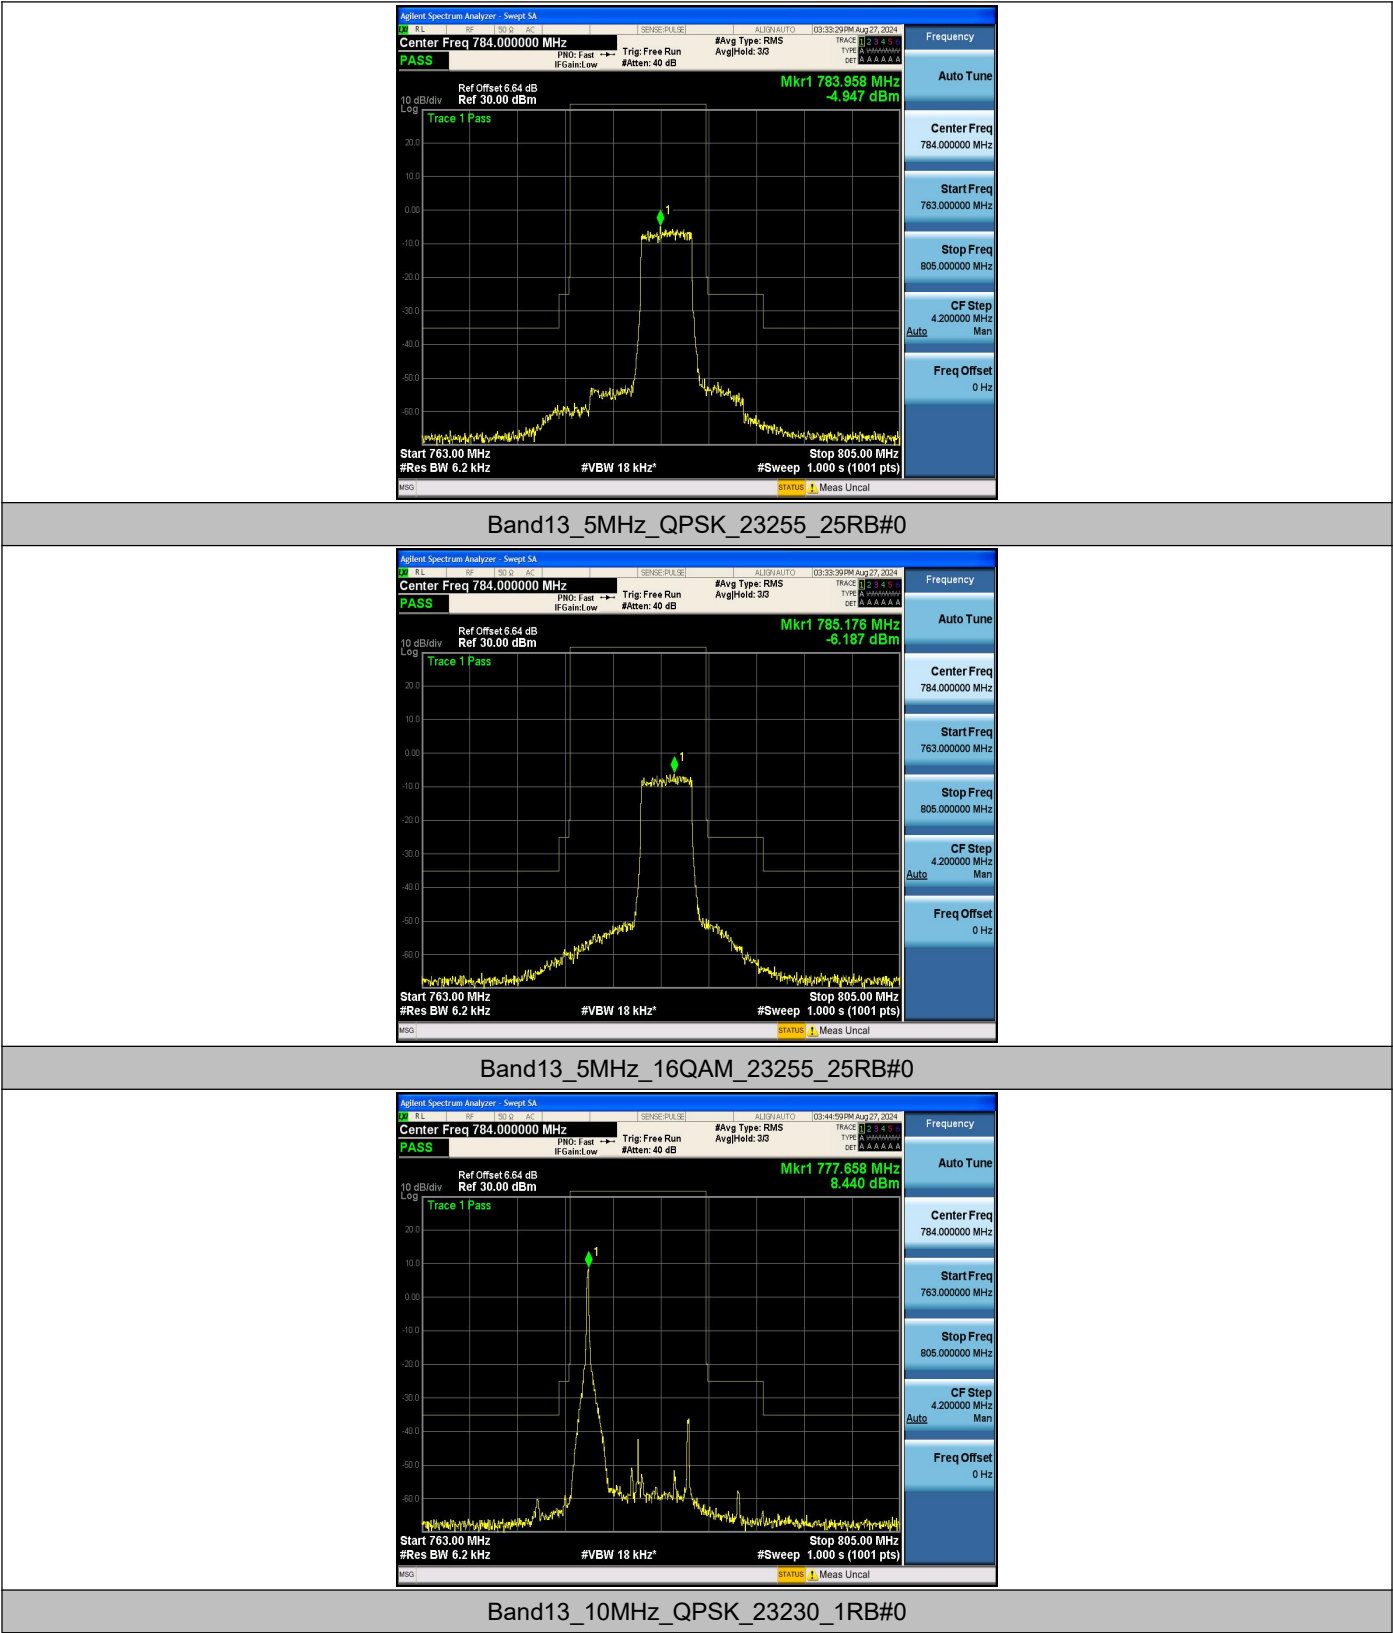

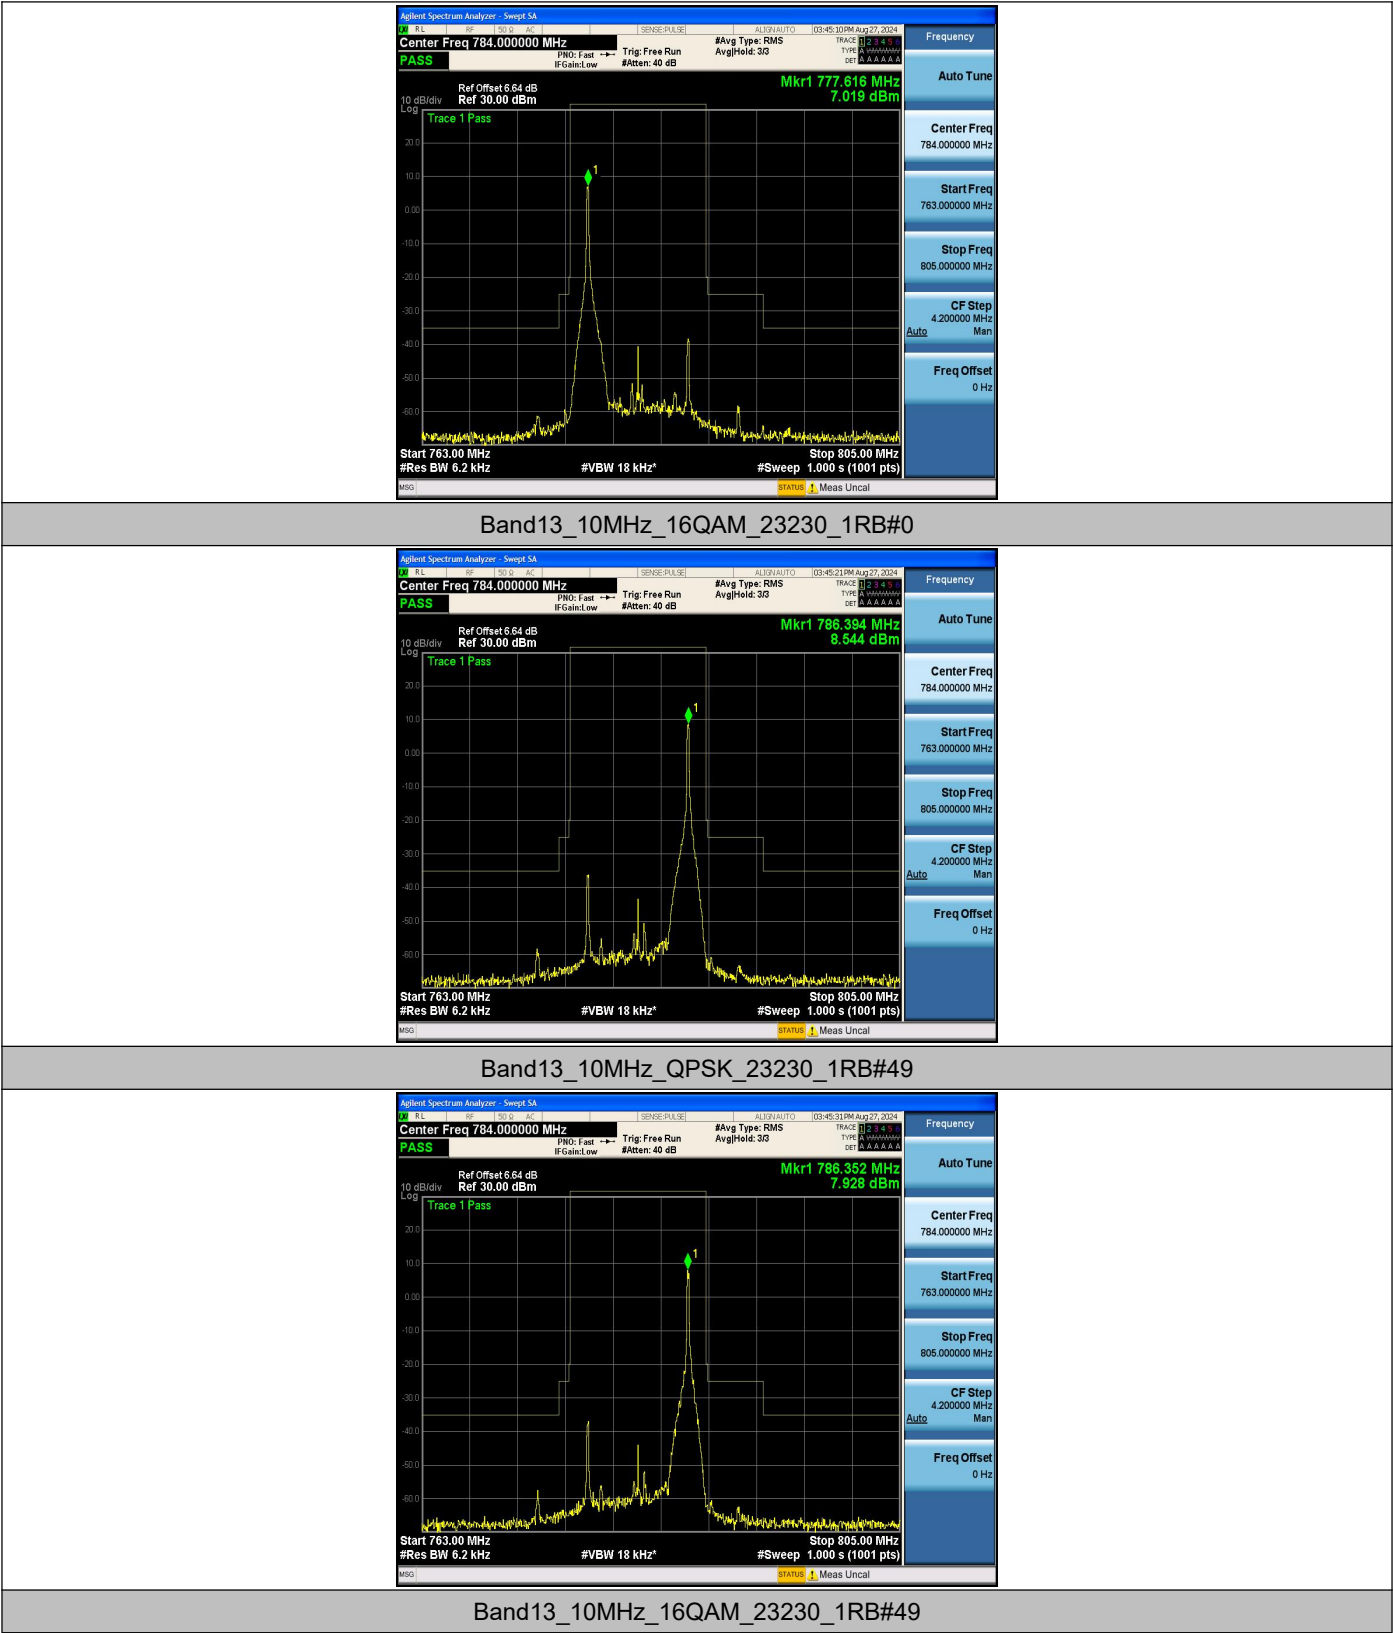




Band13_10MHz_QPSK_23230_50RB#0



Band13_10MHz_16QAM_23230_50RB#0



Band17_5MHz_QPSK_23755_1RB#0

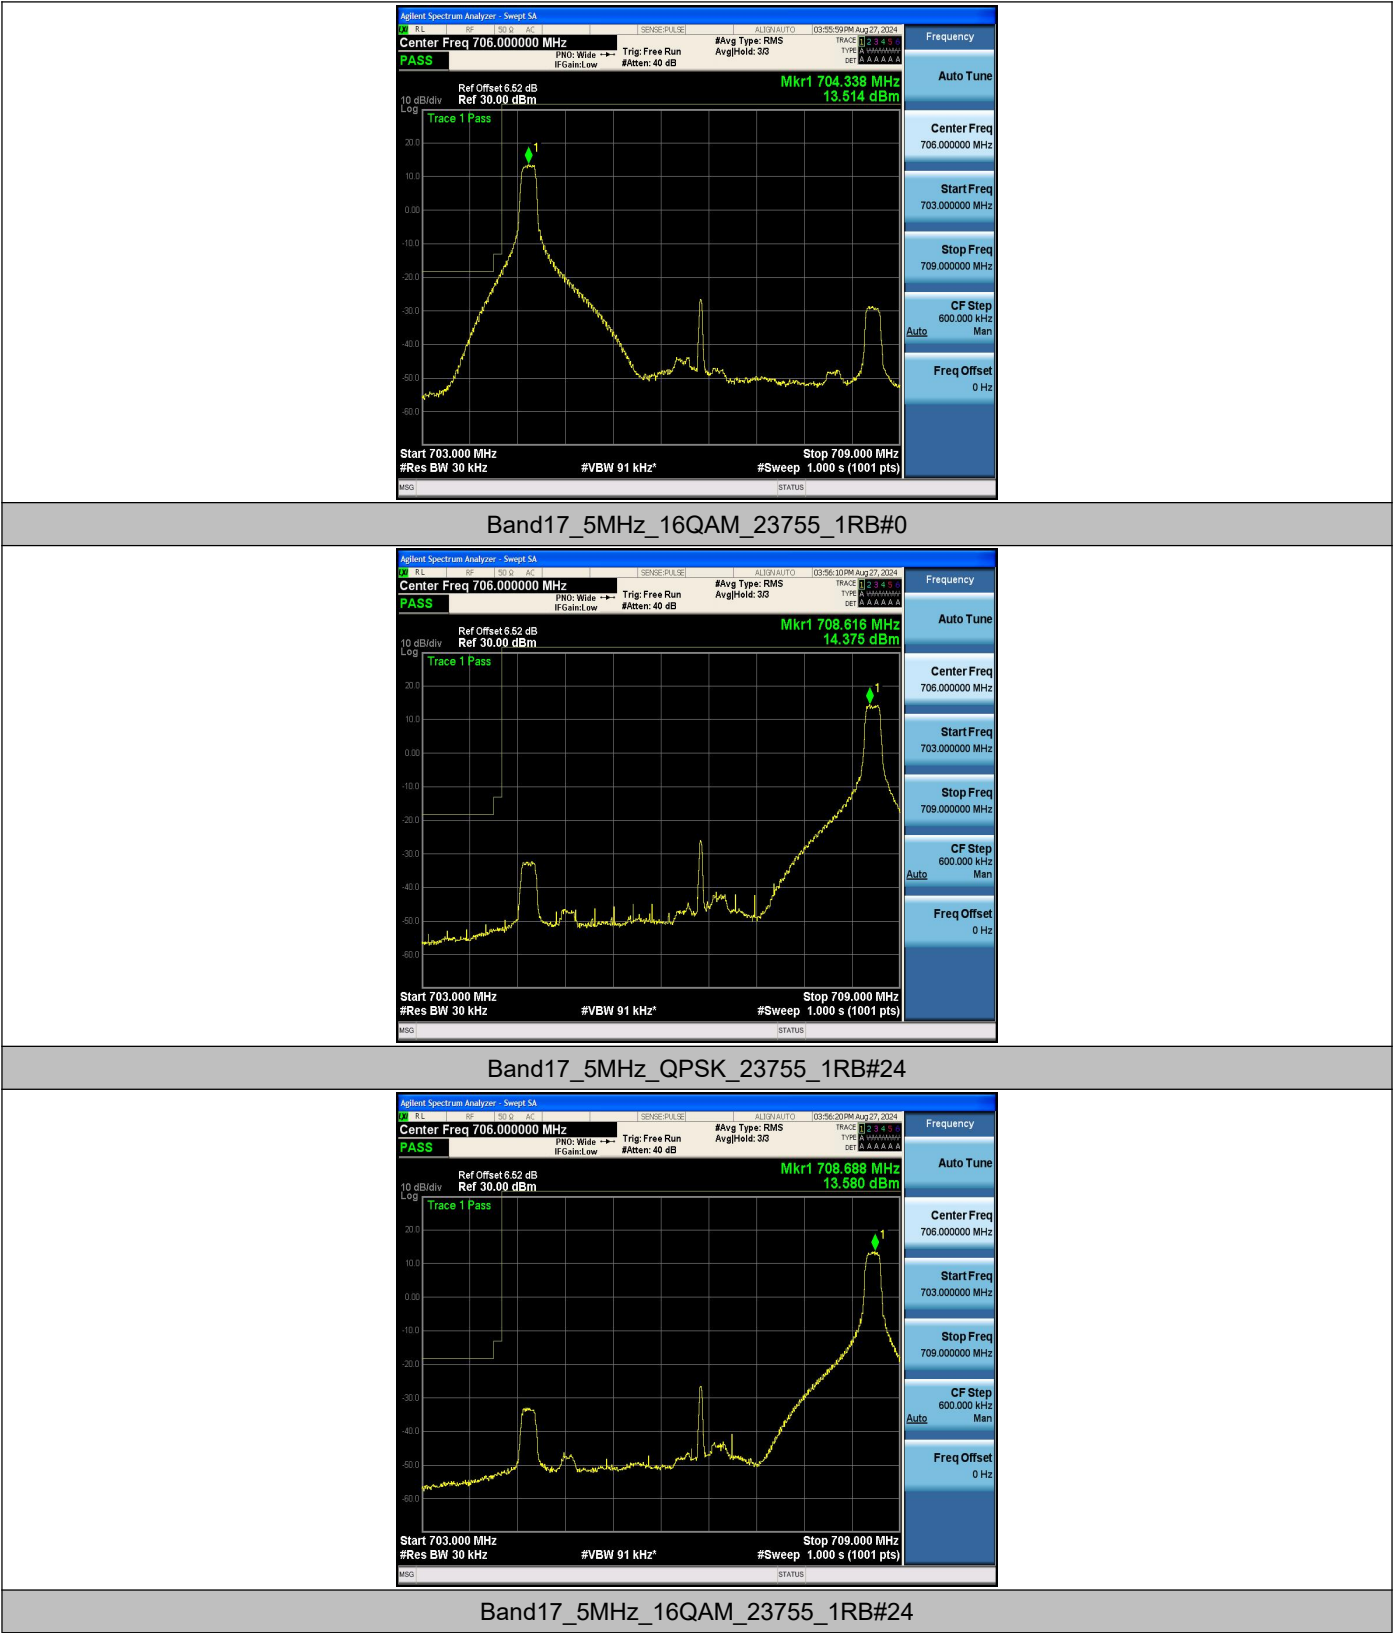

Agilent Spectrum Analyzer - Sweep SA

Center Freq 706.000000 MHz

PASS

Ref Offset 6.52 dB

Ref 30.00 dBm

Trace 1 Pass

Start 703.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 709.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 706.000000 MHz

Start Freq 703.000000 MHz

Stop Freq 709.000000 MHz


CF Step 600.000 kHz

Auto


Freq Offset 0 Hz


Mkr1 708.688 MHz

13.580 dBm

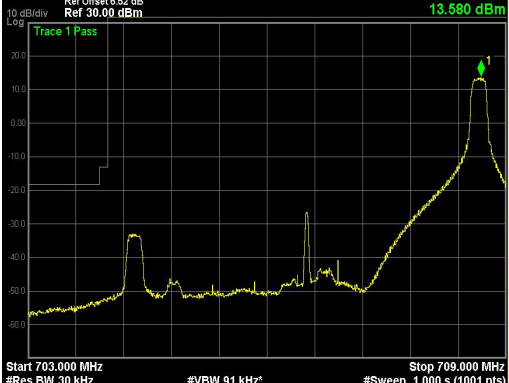

Band17_5MHz_16QAM_23755_1RB#24

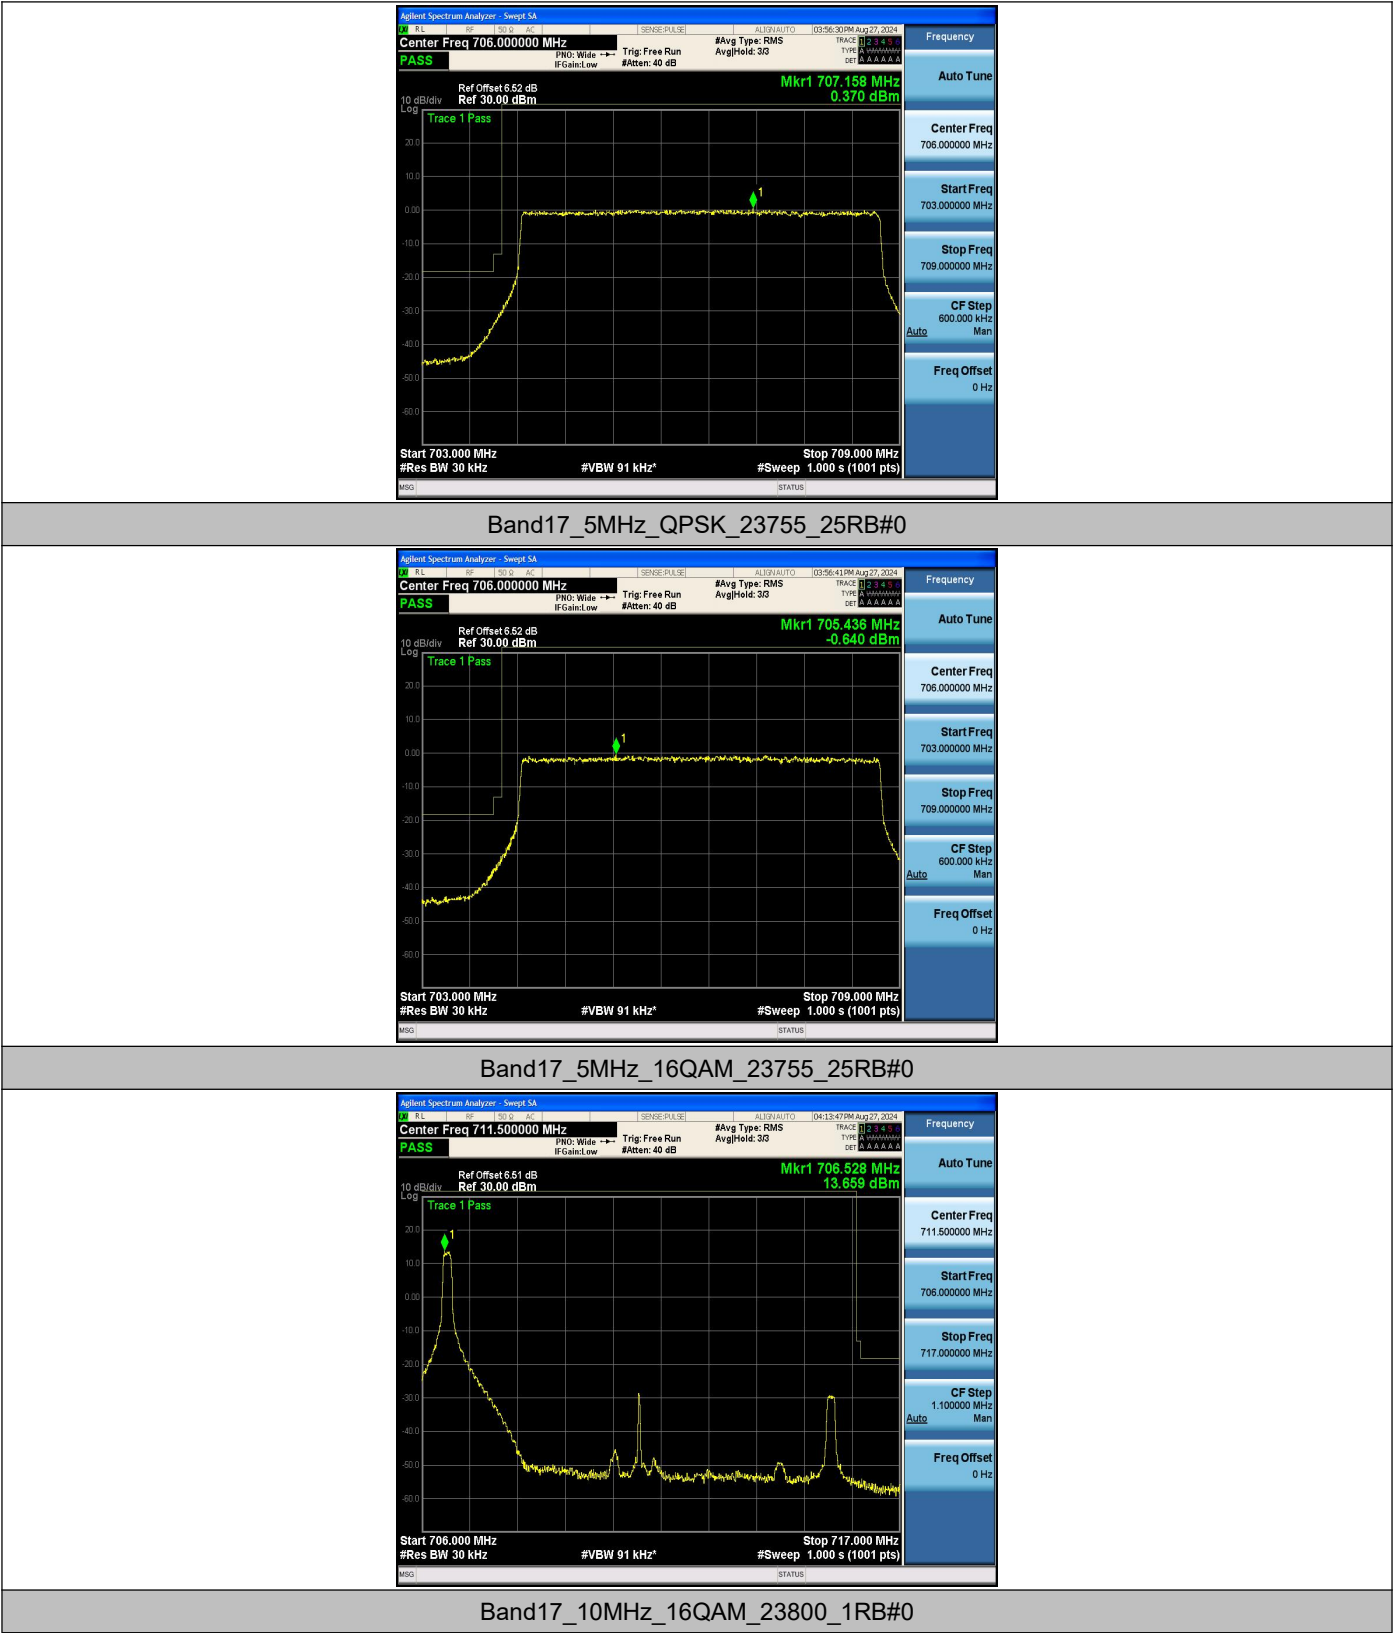

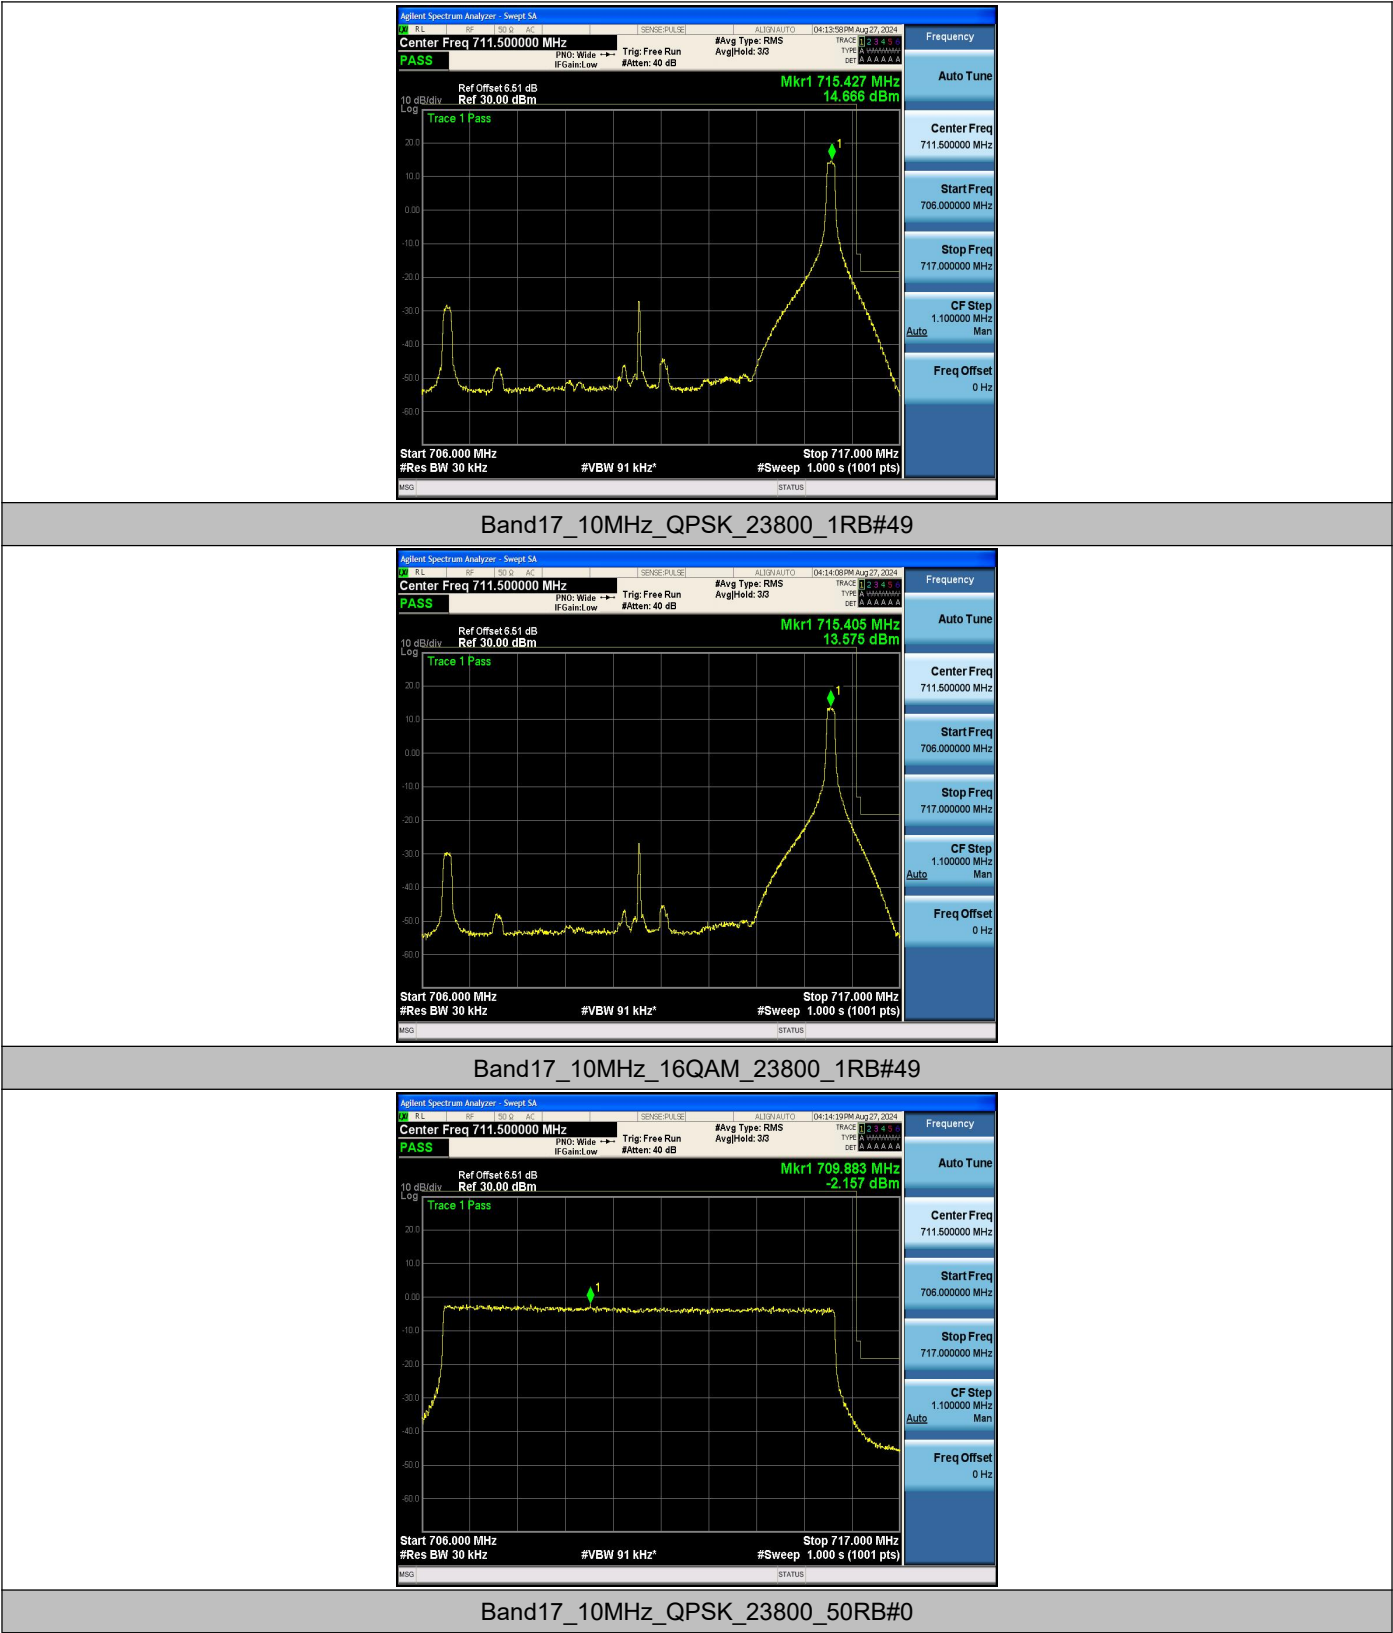

Agilent Spectrum Analyzer - Sweep SA

Center Freq 711.500000 MHz

PASS

Ref Offset 6.51 dB

Ref 30.00 dBm

Trace 1 Pass

Start 706.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 717.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 711.500000 MHz

Start Freq 706.000000 MHz

Stop Freq 717.000000 MHz

CF Step 1.100000 MHz

Auto

Freq Offset 0 Hz

Mkr1 709.883 MHz

-2.167 dBm

10 dB/div

Log

20.0

10.0

0.00

-10.0

-20.0


-30.0

-40.0

-50.0

-60.0

Band17_10MHz_QPSK_23800_50RB#0

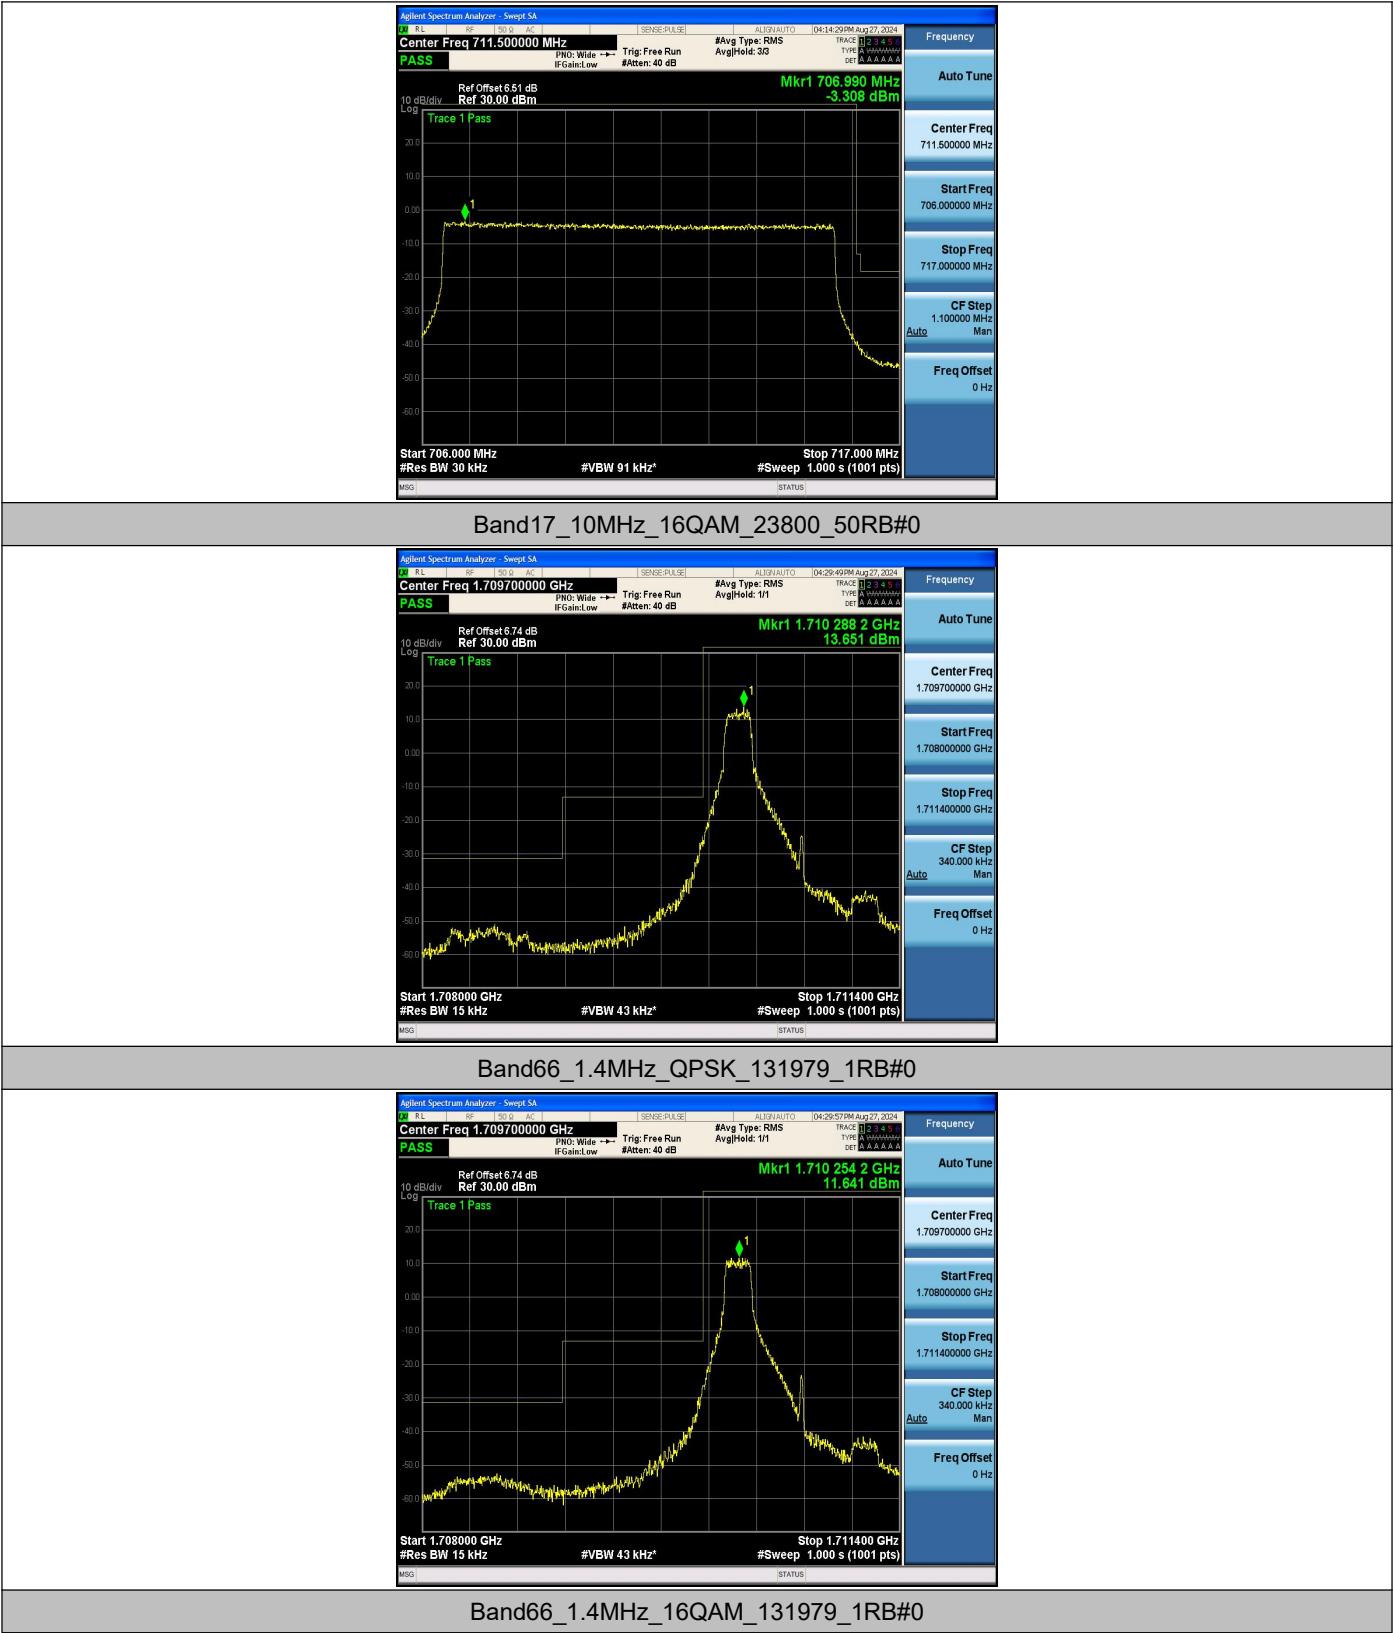

Agilent Spectrum Analyzer - Sweep SA

Center Freq 1.709700000 GHz

PASS

Ref Offset 6.74 dB

Ref 30.00 dBm

Trace 1 Pass

Start 1.708000 GHz

#Res BW 15 kHz

#VBW 43 kHz

Stop 1.711400 GHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 1.709700000 GHz

Start Freq 1.708000000 GHz

Stop Freq 1.711400000 GHz

CF Step 340.000 kHz

Man

Freq Offset 0 Hz

Mkr1 1.710 254 2 GHz

11.641 dBm

Band66_1.4MHz_16QAM_131979_1RB#0