

Appendix C for KSCR220800147101

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date
Dipole	<input type="checkbox"/>	1	CLA150	4025	2021/04/26
	<input checked="" type="checkbox"/>	2	D450V3	1103	2021/04/21
	<input type="checkbox"/>	3	D750V3	1188	2022/03/29
	<input type="checkbox"/>	4	D835V2	4d114	2022/03/31
	<input type="checkbox"/>	5	D900V2	1d079	2022/06/07
	<input type="checkbox"/>	6	D1800V2	2d170	2022/03/31
	<input type="checkbox"/>	7	D1900V2	5d136	2022/06/07
	<input type="checkbox"/>	8	D2000V2	1041	2022/06/06
	<input type="checkbox"/>	9	D2300V2	1096	2022/03/31
	<input type="checkbox"/>	10	D2450V2	817	2022/04/01
	<input type="checkbox"/>	11	D2600V2	1158	2022/03/31
	<input type="checkbox"/>	12	D5GHzV2	1095	2022/06/01
DAE	<input checked="" type="checkbox"/>	13	DAE4	1245	2022/05/30
Probe	<input checked="" type="checkbox"/>	14	EX3DV4	3801	2022/07/21

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com



No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

1 Dipole

1.1 CLA150 - SN 4025

<p>Calibration Laboratory of Schmid & Partner Engineering AG Zughestrasse 43, 8001 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SCS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS-CN (Auden) Certificate No.: CLA150-4025_Apr21</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: CLA150 - SN: 4025</p> <p>Calibration procedure(s): QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz</p> <p>Calibration date: April 26, 2021</p> <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurement (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.</p> <p>Calibration Equipment used (MATE critical for calibration):</p> <table border="1"> <thead> <tr> <th>Primary Standard</th> <th>ID #</th> <th>Cal. Cal. (Calibration No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NRP</td> <td>SN: 104/76</td> <td>05-Apr-21 (No. 217-0329)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103/44</td> <td>05-Apr-21 (No. 217-0329)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103/24</td> <td>06-Apr-21 (No. 217-0329)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NRP-Z91</td> <td>SN: 103/26</td> <td>06-Apr-21 (No. 217-0329)</td> <td>Apr-22</td> </tr> <tr> <td>Trich-N Intensity Meter</td> <td>SN: 00010000000000000000000000000000</td> <td>04-Apr-21 (No. 217-0329)</td> <td>Apr-22</td> </tr> <tr> <td>Reference Probe DEXTRA (D4-4)</td> <td>SN: 3877</td> <td>30-Dec-20 (No. E3X3/177, Dec20)</td> <td>Dec-21</td> </tr> <tr> <td>Reference Probe DEXTRA (D4-4)</td> <td>SN: 664</td> <td>06-Jun-20 (No. D4E4-054, Jun20)</td> <td>Jun-21</td> </tr> </tbody> </table> <p>Secondary Standard</p> <table border="1"> <thead> <tr> <th>ID #</th> <th>Check Date (in house)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Power meter E4441B</td> <td>SN: 03410004/4</td> <td>05-Apr-10 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power meter E4441B</td> <td>SN: 03410005/4</td> <td>05-Apr-10 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Power sensor E4441A</td> <td>SN: 00010210</td> <td>05-Apr-10 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>FF generator HP 8440C</td> <td>SN: US4840U1700</td> <td>04-Apr-09 (in house check Jun-20)</td> <td>In house check: Jun-22</td> </tr> <tr> <td>Network Analyzer Agilent E5080A</td> <td>SN: US4840U0401</td> <td>31-Mar-14 (in house check Oct-20)</td> <td>In house check: Oct-21</td> </tr> </tbody> </table> <p>Calibrated by: Name: Jeffrey Katsurada Function: Laboratory Technician Signature: </p> <p>Approved by: Name: Kaja Polovic Function: Technical Manager Signature: </p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No.: CLA150-4025_Apr21 Page 1 of 6</p>	Primary Standard	ID #	Cal. Cal. (Calibration No.)	Scheduled Calibration	Power meter NRP	SN: 104/76	05-Apr-21 (No. 217-0329)	Apr-22	Power sensor NRP-Z91	SN: 103/44	05-Apr-21 (No. 217-0329)	Apr-22	Power sensor NRP-Z91	SN: 103/24	06-Apr-21 (No. 217-0329)	Apr-22	Power sensor NRP-Z91	SN: 103/26	06-Apr-21 (No. 217-0329)	Apr-22	Trich-N Intensity Meter	SN: 00010000000000000000000000000000	04-Apr-21 (No. 217-0329)	Apr-22	Reference Probe DEXTRA (D4-4)	SN: 3877	30-Dec-20 (No. E3X3/177, Dec20)	Dec-21	Reference Probe DEXTRA (D4-4)	SN: 664	06-Jun-20 (No. D4E4-054, Jun20)	Jun-21	ID #	Check Date (in house)	Scheduled Check	Power meter E4441B	SN: 03410004/4	05-Apr-10 (in house check Jun-20)	In house check: Jun-22	Power meter E4441B	SN: 03410005/4	05-Apr-10 (in house check Jun-20)	In house check: Jun-22	Power sensor E4441A	SN: 00010210	05-Apr-10 (in house check Jun-20)	In house check: Jun-22	FF generator HP 8440C	SN: US4840U1700	04-Apr-09 (in house check Jun-20)	In house check: Jun-22	Network Analyzer Agilent E5080A	SN: US4840U0401	31-Mar-14 (in house check Oct-20)	In house check: Oct-21	<p>Calibration Laboratory of Schmid & Partner Engineering AG Zughestrasse 43, 8001 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SCS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Glossary:</p> <p>TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORM x,y,z N/A: not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <ul style="list-style-type: none"> a) IEEE Std 1526-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices and Measurements Techniques", June 2013 b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016 c) IEC 62209-2, "Measurement procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010 d) KDB 865662, "SAR Measurement Requirements for 100 MHz to 6 GHz" <p>Additional Documentation:</p> <ul style="list-style-type: none"> e) DASY4.5 System Handbook <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> • Measurement Conditions: Further details are available from the Validation Report at the end of this certificate. All figures stated in the certificate are valid at the frequency indicated. • Interpretation Parameters for TSL: The source is mounted in a touch configuration below the center marking of the flat phantom. • Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No.: CLA150-4025_Apr21 Page 2 of 6</p>			
Primary Standard	ID #	Cal. Cal. (Calibration No.)	Scheduled Calibration																																																								
Power meter NRP	SN: 104/76	05-Apr-21 (No. 217-0329)	Apr-22																																																								
Power sensor NRP-Z91	SN: 103/44	05-Apr-21 (No. 217-0329)	Apr-22																																																								
Power sensor NRP-Z91	SN: 103/24	06-Apr-21 (No. 217-0329)	Apr-22																																																								
Power sensor NRP-Z91	SN: 103/26	06-Apr-21 (No. 217-0329)	Apr-22																																																								
Trich-N Intensity Meter	SN: 00010000000000000000000000000000	04-Apr-21 (No. 217-0329)	Apr-22																																																								
Reference Probe DEXTRA (D4-4)	SN: 3877	30-Dec-20 (No. E3X3/177, Dec20)	Dec-21																																																								
Reference Probe DEXTRA (D4-4)	SN: 664	06-Jun-20 (No. D4E4-054, Jun20)	Jun-21																																																								
ID #	Check Date (in house)	Scheduled Check																																																									
Power meter E4441B	SN: 03410004/4	05-Apr-10 (in house check Jun-20)	In house check: Jun-22																																																								
Power meter E4441B	SN: 03410005/4	05-Apr-10 (in house check Jun-20)	In house check: Jun-22																																																								
Power sensor E4441A	SN: 00010210	05-Apr-10 (in house check Jun-20)	In house check: Jun-22																																																								
FF generator HP 8440C	SN: US4840U1700	04-Apr-09 (in house check Jun-20)	In house check: Jun-22																																																								
Network Analyzer Agilent E5080A	SN: US4840U0401	31-Mar-14 (in house check Oct-20)	In house check: Oct-21																																																								
<p>Measurement Conditions DASY system configuration, as far as not shown on page 1:</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY</th> <th>V52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>ELU4 Flat Phantom</td> <td>Shell thickness: 2 ± 0.2 mm</td> </tr> <tr> <td>EUT Positioning</td> <td>Touch Position</td> <td></td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy = 4.0 mm, dz = 1.4 mm</td> <td>Graded Ratio = 1.4 (Z direction)</td> </tr> <tr> <td>Frequency</td> <td colspan="2">150 MHz ± 1 MHz</td> </tr> </tbody> </table> <p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1"> <thead> <tr> <th>Nominal Head TSL parameters</th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>23.0 °C</td> <td>62.3</td> <td>0.75 mNm</td> <td></td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>51.1 ± 6 %</td> <td>0.75 mNm ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>< 0.5 °C</td> <td>---</td> <td>---</td> </tr> </tbody> </table> <p>SAR result with Head TSL</p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>1 W input power</td> <td>3.90 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>3.80 W/kg ± 18.4 % (n=2)</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>Condition</th> <th></th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>1 W input power</td> <td>2.60 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>2.59 W/kg ± 18.0 % (n=2)</td> </tr> </tbody> </table> <p>Certificate No.: CLA150-4025_Apr21 Page 3 of 6</p>	DASY Version	DASY	V52.10.4	Extrapolation	Advanced Extrapolation		Phantom	ELU4 Flat Phantom	Shell thickness: 2 ± 0.2 mm	EUT Positioning	Touch Position		Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)	Frequency	150 MHz ± 1 MHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity	23.0 °C	62.3	0.75 mNm		Measured Head TSL parameters	(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mNm ± 6 %	Head TSL temperature change during test	< 0.5 °C	---	---	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	1 W input power	3.90 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	3.80 W/kg ± 18.4 % (n=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	1 W input power	2.60 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (n=2)	<p>Appendix (Additional assessments outside the scope of SCS 0108)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>47.8 Ω ± 1.5 jΩ</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-31.4 dB</td> </tr> </tbody> </table> <p>Additional EUT Data</p> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPIAG</th> </tr> </thead> </table> <p>Certificate No.: CLA150-4025_Apr21 Page 4 of 6</p>	Impedance, transformed to feed point	47.8 Ω ± 1.5 jΩ	Return Loss	-31.4 dB	Manufactured by	SPIAG
DASY Version	DASY	V52.10.4																																																									
Extrapolation	Advanced Extrapolation																																																										
Phantom	ELU4 Flat Phantom	Shell thickness: 2 ± 0.2 mm																																																									
EUT Positioning	Touch Position																																																										
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)																																																									
Frequency	150 MHz ± 1 MHz																																																										
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																								
23.0 °C	62.3	0.75 mNm																																																									
Measured Head TSL parameters	(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mNm ± 6 %																																																								
Head TSL temperature change during test	< 0.5 °C	---	---																																																								
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																										
SAR measured	1 W input power	3.90 W/kg																																																									
SAR for nominal Head TSL parameters	normalized to 1W	3.80 W/kg ± 18.4 % (n=2)																																																									
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																										
SAR measured	1 W input power	2.60 W/kg																																																									
SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (n=2)																																																									
Impedance, transformed to feed point	47.8 Ω ± 1.5 jΩ																																																										
Return Loss	-31.4 dB																																																										
Manufactured by	SPIAG																																																										

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



DASY5 Validation Report for Head TSL

Date: 26.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DTU: CLA150; Type: CLA150; Serial: CLA150 - SN: 4025

Communication System: UID 0 - CW; Frequency: 150 MHz

Medium parameters used: $\epsilon = 150 \text{ S/m}$; $\epsilon_r = 51$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEC/IEC/ANSI C63.19-2011)

DASY5 Configuration

- Probe: EXIDV4 - SN3877; ConvF(12.51, 12.51, 12.51) @ 150 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA4B Snd654; Calibrated: 26.06.2020
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY5: 52.10.4(1527); SEMCAD X 14.6.14(7483)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan, distz=1.4mm (8x10x8) /Cube 0: Measurement grid: dxz=4mm, dy=4mm, dz=1.4mm

Reference SAR (extrapolated) = 7.36 W/kg

Peak SAR (extrapolated) = 7.36 W/kg


SAR(1 g) = 3.90 W/kg; SAR(10 g) = 2.69 W/kg

Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 30mm)

Ratio of SAR at M2 to SAR at M1 = 80.4%

Maximum value of SAR (measured) = 5.48 W/kg

0 dB = 5.48 W/kg = 7.39 dBW/kg

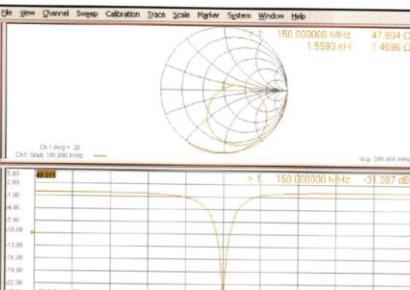1.2 D450V3 - SN 1103

<p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS-CN (Auden) Accreditation No.: SCS 0108</p>	<p>Schweizerischer Kalibrierdienst Service suisse d'kalibrage Servizio italiano di verifiche Servicio suizo de verificación Swiss Calibration Service</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Accreditation No.: SCS 0108</p>																																
<p>CALIBRATION CERTIFICATE</p>																																	
<p>Object: D450V3 - SN:1103</p>																																	
<p>Calibration procedure(s): QA CAL-15 v9 Calibration Procedure for SAR Validation Sources below 700 MHz</p>																																	
<p>Calibration date: April 21, 2021</p>																																	
<p>This calibration certificate documents the traceability to reference standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p>																																	
<p>All calibrations have been conducted in the closed laboratory facility; environment temperature (20 ± 3°C) and humidity - 70%.</p>																																	
<p>Calibration Equipment used (MUST critical for calibration):</p>																																	
<table border="1"> <thead> <tr> <th>Primary Standard</th> <th>Q #</th> <th>Cal Date (Certification No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power meter NIPF</td> <td>SN: 044778</td> <td>09-Apr-21 (No. 217-0281/108092)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor NIPF</td> <td>SN: 03524</td> <td>09-Apr-21 (No. 217-0281)</td> <td>Apr-22</td> </tr> <tr> <td>Power sensor MPR-ZH1</td> <td>SN: 03525</td> <td>09-Apr-21 (No. 217-0281)</td> <td>Apr-22</td> </tr> <tr> <td>Reference 20 dB Attenuator</td> <td>SN: C2020 D96</td> <td>09-Apr-21 (No. 217-0284)</td> <td>Apr-22</td> </tr> <tr> <td>Type N-male/female connector</td> <td>SN: 3-1082 / 0323</td> <td>09-Apr-21 (No. 217-0284)</td> <td>Apr-22</td> </tr> <tr> <td>Type N-male Probe E300V4</td> <td>SN: 04477</td> <td>30-Dec-20 (No. EK3-0077-De20)</td> <td>Dec-21</td> </tr> <tr> <td>DAKE</td> <td>SN: 044</td> <td>30-Jun-20 (No. DAKE 044_Jun20)</td> <td>Jun-21</td> </tr> </tbody> </table>		Primary Standard	Q #	Cal Date (Certification No.)	Scheduled Calibration	Power meter NIPF	SN: 044778	09-Apr-21 (No. 217-0281/108092)	Apr-22	Power sensor NIPF	SN: 03524	09-Apr-21 (No. 217-0281)	Apr-22	Power sensor MPR-ZH1	SN: 03525	09-Apr-21 (No. 217-0281)	Apr-22	Reference 20 dB Attenuator	SN: C2020 D96	09-Apr-21 (No. 217-0284)	Apr-22	Type N-male/female connector	SN: 3-1082 / 0323	09-Apr-21 (No. 217-0284)	Apr-22	Type N-male Probe E300V4	SN: 04477	30-Dec-20 (No. EK3-0077-De20)	Dec-21	DAKE	SN: 044	30-Jun-20 (No. DAKE 044_Jun20)	Jun-21
Primary Standard	Q #	Cal Date (Certification No.)	Scheduled Calibration																														
Power meter NIPF	SN: 044778	09-Apr-21 (No. 217-0281/108092)	Apr-22																														
Power sensor NIPF	SN: 03524	09-Apr-21 (No. 217-0281)	Apr-22																														
Power sensor MPR-ZH1	SN: 03525	09-Apr-21 (No. 217-0281)	Apr-22																														
Reference 20 dB Attenuator	SN: C2020 D96	09-Apr-21 (No. 217-0284)	Apr-22																														
Type N-male/female connector	SN: 3-1082 / 0323	09-Apr-21 (No. 217-0284)	Apr-22																														
Type N-male Probe E300V4	SN: 04477	30-Dec-20 (No. EK3-0077-De20)	Dec-21																														
DAKE	SN: 044	30-Jun-20 (No. DAKE 044_Jun20)	Jun-21																														
<p>Secondary Standards</p>																																	
<table border="1"> <thead> <tr> <th>Q #</th> <th>Check Date (in hours)</th> <th>Scheduled Check</th> </tr> </thead> <tbody> <tr> <td>Point meter E4410B</td> <td>SN: E4410B/00074</td> <td>09-Apr-21 (No. 217-0281/108092)</td> </tr> <tr> <td>Power sensor E4412A</td> <td>SN: MVA1490002</td> <td>09-Apr-16 (in house check) Jun-20</td> </tr> <tr> <td>Power sensor E4412A</td> <td>SN: 00001010</td> <td>09-Apr-16 (in house check) Jun-20</td> </tr> <tr> <td>RF generator RF-BASIC</td> <td>SN: U5401001700</td> <td>09-Aug-19 (in house check) Jun-20</td> </tr> <tr> <td>Handheld Antenna Analyzer E300SA</td> <td>SN: U5401000727</td> <td>31-Mar-14 (in house check) Oct-20</td> </tr> </tbody> </table>		Q #	Check Date (in hours)	Scheduled Check	Point meter E4410B	SN: E4410B/00074	09-Apr-21 (No. 217-0281/108092)	Power sensor E4412A	SN: MVA1490002	09-Apr-16 (in house check) Jun-20	Power sensor E4412A	SN: 00001010	09-Apr-16 (in house check) Jun-20	RF generator RF-BASIC	SN: U5401001700	09-Aug-19 (in house check) Jun-20	Handheld Antenna Analyzer E300SA	SN: U5401000727	31-Mar-14 (in house check) Oct-20														
Q #	Check Date (in hours)	Scheduled Check																															
Point meter E4410B	SN: E4410B/00074	09-Apr-21 (No. 217-0281/108092)																															
Power sensor E4412A	SN: MVA1490002	09-Apr-16 (in house check) Jun-20																															
Power sensor E4412A	SN: 00001010	09-Apr-16 (in house check) Jun-20																															
RF generator RF-BASIC	SN: U5401001700	09-Aug-19 (in house check) Jun-20																															
Handheld Antenna Analyzer E300SA	SN: U5401000727	31-Mar-14 (in house check) Oct-20																															
<p>Calibrated by:</p>	<p>Name: Olafdo Leibler Function: Laboratory Technician </p>																																
<p>Approved by:</p>	<p>Name: Katja Pörsch Function: Technical Manager </p>																																
<p>Issued: April 23, 2021</p>																																	
<p>This calibration certificate should not be reproduced except in full without written approval of the laboratory.</p>																																	
<p>Certificate No.: D450V3-1103_Apr21 Page: 1 of 6</p>																																	
<p>Certificate No.: D450V3-1103_Apr21 Page: 2 of 6</p>																																	

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overhead, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>, and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-Document.aspx>. Any intervention by the Company in the documents does not constitute an endorsement. Any transfer of the document to a third party does not affect the validity of the document. Any alteration of the document by the Client or any third party is illegal and the Client is liable for any damage caused. Any alteration of the document by the Company is done at the Client's request and is subject to the Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN_DocCheck@sasrao.com

中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

<p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr><td>DASY Version</td><td>DAEY5</td><td>V62.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>ELI Par Phantom</td><td>Shell thickness: 2 ± 0.2 mm</td></tr> <tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 6 mm</td><td></td></tr> <tr><td>Frequency</td><td>450 MHz ± 1 MHz</td><td></td></tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1"> <tr><td>SAR averaged over 1 cm³ (1 g) of Head TSL</td><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>SAR measured</td><td>22.0 °C</td><td>43.5</td><td>0.87 mho/m</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>43.1 ± 6 %</td><td>0.87 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>< 0.5 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr><td>SAR averaged over 1 cm³ (1 g) of Head TSL</td><td>Condition</td><td></td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>1.14 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>4.88 W/kg ± 16.1 % (k=2)</td></tr> </table> <table border="1"> <tr><td>SAR averaged over 10 cm³ (10 g) of Head TSL</td><td>Condition</td><td></td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>0.757 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>3.06 W/kg ± 17.5 % (k=2)</td></tr> </table>	DASY Version	DAEY5	V62.10.4	Extrapolation	Advanced Extrapolation		Phantom	ELI Par Phantom	Shell thickness: 2 ± 0.2 mm	Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 6 mm		Frequency	450 MHz ± 1 MHz		SAR averaged over 1 cm ³ (1 g) of Head TSL	Temperature	Permittivity	Conductivity	SAR measured	22.0 °C	43.5	0.87 mho/m	SAR for nominal Head TSL parameters	(22.0 ± 0.2) °C	43.1 ± 6 %	0.87 mho/m ± 6 %	Head TSL temperature change during test	< 0.5 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	1.14 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	4.88 W/kg ± 16.1 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	0.757 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg ± 17.5 % (k=2)	<p>Appendix (Additional assessments outside the scope of SCS 0106)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr><td>Impedance, transformed to feed point</td><td>57.1 Ω ± 2.8 jΩ</td></tr> <tr><td>Return Loss</td><td>-23.0 dB</td></tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr><td>Electrical Delay (one direction)</td><td>1.346 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of this dipole near the feedpoint can be measured. The dipole is made of standard singlelead coaxial cable. The center conductor of the feeding line is directly connected to the second end of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are also present. These are used in order to improve matching when located according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No electrical force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table>	Impedance, transformed to feed point	57.1 Ω ± 2.8 jΩ	Return Loss	-23.0 dB	Electrical Delay (one direction)	1.346 ns	Manufactured by	SPEAG
DASY Version	DAEY5	V62.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	ELI Par Phantom	Shell thickness: 2 ± 0.2 mm																																																											
Distance Dipole Center - TSL	15 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 6 mm																																																												
Frequency	450 MHz ± 1 MHz																																																												
SAR averaged over 1 cm ³ (1 g) of Head TSL	Temperature	Permittivity	Conductivity																																																										
SAR measured	22.0 °C	43.5	0.87 mho/m																																																										
SAR for nominal Head TSL parameters	(22.0 ± 0.2) °C	43.1 ± 6 %	0.87 mho/m ± 6 %																																																										
Head TSL temperature change during test	< 0.5 °C	—	—																																																										
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	1.14 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	4.88 W/kg ± 16.1 % (k=2)																																																											
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	0.757 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg ± 17.5 % (k=2)																																																											
Impedance, transformed to feed point	57.1 Ω ± 2.8 jΩ																																																												
Return Loss	-23.0 dB																																																												
Electrical Delay (one direction)	1.346 ns																																																												
Manufactured by	SPEAG																																																												
<p>Certificate No: D450V3-1103_Apr21 Page 3 of 6</p> <p>DASY5 Validation Report for Head TSL</p> <p>Date: 21.04.2021</p> <p>Test Laboratory: SPEAG, Zurich, Switzerland</p> <p>DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3-3-SN:1103</p> <p>Communication System: UID 0 - CW; Frequency: 450 MHz</p> <p>Medium parameters used: f = 450 MHz; σ = 0.87 S/m; ε_r = 43.1; ρ = 1000 kg/m³</p> <p>Phantom section: Flat Section</p> <p>Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)</p> <p>DASY52 Configuration:</p> <ul style="list-style-type: none"> • Probe: EX3DV4 - SN3877; ConvF10.64, 10.64, 10.64) @ 450 MHz; Calibrated: 30.12.2020 • Sensor-Surface: 1-mm (Mechanical Surface Detection) • Electronics: DAEF4 Soe654; Calibrated: 26.06.2020 • Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP1003 • DASY52 S2.10.4(S27); SEMCAD X 14.6.14(7483) <p>Dipole Calibration for Head Tissue(d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference value: 39.18 V/m; Power Drift = 0.08 dB Peak SAR (extrapolated) = 1.76 W/kg SAR1 g = 1.14 W/kg; SAR10 g = 0.767 W/kg Small differences in peaks to all points 3 dB below: Larger than measurement grid Ratio of SAR at M2 to SAR at M1 = 64.9% Maximum value of SAR (measured) = 1.53 W/kg</p> <p></p> <p>0 dB = 1.53 W/kg = 1.85 dBW/kg</p> <p>Certificate No: D450V3-1103_Apr21 Page 5 of 6</p> <p>Certificate No: D450V3-1103_Apr21 Page 4 of 6</p> <p></p> <p>Certificate No: D450V3-1103_Apr21 Page 6 of 6</p>																																																													

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



1.3 D750V3 - SN 1188

    <p>Client SGS-CN Certificate No: Z22-60103</p> <p>CALIBRATION CERTIFICATE</p> <p>Object D750V3 - SN: 1188</p> <p>Calibration Procedure(s) FF-211-003-01 Calibration Procedures for dipole validation kit</p> <p>Calibration date: March 29, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity<70%.</p> <p>Calibration Equipment used (MATE critical for calibration)</p> <table border="1"> <tr> <td>Primary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Power Meter NRP2</td> <td>105277</td> <td>24-Sep-21 (CITL, No.J21X08329)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP85</td> <td>104291</td> <td>24-Sep-21 (CITL, No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX304VA</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No. EX3-7307...May21)</td> <td>May-22</td> </tr> <tr> <td>DAE SN 1556</td> <td></td> <td>12-Jan-22 (CITL-SPEAG No.22-60007)</td> <td>Jan-23</td> </tr> <tr> <td>Secondary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY46071430</td> <td>13-Jan-22 (CITL, No.J22X0409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CITL, No.J22X0406)</td> <td>Jan-23</td> </tr> </table> <p>Calibrated by: Zhao Jing SAR Test Engineer</p> <p>Reviewed by: Lin Hao SAR Test Engineer</p> <p>Approved by: Qi Dianyuan SAR Project Leader</p> <p>Issued: April 3, 2022</p> <p>Certificate No: Z22-60103 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	105277	24-Sep-21 (CITL, No.J21X08329)	Sep-22	Power sensor NRP85	104291	24-Sep-21 (CITL, No.J21X08326)	Sep-22	Reference Probe EX304VA	SN 7307	26-May-21 (SPEAG No. EX3-7307...May21)	May-22	DAE SN 1556		12-Jan-22 (CITL-SPEAG No.22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY46071430	13-Jan-22 (CITL, No.J22X0409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CITL, No.J22X0406)	Jan-23	   <p>Client SGS-CN Certificate No: Z22-60103</p> <p>Glossary:</p> <p>TSL tissue simulating liquid ConfF sensitivity in TSL / NORMxyz N/A not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IC/IEEE 2029-1992, Standard Test Method for Measurement of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Measurement</p> <p>b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation:</p> <p>c) DASY400 System Handbook</p> <p>Method Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed position under the liquid phantom. The impedance stated is transformed from the measured impedance at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid phantom. The impedance stated is transformed from the measured impedance at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. SAR measured: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60103 Page 2 of 6</p>																					
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																			
Power Meter NRP2	105277	24-Sep-21 (CITL, No.J21X08329)	Sep-22																																																			
Power sensor NRP85	104291	24-Sep-21 (CITL, No.J21X08326)	Sep-22																																																			
Reference Probe EX304VA	SN 7307	26-May-21 (SPEAG No. EX3-7307...May21)	May-22																																																			
DAE SN 1556		12-Jan-22 (CITL-SPEAG No.22-60007)	Jan-23																																																			
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																			
Signal Generator E4438C	MY46071430	13-Jan-22 (CITL, No.J22X0409)	Jan-23																																																			
Network Analyzer E5071C	MY46110673	14-Jan-22 (CITL, No.J22X0406)	Jan-23																																																			
   <p>Client SGS-CN Certificate No: Z22-60103</p> <p>Measurement Conditions</p> <p>DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY92</td> <td>V52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz < 5 mm</td> </tr> <tr> <td>Frequency</td> <td>750 MHz ± 1 MHz</td> </tr> </table> <p>Head TSL parameters</p> <p>The following parameters and calculations were applied.</p> <table border="1"> <tr> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>42.0</td> <td>0.90 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>41.4 ± 6 %</td> <td>0.89 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> <td>—</td> </tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>2.07 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>8.27 W/kg ± 18.8 % (n=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>1.37 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>5.48 W/kg ± 18.7 % (n=2)</td> </tr> </table> <p>Certificate No: Z22-60103 Page 3 of 6</p>	DASY Version	DASY92	V52.10.4	Extrapolation	Advanced Extrapolation	Phantom	Triple Flat Phantom 5.1C	Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz < 5 mm	Frequency	750 MHz ± 1 MHz	Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	SAR measured	250 mW input power	2.07 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (n=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	SAR measured	250 mW input power	1.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (n=2)	   <p>Client SGS-CN Certificate No: Z22-60103</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>53.6Ω ± 1.1Ω</td> </tr> <tr> <td>Return Loss</td> <td>-28.7dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>0.947 ns</td> </tr> </table> <p>After long term use with 100mW radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The matching of the antenna is as required by the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p>Certificate No: Z22-60103 Page 4 of 6</p>	Impedance, transformed to feed point	53.6Ω ± 1.1Ω	Return Loss	-28.7dB	Electrical Delay (one direction)	0.947 ns	Manufactured by	SPEAG
DASY Version	DASY92	V52.10.4																																																				
Extrapolation	Advanced Extrapolation																																																					
Phantom	Triple Flat Phantom 5.1C																																																					
Distance Dipole Center - TSL	15 mm	with Spacer																																																				
Zoom Scan Resolution	dx, dy, dz < 5 mm																																																					
Frequency	750 MHz ± 1 MHz																																																					
Temperature	Permittivity	Conductivity																																																				
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m																																																			
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %																																																			
Head TSL temperature change during test	<1.0 °C	—	—																																																			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																					
SAR measured	250 mW input power	2.07 W/kg																																																				
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (n=2)																																																				
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																					
SAR measured	250 mW input power	1.37 W/kg																																																				
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (n=2)																																																				
Impedance, transformed to feed point	53.6Ω ± 1.1Ω																																																					
Return Loss	-28.7dB																																																					
Electrical Delay (one direction)	0.947 ns																																																					
Manufactured by	SPEAG																																																					


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)5735888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)5735888 f(86-512)57370818 sgs.china@sgs.com




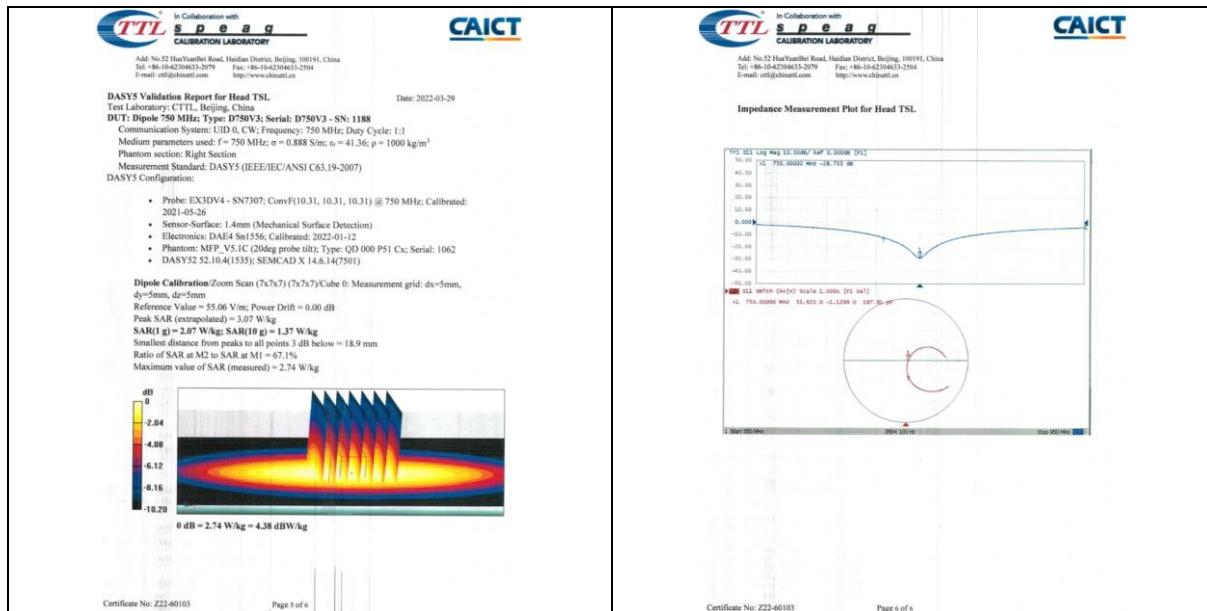


1.4 D835V2 - SN 4d114

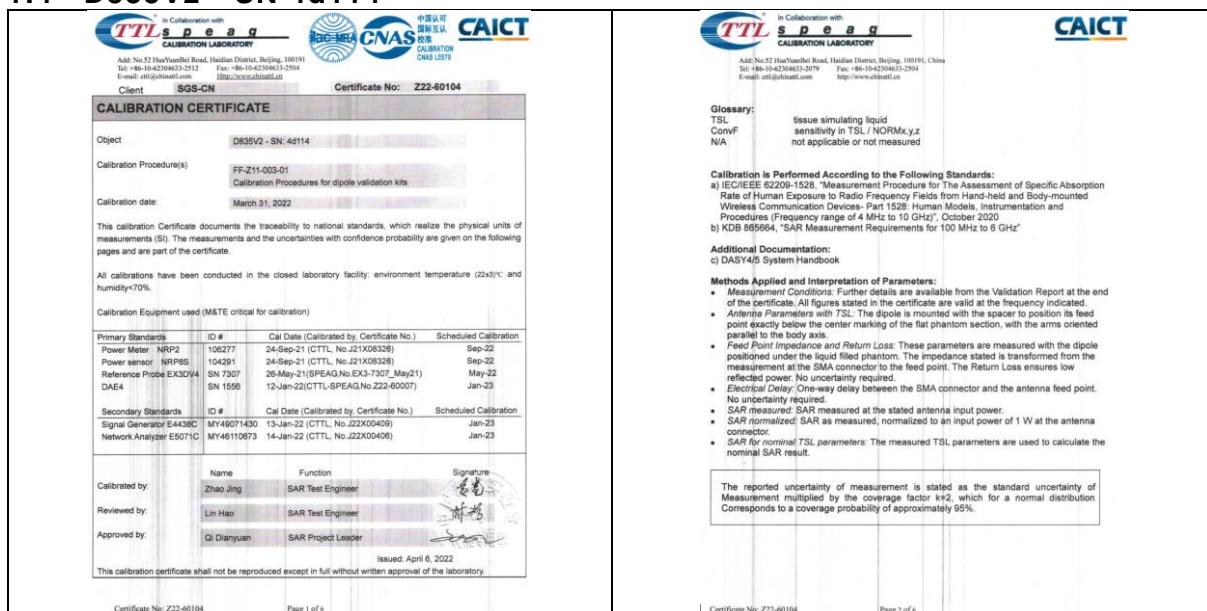

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

If you need the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
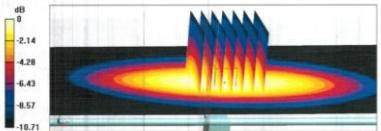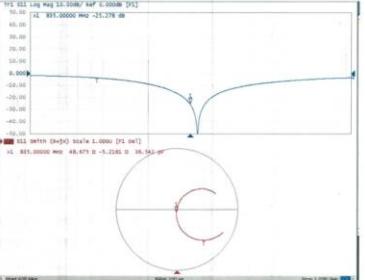
<p>TTI SPEAG CALIBRATION LABORATORY Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42306833-2079 Fax: +86-10-42306833-2564 E-mail: ctt@caict.net</p> <p>CAICT</p> <p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>DASY Version</td><td>DASY2</td><td>V5.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>15 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>835 MHz ± 1 MHz</td><td></td></tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>22.0 °C</td><td>41.5</td><td>0.90 mho/m</td></tr> <tr><td>Nominal Head TSL parameters</td><td></td><td></td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>41.0 ± 6 % 0.91 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power 2.37 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W 9.40 W/kg ± 10.8 % (k=2)</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power 1.54 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W 6.12 W/kg ± 18.7 % (k=2)</td></tr> </table> <p>Certificate No: Z22-60104 Page 3 of 6</p>	DASY Version	DASY2	V5.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	835 MHz ± 1 MHz		Temperature	Permittivity	Conductivity	22.0 °C	41.5	0.90 mho/m	Nominal Head TSL parameters			Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 6 % 0.91 mho/m ± 6 %	Head TSL temperature change during test	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	250 mW input power 2.37 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 9.40 W/kg ± 10.8 % (k=2)	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	250 mW input power 1.54 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 6.12 W/kg ± 18.7 % (k=2)	<p>TTI SPEAG CALIBRATION LABORATORY Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42306833-2079 Fax: +86-10-42306833-2564 E-mail: ctt@caict.net</p> <p>CAICT</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>48.70-5.22Ω</td></tr> <tr><td>Return Loss</td><td>-25.3dB</td></tr> </table> <p>General Antenna Parameters and Design</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Electrical Delay (one direction)</td><td>1.307 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semigrid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is terminated with a non-grounded DC-signals. On some of the dipole arms, there are some sections of the dipole which are not connected in order to improve matching. These are added according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.</p> <p>It is recommended to not use the dipole in these sections, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table> <p>Certificate No: Z22-60104 Page 4 of 6</p>	Impedance, transformed to feed point	48.70-5.22Ω	Return Loss	-25.3dB	Electrical Delay (one direction)	1.307 ns	Manufactured by	SPEAG
DASY Version	DASY2	V5.10.4																																																				
Extrapolation	Advanced Extrapolation																																																					
Phantom	Triple Flat Phantom 5.1C																																																					
Distance Dipole Center - TSL	15 mm	with Spacer																																																				
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																					
Frequency	835 MHz ± 1 MHz																																																					
Temperature	Permittivity	Conductivity																																																				
22.0 °C	41.5	0.90 mho/m																																																				
Nominal Head TSL parameters																																																						
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 6 % 0.91 mho/m ± 6 %																																																				
Head TSL temperature change during test	—	—																																																				
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																					
SAR measured	250 mW input power 2.37 W/kg																																																					
SAR for nominal Head TSL parameters	normalized to 1W 9.40 W/kg ± 10.8 % (k=2)																																																					
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																					
SAR measured	250 mW input power 1.54 W/kg																																																					
SAR for nominal Head TSL parameters	normalized to 1W 6.12 W/kg ± 18.7 % (k=2)																																																					
Impedance, transformed to feed point	48.70-5.22Ω																																																					
Return Loss	-25.3dB																																																					
Electrical Delay (one direction)	1.307 ns																																																					
Manufactured by	SPEAG																																																					
<p>TTI SPEAG CALIBRATION LABORATORY Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42306833-2079 Fax: +86-10-42306833-2564 E-mail: ctt@caict.net</p> <p>CAICT</p> <p>DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2023-03-31</p> <p>DUT: Dipole K35 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114</p> <p>Communication System: UUD 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1</p> <p>Medium parameter used: $\epsilon = 835 \text{ MHz}$; $\sigma = 0.907 \text{ S/m}$; $\rho = 40.98 \text{ }\Omega$; $\mu = 1000 \text{ kg/m}^3$</p> <p>Phantom: Section R1a Section</p> <p>Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)</p> <p>DASY5 Configuration:</p> <ul style="list-style-type: none"> Probe: EXDV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2022-06-26 Sensor-Surface: 1.4mm (Mechanical Surface Detection) Electronics: DA4E-Sn1556; Calibrated: 2022-01-12 Phantom: MFP_V5.1C (2D/3D probe tilt); Type: QD 000 P51 Cx; Serial: 1062 52.10.4(1533); SEMCAD X 14.6.14(501) <p>Probe Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.88 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 3.56 W/kg SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg Smallest distance from peaks to all points 3 dB below = 15.8 mm Ratio of SAR at M2 to SAR at M1 = 66.2% Maximum value of SAR (measured) = 3.17 W/kg</p> <p></p> <p>0 dB = 3.17 W/kg = 5.01 dBW/kg</p> <p>Certificate No: Z22-60104 Page 5 of 6</p>	<p>TTI SPEAG CALIBRATION LABORATORY Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42306833-2079 Fax: +86-10-42306833-2564 E-mail: ctt@caict.net</p> <p>CAICT</p> <p>Impedance Measurement Plot for Head TSL</p> <p></p> <p>Certificate No: Z22-60104 Page 6 of 6</p>																																																					

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



1.5 D900V2 - SN 1d079

   <p>In Collaboration with SPEAG CALIBRATION LABORATORY Add: No. 52 Huayuanti Road, Haidian District, Beijing, 100091, China Tel: +86-10-6291-0017 E-mail: ctt@caict.ac.cn http://www.caict.ac.cn</p> <p>Client: SGS-CN Certificate No: Z22-60184</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: D900V2 - SN: 1d079</p> <p>Calibration Procedure(s): FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: June 7, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity 70%.</p> <p>Calibration Equipment used (MATE critical for calibration)</p> <table border="1"> <thead> <tr> <th>Primary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRPS</td> <td>106277</td> <td>24-Sep-21 (CTTL, No.J2108328)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRPS</td> <td>104291</td> <td>24-Sep-21 (CTTL, No.J2108329)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7464</td> <td>20-Jan-22 (SPEAG No. EX3-7464, Jan22)</td> <td>Jan-23</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL, SPEAG No. Z22-40007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Secondary Standards</th> <th>ID #</th> <th>Cal Date (Calibrated by, Certificate No.)</th> <th>Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator 6438C</td> <td>MY48071430</td> <td>13-Jan-22 (CTTL, No.J22304059)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY48110573</td> <td>14-Jan-22 (CTTL, No.J22304056)</td> <td>Jan-23</td> </tr> </tbody> </table> <p>Calibrated by: Zhao Jing SAR Test Engineer </p> <p>Reviewed by: Lin Hao SAR Test Engineer </p> <p>Approved by: Qi Dianyuan SAR Project Leader </p> <p>Issued: June 13, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60184 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRPS	106277	24-Sep-21 (CTTL, No.J2108328)	Sep-22	Power sensor NRPS	104291	24-Sep-21 (CTTL, No.J2108329)	Sep-22	Reference Probe EX3DV4	SN 7464	20-Jan-22 (SPEAG No. EX3-7464, Jan22)	Jan-23	DAE4	SN 1556	12-Jan-22 (CTTL, SPEAG No. Z22-40007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator 6438C	MY48071430	13-Jan-22 (CTTL, No.J22304059)	Jan-23	Network Analyzer E5071C	MY48110573	14-Jan-22 (CTTL, No.J22304056)	Jan-23	 <p>In Collaboration with SPEAG CALIBRATION LABORATORY Add: No. 52 Huayuanti Road, Haidian District, Beijing, 100091, China Tel: +86-10-6291-0017 E-mail: ctt@caict.ac.cn http://www.caict.ac.cn</p> <p>Glossary:</p> <ul style="list-style-type: none"> TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx.y.z N/A: not applicable or not measured <p>Calibration is Performed According to the Following Standards:</p> <ul style="list-style-type: none"> IEC 62626, "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Handheld and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 KDS 866964, "SAR Measurement Requirements for 100 MHz to 6 GHz" <p>Additional Documentation:</p> <ul style="list-style-type: none"> DAS40-Systemic Interpolation <p>Method, Application and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point at the center of the center mounting of the flat phantom section, with the arm oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole connected to a flat phantom section. The impedance is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay (one way delay between the SMA connector and the antenna feed point): No uncertainty required. SAR measured: SAR measured at the stated antenna input power. Normalized SAR: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60184 Page 2 of 6</p>																						
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																				
Power Meter NRPS	106277	24-Sep-21 (CTTL, No.J2108328)	Sep-22																																																				
Power sensor NRPS	104291	24-Sep-21 (CTTL, No.J2108329)	Sep-22																																																				
Reference Probe EX3DV4	SN 7464	20-Jan-22 (SPEAG No. EX3-7464, Jan22)	Jan-23																																																				
DAE4	SN 1556	12-Jan-22 (CTTL, SPEAG No. Z22-40007)	Jan-23																																																				
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																				
Signal Generator 6438C	MY48071430	13-Jan-22 (CTTL, No.J22304059)	Jan-23																																																				
Network Analyzer E5071C	MY48110573	14-Jan-22 (CTTL, No.J22304056)	Jan-23																																																				
   <p>In Collaboration with SPEAG CALIBRATION LABORATORY Add: No. 52 Huayuanti Road, Haidian District, Beijing, 100091, China Tel: +86-10-6291-0017 E-mail: ctt@caict.ac.cn http://www.caict.ac.cn</p> <p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1"> <thead> <tr> <th>DASY Version</th> <th>DASY2</th> <th>52.10.4</th> </tr> </thead> <tbody> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>15 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>900 MHz ± 1 MHz</td> <td></td> </tr> </tbody> </table> <p>Head TSL parameters: The following parameters and calculations were applied.</p> <table border="1"> <thead> <tr> <th></th> <th>Temperature</th> <th>Permittivity</th> <th>Conductivity</th> </tr> </thead> <tbody> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>41.5</td> <td>0.97 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>(22.0 ± 0.2) °C</td> <td>42.1 ± 9 %</td> <td>0.98 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td>41.0 °C</td> <td>—</td> <td>—</td> </tr> </tbody> </table> <p>SAR result with Head TSL:</p> <table border="1"> <thead> <tr> <th>SAR averaged over 1 cm³ (1 g) of Head TSL</th> <th>Condition</th> </tr> </thead> <tbody> <tr> <td>SAR measured</td> <td>250 mW Input power 2.76 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W 11.0 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <th>SAR averaged over 10 cm³ (10 g) of Head TSL</th> <th>Condition</th> </tr> <tr> <td>SAR measured</td> <td>250 mW Input power 1.78 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W 7.29 W/kg ± 18.7 % (k=2)</td> </tr> </tbody> </table> <p>Certificate No: Z22-60184 Page 3 of 6</p>	DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	15 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	900 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 9 %	0.98 mho/m ± 6 %	Head TSL temperature change during test	41.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	SAR measured	250 mW Input power 2.76 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 11.0 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	SAR measured	250 mW Input power 1.78 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 7.29 W/kg ± 18.7 % (k=2)	 <p>In Collaboration with SPEAG CALIBRATION LABORATORY Add: No. 52 Huayuanti Road, Haidian District, Beijing, 100091, China Tel: +86-10-6291-0017 E-mail: ctt@caict.ac.cn http://www.caict.ac.cn</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <thead> <tr> <th>Impedance, transformed to feed point</th> <th>48.10-6.49(j)</th> </tr> </thead> <tbody> <tr> <td>Return Loss</td> <td>-23.3 dB</td> </tr> </tbody> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <thead> <tr> <th>Electrical Delay (one direction)</th> <th>1.312 ns</th> </tr> </thead> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be observed.</p> <p>The dipole is made of standard ferrite-coated cable. The center conductor of the feed line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited to the ground plane in some of the dipoles, small end caps are added to the dipole arms in order to improve matching when tested according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change.</p> <p>No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <thead> <tr> <th>Manufactured by</th> <th>SPEAG</th> </tr> </thead> </table> <p>Certificate No: Z22-60184 Page 4 of 6</p>	Impedance, transformed to feed point	48.10-6.49(j)	Return Loss	-23.3 dB	Electrical Delay (one direction)	1.312 ns	Manufactured by	SPEAG
DASY Version	DASY2	52.10.4																																																					
Extrapolation	Advanced Extrapolation																																																						
Phantom	Triple Flat Phantom 5.1C																																																						
Distance Dipole Center - TSL	15 mm	with Spacer																																																					
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																						
Frequency	900 MHz ± 1 MHz																																																						
	Temperature	Permittivity	Conductivity																																																				
Nominal Head TSL parameters	22.0 °C	41.5	0.97 mho/m																																																				
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 9 %	0.98 mho/m ± 6 %																																																				
Head TSL temperature change during test	41.0 °C	—	—																																																				
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																						
SAR measured	250 mW Input power 2.76 W/kg																																																						
SAR for nominal Head TSL parameters	normalized to 1W 11.0 W/kg ± 18.8 % (k=2)																																																						
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																						
SAR measured	250 mW Input power 1.78 W/kg																																																						
SAR for nominal Head TSL parameters	normalized to 1W 7.29 W/kg ± 18.7 % (k=2)																																																						
Impedance, transformed to feed point	48.10-6.49(j)																																																						
Return Loss	-23.3 dB																																																						
Electrical Delay (one direction)	1.312 ns																																																						
Manufactured by	SPEAG																																																						


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention is drawn to the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



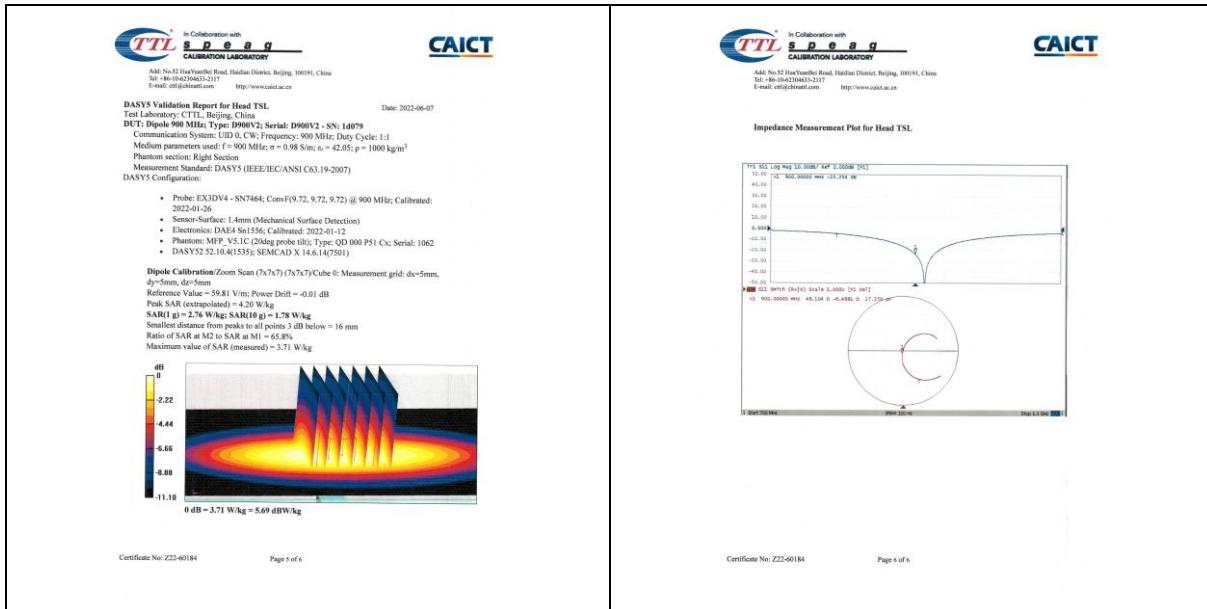

1.6 D1800V2 - SN 2d170

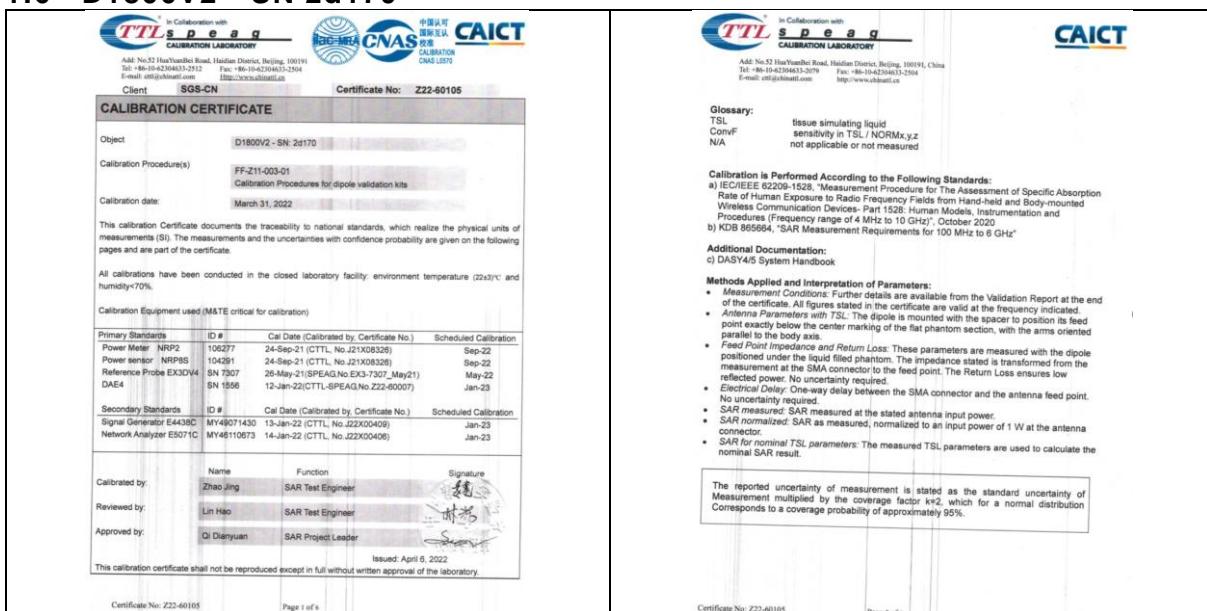

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com



Compliance Certification Services (Kunshan) Inc.
EMC Laboratory

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300

中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn

t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com
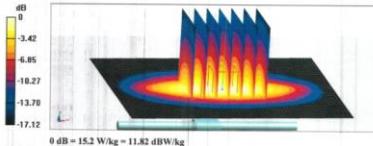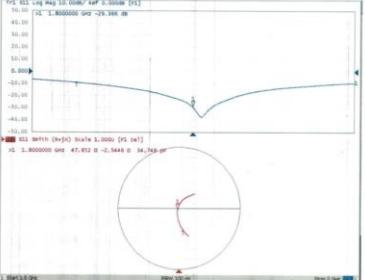
<p>TTL s p e a g CALIBRATION LABORATORY</p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366332-2079 Fax: +86-10-62366332-2504 E-mail: ctll@chinastl.com http://www.chinastl.com</p> <p>CAICT</p> <p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>DASY Version</td><td>DASY52</td><td>52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>1800 MHz ± 1 MHz</td><td></td></tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><th></th><th>Temperature</th><th>Permittivity</th><th>Conductivity</th></tr> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>40.0</td><td>1.40 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>40.6 ± 5 %</td><td>1.41 mho/m ± 5 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>+1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><th></th><th>Condition</th></tr> <tr><td>SAR measured</td><td>250 mW input power 9.73 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W 38.8 W/kg ± 18.8 % (k=2)</td></tr> <tr><td>SAR averaged over 10. cm³ (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power 5.11 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W 20.4 W/kg ± 18.7 % (k=2)</td></tr> </table> <p>Certificate No: Z22-60105 Page 1 of 6</p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	1800 MHz ± 1 MHz			Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 5 %	1.41 mho/m ± 5 %	Head TSL temperature change during test	+1.0 °C	—	—		Condition	SAR measured	250 mW input power 9.73 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 38.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10. cm ³ (10 g) of Head TSL	Condition	SAR measured	250 mW input power 5.11 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 20.4 W/kg ± 18.7 % (k=2)	<p>TTL s p e a g CALIBRATION LABORATORY</p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366332-2079 Fax: +86-10-62366332-2504 E-mail: ctll@chinastl.com http://www.chinastl.com</p> <p>CAICT</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>47.80 ± 2.54Ω</td></tr> <tr><td>Return Loss</td><td>-29.4dB</td></tr> </table> <p>General Antenna Parameters and Design</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Electrical Delay (one direction)</td><td>1.116 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The center conductor of the feeding line is directly soldered to the feed-point of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipole's small end caps are added to the feed-point area some additional resistors, which are soldered according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.</p> <p>No excessive bending of the dipole is recommended, especially in the feed-point area, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table> <p>Certificate No: Z22-60105 Page 4 of 6</p>	Impedance, transformed to feed point	47.80 ± 2.54Ω	Return Loss	-29.4dB	Electrical Delay (one direction)	1.116 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																					
Extrapolation	Advanced Extrapolation																																																						
Phantom	Triple Flat Phantom 5.1C																																																						
Distance Dipole Center - TSL	10 mm	with Spacer																																																					
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																						
Frequency	1800 MHz ± 1 MHz																																																						
	Temperature	Permittivity	Conductivity																																																				
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m																																																				
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.6 ± 5 %	1.41 mho/m ± 5 %																																																				
Head TSL temperature change during test	+1.0 °C	—	—																																																				
	Condition																																																						
SAR measured	250 mW input power 9.73 W/kg																																																						
SAR for nominal Head TSL parameters	normalized to 1W 38.8 W/kg ± 18.8 % (k=2)																																																						
SAR averaged over 10. cm ³ (10 g) of Head TSL	Condition																																																						
SAR measured	250 mW input power 5.11 W/kg																																																						
SAR for nominal Head TSL parameters	normalized to 1W 20.4 W/kg ± 18.7 % (k=2)																																																						
Impedance, transformed to feed point	47.80 ± 2.54Ω																																																						
Return Loss	-29.4dB																																																						
Electrical Delay (one direction)	1.116 ns																																																						
Manufactured by	SPEAG																																																						
<p>TTL s p e a g CALIBRATION LABORATORY</p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366332-2079 Fax: +86-10-62366332-2504 E-mail: ctll@chinastl.com http://www.chinastl.com</p> <p>CAICT</p> <p>DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-03-31</p> <p>DUT: Dipole 1800 MHz; Type: D1800V2; Serial: D1800V2 - SN: 2d170 Communication System: ID 0, CW, Frequency: 1800 MHz, Duty Cycle: 1:1 Medium: Air Medium temperature used: T = 1800 MHz; $\sigma = 1.411 \text{ S/m}$; $\epsilon_r = 40.62$; $\rho = 1000 \text{ kg/m}^3$ Phantom section: Right Sector Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)</p> <p>DASY5 Configuration:</p> <ul style="list-style-type: none"> • Probe: EXDV4 - SN7307; ConvF(8.34, 8.34, 8.34) @ 1800 MHz; Calibrated: 2021-05-26 • Sensor-Surface: 1.4mm (Mechanical Surface Detection) • Electronics: DAE4 Sn1556; Calibrated: 2022-01-12 • Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 • DASY5: 52.10.4(535); SEMCAD X 14.6.14(7501) <p>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 98.14 W/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 18.2 W/kg SAR(1 g) = 9.73 W/kg; SAR(10 g) = 5.11 W/kg Smallest distance from peaks to all points 3 dB below = 10 mm Ratio of SAR at M2 to SAR at M1 = 54% Maximum value of SAR (measured) = 15.2 W/kg</p>  <p>0 dB = 15.2 W/kg = 11.82 dBW/kg</p> <p>Certificate No: Z22-60105 Page 5 of 6</p>	<p>TTL s p e a g CALIBRATION LABORATORY</p> <p>Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62366332-2079 Fax: +86-10-62366332-2504 E-mail: ctll@chinastl.com http://www.chinastl.com</p> <p>CAICT</p> <p>Impedance Measurement Plot for Head TSL</p>  <p>Impedance (real): 47.80 ± 2.54Ω</p> <p>Impedance (imaginary): 2.54 ± 0.58j Ω</p> <p>Certificate No: Z22-60105 Page 6 of 6</p>																																																						

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



1.7 D1900V2 - SN 5d136

<div style="border: 1px solid black; padding: 10px;"> <p style="text-align: center;">    CALIBRATION CERTIFICATE </p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Object</td> <td colspan="2">D1900V2 - SN: 5d136</td> </tr> <tr> <td>Calibration Procedure(s)</td> <td colspan="2">FF-Z1-053-01 Calibration Procedures for dipole validation kits</td> </tr> <tr> <td>Calibration date</td> <td colspan="2">June 7, 2022</td> </tr> <tr> <td colspan="3">This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</td> </tr> <tr> <td colspan="3">All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity >70%.</td> </tr> <tr> <td colspan="3">Calibration Equipment used (M&TE critical for calibration)</td> </tr> <tr> <td>Primary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Power Meter NRP2</td> <td>105377</td> <td>24-Sep-21 (CTTL No.21X08528)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP8</td> <td>04289</td> <td>24-Sep-21 (CTTL No.21X08529)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX2DV4</td> <td>SN 7454</td> <td>20-Jun-22 (CTTL-SPEAG No.22Z40007)</td> <td>Jan-23</td> </tr> <tr> <td>DKE4</td> <td>SN 1559</td> <td>12-Jan-22 (CTTL-SPEAG No.22Z40007)</td> <td>Jan-23</td> </tr> <tr> <td>Secondary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49071430</td> <td>13-Jan-22 (CTTL No.22Z00460)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY8110972</td> <td>14-Jan-22 (CTTL No.22Z00460)</td> <td>Jan-23</td> </tr> <tr> <td>Calibrated by:</td> <td>Name</td> <td>Function</td> <td>Signature</td> </tr> <tr> <td>Zhao Jing</td> <td>SAR Test Engineer</td> <td></td> <td></td> </tr> <tr> <td>Reviewed by:</td> <td>Liu Hao</td> <td>SAR Test Engineer</td> <td></td> </tr> <tr> <td>Approved by:</td> <td>Qi Dianyuan</td> <td>SAR Project Leader</td> <td></td> </tr> <tr> <td colspan="4" style="text-align: center;">Issued: June 13, 2022</td> </tr> <tr> <td colspan="4">This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</td> </tr> </table> <p style="text-align: center;">Certificate No: Z22-60185 Page 1 of 6</p> </div>	Object	D1900V2 - SN: 5d136		Calibration Procedure(s)	FF-Z1-053-01 Calibration Procedures for dipole validation kits		Calibration date	June 7, 2022		This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity >70%.			Calibration Equipment used (M&TE critical for calibration)			Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	105377	24-Sep-21 (CTTL No.21X08528)	Sep-22	Power sensor NRP8	04289	24-Sep-21 (CTTL No.21X08529)	Sep-22	Reference Probe EX2DV4	SN 7454	20-Jun-22 (CTTL-SPEAG No.22Z40007)	Jan-23	DKE4	SN 1559	12-Jan-22 (CTTL-SPEAG No.22Z40007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.22Z00460)	Jan-23	Network Analyzer E5071C	MY8110972	14-Jan-22 (CTTL No.22Z00460)	Jan-23	Calibrated by:	Name	Function	Signature	Zhao Jing	SAR Test Engineer			Reviewed by:	Liu Hao	SAR Test Engineer		Approved by:	Qi Dianyuan	SAR Project Leader		Issued: June 13, 2022				This calibration certificate shall not be reproduced except in full without written approval of the laboratory.				<div style="border: 1px solid black; padding: 10px;"> <p style="text-align: center;">    </p> <p>Glossary:</p> <ul style="list-style-type: none"> TSL: Issue simulating liquid ConvF: sensitivity in TSL / NORMx,y,z N/A: not applicable or not measured <p>Calibration is Performed According to the Following Standards:</p> <ol style="list-style-type: none"> a) IEC 626271-1, "Standard Test Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedure (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDDI 05564, "SAR Measurement Requirements for 100 MHz to 6 GHz" <p>Additional Documentation:</p> <ul style="list-style-type: none"> c) DASY45 and Harmonic <p>Methods Applied and Parameters:</p> <ul style="list-style-type: none"> • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the mounting of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned in the flat phantom section. The values stated are taken from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: No delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • Normalized SAR: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <div style="border: 1px solid black; padding: 5px; margin-top: 10px;"> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> </div> <p style="text-align: center;">Certificate No: Z22-60185 Page 2 of 6</p> </div>
Object	D1900V2 - SN: 5d136																																																																										
Calibration Procedure(s)	FF-Z1-053-01 Calibration Procedures for dipole validation kits																																																																										
Calibration date	June 7, 2022																																																																										
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.																																																																											
All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity >70%.																																																																											
Calibration Equipment used (M&TE critical for calibration)																																																																											
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																																								
Power Meter NRP2	105377	24-Sep-21 (CTTL No.21X08528)	Sep-22																																																																								
Power sensor NRP8	04289	24-Sep-21 (CTTL No.21X08529)	Sep-22																																																																								
Reference Probe EX2DV4	SN 7454	20-Jun-22 (CTTL-SPEAG No.22Z40007)	Jan-23																																																																								
DKE4	SN 1559	12-Jan-22 (CTTL-SPEAG No.22Z40007)	Jan-23																																																																								
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																																								
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.22Z00460)	Jan-23																																																																								
Network Analyzer E5071C	MY8110972	14-Jan-22 (CTTL No.22Z00460)	Jan-23																																																																								
Calibrated by:	Name	Function	Signature																																																																								
Zhao Jing	SAR Test Engineer																																																																										
Reviewed by:	Liu Hao	SAR Test Engineer																																																																									
Approved by:	Qi Dianyuan	SAR Project Leader																																																																									
Issued: June 13, 2022																																																																											
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																																																											
<div style="border: 1px solid black; padding: 10px;"> <p style="text-align: center;">    </p> <p>Measurement Conditions DASY45 system configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>DASY Version</td> <td>DASY2</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td colspan="2">Advanced Extrapolation</td> </tr> <tr> <td>Phantom</td> <td colspan="2">Triple Flat Phantom 5.1C</td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz = 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td colspan="2">1900 MHz ± 1 MHz</td> </tr> </table> <p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>22.0 °C</td> <td>40.0</td> <td>1.40 mho/m</td> </tr> </table> <p>Nominal Head TSL parameters (22.0 ± 0.2) °C 39.9 ± 6 % 1.39 mho/m ± 6 %</p> <p>Measured Head TSL parameters (21.6 ± 0.2) °C 39.9 ± 6 % 1.39 mho/m ± 6 %</p> <p>Head TSL temperature change during test +1.6 °C --- ---</p> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>9.95 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>40.0 W/kg ± 18.6 % (n=2)</td> </tr> </table> <p>SAR averaged over 10 cm³ (10 g) of Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.18 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>20.8 W/kg ± 18.7 % (n=2)</td> </tr> </table> <p style="text-align: center;">Certificate No: Z22-60185 Page 1 of 6</p> </div>	DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	1900 MHz ± 1 MHz		Temperature	Permittivity	Conductivity	22.0 °C	40.0	1.40 mho/m	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	9.95 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.6 % (n=2)	SAR measured	250 mW input power	5.18 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (n=2)	<div style="border: 1px solid black; padding: 10px;"> <p style="text-align: center;">    </p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Impedance, transformed to feed point</td> <td>51.20 ± 7.88Ω</td> </tr> <tr> <td>Return Loss</td> <td>-22.4dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Electrical Delay (one direction)</td> <td>1.109 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The antenna is made of standard aluminum coaxial cable. The center conductor of the feedline has a diameter of the second arm of the dipole. The antenna is inserted into a connector for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when used according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by the addition of the end caps, as they are not considered according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p style="text-align: center;">Certificate No: Z22-60185 Page 4 of 6</p> </div>	Impedance, transformed to feed point	51.20 ± 7.88Ω	Return Loss	-22.4dB	Electrical Delay (one direction)	1.109 ns	Manufactured by	SPEAG																											
DASY Version	DASY2	52.10.4																																																																									
Extrapolation	Advanced Extrapolation																																																																										
Phantom	Triple Flat Phantom 5.1C																																																																										
Distance Dipole Center - TSL	10 mm	with Spacer																																																																									
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																																										
Frequency	1900 MHz ± 1 MHz																																																																										
Temperature	Permittivity	Conductivity																																																																									
22.0 °C	40.0	1.40 mho/m																																																																									
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																																										
SAR measured	250 mW input power	9.95 W/kg																																																																									
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 18.6 % (n=2)																																																																									
SAR measured	250 mW input power	5.18 W/kg																																																																									
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (n=2)																																																																									
Impedance, transformed to feed point	51.20 ± 7.88Ω																																																																										
Return Loss	-22.4dB																																																																										
Electrical Delay (one direction)	1.109 ns																																																																										
Manufactured by	SPEAG																																																																										


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention is drawn to the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



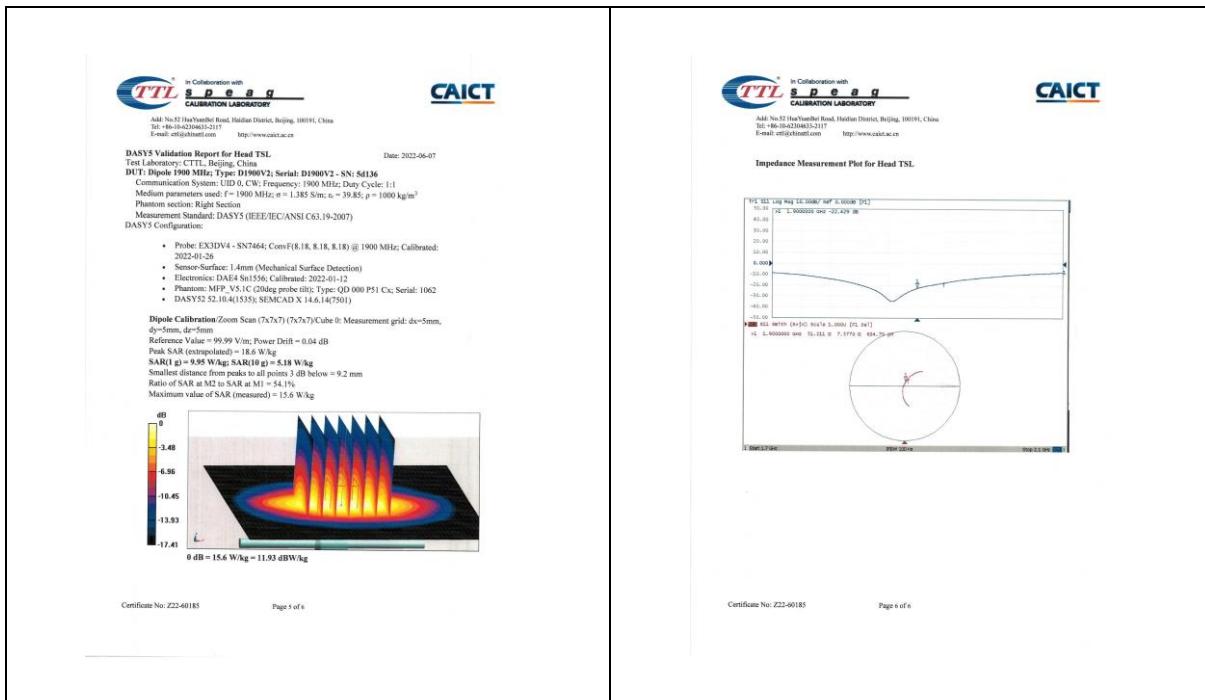

1.8 D2000V2 - SN 1041

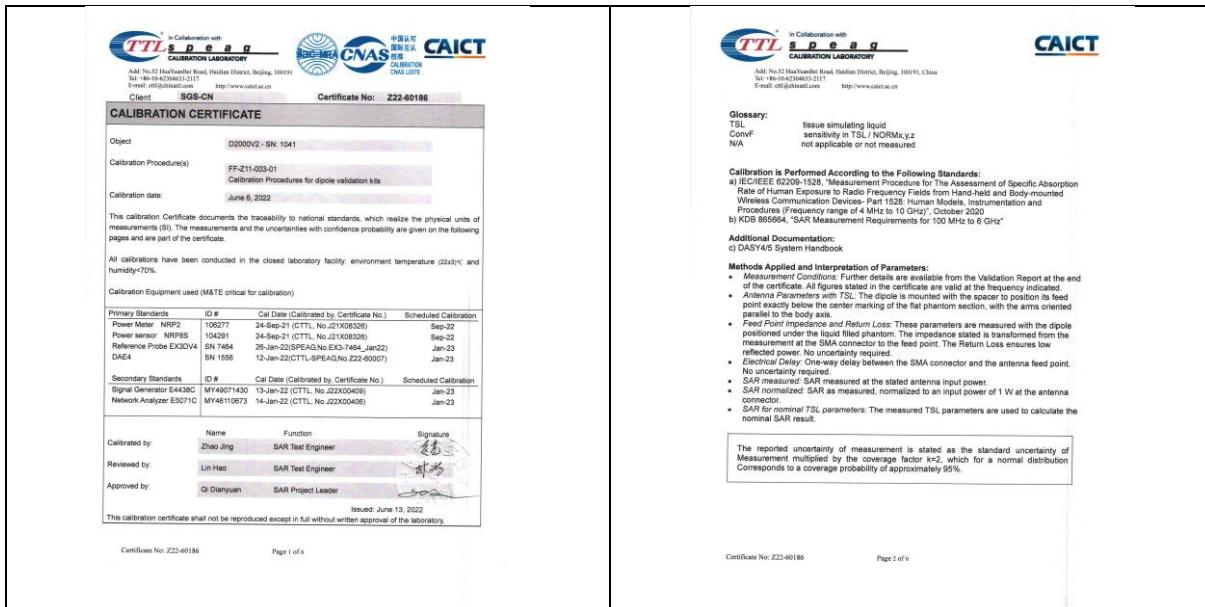

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

<p>SGS</p> <p>CAICT</p> <p>SGS in Collaboration with CAICT CALIBRATION LABORATORY Add: No.57 HuaYuanRoad, Haidian District, Beijing, 100091, China Tel: +86-10-64394613-2117 E-mail: caict@caict.ac.cn http://www.caict.ac.cn</p> <p>Measurement Conditions DASY5 system configuration, as far as given on page 1</p> <table border="1"> <tr><td>DASY Version</td><td>DASY52</td><td>52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zero Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>2000 MHz ± 1 MHz</td><td></td></tr> </table> <p>Head TSL parameters The following parameters and calculations were applied:</p> <table border="1"> <tr><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>40.0</td><td>1.40 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>40.2 ± 6 %</td><td>1.39 mho/m ± 9 %</td></tr> <tr><td>Head TSL temperature change during test</td><td>+1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr><td>SAR averaged over 1 cm³ (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>10.4 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>41.8 W/kg ± 18.8 % (n=2)</td></tr> <tr><td>SAR averaged over 10 cm³ (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>6.30 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>21.3 W/kg ± 16.7 % (n=2)</td></tr> </table> <p>Certificate No: Z22-60186 Page 1 of 6</p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zero Scan Resolution	dx, dy, dz = 5 mm		Frequency	2000 MHz ± 1 MHz		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 9 %	Head TSL temperature change during test	+1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	SAR measured	250 mW input power	10.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 18.8 % (n=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	SAR measured	250 mW input power	6.30 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 16.7 % (n=2)	<p>SGS in Collaboration with CAICT CALIBRATION LABORATORY Add: No.57 HuaYuanRoad, Haidian District, Beijing, 100091, China Tel: +86-10-64394613-2117 E-mail: caict@caict.ac.cn http://www.caict.ac.cn</p> <p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr><td>Impedance, Transformed to feed point</td><td>48.4Ω ± 0.7Ω</td></tr> <tr><td>Return Loss</td><td>-34.9dB</td></tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr><td>Electrical Delay (one direction)</td><td>1.088 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the other arms of the dipole, the center conductor is connected to the outer shield. The outer shield is soldered according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.</p> <p>No metal parts are soldered to the outer shield of the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table> <p>Certificate No: Z22-60186 Page 4 of 6</p>	Impedance, Transformed to feed point	48.4Ω ± 0.7Ω	Return Loss	-34.9dB	Electrical Delay (one direction)	1.088 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																								
Extrapolation	Advanced Extrapolation																																																									
Phantom	Triple Flat Phantom 5.1C																																																									
Distance Dipole Center - TSL	10 mm	with Spacer																																																								
Zero Scan Resolution	dx, dy, dz = 5 mm																																																									
Frequency	2000 MHz ± 1 MHz																																																									
Temperature	Permittivity	Conductivity																																																								
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m																																																							
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 9 %																																																							
Head TSL temperature change during test	+1.0 °C	—	—																																																							
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																									
SAR measured	250 mW input power	10.4 W/kg																																																								
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 18.8 % (n=2)																																																								
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																									
SAR measured	250 mW input power	6.30 W/kg																																																								
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 16.7 % (n=2)																																																								
Impedance, Transformed to feed point	48.4Ω ± 0.7Ω																																																									
Return Loss	-34.9dB																																																									
Electrical Delay (one direction)	1.088 ns																																																									
Manufactured by	SPEAG																																																									
<p>SGS in Collaboration with CAICT CALIBRATION LABORATORY Add: No.57 HuaYuanRoad, Haidian District, Beijing, 100091, China Tel: +86-10-64394613-2117 E-mail: caict@caict.ac.cn http://www.caict.ac.cn</p> <p>DASY5 Validation Plot for Head TSL Date: 2022-06-06</p> <p>Test Laboratory: CAICT, Beijing, China DUT: Dipole 2000 MHz, Type: D2000V2, Serial: D2000V2 - SN: 1841 Communication System: UUD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2000 MHz; ε = 1.392; S/m; n = 40.21; ρ = 1000 kg/m³ Phantom: Triple, Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p> <ul style="list-style-type: none"> Probe: EX3DV4 - SN7464; ConvF(8.2, 8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26 Sensor-Surface: 1.4mm (Mechanical Surface Detection) Electronics: DASA-Sn1556; Calibrated: 2022-01-12 Phantom: MFP V3.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 DASY52 S2.10.14(1535); NEMCAD X 14.6(14750) <p>Dipole Calibration/Zoom Scan (7x7) (7x7) Cube: Measurement grid: dx=5mm, dy=5mm, dz=5mm</p> <p>Reference Value = 10.4 V/m; Power Drift = 0.03 dB</p> <p>Peak SAR (extrapolated) = 19.6 W/kg</p> <p>SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg</p> <p>Small peaks in SAR values at all points > 8 dB below ~9.1 mm</p> <p>Ratio of SAR at M2 to SAR at M1 = 1.89</p> <p>Maximum value of SAR (measured) = 16.3 W/kg</p> <p></p> <p>Certificate No: Z22-60186 Page 5 of 6</p>	<p>SGS in Collaboration with CAICT CALIBRATION LABORATORY Add: No.57 HuaYuanRoad, Haidian District, Beijing, 100091, China Tel: +86-10-64394613-2117 E-mail: caict@caict.ac.cn http://www.caict.ac.cn</p> <p>Impedance Measurement Plot for Head TSL</p> <p></p> <p>Certificate No: Z22-60186 Page 6 of 6</p>																																																									

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



1.9 D2300V2 - SN 1096

    <p>Client: SGS-CN Certificate No: Z22-60106</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: D2300V2 - SN 1096</p> <p>Calibration Procedure(s): FF-211-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: March 31, 2022</p> <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.</p> <p>Calibration equipment used (M&TE critical for calibration):</p> <table border="1"> <tr> <td>Primary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Power Meter NRP2</td> <td>105277</td> <td>24-Sep-21 (CTTL No.J21X05326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP85</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X05326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No. EX3-2307, May21)</td> <td>May-22</td> </tr> <tr> <td>DAE</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL SPEAG No. Z22-60007)</td> <td>Jan-23</td> </tr> <tr> <td>Secondary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Signal Generator E4438C</td> <td>MY49014130</td> <td>13-Jan-22 (CTTL No.J22X0409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL No.J22X0406)</td> <td>Jan-23</td> </tr> </table> <p>Calibrated by: Zhao Jing SAR Test Engineer Reviewed by: Lin Hao SAR Test Engineer Approved by: Qi Dianyuan SAR Project Leader</p> <p>Issued: April 6, 2022</p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Certificate No: Z22-60106 Page 1 of 6</p>		Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	105277	24-Sep-21 (CTTL No.J21X05326)	Sep-22	Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X05326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No. EX3-2307, May21)	May-22	DAE	SN 1556	12-Jan-22 (CTTL SPEAG No. Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4438C	MY49014130	13-Jan-22 (CTTL No.J22X0409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X0406)	Jan-23	  <p>In Collaboration with TTL s p e a g CALIBRATION LABORATORY</p> <p>Add: No.52 HuaYanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304813-2112 Fax: +86-10-62304813-2504 E-mail: off@caict.net.cn</p> <p>Glossary: TSL tissue simulating liquid ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards: IEC 62209-1523 "Measurement Procedure for the Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand- and Body-mounted Wireless Communication Devices- Part 1523: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KOB 865668 "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation: c) DASY4.6 System Handbook</p> <p>Methods Applied and Interpretation of Parameters:</p> <ul style="list-style-type: none"> Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point at the center of the center marking of the flat phantom section, with the arms oriented parallel to the body axis. Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid phantom. The impedance stated is transformed from the measured at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. Q-factor: SAR measured at the stated antenna input power. SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result. <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60106 Page 2 of 6</p>																		
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																	
Power Meter NRP2	105277	24-Sep-21 (CTTL No.J21X05326)	Sep-22																																																	
Power sensor NRP85	104291	24-Sep-21 (CTTL No.J21X05326)	Sep-22																																																	
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No. EX3-2307, May21)	May-22																																																	
DAE	SN 1556	12-Jan-22 (CTTL SPEAG No. Z22-60007)	Jan-23																																																	
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																	
Signal Generator E4438C	MY49014130	13-Jan-22 (CTTL No.J22X0409)	Jan-23																																																	
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X0406)	Jan-23																																																	
  <p>In Collaboration with TTL s p e a g CALIBRATION LABORATORY</p> <p>Add: No.52 HuaYanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304813-2079 Fax: +86-10-62304813-2504 E-mail: off@caict.net.cn</p> <p>Measurement Conditions DASY system configuration, as far as not given on page 1.</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY2</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz < 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2300 MHz ± 1 MHz</td> <td></td> </tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1"> <tr> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>22.0 °C</td> <td>39.5</td> <td>1.67 mho/m</td> </tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>12.4 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>48.2 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10 g) of Head TSL</td> <td>Condition</td> <td></td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power</td> <td>5.88 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W</td> <td>23.4 W/kg ± 18.7 % (k=2)</td> </tr> </table> <p>Certificate No: Z22-60106 Page 3 of 6</p>		DASY Version	DASY2	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz < 5 mm		Frequency	2300 MHz ± 1 MHz		Temperature	Permittivity	Conductivity	22.0 °C	39.5	1.67 mho/m	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	12.4 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	48.2 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	5.88 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)	<p>Appendix: Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>49.20.4.96(j)</td> </tr> <tr> <td>Return Loss</td> <td>-28.6dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.083 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi rigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded with the liquid phantom. Measurements are made with the center conductor short-circuited. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p>Certificate No: Z22-60106 Page 4 of 6</p>	Impedance, transformed to feed point	49.20.4.96(j)	Return Loss	-28.6dB	Electrical Delay (one direction)	1.083 ns	Manufactured by	SPEAG
DASY Version	DASY2	52.10.4																																																		
Extrapolation	Advanced Extrapolation																																																			
Phantom	Triple Flat Phantom 5.1C																																																			
Distance Dipole Center - TSL	10 mm	with Spacer																																																		
Zoom Scan Resolution	dx, dy, dz < 5 mm																																																			
Frequency	2300 MHz ± 1 MHz																																																			
Temperature	Permittivity	Conductivity																																																		
22.0 °C	39.5	1.67 mho/m																																																		
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																			
SAR measured	250 mW input power	12.4 W/kg																																																		
SAR for nominal Head TSL parameters	normalized to 1W	48.2 W/kg ± 18.8 % (k=2)																																																		
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																			
SAR measured	250 mW input power	5.88 W/kg																																																		
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)																																																		
Impedance, transformed to feed point	49.20.4.96(j)																																																			
Return Loss	-28.6dB																																																			
Electrical Delay (one direction)	1.083 ns																																																			
Manufactured by	SPEAG																																																			


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com




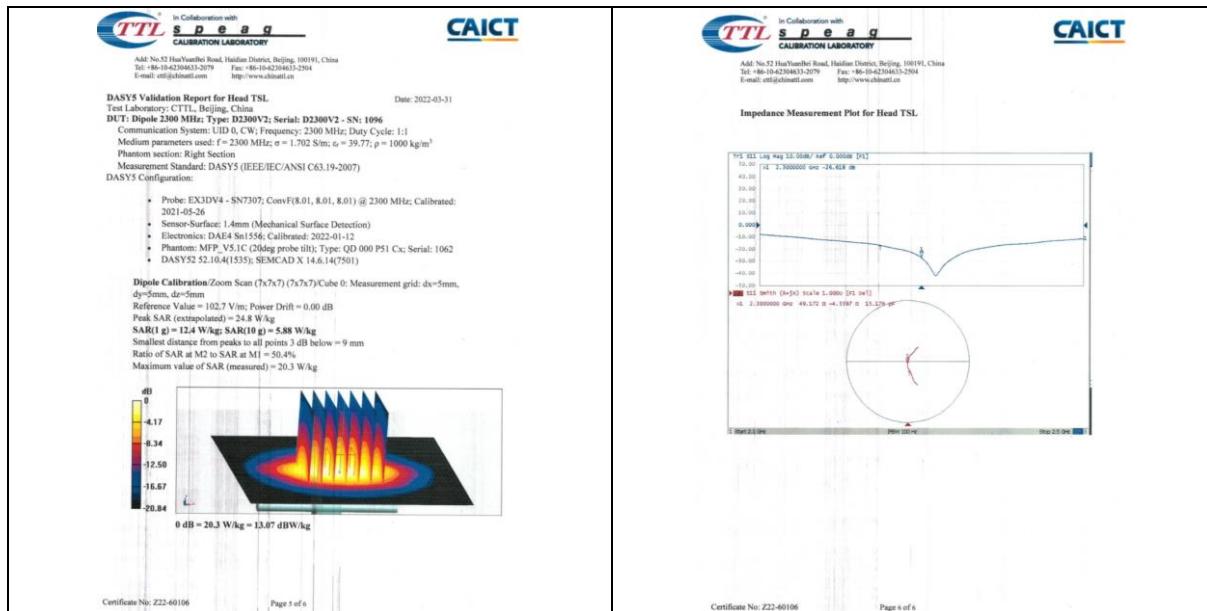


1.10 D2450V2 - SN 817

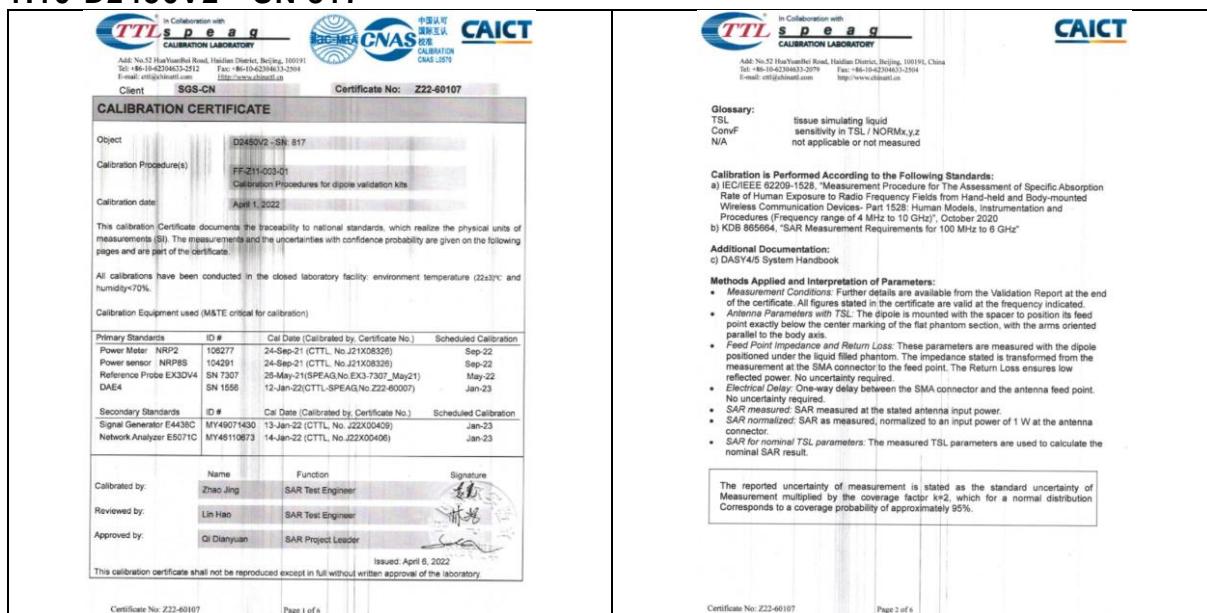

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To seek the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
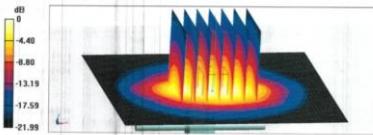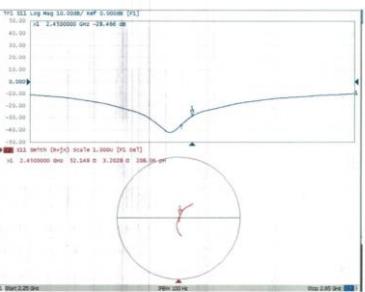
<p>Measurement Conditions DASY5 configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>DASY Version</td><td>DASY52</td><td>52.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Flat Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>dx, dy, dz = 5 mm</td><td></td></tr> <tr><td>Frequency</td><td>2450 MHz ± 1 MHz</td><td></td></tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>Temperature</td><td>Permittivity</td><td>Conductivity</td></tr> <tr><td>SAR measured</td><td>22.0 °C</td><td>39.2</td><td>1.80 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>39.5 ± 6 %</td><td>1.79 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm³ (1 g) of Head TSL</td><td>Condition</td><td></td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>13.2 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>63.6 W/kg ± 18.8 % (k=2)</td></tr> <tr><td>SAR averaged over 10 cm³ (10 g) of Head TSL</td><td>Condition</td><td></td></tr> <tr><td>SAR measured</td><td>250 mW input power</td><td>6.15 W/kg</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td><td>24.7 W/kg ± 18.7 % (k=2)</td></tr> </table> <p>Certificate No: Z22-60107 Page 2 of 6</p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz = 5 mm		Frequency	2450 MHz ± 1 MHz		Nominal Head TSL parameters	Temperature	Permittivity	Conductivity	SAR measured	22.0 °C	39.2	1.80 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		SAR measured	250 mW input power	13.2 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	63.6 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		SAR measured	250 mW input power	6.15 W/kg	SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)	<p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>52.1Ω ± 3.2Ω(j)</td></tr> <tr><td>Return Loss</td><td>-28.5dB</td></tr> </table> <p>General Antenna Parameters and Design</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Electrical Delay (one direction)</td><td>1.096 ns</td></tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semi-rigid coaxial cable. The outer conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited at DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this modification, because the dipole is still according to the Standard.</p> <p>No excessive force must be applied to the dipole antenna, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Manufactured by</td><td>SPEAG</td></tr> </table> <p>Certificate No: Z22-60107 Page 4 of 6</p>	Impedance, transformed to feed point	52.1Ω ± 3.2Ω(j)	Return Loss	-28.5dB	Electrical Delay (one direction)	1.096 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																											
Extrapolation	Advanced Extrapolation																																																												
Phantom	Triple Flat Phantom 5.1C																																																												
Distance Dipole Center - TSL	10 mm	with Spacer																																																											
Zoom Scan Resolution	dx, dy, dz = 5 mm																																																												
Frequency	2450 MHz ± 1 MHz																																																												
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity																																																										
SAR measured	22.0 °C	39.2	1.80 mho/m																																																										
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.5 ± 6 %	1.79 mho/m ± 6 %																																																										
Head TSL temperature change during test	<1.0 °C	—	—																																																										
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	13.2 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	63.6 W/kg ± 18.8 % (k=2)																																																											
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition																																																												
SAR measured	250 mW input power	6.15 W/kg																																																											
SAR for nominal Head TSL parameters	normalized to 1W	24.7 W/kg ± 18.7 % (k=2)																																																											
Impedance, transformed to feed point	52.1Ω ± 3.2Ω(j)																																																												
Return Loss	-28.5dB																																																												
Electrical Delay (one direction)	1.096 ns																																																												
Manufactured by	SPEAG																																																												
<p>DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-04-01</p> <p>DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 817 Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1 Medium: Water bath used; f = 2450 MHz; $\sigma = 1.79$ S/m; $\epsilon_r = 39.52$; $\rho = 1000$ kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration:</p> <ul style="list-style-type: none"> • Probe: EXIDV4 - SN7307; ConvF(7.75, 7.75, 7.75) @ 2450 MHz; Calibrated: 2021-05-26 • Sensor-Surface: 1.4mm (Mechanical Surface Detection) • Electronics: DAE4 S11556; Calibrated: 2022-01-12 • Phantom: MFP, V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 • DASY52 52.10.4(1535); SEMICAD X 14.6.14(7501) <p>Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 104.4 V/m; Power Drift = -0.03 dB Peak SAR (extrapolated) = 27.0 W/kg SAR(1 g) = 13.2 W/kg; SAR(10 g) = 6.15 W/kg Smallest distance from peaks to all points 3 dB below = 8.9 mm Ratio of SAR at M2 to SAR at M1 = 49.2% Maximum value of SAR (measured) = 22.1 W/kg</p>  <p>Certificate No: Z22-60107 Page 5 of 6</p>	<p>Impedance Measurement Plot for Head TSL</p>  <p>Certificate No: Z22-60107 Page 6 of 6</p>																																																												

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.


Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



1.11 D2600V2 - SN 1158

    <p>in Collaboration with TTL Speag CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-62304083-2512 Fax: +86-10-62304083-2504 E-mail: cn@caict.com</p> <p>Client SGS-CN Certificate No: Z22-60108</p> <p>CALIBRATION CERTIFICATE</p> <p>Object D2600V2 - SN: 1158</p> <p>Calibration Procedure(s) FF-Z11-003-01 Calibration Procedures for dipole validation kits</p> <p>Calibration date: March 31, 2022</p> <p>This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility: environment temperature (22±1)°C and humidity<70%.</p> <p>Calibration equipment used (M&TE critical for calibration)</p> <table border="1"> <tr> <td>Primary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Power Meter NRP2</td> <td>105277</td> <td>24-Sep-21 (CTTL No.J21X05326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRP83</td> <td>104291</td> <td>24-Sep-21 (CTTL No.J21X05326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV2</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No. EX3-7307, May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1595</td> <td>12-Jan-22 (CTTL-SPEAG No.Z22-60007)</td> <td>Jan-23</td> </tr> <tr> <td>Secondary Standards</td> <td>ID #</td> <td>Cal Date (Calibrated by, Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Signal Generator E4348C</td> <td>MY46017430</td> <td>13-Jan-22 (CTTL No.J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY4610673</td> <td>14-Jan-22 (CTTL No.J22X00406)</td> <td>Jan-23</td> </tr> </table> <p>Calibrated by: Zhao Jing SAR Test Engineer Reviewed by: Lin Hao SAR Test Engineer Approved by: Qi Dianyuan SAR Project Leader</p> <p>Issued: April 6, 2022</p> <p>Certificate No: Z22-60108 Page 1 of 6</p>	Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Power Meter NRP2	105277	24-Sep-21 (CTTL No.J21X05326)	Sep-22	Power sensor NRP83	104291	24-Sep-21 (CTTL No.J21X05326)	Sep-22	Reference Probe EX3DV2	SN 7307	26-May-21 (SPEAG No. EX3-7307, May21)	May-22	DAE4	SN 1595	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration	Signal Generator E4348C	MY46017430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyzer E5071C	MY4610673	14-Jan-22 (CTTL No.J22X00406)	Jan-23	  <p>in Collaboration with TTL Speag CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304083-2512 Fax: +86-10-62304083-2504 E-mail: cn@caict.com</p> <p>Glossary: TSL tissue simulating liquid ConvF sensitivity in TSL / NORMx,y,z N/A not applicable or not measured</p> <p>Calibration is Performed According to the Following Standards: IEC/EN62209-1522:2019 "Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1522: Human Models, Instrumentation and Procedures (Frequency range 4 MHz to 10 GHz)", October 2020 b) K05 86596 "SAR Measurement Requirements for 100 MHz to 6 GHz"</p> <p>Additional Documentation: c) DASY4/5 System Handbook</p> <p>Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with a spacer to position its feed measurement at the same center marking of the fat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measured at the feed point to the feed-point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.</p> <p>The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.</p> <p>Certificate No: Z22-60108 Page 2 of 6</p>																		
Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																
Power Meter NRP2	105277	24-Sep-21 (CTTL No.J21X05326)	Sep-22																																																
Power sensor NRP83	104291	24-Sep-21 (CTTL No.J21X05326)	Sep-22																																																
Reference Probe EX3DV2	SN 7307	26-May-21 (SPEAG No. EX3-7307, May21)	May-22																																																
DAE4	SN 1595	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23																																																
Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration																																																
Signal Generator E4348C	MY46017430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																																																
Network Analyzer E5071C	MY4610673	14-Jan-22 (CTTL No.J22X00406)	Jan-23																																																
  <p>in Collaboration with TTL Speag CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62304083-2512 Fax: +86-10-62304083-2504 E-mail: cn@caict.com</p> <p>Measurement Conditions DASY system configuration, as far as given on page 1.</p> <table border="1"> <tr> <td>DASY Version</td> <td>DASY52</td> <td>52.10.4</td> </tr> <tr> <td>Extrapolation</td> <td>Advanced Extrapolation</td> <td></td> </tr> <tr> <td>Phantom</td> <td>Triple Flat Phantom 5.1C</td> <td></td> </tr> <tr> <td>Distance Dipole Center - TSL</td> <td>10 mm</td> <td>with Spacer</td> </tr> <tr> <td>Zoom Scan Resolution</td> <td>dx, dy, dz < 5 mm</td> <td></td> </tr> <tr> <td>Frequency</td> <td>2800 MHz ± 1 MHz</td> <td></td> </tr> </table> <p>Head TSL parameters The following parameters and calculations were applied.</p> <table border="1"> <tr> <td>Temperature</td> <td>Permittivity</td> <td>Conductivity</td> </tr> <tr> <td>Nominal Head TSL parameters</td> <td>22.0 °C</td> <td>39.0 1.96 mho/m</td> </tr> <tr> <td>Measured Head TSL parameters</td> <td>22.0 ± 0.2 °C</td> <td>38.7 ± 6 % 1.96 mho/m ± 6 %</td> </tr> <tr> <td>Head TSL temperature change during test</td> <td><1.0 °C</td> <td>—</td> </tr> </table> <p>SAR result with Head TSL</p> <table border="1"> <tr> <td>SAR averaged over 1 cm³ (1g) of Head TSL</td> <td>Condition</td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power 13.7 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W 54.8 W/kg ± 18.8 % (k=2)</td> </tr> <tr> <td>SAR averaged over 10 cm³ (10g) of Head TSL</td> <td>Condition</td> </tr> <tr> <td>SAR measured</td> <td>250 mW input power 6.12 W/kg</td> </tr> <tr> <td>SAR for nominal Head TSL parameters</td> <td>normalized to 1W 24.5 W/kg ± 18.7 % (k=2)</td> </tr> </table> <p>Certificate No: Z22-60108 Page 3 of 6</p>	DASY Version	DASY52	52.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Flat Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	dx, dy, dz < 5 mm		Frequency	2800 MHz ± 1 MHz		Temperature	Permittivity	Conductivity	Nominal Head TSL parameters	22.0 °C	39.0 1.96 mho/m	Measured Head TSL parameters	22.0 ± 0.2 °C	38.7 ± 6 % 1.96 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	SAR averaged over 1 cm ³ (1g) of Head TSL	Condition	SAR measured	250 mW input power 13.7 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 54.8 W/kg ± 18.8 % (k=2)	SAR averaged over 10 cm ³ (10g) of Head TSL	Condition	SAR measured	250 mW input power 6.12 W/kg	SAR for nominal Head TSL parameters	normalized to 1W 24.5 W/kg ± 18.7 % (k=2)	<p>Appendix (Additional assessments outside the scope of CNAS L0570)</p> <p>Antenna Parameters with Head TSL</p> <table border="1"> <tr> <td>Impedance, transformed to feed point</td> <td>49.9Ω 6.4ΩΩ</td> </tr> <tr> <td>Return Loss</td> <td>-23.9dB</td> </tr> </table> <p>General Antenna Parameters and Design</p> <table border="1"> <tr> <td>Electrical Delay (one direction)</td> <td>1.053 ns</td> </tr> </table> <p>After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.</p> <p>The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded with a phantom. This is mentioned in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is as stated in the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.</p> <p>Additional EUT Data</p> <table border="1"> <tr> <td>Manufactured by</td> <td>SPEAG</td> </tr> </table> <p>Certificate No: Z22-60108 Page 4 of 6</p>	Impedance, transformed to feed point	49.9Ω 6.4ΩΩ	Return Loss	-23.9dB	Electrical Delay (one direction)	1.053 ns	Manufactured by	SPEAG
DASY Version	DASY52	52.10.4																																																	
Extrapolation	Advanced Extrapolation																																																		
Phantom	Triple Flat Phantom 5.1C																																																		
Distance Dipole Center - TSL	10 mm	with Spacer																																																	
Zoom Scan Resolution	dx, dy, dz < 5 mm																																																		
Frequency	2800 MHz ± 1 MHz																																																		
Temperature	Permittivity	Conductivity																																																	
Nominal Head TSL parameters	22.0 °C	39.0 1.96 mho/m																																																	
Measured Head TSL parameters	22.0 ± 0.2 °C	38.7 ± 6 % 1.96 mho/m ± 6 %																																																	
Head TSL temperature change during test	<1.0 °C	—																																																	
SAR averaged over 1 cm ³ (1g) of Head TSL	Condition																																																		
SAR measured	250 mW input power 13.7 W/kg																																																		
SAR for nominal Head TSL parameters	normalized to 1W 54.8 W/kg ± 18.8 % (k=2)																																																		
SAR averaged over 10 cm ³ (10g) of Head TSL	Condition																																																		
SAR measured	250 mW input power 6.12 W/kg																																																		
SAR for nominal Head TSL parameters	normalized to 1W 24.5 W/kg ± 18.7 % (k=2)																																																		
Impedance, transformed to feed point	49.9Ω 6.4ΩΩ																																																		
Return Loss	-23.9dB																																																		
Electrical Delay (one direction)	1.053 ns																																																		
Manufactured by	SPEAG																																																		


Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com


No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



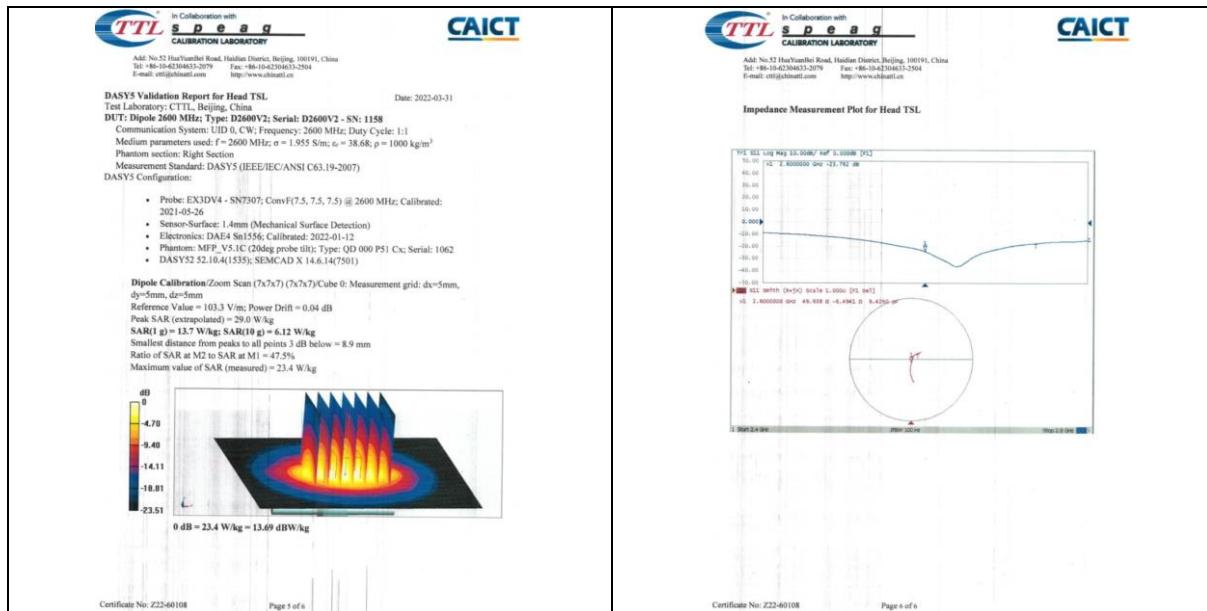

1.12 D5GHzV2 - SN 1095

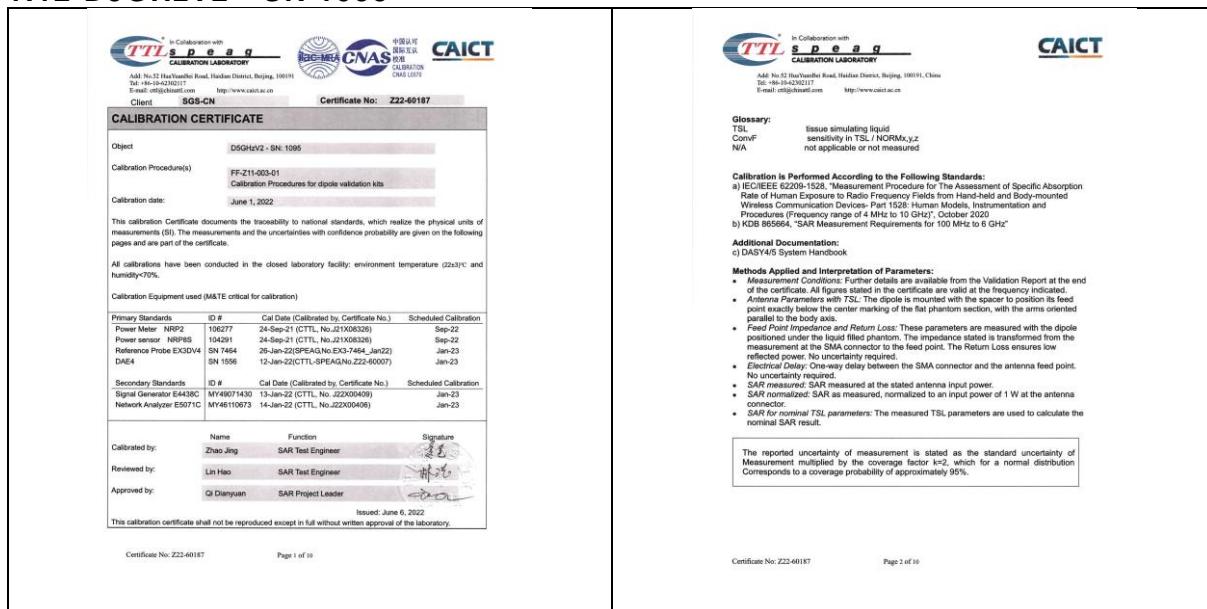

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com



<div style="text-align: center;">  <p>In Collaboration with CAICT</p> <p>Add: No.52 HuYanBei Road, Haidian District, Beijing, 100081, China Tel: +86-10-62302117 E-mail: cttj@caict.ac.cn http://www.caict.ac.cn</p> <p>Measurement Conditions CNAS test configuration, as far as not given on page 1.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>DASY Version</td><td>DASY2</td><td>S2.10.4</td></tr> <tr><td>Extrapolation</td><td>Advanced Extrapolation</td><td></td></tr> <tr><td>Phantom</td><td>Triple Pad Phantom 5.1C</td><td></td></tr> <tr><td>Distance Dipole Center - TSL</td><td>10 mm</td><td>with Spacer</td></tr> <tr><td>Zoom Scan Resolution</td><td>$dx = 4 \text{ mm}$, $dz = 1.4 \text{ mm}$</td><td>Graded Ratio = 1.4 (Z direction)</td></tr> <tr><td>Frequency</td><td>5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz</td><td></td></tr> </table> <p>Head TSL parameters at 5200MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>SAR result with Head TSL at 5200MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>Head TSL parameters at 5200MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.5</td><td>0.07 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>35.4 ± 6 %</td><td>0.06 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL at 5200MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>250 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>Head TSL parameters at 5300MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.9</td><td>4.76 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>35.2 ± 6 %</td><td>4.73 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL at 5300MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>Head TSL parameters at 5500MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.6</td><td>4.96 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>34.8 ± 6 %</td><td>4.94 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL at 5500MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>Head TSL parameters at 5800MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.3</td><td>5.27 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>34.7 ± 6 %</td><td>5.20 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL at 5800MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>Head TSL parameters at 5800MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.5</td><td>5.27 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>34.4 ± 6 %</td><td>5.20 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL at 5800MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> </div>	DASY Version	DASY2	S2.10.4	Extrapolation	Advanced Extrapolation		Phantom	Triple Pad Phantom 5.1C		Distance Dipole Center - TSL	10 mm	with Spacer	Zoom Scan Resolution	$dx = 4 \text{ mm}$, $dz = 1.4 \text{ mm}$	Graded Ratio = 1.4 (Z direction)	Frequency	5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz		SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	250 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	250 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	250 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	250 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	Nominal Head TSL parameters	22.0 °C	35.5	0.07 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	0.06 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	250 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	250 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.20 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	Nominal Head TSL parameters	22.0 °C	35.5	5.27 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.20 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	<div style="text-align: center;">  <p>In Collaboration with CAICT</p> <p>Add: No.52 HuYanBei Road, Haidian District, Beijing, 100081, China Tel: +86-10-62302117 E-mail: cttj@caict.ac.cn http://www.caict.ac.cn</p> <p>Head TSL parameters at 5300MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.9</td><td>4.76 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>35.2 ± 6 %</td><td>4.73 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL at 5300MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>Head TSL parameters at 5500MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.6</td><td>4.96 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>34.8 ± 6 %</td><td>4.94 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL at 5500MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>Head TSL parameters at 5800MHz The following parameters and calculations were applied.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Nominal Head TSL parameters</td><td>22.0 °C</td><td>35.3</td><td>5.27 mho/m</td></tr> <tr><td>Measured Head TSL parameters</td><td>(22.0 ± 0.2) °C</td><td>34.7 ± 6 %</td><td>5.20 mho/m ± 6 %</td></tr> <tr><td>Head TSL temperature change during test</td><td><1.0 °C</td><td>—</td><td>—</td></tr> </table> <p>SAR result with Head TSL at 5800MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>SAR averaged over 1 cm^3 (1 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> <tr><td>SAR averaged over 10 cm^3 (10 g) of Head TSL</td><td>Condition</td></tr> <tr><td>SAR measured</td><td>100 mW input power</td></tr> <tr><td>SAR for nominal Head TSL parameters</td><td>normalized to 1W</td></tr> </table> <p>Antenna Parameters with Head TSL at 5200MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>48.10-6.03jΩ</td></tr> <tr><td>Return Loss</td><td>-23.6dB</td></tr> </table> <p>Antenna Parameters with Head TSL at 5300MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>47.80-2.43jΩ</td></tr> <tr><td>Return Loss</td><td>-29.5dB</td></tr> </table> <p>Antenna Parameters with Head TSL at 5500MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>50.30-4.26jΩ</td></tr> <tr><td>Return Loss</td><td>-27.4dB</td></tr> </table> <p>Antenna Parameters with Head TSL at 5600MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>54.50-4.85jΩ</td></tr> <tr><td>Return Loss</td><td>-24.0dB</td></tr> </table> <p>Antenna Parameters with Head TSL at 5800MHz</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr><td>Impedance, transformed to feed point</td><td>51.50-5.81jΩ</td></tr> <tr><td>Return Loss</td><td>-24.9dB</td></tr> </table> </div>	Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m	Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.20 mho/m ± 6 %	Head TSL temperature change during test	<1.0 °C	—	—	SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition	SAR measured	100 mW input power	SAR for nominal Head TSL parameters	normalized to 1W	Impedance, transformed to feed point	48.10-6.03jΩ	Return Loss	-23.6dB	Impedance, transformed to feed point	47.80-2.43jΩ	Return Loss	-29.5dB	Impedance, transformed to feed point	50.30-4.26jΩ	Return Loss	-27.4dB	Impedance, transformed to feed point	54.50-4.85jΩ	Return Loss	-24.0dB	Impedance, transformed to feed point	51.50-5.81jΩ	Return Loss	-24.9dB
DASY Version	DASY2	S2.10.4																																																																																																																																																																																																																																																													
Extrapolation	Advanced Extrapolation																																																																																																																																																																																																																																																														
Phantom	Triple Pad Phantom 5.1C																																																																																																																																																																																																																																																														
Distance Dipole Center - TSL	10 mm	with Spacer																																																																																																																																																																																																																																																													
Zoom Scan Resolution	$dx = 4 \text{ mm}$, $dz = 1.4 \text{ mm}$	Graded Ratio = 1.4 (Z direction)																																																																																																																																																																																																																																																													
Frequency	5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz																																																																																																																																																																																																																																																														
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	250 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	250 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	250 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	250 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Nominal Head TSL parameters	22.0 °C	35.5	0.07 mho/m																																																																																																																																																																																																																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	0.06 mho/m ± 6 %																																																																																																																																																																																																																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																																																																																																																																																												
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	250 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	250 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m																																																																																																																																																																																																																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %																																																																																																																																																																																																																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																																																																																																																																																												
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m																																																																																																																																																																																																																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %																																																																																																																																																																																																																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																																																																																																																																																												
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m																																																																																																																																																																																																																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.20 mho/m ± 6 %																																																																																																																																																																																																																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																																																																																																																																																												
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Nominal Head TSL parameters	22.0 °C	35.5	5.27 mho/m																																																																																																																																																																																																																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.20 mho/m ± 6 %																																																																																																																																																																																																																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																																																																																																																																																												
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m																																																																																																																																																																																																																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %																																																																																																																																																																																																																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																																																																																																																																																												
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m																																																																																																																																																																																																																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %																																																																																																																																																																																																																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																																																																																																																																																												
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m																																																																																																																																																																																																																																																												
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.20 mho/m ± 6 %																																																																																																																																																																																																																																																												
Head TSL temperature change during test	<1.0 °C	—	—																																																																																																																																																																																																																																																												
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
SAR averaged over 10 cm^3 (10 g) of Head TSL	Condition																																																																																																																																																																																																																																																														
SAR measured	100 mW input power																																																																																																																																																																																																																																																														
SAR for nominal Head TSL parameters	normalized to 1W																																																																																																																																																																																																																																																														
Impedance, transformed to feed point	48.10-6.03jΩ																																																																																																																																																																																																																																																														
Return Loss	-23.6dB																																																																																																																																																																																																																																																														
Impedance, transformed to feed point	47.80-2.43jΩ																																																																																																																																																																																																																																																														
Return Loss	-29.5dB																																																																																																																																																																																																																																																														
Impedance, transformed to feed point	50.30-4.26jΩ																																																																																																																																																																																																																																																														
Return Loss	-27.4dB																																																																																																																																																																																																																																																														
Impedance, transformed to feed point	54.50-4.85jΩ																																																																																																																																																																																																																																																														
Return Loss	-24.0dB																																																																																																																																																																																																																																																														
Impedance, transformed to feed point	51.50-5.81jΩ																																																																																																																																																																																																																																																														
Return Loss	-24.9dB																																																																																																																																																																																																																																																														

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention is drawn to the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

Compliance Certification Services (Kunshan) Inc.
EMC Laboratory
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300



<p>TTL s p e a g CALIBRATION LABORATORY In Collaboration with Add No. 15-21 Huayuanbeilu Road, Haidian District, Beijing, 100091, China Tel: +86-10-84230217 E-mail: ctt@cttcal.com http://www.cttcal.com</p> <p>CAICT</p> <p>Dipole Calibration (Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 29.8 W/kg; SAR(1 g) = 2.22 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 18.3 W/kg</p> <p>Dipole Calibration (Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.8 W/kg; SAR(1 g) = 2.34 W/kg SAR(1 g) = 8.28 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg</p> <p>Dipole Calibration (Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.0 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.3 W/kg; SAR(1 g) = 2.35 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.35 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg</p> <p>Dipole Calibration (Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.0 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 34.8 W/kg; SAR(1 g) = 2.16 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg</p> <p></p> <p>Certificate No: Z22-60187 Page 9 of 10</p>
--

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overhead, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>, and for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced in full or without prior written permission of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the full extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.DocCheck@sgs.com

中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

2 DAE4 - SN 1245

<div style="border: 1px solid black; padding: 10px;"> <p>s p e a g</p> <p>IMPORTANT NOTICE</p> <p>USAGE OF THE DAE4</p> <p>The DAE4 unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points:</p> <p>Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw. Over tightening the screw may cause the threads inside the DAE to wear.</p> <p>Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the battery and pack the DAE in a sturdy shipping box. It is recommended to use a padded box or a larger box in a container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside.</p> <p>E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may damage any of these magnets. Touch and collision errors are often caused by dust and dirt accumulation on the E-stop. To prevent damage, always handle the DAE4 unit with care and store it in a non-dusty environment if not used for measurements.</p> <p>Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair necessary if rough unprofessional handling caused the defect.</p> <p>DAE Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MΩ is given in the corresponding configuration file.</p> <p>Important Note: Warning and calibration is void if the DAE unit is disassembled partly or fully by the Customer.</p> <p>Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop must be performed by certified SPEAG personnel only and is part of the annual calibration procedure.</p> <p>Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disassembling the probe from the DAE.</p> <p>TN_IH190306AE DAE4.docx 07.03.2019</p> </div>	<div style="border: 1px solid black; padding: 10px;"> <p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 0750, Fax +41 44 245 9779 e-mail: Schmid@sp-eag.com</p> <p>Accreditation No.: SCS 0108</p> <p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: SGS-CN (Auden) Certificate No.: DAE4-1245_May22</p> <p>CALIBRATION CERTIFICATE</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Object:</td> <td>DAE4 - SD 000 D04 BM - SN: 1245</td> </tr> <tr> <td>Calibration procedure(s):</td> <td>QA CAL-06 v30 Calibration procedure for the data acquisition electronics (DAE).</td> </tr> <tr> <td>Calibration date:</td> <td>May 30, 2022</td> </tr> </table> <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 3)°C and humidity < 70%.</p> <p>Calibration Equipment used (MATE: critical for calibration)</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Primary Standards</td> <td>ID #</td> <td>Cal Date (Certificate No.)</td> <td>Scheduled Calibration</td> </tr> <tr> <td>Kathrein Multimeter Type 2001</td> <td>SN: 0810078</td> <td>31-Aug-21 (No. 2168)</td> <td>Aug-22</td> </tr> <tr> <td style="width: 10%;">Secondary Standards</td> <td>ID #</td> <td>Check Date (in house)</td> <td>Scheduled Check</td> </tr> <tr> <td>Auto DAE Calibration Unit</td> <td>BE UMS 003 AA 1001</td> <td>24-Jan-22 (in house check)</td> <td>In house check: Jan-23</td> </tr> <tr> <td></td> <td>BE UMS 006 AA 1002</td> <td>24-Jan-22 (in house check)</td> <td>In house check: Jan-23</td> </tr> </table> <p>Calibrated by: Name: Dominique Steffen Function: Laboratory Technician Signature: </p> <p>Approved by: Name: Sven Kühn Function: Technical Manager Signature: </p> <p>This calibration certificate shall not be reproduced except in full without written approval of the laboratory.</p> <p>Issued: May 30, 2022</p> <p>Certificate No: DAE4-1245_May22 Page 1 of 5</p> </div>	Object:	DAE4 - SD 000 D04 BM - SN: 1245	Calibration procedure(s):	QA CAL-06 v30 Calibration procedure for the data acquisition electronics (DAE).	Calibration date:	May 30, 2022	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Kathrein Multimeter Type 2001	SN: 0810078	31-Aug-21 (No. 2168)	Aug-22	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Auto DAE Calibration Unit	BE UMS 003 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23		BE UMS 006 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23
Object:	DAE4 - SD 000 D04 BM - SN: 1245																										
Calibration procedure(s):	QA CAL-06 v30 Calibration procedure for the data acquisition electronics (DAE).																										
Calibration date:	May 30, 2022																										
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																								
Kathrein Multimeter Type 2001	SN: 0810078	31-Aug-21 (No. 2168)	Aug-22																								
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																								
Auto DAE Calibration Unit	BE UMS 003 AA 1001	24-Jan-22 (in house check)	In house check: Jan-23																								
	BE UMS 006 AA 1002	24-Jan-22 (in house check)	In house check: Jan-23																								
<div style="border: 1px solid black; padding: 10px;"> <p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland</p> <p>Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Glossary DAE data acquisition electronics Connector angle information used in DASY system to align probe sensor X to the robot coordinate system</p> <p>Method Applied for the Determination of Parameters</p> <ul style="list-style-type: none"> • DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. • Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. • The following parameters as documented in the Appendix contain technical information as a reference for the performance test and require no uncertainty: <ul style="list-style-type: none"> • DC Voltage Measurement Linearity: Verification of the Linearity at -10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. • Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. • Channel separation: Influence of a voltage on the neighbor channels not subject to an AD converter. • AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage • Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. • Input Offset Current: Typical value for information: Maximum channel input offset current not considering the input resistance. • Input resistance: Typical value for information: DAE input resistance at the connector, measured with the probe connected and during measurement. • Low Voltage Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. • Power consumption: Typical value for information. Supply currents in various operating modes. <p>Certificate No: DAE4-1245_May22 Page 2 of 5</p> </div>	<div style="border: 1px solid black; padding: 10px;"> <p>DC Voltage Measurement</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">AD - Converter nominal</td> <td>5 mV</td> <td>full range = -10...+100 mV</td> </tr> <tr> <td>High Range:</td> <td>1.538 =</td> <td>5 mV</td> </tr> <tr> <td>Low Range:</td> <td>1.538 =</td> <td>5 mV</td> </tr> <tr> <td colspan="3">DASY measurement parameters: Auto Zero, Time: 3 sec, Measuring time: 3 sec</td> </tr> </table> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Calibration Factors</td> <td>X</td> <td>Y</td> <td>Z</td> </tr> <tr> <td>High Range:</td> <td>405.395 ± 0.02% (n=2)</td> <td>405.974 ± 0.02% (n=2)</td> <td>405.092 ± 0.02% (n=2)</td> </tr> <tr> <td>Low Range:</td> <td>3.99534 ± 1.50% (n=2)</td> <td>3.89908 ± 1.50% (n=2)</td> <td>4.01015 ± 1.50% (n=2)</td> </tr> </table> <p>Connector Angle</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 10%;">Connector Angle to be used in DASY system</td> <td>90.0 ± 1°</td> </tr> </table> <p>Certificate No: DAE4-1245_May22 Page 3 of 5</p> </div>	AD - Converter nominal	5 mV	full range = -10...+100 mV	High Range:	1.538 =	5 mV	Low Range:	1.538 =	5 mV	DASY measurement parameters: Auto Zero, Time: 3 sec, Measuring time: 3 sec			Calibration Factors	X	Y	Z	High Range:	405.395 ± 0.02% (n=2)	405.974 ± 0.02% (n=2)	405.092 ± 0.02% (n=2)	Low Range:	3.99534 ± 1.50% (n=2)	3.89908 ± 1.50% (n=2)	4.01015 ± 1.50% (n=2)	Connector Angle to be used in DASY system	90.0 ± 1°
AD - Converter nominal	5 mV	full range = -10...+100 mV																									
High Range:	1.538 =	5 mV																									
Low Range:	1.538 =	5 mV																									
DASY measurement parameters: Auto Zero, Time: 3 sec, Measuring time: 3 sec																											
Calibration Factors	X	Y	Z																								
High Range:	405.395 ± 0.02% (n=2)	405.974 ± 0.02% (n=2)	405.092 ± 0.02% (n=2)																								
Low Range:	3.99534 ± 1.50% (n=2)	3.89908 ± 1.50% (n=2)	4.01015 ± 1.50% (n=2)																								
Connector Angle to be used in DASY system	90.0 ± 1°																										

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.DocCheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



Appendix (Additional assessments outside the scope of SCS0108)																																																																																	
1. DC Voltage Linearity <small>DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec</small> <table border="1"> <thead> <tr> <th>High Range</th> <th>Reading (mV)</th> <th>Difference (mV)</th> <th>Error (%)</th> </tr> </thead> <tbody> <tr><td>Channel X + Input</td><td>199994.45</td><td>1.83</td><td>0.06</td></tr> <tr><td>Channel X - Input</td><td>200004.58</td><td>2.22</td><td>0.01</td></tr> <tr><td>Channel X + Input</td><td>-20000.14</td><td>1.12</td><td>-0.01</td></tr> <tr><td>Channel Y + Input</td><td>199994.72</td><td>1.98</td><td>0.00</td></tr> <tr><td>Channel Y - Input</td><td>200012.22</td><td>-1.00</td><td>-0.00</td></tr> <tr><td>Channel Z + Input</td><td>-20005.05</td><td>-1.57</td><td>0.01</td></tr> <tr><td>Channel Z + Input</td><td>199992.64</td><td>0.19</td><td>0.00</td></tr> <tr><td>Channel Z + Input</td><td>20003.58</td><td>0.98</td><td>0.00</td></tr> <tr><td>Channel Z - Input</td><td>-20001.73</td><td>-0.27</td><td>0.00</td></tr> </tbody> </table> <table border="1"> <thead> <tr> <th>Low Range</th> <th>Reading (mV)</th> <th>Difference (mV)</th> <th>Error (%)</th> </tr> </thead> <tbody> <tr><td>Channel X + Input</td><td>2001.91</td><td>0.41</td><td>0.07</td></tr> <tr><td>Channel X - Input</td><td>2001.53</td><td>0.55</td><td>0.30</td></tr> <tr><td>Channel X - Input</td><td>-197.86</td><td>0.07</td><td>-0.04</td></tr> <tr><td>Channel Y + Input</td><td>2022.05</td><td>0.59</td><td>0.03</td></tr> <tr><td>Channel Y + Input</td><td>201.27</td><td>-0.57</td><td>-0.28</td></tr> <tr><td>Channel Y - Input</td><td>-198.23</td><td>-0.06</td><td>0.03</td></tr> <tr><td>Channel Z + Input</td><td>2001.36</td><td>0.08</td><td>0.00</td></tr> <tr><td>Channel Z + Input</td><td>200.59</td><td>-1.53</td><td>-0.76</td></tr> <tr><td>Channel Z - Input</td><td>-199.85</td><td>-1.57</td><td>0.79</td></tr> </tbody> </table>		High Range	Reading (mV)	Difference (mV)	Error (%)	Channel X + Input	199994.45	1.83	0.06	Channel X - Input	200004.58	2.22	0.01	Channel X + Input	-20000.14	1.12	-0.01	Channel Y + Input	199994.72	1.98	0.00	Channel Y - Input	200012.22	-1.00	-0.00	Channel Z + Input	-20005.05	-1.57	0.01	Channel Z + Input	199992.64	0.19	0.00	Channel Z + Input	20003.58	0.98	0.00	Channel Z - Input	-20001.73	-0.27	0.00	Low Range	Reading (mV)	Difference (mV)	Error (%)	Channel X + Input	2001.91	0.41	0.07	Channel X - Input	2001.53	0.55	0.30	Channel X - Input	-197.86	0.07	-0.04	Channel Y + Input	2022.05	0.59	0.03	Channel Y + Input	201.27	-0.57	-0.28	Channel Y - Input	-198.23	-0.06	0.03	Channel Z + Input	2001.36	0.08	0.00	Channel Z + Input	200.59	-1.53	-0.76	Channel Z - Input	-199.85	-1.57	0.79
High Range	Reading (mV)	Difference (mV)	Error (%)																																																																														
Channel X + Input	199994.45	1.83	0.06																																																																														
Channel X - Input	200004.58	2.22	0.01																																																																														
Channel X + Input	-20000.14	1.12	-0.01																																																																														
Channel Y + Input	199994.72	1.98	0.00																																																																														
Channel Y - Input	200012.22	-1.00	-0.00																																																																														
Channel Z + Input	-20005.05	-1.57	0.01																																																																														
Channel Z + Input	199992.64	0.19	0.00																																																																														
Channel Z + Input	20003.58	0.98	0.00																																																																														
Channel Z - Input	-20001.73	-0.27	0.00																																																																														
Low Range	Reading (mV)	Difference (mV)	Error (%)																																																																														
Channel X + Input	2001.91	0.41	0.07																																																																														
Channel X - Input	2001.53	0.55	0.30																																																																														
Channel X - Input	-197.86	0.07	-0.04																																																																														
Channel Y + Input	2022.05	0.59	0.03																																																																														
Channel Y + Input	201.27	-0.57	-0.28																																																																														
Channel Y - Input	-198.23	-0.06	0.03																																																																														
Channel Z + Input	2001.36	0.08	0.00																																																																														
Channel Z + Input	200.59	-1.53	-0.76																																																																														
Channel Z - Input	-199.85	-1.57	0.79																																																																														
2. Common mode sensitivity <small>DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec</small> <table border="1"> <thead> <tr> <th>Common mode Input Voltage (mV)</th> <th>High Range Average Reading (μV)</th> <th>Low Range Average Reading (μV)</th> </tr> </thead> <tbody> <tr><td>200</td><td>-5.97</td><td>-7.69</td></tr> <tr><td>-200</td><td>5.12</td><td>7.79</td></tr> <tr><td>200</td><td>-6.68</td><td>-9.28</td></tr> <tr><td>-200</td><td>6.82</td><td>8.58</td></tr> <tr><td>200</td><td>-5.25</td><td>-5.60</td></tr> <tr><td>-200</td><td>5.68</td><td>8.06</td></tr> </tbody> </table>		Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)	200	-5.97	-7.69	-200	5.12	7.79	200	-6.68	-9.28	-200	6.82	8.58	200	-5.25	-5.60	-200	5.68	8.06																																																											
Common mode Input Voltage (mV)	High Range Average Reading (μV)	Low Range Average Reading (μV)																																																																															
200	-5.97	-7.69																																																																															
-200	5.12	7.79																																																																															
200	-6.68	-9.28																																																																															
-200	6.82	8.58																																																																															
200	-5.25	-5.60																																																																															
-200	5.68	8.06																																																																															
3. Channel separation <small>DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec</small> <table border="1"> <thead> <tr> <th>Input Voltage (mV)</th> <th>Channel X (μV)</th> <th>Channel Y (μV)</th> <th>Channel Z (μV)</th> </tr> </thead> <tbody> <tr><td>200</td><td>-</td><td>4.07</td><td>-5.14</td></tr> <tr><td>200</td><td>9.95</td><td>-</td><td>4.27</td></tr> <tr><td>200</td><td>10.11</td><td>7.14</td><td>-</td></tr> </tbody> </table>		Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)	200	-	4.07	-5.14	200	9.95	-	4.27	200	10.11	7.14	-																																																																
Input Voltage (mV)	Channel X (μV)	Channel Y (μV)	Channel Z (μV)																																																																														
200	-	4.07	-5.14																																																																														
200	9.95	-	4.27																																																																														
200	10.11	7.14	-																																																																														
<small>Certificate No: DAIE-1246, May22</small>																																																																																	
<small>Page 4 of 5</small>																																																																																	
<small>Certificate No: DAIE-1246, May22</small>																																																																																	
<small>Page 5 of 5</small>																																																																																	

3 EX3DV4 - SN 3801

<p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8043 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Client: Auden Certificate No: EX-3801_Jul22</p> <p>CALIBRATION CERTIFICATE</p> <p>Object: EX3DV4 - SN-3801</p> <p>Calibration procedure(s): QA CAL_01.v9, QA CAL_12.v9, QA CAL_14.v6, QA CAL_23.v5, QA CAL_25.v7</p> <p>Calibration procedure for dielectric E-field probes</p> <p>Calibration date: July 21, 2022</p> <p>This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.</p> <p>All calibrations have been conducted in the closest laboratory facility, environment temperature (22 ± 5)°C and humidity < 70%.</p> <p>Calibration equipment used (WATT offset for calibration):</p> <table border="1"> <tr> <td>Power Source: NIPW</td> <td>SN: 704079</td> <td>Cal Date: Certificate No:</td> <td>Calibrated On:</td> </tr> <tr> <td>Power Source: NIPW-251</td> <td>SN: 1020844</td> <td>05-Apr-22 (No. 217-00384)</td> <td>05-Apr-22</td> </tr> <tr> <td>Power Source: E412A</td> <td>SN: 1020845</td> <td>05-Apr-22 (No. 217-00385)</td> <td>05-Apr-22</td> </tr> <tr> <td>DCP DAS (20 dB Attenuator)</td> <td>SN: 1016</td> <td>20-Dec-21 (CPD-DAS-20-1016-Dest1)</td> <td>05-Apr-22</td> </tr> <tr> <td>DCP DAS (20 dB Attenuator)</td> <td>SN: 669</td> <td>13-Dec-21 (No. 5414-466-Dest1)</td> <td>05-Apr-22</td> </tr> <tr> <td>Reference Probe E3002</td> <td>SN: 3010</td> <td>27-Dec-21 (No. E3-3013-Dest1)</td> <td>05-Apr-22</td> </tr> </table> <p>Calibrated by: Last Name: Function: Signature: Issued: July 21, 2022</p> <p>Approved by: Sven Kühn: Technical Manager: Signature: Issued: July 21, 2022</p> <p>Certified No: EX-3801_Jul22</p> <p>Page 1 of 22</p>	Power Source: NIPW	SN: 704079	Cal Date: Certificate No:	Calibrated On:	Power Source: NIPW-251	SN: 1020844	05-Apr-22 (No. 217-00384)	05-Apr-22	Power Source: E412A	SN: 1020845	05-Apr-22 (No. 217-00385)	05-Apr-22	DCP DAS (20 dB Attenuator)	SN: 1016	20-Dec-21 (CPD-DAS-20-1016-Dest1)	05-Apr-22	DCP DAS (20 dB Attenuator)	SN: 669	13-Dec-21 (No. 5414-466-Dest1)	05-Apr-22	Reference Probe E3002	SN: 3010	27-Dec-21 (No. E3-3013-Dest1)	05-Apr-22	<p>Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8043 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates</p> <p>Glossary</p> <p>TSL: Issue simulating liquid NORMA,y,z: Uncertainty in the slope Conv: Convolution of two signals DCP: DC offset compensation point CP: Convolution of two signals Polarization v: Polarization vector Polarization a: Polarization angle Corrector Angle: Information used in DASY system to align probe sensor X to the probe coordinate system</p> <p>Calibration is Performed According to the Following Standards:</p> <p>a) IEC/IEEE 62209-1526: "Measurement Procedure For The Assessment Of Specific Absorption Rate CI Human Exposure To Radio Frequency Fields From Handheld and Body-worn Wireless Communication Devices - Part 1526: Human Models, Instrumentation and Procedures (Frequency Range of 100 MHz to 10 GHz)", October 2008. b) KDB 86564: "SAR Measurement Requirements for 100MHz to 1GHz"</p> <p>Methods Applied and Interpretation of Parameters:</p> <p>- NORMA,y,z: Assessed for E-field polarization if $\theta \neq 0$ ± 90° in TEM-cell, $f > 10000\text{MHz}$: R22 uncertainty. NORMA,y,z are only intermediate values, i.e., the uncertainties of NORMA,y,z does not affect the E-field uncertainty made TSL (see below). The uncertainty of the polarization angle is not taken into account. - NORMA,y,z, x, y, z: Frequency response (see Frequency Response Chart). This linearization is implemented in DASY software. The uncertainty of the frequency response is related to the stated uncertainty of Conv. - DCP: DC offset compensation parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency or media. - PWR: PWR is the Power-to-Average Ratio that is not calibrated but determined based on the signal characteristics (e.g. noise level, signal-to-noise ratio, etc.). PWR is used to convert the measured power to the maximum data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum voltage of the power sweep. - Conv and Boundary Effect Parameters: Assessed in flat phantom using E-field or Temperature Transfer Standard for boundary effect calibration using antipodal field distributions based on power measurements for $f > 8000\text{MHz}$. The same values are used for all frequencies. The uncertainty of the boundary effect parameters is the same as the overall uncertainty value. These parameters are used in DASY software to improve probe accuracy close to the boundary. The uncertainty of the boundary effect parameters is not taken into account. - ConvF: Frequency dependent Conv is used in DASY version 4.4 and higher which allows extending the validity from 100MHz to 10GHz. - Several isotropy (3D deviation from isotropy): In a field of low gradients realized using a flat phantom exposed by a patch antenna. - Sensor Offset: The sensor offset corresponds to the offset of visual measurement center from the probe tip (on probe axis). No tolerance required. - Corrector Angle: The angle is assessed using the information gained by determining the NORMA (no uncertainty required).</p> <p>Certified No: EX-3801_Jul22</p> <p>Page 2 of 22</p>
Power Source: NIPW	SN: 704079	Cal Date: Certificate No:	Calibrated On:																						
Power Source: NIPW-251	SN: 1020844	05-Apr-22 (No. 217-00384)	05-Apr-22																						
Power Source: E412A	SN: 1020845	05-Apr-22 (No. 217-00385)	05-Apr-22																						
DCP DAS (20 dB Attenuator)	SN: 1016	20-Dec-21 (CPD-DAS-20-1016-Dest1)	05-Apr-22																						
DCP DAS (20 dB Attenuator)	SN: 669	13-Dec-21 (No. 5414-466-Dest1)	05-Apr-22																						
Reference Probe E3002	SN: 3010	27-Dec-21 (No. E3-3013-Dest1)	05-Apr-22																						

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Please note that the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention is drawn to the fact that the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300



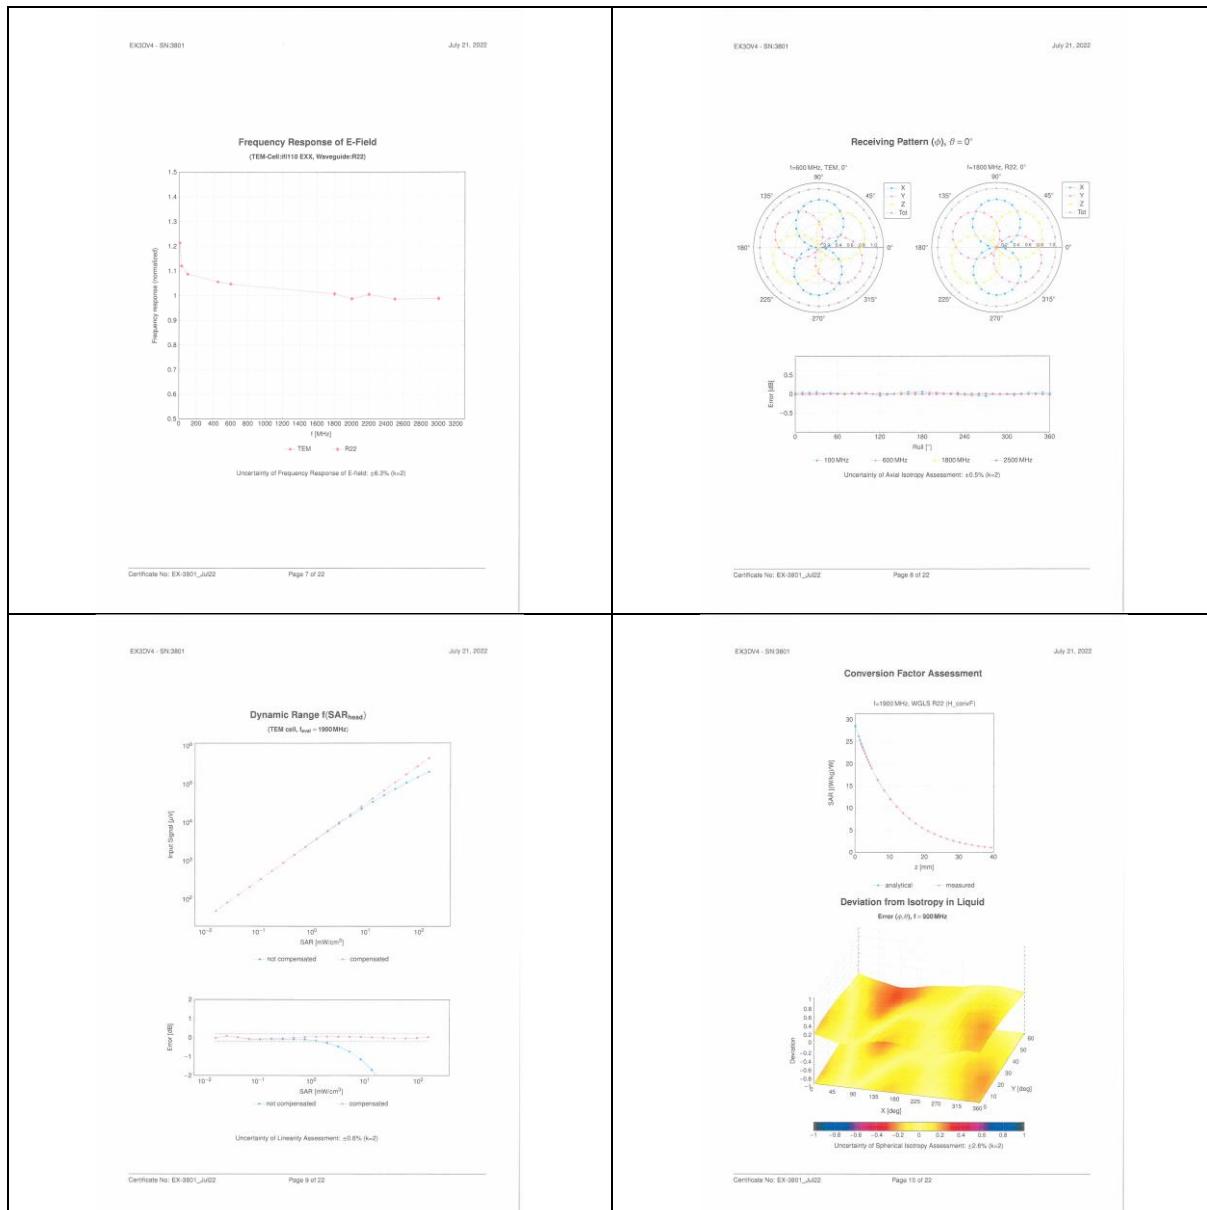

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To need the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility will be its Client and this document does not exonerate the parties to a transaction from exercising all their rights and obligations under the transactional document. This document cannot be reproduced except in full, without prior written permission of the company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s), test and, where applicable, the test method(s) used. The results are retained for 31 days unless otherwise agreed.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, e-mail: info@cnis.org

or email: CN.Doccheck@sgs.com
No.10, Weiye Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overhead, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx>, and for electronic format documents subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions given. The Company's sole responsibility is to the Client and this document does not entitle parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /Inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

or email: CN.Doccheck@gcs.com | No.10, Weivei Road, Innovation Park, Kunshan, Jiangsu, China 215300 t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn

No.10, Wuyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园佳业路10号 邮编 215300
(+86-512) 57355888
f/86-512-57355888
f/86-512-573570818
sqs.china@sgs.com

中国·江苏·昆山市苗子王创业园伟业路10号 邮编 215300

t(86-512)57355888 t(86-512)57370818 sgs.china@sgs.com

1(86-512)57355888 1(86-512)57370818 sys.china@sys.com

4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/26	-31.4	/	47.8	/
2022/4/26	-30.9	1.59%	47.2	0.6
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	ΔΩ
2021/4/21	-23	/	57.1	/
2022/4/21	-22.9	0.43%	56.9	0.2

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

No.10, Weiyi Road, Innovation Park, Kunshan, Jiangsu, China 215300
中国·江苏·昆山市留学生创业园伟业路10号 邮编 215300

t(86-512)57355888 f(86-512)57370818 www.sgsgroup.com.cn
t(86-512)57355888 f(86-512)57370818 sgs.china@sgs.com

