

# Appendix A

## Detailed System Check Results

1. System Performance Check
-----------------------------

System Performance Check 2450 MHz Head
--



**System Performance Check 2450 MHz Head****D2450V2-SN 733**

Communication System: ; Frequency: 2450.000

Medium: Head Simulating Liquid. Medium parameters used:  $f= 2450.000$  MHz;  $\sigma= 1.75$  S/m;  $\epsilon_r = 39.9$

DASY8 Configuration:

- Probe: EX3DV4 - SN7838; ConvF(7.13, 6.8, 7.01); Calibrated: 2024-11-20
- Sensor-Surface: 1.4 mm
- Electronics: DAE4ip Sn1803; Calibrated: 2024-08-08
- Phantom: Twin-SAM V8.0 (30deg probe tilt); Serial: 2156
- Measurement Software: cDASY8 V16.4.0.5005

**Area Scan (40.0 mm x 90.0 mm):** Measurement Grid: 10.0 mm x 15.0 mm

SAR (1g) = 13.7 W/kg; SAR (10g) = 6.56 W/kg;


**Zoom Scan (30.0 mm x 30.0 mm x 30.0 mm):** Measurement Grid: 5.0 mm x 5.0 mm x 1.5 mm

Power Drift = -0.00 dB

**SAR (1g) = 14.1 W/kg; SAR (10g) = 6.53 W/kg;**

M2/M1 [%]=79.8

Dist 3dB Peak [mm]=9.0

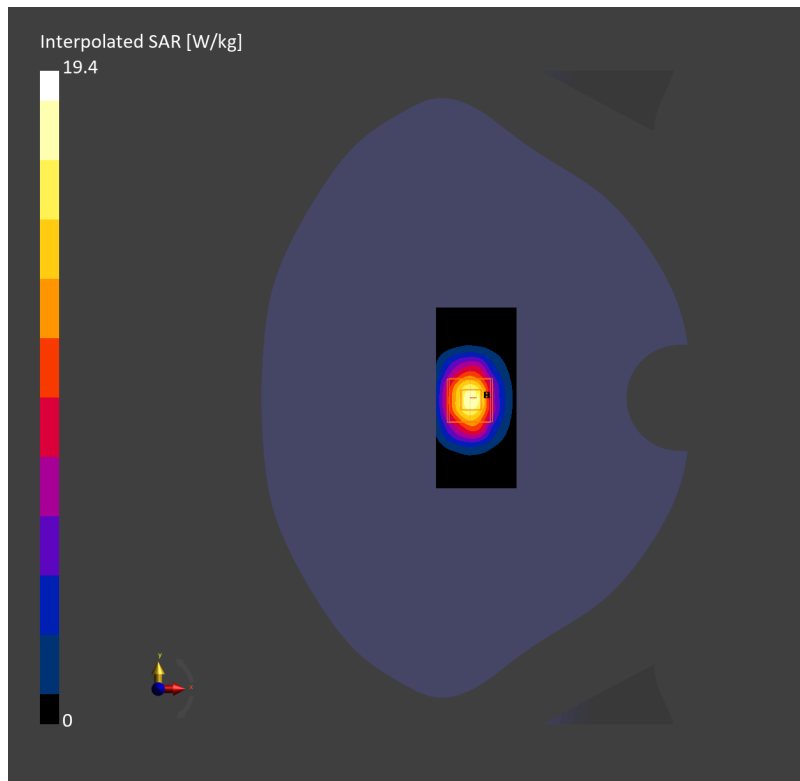

- End of the Appendix -