Test Laboratory: Shenzhen EMTEK Co.,Ltd. Date: 2023/5/6

2.4G

DUT: Endosecpe

Communication System:802.11b; Frequency: 2437 MHz;Duty Cycle: 1:1
Medium: H2450 Medium parameters used: f = 2437 MHz; σ = 1.776 S/m; ε_r = 40.424; ρ = 1000 kg/m^3
Ambient Temperature：22.2 ℃; Liquid Temperature：22.4 ℃

DASY5 Configuration:
- Probe: EX3DV4 - SN7336; ConvF(7.91, 7.91, 7.91); Calibrated: 2022/12/02;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn373; Calibrated: 2022/12/28
- Phantom: ELI v5.0; Type: QDOVA002AA; Serial: TP:1231
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Bottom-Ant1/Area Scan (7x11x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 0.847 W/kg

Bottom-Ant1/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 1.268 V/m; Power Drift = -0.15 dB
Peak SAR (extrapolated) = 2.00 W/kg
SAR(1 g) = 0.877 W/kg; SAR(10 g) = 0.362 W/kg
Maximum value of SAR (measured) = 0.979 W/kg

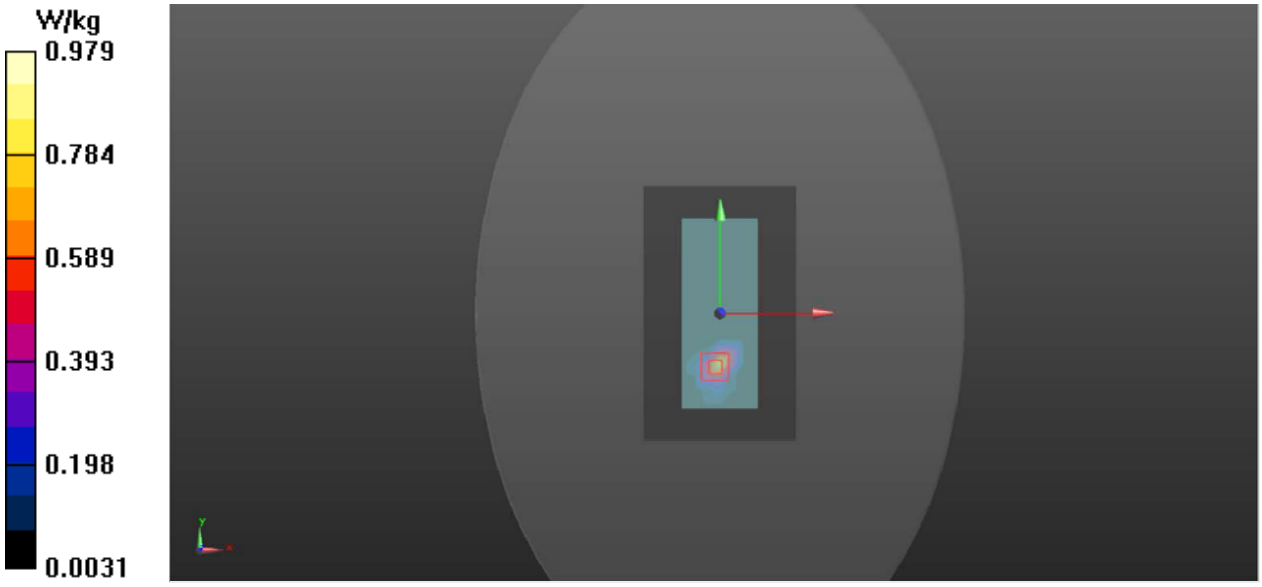

Test Laboratory: Shenzhen EMTEK Co.,Ltd. Date: 2023/5/6

2.4G

DUT: Endosecpe

Communication System:802.11b; Frequency: 2437 MHz;Duty Cycle: 1:1
Medium: H2450 Medium parameters used: f = 2437 MHz; σ = 1.776 S/m; ε_r = 40.424; ρ = 1000 kg/m^3
Ambient Temperature：22.2 ℃; Liquid Temperature：22.4 ℃

DASY5 Configuration:
- Probe: EX3DV4 - SN7336; ConvF(7.91, 7.91, 7.91); Calibrated: 2022/12/02;
- Sensor-Surface: 4mm (Mechanical Surface Detection)
- Electronics: DAE3 Sn373; Calibrated: 2022/12/28
- Phantom: ELI v5.0; Type: QDOVA002AA; Serial: TP:1231
- Measurement SW: DASY52, Version 52.8 (7); SEMCAD X Version 14.6.10 (7164)

Bottom-Ant2/Area Scan (7x11x1): Measurement grid: dx=10mm, dy=10mm

Maximum value of SAR (measured) = 0.676 W/kg

Bottom-Ant2/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 0.545 V/m; Power Drift = -0.16 dB
Peak SAR (extrapolated) = 1.84 W/kg
SAR(1 g) = 0.790 W/kg; SAR(10 g) = 0.314 W/kg
Maximum value of SAR (measured) = 0.941 W/kg