




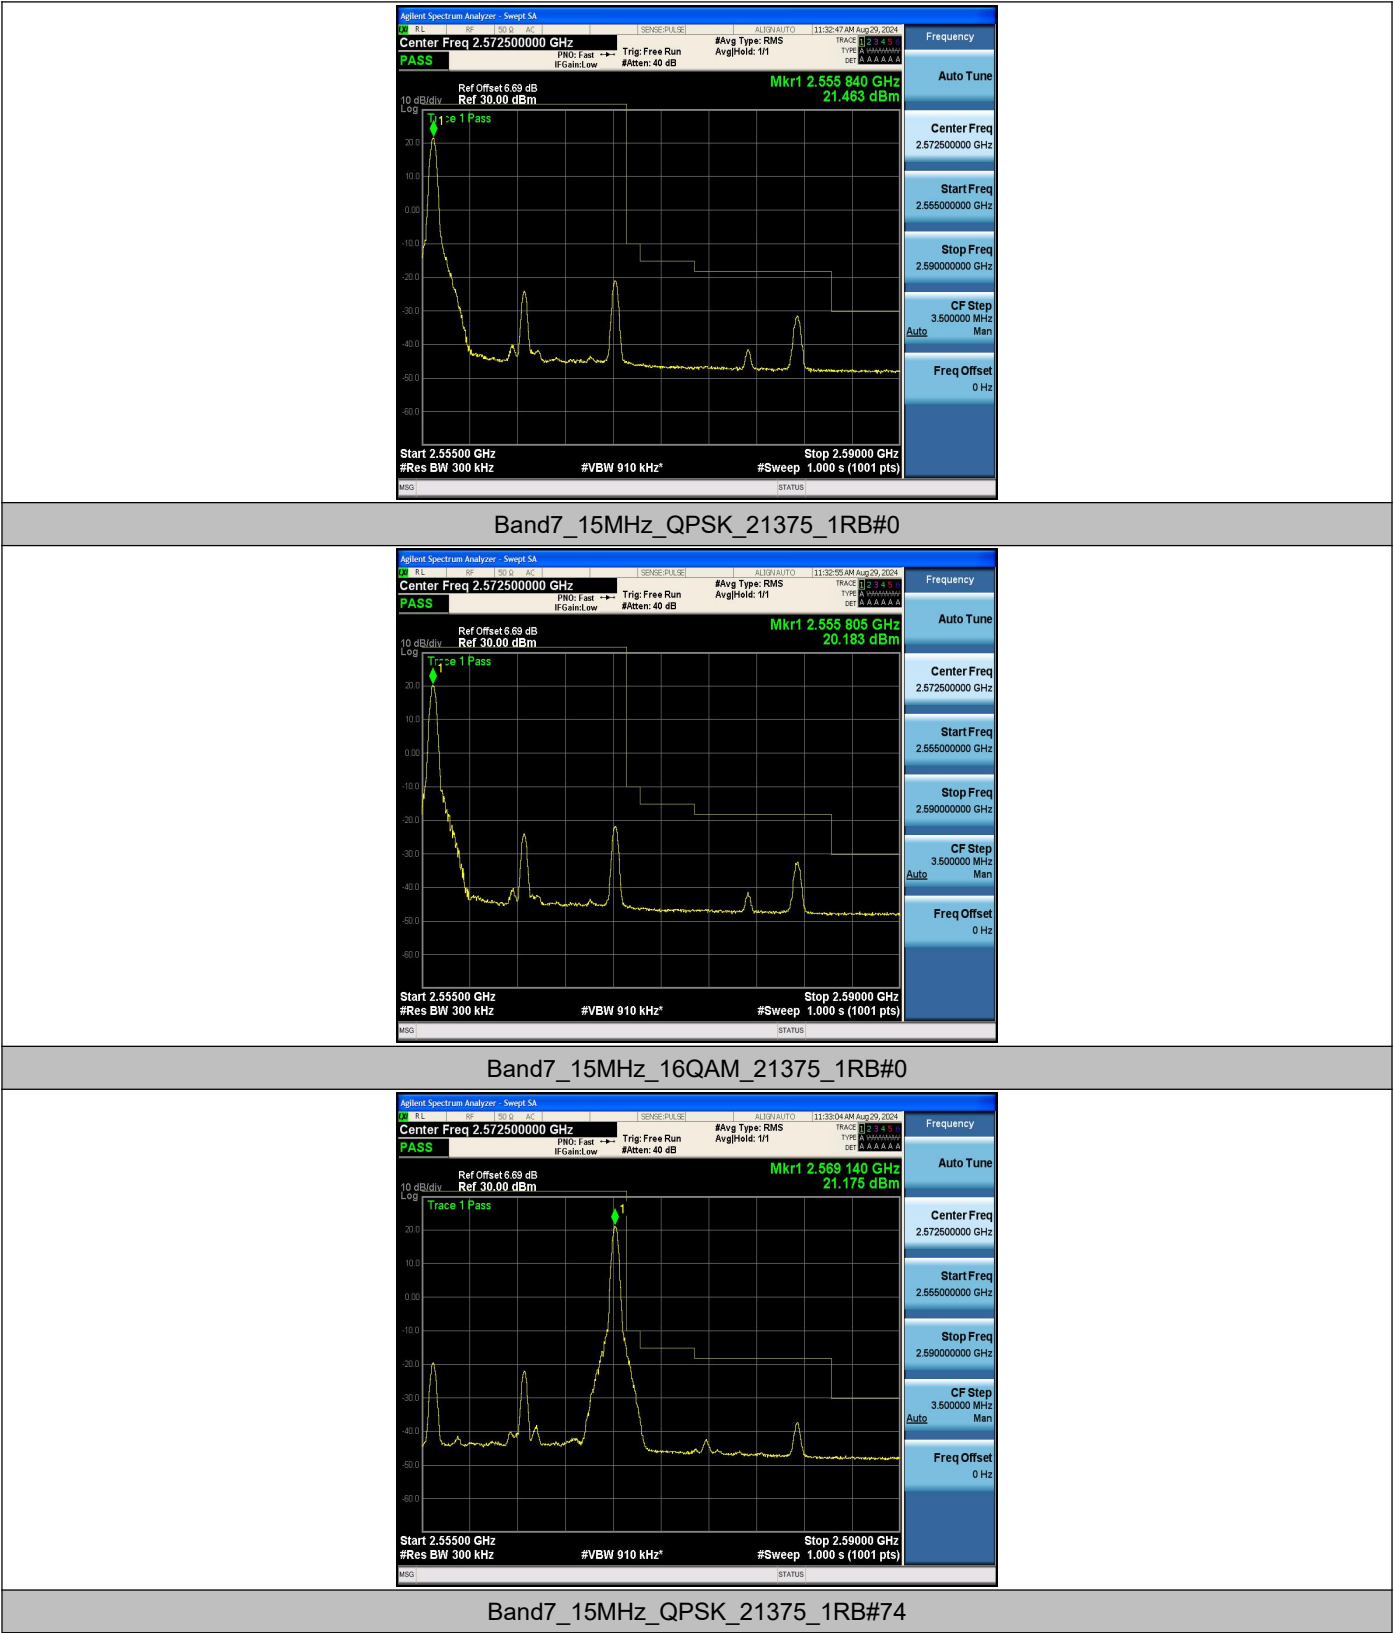


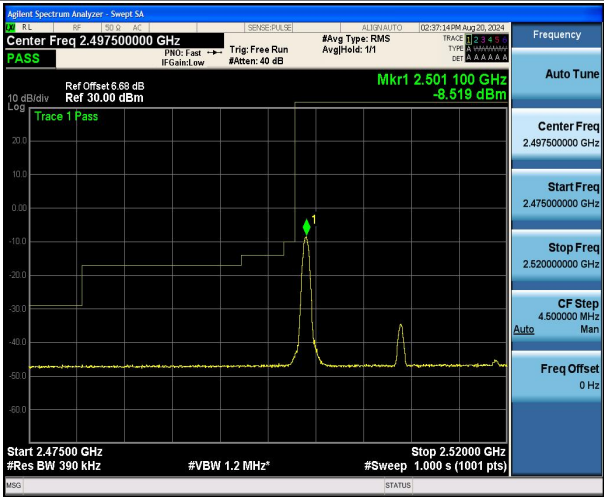

Band7_20MHz_QPSK_20850_1RB#0

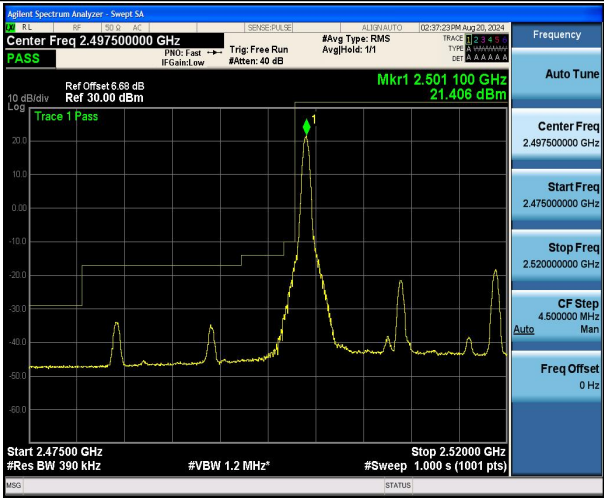

Band7_20MHz_16QAM_20850_1RB#0

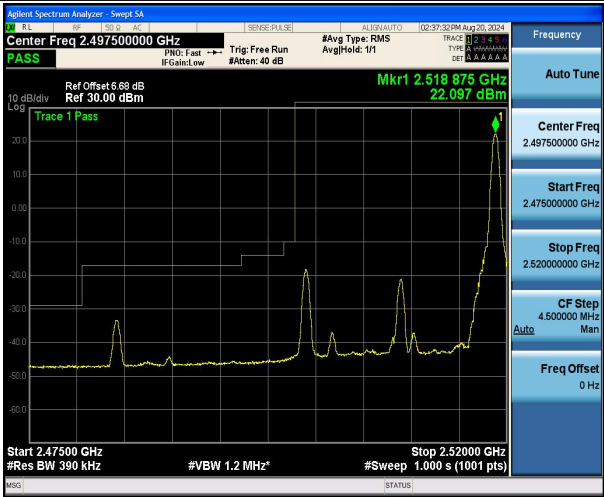

Band7_20MHz_QPSK_20850_1RB#99





Agilent Spectrum Analyzer - Swept SA

Center Freq 2.572500000 GHz

PASS

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.55500 GHz

Res BW 300 kHz

Stop 2.59000 GHz

Sweep 1.000 s (1001 pts)

11:33:29 AM Aug 29, 2024

Trig: Free Run

#Att: 40 dB

#Avg Type: RMS

Avg Hold: 1/1

Trace 1 1

TYPE A

DEF A

10 dB/div

Log

Mkr1 2.556 225 GHz

4.599 dBm

Frequency

Auto Tune

Center Freq

2.572500000 GHz

Start Freq

2.555000000 GHz

Stop Freq

2.590000000 GHz

CF Step

3.500000 MHz

Auto

Man

Freq Offset

0 Hz

Band7_15MHz_16QAM_21375_75RB#0



Agilent Spectrum Analyzer - Sweep SA

Center Freq 2.572500000 GHz

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.550000 GHz

Stop 2.595000 GHz

Res BW 390 kHz

VBW 1.2 MHz

Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq2.572500000 GHz

Start Freq2.550000000 GHz

Stop Freq2.595000000 GHz

CF Step4.500000 MHz

Auto

Freq Offset0 Hz

Band7_20MHz_16QAM_21350_1RB#0

Agilent Spectrum Analyzer - Sweep SA

Center Freq 2.572500000 GHz

Ref Offset 6.69 dB

Ref 30.00 dBm

Trace 1 Pass

Start 2.550000 GHz

Stop 2.595000 GHz

Res BW 390 kHz

VBW 1.2 MHz

Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq2.572500000 GHz

Start Freq2.550000000 GHz

Stop Freq2.595000000 GHz


CF Step4.500000 MHz


Auto


Freq Offset0 Hz



Band7_20MHz_QPSK_21350_1RB#99




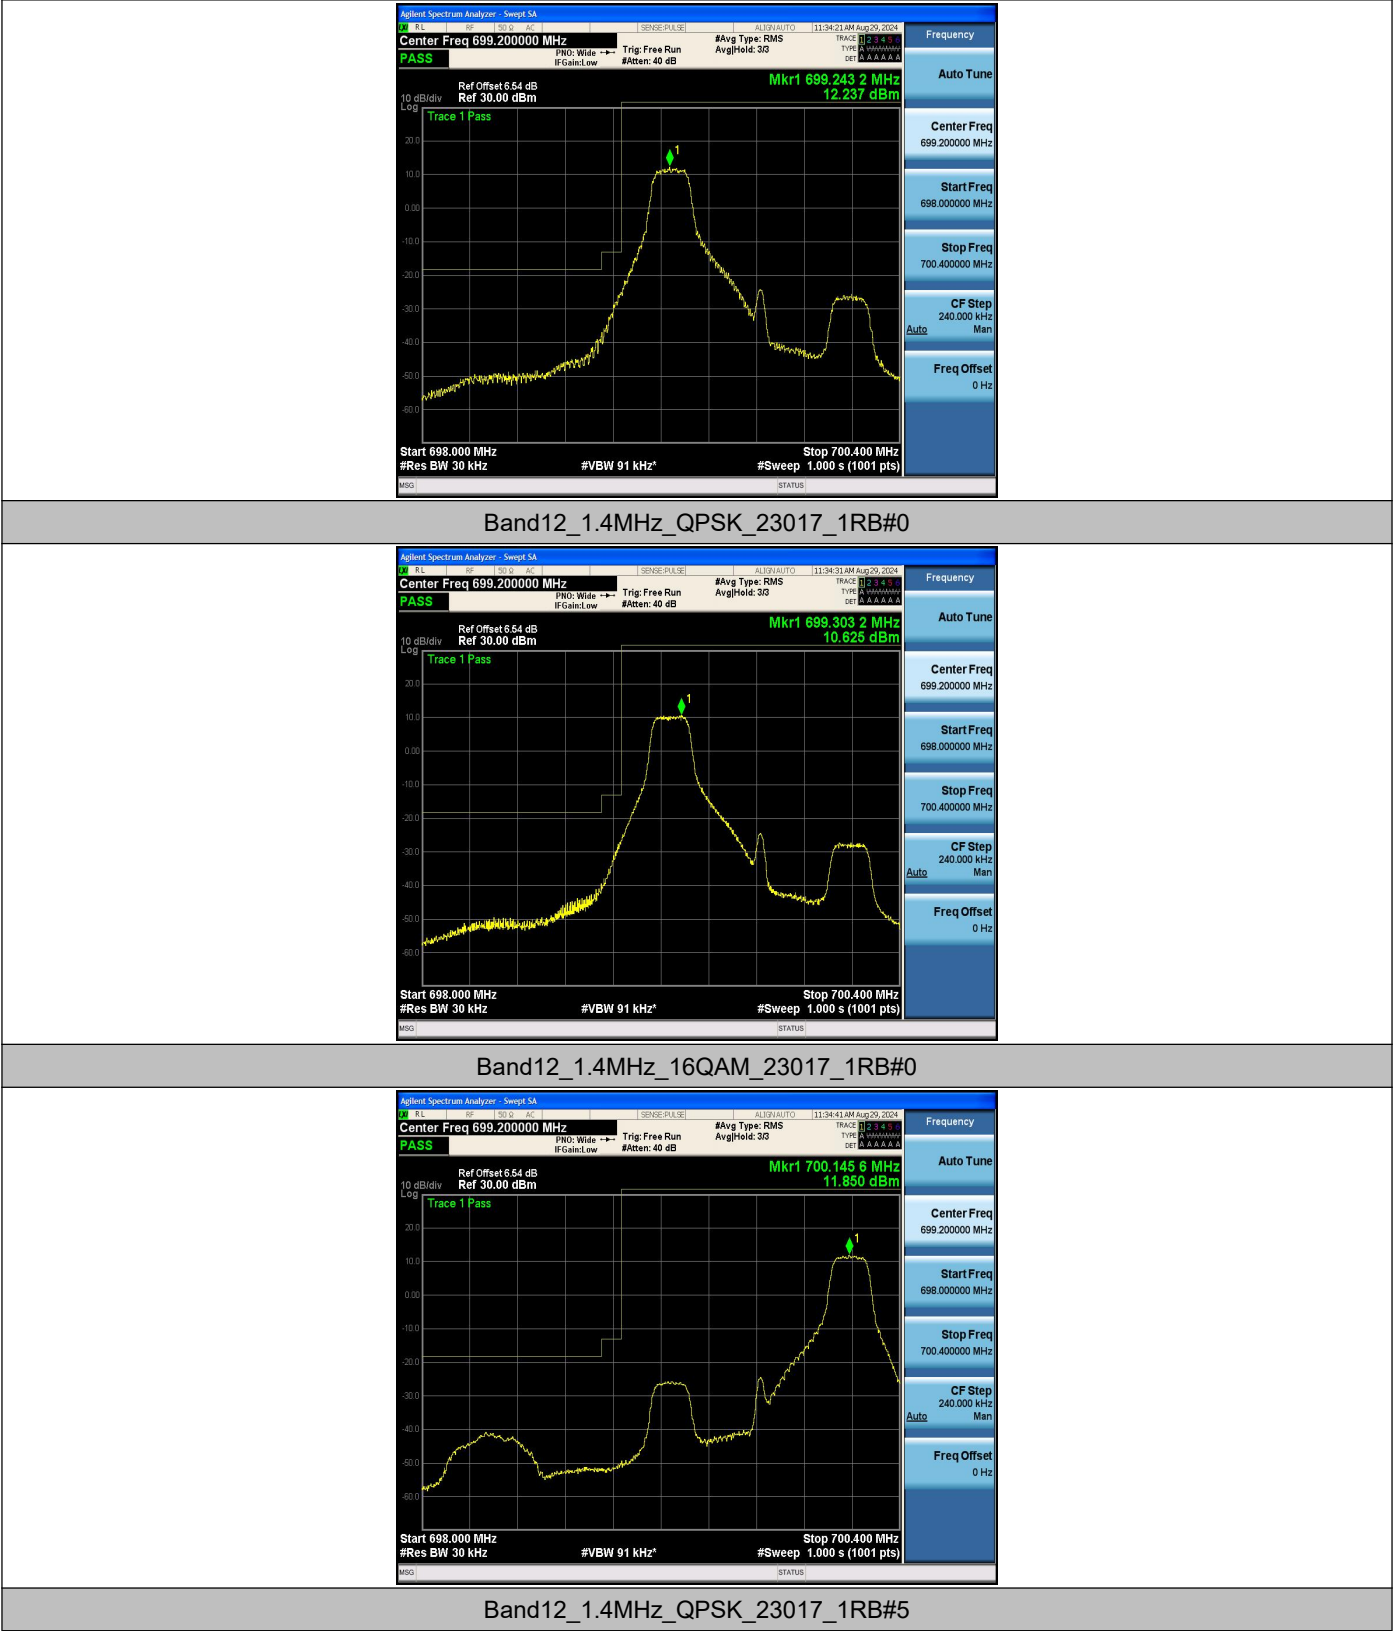

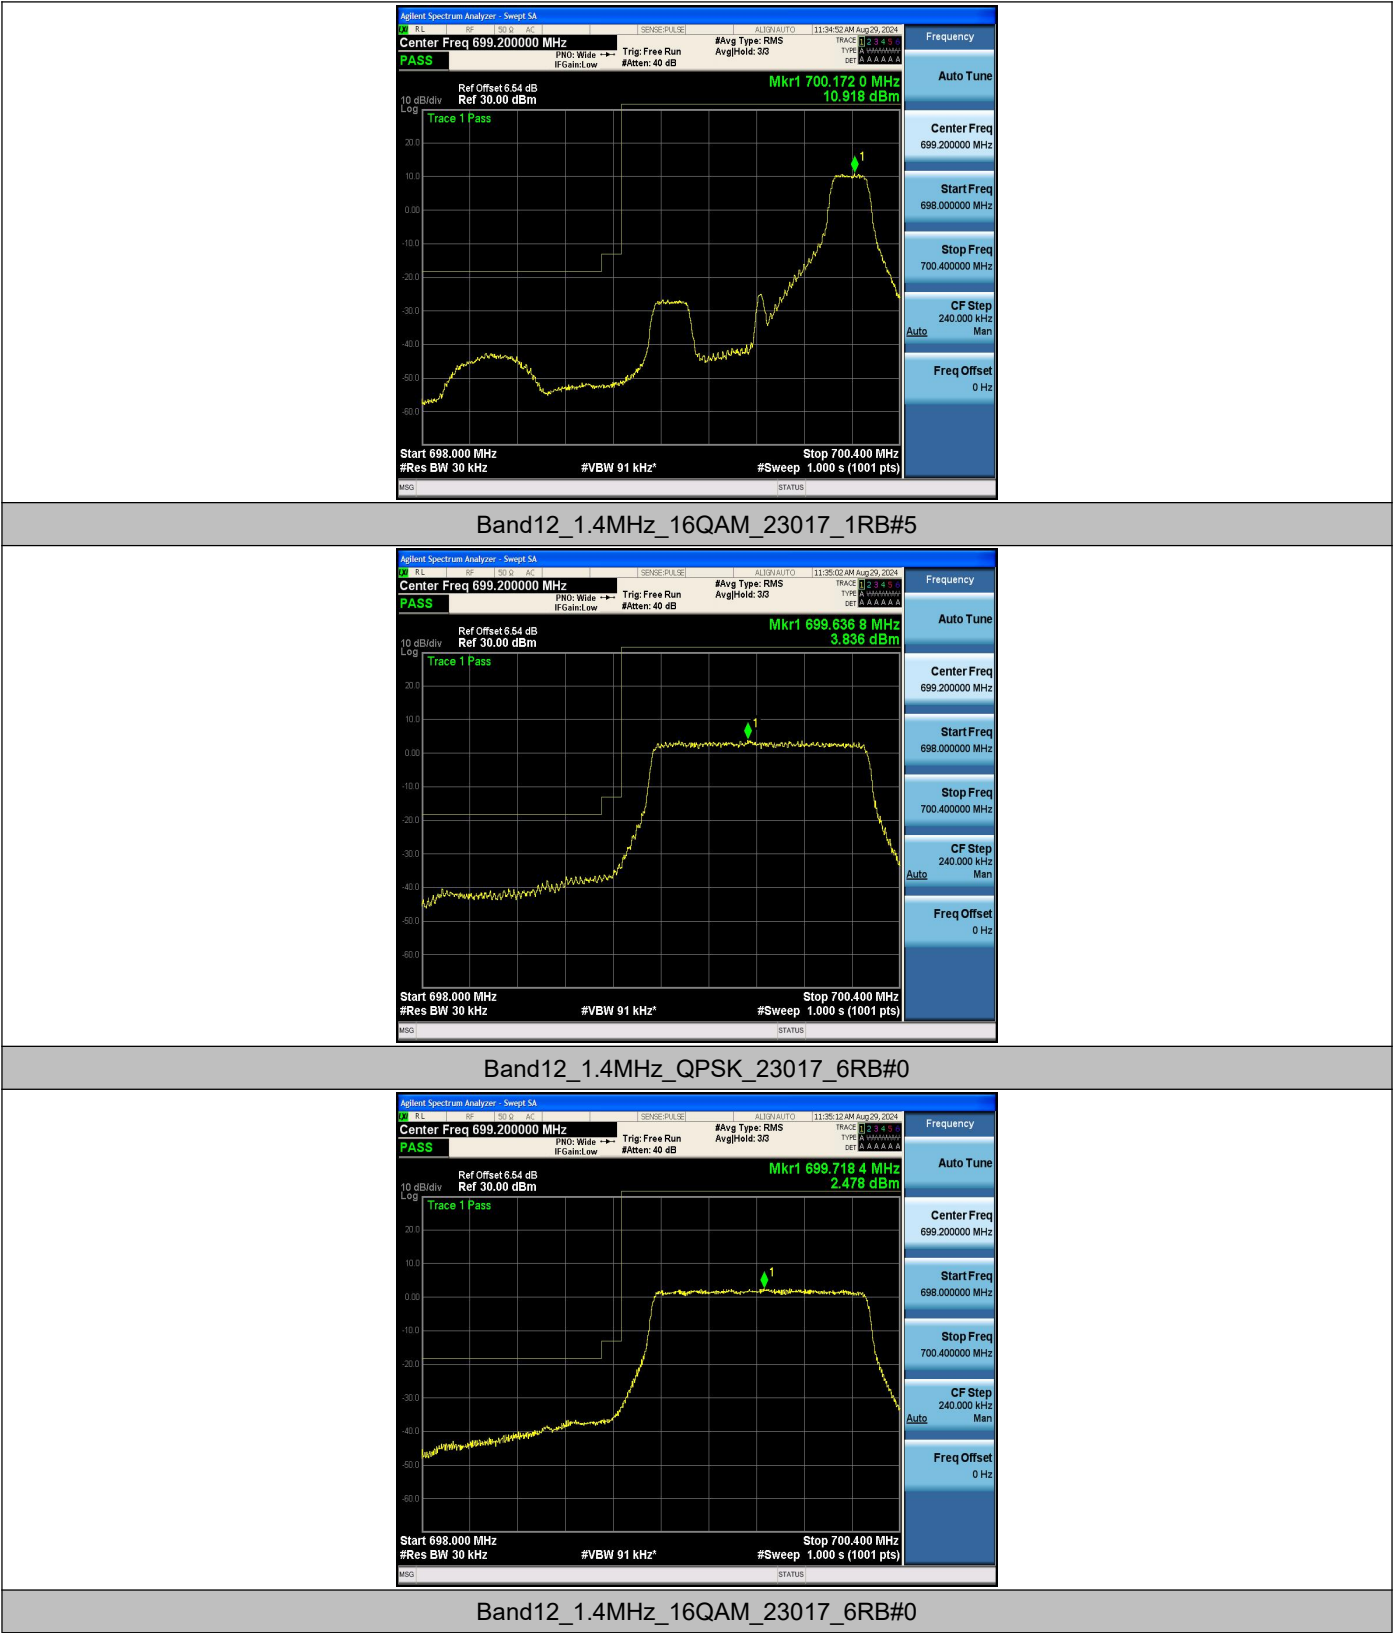

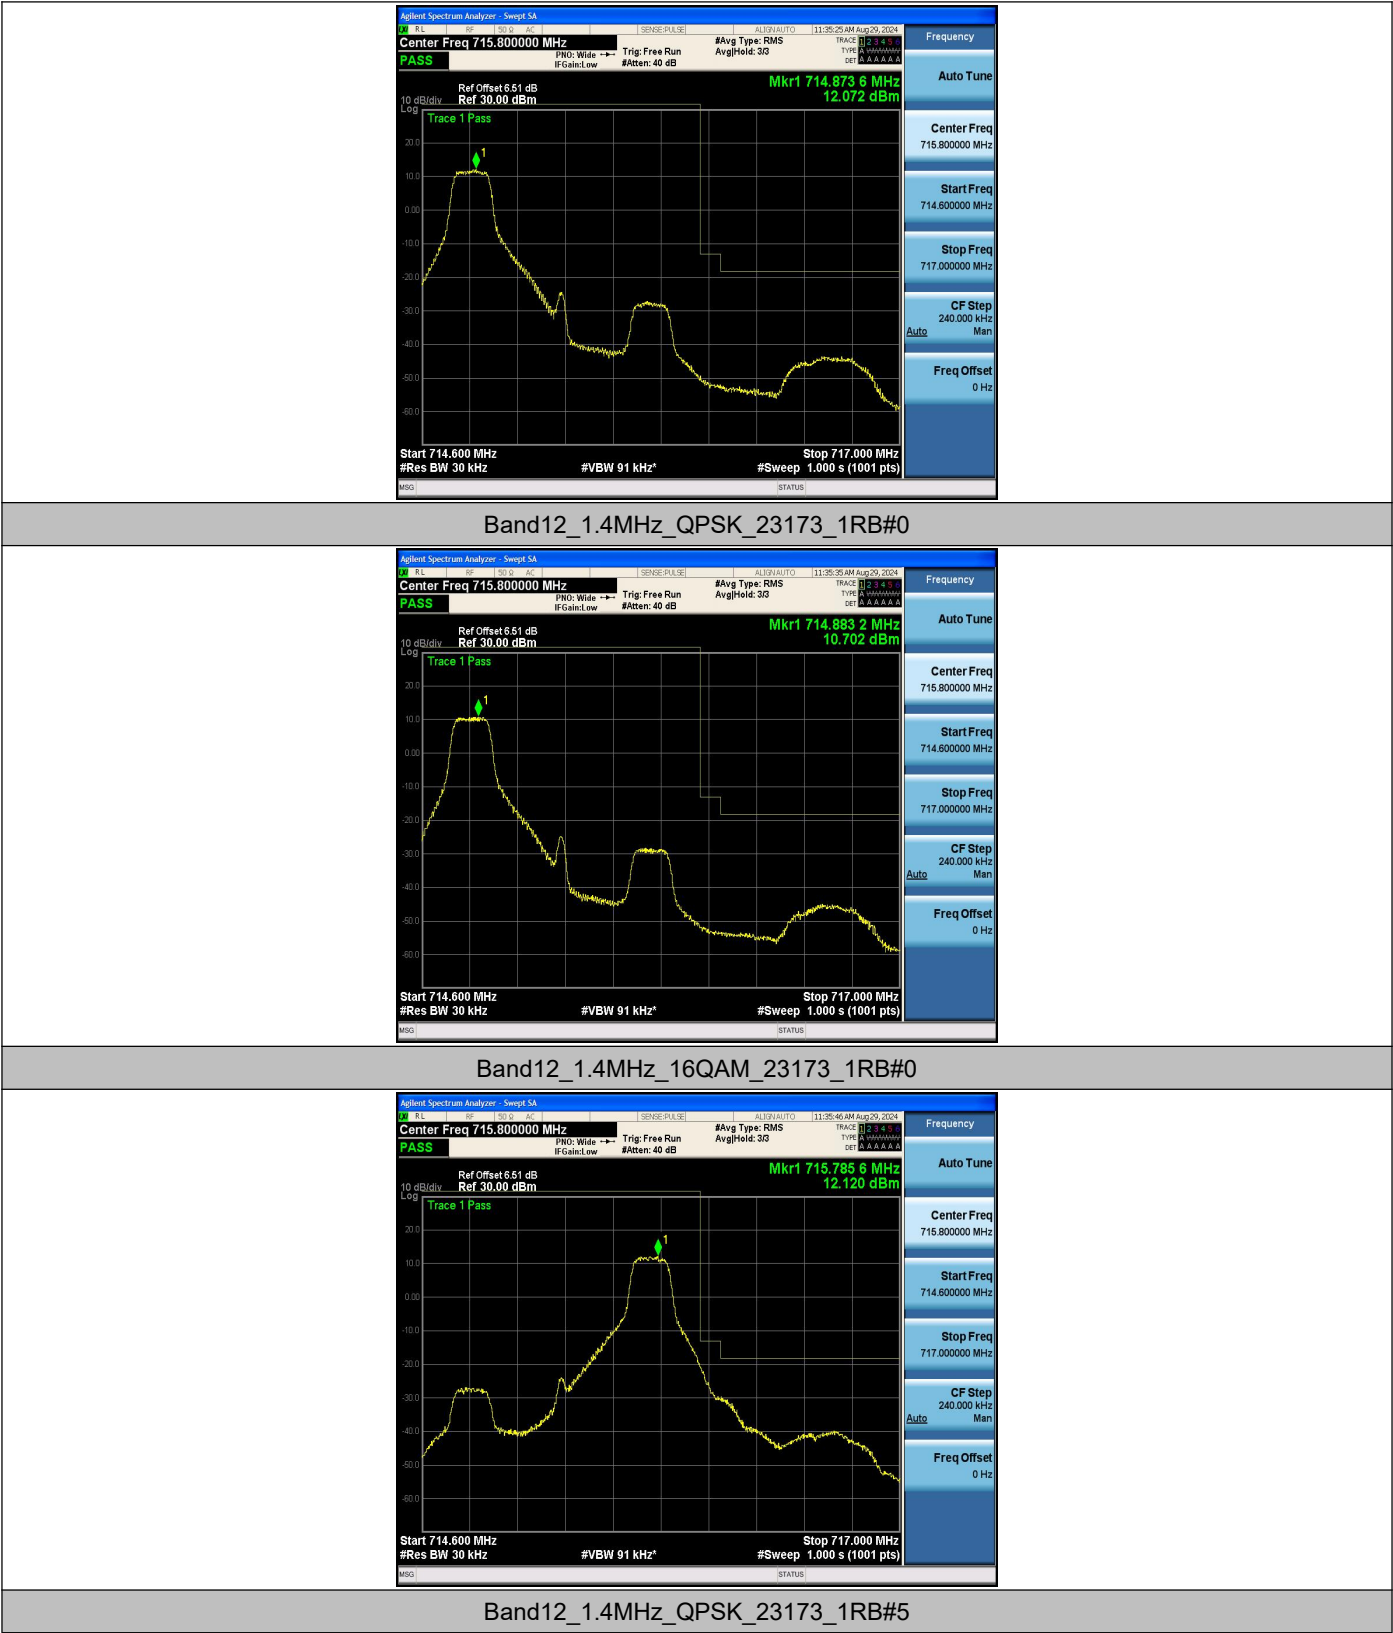



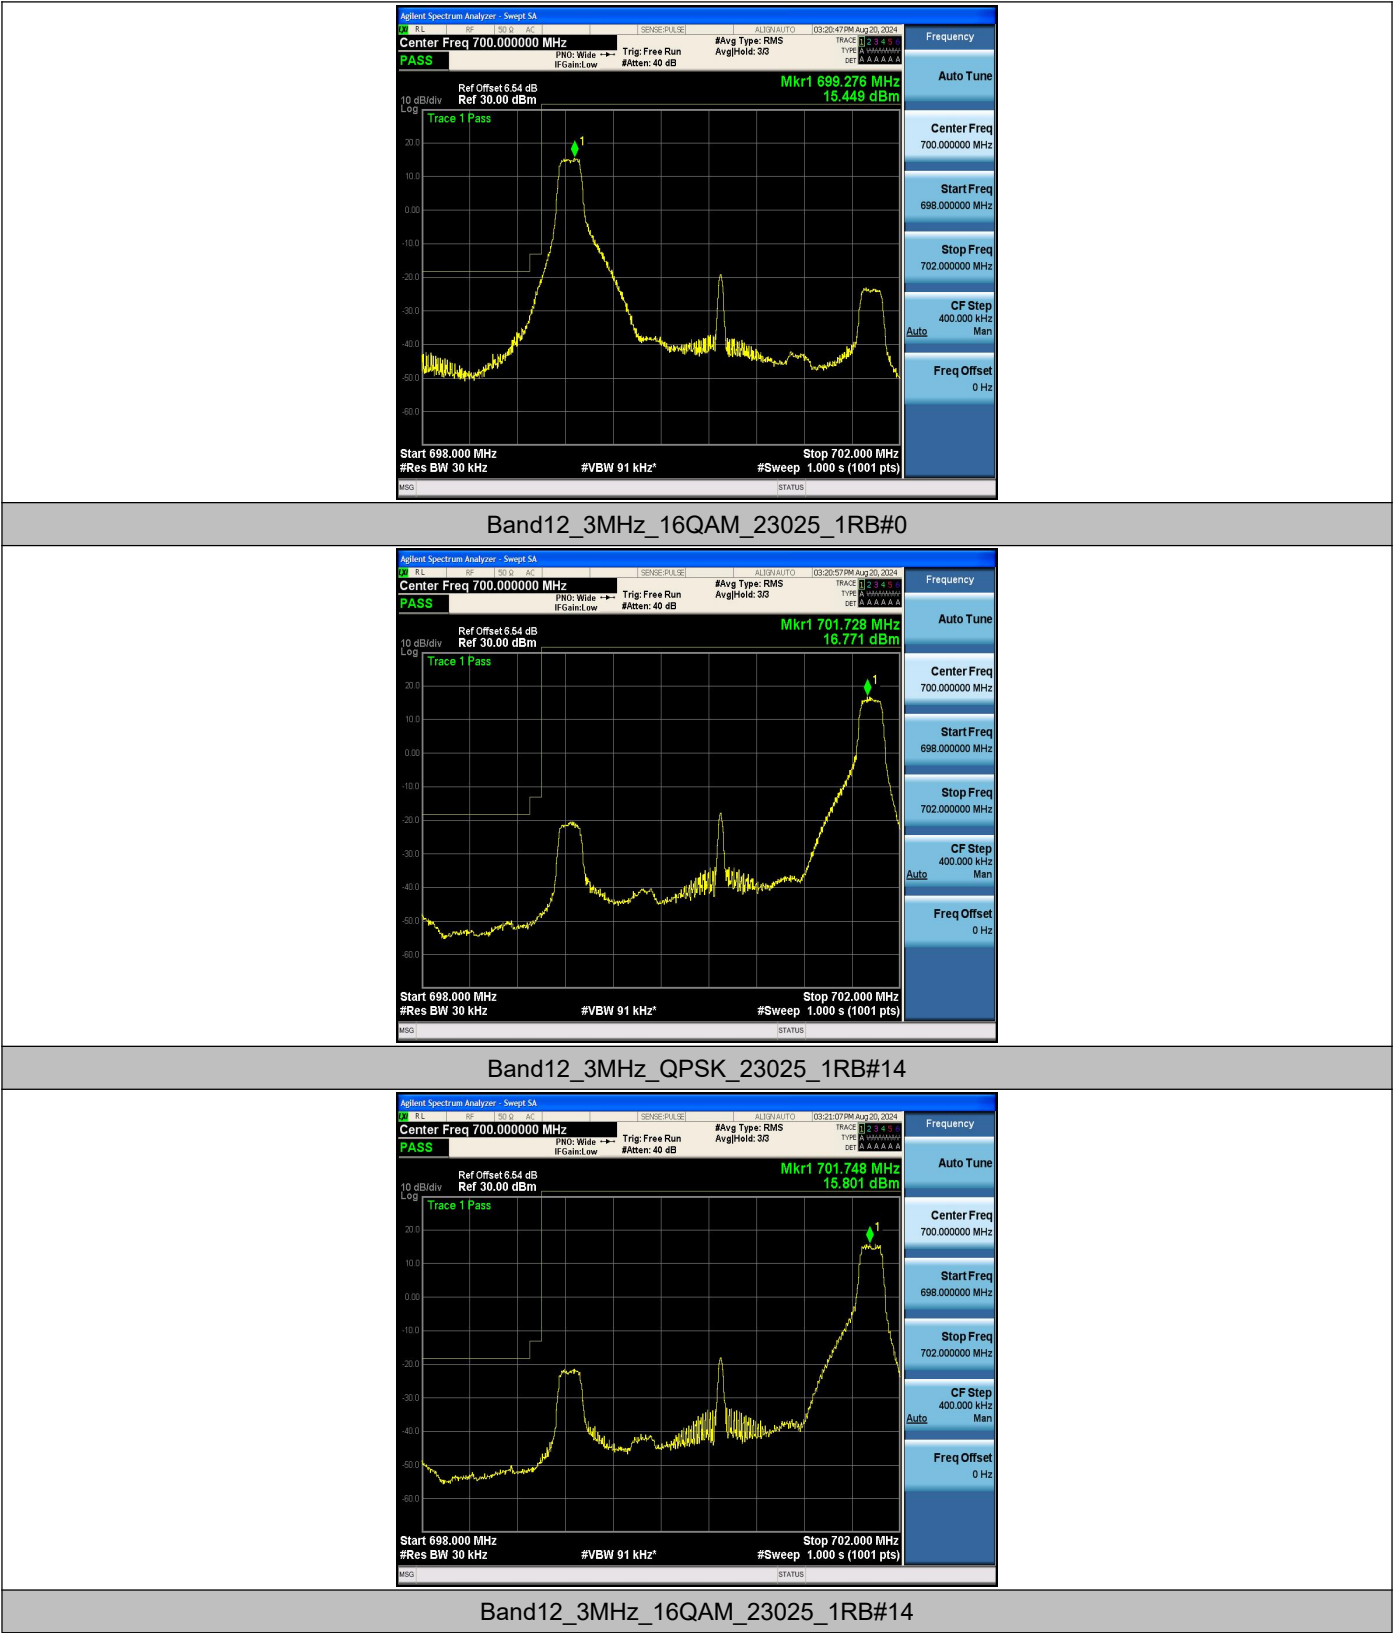

Agilent Spectrum Analyzer - Sweep SA

Center Freq 700.000000 MHz

PASS

Ref Offset 6.54 dB

Ref 30.00 dBm

Trace 1 Pass

Start 698.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 702.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 700.000000 MHz

Start Freq 698.000000 MHz

Stop Freq 702.000000 MHz

CF Step 400.000 kHz


Auto

Freq Offset 0 Hz

Mkr1 701.748 MHz

15.801 dBm

Band12_3MHz_16QAM_23025_1RB#14

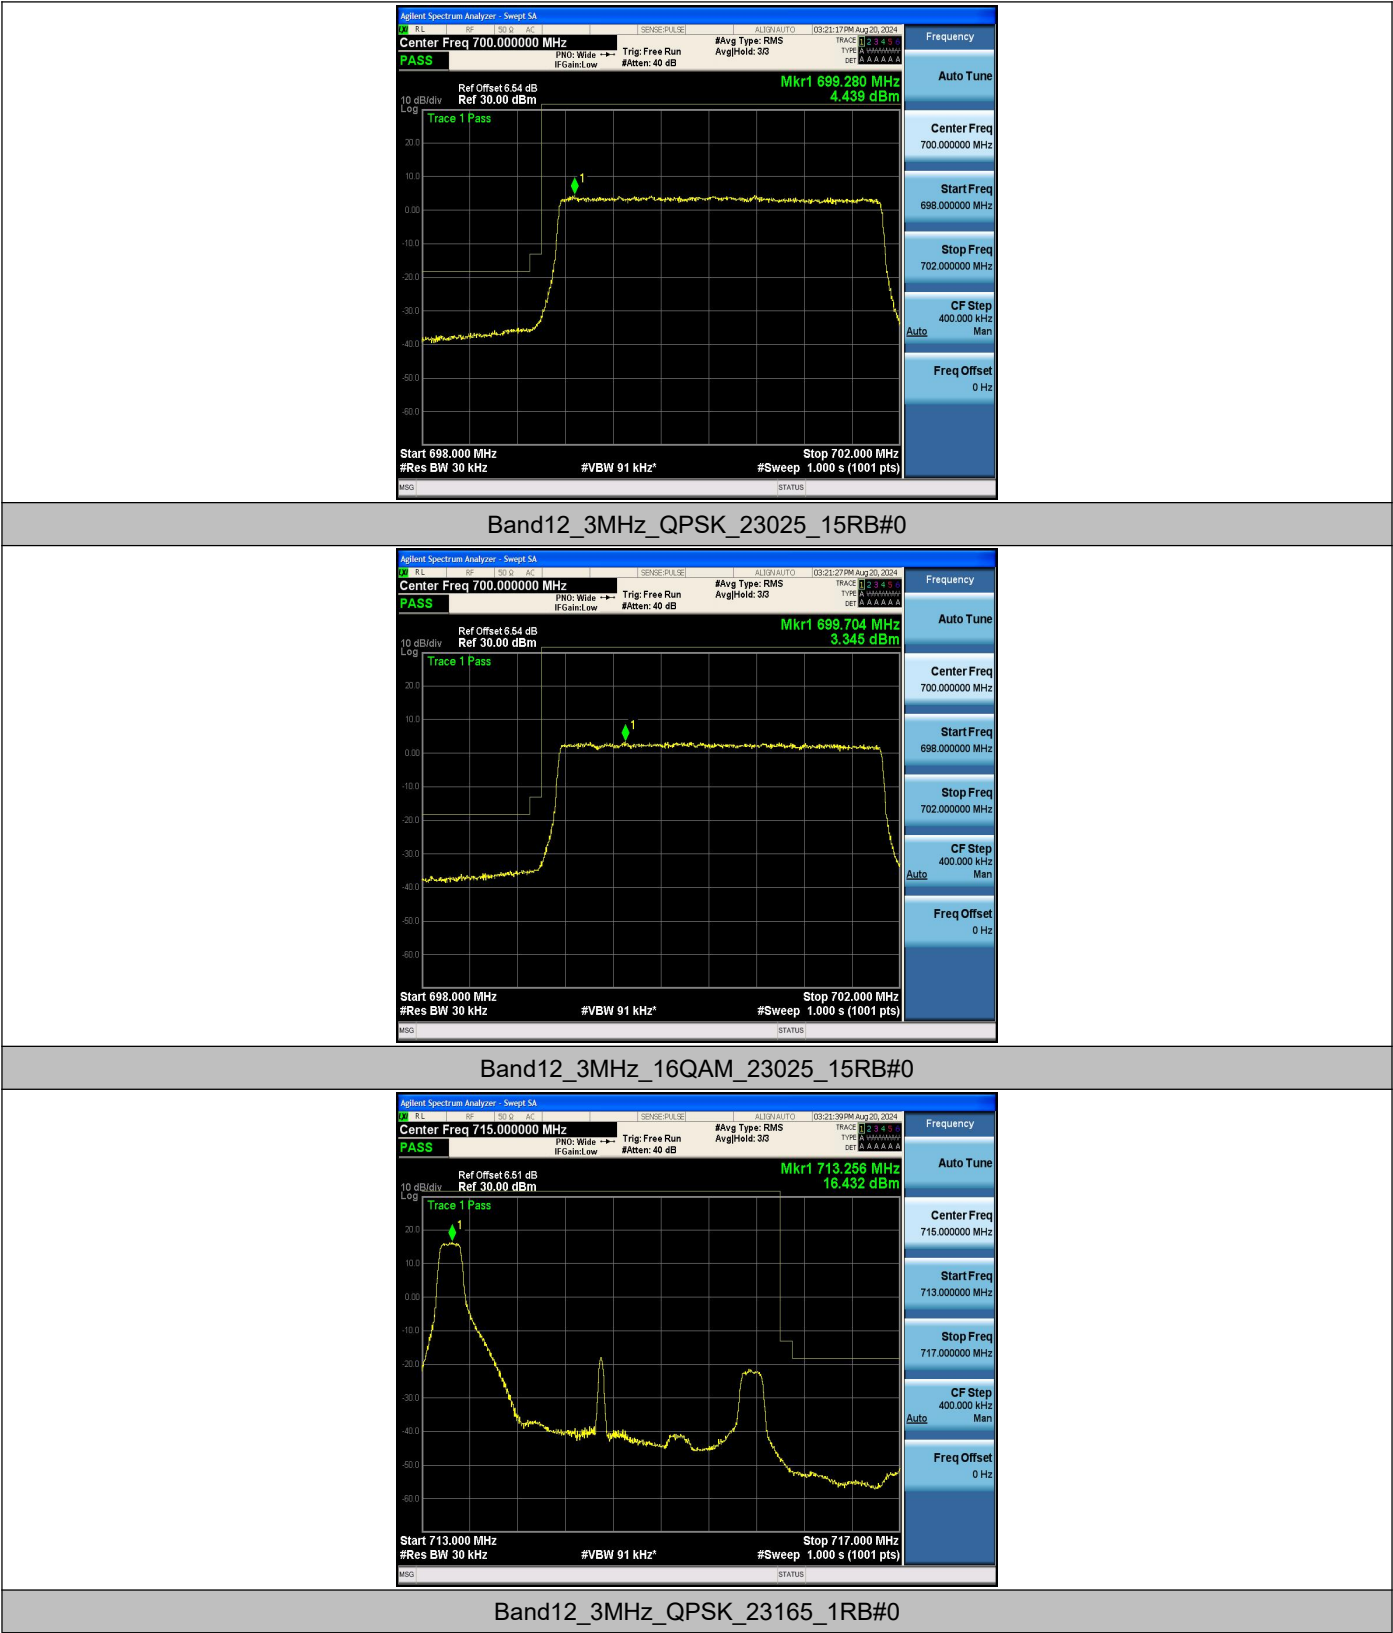



Band12_3MHz_16QAM_23165_1RB#0



Band12_1.4MHz_16QAM_23173_6RB#0



Band12_3MHz_QPSK_23165_1RB#14




Band12_3MHz_16QAM_23165_1RB#14



Band12_3MHz_QPSK_23165_15RB#0



Band12_3MHz_16QAM_23165_15RB#0

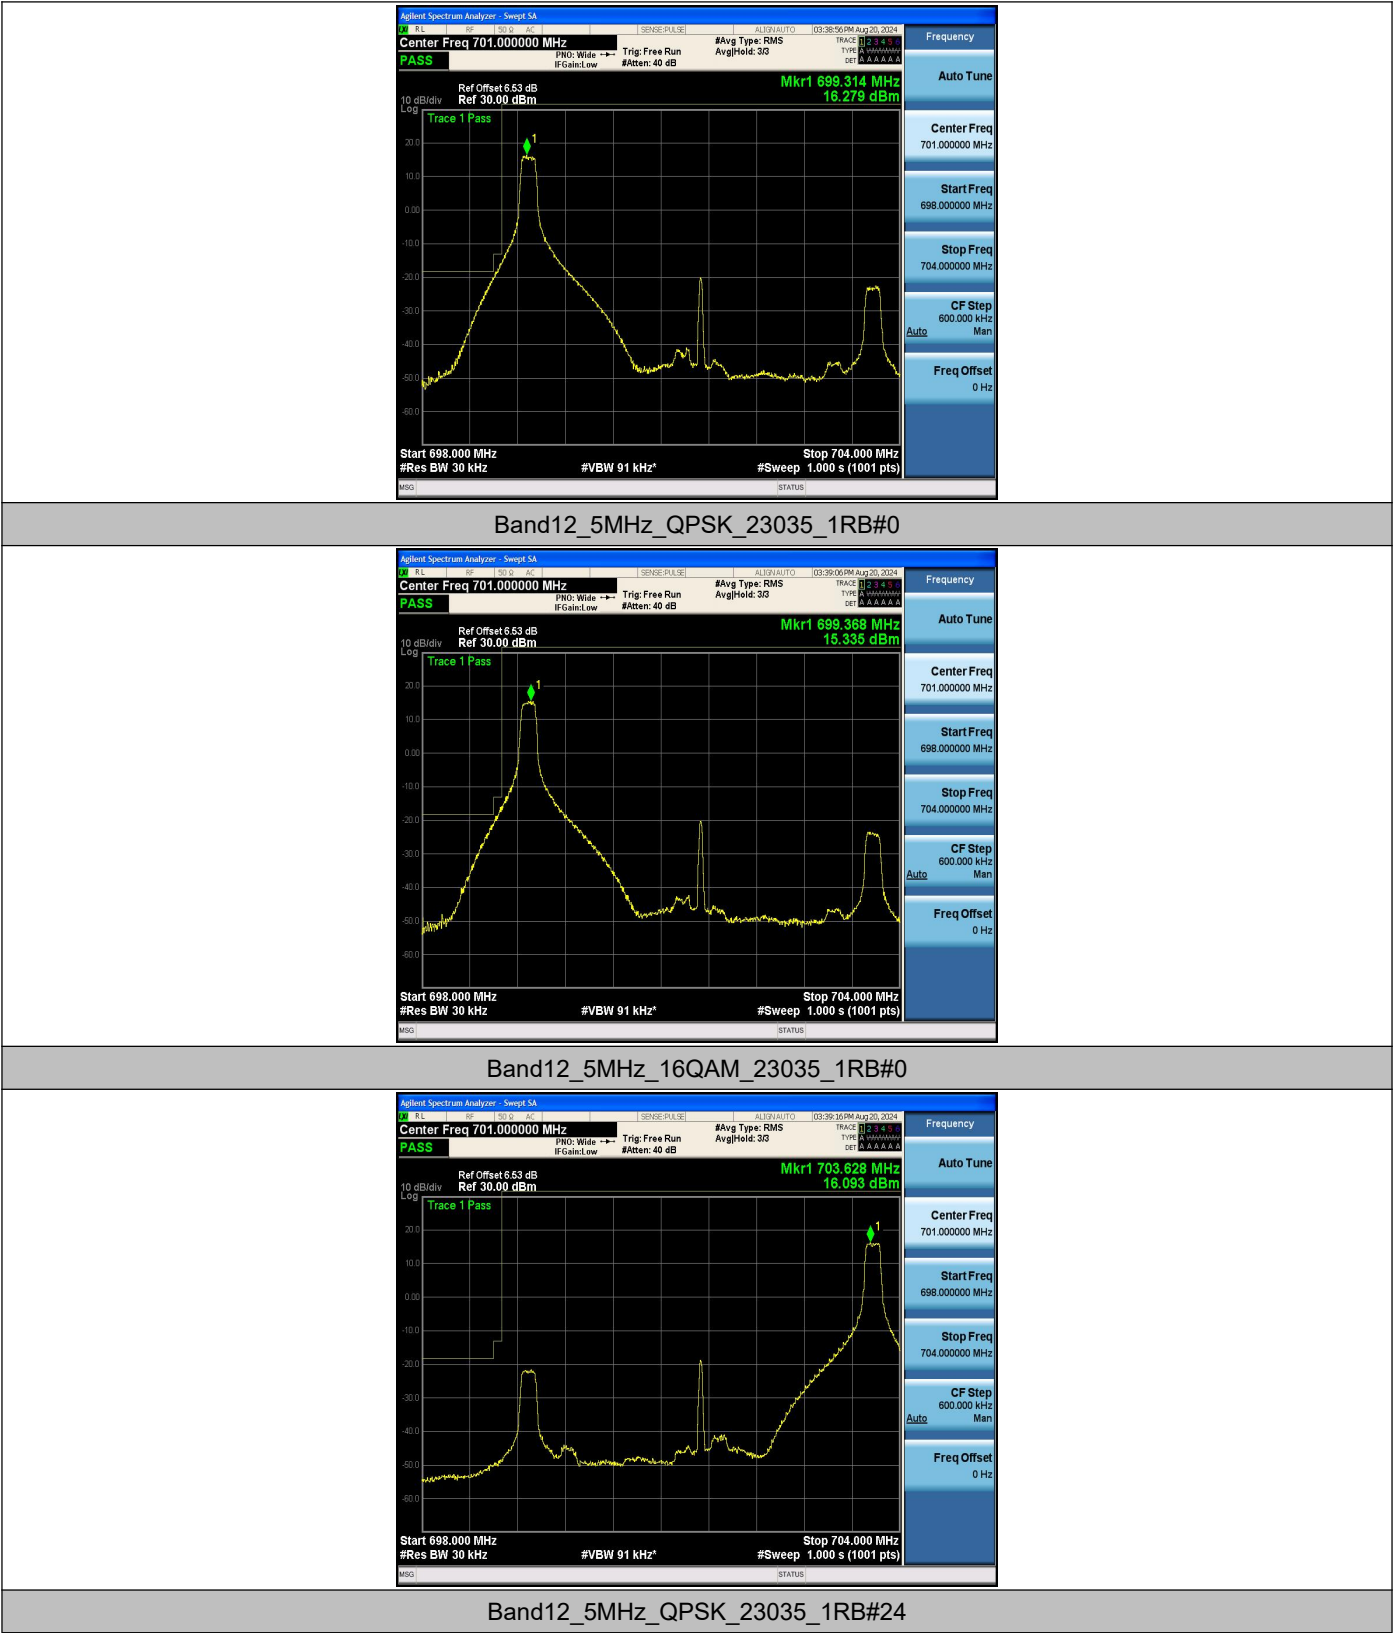

Agilent Spectrum Analyzer - Sweep SA

Center Freq 701.000000 MHz

PASS

Ref Offset 6.53 dB

Ref 30.00 dBm

Trace 1 Pass

Start 698.000 MHz

#Res BW 30 kHz

#VBW 91 kHz

Stop 704.000 MHz

#Sweep 1.000 s (1001 pts)

Frequency

Auto Tune

Center Freq 701.000000 MHz

Start Freq 698.000000 MHz

Stop Freq 704.000000 MHz

CF Step 600.000 kHz


Auto

Man

Freq Offset 0 Hz

Mkr1 703.628 MHz

16.093 dBm

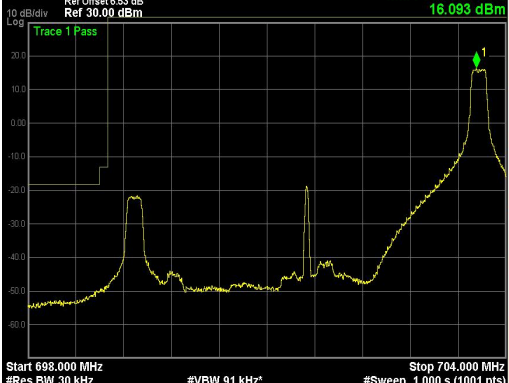

Band12_5MHz_QPSK_23035_1RB#24