

Appendix C for KSCR231000185801

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date	Due date of calibration
Dipole	☐	1	CLA150	4025	2021/04/26	2024/04/25
	☐	2	D450V3	1103	2021/04/21	2024/04/20
	☐	3	D750V3	1188	2022/03/29	2025/03/28
	☐	4	D835V2	4d114	2022/03/31	2025/03/30
	☐	5	D900V2	1d079	2022/06/07	2025/06/06
	☐	6	D1800V2	2d170	2022/03/31	2025/03/30
	☐	7	D1900V2	5d136	2022/06/07	2025/06/06
	☐	8	D2000V2	1041	2022/06/06	2025/06/05
	☐	9	D2300V2	1096	2022/03/31	2025/03/30
	☒	10	D2450V2	817	2022/04/01	2025/03/31
	☐	11	D2600V2	1158	2022/03/31	2025/03/30
	☒	12	D5GHzV2	1095	2022/06/01	2025/05/31
DAE	☒	13	DAE4	1245	2023/04/25	2024/04/24
Probe	☒	14	EX3DV4	3801	2023/06/23	2024/06/22

1 Dipole

1.1 CLA150 - SN 4025

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Client: SGS-CN (Auden)		Certificate No: CLA150-4025_Apr21	
CALIBRATION CERTIFICATE			
Object: CLA150 - SN: 4025			
Calibration procedure(s): QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz			
Calibration date: April 26, 2021			
This calibration certificate documents the traceability to national standards, which require the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 10476	09-Apr-21 (No. 217-03201/03202)	Apr-22
Power sensor NRP Z91	SN: 103344	09-Apr-21 (No. 217-03201)	Apr-22
Power sensor NRP Z91	SN: 103345	09-Apr-21 (No. 217-03202)	Apr-22
Reference 20 dB Attenuator	SN: C23862 (200)	09-Apr-21 (No. 217-03343)	Apr-22
Type-N mismatch combination	SN: 310902 / 0007	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe EX30N4	SN: 3877	30-Dec-20 (No. EX3-0877_Dec20)	Dec-21
ENEA	SN: 664	26-Jan-20 (No. DMS4-654_Jan20)	Jun-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter S44185	SN: G841203074	09-Apr-16 (in house check Jun-20)	In house check: Jun-20
Power sensor E4113A	SN: MY4148067	06-Apr-16 (in house check Jun-20)	In house check: Jun-20
Power sensor E4113A	SN: 000110210	06-Apr-16 (in house check Jun-20)	In house check: Jun-20
RF generator HP 8594D	SN: US8401001709	04-Aug-09 (in house check Jun-20)	In house check: Jun-20
Network Analyzer Agilent E8363A	SN: US41000477	31-Mar-14 (in house check Oct-20)	In house check: Oct-21
Calibrated by:	Name: Jeffrey Katman	Function: Laboratory Technician	Signature:
Approved by:	Name: Kaja Polovic	Function: Technical Manager	Signature:
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: April 26, 2021			
Certificate No: CLA150-4025_Apr21 Page 1 of 6			

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108	
Glossary:			
TSL	Issue simulating liquid		
ConvF	sensitivity in TSL / NORM x,y,z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013			
b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016			
c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010			
d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
e) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in this certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.			
• Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: CLA150-4025_Apr21 Page 2 of 6			

Measurement Conditions		
DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELIA Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	dx, dy = 4.0 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz ± 1 MHz	

Head TSL parameters			
The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	52.3	0.75 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	51.1 ± 6 %	0.75 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL		
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.90 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.88 W/kg ± 19.4 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.60 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	2.59 W/kg ± 18.0 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)	
Antenna Parameters with Head TSL	
Impedance, transformed to feed point	47.9 Ω ± 1.5 (j)
Return Loss	-31.4 dB
Additional EUT Data	
Manufactured by	SPEAG

Certificate No: CLA150-4025_Apr21	
Page 3 of 6	Page 4 of 6

DASY5 Validation Report for Head TSL

Date: 26.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4025

Communication System: UID 0 - CW; Frequency: 150 MHz
Medium parameters used: $f = 150$ MHz; $\sigma = 0.76$ S/m; $\epsilon_0 = 51.1$; $\rho = 1000$ kg/m³
Phantom section: Flat Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(12.51, 12.51, 12.51) @ 150 MHz; Calibrated: 30.12.2020
- Sensor Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA84 SN654; Calibrated: 26.06.2020
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP.1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan,

dist=1.4mm (8x10x8)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 85.93 W/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 7.36 W/kg

SAR(1 g) = 3.90 W/kg; SAR(10 g) = 2.60 W/kg

Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 30mm)


Ratio of SAR at M2 to SAR at M1 = 80.4%

Maximum value of SAR (measured) = 5.48 W/kg

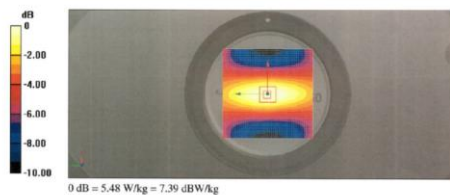

Certificate No: CLA150-4025_Apr21

Page 5 of 6

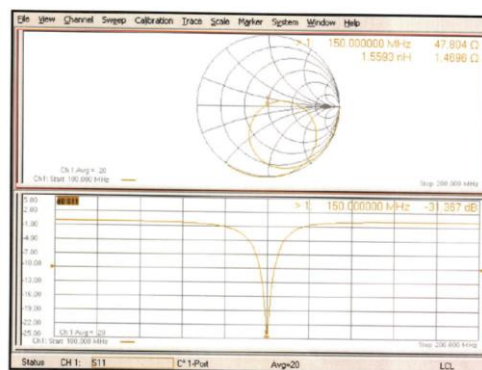

Certificate No: CLA150-4025_Apr21

Page 6 of 6

1.2 D450V3 - SN 1103

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client: SGS-CN (Aude)

Certificate No: D450V3-1103_Apr21

CALIBRATION CERTIFICATE

Object	D450V3 - SN: 1103		
Calibration procedure(s)	QA CAL-15_v9 Calibration Procedure for SAR Validation Sources below 700 MHz		
Calibration date:	April 21, 2021		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 2) °C and humidity < 70%.			
Calibration Equipment used (MPE critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03021/03020)	Apr-22
Power sensor NRP-291	SN: 103244	09-Apr-21 (No. 217-03021)	Apr-22
Power sensor NRP-291	SN: 103245	09-Apr-21 (No. 217-03020)	Apr-22
Reference 20 dB Attenuator	SN: CC2852 (200)	09-Apr-21 (No. 217-03345)	Apr-22
Type-N mismatch combination	SN: 310852 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe E3030A	SN: 3877	30-Dec-20 (No. E30-3877 Dec20)	Dec-21
DAEA	SN: 654	26-Jun-20 (No. D454-654-Jun20)	Jun-21
Secondary Standards	ID #	Check Date (In house)	Scheduled Check
Power meter E4418B	SN: G841200274	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Power sensor E4412A	SN: MY41496027	06-Apr-16 (In house check Jun-20)	In house check Jun-22
Power sensor E4412A	SN: 00018010	06-Apr-16 (In house check Jun-20)	In house check Jun-22
RF generator HP 8548C	SN: U503460101700	06-Aug-09 (In house check Jun-20)	In house check Jun-22
Network Analyzer Agilent E8308A	SN: U841980477	31-Mar-14 (In house check Oct-20)	In house check Oct-21
Calibrated by:	Name: Claudio Leubler	Function: Laboratory Technician	Signature: [Signature]
Approved by:	Name: Kello Polovic	Function: Technical Manager	Signature: [Signature]
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: April 23, 2021			

Certificate No: D450V3-1103_Apr21

Page 1 of 6

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL: Issue simulating liquid
ConvF: sensitivity in TSL / NORM x,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC 61010-1:2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21

Page 2 of 6

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V62.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELJ4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	$dx, dy, dz = 5$ mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.57 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	43.1 $\pm$ 6 %	0.57 mho/m $\pm$ 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.55 W/kg $\pm$ 18.1 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	0.757 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg $\pm$ 17.6 % (k=2)

Certificate No: D450V3-1103_Apr21

Page 5 of 6

DASY5 Validation Report for Head TSL

Test Laboratory: SPEAG, Zurich, Switzerland

Date: 21.04.2021

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450$ MHz; $\alpha = 0.87$ S/m; $\epsilon_r = 43.1$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.64, 10.64, 10.64) @ 450 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 26.06.2020
- Phantom: ELJ v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 39.18 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 1.76 W/kg

SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.767 W/kg

Smallest distance from peaks to all points 3 dB below: Larger than measurement grid

Ratio of SAR at M2 to SAR at M1 = 64.9%

Maximum value of SAR (measured) = 1.53 W/kg

0 dB = 1.53 W/kg = 1.85 dBW/kg

Certificate No: D450V3-1103_Apr21

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	57.1 Ω - 2.8 j Ω
Return Loss	-23.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.346 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when twisted according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: D450V3-1103_Apr21

Page 6 of 6

Certificate No: D450V3-1103_Apr21

Page 6 of 6


1.3 D750V3 - SN 1188

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Client: SGS-CN		Certificate No: Z22-60103	
CALIBRATION CERTIFICATE			
Object	D750V3 - SN: 1188		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 28, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	104277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP88	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator S4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23
Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: [Signature]
Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: [Signature]
Approved by:	Name: Qi Dianyan	Function: SAR Project Leader	Signature: [Signature]
Issued: April 3, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60103		Page 1 of 6	

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY52	VS2.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	750 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.07 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.37 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60103		Page 3 of 6	

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Glossary: TSL tissue simulating liquid ConvF sensitivity in TSL / NORMx.y.z N/A not applicable or not measured			
Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation: c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters: - Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. - Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. - Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. - Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. - SAR measured: SAR measured at the stated antenna input power. - SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. - SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60103		Page 2 of 6	

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	53.60-1.13jΩ		
Return Loss	-28.7dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	0.947 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60103		Page 4 of 6	

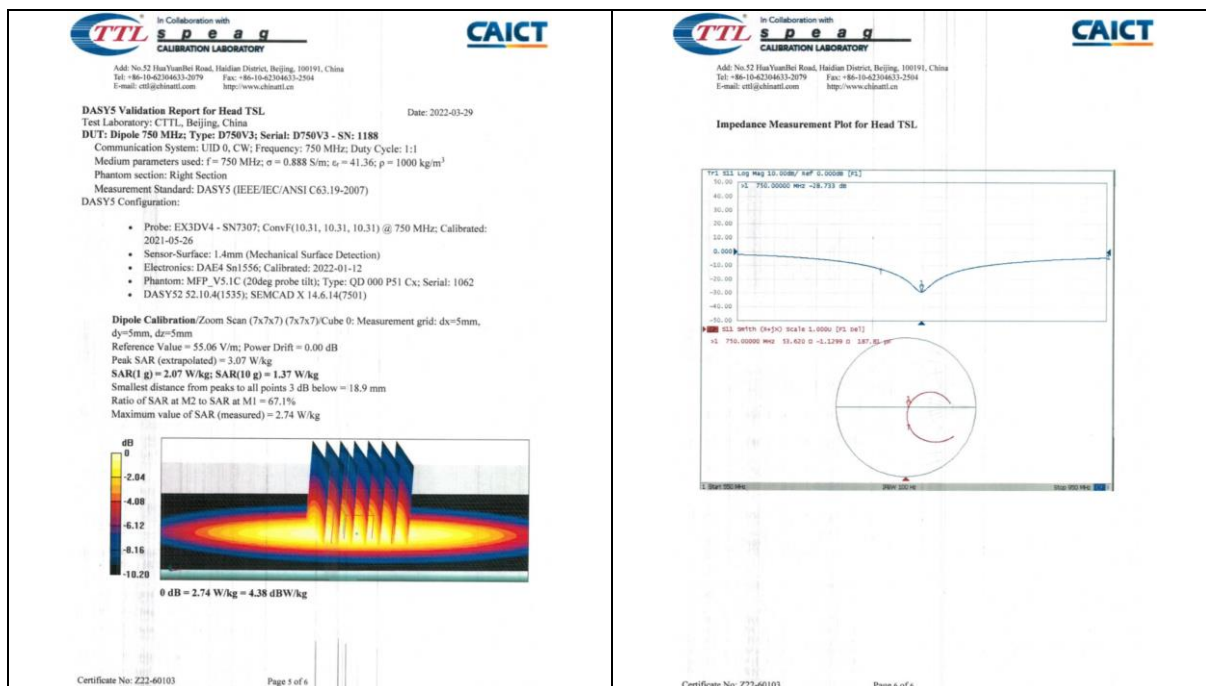

1.4 D835V2 - SN 4d114

TTL Calibration Laboratory In Collaboration with **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60104**

CALIBRATION CERTIFICATE

Object: **D835V2 - SN: 4d114**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This Calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL, No.J21X08326)	Sep-22
Power sensor NRPBS	104261	24-Sep-21 (CTTL, No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG, No. EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG, No. Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL, No.J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL, No.J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer

Reviewed by: **Lin Hao** SAR Test Engineer

Approved by: **Qi Dianyan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60104 Page 1 of 6

TTL Calibration Laboratory In Collaboration with **CAICT**

Address: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-4204633-2079 Fax: +86-10-4204633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:

TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook


Methods Applied and Interpretation of Parameters:


- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60104 Page 2 of 6

TTL SPEAG CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	VS2 10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	835 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 5 %	0.91 mho/m ± 5 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.37 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	9.40 W/kg ± 18.5 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.54 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	6.12 W/kg ± 18.7 % (k=2)	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.70 - j22.0Q		
Return Loss	-25.3dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.307 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60104 Page 3 of 6			

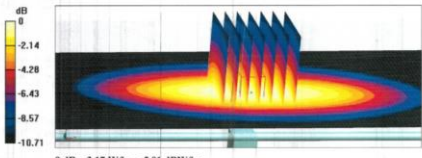TTL SPEAG CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d114 Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1 Medium parameters used: f = 835 MHz; σ = 0.907 S/m; ε _r = 40.98; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7307; ConvF(10.13, 10.13, 10.13) @ 835 MHz; Calibrated: 2021-05-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA4 E4 Sn1556; Calibrated: 2022-01-12 - Phantom: MFP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501)			
Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 57.88 V/m; Power Drift = 0.04 dB Peak SAR (extrapolated) = 3.56 W/kg SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.54 W/kg Smallest distance from peaks to all points 3 dB below = 15.8 mm Ratio of SAR at M2 to SAR at M1 = 66.2% Maximum value of SAR (measured) = 3.17 W/kg			
			
0 dB = 3.17 W/kg = 5.01 dBW/kg			
Certificate No: Z22-60104 Page 5 of 6			

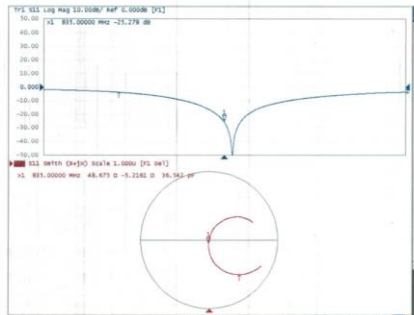TTL SPEAG CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@china.ttl.com http://www.china.ttl.com	
Impedance Measurement Plot for Head TSL			
			
Certificate No: Z22-60104 Page 6 of 6			


1.5 D900V2 - SN 1d079

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION CNAS 1079	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Client: SGS-CN		Certificate No: Z22-60184	
CALIBRATION CERTIFICATE			
Object	D900V2 - SN: 1d079		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	June 7, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (S). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±1)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7464	28-Jan-22 (SPEAG No.EK3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.Z22X00409)	Jan-23
Network Analyzer E5071C	MY49110673	14-Jan-22 (CTTL No.Z22X00409)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: June 13, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60184		Page 1 of 6	

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION CNAS 1079	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	900 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.97 nholm
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 nholm ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.70 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.5 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.73 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60184		Page 3 of 6	

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION CNAS 1079	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Glossary: TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx,y,z N/A: not applicable or not measured			
Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" c) DASY4/5 System Handbook			
Additional Documentation: c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60184		Page 2 of 6	

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION CNAS 1079	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.10 - 8.49jΩ		
Return Loss	-23.3 dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.312 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60184		Page 4 of 6	

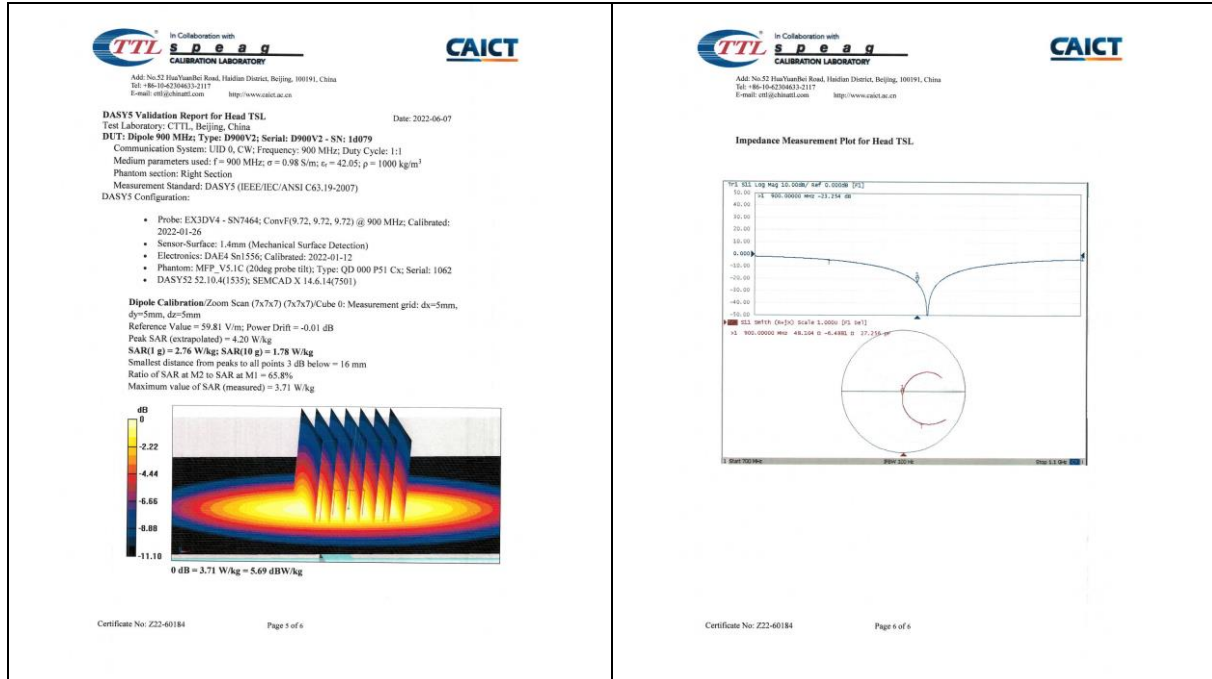

1.6 D1800V2 - SN 2d170

TTL In Collaboration with **CAICT**
Calibration Laboratory

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117 Fax: +86-10-42306033-2117
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Lin Hao** SAR Test Engineer
Approved by: **Qi Diqian** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

TTL In Collaboration with **CAICT**
Calibration Laboratory

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2079 Fax: +86-10-42306033-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"


Additional Documentation:
c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6

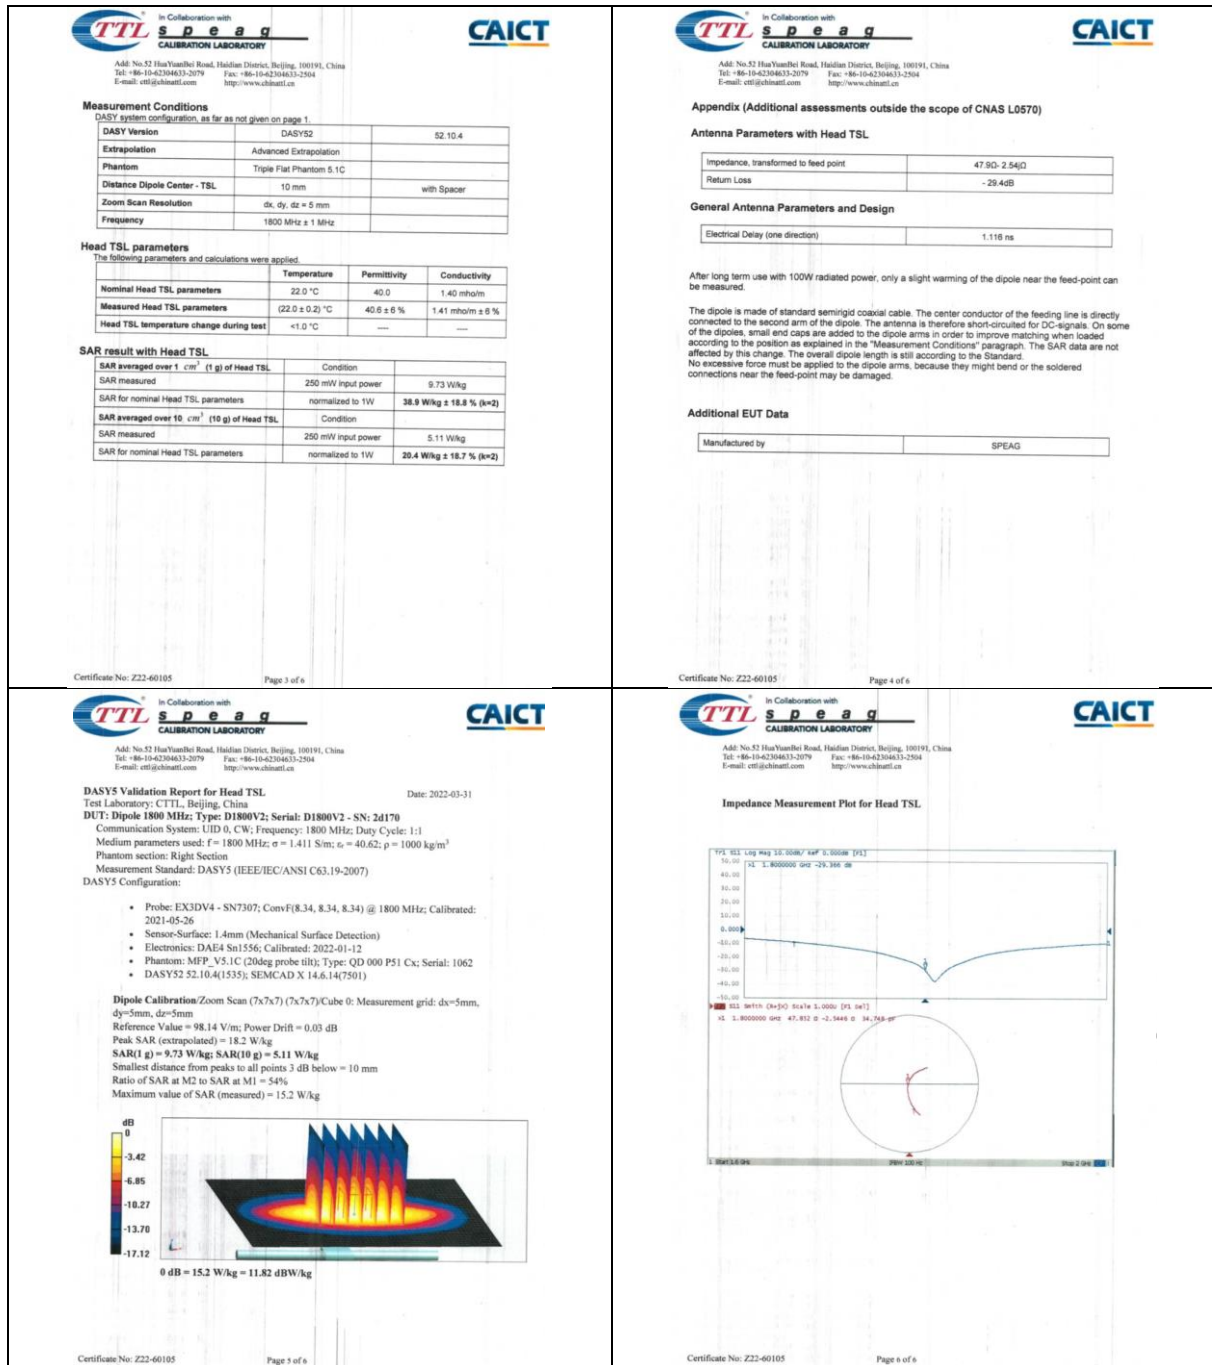

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	47.90-2.54j Ω
Return Loss	-29.4dB

General Antenna Parameters and Design



Electrical Delay (one direction)	1.116 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

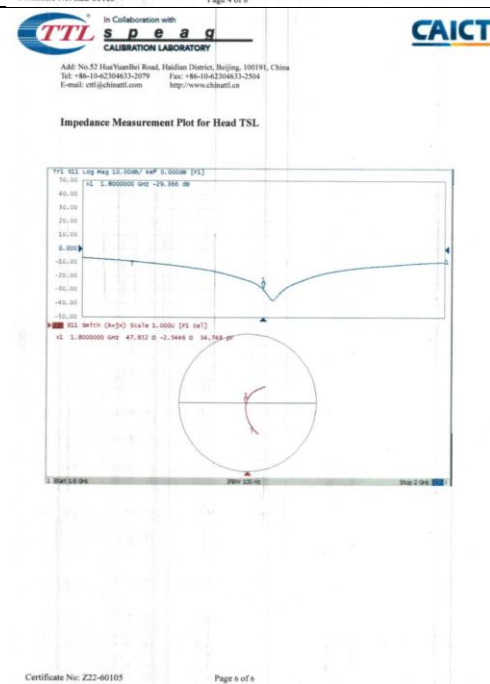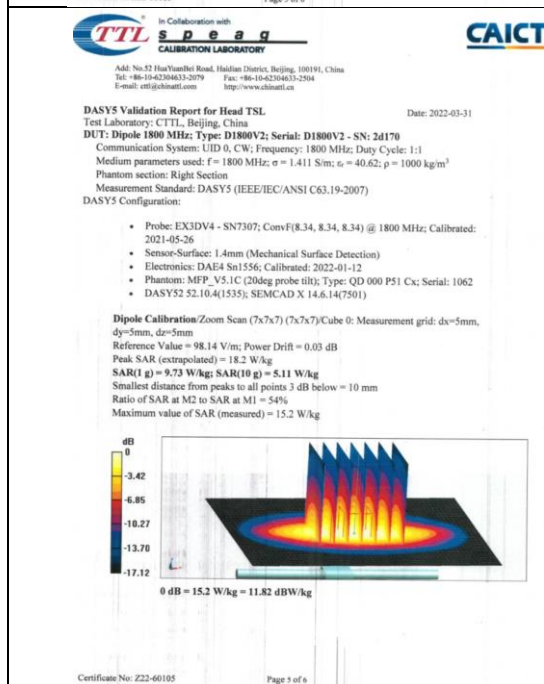


1.7 D1900V2 - SN 5d136

TTL S p e a g		CAICT	
In Collaboration with CALIBRATION LABORATORY		中国认可 国家认证 CALIBRATION CNAS	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com	
Client: SGS-CN		Certificate No: Z22-60185	
CALIBRATION CERTIFICATE			
Object	D1900V2 - SN: 5d136		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	June 7, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±1)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP6S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EXSDV4	SN 7464	28-Jan-22 (SPEAG No EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyser E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00409)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: June 13, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60185		Page 1 of 6	


TTL S p e a g		CAICT	
In Collaboration with CALIBRATION LABORATORY		中国认可 国家认证 CALIBRATION CNAS	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com	
Glossary:		TSL: tissue simulating liquid CorrF: sensitivity in TSL / NORMx.y.z N/A: not applicable or not measured	
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865984, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60185		Page 2 of 6	

TTL S p e a g		CAICT	
In Collaboration with CALIBRATION LABORATORY		中国认可 国家认证 CALIBRATION CNAS	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com	
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	1900 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	32.0 °C	40.0	1.40 mS/m
Measured Head TSL parameters	(22.0 ± 0.3) °C	39.9 ± 6 %	1.39 mS/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	9.65 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 16.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.18 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60185		Page 3 of 6	

TTL S p e a g		CAICT	
In Collaboration with CALIBRATION LABORATORY		中国认可 国家认证 CALIBRATION CNAS	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	51.02 ± 7.58Ω		
Return Loss	-22.4dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.109 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60185		Page 4 of 6	

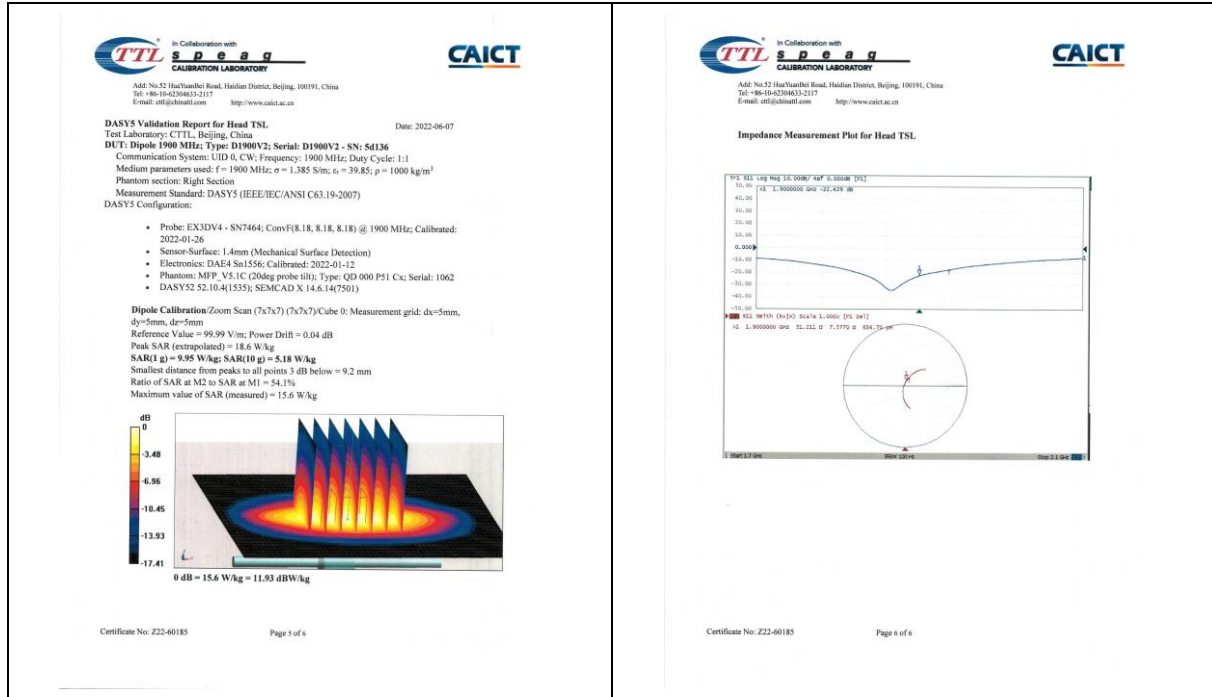

1.8 D2000V2 - SN 1041

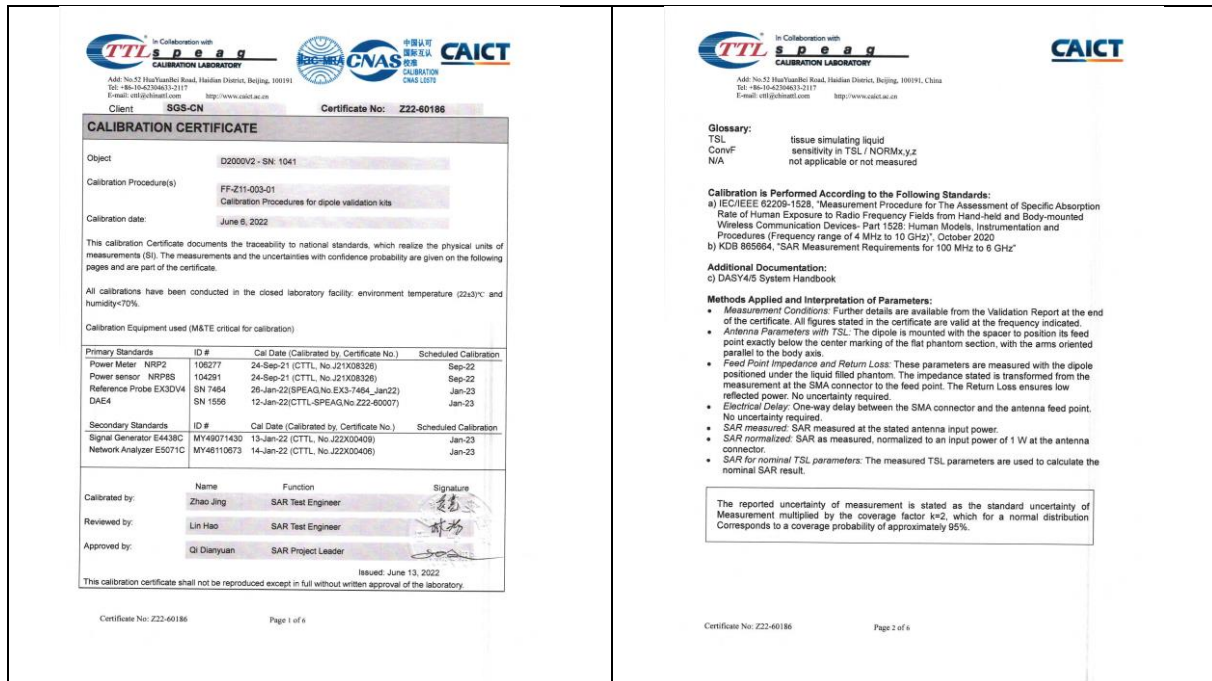

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62306633-2117
E-mail: ott@china.ttl.com http://www.caict.ac.cn

CAICT

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY52	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2000 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.4 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 16.8 % (k=2)
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	5.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 16.7 % (k=2)

Certificate No: Z22-60186

Page 3 of 6

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62306633-2117
E-mail: ott@china.ttl.com http://www.caict.ac.cn

CAICT

Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	48.4Ω ± 0.74Ω
Return Loss	-34.9dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.088 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: Z22-60186

Page 4 of 6

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62306633-2117
E-mail: ott@china.ttl.com http://www.caict.ac.cn

CAICT

DASY5 Validation Report for Head TSL

Test Laboratory: CTTL, Beijing, China

Date: 2022-06-06

DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041

Communication System: UTD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1

Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε_r = 40.21; ρ = 1000 kg/m³

Phantom section: Right Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY5 Configuration:

- Probe: EX3DV4 - SN7464; ConvF(8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26
- Sensor Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA64 Sn1556; Calibrated: 2022-01-12
- Phantom: MPP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062
- DASY52: 52.10.4(1555); SEMCAD X 14.6.14(7501)

Dipole Calibration/Zoom Scan (7x7x7) (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 103.4 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 19.6 W/kg

SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg

Smallest distance from peaks to all points 3 dB below = 9.1 mm

Ratio of SAR at M2 to SAR at M1 = 53.6%

Maximum value of SAR (measured) = 16.3 W/kg

Certificate No: Z22-60186

Page 5 of 6

In Collaboration with
TTL **s p e a g**
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62306633-2117
E-mail: ott@china.ttl.com http://www.caict.ac.cn

CAICT


Impedance Measurement Plot for Head TSL

Certificate No: Z22-60186

Page 6 of 6

1.9 D2300V2 - SN 1096

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Client	SGS-CN	Certificate No.	Z22-60106
CALIBRATION CERTIFICATE			
Object	D2300V2 - SN: 1096		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Diqiyuan	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60106		Page 1 of 6	
TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Measurement Conditions			
DASY system configuration, as far as not given on page 1:			
DASY Version	DASY32	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2300 MHz ± 1 MHz		
Head TSL parameters			
The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	12.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.88 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60106		Page 3 of 6	
TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Certificate No: Z22-60106		Page 2 of 6	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NCRMx,y,z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)"; October 2020			
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. - Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. - Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. - Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. - SAR measured: SAR measured at the stated antenna input power. - SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. - SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60106		Page 2 of 6	
TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.20-4.56jΩ		
Return Loss	-26.6dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.083 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for OC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60106		Page 4 of 6	

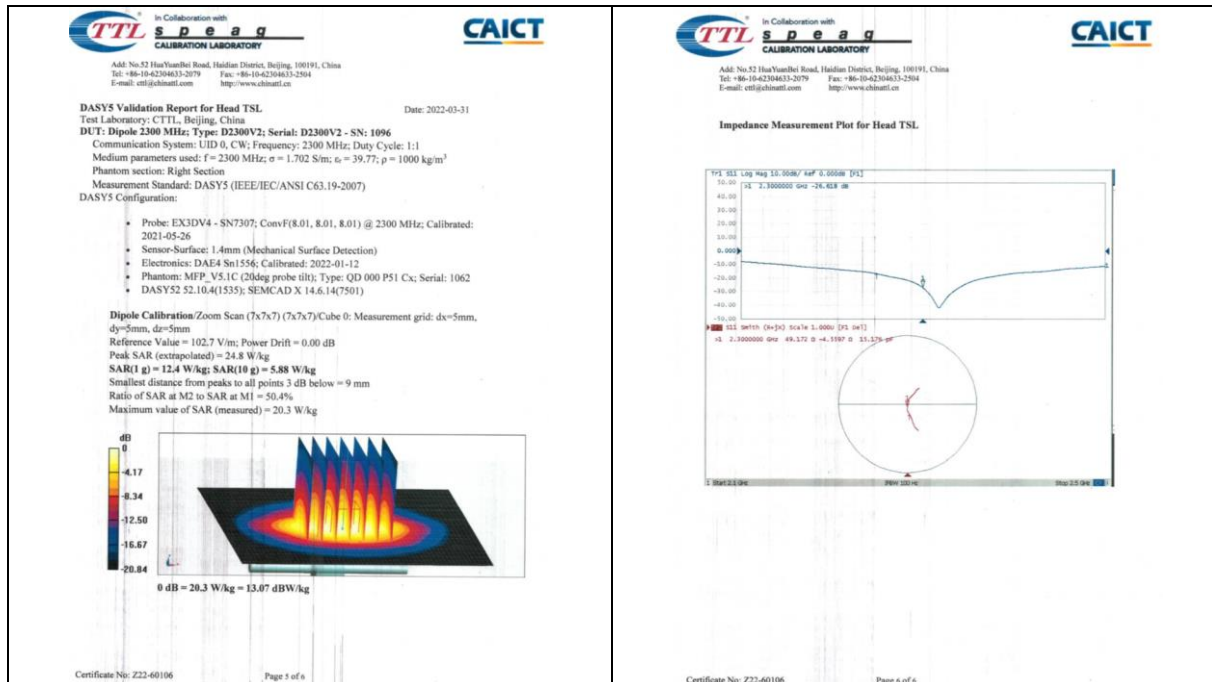

1.10 D2450V2 - SN 817

TTL In Collaboration with **CAICT**
SPEAG
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60107**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN: 817**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **April 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor: NRP8S	104291	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe EX3DV4	SN 7307	25-May-21(SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by, Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Lin Hao** SAR Test Engineer
Approved by: **Qi Danyuan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 6

TTL In Collaboration with **CAICT**
SPEAG
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"


Additional Documentation:
c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 6

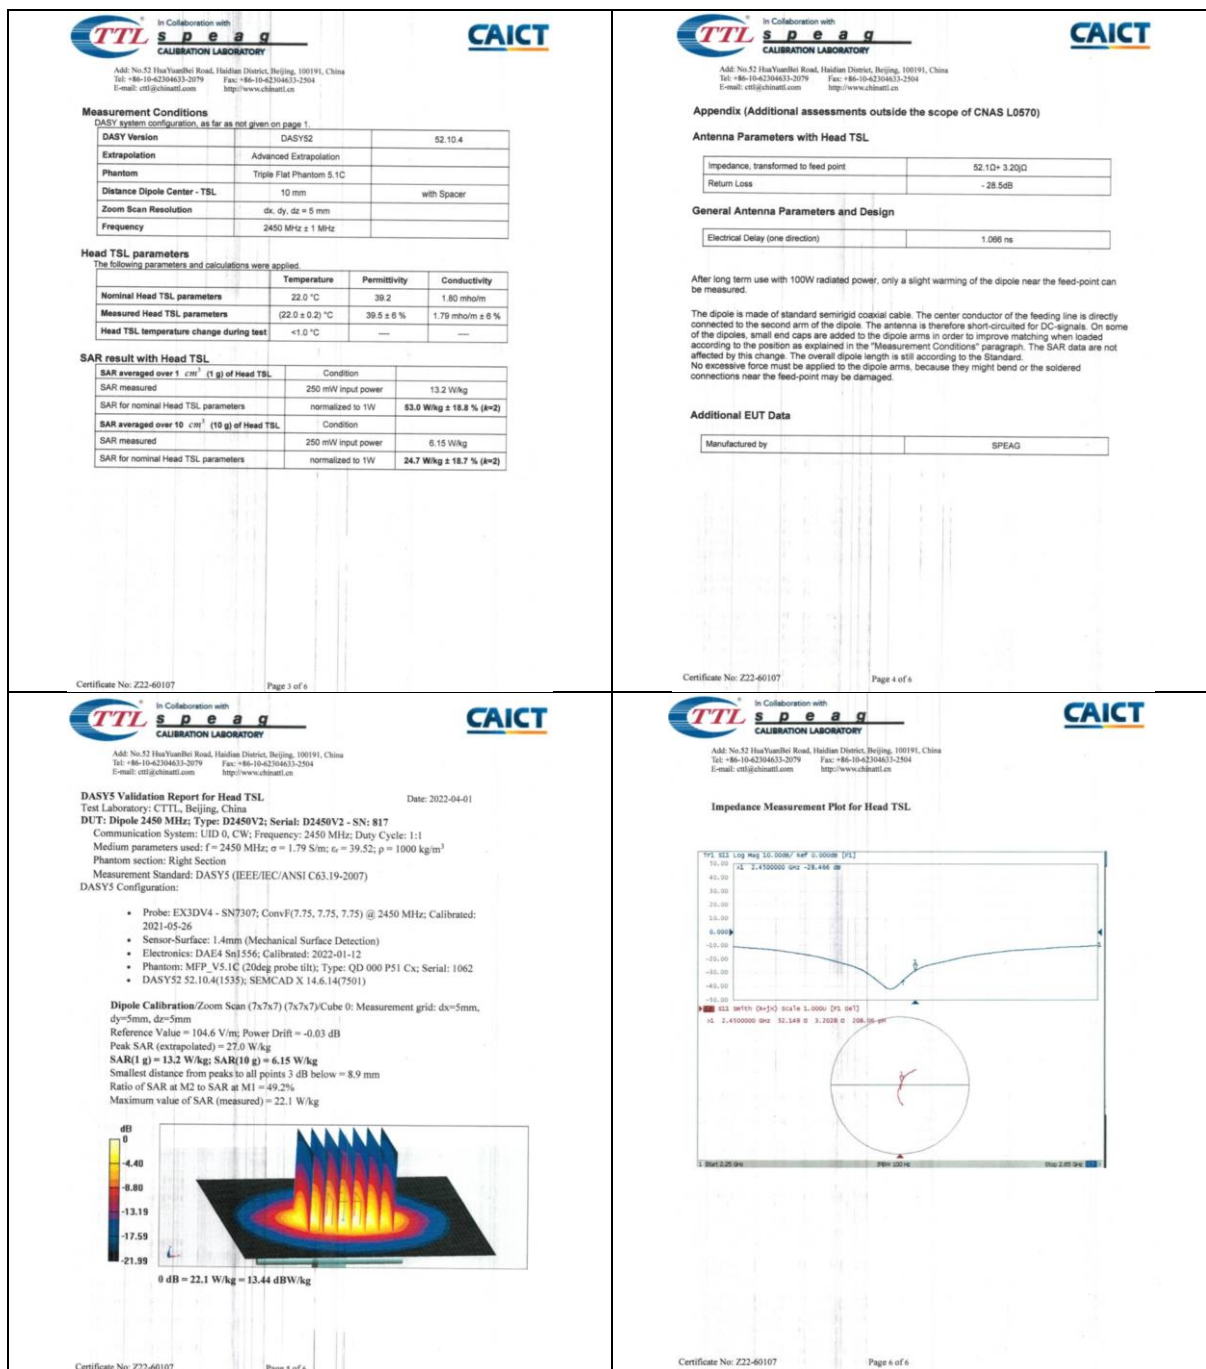


1.11 D2600V2 - SN 1158

TTL Speaq Calibration Laboratory		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinafl.com.cn http://www.chinafl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafl.com.cn http://www.chinafl.cn	
Client: SGS-CN		Certificate No: Z22-60108	
CALIBRATION CERTIFICATE			
Object	D2600V2 - SN: 1158		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1158	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: [Signature]
Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: [Signature]
Approved by:	Name: Qi Dianyan	Function: SAR Project Leader	Signature: [Signature]
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60108		Page 1 of 6	

TTL Speaq Calibration Laboratory		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafl.com.cn http://www.chinafl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafl.com.cn http://www.chinafl.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2600 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.7 ± 6 %	1.96 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	13.7 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	6.12 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg ± 18.7 % (k=2)	

TTL Speaq Calibration Laboratory		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafl.com.cn http://www.chinafl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafl.com.cn http://www.chinafl.cn	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/S System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			

TTL Speaq Calibration Laboratory		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafl.com.cn http://www.chinafl.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafl.com.cn http://www.chinafl.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.90-6.49jΩ		
Return Loss	-23.8dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.053 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		

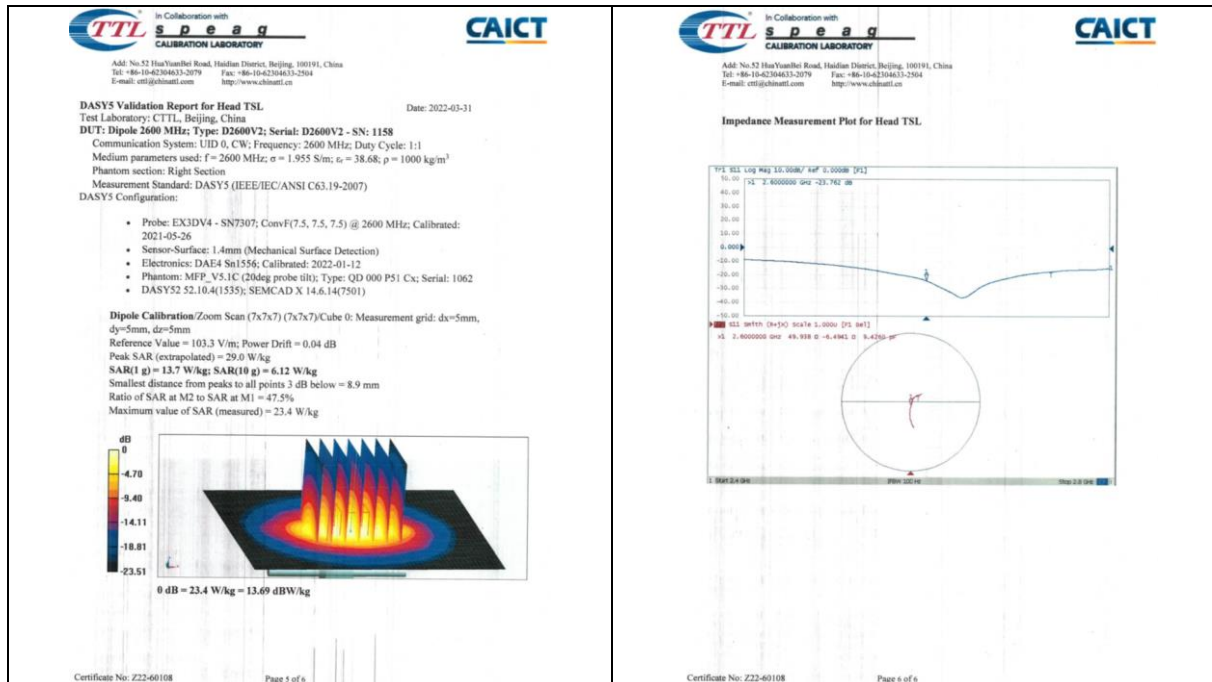

1.12 D5GHZV2 - SN 1095

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Client: SGS-CN Certificate No: Z22-60187

CALIBRATION CERTIFICATE

Object: D5GHZV2 - SN: 1095

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 1, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464, Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyan SAR Project Leader

Issued: June 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60187 Page 1 of 10

TTL Speaq
CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Glossary:

TSL: Issue simulating liquid

CompF: sensitivity in TSL / NORMx,y,z

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60187 Page 2 of 10

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY2	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz $\pm$ 1 MHz 5200 MHz $\pm$ 1 MHz 5500 MHz $\pm$ 1 MHz 5800 MHz $\pm$ 1 MHz	

Head TSL parameters at 5200MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	35.4 $\pm$ 6 %	4.62 mho/m $\pm$ 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5200MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	250 mW input power	7.79 W/kg
SAR measured	100 mW input power	7.79 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.6 W/kg $\pm$ 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.22 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg $\pm$ 24.2 % (k=2)

Head TSL parameters at 5300MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	35.2 $\pm$ 6 %	4.73 mho/m $\pm$ 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5300MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	100 mW input power	7.94 W/kg
SAR measured	100 mW input power	7.94 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg $\pm$ 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg $\pm$ 24.2 % (k=2)

Head TSL parameters at 5500MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.8	4.96 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	34.8 $\pm$ 6 %	4.94 mho/m $\pm$ 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5500MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	100 mW input power	6.29 W/kg
SAR measured	100 mW input power	6.29 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	62.6 W/kg $\pm$ 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg $\pm$ 24.2 % (k=2)

Head TSL parameters at 5600MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	34.7 $\pm$ 6 %	5.05 mho/m $\pm$ 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5600MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	100 mW input power	8.12 W/kg
SAR measured	100 mW input power	8.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg $\pm$ 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg $\pm$ 24.2 % (k=2)

Head TSL parameters at 5800MHz

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	34.4 $\pm$ 6 %	5.25 mho/m $\pm$ 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5800MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	100 mW input power	7.71 W/kg
SAR measured	100 mW input power	7.71 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg $\pm$ 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.16 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.6 W/kg $\pm$ 24.2 % (k=2)

Appendix (Additional assessments outside the scope of CNAS L0570)**Antenna Parameters with Head TSL at 5200MHz**

Impedance, transformed to feed point	48.1D-5.03jΩ
Return Loss	-23.6dB

Antenna Parameters with Head TSL at 5300MHz

Impedance, transformed to feed point	47.8D-2.42jΩ
Return Loss	-28.5dB

Antenna Parameters with Head TSL at 5500MHz



Impedance, transformed to feed point	50.3D-4.26jΩ
Return Loss	-27.4dB

Antenna Parameters with Head TSL at 5600MHz

Impedance, transformed to feed point	54.5D-4.80jΩ
Return Loss	-24.0dB

Antenna Parameters with Head TSL at 5800MHz

Impedance, transformed to feed point	51.5D-5.61jΩ
Return Loss	-24.9dB

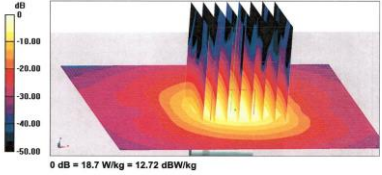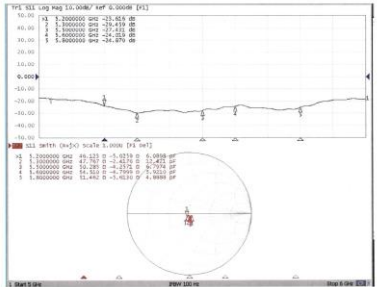In Collaboration with TTL s p e a q CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@chinaetl.com http://www.caict.ac.cn CAICT General Antenna Parameters and Design <table border="1"><tr><td>Electrical Delay (one direction)</td><td>1.101 ns</td></tr></table> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data <table border="1"><tr><td>Manufactured by</td><td>SPEAG</td></tr></table> Certificate No: Z22-60187 Page 7 of 10	Electrical Delay (one direction)	1.101 ns	Manufactured by	SPEAG	In Collaboration with TTL s p e a q CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@chinaetl.com http://www.caict.ac.cn CAICT DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China Date: 2022-06-01 DUT: Dipole 5Ghz; Type: D5GhzV2; Serial: D5GhzV2 - SN: 1095 Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: f = 5200 MHz; $\sigma = 4.62$ S/m; $\epsilon_r = 35.39$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5300 MHz; $\sigma = 4.73$ S/m; $\epsilon_r = 35.19$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5500 MHz; $\sigma = 4.939$ S/m; $\epsilon_r = 34.83$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5600 MHz; $\sigma = 5.051$ S/m; $\epsilon_r = 34.69$; $\rho = 1000$ kg/m³ Medium parameters used: f = 5800 MHz; $\sigma = 5.247$ S/m; $\epsilon_r = 34.42$; $\rho = 1000$ kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA64 Sn1556; Calibrated: 2022-01-12 - Phantom: MPF_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 18.3 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg Certificate No: Z22-60187 Page 8 of 10
Electrical Delay (one direction)	1.101 ns				
Manufactured by	SPEAG				
In Collaboration with TTL s p e a q CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@chinaetl.com http://www.caict.ac.cn CAICT Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.28 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.2 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg  Certificate No: Z22-60187 Page 9 of 10	In Collaboration with TTL s p e a q CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@chinaetl.com http://www.caict.ac.cn CAICT Impedance Measurement Plot for Head TSL  Certificate No: Z22-60187 Page 10 of 10				

2 DAE4 - SN 1245

Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 www.speag.ch, info@speag.ch s p e a g IMPORTANT NOTICE USAGE OF THE DAE4 The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points: Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE to wear out. Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an anti-static bag. This anti-static bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside. E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and get accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements. Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect. DASY Configuration Files: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MΩ is given in the corresponding configuration file. Important Note: Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer. Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure. Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body over the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE. TH_EH190306AE DAE4.docx 07.03.2019	Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Client: SGS Kunshan City, China Certificate No.: DAE4-1245_Apr23 CALIBRATION CERTIFICATE Object: DAE4 - SD 000 D04 BM - SN: 1245 Calibration procedure(s): QA CAL-06.v30 Calibration procedure for the data acquisition electronics (DAE) Calibration date: April 25, 2023 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22 $\pm$ 3)°C and humidity < 70%. Calibration Equipment used (MATE critical for calibration) <table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Kathrein Multimeter Type 2001</td><td>SN: 0810278</td><td>29-Aug-22 (No. 34389)</td><td>Aug-23</td></tr></tbody></table> <table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Check Date (in house)</th><th>Scheduled Check</th></tr></thead><tbody><tr><td>Auto DAE Calibration Unit</td><td>SE UMS 002 AA 1001</td><td>27-Jan-23 (in house check)</td><td>In house check: Jan-24</td></tr><tr><td>Calibrator flow 12.1</td><td>SE UMS 006 AA 1002</td><td>27-Jan-23 (in house check)</td><td>In house check: Jan-24</td></tr></tbody></table> Calibrated by: Dominique Sutter (Name), Laboratory Technician (Function), <i>[Signature]</i> (Signature) Approved by: Sven Kuhn (Name), Technical Manager (Function), <i>[Signature]</i> (Signature) This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued April 25, 2023 Certificate No.: DAE4-1245_Apr23 Page 1 of 5	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Kathrein Multimeter Type 2001	SN: 0810278	29-Aug-22 (No. 34389)	Aug-23	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Auto DAE Calibration Unit	SE UMS 002 AA 1001	27-Jan-23 (in house check)	In house check: Jan-24	Calibrator flow 12.1	SE UMS 006 AA 1002	27-Jan-23 (in house check)	In house check: Jan-24
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																		
Kathrein Multimeter Type 2001	SN: 0810278	29-Aug-22 (No. 34389)	Aug-23																		
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																		
Auto DAE Calibration Unit	SE UMS 002 AA 1001	27-Jan-23 (in house check)	In house check: Jan-24																		
Calibrator flow 12.1	SE UMS 006 AA 1002	27-Jan-23 (in house check)	In house check: Jan-24																		
Calibration Laboratory of Schmid & Partner Engineering AG Zugstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108 Glossary DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system. Methods Applied and Interpretation of Parameters • DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. • Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. • The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty. • DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. • Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. • Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage. • AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage. • Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. • Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance. • Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement. • Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. • Power consumption: Typical value for information. Supply currents in various operating modes. Certificate No.: DAE4-1245_Apr23 Page 2 of 5	DC Voltage Measurement AD - Converter Resolution nominal: 5.1 μV High Range: 1LSB = 6.1 μV, full range = -100...+300 mV Low Range: 1LSB = 61 nV, full range = -1...+30 mV DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec <table border="1"><thead><tr><th>Calibration Factors</th><th>X</th><th>Y</th><th>Z</th></tr></thead><tbody><tr><td>High Range</td><td>405.243 $\pm$ 0.02% (k=2)</td><td>403.938 $\pm$ 0.02% (k=2)</td><td>405.064 $\pm$ 0.02% (k=2)</td></tr><tr><td>Low Range</td><td>3.99474 $\pm$ 1.50% (k=2)</td><td>3.99478 $\pm$ 1.50% (k=2)</td><td>4.00994 $\pm$ 1.50% (k=2)</td></tr></tbody></table> Connector Angle <table border="1"><thead><tr><th>Connector Angle to be used in DASY system</th><th></th></tr></thead><tbody><tr><td></td><td>32.0° $\pm$ 1°</td></tr></tbody></table> Certificate No.: DAE4-1245_Apr23 Page 3 of 5	Calibration Factors	X	Y	Z	High Range	405.243 $\pm$ 0.02% (k=2)	403.938 $\pm$ 0.02% (k=2)	405.064 $\pm$ 0.02% (k=2)	Low Range	3.99474 $\pm$ 1.50% (k=2)	3.99478 $\pm$ 1.50% (k=2)	4.00994 $\pm$ 1.50% (k=2)	Connector Angle to be used in DASY system			32.0° $\pm$ 1°				
Calibration Factors	X	Y	Z																		
High Range	405.243 $\pm$ 0.02% (k=2)	403.938 $\pm$ 0.02% (k=2)	405.064 $\pm$ 0.02% (k=2)																		
Low Range	3.99474 $\pm$ 1.50% (k=2)	3.99478 $\pm$ 1.50% (k=2)	4.00994 $\pm$ 1.50% (k=2)																		
Connector Angle to be used in DASY system																					
	32.0° $\pm$ 1°																				

Appendix (Additional assessments outside the scope of SCS0108)

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	19998.60	2.90	0.00
Channel X - Input	20005.77	2.75	0.01
Channel Y + Input	19999.65	2.19	-0.01
Channel Y - Input	19999.60	1.08	0.00
Channel Z + Input	20003.12	0.26	0.00
Channel Z - Input	-20000.51	0.53	-0.00
Channel X + Input	19999.62	-1.05	-0.00
Channel Z + Input	20002.17	-0.70	-0.00
Channel Z - Input	-20001.94	-0.91	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2002.91	0.81	0.04
Channel X - Input	203.06	0.73	0.36
Channel Y + Input	-195.56	0.88	-0.45
Channel Y - Input	2002.33	0.29	0.01
Channel Z + Input	201.91	-0.39	-0.19
Channel Z - Input	-196.22	-0.79	0.40
Channel X + Input	2002.20	0.24	0.01
Channel Z + Input	201.28	-0.68	-0.44
Channel Z - Input	-196.93	-1.36	0.69

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X		
200	-6.42	-8.27
-200	8.81	8.00
Channel Y		
200	7.04	7.13
-200	-14.70	-15.29
Channel Z		
200	4.52	-5.35
-200	3.90	3.52

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200		
Channel Y	200	9.08	-3.29
Channel Z	200	10.03	7.20

Certificate No: DAE4-1245_Apr23

Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16001	16100
Channel Y	16079	16951
Channel Z	16040	15991

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	0.77	-0.83	1.89	0.49
Channel Y	-0.24	-1.72	1.19	0.52
Channel Z	-0.85	-2.62	0.99	0.61

6. Input Offset Current

Nominal input circuitry offset current on all channels: <25pA

7. Input Resistance (Typical values for information)

	Zeroing (MΩ)	Measuring (MΩ)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DAE4-1245_Apr23

Page 5 of 5

3 EX3DV4 - SN 3801

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zugstrasse 43, 8004 Zurich, SwitzerlandSchweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

Auden

Taoyuan City

Certificate No.

EX-3801_Jun23

CALIBRATION CERTIFICATE

Object

EX3DV4 - SN3801

Calibration procedure(s)

QA CAL-01.v10, QA CAL-12.v10, QA CAL-14.v7, QA CAL-23.v6,
QA CAL-25.v6
Calibration procedure for dosimetric E-field probes

Calibration date

June 23, 2023

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.
All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3) °C and humidity < 70%.
Calibration Equipment used (MATE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP-201	SR 104778	30-Mar-23 (No. 217-03804/03895)	Mar-24
Power sensor NRP-201	SR 102844	30-Mar-23 (No. 217-03804)	Mar-24
DCP GAK-3.5 (range 1mV)	SR 1246	20-Oct-22 (DCP GAK-3.5 L48, Oct22)	Oct-23
DCP GAK-12	SR 1016	20-Oct-22 (DCP GAK-12 1916, Oct22)	Oct-23
Reference 30 dB Attenuator	SR 025555 (20)	30-Mar-23 (No. 217-03805)	Mar-24
DAE4	SR 860	16-Mar-23 (No. SAE4-860, Mar23)	Mar-24
Reference Probe ESE272	SR 3013	06-Jun-23 (No. ESE-3013, Jun23)	Jun-24

Secondary Standards	ID	Check Date (In House)	Scheduled Check
Power meter E4419B	SR 084793874	06-Apr-19 (in house check Jun-22)	In house check Jun-24
Power sensor E4419A	SR MVA148887	06-Apr-19 (in house check Jun-22)	In house check Jun-24
Power sensor E4419A	SR 50011019	06-Apr-19 (in house check Jun-22)	In house check Jun-24
RF generator HP 8640C	SR U3540101700	04-Aug-19 (in house check Jun-22)	In house check Jun-24
Network Analyzer B8568A	SR U3041060677	31-Mar-19 (in house check Oct-22)	In house check Oct-24

Name

Jeton Kaestli

Function

Laboratory Technician

Signature

Approved by

Sven Kühn

Technical Manager

Signature

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX-3801_Jun23

Page 1 of 22

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zugstrasse 43, 8004 Zurich, SwitzerlandSchweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Glossary

TSL: Issue simulating liquid
NORMA_{x,y,z}: sensitivity in free space
Conf#: sensitivity in TSL - NORMA_{x,y,z}
DCP: diode compression point
CF: crest factor (1 duty cycle) of the RF signal
A, B, C, D: modulation dependent linearization parameters
Polarization ψ : ψ notation around probe axis
Polarization θ : θ notation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\theta = 0$ is normal to probe axis
Connector Angle: information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
b) K2B 805664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMA_{x,y,z}: Assessed for E-field polarization $\theta = 0$ ($\theta = 90^\circ$ MHz in TEM-cell; $f > 100$ MHz; R22 waveguide); NORMA_{x,y,z} are only intermediate values, i.e., the uncertainties of NORMA_{x,y,z} does not affect the E-field uncertainty inside TSL (see below Conf#).
- NORMA_{x,y,z} - NORMA_{x,y,z} - frequency response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of Conf#.
- DCP_{x,y,z}: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.
- RFR: RFR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.
- A, B, C, D: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- Conf# and Boundary Effect Parameter: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f > 300$ MHz) and made waveguide using analytical field distributions based on power measurements for $f > 300$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha), depth of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMA_{x,y,z} - Conf# whereby the uncertainty corresponds to that given for Conf#. A frequency dependent Conf# is used in DASY version 4.4 and higher which allows extending the validity from <50 MHz to >100 MHz.
- Spherical Isotropy (3D deviation from isotropy): In a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMA (no uncertainty required).

Certificate No: EX-3801_Jun23

Page 2 of 22

EX3DV4 - SN3801

June 23, 2023

Parameters of Probe: EX3DV4 - SN3801

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k = 2)
Norm ($\mu V/V/m^2$) ^A	0.51	0.58	0.42	±10.1%
DCP (mV) ^B	162.0	101.5	104.0	±4.7%

Calibration Results for Modulation Response

UID	Communication System Name	A dB	B dB $\sqrt{V/V}$	C	D dB	VR mV	Max dev.	Max Unc ^C k = 2
0	CW	X 0.00 Y 0.00 Z 0.00	0.00 0.00 0.00	1.00 1.00 1.00	0.00 188.1 188.8	188.1 188.1 188.8	±3.3%	±4.7%
10352	Pulse Waveform (200Hz, 19%)	X 20.00 Y 20.00 Z 20.00	91.23 96.19 95.56	20.86 20.56 20.56	10.00 80.0 80.0	10.00 80.0 80.0	±3.5%	±9.6%
10353	Pulse Waveform (200Hz, 29%)	X 20.00 Y 20.00 Z 20.00	91.18 88.83 91.24	19.59 19.38 19.37	6.69 80.0 80.0	80.0 80.0 80.0	±1.8%	±9.6%
10354	Pulse Waveform (200Hz, 40%)	X 20.00 Y 20.00 Z 20.00	92.89 98.29 91.43	19.05 18.48 18.43	3.88 95.0 95.0	95.0 95.0 95.0	±1.1%	±9.6%
10355	Pulse Waveform (200Hz, 65%)	X 20.00 Y 20.00 Z 20.00	91.14 91.15 91.15	16.83 17.67 17.67	2.22 120.0 120.0	120.0 120.0 120.0	±1.0%	±9.6%
10387	QPSK Waveform, 1 MHz	X 1.48 Y 1.88 Z 1.43	65.05 65.16 63.76	13.76 14.18 13.25	1.00 150.0 150.0	150.0 150.0 150.0	±3.1%	±9.6%
10388	QPSK Waveform, 10 MHz	X 2.81 Y 2.11 Z 1.88	66.70 67.04 65.47	14.69 14.97 14.01	0.09 130.0 150.0	130.0 150.0 150.0	±1.0%	±9.6%
10396	64-QAM Waveform, 100 MHz	X 2.53 Y 3.08 Z 3.02	67.49 70.24 70.72	17.24 16.85 16.59	3.01 150.0 150.0	150.0 150.0 150.0	±0.7%	±9.6%
10398	64-QAM Waveform, 40 MHz	X 3.38 Y 3.45 Z 3.38	66.66 66.78 65.89	15.32 15.44 14.88	0.00 150.0 150.0	150.0 150.0 150.0	±0.6%	±9.6%
10414	WLAN COOF, 64-QAM, 40 MHz	X 4.78 Y 4.85 Z 4.67	66.60 65.58 64.97	15.38 15.41 14.98	0.00 150.0 150.0	150.0 150.0 150.0	±4.8%	±9.6%

Note: For details on UID parameters see Appendix

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the E_{Field} uncertainty result TSL (see Page 5 and 6).^B Limitation parameter uncertainty for maximum specified test strength.^C Uncertainty is determined using the max. deviation from linear regression applying rectangular distribution and is expressed for the square of the field value.

Certificate No: EX-3801_Aun23

Page 3 of 22

EX3DV4 - SN3801

June 23, 2023

Parameters of Probe: EX3DV4 - SN3801

Sensor Model Parameters

	C1 dB	C2 dB	a V ⁻¹	T1 mV/V ²	T2 mV/V ²	T3 mV/V ²	T4 mV/V ²	T5 mV/V ²	T6 mV/V ²
x	41.4	310.28	35.39	15.41	6.54	5.19	0.06	0.47	1.01
y	46.4	347.34	35.39	26.16	8.21	5.10	0.72	0.49	1.01
z	42.7	333.62	34.88	17.55	9.54	5.07	1.53	0.54	1.01

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle	153.7°
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	237 mm
Probe Body Diameter	16 mm
Tip Length	9 mm
Tip Diameter	1 mm
Probe Tip to Sensor X Calibration Point	2.5 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.

Certificate No: EX-3801_Aun23

Page 4 of 22

EX3DV4 - SN3801

June 23, 2023

Parameters of Probe: EX3DV4 - SN3801

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^A	Relative Permittivity ^B	Conductivity ^B (S/m)	Const# X	Const# Y	Const# Z	Alpha ^B	Depth ^B (mm)	Unc (k = 2)
150	52.3	0.76	11.02	11.02	11.02	0.00	1.00	±13.3%
450	42.5	0.27	10.11	10.11	10.11	0.16	1.30	±13.3%
750	41.5	0.09	9.49	9.49	9.49	0.40	0.85	±12.0%
855	41.5	0.90	9.17	9.17	9.17	0.40	0.80	±12.0%
800	41.5	0.97	9.08	9.08	9.08	0.42	0.89	±12.0%
1450	40.5	1.20	8.32	8.32	8.32	0.36	0.80	±12.0%
1750	40.1	1.37	8.22	8.22	8.22	0.18	0.86	±12.0%
1900	40.0	1.40	7.93	7.93	7.93	0.27	0.86	±12.0%
2100	39.8	1.49	7.87	7.87	7.87	0.31	0.86	±12.0%
2300	39.8	1.67	7.62	7.62	7.62	0.30	0.90	±12.0%
2450	39.2	1.80	7.38	7.38	7.38	0.30	0.90	±12.0%
2600	39.0	1.96	7.16	7.16	7.16	0.32	0.90	±12.0%
3300	38.2	2.71	6.52	6.52	6.52	0.30	1.30	±14.0%
3500	37.9	2.81	6.46	6.46	6.46	0.35	1.30	±14.0%
3700	37.7	3.12	6.40	6.40	6.40	0.35	1.30	±14.0%
3900	37.5	3.32	6.33	6.33	6.33	0.40	1.80	±14.0%
4100	37.3	3.53	5.98	5.98	5.98	0.40	1.80	±14.0%
4200	37.1	3.63	5.95	5.95	5.95	0.40	1.80	±14.0%
4400	36.9	3.84	5.74	5.74	5.74	0.40	1.75	±14.0%
4600	36.7	4.04	5.73	5.73	5.73	0.40	1.75	±14.0%
4800	36.4	4.25	5.72	5.72	5.72	0.40	1.80	±14.0%
4950	36.3	4.40	5.38	5.38	5.38	0.40	1.80	±14.0%
5250	35.9	4.71	5.19	5.19	5.19	0.40	1.80	±14.0%
5600	35.5	5.07	4.60	4.60	4.60	0.40	1.80	±14.0%
5750	35.4	5.22	4.89	4.89	4.89	0.40	1.80	±14.0%

^A Frequency validity above 300 MHz or ±100 MHz only applies for DASY v4.4 and higher (see Page 5), else it is restricted to ±50 MHz. The uncertainty is the RSS of the Const# uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ±1%, 2%, 4%, 8% and 10% for Const# assessments at 20, 40, 60, 100 and 200 MHz respectively. Validity of Const# assessed at 60 MHz, and Const# assessed at 130 MHz is ±5% for 50 MHz frequency validity can be extended to ±10 MHz.^B The probes are calibrated using tissue simulating liquid (TSL) that deviates for x and y by less than ±5% from the target value (typically better than ±2%) and are valid for TSL with deviations of up to ±10%. If TSL with deviations from the target of less than ±5% are used, the calibration uncertainties are ±11.1% for 0.7 - 3 GHz and ±13.1% for 3 - 6 GHz.^C Alpha/Depth are determined during calibration. DEEAD warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz and below ±2% for frequencies between 3-6 GHz at an distance larger than half the probe tip diameter from the boundary.

Certificate No: EX-3801_Aun23

Page 5 of 22

EX3DV4 - SN3801

June 23, 2023

Parameters of Probe: EX3DV4 - SN3801

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^A	Relative Permittivity ^B	Conductivity ^B (S/m)	Const# X	Const# Y	Const# Z	Alpha ^B	Depth ^B (mm)	Unc (k = 2)
6500	34.8	6.07	5.20	5.20	5.20	5.20	2.50	±18.6%


^A Frequency validity of 6.5 GHz is -4000 to 700 MHz, and ±700 MHz at or above 700 MHz. The uncertainty is the RSS of the Const# uncertainty at calibration frequency and the uncertainty for the indicated frequency band. The probes are calibrated using tissue simulating liquid (TSL) that deviates for x and y by less than ±10% from the target value (typically better than ±5%) and are valid for TSL with deviations of up to ±10%.^B Alpha/Depth are determined during calibration. DEEAD warrants that the remaining deviation due to the boundary effect after compensation is always less than ±1% for frequencies below 3 GHz, below ±2% for frequencies between 3-6 GHz, and below ±4% for frequencies between 6-10 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX-3801_Aun23

Page 6 of 22

EX3DV4 - SN3801

June 23, 2023

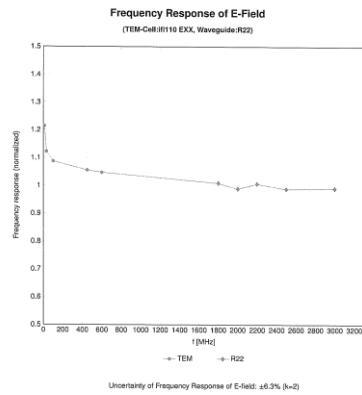


Certificate No: EX-3801_Jun23

Page 7 of 22

EX3DV4 - SN3801

June 23, 2023

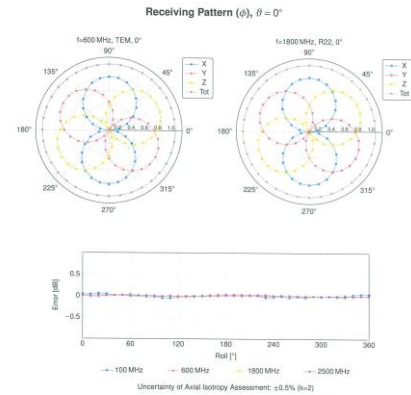


Certificate No: EX-3801_Jun23

Page 8 of 22

EX3DV4 - SN3801

June 23, 2023


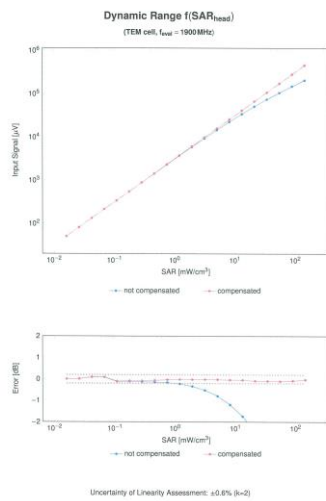


Certificate No: EX-3801_Jun23

Page 9 of 22

EX3DV4 - SN3801

June 23, 2023

Conversion Factor Assessment**Deviation from Isotropy in Liquid**Error (ϕ, θ), f = 900 MHz

Certificate No: EX-3801_Jun23

Page 10 of 22