Tech Book

We refer to the safety regulations and technical information related to Orka Two here.



Contents

1. Safety and health information ————————————————————————————————————	05
Intended use	05
Indications for use	05
Hearing health care information	05
Important safety instructions	08
Warnings	09
Cautions	10
Contraindications	10
2. Product specifications	11
Dimensions and weight	11
Compatibility	11
Performance parameters	12
Power supply specification	14
Transport and storage conditions	14
3. Regulatory and legal information	15
Compliance information	15

Classification	20
Expected service life of product and components	20
Disposals	20
Privacy policy	21
Limited warranty	21
Returns and exchanges	21
Information of symbols	22

1. Safety and health information

Intended use

The Orka Two™ hearing aids are designed for people who have perceived mild to moderate hearing loss. They are wireless air conduction hearing aids that can be customized to fit the user's needs.

Indication for use

The Orka Two™ hearing aids are meant to increase the volume of sound for people who have perceived mild to moderate hearing loss. The user can adjust the device according to their individual hearing needs without any pre-programming or hearing test. These hearing aids are designed for direct-to-consumer sale and usage, without the involvement of a hearing care professional.

Hearing health care information

WARNING: People younger than 18 should go to a doctor before using this.

People younger than 18 years old need specialized care, and using this without a medical evaluation may worsen impairment or disability. A hearing aid user who is younger than 18 should have a recent medical evaluation from a doctor, preferably an ear-nose-throat doctor (an ENT). Before using this, a doctor should determine that the use of a hearing aid is appropriate.

WARNING to Hearing Aid Dispensers:

You should advise a prospective hearing aid user to consult promptly with a doctor, preferably an ear specialist such as an ENT, before dispensing a hearing aid if you determine through inquiry, actual observation, or review of any other available information concerning the prospective user, that the prospective user has any of the following conditions:

- · Visible deformity of the ear, either congenital or traumatic
- Fluid, pus, or blood coming out of the ear within the previous 6 months
- · Pain or discomfort in the ear
- History of excessive ear wax or suspicion that something is in the ear canal
- · Dizziness, either recent or long-standing
- Sudden, quickly worsening, or fluctuating hearing loss within the previous 6 months
- Hearing loss or ringing (tinWnitus) only in one ear or a noticeable difference in hearing between ears
- Audiometric air-bone gap equal to or greater than 15 dB at 500 Hz, 1000 Hz, and 2000 Hz

WARNING to Hearing Aid Dispenser, Outputs over 132 dB SPL:

You should exercise special care in selecting and fitting a hearing aid with a maximum output that exceeds 132 dB SPL because it may impair the remaining hearing of the hearing aid user.

Caution: This is not hearing protection.

You should remove this device if you experience overly loud sounds, whether short or long-lasting. If you're in a loud place, you should use the right kind of hearing protection instead of wearing this device. In general, if you would use ear plugs in a loud place, you should remove this device and use ear plugs.

Caution: The sound output should not be uncomfortable or painful.

You should turn down the volume or remove the device if the sound output is uncomfortably loud or painful. If you consistently need to turn the volume down, you may need to further adjust your device.

Caution: You might need medical help if a piece gets stuck in your ear.

If any part of your hearing aid, like the eartip, gets stuck in your ear, and you can't easily remove it with your fingers, get medical help as soon as you can. You should not try to use tweezers or cotton swabs because they can push the part farther into your ear, injuring your eardrum or ear canal, possibly seriously.

Note: What you might expect when you start using a hearing aid

A hearing aid can benefit many people with hearing loss. However, you should know it will not restore normal hearing, and you may still have some difficulty hearing over noise. Further, a hearing aid will not prevent or improve a medical condition that causes hearing loss. People who start using hearing aids sometimes need a few weeks to get used to them. Similarly, many people find that training or counseling can help them get more out of their devices. If you have hearing loss in both ears, you might get more out of using hearing aids in both, especially in situations that make you tired from listening-for example, noisy environments.

Note: Tell FDA about injuries, malfunctions, or other adverse events.

To report a problem involving your hearing aid, you should submit information to FDA as soon as possible after the problem. FDA calls them "adverse events," and they might include: skin irritation in your ear, injury from the device (like cuts or scratches, or burns from an overheated battery), pieces of the device getting stuck in your ear, suddenly worsening hearing loss from using the device, etc. Instructions for reporting are available at https://www.fda.gov/Safety/MedWatch, or call 1-800-FDA-1088. You can also download a form to mail to FDA.

Note: Hearing loss in people younger than 18

- People younger than 18 should see a doctor first, preferably an earnose-throat doctor (an ENT), because they may have different needs than adults.
- The doctor will identify and treat medical conditions as appropriate.
- The doctor may refer the person to an audiologist for a separate test, a hearing aid evaluation.
- The hearing aid evaluation will help the audiologist select and fit the appropriate hearing aid.

A person who is younger than 18 years old with hearing loss should have a medical evaluation by a doctor, preferably an ENT, before buying a hearing aid. The purpose of a medical evaluation is to identify and treat medical conditions that may affect hearing but that a hearing aid won't treat on its own.

Following the medical evaluation and if appropriate, the doctor will provide a written statement that the hearing loss has been medically evaluated and the person is a candidate for a hearing aid. The doctor may refer the person to an audiologist for a hearing aid evaluation, which is different from the medical evaluation and is intended to identify the appropriate hearing aid.

The audiologist will conduct a hearing aid evaluation to assess the person's ability to hear with and without a hearing aid. This will enable the audiologist to select and fit a hearing aid for the person's individual needs. An audiologist can also provide evaluation and rehabilitation since, for people younger than 18, hearing loss may cause problems in language development and educational and social growth. An audiologist is qualified by training and experience to assist in the evaluation and rehabilitation of hearing loss in people younger than 18.

Important safety instructions

- If you have acute otitis externa, tympanitis, chronic suppurative otitis media (in the phase of purulent infection), or acute suppurative otitis media, please avoid using the product.
- When you first start using the product, you may experience minor itchiness, redness, or irritation as your ear gets used to having an object in it. If you experience any discomfort or related issues, please contact Orka for assistance.
- Use only the attachments/components that are specified by the manufacturer. There are no internal
 parts of the product that users can repair.
- The battery that comes with the product may cause a chemical burn if it is mishandled.
- Dispose of electronic waste according to local regulations.
- Do NOT modify the product without authorization.
- Use the hearing aids only with the supplied eartips attached.

- The product contains magnetic material, so if you have an implantable medical device, consult your
 physician to determine if it may be affected by this product.
- **Do not use the hearing aids if any part of the device is damaged.** Contact Orka immediately if you experience any unusual situations.
- If you have any active implants, keep the hearing aids away from them.
- Unauthorized alterations to the hearing aids should not be made. The Orka Two devices contain rechargeable batteries that cannot be replaced.
- · Only use accessories provided by Orka.

▲ WARNINGS

- Keep the device and its components out of reach of children, as they contain small parts that may pose a choking hazard.
- Do NOT use the hearing aids in explosive or oxygen-enriched atmospheres, as this may cause a fire or explosion.
- Check before using the hearing aids in areas where electronics or wireless devices are restricted, as this may cause interference.
- The hearing aids are intended for use by a single user, and reselling or sharing them with others is not recommended. This may lead to infection.
- Keep the product away from fire and excessive heat (e.g., from storage in direct sunlight, near candles, or in a hot car) to avoid burns or damage to product.
- Do NOT submerge in water, wear in the shower, or wear while participating in water sports, e.g., swimming, waterskiing, surfing, etc. Prolonged exposure to water may damage the hearing aids.

CAUTIONS

- Be aware that some sounds may sound different when using the hearing aids, so keep this in mind when you need to be aware of your surroundings. You should adjust to this over time.
- When adjusting the volume, turn it up gradually until you reach a comfortable listening level.
- Do NOT use the hearing aids or their components if any part of them is damaged, if they emit loud unusual noise, if you experience a warming sensation, or if you experience a loss of audio. If any of these happen, remove the hearing aids immediately, power them off, and contact the Orka Team for assistance.
- The product contains non-removable rechargeable lithium batteries that can be carried as checked baggage.
- Follow the power supply specifications (refer to page 14) when charging the hearing aids. Charging should only occur when the hearing aids are placed in the charging case, otherwise the product may be damaged.
- If the battery leaks, do not allow the liquid to come in contact with the skin or eyes, and seek medical advice if contact is made.
- For protection, the product will turn off when placed in an electrostatic discharge environment and will resume operation when placed in the charging case and switched back on.

Contraindications

- Patients with acute otitis externa, tympanitis, chronic suppurative otitis media (during the period of infection with discharge), and acute suppurative otitis media should not use the product.
- · Patients who are allergic to the material of the product should not use it.

2. Product specifications


Dimensions and weight

Dimensions	Hearing aid (without receiver wire)	13.6mm*9mm*28.9mm	
Charging case		82mm*56mm*31.5mm	
Woight	Hearing aid (Single)	3.4g	
Weight	Charging case	75g	

Compatibility

Device compatibility	iOS 14 and later, Android 7 and later	
Bluetooth	4.2/5.0/5.1/5.2/5.3	

Performance parameters

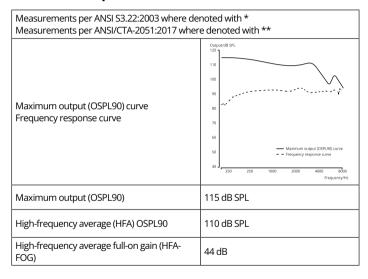

Reference test gain	33 dB	
Frequency range	< 200 – 8000 Hz	
Harmonic distortion	≤ 3% max	
Equivalent input noise	≤ 23 dB SPL max	
Input-output curve	Output/d8 SPL 110 90 80	
Latency**	10.2ms	
Attack time* at 250Hz/500Hz/1000Hz/2000Hz/4000Hz (ms)	10/30/30/10/90	
Release time* at 250Hz/500Hz/1000Hz/2000Hz/4000Hz (ms)	200/330/380/280/100	

Power supply specification

Power adapter input voltage	100-240V 50/60Hz 0.2A	
Nominal input	5V d.c. 50mA (Hearing Aid) 5V d.c. 470mA (Charging Case)	
USB cable specifications	USB 2.0 Type-C	
Wireless Charging	1W	

Transport and storage conditions

	Temperature range	Humidity range	Atmospheric pressure
Transport conditions	5°C – 40°C	5 – 93% RH	860hPa - 1060hPa
Storage	-20°C – 55°C	5 – 93% RH	860hPa - 1060hPa

3. Regulatory and legal information

Compliance information

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Changes or modifications not directly approved by Orka may void the user's authority to operate this equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions:

- (1) This device may not cause harmful interference, and
- (2) This device must accept any interference received, including interference that may cause undesired operation.

This device complies with FCC radiation exposure limits set forth for general population. This transmitter must not be co-located or operating in conjunction with any other antenna or transmitter.

Hearing aids FCC ID: 2BBZIH020S; Charging case FCC ID: 2BBZIC020S

This equipment has been tested and found to comply with the limits per CISPR 11 class B.

Guidance and manufacturer's declaration-electromagnetic emissions

The hearing aid is intended for use in the electromagnetic environment specified below. Users must ensure the hearing aid is used in such a specified electromagnetic environment.

Emission test	lec 60601 test level	l •	Electromagnetic environment guidance
RF emis- sions CISPR 11	Group 1	Group 1	The hearing aid uses RF energy only for its internal function. Therefore, its RF emissions are very low and is not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	Class B	The hearing aid is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.

Guidance and manufacturer's declaration-electromagnetic immunity

The hearing aid is intended for use in the electromagnetic environment specified below. The user of the hearing aid should assure that it is used in such an environment.

Immuni- ty test	Standard	lec 60601 test level	Compliance level
Electro- static discharge (ESD)	IEC 61000-4- 2	+/- 8 kV contact +/- 15 kV air	+/- 8 kV contact +/- 15 kV air
Radiated RF EM Fields	IEC 61000-4-	10 V/m 80 MHz – 2.7 GHz 80% AM at 1 kHz	10 V/m 80 MHz – 2.7 GHz 80% AM at 1 kHz

Immunity test	Standard	lec 60601 test level	Compliance level
Proximity fields from RF wireless commu- nications equipent	IEC 61000-4-3	9 V/m; 710, 745, 780 MHz; Pulse modulation 217 Hz 9 V/m; 5240, 5500, 5785 MHz; Pulse modulation 217 Hz 27 V/m; 385 MHz; Pulse modulation 18 Hz 28 V/m; 450 MHz FM +/- 5 kHz devia- tion; 1 kHz sine 28 V/m; 810, 870, 930 MHz; Pulse modulation 18 Hz 28 V/m; 1720, 1845, 1970, 2450 MHz; Pulse modu- lation 217 Hz	9 V/m; 710, 745, 780 MHz; Pulse modulation 217 Hz 9 V/m; 5240, 5500, 5785 MHz; Pulse modulation 217 Hz 27 V/m; 385 MHz; Pulse modulation 18 Hz 28 V/m; 450 MHz FM +/- 5 kHz deviation; 450 MHz FM +/- 5 kHz deviation; 1 kHz sine 28 V/m; 810, 870, 930 MHz; Pulse modulation 18 Hz 28 V/m; 1720, 1845, 1970, 2450 MHz; Pulse modulation 217 Hz

Classification

The hearing aids are classified as a Type B Applied Part, IEC 60601-2-66

Expected service life of product and components

3 Years

Disposals

The Orka Two™ hearing aids and components are electronic components which should be discarded in accordance with national, regional, and local regulations.

The Orka Two™ hearing aids comply with the following regulations for medical devices:

IEC 60601-1:2005 IEC 60601-1-2:2014 IEC 60601-2-66:2019 ANSI/ASA S3.22-2014 FCC 47 Part 15.247

Privacy policy

The Orka Privacy Policy is available at: www.hiorka.com

Orka, Orka Two, and the Orka Health app icon are trademarks of Orka Health Co., Ltd.

©2023 Orka Health Co., Ltd. No part of this work may be reproduced, modified, distributed, or otherwise used without prior written permission.

Limited warranty

The hearing aids are covered by a limited warranty. Visit our website at: www.hiorka.com for details of the limited warranty.


Returns and exchanges

Satisfaction is guaranteed on all Orka products purchased by consumers directly from Orka. We want you to be thrilled, so if you're not satisfied with your purchase for any reason, simply return it within the trial period for a full refund. Please see the Orka Support page at: www.hiorka.com for details.

Information of symbols

\triangle	General warning sign	<u></u>	Manufacturer
†	Type B applied part		Fragile, handle with care
*	Keep dry	\mathbb{A}	Date of manufacture
SN	Serial number		Power supply with double isolation
93%	Humidity range	7	Rechargeable battery
1060hPa	Pressure range	③	Follow instructions for use or follow electronic instructions for use.
5°C 40°C	Temperature range	(i	Consult instructions for use or consult electronic instructions for use

®	Do not use if package is damaged and consult instructions for use.
Z	"Not for general waste". When a product is to be discarded, it must be sent to a designated collection point for recycling and recovery to prevent from harming the environment or human health due to the hazardous substances contained.
Æ	This symbol confers that the electromagnetic interference from the device is under limits approved by the US Federal Communications Commission.



After-sales service provided by:

ORKA HEALTH CO., LTD. ROOM 01B101,BUILDING 2, NO. 118 RONGKE ROAD, SHANGHAI, 201203, CHINA

Period of use:

3 years

Information in this brochure is subject to change without notice.

©2023 ORKA HEALTH CO., LTD. All rights reserved.

Website: www.hiorka.com Tel: (800) 653-6022 Email: support@hiorka.com