

Appendix C for KSCR230900158901

Calibration Certificate

Object	Apply	No	Model	SN	Calibration Date	Due date of calibration
Dipole	☒	1	CLA150	4025	2021/04/26	2024/04/25
	☐	2	D450V3	1103	2021/04/21	2024/04/20
	☐	3	D750V3	1188	2022/03/29	2025/03/28
	☐	4	D835V2	4d114	2022/03/31	2025/03/30
	☐	5	D900V2	1d079	2022/06/07	2025/06/06
	☐	6	D1800V2	2d170	2022/03/31	2025/03/30
	☐	7	D1900V2	5d136	2022/06/07	2025/06/06
	☐	8	D2000V2	1041	2022/06/06	2025/06/05
	☐	9	D2300V2	1096	2022/03/31	2025/03/30
	☐	10	D2450V2	817	2022/04/01	2025/03/31
	☐	11	D2600V2	1158	2022/03/31	2025/03/30
	☐	12	D5GHzV2	1095	2022/06/01	2025/05/31
DAE	☒	13	DAE4	1245	2023/04/25	2024/04/24
Probe	☒	14	EX3DV4	7767	2022/10/28	2023/10/27

1 Dipole

1.1 CLA150 - SN 4025

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service		Accreditation No.: SCS 0108	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108		The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates	
Client: SGS-CN (Auden)		Certificate No: CLA150-4025_Apr21			
CALIBRATION CERTIFICATE					
Object: CLA150 - SN: 4025					
Calibration procedure(s): QA CAL-15.v9 Calibration Procedure for SAR Validation Sources below 700 MHz					
Calibration date: April 26, 2021					
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.					
All calibrations have been conducted in the closed laboratory facility: environment temperature $22 \pm 3^\circ\text{C}$ and humidity $< 70\%$.					
Calibration Equipment used (M&TE critical for calibration)					
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration		
Power meter NRP	SN: 10476	09-Apr-21 (No. 217-03201/03202)	Apr-22		
Power sensor NRP Z91	SN: 103344	09-Apr-21 (No. 217-03201)	Apr-22		
Power sensor NRP Z91	SN: 103345	09-Apr-21 (No. 217-03202)	Apr-22		
Reference 20 dB Attenuator	SN: C22562 (200)	09-Apr-21 (No. 217-03343)	Apr-22		
Type-N mismatch combination	SN: 310952 / 00357	09-Apr-21 (No. 217-03344)	Apr-22		
Reference Probe EX30N4	SN: 3877	30-Dec-20 (No. C3X3077_Dec20)	Dec-21		
ENEA4	SN: 684	26-Jan-20 (No. D454-654_Jan20)	Jun-21		
Secondary Standards	ID #	Check Date (in house)	Scheduled Check		
Power meter S44135	SN: G841203074	06-Apr-15 (in house check Jun-20)	In house check Jun-22		
Power sensor E4413A	SN: MY4149067	06-Apr-15 (in house check Jun-20)	In house check Jun-22		
Power sensor E4413A	SN: 000100210	06-Apr-15 (in house check Jun-20)	In house check Jun-22		
RF generator HP 8594D	SN: U504001070	04-Aug-09 (in house check Jun-20)	In house check Jun-22		
Network Analyser Agilent E8363A	SN: U541000477	31-Mar-14 (in house check Oct-20)	In house check Oct-21		
Calibrated by:	Name: Jeffrey Katzman	Function: Laboratory Technician	Signature:		
Approved by:	Name: Kaja Polovic	Function: Technical Manager	Signature:		
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.					
Issued: April 26, 2021					
Certificate No: CLA150-4025_Apr21					
Page 1 of 6					

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service		Accreditation No.: SCS 0108	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108		The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates	
Client: SGS-CN (Auden)		Certificate No: CLA150-4025_Apr21			
Glossary:					
TSL		tissue simulating liquid			
ConvF		sensitivity in TSL / NORM x,y,z			
N/A		not applicable or not measured			
Calibration is Performed According to the Following Standards:					
a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Technique", June 2013					
b) IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016					
c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010					
d) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"					
Additional Documentation:					
e) DASY4/5 System Handbook					
Methods Applied and Interpretation of Parameters:					
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.					
• Antenna Parameters with TSL: The source is mounted in a touch configuration below the center marking of the flat phantom.					
• Return Loss: This parameter is measured with the source positioned under the liquid filled phantom (as described in the measurement condition clause). The Return Loss ensures low reflected power. No uncertainty required.					
• SAR measured: SAR measured at the stated antenna input power.					
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.					
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.					
The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.					
Certificate No: CLA150-4025_Apr21					
Page 2 of 6					

Measurement Conditions		
DASY system configuration, as far as not given on page 1.		
DASY Version	DASY5	V52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELIA Flat Phantom	Shell thickness: 2 ± 0.2 mm
EUT Positioning	Touch Position	
Zoom Scan Resolution	$dx, dy = 4.0$ mm, $dz = 1.4$ mm	Graded Ratio = 1.4 (Z direction)
Frequency	150 MHz $\pm$ 1 MHz	

Head TSL parameters			
The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0°C	52.3	0.75 mho/m
Measured Head TSL parameters	$(22.0 \pm 0.2)^\circ\text{C}$	$51.1 \pm 6\%$	0.75 mho/m $\pm 6\%$
Head TSL temperature change during test	$< 0.5^\circ\text{C}$	---	---

SAR result with Head TSL		
SAR averaged over 1 cm^3 (1 g) of Head TSL	Condition	
SAR measured	1 W input power	3.90 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	$3.88\text{ W/kg} \pm 19.4\%$ (k=2)
SAR averaged over 10 cm^3 (10 g) of Head TSL	condition	
SAR measured	1 W input power	2.60 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	$2.59\text{ W/kg} \pm 18.0\%$ (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)	
Antenna Parameters with Head TSL	
Impedance, transformed to feed point	$47.9\Omega \pm 1.5\Omega$
Return Loss	-31.4 dB
Additional EUT Data	
Manufactured by	SPEAG

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service		Accreditation No.: SCS 0108	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108		The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates	
Client: SGS-CN (Auden)		Certificate No: CLA150-4025_Apr21			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.					
Issued: April 26, 2021					
Certificate No: CLA150-4025_Apr21					
Page 3 of 6					

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland		S Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service		Accreditation No.: SCS 0108	
Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates		Accreditation No.: SCS 0108		The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates	
Client: SGS-CN (Auden)		Certificate No: CLA150-4025_Apr21			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.					
Issued: April 26, 2021					
Certificate No: CLA150-4025_Apr21					
Page 4 of 6					

DASY5 Validation Report for Head TSL

Date: 26.04.2021

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: CLA150; Type: CLA150; Serial: CLA150 - SN: 4025

Communication System: UID 0 - CW; Frequency: 150 MHz
Medium parameters used: $f = 150$ MHz; $\sigma = 0.76$ S/m; $\epsilon_0 = 51.1$; $\rho = 1000$ kg/m³
Phantom section: Flat Section
Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(12.51, 12.51, 12.51) @ 150 MHz; Calibrated: 30.12.2020
- Sensor Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DA84 SN654; Calibrated: 26.06.2020
- Phantom: ELI v4.0; Type: QDOVA001BB; Serial: TP.1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

CLA Calibration for HSL-LF Tissue/CLA150, touch configuration, Pin=1W/Zoom Scan,

dist=1.4mm (8x10x8)/Cube 0; Measurement grid: dx=4mm, dy=4mm, dz=1.4mm

Reference Value = 85.93 W/m; Power Drift = -0.02 dB


Peak SAR (extrapolated) = 7.36 W/kg

SAR(1 g) = 3.90 W/kg; SAR(10 g) = 2.60 W/kg

Smallest distance from peaks to all points 3 dB below: Larger than measurement grid (> 30mm)


Ratio of SAR at M2 to SAR at M1 = 80.4%

Maximum value of SAR (measured) = 5.48 W/kg

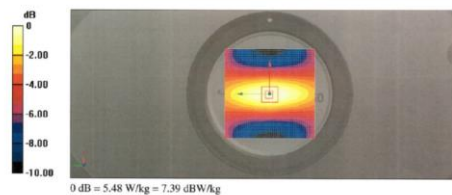

Certificate No: CLA150-4025_Apr21

Page 5 of 6

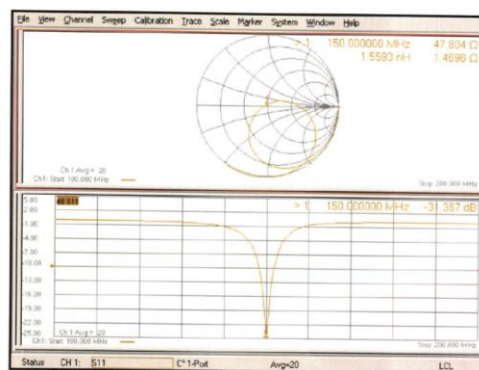

Certificate No: CLA150-4025_Apr21

Page 6 of 6

1.2 D450V3 - SN 1103

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio italiano di taratura
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client: SGS-CN (Aude)

Certificate No: D450V3-1103_Apr21

CALIBRATION CERTIFICATE

Object	D450V3 - SN: 1103		
Calibration procedure(s)	QA CAL-15_v9 Calibration Procedure for SAR Validation Sources below 700 MHz		
Calibration date:	April 21, 2021		
This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (20 ± 2) °C and humidity < 70%.			
Calibration Equipment used (MPE critical for calibration)			
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	09-Apr-21 (No. 217-03021/03020)	Apr-22
Power sensor NRP-291	SN: 103244	09-Apr-21 (No. 217-03021)	Apr-22
Power sensor NRP-291	SN: 103245	09-Apr-21 (No. 217-03020)	Apr-22
Reference 20 dB Attenuator	SN: CC2852 (200)	09-Apr-21 (No. 217-03345)	Apr-22
Type-N mismatch combination	SN: 310852 / 06327	09-Apr-21 (No. 217-03344)	Apr-22
Reference Probe E3030A	SN: 3877	30-Dec-20 (No. E30-3877_Dec20)	Dec-21
DAEA	SN: 654	26-Jun-20 (No. D454-654_Jun20)	Jun-21
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB41200274	06-Apr-16 (in house check Jun-20)	In house check Jun-22
Power sensor E4412A	SN: MY41496027	06-Apr-16 (in house check Jun-20)	In house check Jun-22
Power sensor E4412A	SN: 00018010	06-Apr-16 (in house check Jun-20)	In house check Jun-22
RF generator HP 8548C	SN: U503460101700	06-Aug-09 (in house check Jun-20)	In house check Jun-22
Network Analyzer Agilent E8358A	SN: U841980477	31-Mar-14 (in house check Oct-20)	In house check Oct-21
Calibrated by:	Name: Claudio Leiber	Function: Laboratory Technician	Signature: [Signature]
Approved by:	Name: Kello Polovic	Function: Technical Manager	Signature: [Signature]
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Issued: April 23, 2021			

Certificate No: D450V3-1103_Apr21

Page 1 of 6

Calibration Laboratory of
Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland



S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
S Servizio italiano di taratura
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL: Issue simulating liquid
ConvF: sensitivity in TSL / NORM x,y,z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEC 61010-1:2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D450V3-1103_Apr21

Page 2 of 6

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V62.10.4
Extrapolation	Advanced Extrapolation	
Phantom	ELJ4 Flat Phantom	Shell thickness: 2 ± 0.2 mm
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	$dx, dy, dz \leq 5$ mm	
Frequency	450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied:

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	43.5	0.57 mho/m
Measured Head TSL parameters	(22.0 $\pm$ 0.2) °C	43.1 $\pm$ 6 %	0.07 mho/m $\pm$ 8 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	1.14 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	4.58 W/kg $\pm$ 18.1 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	0.757 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	3.06 W/kg $\pm$ 17.6 % (k=2)

Certificate No: D450V3-1103_Apr21

Page 3 of 6

DASY5 Validation Report for Head TSL

Test Laboratory: SPEAG, Zurich, Switzerland

Date: 21.04.2021

DUT: Dipole 450 MHz; Type: D450V3; Serial: D450V3 - SN:1103

Communication System: UID 0 - CW; Frequency: 450 MHz

Medium parameters used: $f = 450 \text{ MHz}$; $\alpha = 0.87 \text{ S/m}$; $\epsilon_r = 43.1$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN3877; ConvF(10.64, 10.64, 10.64) @ 450 MHz; Calibrated: 30.12.2020
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn654; Calibrated: 26.06.2020
- Phantom: ELJ v4.0; Type: QDOVA001BB; Serial: TP:1003
- DASY52 52.10.4(1527); SEMCAD X 14.6.14(7483)

Dipole Calibration for Head Tissue/d=15mm, Pin=250mW/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 39.18 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 1.76 W/kg

SAR(1 g) = 1.14 W/kg; SAR(10 g) = 0.767 W/kg

Smallest distance from peaks to all points 3 dB below: Larger than measurement grid

Ratio of SAR at M2 to SAR at M1 = 64.9%

Maximum value of SAR (measured) = 1.53 W/kg

Certificate No: D450V3-1103_Apr21

Page 5 of 6

Appendix (Additional assessments outside the scope of SCS 0106)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	57.1 $\Omega - 2.8 j\Omega$
Return Loss	-23.0 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.346 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

Certificate No: D450V3-1103_Apr21

Page 4 of 6

Certificate No: D450V3-1103_Apr21

Page 6 of 6


1.3 D750V3 - SN 1188

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		中国认可 国家承认 校准 CAICT CNAS L0570	
Client	SGS-CN	Certificate No.	Z22-60103
CALIBRATION CERTIFICATE			
Object	D750V3 - SN: 1188		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 28, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	104277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP88	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX30V4	SN 7307	26-May-21(SPEAG.No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG.No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator S4436C	MY48671430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00409)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: April 3, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60103	Page 1 of 6		


TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		中国认可 国家承认 校准 CAICT CNAS L0570	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY52	VS2.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	750 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	42.0	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.4 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.07 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	8.27 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.37 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	5.48 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60103	Page 3 of 6		


TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		中国认可 国家承认 校准 CAICT CNAS L0570	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60103	Page 2 of 6		

TTL Speag CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaetl.com http://www.chinaetl.cn		中国认可 国家承认 校准 CAICT CNAS L0570	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	53.60-1.13jΩ		
Return Loss	-28.7dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	0.947 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.			
No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60103	Page 4 of 6		

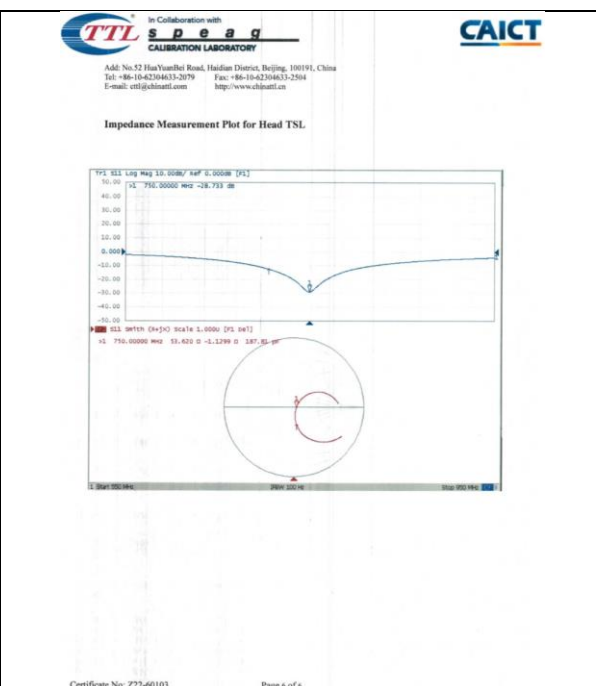

TSL CALIBRATION LABORATORY Address: No.52 JiaYuanJie Road, Haidian District, Beijing, 100191 Tel: +86-10-62504633-2312 Fax: +86-10-62504633-2504 E-mail: cti@chinaulm.com Http://www.chinaulm.com	CNAN 中国认证 认可 校准 CALIBRATION CNAS LISTED	Client SOS-CN Certificate No: Z22-60104																																
CALIBRATION CERTIFICATE																																		
Object D835V2 - SN: d4114 Calibration Procedure(s) FF-Z11-003-01 Calibration Procedures for dipole validation kits Calibration date: March 31, 2022 This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%. Calibration Equipment used (MATE critical for calibration)																																		
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="text-align: left;">Primary Standards</th> <th style="text-align: left;">ID #</th> <th style="text-align: left;">Cal Date (Calibrated by: Certificate No.)</th> <th style="text-align: left;">Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Power Meter NRP2</td> <td>100277</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Power sensor NRPBS</td> <td>104261</td> <td>24-Sep-21 (CTTL No.J21X08326)</td> <td>Sep-22</td> </tr> <tr> <td>Reference Probe EX3DV4</td> <td>SN 7307</td> <td>26-May-21 (SPEAG No.EX3-7307_May21)</td> <td>May-22</td> </tr> <tr> <td>DAE4</td> <td>SN 1556</td> <td>12-Jan-22 (CTTL-SPEAG No.Z22-60007)</td> <td>Jan-23</td> </tr> </tbody> </table> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="text-align: left;">Secondary Standards</th> <th style="text-align: left;">ID #</th> <th style="text-align: left;">Cal Date (Calibrated by: Certificate No.)</th> <th style="text-align: left;">Scheduled Calibration</th> </tr> </thead> <tbody> <tr> <td>Signal Generator E438C</td> <td>MY46071430</td> <td>13-Jan-22 (CTTL No.J22X00409)</td> <td>Jan-23</td> </tr> <tr> <td>Network Analyzer E5071C</td> <td>MY46110673</td> <td>14-Jan-22 (CTTL No.J22X00405)</td> <td>Jan-23</td> </tr> </tbody> </table>			Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration	Power Meter NRP2	100277	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Power sensor NRPBS	104261	24-Sep-21 (CTTL No.J21X08326)	Sep-22	Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22	DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23	Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration	Signal Generator E438C	MY46071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23	Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00405)	Jan-23
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration																															
Power Meter NRP2	100277	24-Sep-21 (CTTL No.J21X08326)	Sep-22																															
Power sensor NRPBS	104261	24-Sep-21 (CTTL No.J21X08326)	Sep-22																															
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22																															
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23																															
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration																															
Signal Generator E438C	MY46071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23																															
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No.J22X00405)	Jan-23																															
<table style="width: 100%;"> <tr> <td style="width: 33%;">Calibrated by:</td> <td style="width: 33%; text-align: center;"> Name Function Zhao Jing SAR Test Engineer </td> <td style="width: 33%; text-align: center;"> Signature </td> </tr> <tr> <td>Reviewed by:</td> <td style="text-align: center;"> Lin Hao SAR Test Engineer </td> <td style="text-align: center;"> </td> </tr> <tr> <td>Approved by:</td> <td style="text-align: center;"> Qi Dianyan SAR Project Leader </td> <td style="text-align: center;"> </td> </tr> </table>			Calibrated by:	Name Function Zhao Jing SAR Test Engineer	Signature	Reviewed by:	Lin Hao SAR Test Engineer		Approved by:	Qi Dianyan SAR Project Leader																								
Calibrated by:	Name Function Zhao Jing SAR Test Engineer	Signature																																
Reviewed by:	Lin Hao SAR Test Engineer																																	
Approved by:	Qi Dianyan SAR Project Leader																																	
Issued: April 6, 2022 This calibration certificate shall not be reproduced except in full without written approval of the laboratory.																																		

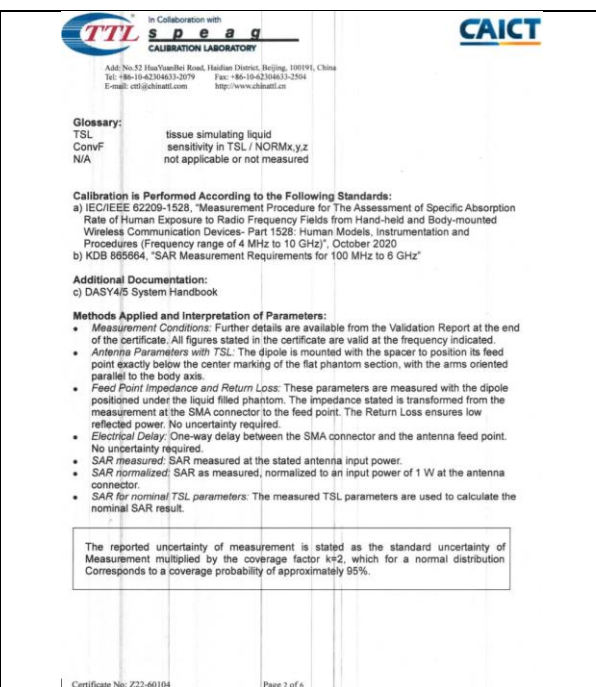

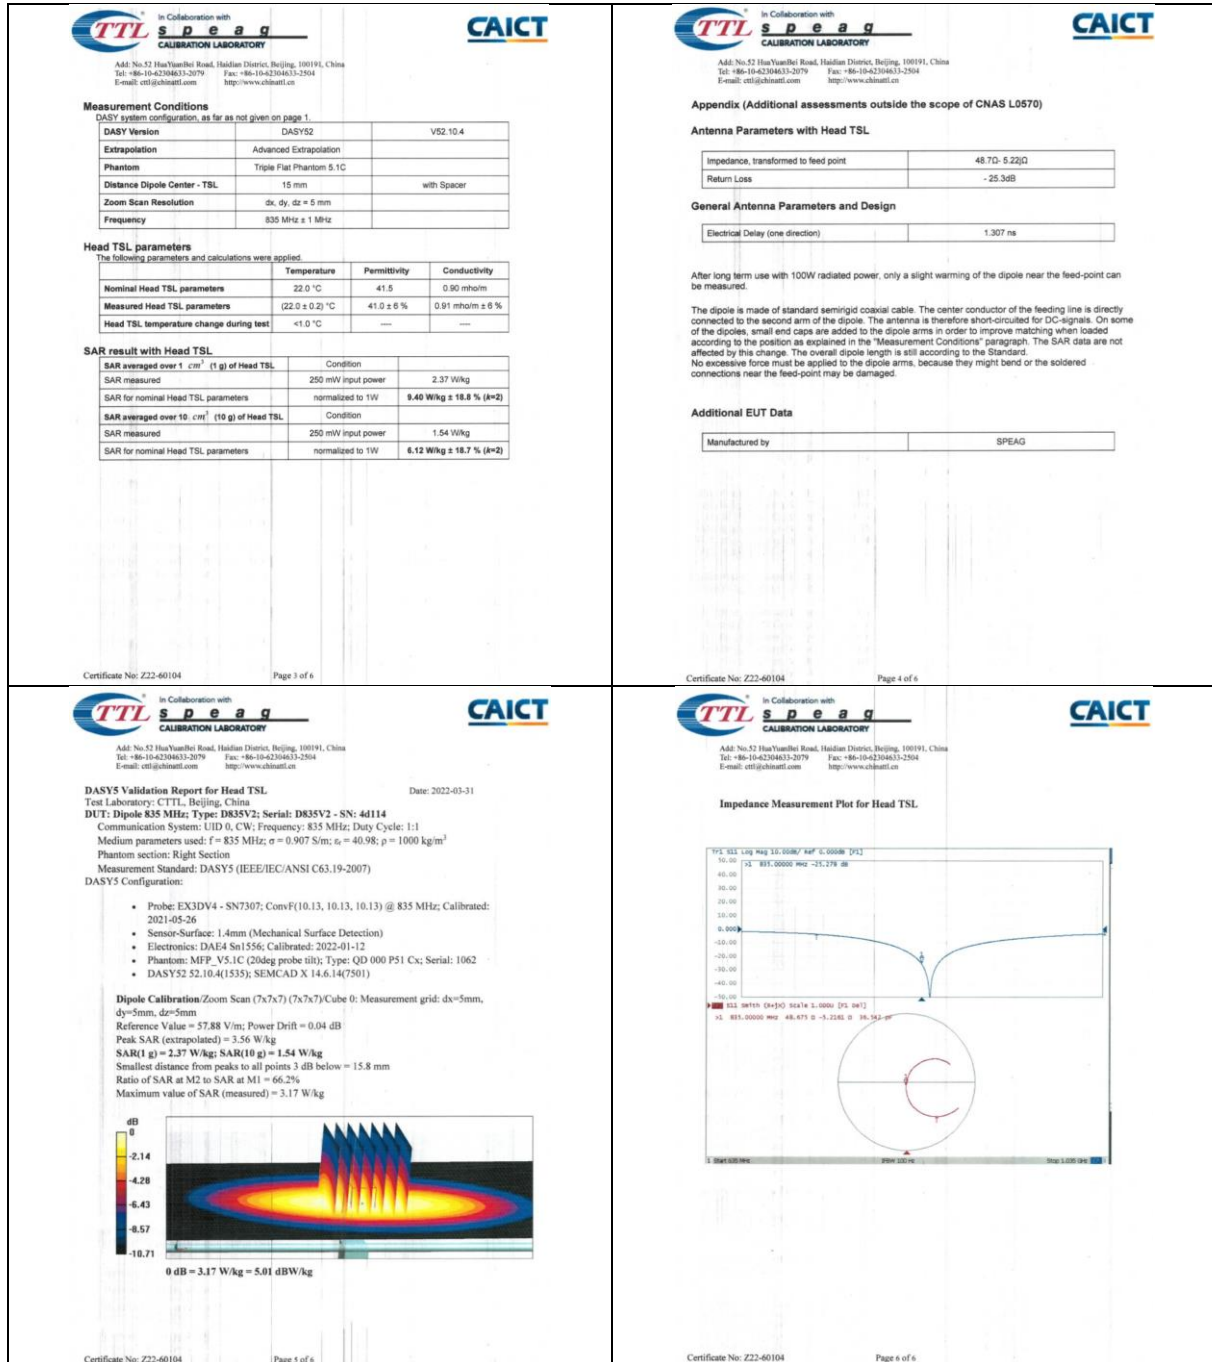


1.5 D900V2 - SN 1d079

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION CNAS 1079	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-6259633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6259633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Client: SGS-CN		Certificate No: Z22-60184	
CALIBRATION CERTIFICATE			
Object	D900V2 - SN: 1d079		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	June 7, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (S). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7464	28-Jan-22 (SPEAG No.EK3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.Z22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.Z22X00409)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: June 13, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60184		Page 1 of 6	

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION CNAS 1079	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6259633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6259633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	15 mm	with Spacer	
Zoom Scan Resolution	dk, dz: ±5 mm		
Frequency	900 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied.			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.97 nholm
Measured Head TSL parameters	(22.0 ± 0.2) °C	42.1 ± 6 %	0.98 nholm ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	2.70 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	11.0 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	1.73 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	7.09 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60184		Page 3 of 6	

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION CNAS 1079	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6259633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6259633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Glossary: TSL: tissue simulating liquid ConvF: sensitivity in TSL / NORMx,y,z N/A: not applicable or not measured			
Calibration is Performed According to the Following Standards: a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020 b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz" c) DASY4/5 System Handbook			
Additional Documentation: DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters: • Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated. • Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis. • Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required. • Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required. • SAR measured: SAR measured at the stated antenna input power. • SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector. • SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60184		Page 2 of 6	

In Collaboration with TTL s p e a g CALIBRATION LABORATORY		In Collaboration with CAICT CALIBRATION CNAS 1079	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6259633-2117 E-mail: cti@speag.com http://www.speag.com		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6259633-2117 E-mail: cti@caict.ac.cn http://www.caict.ac.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.10 - 8.49jΩ		
Return Loss	-23.3 dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.312 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60184		Page 4 of 6	

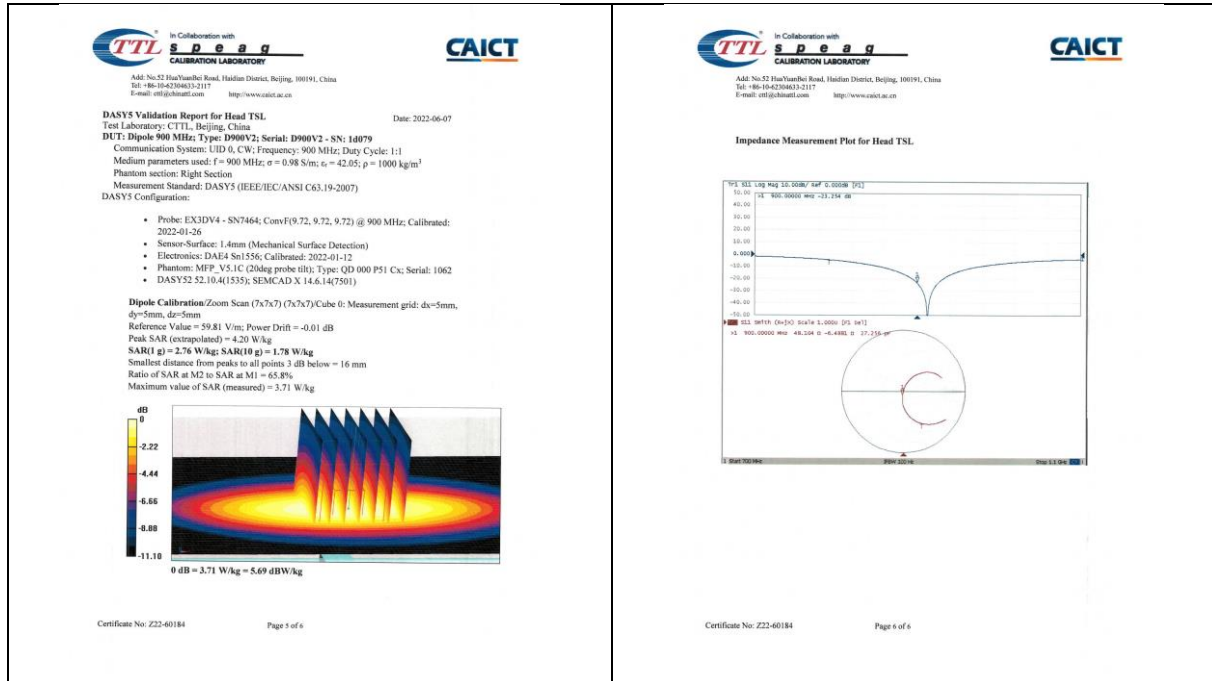

1.6 D1800V2 - SN 2d170

TTL In Collaboration with **CAICT**
SPEAG CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2117 Fax: +86-10-42306033-2117
E-mail: cti@china.ttl.com http://www.china.ttl.com

Client: **SGS-CN** Certificate No: **Z22-60105**

CALIBRATION CERTIFICATE

Object: **D1800V2 - SN: 2d170**

Calibration Procedure(s): **FF-Z11-003-01**
Calibration Procedures for dipole validation kits

Calibration date: **March 31, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility, environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY46110573	14-Jan-22 (CTTL No.J22X00409)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Lin Hao** SAR Test Engineer
Approved by: **Qi Diqian** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60105 Page 1 of 6

TTL In Collaboration with **CAICT**
SPEAG CALIBRATION LABORATORY

Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-42306033-2079 Fax: +86-10-42306033-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"


Additional Documentation:
c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60105 Page 2 of 6

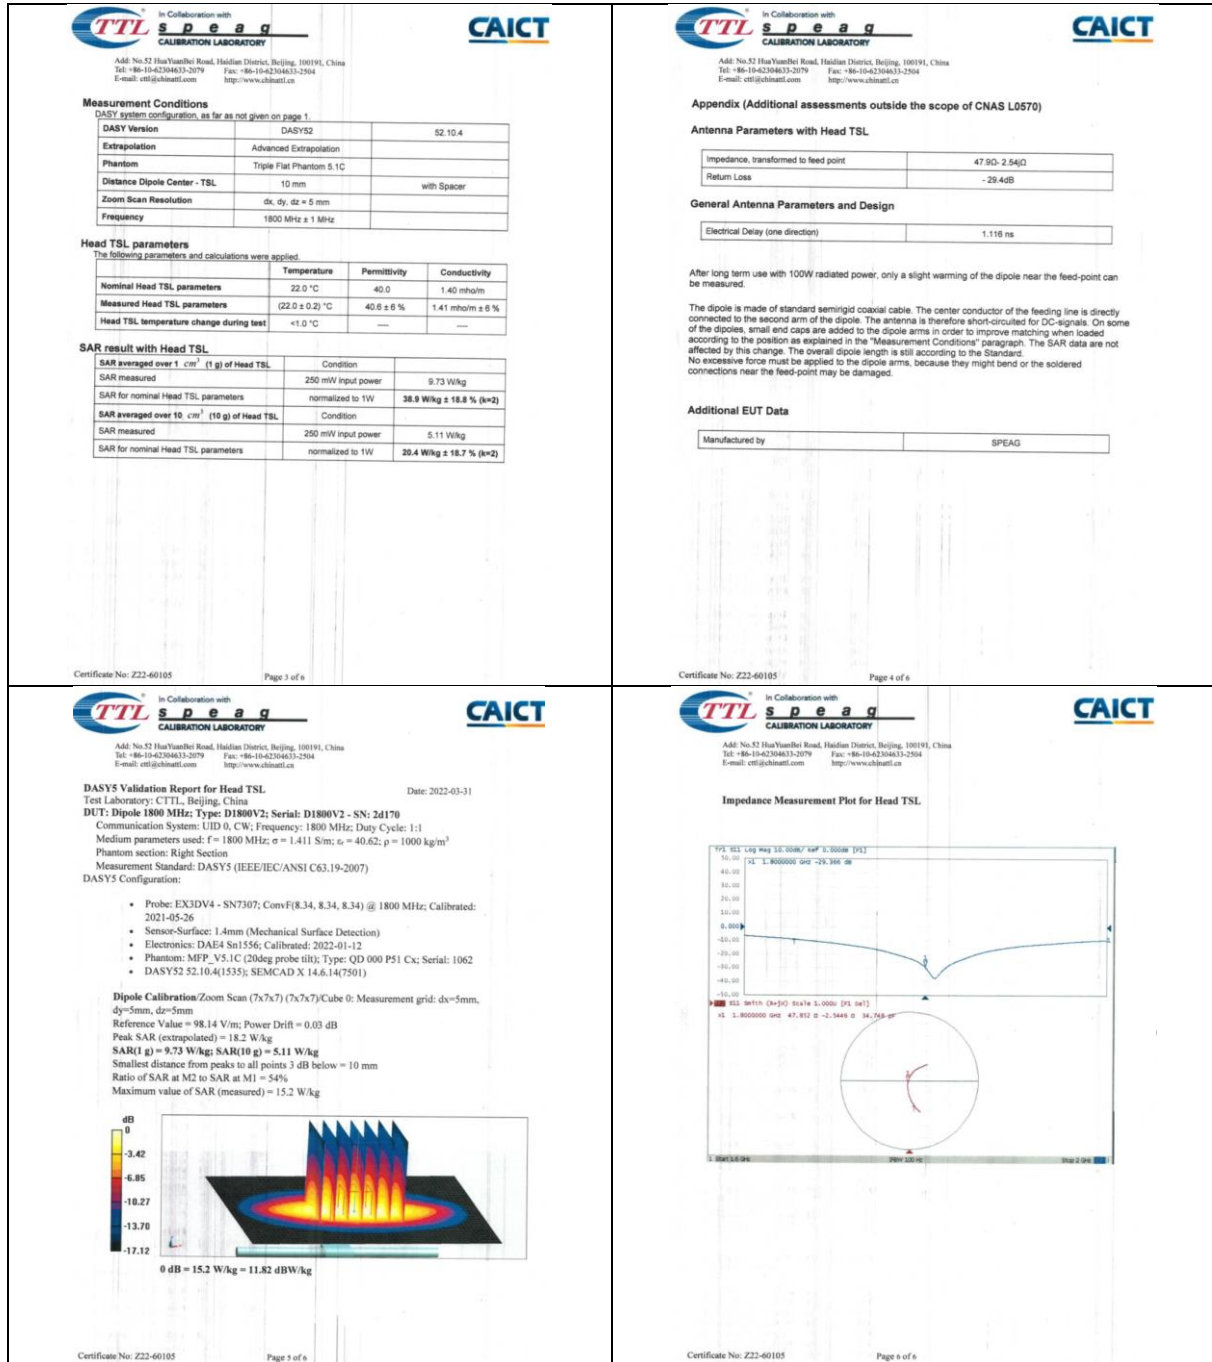


1.7 D1900V2 - SN 5d136

TTL S p e a g		CAICT	
In Collaboration with CALIBRATION LABORATORY		中国合格评定国家认可委员会 CALIBRATION	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com	
Client	SGS-CN	Certificate No.	Z22-60185
CALIBRATION CERTIFICATE			
Object	D1900V2 - SN: 5d136		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	June 7, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP6S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EXSDV4	SN 7464	28-Jan-22(SPEAG No EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No.J22X00409)	Jan-23
Network Analyzer E5071C	MY48110073	14-Jan-22 (CTTL No.J22X00409)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyan	SAR Project Leader	
Issued: June 13, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60185		Page 1 of 6	

TTL S p e a g		CAICT	
In Collaboration with CALIBRATION LABORATORY		中国合格评定国家认可委员会 CALIBRATION	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com	
Glossary:			
TSL	tissue simulating liquid		
ConF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865984, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60185		Page 2 of 6	

TTL S p e a g		CAICT	
In Collaboration with CALIBRATION LABORATORY		中国合格评定国家认可委员会 CALIBRATION	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com	
Measurement Conditions			
DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	1900 MHz ± 1 MHz		
Head TSL parameters			
The following parameters and calculations were applied:			
Nominal Head TSL parameters	Temperature	Permittivity	Conductivity
	32.0 °C	40.0	1.40 nS/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.9 ± 6 %	1.39 nS/m ± 6 %
Head TSL temperature change during test	<1.0 °C		
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	9.65 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	40.0 W/kg ± 16.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.18 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	20.8 W/kg ± 18.7 % (k=2)	
Certificate No: Z22-60185		Page 3 of 6	

TTL S p e a g		CAICT	
In Collaboration with CALIBRATION LABORATORY		中国合格评定国家认可委员会 CALIBRATION	
Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com		Add: No.52 Huayuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-4220603-2117 E-mail: cti@china-test.com	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	51.02 ± 7.58Ω		
Return Loss	-22.4dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.109 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC signals. On some of the dipoles, small and caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60185		Page 4 of 6	

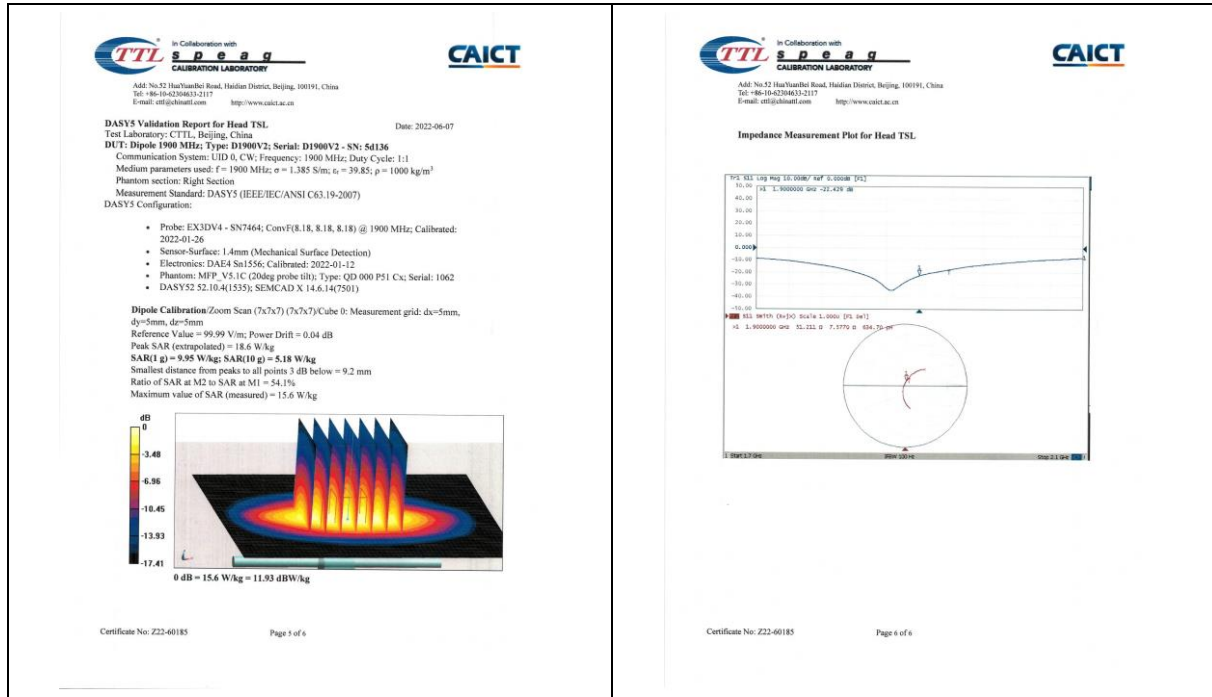

1.8 D2000V2 - SN 1041

TTL *speaq* **CAICT**

Address: No.52 Huayuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62586311-3117
E-mail: cti@ttsl.com.cn http://www.caict.ac.cn

Client: **SGS-CN** Certificate No: **Z22-60188**

CALIBRATION CERTIFICATE

Object: D2000V2 - SN: 1041

Calibration Procedure(s): FF-Z11-003-01
Calibration Procedures for dipole validation kits

Calibration date: June 8, 2022

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (B). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No. J21X08328)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No. J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22 (SPEAG No. EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No. Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No. J22X00409)	Jan-23

Calibrated by: Zhao Jing SAR Test Engineer

Reviewed by: Lin Hao SAR Test Engineer

Approved by: Qi Dianyuan SAR Project Leader

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60188 Page 1 of 6

TTL *speaq* **CAICT**

Address: No.52 Huayuan Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62586311-3117
E-mail: cti@ttsl.com.cn http://www.caict.ac.cn

Glossary:

TSL: Issue simulating liquid

ConvF: sensitivity in TSL / NORMx.y.z

N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020

b) KDS 865964, "SAR Measurement Requirements for 100 MHz to 8 GHz"

Additional Documentation:

c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:


- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.


The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60188 Page 2 of 6

In Collaboration with TTL CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230632-2117 E-mail: ott@china.ttl.com http://www.caict.ac.cn			
Measurement Conditions DASY system configuration, as far as not given on page 1.			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom S.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2000 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	1.39 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	10.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	41.8 W/kg ± 16.8 % (k=2)	
SAR averaged over 10 cm ³ (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.30 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	21.3 W/kg ± 16.7 % (k=2)	
Certificate No: Z22-60186 Page 3 of 6			

In Collaboration with TTL CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230632-2117 E-mail: ott@china.ttl.com http://www.caict.ac.cn			
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	48.4Ω ± 0.74Ω		
Return Loss	-34.9dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.088 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60186 Page 4 of 6			

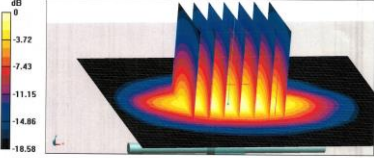In Collaboration with TTL CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230632-2117 E-mail: ott@china.ttl.com http://www.caict.ac.cn			
DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 2000 MHz; Type: D2000V2; Serial: D2000V2 - SN: 1041 Communication System: UTD 0, CW; Frequency: 2000 MHz; Duty Cycle: 1:1 Medium parameters used: f = 2000 MHz; σ = 1.392 S/m; ε = 40.21; ρ = 1000 kg/m ³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7464; ConvF(8.2, 8.2) @ 2000 MHz; Calibrated: 2022-01-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA64 Sn1556; Calibrated: 2022-01-12 - Phantom: MPP_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52: 52.10.4(1555); SEMCAD X 14.6.14(7501) Dipole Calibration/Zoom Scan (7x7x7) (7x7x7) Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm Reference Value = 103.4 V/m; Power Drift = 0.03 dB Peak SAR (extrapolated) = 19.6 W/kg SAR(1 g) = 10.4 W/kg; SAR(10 g) = 5.3 W/kg Smallest distance from peaks to all points 3 dB below = 9.1 mm Ratio of SAR at M2 to SAR at M1 = 53.6% Maximum value of SAR (measured) = 16.3 W/kg			
			
Certificate No: Z22-60186 Page 5 of 6			

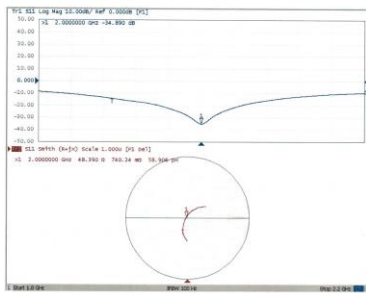In Collaboration with TTL CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-6230632-2117 E-mail: ott@china.ttl.com http://www.caict.ac.cn			
Impedance Measurement Plot for Head TSL			
			
Certificate No: Z22-60186 Page 6 of 6			


1.9 D2300V2 - SN 1096

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Client: SGS-CN		Certificate No: Z22-60106	
CALIBRATION CERTIFICATE			
Object	D2300V2 - SN: 1096		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	108277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No.EK3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Diqiyuan	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60106		Page 1 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY2	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2300 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.5	1.67 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.8 ± 6 %	1.70 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	12.4 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	49.2 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	5.88 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	23.4 W/kg ± 18.7 % (k=2)	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Glossary:			
TSL	Issue simulating liquid		
ConvF	sensitivity in TSL / NORMx,y,z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/5 System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60106		Page 2 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn		Add: No.52 HuaYuanbei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinaatl.com http://www.chinaatl.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.20 - 4.56jΩ		
Return Loss	- 26.6dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.083 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		
Certificate No: Z22-60106		Page 4 of 6	

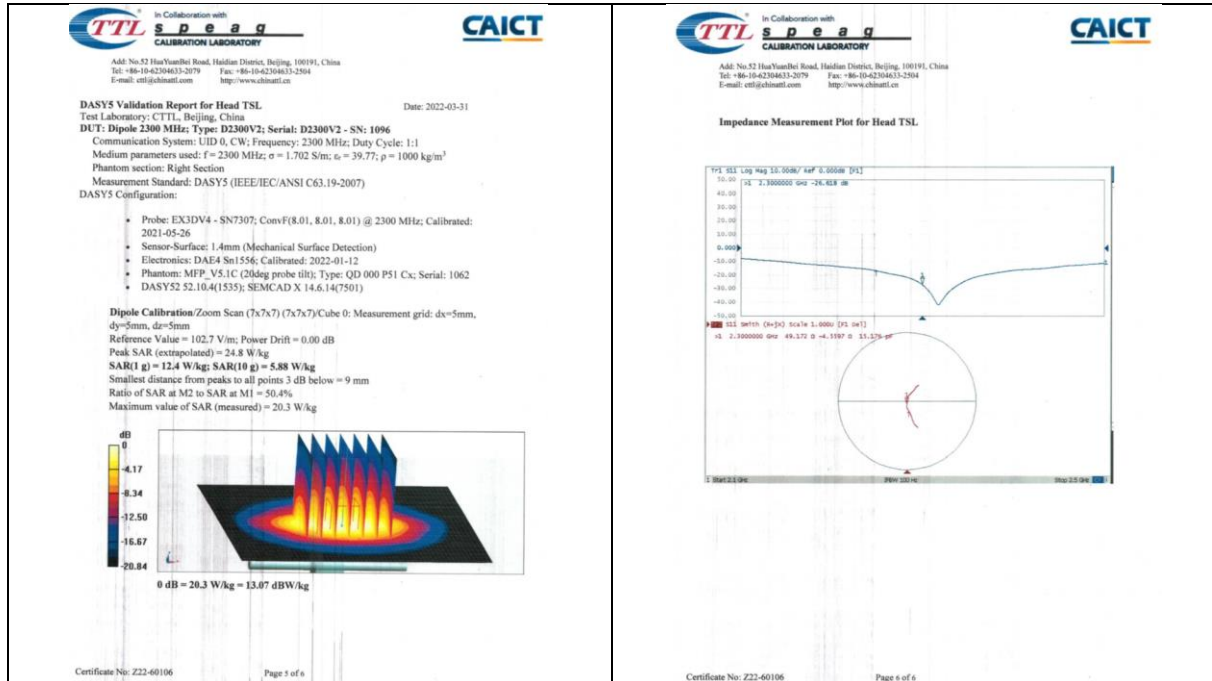

1.10 D2450V2 - SN 817

TTL Speaq Calibration Laboratory
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China
Tel: +86-10-62504633-2079 Fax: +86-10-62504633-2504
E-mail: cti@china.ttl.com http://www.china.ttl.com

CAICT

Client: **SGS-CN** Certificate No: **Z22-60107**

CALIBRATION CERTIFICATE

Object: **D2450V2 - SN: 817**

Calibration Procedure(s): **FF-Z11-003-Q1**
Calibration Procedures for dipole validation kits

Calibration date: **April 1, 2022**

This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity<70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter: NRP2	106277	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Power sensor: NRP8S	104291	24-Sep-21 (CTTL No.J21X08320)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21(SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No Z22-60007)	Jan-23

Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23

Calibrated by: **Zhao Jing** SAR Test Engineer
Reviewed by: **Lin Hao** SAR Test Engineer
Approved by: **Qi Dianyuan** SAR Project Leader

Issued: April 6, 2022

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: Z22-60107 Page 1 of 6

Glossary:
TSL: tissue simulating liquid
ConvF: sensitivity in TSL / NORMx.y.z
N/A: not applicable or not measured

Calibration is Performed According to the Following Standards:
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices- Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020
b) KDB 855664, "SAR Measurement Requirements for 100 MHz to 6 GHz"


Additional Documentation:
c) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor $k=2$, which for a normal distribution Corresponds to a coverage probability of approximately 95%.

Certificate No: Z22-60107 Page 2 of 6

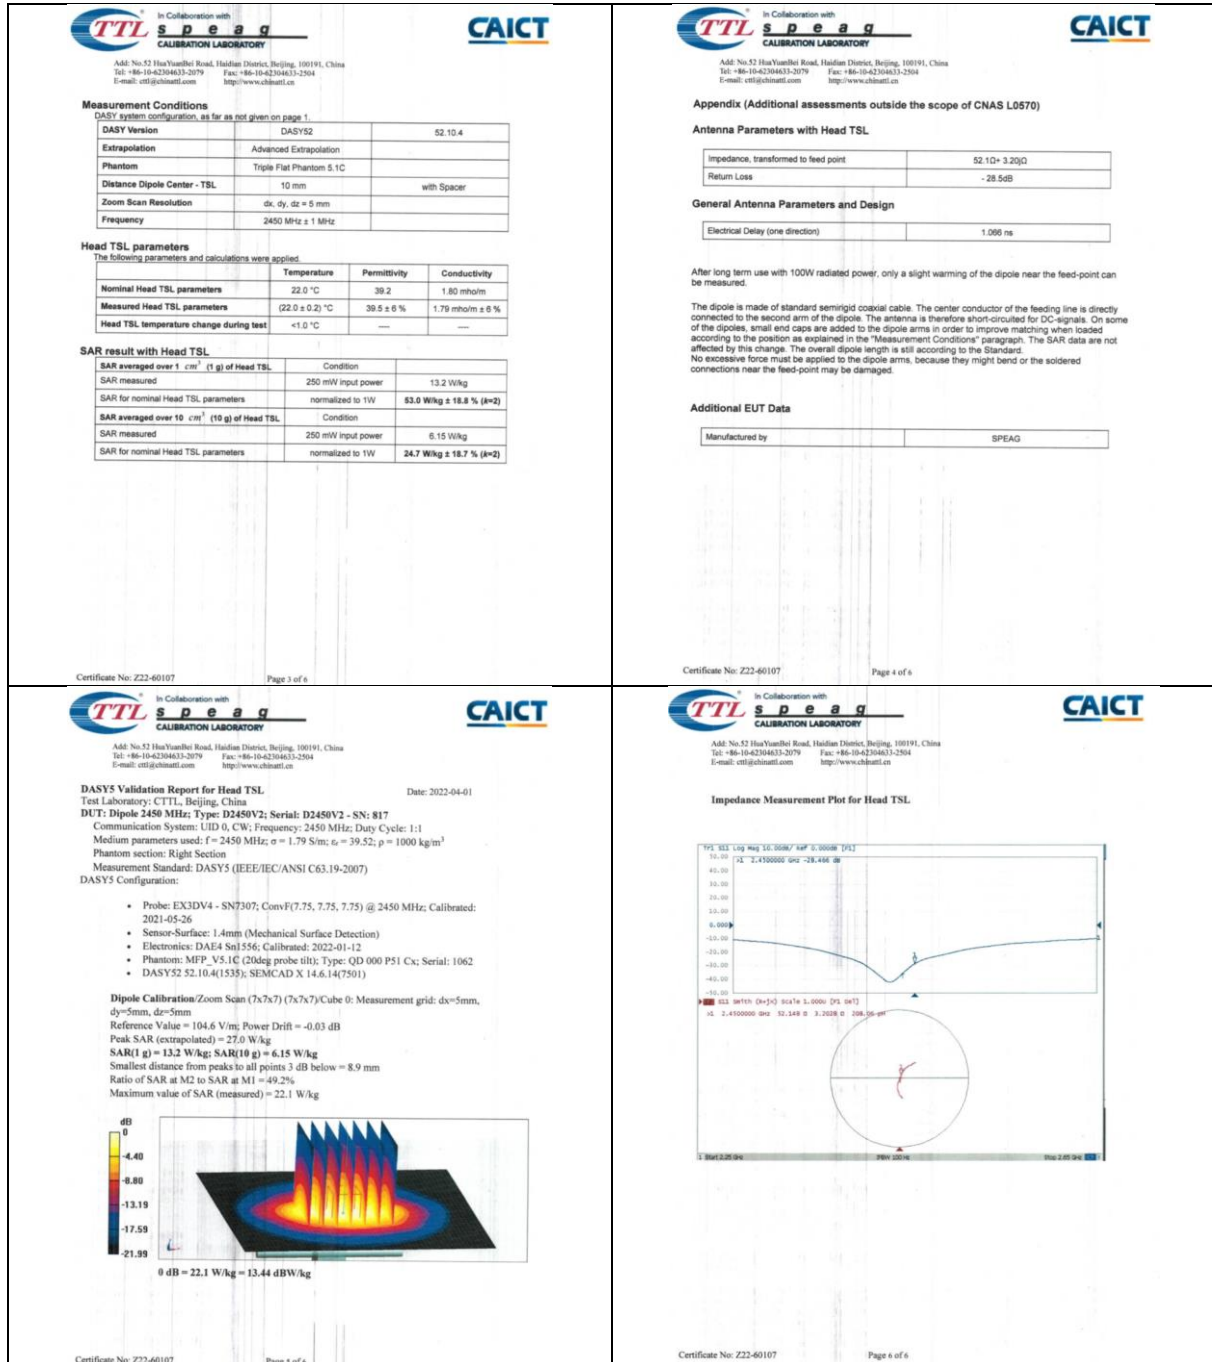


1.11 D2600V2 - SN 1158

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191 Tel: +86-10-42304633-2512 Fax: +86-10-42304633-2504 E-mail: cti@chinafil.com http://www.chinafil.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafil.com http://www.chinafil.cn	
Client	SGS-CN	Certificate No.	Z22-40108
CALIBRATION CERTIFICATE			
Object	D2600V2 - SN: 1158		
Calibration Procedure(s)	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	March 31, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (22±3)°C and humidity <70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08326)	Sep-22
Reference Probe EX3DV4	SN 7307	26-May-21 (SPEAG No EX3-7307_May21)	May-22
DAE4	SN 1556	12-Jan-22 (CTTL-SPEAG No Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY49071430	13-Jan-22 (CTTL No.J22X00406)	Jan-23
Network Analyzer E5071C	MY48110673	14-Jan-22 (CTTL No.J22X00406)	Jan-23
Calibrated by:	Name	Function	Signature
	Zhao Jing	SAR Test Engineer	
Reviewed by:	Lin Hao	SAR Test Engineer	
Approved by:	Qi Dianyuan	SAR Project Leader	
Issued: April 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-40108		Page 1 of 6	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafil.com http://www.chinafil.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafil.com http://www.chinafil.cn	
Measurement Conditions DASY system configuration, as far as not given on page 1:			
DASY Version	DASY52	52.10.4	
Extrapolation	Advanced Extrapolation		
Phantom	Triple Flat Phantom 5.1C		
Distance Dipole Center - TSL	10 mm	with Spacer	
Zoom Scan Resolution	dx, dy, dz = 5 mm		
Frequency	2600 MHz ± 1 MHz		
Head TSL parameters The following parameters and calculations were applied:			
	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.0	1.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	36.7 ± 6 %	1.96 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---
SAR result with Head TSL			
SAR averaged over 1 cm ² (1 g) of Head TSL	Condition		
SAR measured	250 mW input power	13.7 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	54.8 W/kg ± 18.8 % (k=2)	
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition		
SAR measured	250 mW input power	6.12 W/kg	
SAR for nominal Head TSL parameters	normalized to 1W	24.6 W/kg ± 18.7 % (k=2)	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafil.com http://www.chinafil.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafil.com http://www.chinafil.cn	
Glossary:			
TSL	tissue simulating liquid		
ConvF	sensitivity in TSL / NORMx.y.z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices - Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 865864, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4/S System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafil.com http://www.chinafil.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-42304633-2079 Fax: +86-10-42304633-2504 E-mail: cti@chinafil.com http://www.chinafil.cn	
Appendix (Additional assessments outside the scope of CNAS L0570)			
Antenna Parameters with Head TSL			
Impedance, transformed to feed point	49.90- 6.49jΩ		
Return Loss	- 23.8dB		
General Antenna Parameters and Design			
Electrical Delay (one direction)	1.053 ns		
After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured.			
The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged.			
Additional EUT Data			
Manufactured by	SPEAG		

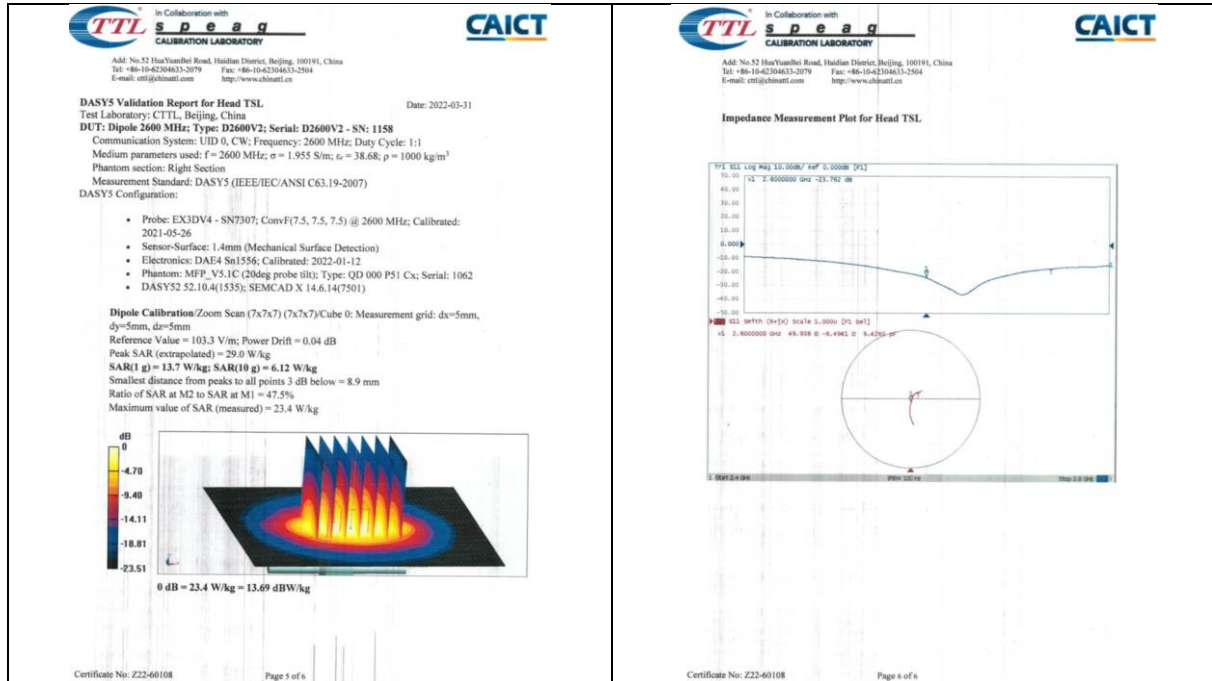

1.12 D5GHZV2 - SN 1095

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Client: SGS-CN		Certificate No: Z22-60187	
CALIBRATION CERTIFICATE			
Object:	D5GHZV2 - SN: 1095		
Calibration Procedure(s):	FF-Z11-003-01 Calibration Procedures for dipole validation kits		
Calibration date:	June 1, 2022		
This calibration Certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.			
All calibrations have been conducted in the closed laboratory facility: environment temperature (23±3)°C and humidity<70%.			
Calibration Equipment used (M&TE critical for calibration)			
Primary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Power Meter NRP2	106277	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Power sensor NRP8S	104291	24-Sep-21 (CTTL No.J21X08328)	Sep-22
Reference Probe EX3DV4	SN 7464	26-Jan-22(SPEAG No EX3-7464_Jan22)	Jan-23
DAE4	SN 1556	12-Jan-22(CTTL-SPEAG No.Z22-60007)	Jan-23
Secondary Standards	ID #	Cal Date (Calibrated by: Certificate No.)	Scheduled Calibration
Signal Generator E4438C	MY48071430	13-Jan-22 (CTTL No. J22X00409)	Jan-23
Network Analyzer E5071C	MY46110673	14-Jan-22 (CTTL No. J22X00406)	Jan-23
Calibrated by:	Name: Zhao Jing	Function: SAR Test Engineer	Signature: [Signature]
Reviewed by:	Name: Lin Hao	Function: SAR Test Engineer	Signature: [Signature]
Approved by:	Name: Qi Dianyan	Function: SAR Project Leader	Signature: [Signature]
Issued: June 6, 2022			
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			
Certificate No: Z22-60187		Page 1 of 10	

TTL Speaq CALIBRATION LABORATORY		CAICT	
Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn		Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62104633-2079 Fax: +86-10-62104633-2504 E-mail: cti@chinaul.com http://www.chinaul.cn	
Glossary:			
TSL	Issue simulating liquid		
ConF	sensitivity in TSL / NORMx,y,z		
N/A	not applicable or not measured		
Calibration is Performed According to the Following Standards:			
a) IEC/IEEE 62209-1528, "Measurement Procedure for The Assessment of Specific Absorption Rate of Human Exposure to Radio Frequency Fields from Hand-held and Body-mounted Wireless Communication Devices-Part 1528: Human Models, Instrumentation and Procedures (Frequency range of 4 MHz to 10 GHz)", October 2020			
b) KDB 665664, "SAR Measurement Requirements for 100 MHz to 6 GHz"			
Additional Documentation:			
c) DASY4S System Handbook			
Methods Applied and Interpretation of Parameters:			
• Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.			
• Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.			
• Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.			
• Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.			
• SAR measured: SAR measured at the stated antenna input power.			
• SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.			
• SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.			
The reported uncertainty of measurement is stated as the standard uncertainty of Measurement multiplied by the coverage factor k=2, which for a normal distribution Corresponds to a coverage probability of approximately 95%.			
Certificate No: Z22-60187		Page 2 of 10	



In Collaboration with

s p e a q

CALIBRATION LABORATORY

Addr: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62302117

E-mail: cnlg@china.ttl.com

<http://www.caict.ac.cn>



Measurement Conditions
DAISY system configuration, as far as not given on page 1.

DASY Version	DAISY2	52.10.4
Extrapolation	Advanced Extrapolation	
Phantom	Triple Flat Phantom 5.1C	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy = 4 mm, dz = 1.4 mm	Graded Ratio = 1.4 (Z direction)
Frequency	5200 MHz ± 1 MHz 5200 MHz ± 1 MHz 5500 MHz ± 1 MHz 5800 MHz ± 1 MHz	

Head TSL parameters at 5200MHz
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	36.0	4.66 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.4 ± 6 %	4.62 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5200MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	250 mW input power	7.79 W/kg
SAR measured	100 mW input power	7.79 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	77.6 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.22 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.1 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187

Page 3 of 10



In Collaboration with

s p e a q

CALIBRATION LABORATORY

Addr: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62302117

E-mail: cnlg@china.ttl.com

<http://www.caict.ac.cn>



Head TSL parameters at 5300MHz
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.9	4.76 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	35.2 ± 6 %	4.73 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5300MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	100 mW input power	7.94 W/kg
SAR measured	100 mW input power	7.94 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	79.1 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.27 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.6 W/kg ± 24.2 % (k=2)

Head TSL parameters at 5500MHz
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.6	4.96 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.8 ± 6 %	4.94 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5500MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	100 mW input power	6.29 W/kg
SAR measured	100 mW input power	6.29 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	82.6 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	23.3 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187

Page 4 of 10



In Collaboration with

s p e a q

CALIBRATION LABORATORY

Addr: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62302117

E-mail: cnlg@china.ttl.com

<http://www.caict.ac.cn>



Head TSL parameters at 5600MHz
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.5	5.07 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.7 ± 6 %	5.05 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5600MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	100 mW input power	8.12 W/kg
SAR measured	100 mW input power	8.12 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	80.8 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.30 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	22.9 W/kg ± 24.2 % (k=2)

Head TSL parameters at 5800MHz
The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	35.3	5.27 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	34.4 ± 6 %	5.25 mho/m ± 6 %
Head TSL temperature change during test	<1.0 °C	---	---

SAR result with Head TSL at 5800MHz

	Condition	
SAR averaged over 1 cm ² (1 g) of Head TSL	100 mW input power	7.71 W/kg
SAR measured	100 mW input power	7.71 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	76.7 W/kg ± 24.4 % (k=2)
SAR averaged over 10 cm ² (10 g) of Head TSL	Condition	
SAR measured	100 mW input power	2.16 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.8 W/kg ± 24.2 % (k=2)

Certificate No: Z22-60187

Page 5 of 10



In Collaboration with

s p e a q

CALIBRATION LABORATORY

Addr: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China

Tel: +86-10-62302117

E-mail: cnlg@china.ttl.com

<http://www.caict.ac.cn>



Appendix (Additional assessments outside the scope of CNAS L0570)

Antenna Parameters with Head TSL at 5200MHz

Impedance, transformed to feed point	48.1D-5.03jΩ
Return Loss	-23.6dB

Antenna Parameters with Head TSL at 5300MHz

Impedance, transformed to feed point	47.8D-2.42jΩ
Return Loss	-28.5dB

Antenna Parameters with Head TSL at 5500MHz

Impedance, transformed to feed point	50.3D-4.26jΩ
Return Loss	-27.4dB

Antenna Parameters with Head TSL at 5600MHz



Impedance, transformed to feed point	54.5D-4.80jΩ
Return Loss	-24.0dB

Antenna Parameters with Head TSL at 5800MHz

Impedance, transformed to feed point	51.5D-5.61jΩ
Return Loss	-24.9dB

Certificate No: Z22-60187

Page 6 of 10

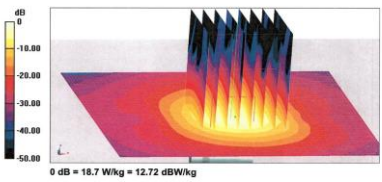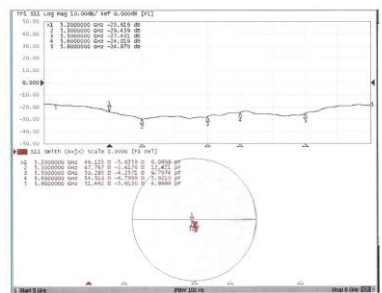In Collaboration with TTL s p e a q CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@chinaeet.com http://www.caict.ac.cn CAICT General Antenna Parameters and Design <table border="1"><tr><td>Electrical Delay (one direction)</td><td>1.101 ns</td></tr></table> After long term use with 100W radiated power, only a slight warming of the dipole near the feed-point can be measured. The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard. No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feed-point may be damaged. Additional EUT Data <table border="1"><tr><td>Manufactured by</td><td>SPEAG</td></tr></table> Certificate No: Z22-60187 Page 7 of 10	Electrical Delay (one direction)	1.101 ns	Manufactured by	SPEAG	In Collaboration with TTL s p e a q CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@chinaeet.com http://www.caict.ac.cn CAICT DASY5 Validation Report for Head TSL Test Laboratory: CTTL, Beijing, China DUT: Dipole 5Ghz; Type: D5GhzV2; Serial: D5GhzV2 - SN: 1095 Communication System: CW; Frequency: 5200 MHz; Frequency: 5300 MHz; Frequency: 5500 MHz; Frequency: 5600 MHz; Frequency: 5800 MHz; Duty Cycle: 1:1 Medium parameters used: f = 5200 MHz; σ = 4.62 S/m; ϵ_r = 35.39; ρ = 1000 kg/m³ Medium parameters used: f = 5300 MHz; σ = 4.73 S/m; ϵ_r = 35.19; ρ = 1000 kg/m³ Medium parameters used: f = 5500 MHz; σ = 4.939 S/m; ϵ_r = 34.83; ρ = 1000 kg/m³ Medium parameters used: f = 5600 MHz; σ = 5.051 S/m; ϵ_r = 34.69; ρ = 1000 kg/m³ Medium parameters used: f = 5800 MHz; σ = 5.247 S/m; ϵ_r = 34.42; ρ = 1000 kg/m³ Phantom section: Right Section Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007) DASY5 Configuration: - Probe: EX3DV4 - SN7484; ConvF(5.6, 5.6, 5.6) @ 5200 MHz; ConvF(5.32, 5.32, 5.32) @ 5300 MHz; ConvF(5.11, 5.11, 5.11) @ 5500 MHz; ConvF(4.91, 4.91, 4.91) @ 5600 MHz; ConvF(5, 5, 5) @ 5800 MHz; Calibrated: 2022-01-26 - Sensor-Surface: 1.4mm (Mechanical Surface Detection) - Electronics: DA64 Sn1556; Calibrated: 2022-01-12 - Phantom: MPF_V5.1C (20deg probe tilt); Type: QD 000 P51 Cx; Serial: 1062 - DASY52 52.10.4(1535); SEMCAD X 14.6.14(7501) Dipole Calibration /Pin=100mW, d=10mm, f=5200 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 60.80 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 29.8 W/kg SAR(1 g) = 7.79 W/kg; SAR(10 g) = 2.22 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 66.8% Maximum value of SAR (measured) = 18.3 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5300 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 31.5 W/kg SAR(1 g) = 7.94 W/kg; SAR(10 g) = 2.27 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 65.5% Maximum value of SAR (measured) = 19.0 W/kg Certificate No: Z22-60187 Page 8 of 10
Electrical Delay (one direction)	1.101 ns				
Manufactured by	SPEAG				
In Collaboration with TTL s p e a q CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@chinaeet.com http://www.caict.ac.cn CAICT Dipole Calibration /Pin=100mW, d=10mm, f=5500 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 61.92 V/m; Power Drift = -0.08 dB Peak SAR (extrapolated) = 34.7 W/kg SAR(1 g) = 8.20 W/kg; SAR(10 g) = 2.34 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 63.9% Maximum value of SAR (measured) = 20.2 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5600 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 65.08 V/m; Power Drift = -0.07 dB Peak SAR (extrapolated) = 35.2 W/kg SAR(1 g) = 8.12 W/kg; SAR(10 g) = 2.3 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 62.5% Maximum value of SAR (measured) = 19.1 W/kg Dipole Calibration /Pin=100mW, d=10mm, f=5800 MHz/Zoom Scan, dist=1.4mm (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm Reference Value = 62.13 V/m; Power Drift = -0.06 dB Peak SAR (extrapolated) = 34.8 W/kg SAR(1 g) = 7.71 W/kg; SAR(10 g) = 2.16 W/kg Smallest distance from peaks to all points 3 dB below = 7.2 mm Ratio of SAR at M2 to SAR at M1 = 61.6% Maximum value of SAR (measured) = 18.7 W/kg  Certificate No: Z22-60187 Page 9 of 10	In Collaboration with TTL s p e a q CALIBRATION LABORATORY Add: No.52 HuaYuanBei Road, Haidian District, Beijing, 100191, China Tel: +86-10-62302117 E-mail: csl@chinaeet.com http://www.caict.ac.cn CAICT Impedance Measurement Plot for Head TSL  Certificate No: Z22-60187 Page 10 of 10				

2 DAE4 - SN 1245

Schmid & Partner Engineering AG Zugheggenstrasse 43, 8004 Zurich, Switzerland Phone +41 44 245 9700, Fax +41 44 245 9779 www.speag.com, info@speag.com s p e a g IMPORTANT NOTICE USAGE OF THE DAE4 The DAE unit is a delicate, high precision instrument and requires careful treatment by the user. There are no serviceable parts inside the DAE. Special attention shall be given to the following points: Battery Exchange: The battery cover of the DAE4 unit is fixed using a screw, over tightening the screw may cause the threads inside the DAE to wear out. Shipping of the DAE: Before shipping the DAE to SPEAG for calibration, remove the batteries and pack the DAE in an anti-static bag. This anti-static bag shall then be packed into a larger box or container which protects the DAE from impacts during transportation. The package shall be marked to indicate that a fragile instrument is inside. E-Stop Failures: Touch detection may be malfunctioning due to broken magnets in the E-stop. Rough handling of the E-stop may lead to damage of these magnets. Touch and collision errors are often caused by dust and get accumulated in the E-stop. To prevent E-stop failure, the customer shall always mount the probe to the DAE carefully and keep the DAE unit in a non-dusty environment if not used for measurements. Repair: Minor repairs are performed at no extra cost during the annual calibration. However, SPEAG reserves the right to charge for any repair especially if rough unprofessional handling caused the defect. DASY Configuration File: Since the exact values of the DAE input resistances, as measured during the calibration procedure of a DAE unit, are not used by the DASY software, a nominal value of 200 MΩ is given in the corresponding configuration file. Important Note: Warranty and calibration is void if the DAE unit is disassembled partly or fully by the Customer. Important Note: Never attempt to grease or oil the E-stop assembly. Cleaning and readjusting of the E-stop assembly is allowed by certified SPEAG personnel only and is part of the annual calibration procedure. Important Note: To prevent damage of the DAE probe connector pins, use great care when installing the probe to the DAE. Carefully connect the probe with the connector notch oriented in the mating position. Avoid any rotational movement of the probe body versus the DAE while turning the locking nut of the connector. The same care shall be used when disconnecting the probe from the DAE. TH_EH190309AE DAE4.docx 07.03.2019	Calibration Laboratory of Schmid & Partner Engineering AG Zugheggenstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Client: SGS Kunshan City, China Certificate No.: DAE4-1245_Apr23 Accreditation No.: SCS 0108 Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service CALIBRATION CERTIFICATE Object: DAE4 - SD 000 D04 BM - SN: 1245 Calibration procedure(s): QA CAL-06.v30 Calibration procedure for the data acquisition electronics (DAE) Calibration date: April 25, 2023 This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate. All calibrations have been conducted in the closed laboratory facility, environment temperature (22 ± 3)°C and humidity < 70%. Calibration Equipment used (MATE critical for calibration) <table border="1"><thead><tr><th>Primary Standards</th><th>ID #</th><th>Cal Date (Certificate No.)</th><th>Scheduled Calibration</th></tr></thead><tbody><tr><td>Kathley Multimeter Type 2001</td><td>SN: 0810279</td><td>29-Aug-22 (No. 34388)</td><td>Aug-23</td></tr></tbody></table> <table border="1"><thead><tr><th>Secondary Standards</th><th>ID #</th><th>Check Date (in house)</th><th>Scheduled Check</th></tr></thead><tbody><tr><td>Auto DAE Calibration Unit</td><td>SE UMS 032 AA 1001</td><td>27-Jan-23 (in house check)</td><td>In house check: Jan-24</td></tr><tr><td>Calibrator line C2.1</td><td>SE UMS 008 AA 1002</td><td>27-Jan-23 (in house check)</td><td>In house check: Jan-24</td></tr></tbody></table> Calibrated by: Domènec Sallent (Name), Laboratory Technician (Function), <i>[Signature]</i> (Signature) Approved by: Stefan Kuhn (Name), Technical Manager (Function), <i>[Signature]</i> (Signature) This calibration certificate shall not be reproduced except in full without written approval of the laboratory. Issued April 25, 2023 Certificate No: DAE4-1245_Apr23 Page 1 of 5	Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration	Kathley Multimeter Type 2001	SN: 0810279	29-Aug-22 (No. 34388)	Aug-23	Secondary Standards	ID #	Check Date (in house)	Scheduled Check	Auto DAE Calibration Unit	SE UMS 032 AA 1001	27-Jan-23 (in house check)	In house check: Jan-24	Calibrator line C2.1	SE UMS 008 AA 1002	27-Jan-23 (in house check)	In house check: Jan-24
Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration																		
Kathley Multimeter Type 2001	SN: 0810279	29-Aug-22 (No. 34388)	Aug-23																		
Secondary Standards	ID #	Check Date (in house)	Scheduled Check																		
Auto DAE Calibration Unit	SE UMS 032 AA 1001	27-Jan-23 (in house check)	In house check: Jan-24																		
Calibrator line C2.1	SE UMS 008 AA 1002	27-Jan-23 (in house check)	In house check: Jan-24																		
Calibration Laboratory of Schmid & Partner Engineering AG Zugheggenstrasse 43, 8004 Zurich, Switzerland Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates Accreditation No.: SCS 0108 Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service Glossary DAE: data acquisition electronics Connector angle: information used in DASY system to align probe sensor X to the robot coordinate system. Methods Applied and Interpretation of Parameters • DC Voltage Measurement: Calibration Factor assessed for use in DASY system by comparison with a calibrated instrument traceable to national standards. The figure given corresponds to the full scale range of the voltmeter in the respective range. • Connector angle: The angle of the connector is assessed measuring the angle mechanically by a tool inserted. Uncertainty is not required. • The following parameters as documented in the Appendix contain technical information as a result from the performance test and require no uncertainty. • DC Voltage Measurement Linearity: Verification of the Linearity at +10% and -10% of the nominal calibration voltage. Influence of offset voltage is included in this measurement. • Common mode sensitivity: Influence of a positive or negative common mode voltage on the differential measurement. • Channel separation: Influence of a voltage on the neighbor channels not subject to an input voltage. • AD Converter Values with inputs shorted: Values on the internal AD converter corresponding to zero input voltage. • Input Offset Measurement: Output voltage and statistical results over a large number of zero voltage measurements. • Input Offset Current: Typical value for information; Maximum channel input offset current, not considering the input resistance. • Input resistance: Typical value for information; DAE input resistance at the connector, during internal auto-zeroing and during measurement. • Low Battery Alarm Voltage: Typical value for information. Below this voltage, a battery alarm signal is generated. • Power consumption: Typical value for information. Supply currents in various operating modes. Certificate No: DAE4-1245_Apr23 Page 2 of 5	DC Voltage Measurement AD - Converter Resolution nominal: 6.1μV High Range: 1LSB = 6.1μV, full range = -100...+300 mV Low Range: 1LSB = 61nV, full range = -1...+30mV DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec <table border="1"><thead><tr><th>Calibration Factors</th><th>X</th><th>Y</th><th>Z</th></tr></thead><tbody><tr><td>High Range</td><td>405.243 ± 0.02% (k=2)</td><td>403.938 ± 0.02% (k=2)</td><td>405.064 ± 0.02% (k=2)</td></tr><tr><td>Low Range</td><td>3.99474 ± 1.50% (k=2)</td><td>3.99478 ± 1.50% (k=2)</td><td>4.00994 ± 1.50% (k=2)</td></tr></tbody></table> Connector Angle <table border="1"><thead><tr><th>Connector Angle to be used in DASY system</th><th>32.0° ± 1°</th></tr></thead></table> Certificate No: DAE4-1245_Apr23 Page 3 of 5	Calibration Factors	X	Y	Z	High Range	405.243 ± 0.02% (k=2)	403.938 ± 0.02% (k=2)	405.064 ± 0.02% (k=2)	Low Range	3.99474 ± 1.50% (k=2)	3.99478 ± 1.50% (k=2)	4.00994 ± 1.50% (k=2)	Connector Angle to be used in DASY system	32.0° ± 1°						
Calibration Factors	X	Y	Z																		
High Range	405.243 ± 0.02% (k=2)	403.938 ± 0.02% (k=2)	405.064 ± 0.02% (k=2)																		
Low Range	3.99474 ± 1.50% (k=2)	3.99478 ± 1.50% (k=2)	4.00994 ± 1.50% (k=2)																		
Connector Angle to be used in DASY system	32.0° ± 1°																				

Appendix (Additional assessments outside the scope of SC50108)

1. DC Voltage Linearity

High Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	19998.60	2.90	0.00
Channel X - Input	20005.77	2.75	0.01
Channel X + Input	-19998.65	2.19	-0.01
Channel Y + Input	19999.60	1.08	0.00
Channel Y - Input	20003.12	0.26	0.00
Channel Z + Input	-20000.51	-1.06	-0.00
Channel Z - Input	19999.62	-1.06	-0.00
Channel Z + Input	20002.17	-0.70	-0.00
Channel Z - Input	-20001.94	-0.91	0.00

Low Range	Reading (µV)	Difference (µV)	Error (%)
Channel X + Input	2002.91	0.81	0.04
Channel X - Input	203.06	0.73	0.36
Channel X + Input	-196.56	0.88	-0.45
Channel Y + Input	2002.33	0.29	0.01
Channel Y - Input	201.91	-0.39	-0.19
Channel Z + Input	-196.22	-0.79	0.40
Channel Z - Input	2002.29	0.24	0.01
Channel Z + Input	201.28	-0.88	-0.44
Channel Z - Input	-198.03	-1.36	0.69

2. Common mode sensitivity

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Common mode Input Voltage (mV)	High Range Average Reading (µV)	Low Range Average Reading (µV)
Channel X	200	-8.42	-8.27
	-200	8.81	8.00
Channel Y	200	7.04	7.13
	-200	-14.70	-15.29
Channel Z	200	-4.52	-5.35
	-200	3.50	3.52

3. Channel separation

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	Input Voltage (mV)	Channel X (µV)	Channel Y (µV)	Channel Z (µV)
Channel X	200	-	3.29	-3.29
Channel Y	200	9.00	-	4.00
Channel Z	200	10.03	7.20	-

Certificate No: DA-E4-1245_Apr23

Page 4 of 5

4. AD-Converter Values with inputs shorted

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

	High Range (LSB)	Low Range (LSB)
Channel X	16001	16100
Channel Y	16079	16051
Channel Z	16040	15891

5. Input Offset Measurement

DASY measurement parameters: Auto Zero Time: 3 sec; Measuring time: 3 sec

Input (mV)	Average (µV)	min. Offset (µV)	max. Offset (µV)	Std. Deviation (µV)
Channel X	0.77	-0.83	1.89	0.49
Channel Y	-0.24	-1.72	1.19	0.52
Channel Z	-0.85	-2.62	0.59	0.61

6. Input Offset Current

Nominal input circuitry offset current on all channels: <25nA

7. Input Resistance (Typical values for information)

	Zeroing (kOhm)	Measuring (Mohm)
Channel X	200	200
Channel Y	200	200
Channel Z	200	200

8. Low Battery Alarm Voltage (Typical values for information)

Typical values	Alarm Level (VDC)
Supply (+ Vcc)	+7.9
Supply (- Vcc)	-7.6

9. Power Consumption (Typical values for information)

Typical values	Switched off (mA)	Stand by (mA)	Transmitting (mA)
Supply (+ Vcc)	+0.01	+6	+14
Supply (- Vcc)	-0.01	-8	-9

Certificate No: DA-E4-1245_Apr23

Page 5 of 5

3 EX3DV4 - SN 7767

Calibration Laboratory of
Schmid & Partner
Engineering AGAccredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificatesS Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Client: SGS-CN (Auden)

Certificate No: EX-7767_Oct22

CALIBRATION CERTIFICATE

Object: EX3DV4 - SN:7767

Calibration procedures: QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v6, QA CAL-23.v5,
QA CAL-25.v7
Calibration procedure for dosimetric E-field probes

Calibration date: October 28, 2022

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3) °C and humidity < 70%.

Calibration Equipment used (DATE critical for calibration)

Primary Standards	ID	Cal. Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-22 (No. 217-03528-03504)	Apr-23
Power sensor NRP-291	SN: 103944	04-Apr-22 (No. 217-03504)	Apr-23
DCP DAK-3.1 (Impedance)	SN: 1548	25-Oct-22 (DCP DAK3-1548_Oct22)	Oct-23
DCP DAK-12	SN: 1018	25-Oct-22 (DCP DAK3-1018_Oct22)	Oct-23
Reference 50 dB Attenuator	SN: C05582 (50)	04-Apr-22 (No. 217-03607)	Apr-23
DAE4	SN: 981	19-Oct-22 (No. DA-E4-880_Oct22)	Oct-23
Reference Probe E53202	SN: 3013	07-Dec-21 (No. 553-3013_Oct21)	Dec-22

Secondary Standards	ID	Check Date (in house)	Scheduled Check
Power meter E411B	SN: GB41268074	05-Apr-16 (in house check Jun-20)	In house check: Jun-24
Power sensor E411A	SN: E411A-09887	05-Apr-16 (in house check Jun-20)	In house check: Jun-24
Power sensor E4415A	SN: 00011210	05-Apr-16 (in house check Jun-20)	In house check: Jun-24
RF generator HP 8540C	SN: US840J01705	04-Aug-09 (in house check Jun-20)	In house check: Jun-24
Network Analyzer F855A	SN: E411A0477	31-May-14 (in house check Oct-20)	In house check: Oct-24

Calibrated by:	Name	Function	Signature
	Aldona Georgiadou	Laboratory Technician	
Approved by:	Ewen Kohn	Technical Manager	

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: EX-7767_Oct22

Page 1 of 9

Calibration Laboratory of
Schmid & Partner
Engineering AGAccredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificatesS Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Glossary

TSL	Issue simulating liquid
NORM _{xyz}	sensitivity in free space
ConF	sensitivity in TSL, NORM _{xyz}
DCP	diode compression point
CP	crest factor (100% cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
γ	γ rotation around probe axis
φ	φ rotation around air axis that is in the plane normal to probe axis (at measurement center), i.e., φ = 0 is normal to probe axis
Polarization θ	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEC61010-1:2010, "Measurement Procedure For The Assessment Of Specific Absorption Rate Of Human Exposure To Radio Frequency Fields From Hand-Held And Body-Worn Wireless Communication Devices - Part 1: 1528: Human Models, Instrumentation And Procedures (Frequency Range of 4 MHz to 10 GHz)", October 2020.
- b) IEC 60958, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORM_{xyz}: Assessed for E-field polarization θ = 0 (f < 800 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORM_{xyz} are only intermediate values, i.e., the uncertainties of NORM_{xyz} does not affect the E-field uncertainty made TSL (see below ConF).
- NORM_{xyz} = NORM_{xyz} * frequency response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConF.

- DCP: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal. DCP does not depend on frequency nor media.

- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics.

- A_{xyz}, B_{xyz}, C_{xyz}, D_{xyz}, V_{RF,xyz}, A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. V_{RF} is the maximum calibration range expressed in RMS voltage across the diode.

- ConF and Boundary Effect Parameters: Assessed in far phantom using E-field or Temperature Transfer Standard for f > 800 MHz and made waveguide using analytical field distribution based on power measurements for f < 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{xyz} * ConF whereby the uncertainty corresponds to that given for ConF. A frequency dependent ConF is used in DASY version 4.4 and higher which allows extending the validity from < 50 MHz to > 100 MHz.

- Spherical isotropy (3D deviation from isotropy): In a field of low gradients realized using a flat phantom exposed by a patch antenna.

- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.

- Connector Angle: The angle is assessed using the information gained by determining the NORM (no uncertainty required).

Certificate No: EX-7767_Oct22

Page 2 of 9

EX3DV4 - SN:7767

October 28, 2022

Parameters of Probe: EX3DV4 - SN:7767

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k = 2)
Norm (μA/(Vmm ²)) ^A	0.67	0.69	0.56	±10.1%
DCP (mV) ^B	103.4	107.3	105.7	±4.7%

Calibration Results for Modulation Response

URS	Communication System Name	A dB	B dB/μV	C	D dB	VR mV	Max dec.	Max Unc ^C k = 2
0	CW	X 0.00	0.00	1.00	0.00	184.7	±3.5%	±4.7%
		Y 0.00	0.00	1.00		186.7		
		Z 0.00	0.00	1.00		179.3		

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of Norm X,Y,Z do not affect the $k=2$ total uncertainty inside T85 (see Page 5).

^B Uncertainty parameter uncertainty for maximum specified field strength.

^C Uncertainty is determined using the min. deviation from three responses applying rectangular distribution and is expressed for the square of the test value.

Certificate No: EX-7767_Oct22

Page 5 of 9

EX3DV4 - SN:7767

October 28, 2022

Parameters of Probe: EX3DV4 - SN:7767

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle	144.8°
Mechanical Surface Detection Mode	disabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	16 mm
Tip Length	3 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	1.4 mm

Note: Measurement distance from surface can be increased to 3-4 mm for an Area Scan job.

Certificate No: EX-7767_Oct22

Page 4 of 9

EX3DV4 - SN:7767

October 28, 2022

Parameters of Probe: EX3DV4 - SN:7767

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^D	Relative Permittivity ^E	Conductivity ^F (S/m)	CompF X	CompF Y	CompF Z	Alpha ^G	Depth ^H (mm)	Unc (k = 2)
150	52.3	0.79	14.08	14.08	14.08	0.00	1.00	±13.2%
450	43.5	0.97	11.90	11.90	11.90	0.16	1.20	±13.3%
750	41.9	0.99	10.26	10.26	10.26	0.50	0.80	±12.0%
835	41.5	0.90	10.00	10.00	10.00	0.43	0.80	±12.0%
1750	40.1	1.37	9.32	9.32	9.32	0.36	0.86	±12.0%
1900	40.0	1.40	8.91	8.91	8.91	0.33	0.86	±12.0%
2100	39.8	1.49	8.60	8.60	8.60	0.30	0.86	±12.0%
2200	39.5	1.67	8.44	8.44	8.44	0.33	0.90	±12.0%
2450	39.2	1.80	8.24	8.24	8.24	0.32	0.90	±12.0%
2600	39.0	1.96	7.99	7.99	7.99	0.27	0.90	±12.0%
3000	38.2	2.71	7.55	7.55	7.55	0.30	1.25	±13.1%
3600	37.9	2.91	7.45	7.45	7.45	0.30	1.35	±13.1%
3700	37.7	3.12	7.20	7.20	7.20	0.30	1.35	±13.1%
3900	37.5	3.32	6.84	6.84	6.84	0.40	1.69	±13.1%
4100	37.2	3.53	6.63	6.63	6.63	0.40	1.80	±13.1%
4300	37.1	3.65	6.39	6.39	6.39	0.40	1.70	±13.1%
4400	36.9	3.84	6.17	6.17	6.17	0.40	1.70	±13.1%
4600	36.7	4.04	6.15	6.15	6.15	0.40	1.70	±13.1%
4800	36.4	4.26	6.13	6.13	6.13	0.45	1.90	±13.1%
4900	36.3	4.40	6.07	6.07	6.07	0.40	1.80	±13.1%
5200	36.0	4.66	5.65	5.65	5.65	0.40	1.80	±13.1%
5300	35.9	4.76	5.48	5.48	5.48	0.40	1.80	±13.1%
5500	35.6	4.96	5.30	5.30	5.30	0.40	1.80	±13.1%
5900	35.5	5.07	5.14	5.14	5.14	0.40	1.80	±13.1%
5900	35.3	5.27	5.10	5.10	5.10	0.40	1.80	±13.1%

^D Frequency validity above 300 MHz at ±100 MHz only applies for CDP v4.4 and higher (see Page 5), while it is reserved to ±50 MHz. The uncertainty is the RMS of the CompF parameter in calibration frequency and the constant for the relative frequency trend. Frequency validity below 300 MHz is ±1%, 2%, 4%, 5% and 10% for CDP assessments at 30, 60, 120, 150 and 300 MHz respectively. Validity of CompF assessed at 60 MHz is ±4.60%, and CompF assessed at 150 MHz is 0.16 MHz. Above 300 MHz, the validity of CompF is not determined in this table.

^E As frequencies below 3 GHz, the validity of tissue parameters (α and σ) can be related to a 10% liquid composition formula is applied to measure S10 values. At frequencies above 3 GHz, the validity of tissue parameters (α and σ) is related to a 10%. The uncertainty is the RMS of the CompF uncertainty for individual target tissue parameters.


^G AlphaDepth are determined during calibration. SRFAD warns that the remaining distance due to the uncertainty when the probe is placed less than ±1% for frequencies below 3 GHz and below ±2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: EX-7767_Oct22

Page 5 of 9

EX3DV4 - SN:7767

October 28, 2022

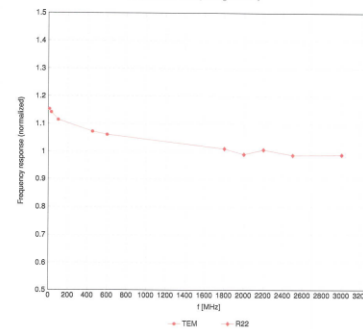Frequency Response of E-Field
(TEM-Cell:01110 EXX, Waveguide:R22)


Uncertainty of Frequency Response of E-Field: ±5.3% (k=2)

Certificate No: EX-7767_Oct22

Page 6 of 9

EX30V4 - SN:7767

October 26, 2022

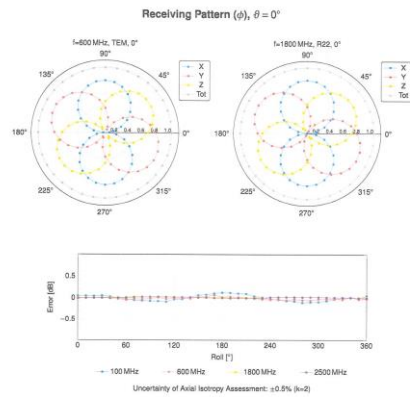


Certificate No: EX-7767_Oct22

Page 7 of 9

EX30V4 - SN:7767

October 26, 2022

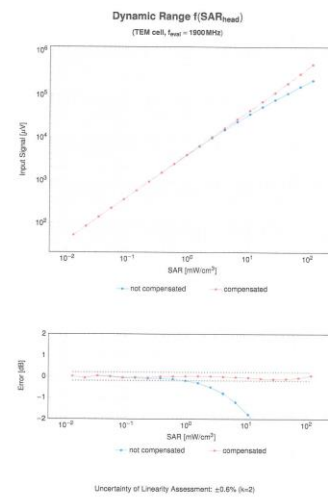


Certificate No: EX-7767_Oct22

Page 8 of 9


EX30V4 - SN:7767

October 26, 2022

Conversion Factor Assessment



Deviation from Isotropy in Liquid



Certificate No: EX-7767_Oct22

Page 9 of 9

4 Impedance and return loss

Dipole CLA150 SN 4025				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2021/4/26	-31.4	/	47.8	/
2022/4/26	-32.5	-3.5%	47.1	0.7
2023/4/26	-32.3	-2.87%	46.5	1.3
Dipole D450V3 SN 1103				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2021/4/21	-23	/	57.1	/
2022/4/26	-23.4	-1.74%	56.6	0.5
2023/4/26	-23.9	-3.91%	56.2	0.9
Dipole D750V3 SN 1188				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/29	-28.7	/	53.6	/
2023/3/29	-28.3	1.39%	53.2	0.4
Dipole D835V2 SN 4d114				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-25.3	/	48.7	/
2023/3/31	-24.6	2.77%	49.1	0.4
Dipole D900V2 SN 1d079				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/7	-23.3	/	48.1	/
2023/6/7	-23.6	-1.29%	48.3	0.2
Dipole D1800V2 SN 2d170				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-29.4	/	47.9	/
2023/3/31	-28.9	1.70%	47.2	0.7
Dipole D1900V2 SN 5d136				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/7	-22.4	/	51.2	/
2023/6/7	-22.9	-2.23%	51.6	-0.4
Dipole D2000V2 SN 1041				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/6	-34.9	/	48.4	/
2023/6/6	-33.5	4.01%	49.1	-0.7
Dipole D2300V2 SN 1096				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$

2022/3/31	-26.6	/	49.2	/
2023/3/31	-27.1	-1.88%	49.4	0.2
Dipole D2450V2 SN 817				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/4/1	-28.5	/	52.1	/
2023/4/1	-28.0	1.75%	51.6	0.5
Dipole D2600V2 SN 1158				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/3/31	-23.8	/	49.9	/
2023/3/31	-23.3	2.10%	50.3	0.4
Dipole D5GHzV2 SN 1095 for 5200				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-23.6	/	46.1	/
2023/6/1	-23.1	2.12%	45.6	0.5
Dipole D5GHzV2 SN 1095 for 5300				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-29.5	/	47.8	/
2023/6/1	-28.8	2.37%	46.9	0.9
Dipole D5GHzV2 SN 1095 for 5500				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-27.4	/	50.3	/
2023/6/1	-27.6	-0.73%	50.8	-0.5
Dipole D5GHzV2 SN 1095 for 5600				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-24.0	/	54.5	/
2023/6/1	-23.6	1.67%	54.9	-0.4
Dipole D5GHzV2 SN 1095 for 5800				
Head Liquid				
Date of Measurement	Return Loss(dB)	Δ %	Impedance (Ω)	$\Delta\Omega$
2022/6/1	-24.9	/	51.5	/
2023/6/1	-24.3	2.41%	51.0	0.5