

Geri-Safe | Medi-Trust GS01


User's Guide

1 Homepage overview


1.1 Main pages (1 & 2 & 3)

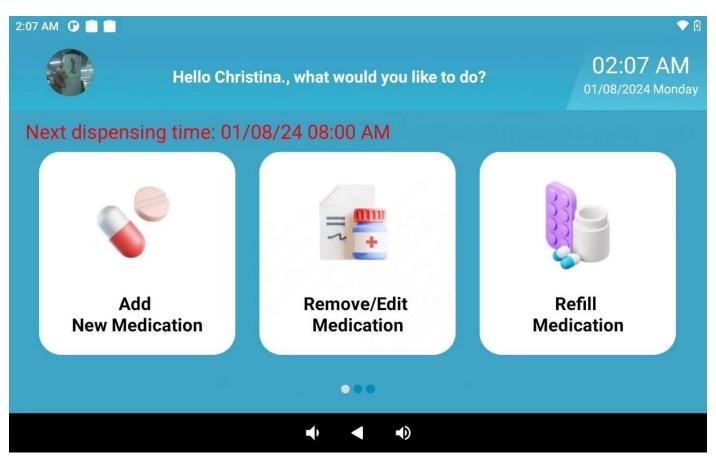

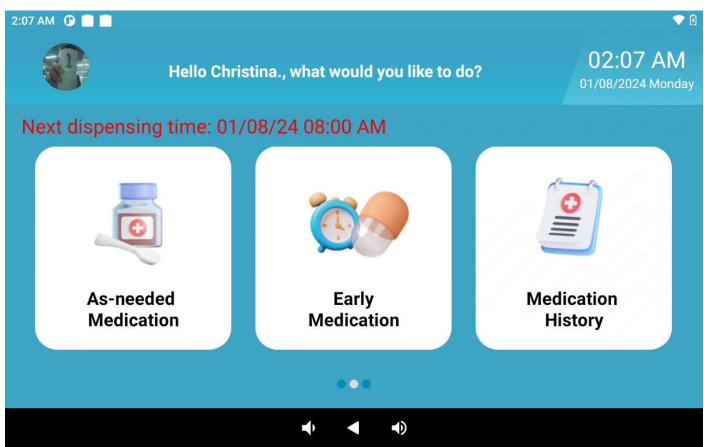


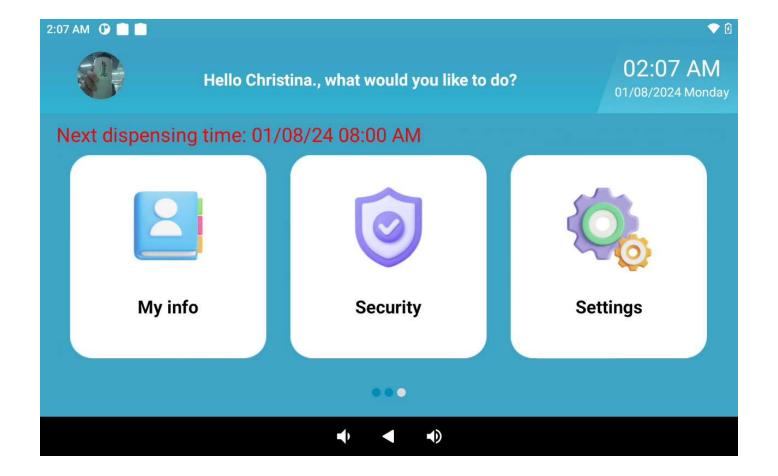


1.2 Verify system time

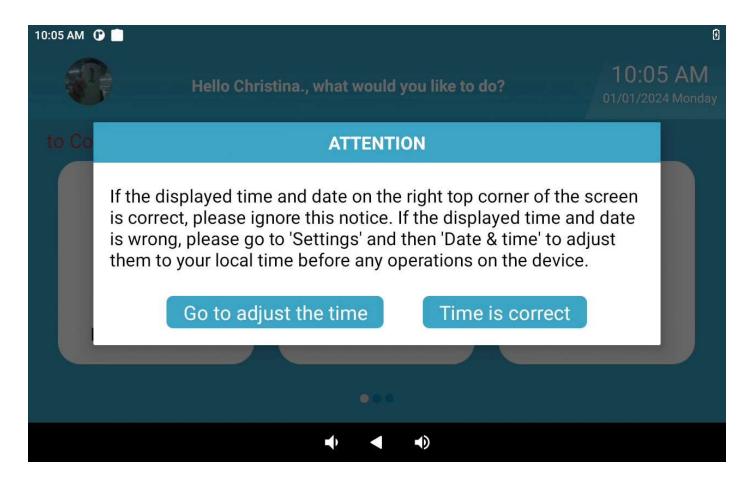


1.3 Pickup medication in advance based on plan

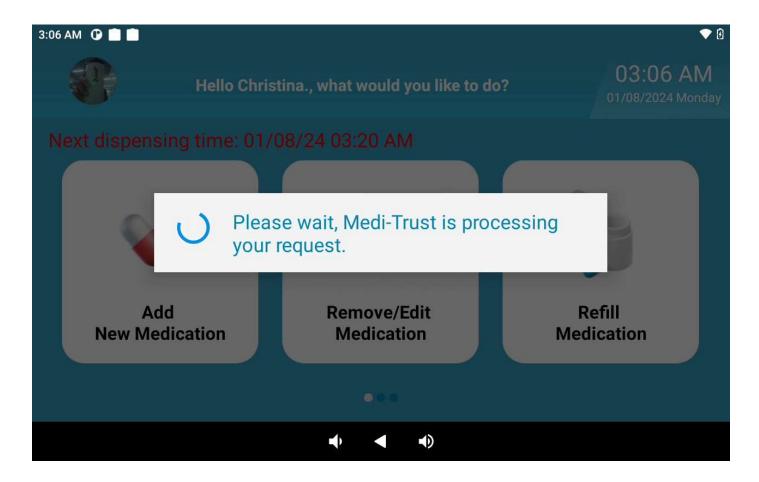


1.4 Waiting for medication

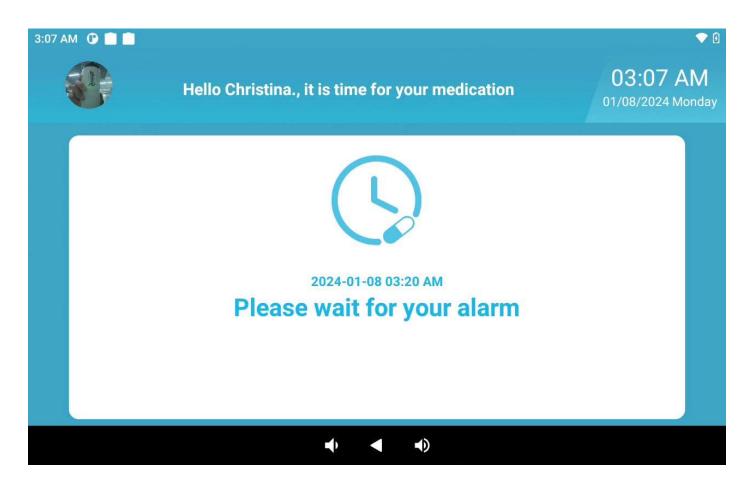


1.5 Fingerprint or password recognition for medication

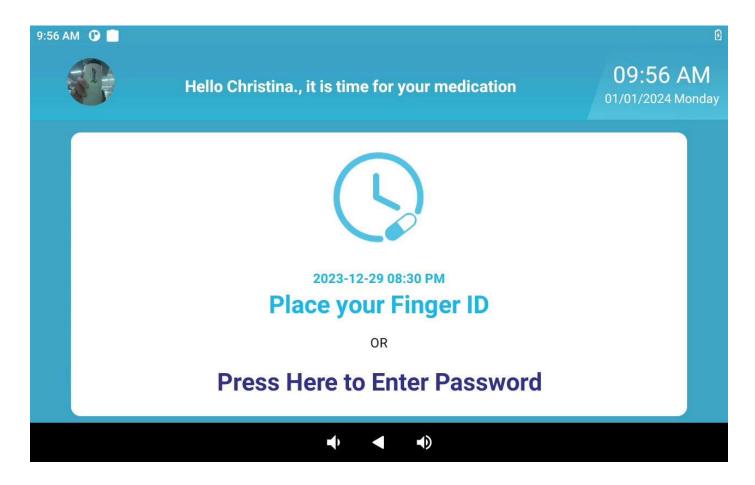


1.6 Reset password

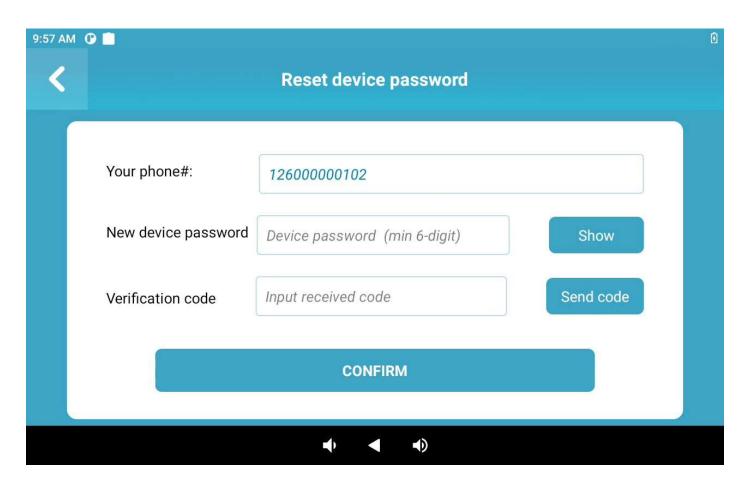

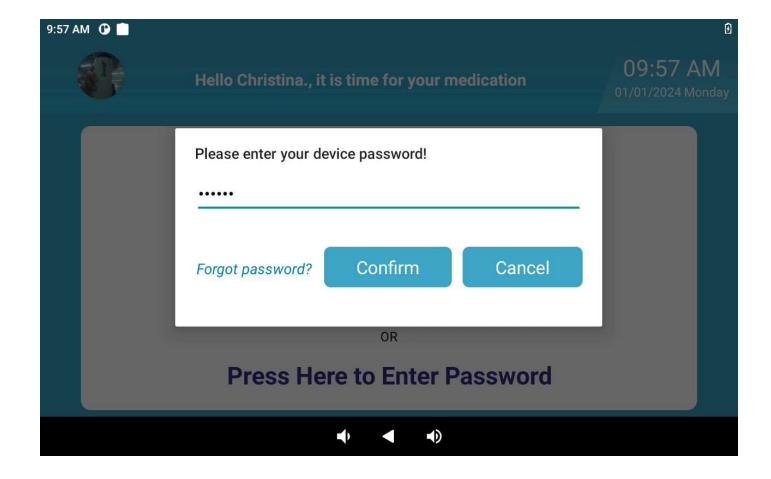


2 Fill in personal information


2.1 contact information

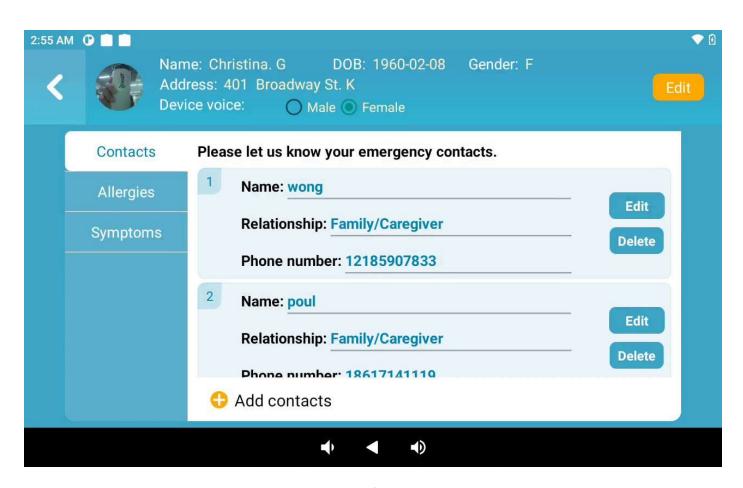


2.2 Fill in related contact persons information

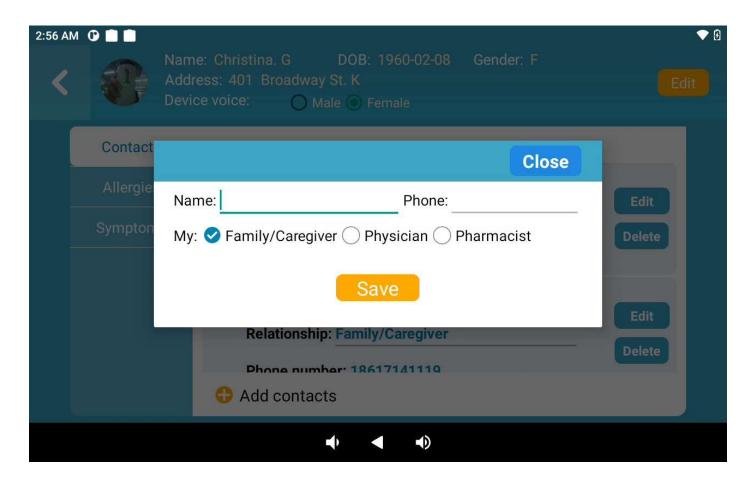

2.3 Fill in allergies information

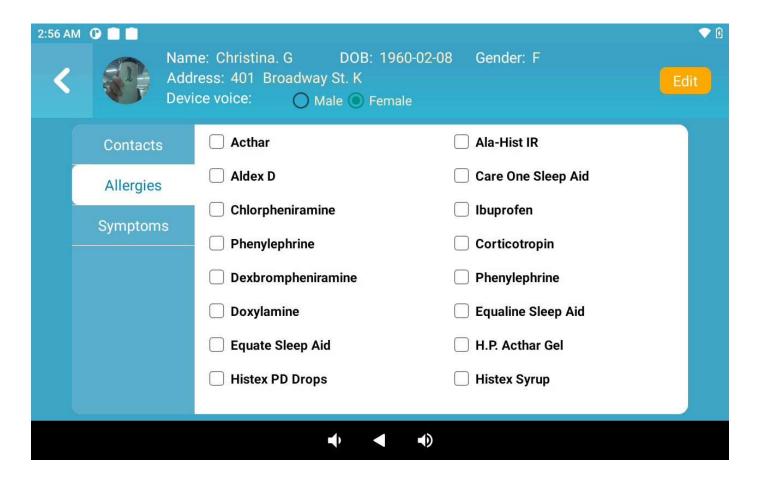


2.4 Fill in symptoms information

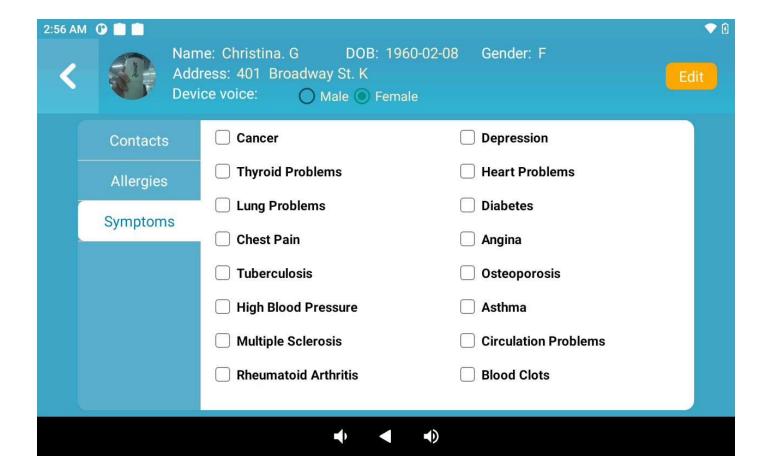


3 Add a new medication


3.1 Fill in medication information

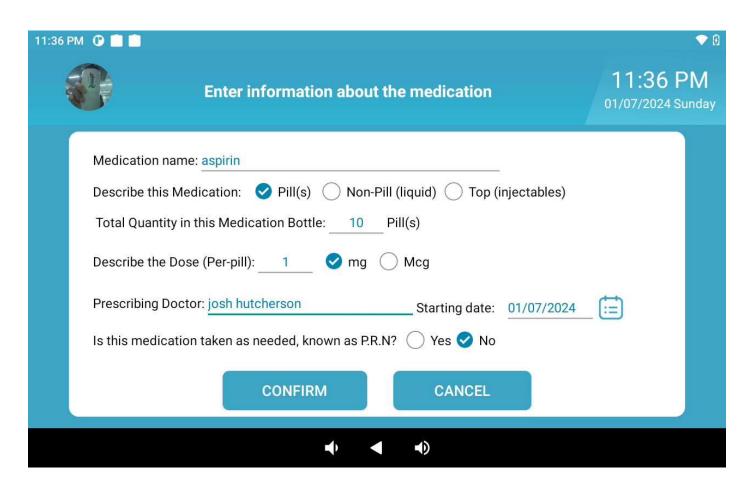


3.2 Fill in a medication plan

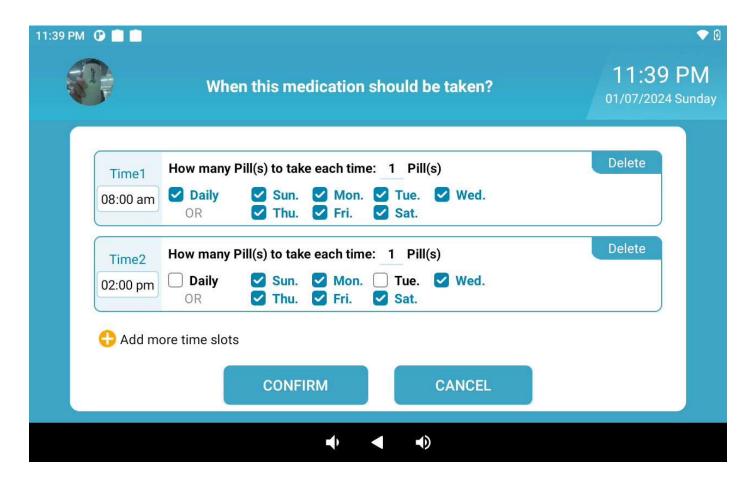


3.3 Send out a medication cup for loading

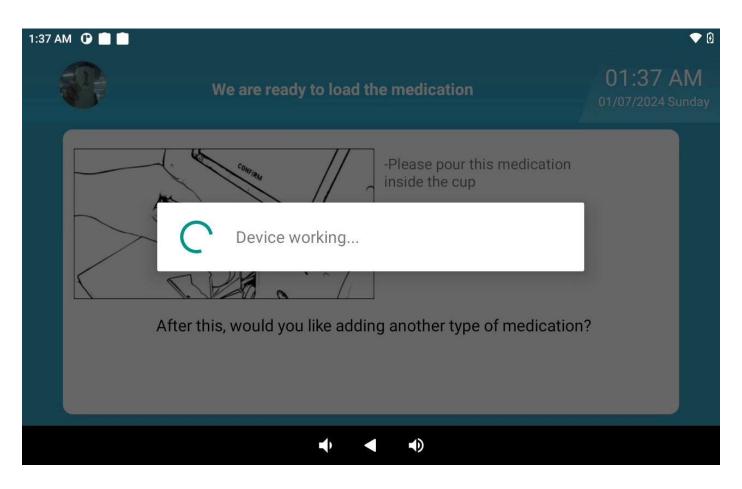


3.4 Taking back the medication cup

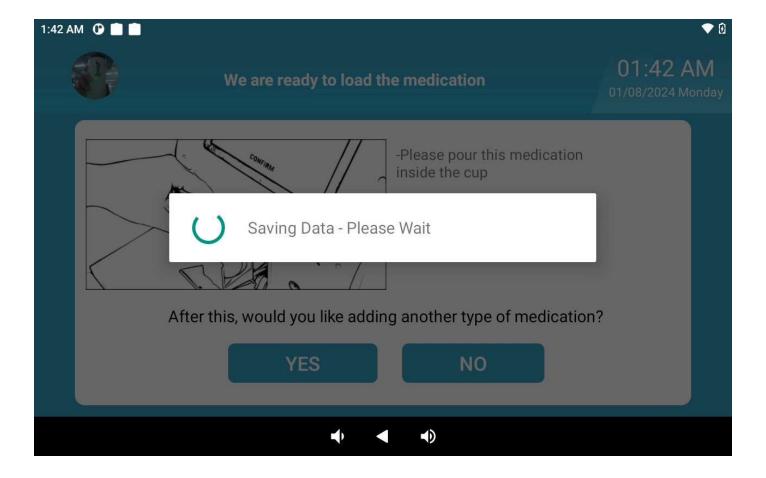


3.5 Loading another medication?

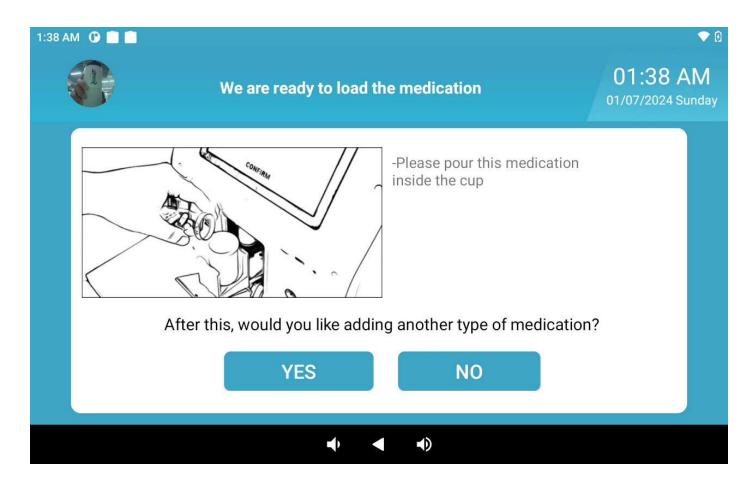


3.6 Loading side bin medication (for liquid or special medications)

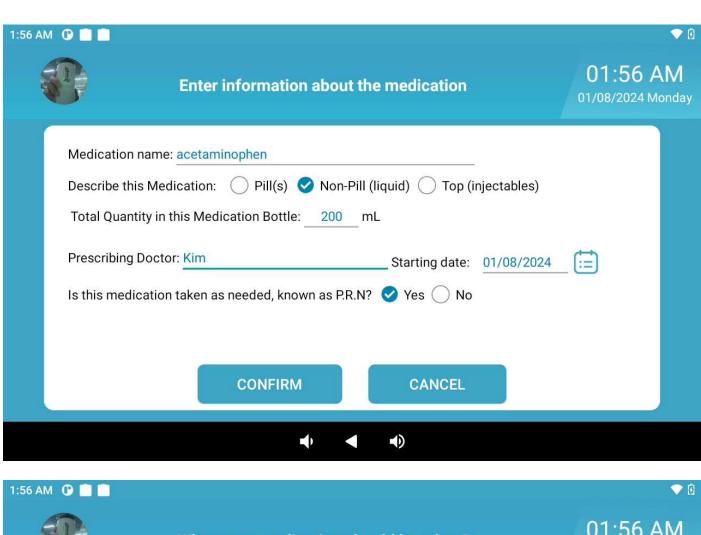


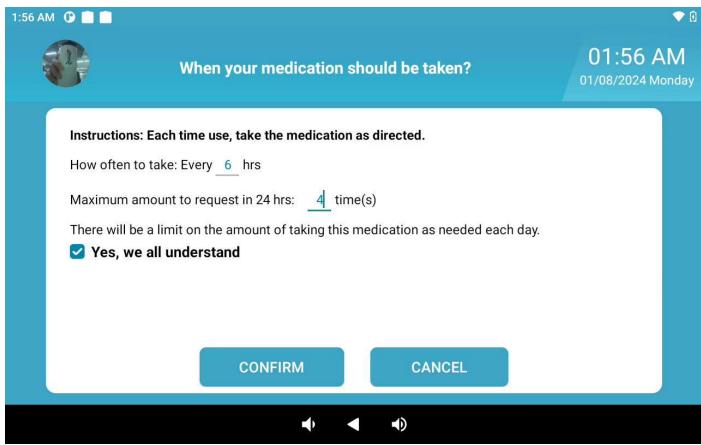

3.7 Loading more medications?

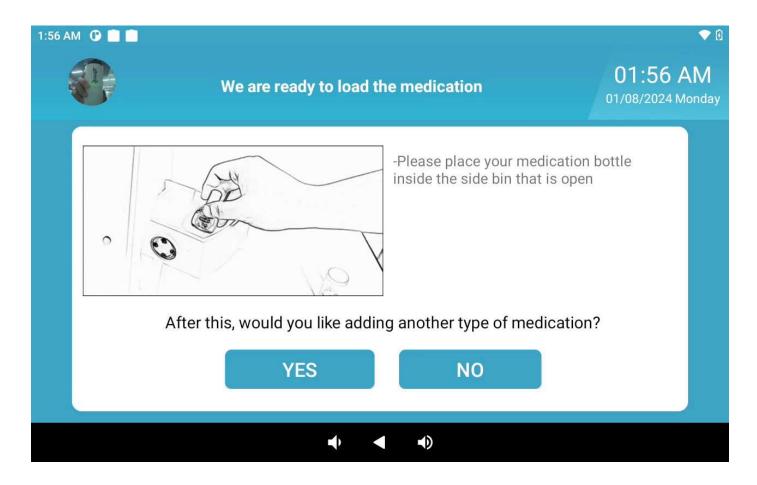


3.8 Loading top bin medication (for liquid or special medications)

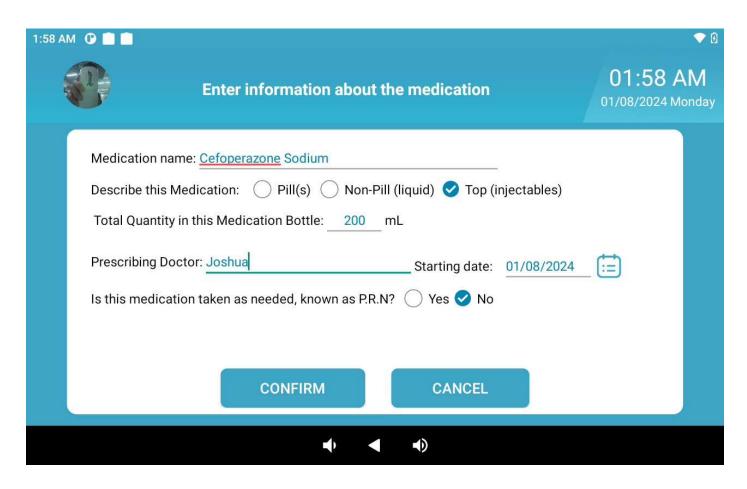


4 Taking medication (including as-needed medications)


4.1 Select a medication (only for as-needed medications)

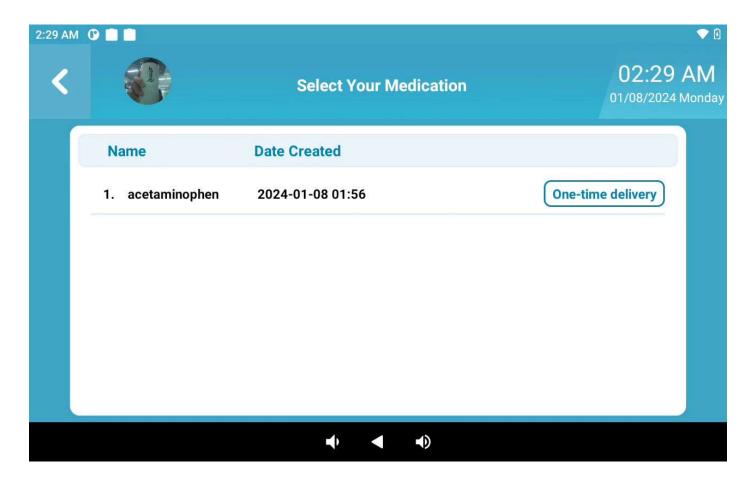


4.2 Pickup and deliver medication accordingly

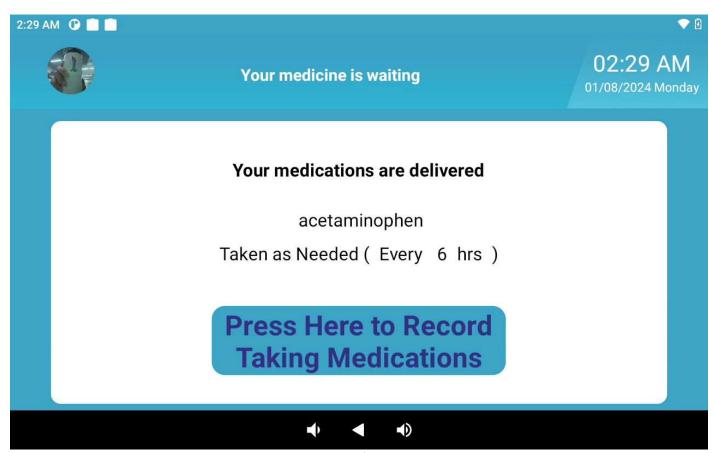


4.3 Taking medication

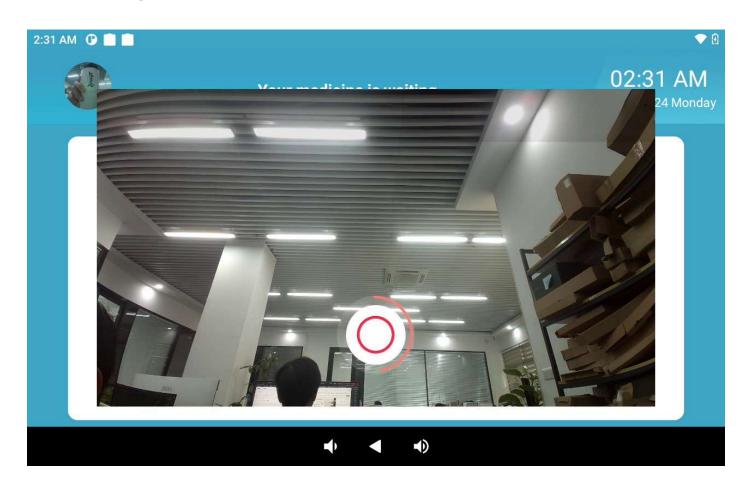


4.4 Taking back the medication cup

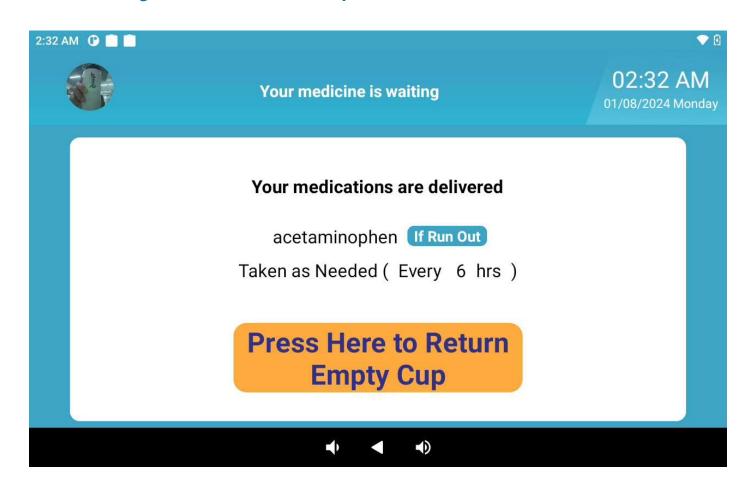

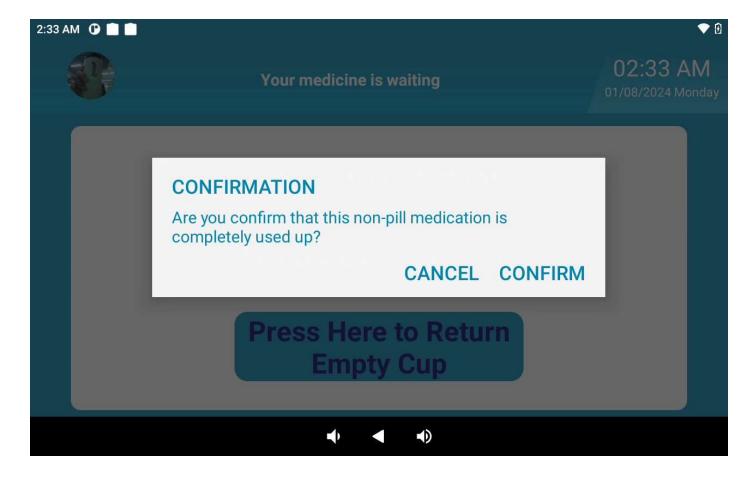


5 Refill medications


5.1 Select a medication for refilling

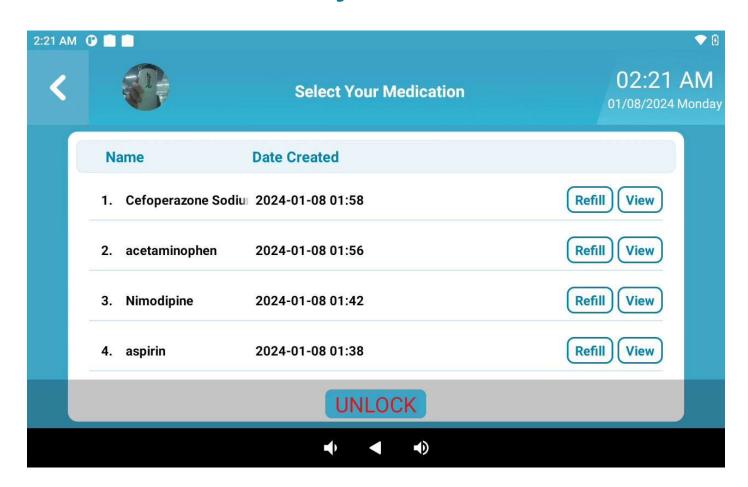


5.2 Password recognition

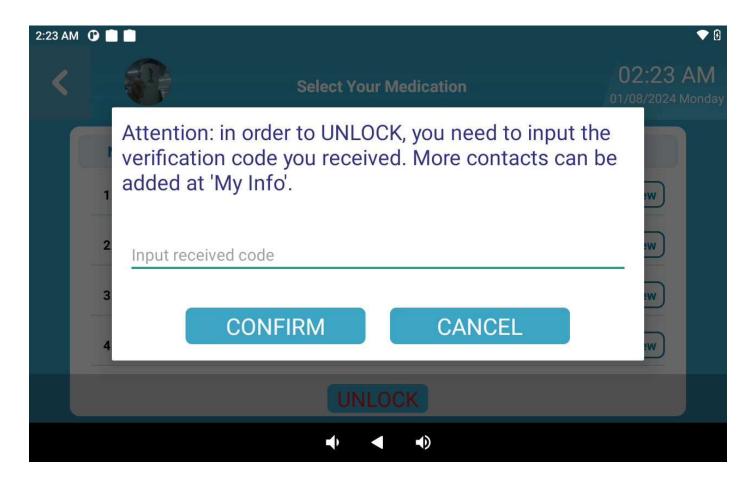


5.3 Password double confirmation

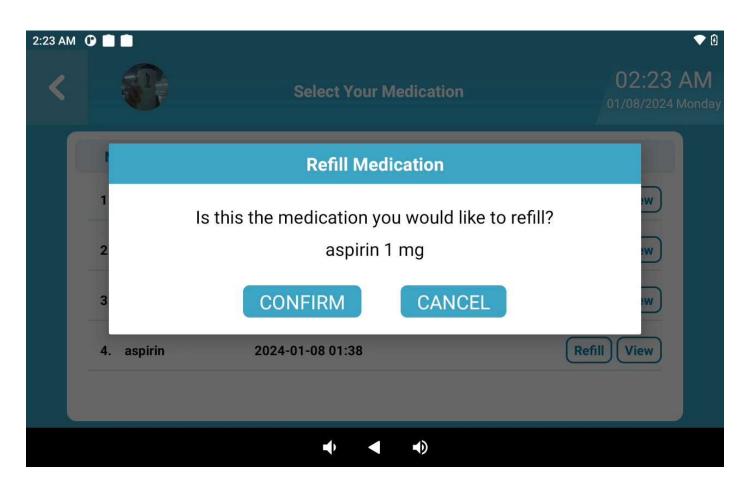


5.4 Deliver the medication cup

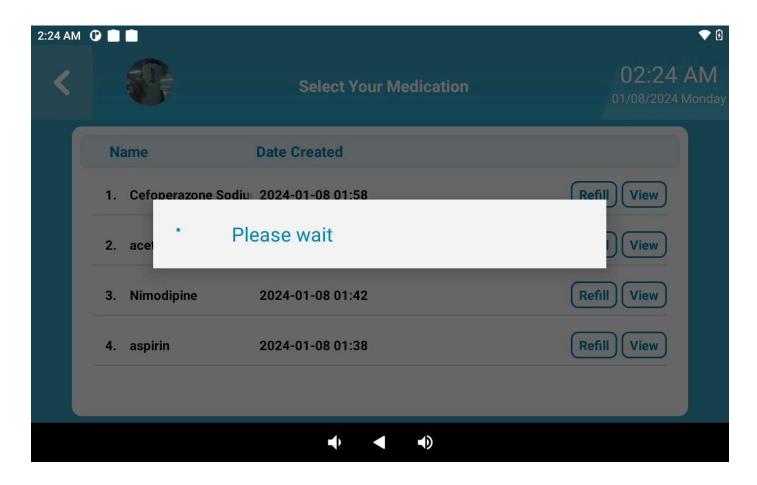


5.5 Fill in refilling quantity

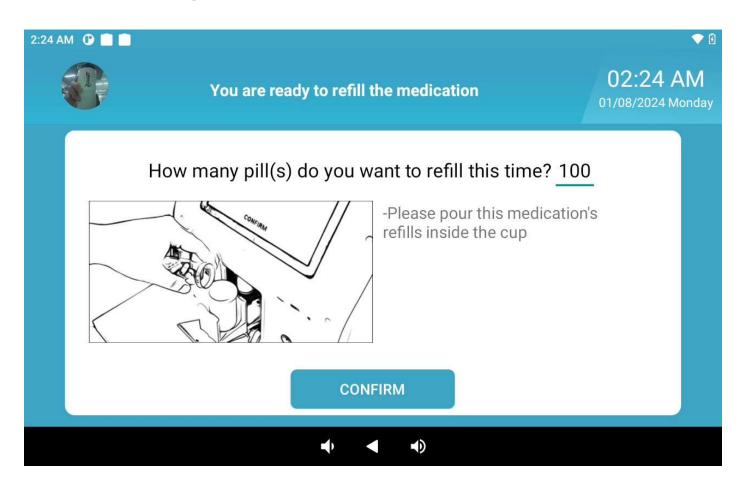


5.6 Double confirm the refilling information

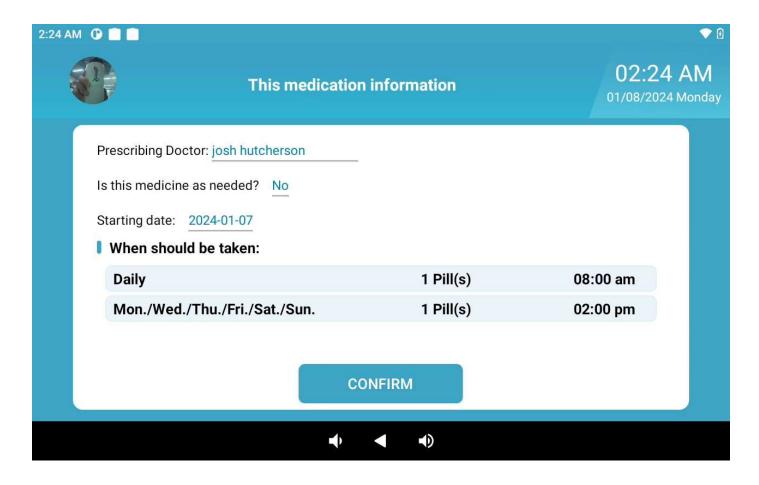

5.7 Take back the refilling medication cup

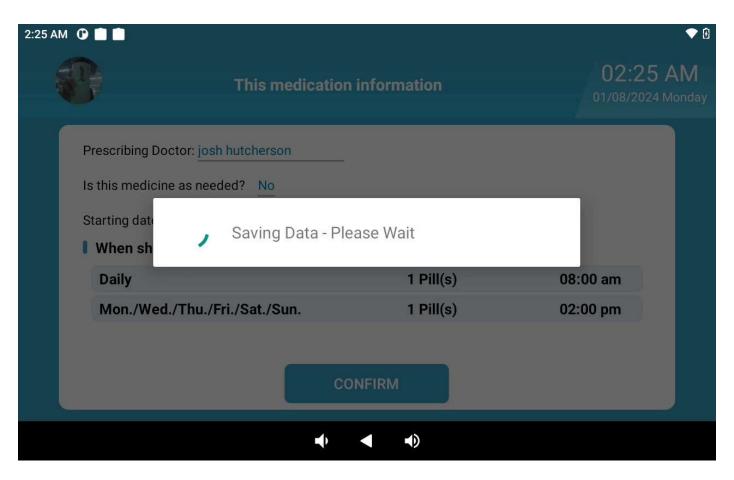


5.8 Confirm the refilling activity

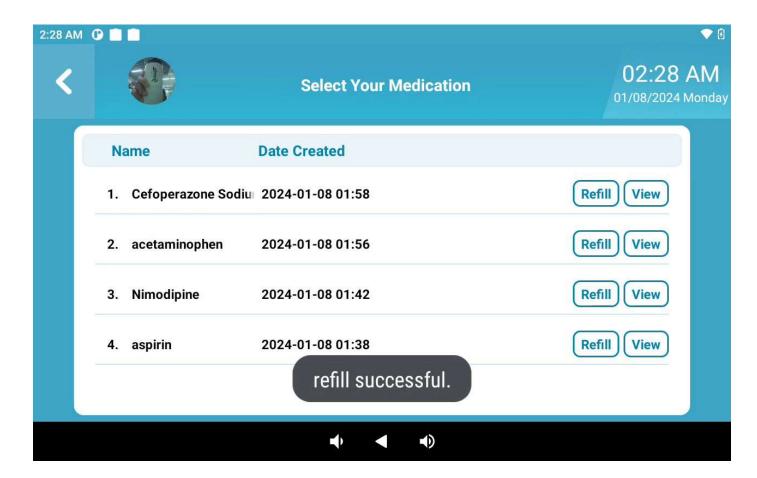


6 Delete for edit a medication


6.1 Unlock first

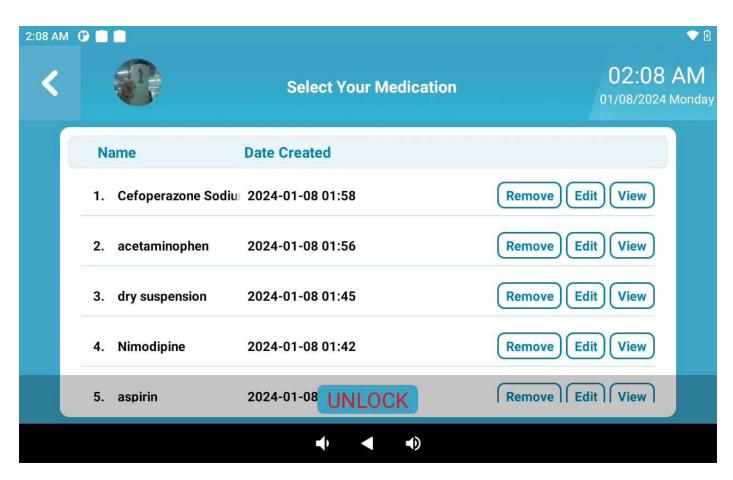


6.2 Input verification code

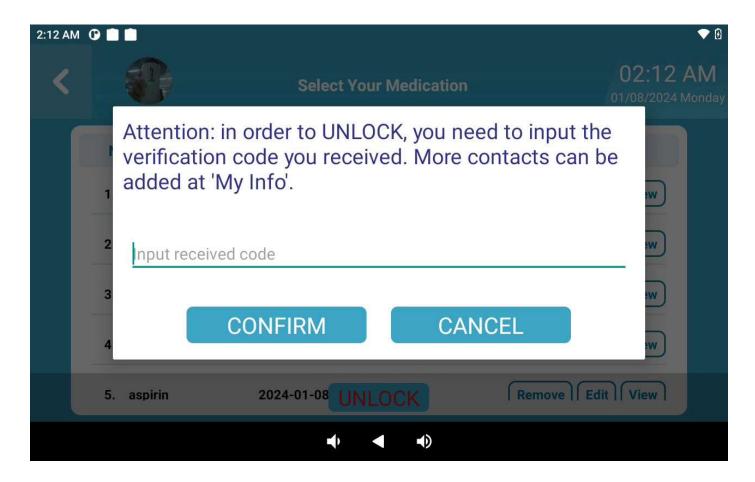


6.3 Select the delegate people

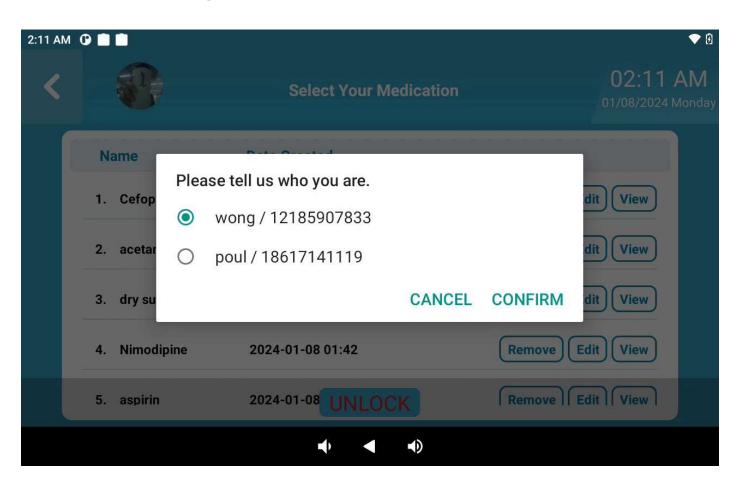


6.4 Confirm to remove the medication

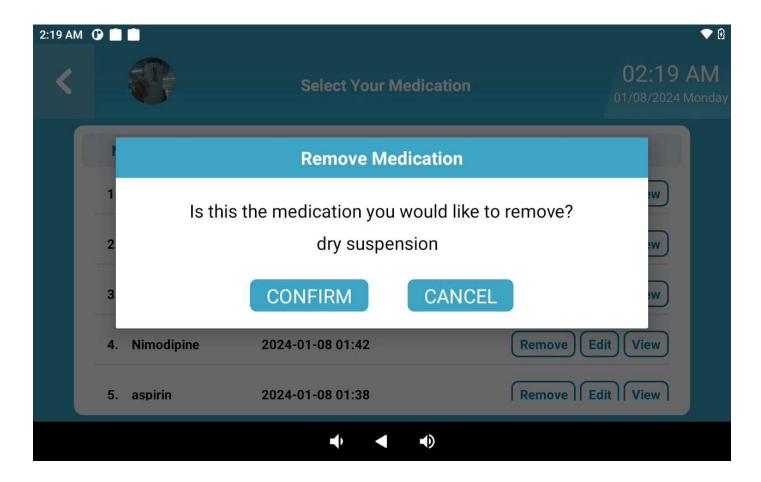


6.5 Double confirm to remove the medication

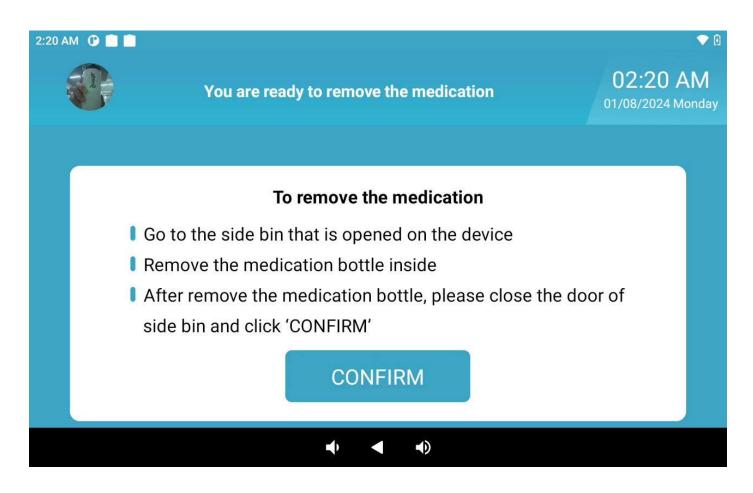


6.6 Re-edit a medication information

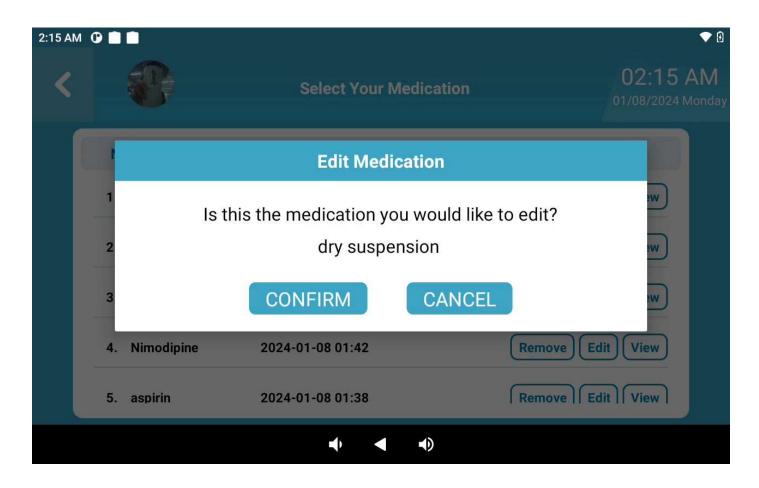


6.7 Re-edit time for a medication

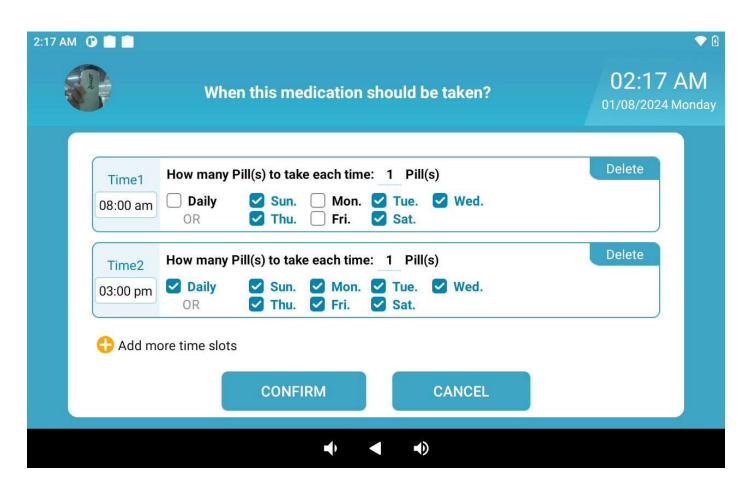

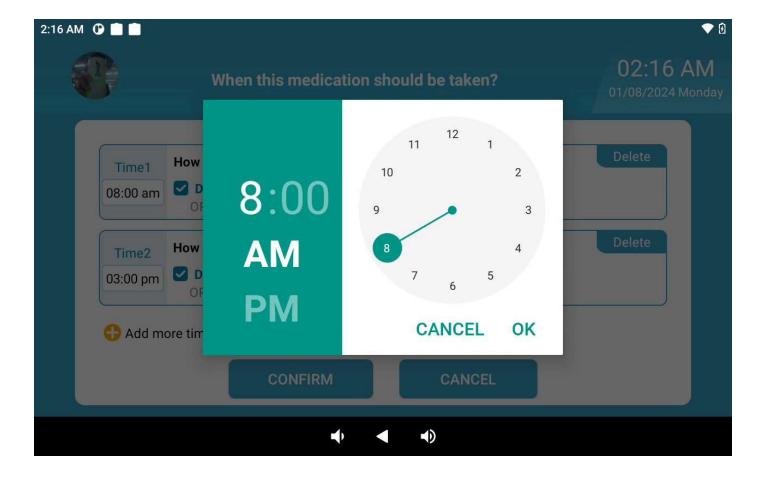



6.8 Check a medication information

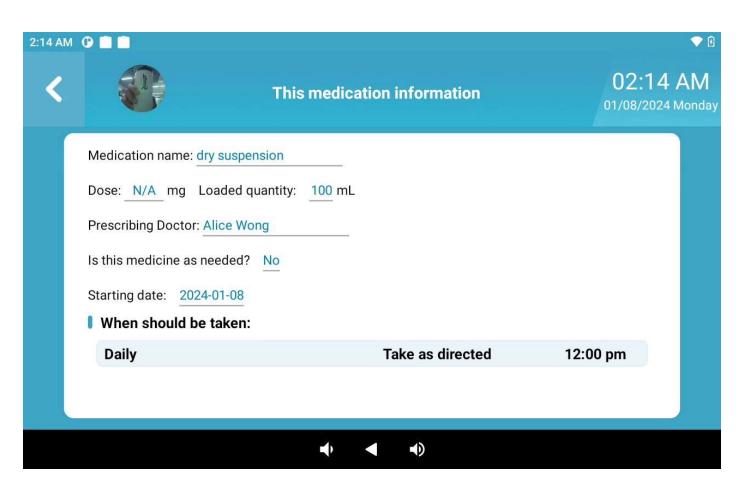


7 Dispense the early medications

7.1 Unlock to take the early medications

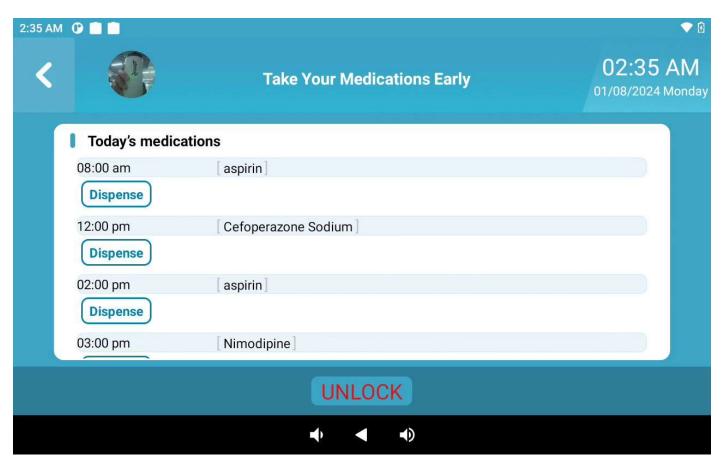


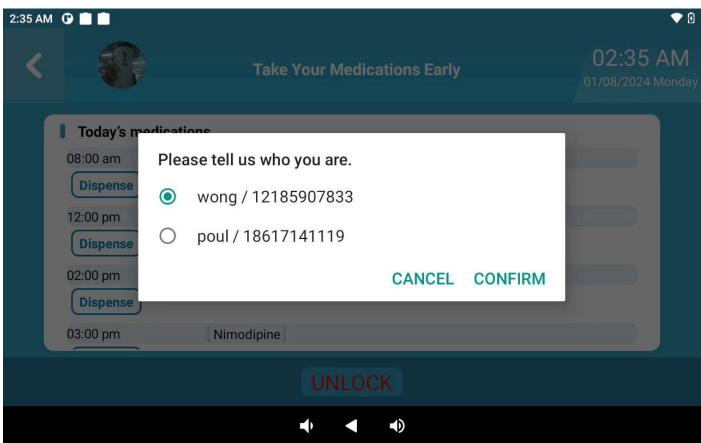


7.2 Select the early medications

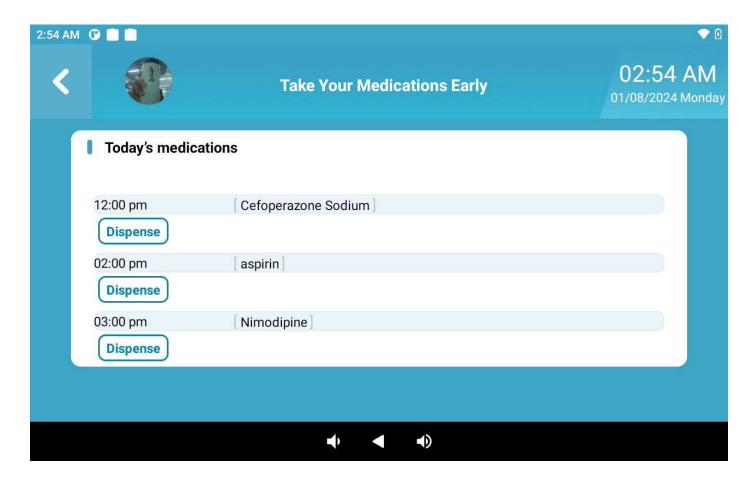


7.3 Taking out the early medications

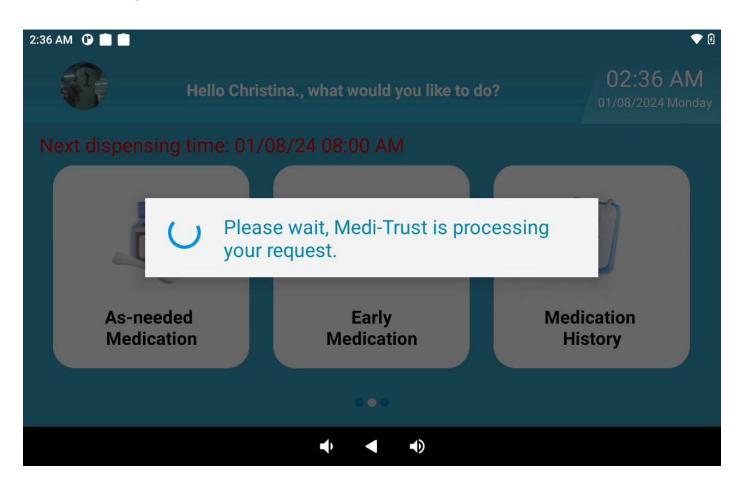


7.4 Password confirmation for the early medications

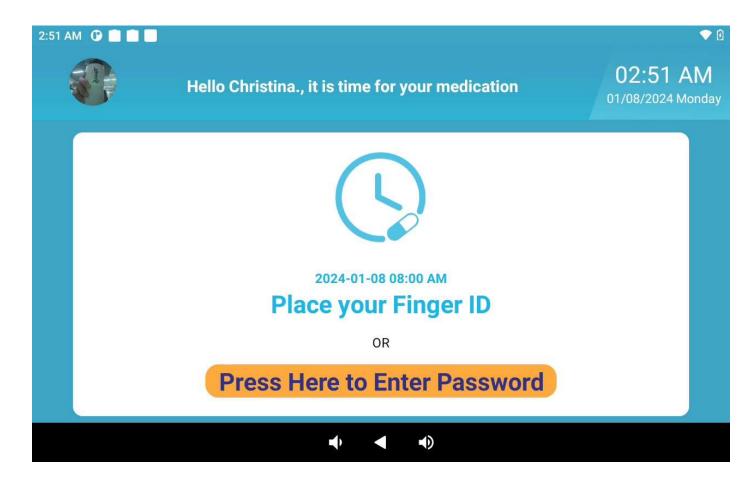


7.5 Delivering out the cup for early medications

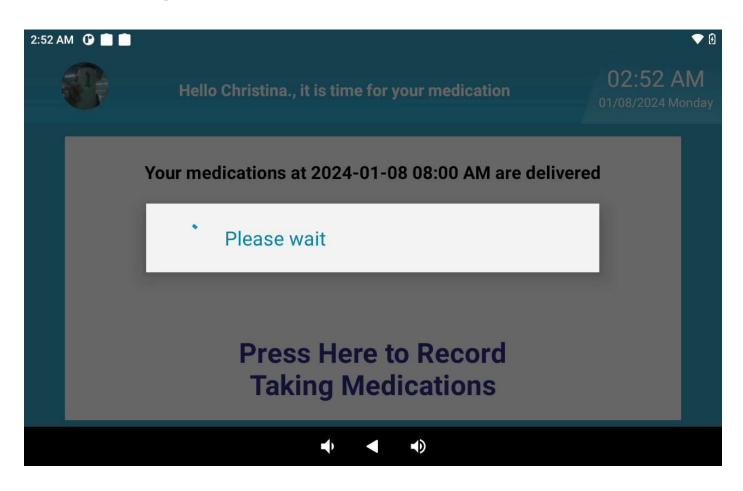


7.6 listing the early medications information

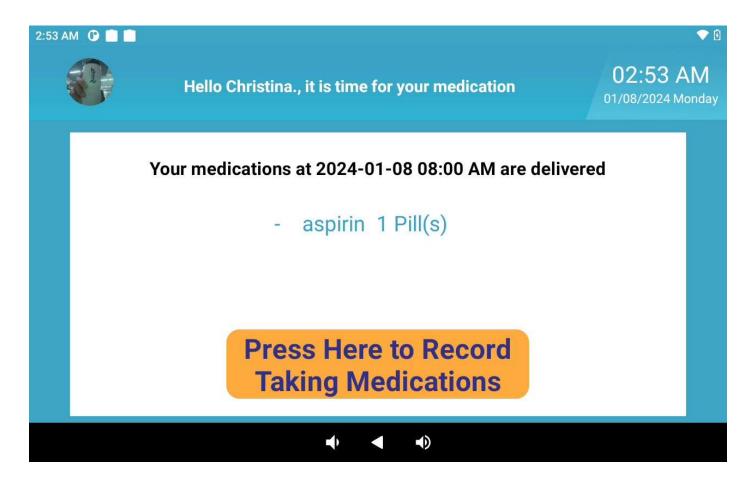


7.7 Taking a video for the early medications

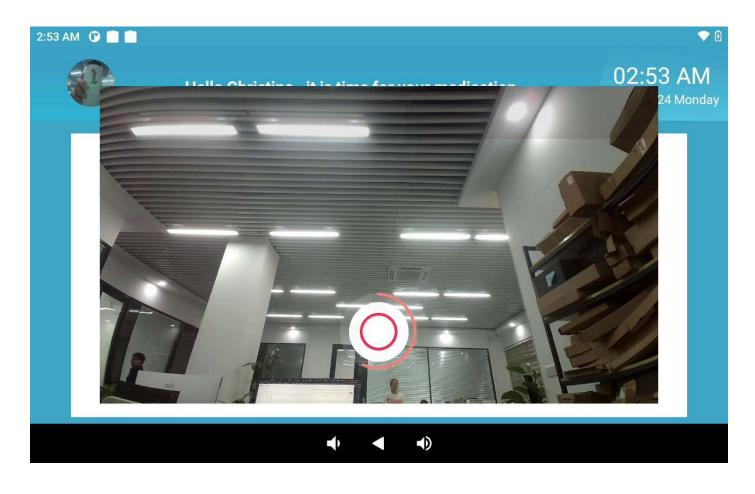

7.8 Taking back the early medications cup

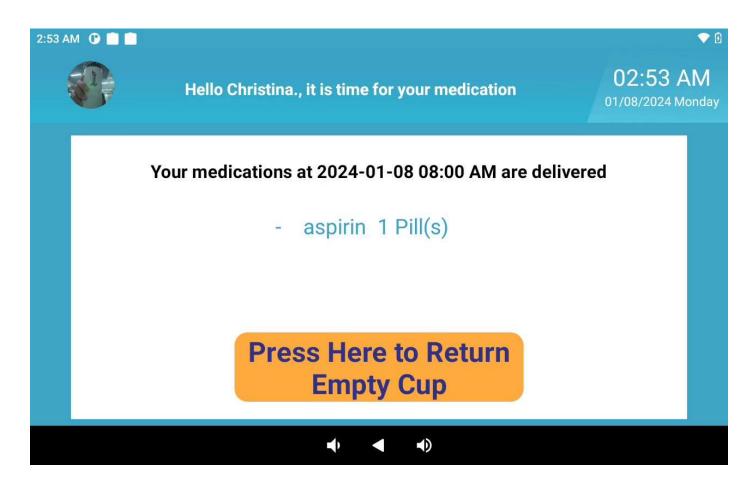


8 View the medications record

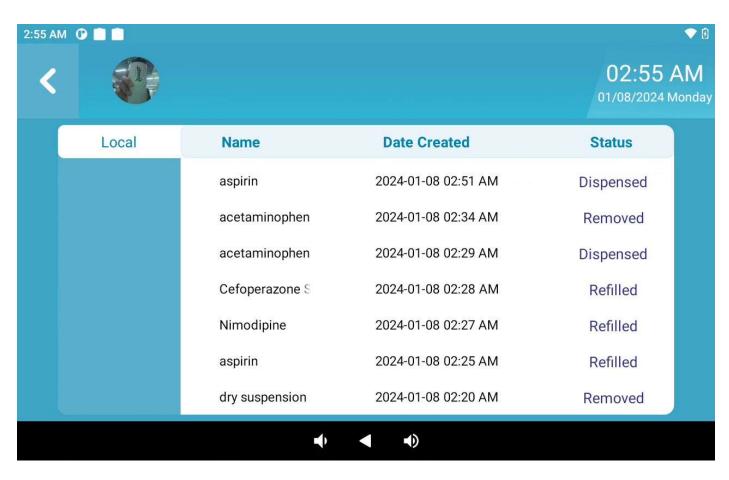



9 Fingerprint recognition and password

9.1 Input a new password

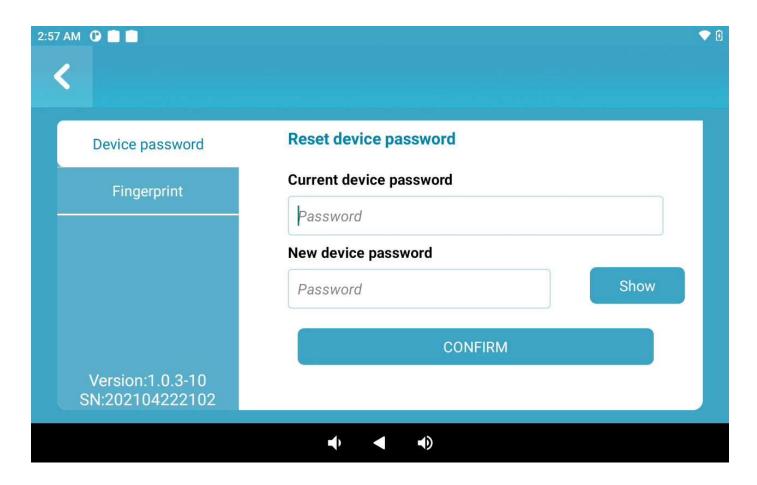


9.2 Add a new fingerprint

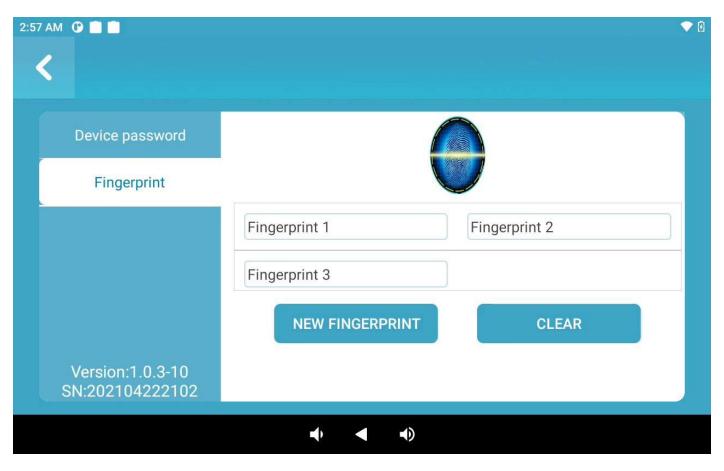


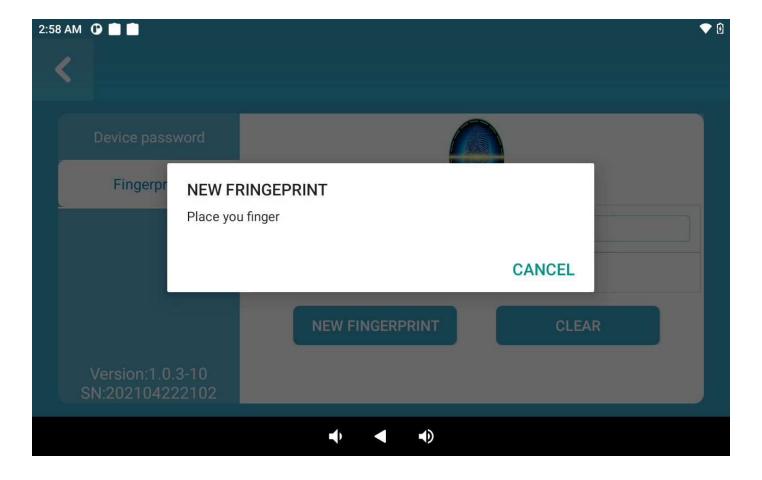


9.3 Input a new fingerprint

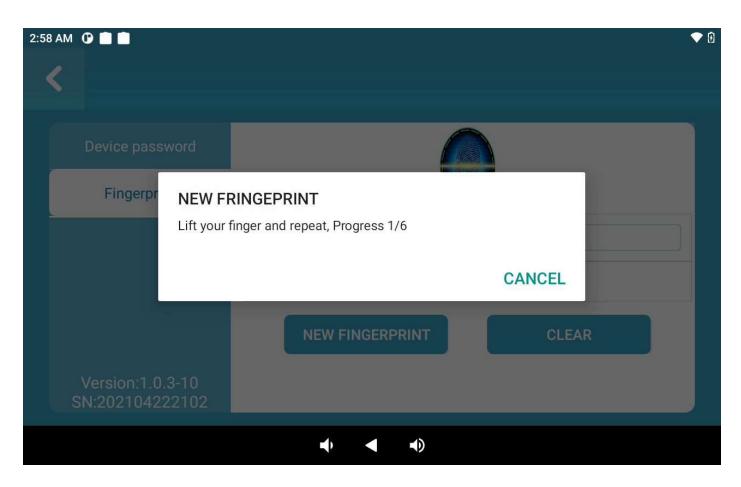

9.4 Success to add a new fingerprint

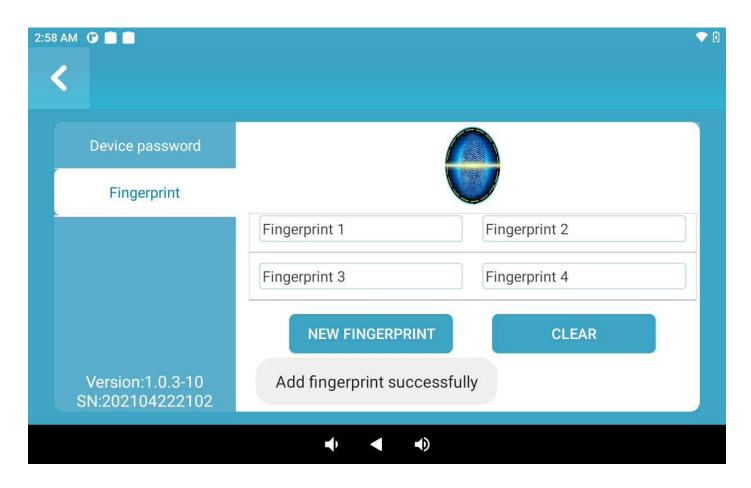


9.5 Delete all fingerprints

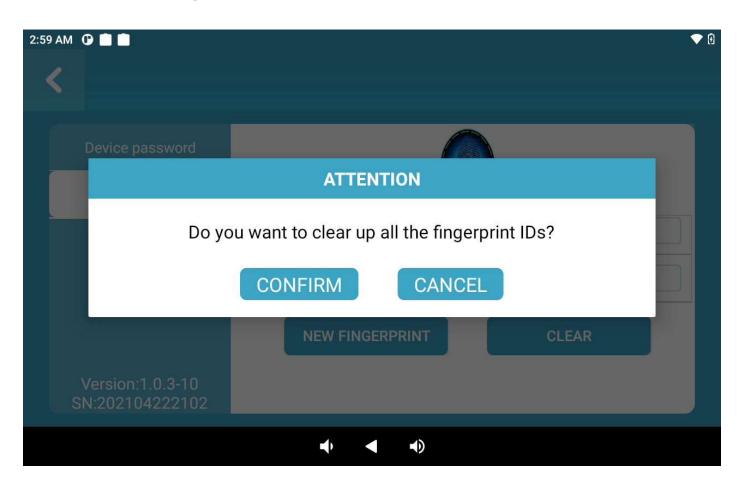


10 System setting


10.1 System setting overview

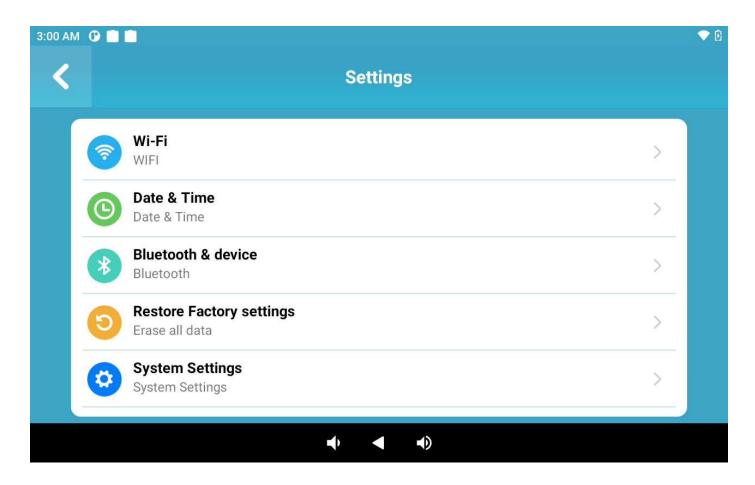

10.2 Date & time setting

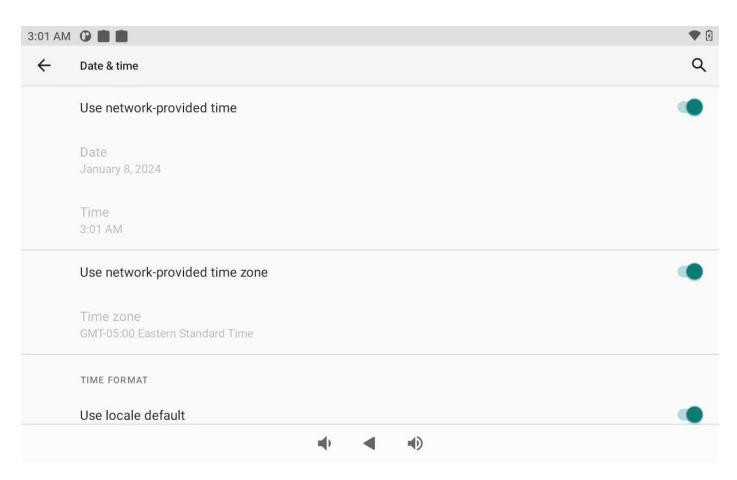

10.3 WiFi setting

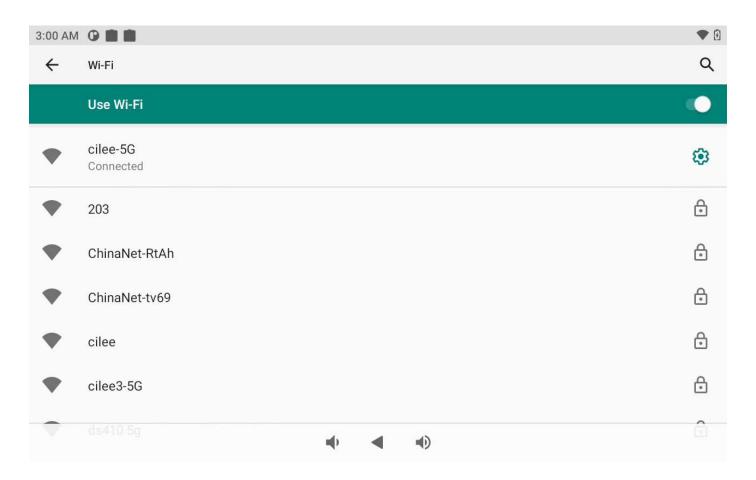

FCC Warning

This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- · Reorient or relocate the receiving antenna.
- · Increase the separation between the equipment and receiver.
- · Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- · Consult the dealer or an experienced radio/TV technician for help.

Radiation Exposure Statement

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment. This equipment should be installed and operated with minimum distance 20cm between the radiator and your body.