



## COMOSAR E-Field Probe Calibration Report

Ref : ACR.193.11.24.BES.B

Cancel and replace the report ACR.193.11.24.BES.A

### **WALTEK TESTING GROUP (SHENZHEN) CO., LTD**

**1/F., ROOM 101, BUILDING 1, HONGWEI INDUSTRIAL  
PARK, LIUXIAN 2ND ROAD, BLOCK 70 BAO'AN DISTRICT,  
SHENZHEN, GUANGDONG, 518101 CHINA**

### **MVG COMOSAR DOSIMETRIC E-FIELD PROBE**

**SERIAL NO.: 3823-EPGO-435**

**Calibrated at MVG**

**Z.I. de la pointe du diable**

**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**

**29280 PLOUZANE - FRANCE**

**Calibration date: 07/11/2024**



Accreditations #2-6789  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

#### **Summary:**

This document presents the method and results from an accredited COMOSAR Dosimetric E-Field Probe calibration performed at MVG, using the CALIPROBE test bench, for use with a MVG COMOSAR system only. The test results covered by accreditation are traceable to the International System of Units (SI).



|                                   | <i>Name</i>  | <i>Function</i>         | <i>Date</i>     | <i>Signature</i>                                                                             |
|-----------------------------------|--------------|-------------------------|-----------------|----------------------------------------------------------------------------------------------|
| <i>Prepared by :</i>              | Pedro Ruiz   | Measurement Responsible | 7/30/2024       |           |
| <i>Checked &amp; approved by:</i> | Jérôme Luc   | Technical Manager       | 7/11/2024       |           |
| <i>Authorized by:</i>             | Yann Toutain | Laboratory Director     | Yann Toutain ID | <div>Signature numérique de Yann<br/>Toutain ID<br/>Date : 2024.07.31 10:15:14 +02'00'</div> |

|                       | <i>Customer Name</i>                              |
|-----------------------|---------------------------------------------------|
| <i>Distribution :</i> | WALTEK<br>TESTING GROUP<br>(SHENZHEN) CO.,<br>LTD |

| <i>Issue</i> | <i>Name</i>   | <i>Date</i> | <i>Modifications</i> |
|--------------|---------------|-------------|----------------------|
| A            | Cyrille ONNEE | 7/11/2024   | Initial release      |
| B            | Pedro Ruiz    | 7/30/2024   | Customer info update |
|              |               |             |                      |
|              |               |             |                      |



## TABLE OF CONTENTS

|     |                                 |   |
|-----|---------------------------------|---|
| 1   | Device Under Test .....         | 4 |
| 2   | Product Description .....       | 4 |
| 2.1 | General Information .....       | 4 |
| 3   | Measurement Method .....        | 4 |
| 3.1 | Sensitivity .....               | 4 |
| 3.2 | Linearity .....                 | 5 |
| 3.3 | Isotropy .....                  | 5 |
| 3.4 | Boundary Effect .....           | 5 |
| 3.5 | Probe Modulation Response ..... | 6 |
| 4   | Measurement Uncertainty .....   | 6 |
| 5   | Calibration Results .....       | 6 |
| 5.1 | Calibration in air .....        | 6 |
| 5.2 | Calibration in liquid .....     | 7 |
| 6   | Verification Results .....      | 8 |
| 7   | List of Equipment .....         | 9 |

## 1 DEVICE UNDER TEST

| Device Under Test                        |                                                                                                                   |
|------------------------------------------|-------------------------------------------------------------------------------------------------------------------|
| Device Type                              | COMOSAR DOSIMETRIC E FIELD PROBE                                                                                  |
| Manufacturer                             | MVG                                                                                                               |
| Model                                    | SSE2                                                                                                              |
| Serial Number                            | 3823-EPGO-435                                                                                                     |
| Product Condition (new / used)           | New                                                                                                               |
| Frequency Range of Probe                 | 0.15 GHz-7.5GHz                                                                                                   |
| Resistance of Three Dipoles at Connector | Dipole 1: $R1=0.189\text{ M}\Omega$<br>Dipole 2: $R2=0.212\text{ M}\Omega$<br>Dipole 3: $R3=0.216\text{ M}\Omega$ |

## 2 PRODUCT DESCRIPTION

### 2.1 GENERAL INFORMATION

MVG's COMOSAR E field Probes are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards.



**Figure 1 – MVG COMOSAR Dosimetric E field Probe**

|                                            |        |
|--------------------------------------------|--------|
| Probe Length                               | 330 mm |
| Length of Individual Dipoles               | 2 mm   |
| Maximum external diameter                  | 8 mm   |
| Probe Tip External Diameter                | 2.5 mm |
| Distance between dipoles / probe extremity | 1 mm   |

## 3 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide recommended practices for the probe calibrations, including the performance characteristics of interest and methods by which to assess their effect. All calibrations / measurements performed meet the fore-mentioned standards.

### 3.1 SENSITIVITY

The sensitivity factors of the three dipoles were determined using a two step calibration method (air and tissue simulating liquid) using waveguides as outlined in the standards for frequency range 600-7500MHz and using the calorimeter cell method (transfer method) as outlined in the standards for frequency 150-450 MHz.

### 3.2 LINEARITY

The evaluation of the linearity was done in free space using the waveguide, performing a power sweep to cover the SAR range 0.01W/kg to 100W/kg.

### 3.3 ISOTROPY

The axial isotropy was evaluated by exposing the probe to a reference wave from a standard dipole with the dipole mounted under the flat phantom in the test configuration suggested for system validations and checks. The probe was rotated along its main axis from 0 to 360 degrees in 15-degree steps. The hemispherical isotropy is determined by inserting the probe in a thin plastic box filled with tissue-equivalent liquid, with the plastic box illuminated with the fields from a half wave dipole. The dipole is rotated about its axis (0°–180°) in 15° increments. At each step the probe is rotated about its axis (0°–360°).

### 3.4 BOUNDARY EFFECT

The boundary effect is defined as the deviation between the SAR measured data and the expected exponential decay in the liquid when the probe is oriented normal to the interface. To evaluate this effect, the liquid filled flat phantom is exposed to fields from either a reference dipole or waveguide. With the probe normal to the phantom surface, the peak spatial average SAR is measured and compared to the analytical value at the surface.

The boundary effect uncertainty can be estimated according to the following uncertainty approximation formula based on linear and exponential extrapolations between the surface and  $d_{be} + d_{step}$  along lines that are approximately normal to the surface:

$$SAR_{uncertainty} [\%] = \Delta SAR_{be} \frac{(d_{be} + d_{step})^2}{2d_{step}} \frac{(e^{-d_{be}/\delta})}{\delta/2} \quad \text{for } (d_{be} + d_{step}) < 10 \text{ mm}$$

where

|                     |                                                                                                                                                                                                      |
|---------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| $SAR_{uncertainty}$ | is the uncertainty in percent of the probe boundary effect                                                                                                                                           |
| $d_{be}$            | is the distance between the surface and the closest <i>zoom-scan</i> measurement point, in millimetre                                                                                                |
| $\Delta_{step}$     | is the separation distance between the first and second measurement points that are closest to the phantom surface, in millimetre, assuming the boundary effect at the second location is negligible |
| $\delta$            | is the minimum penetration depth in millimetres of the head tissue-equivalent liquids defined in this standard, i.e., $\delta \approx 14 \text{ mm}$ at 3 GHz;                                       |
| $\Delta SAR_{be}$   | in percent of SAR is the deviation between the measured SAR value, at the distance $d_{be}$ from the boundary, and the analytical SAR value.                                                         |

The measured worst case boundary effect  $SAR_{uncertainty}[\%]$  for scanning distances larger than 4mm is 1.0% Limit ,2%).

### 3.5 PROBE MODULATION RESPONSE

MVG's probe were evaluated experimentally with various modulated signal and the deviation from CW response were found neglectable in the used power range of the probe. So the correction to taking into account the linearization parameters for different modulation is null, therefore the CW factor given in this report can be used whatever the measured modulation

## 4 MEASUREMENT UNCERTAINTY

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty associated with a SAR probe calibration using the waveguide or calorimetric cell technique depending on the frequency.

The estimated expanded uncertainty (k=2) in calibration for SAR (W/kg) is +/-11% for the frequency range 150-450MHz.


The estimated expanded uncertainty (k=2) in calibration for SAR (W/kg) is +/-14% for the frequency range 600-7500MHz.

## 5 CALIBRATION RESULTS

| Ambient condition  |             |
|--------------------|-------------|
| Liquid Temperature | 20 +/- 1 °C |
| Lab Temperature    | 20 +/- 1 °C |
| Lab Humidity       | 30-70 %     |

### 5.1 CALIBRATION IN AIR

The following curve represents the measurement in waveguide of the voltage picked up by the probe toward the E-field generated inside the waveguide.

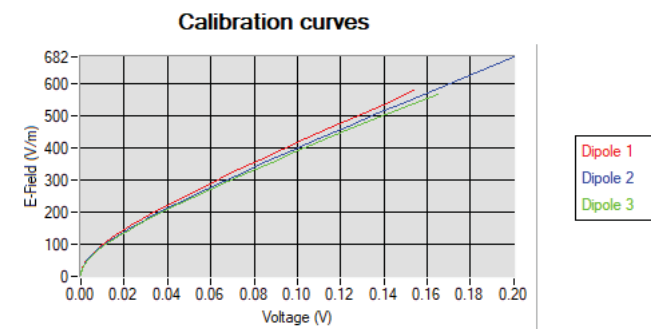

From this curve, the sensitivity in air is calculated using the below formula.

$$E^2 = \sum_{i=1}^3 \frac{V_i (1 + V_i / DCP_i)}{Norm_i}$$

where

$V_i$ =voltage readings on the 3 channels of the probe

DCPi=diode compression point given below for the 3 channels of the probe

Normi=dipole sensitivity given below for the 3 channels of the probe

| Normx dipole<br>1 ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) | Normy dipole<br>2 ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) | Normz dipole<br>3 ( $\mu\text{V}/(\text{V}/\text{m})^2$ ) |
|-----------------------------------------------------------|-----------------------------------------------------------|-----------------------------------------------------------|
| 1.11                                                      | 1.18                                                      | 1.22                                                      |

| DCP dipole 1<br>(mV) | DCP dipole 2<br>(mV) | DCP dipole 3<br>(mV) |
|----------------------|----------------------|----------------------|
| 112                  | 115                  | 120                  |

## 5.2 CALIBRATION IN LIQUID

The calorimeter cell or the waveguide is used to determine the calibration in liquid using the formula below.

$$ConvF = \frac{E_{liquid}^2}{E_{air}^2}$$

The E-field in the liquid is determined from the SAR measurement according to the below formula.

$$E_{liquid}^2 = \frac{\rho SAR}{\sigma}$$

where

$\sigma$ =the conductivity of the liquid

$\rho$ =the volumetric density of the liquid

SAR=the SAR measured from the formula that depends on the setup used. The SAR formulas are given below

For the calorimeter cell (150-450 MHz), the formula is:

$$SAR = c \frac{dT}{dt}$$

where

$c$ =the specific heat for the liquid

$dT/dt$ =the temperature rises over the time

For the waveguide setup (600-75000 MHz), the formula is:

$$SAR = \frac{4P_W}{ab\delta} e^{-\frac{2z}{\delta}}$$

where

a=the larger cross-sectional of the waveguide

b=the smaller cross-sectional of the waveguide



$\delta$ =the skin depth for the liquid in the waveguide

Pw=the power delivered to the liquid

The below table summarize the ConvF for the calibrated liquid. The curves give examples for the measured SAR depending on the voltage in some liquid.


| Liquid | Frequency (MHz*) | ConvF |
|--------|------------------|-------|
| HL750  | 750              | 1.27  |
| HL850  | 835              | 1.28  |
| HL1800 | 1800             | 1.37  |
| HL2000 | 2000             | 1.50  |
| HL2300 | 2300             | 1.54  |
| HL2450 | 2450             | 1.62  |
| HL2600 | 2600             | 1.50  |
| HL3300 | 3300             | 1.31  |
| HL3500 | 3500             | 1.28  |
| HL3700 | 3700             | 1.25  |
| HL3900 | 3900             | 1.21  |
| HL4100 | 4100             | 1.15  |
| HL5200 | 5200             | 1.05  |
| HL5400 | 5400             | 0.99  |
| HL5600 | 5600             | 0.96  |
| HL5800 | 5800             | 0.97  |

(\*) Frequency validity is +/-50MHz below 600MHz, +/-100MHz from 600MHz to 6GHz and +/-700MHz above 6GHz

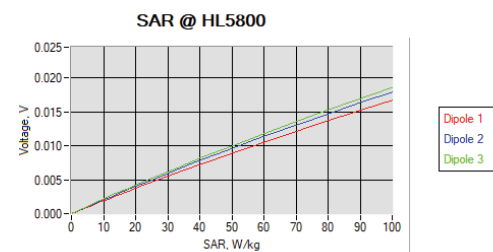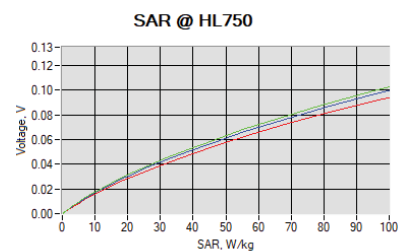


## 6 VERIFICATION RESULTS

The figures below represent the measured linearity and axial isotropy for this probe. The probe specification is +/-0.2 dB for linearity and +/-0.15 dB for axial isotropy.

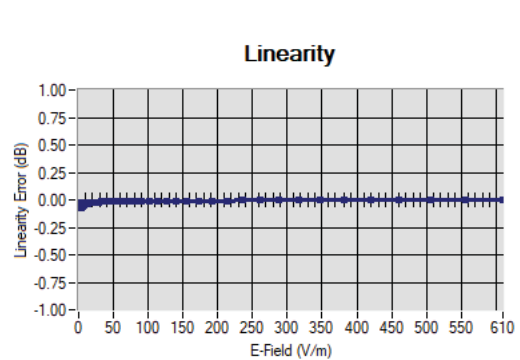

Linearity: +/-1.77% (+/-0.08dB)

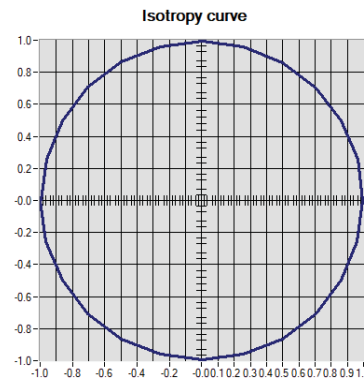

Isotropy: +/-0.26% (+/-0.01dB)

## 7 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                         |                                               |                                               |
|------------------------------------|-------------------------|-------------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No.      | Current Calibration Date                      | Next Calibration Date                         |
| CALIPROBE Test Bench               | Version 2               | NA                      | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203                  | 08/2021                                       | 08/2024                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223                  | 07/2022                                       | 07/2025                                       |
| Multimeter                         | Keithley 2000           | 4013982                 | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589                  | 03/2022                                       | 03/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002         | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013               | 06/2021                                       | 06/2026                                       |
| USB Sensor                         | Keysight U2000A         | SN: MY62340002          | 10/2022                                       | 10/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467                  | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Fluoroptic Thermometer             | LumaSense Luxtron 812   | 94264                   | 09/2022                                       | 09/2025                                       |
| Coaxial cell                       | MVG                     | SN 32/16 COAXCELL_1     | Validated. No cal required.                   | Validated. No cal required.                   |
| Waveguide                          | MVG                     | SN 32/16 WG2_1          | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                     | SN 32/16 WGLIQ_0G600_1  | Validated. No cal required.                   | Validated. No cal required.                   |
| Waveguide                          | MVG                     | SN 32/16 WG4_1          | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                     | SN 32/16 WGLIQ_0G900_1  | Validated. No cal required.                   | Validated. No cal required.                   |
| Waveguide                          | MVG                     | SN 32/16 WG6_1          | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                     | SN 32/16 WGLIQ_1G500_1  | Validated. No cal required.                   | Validated. No cal required.                   |
| Waveguide                          | MVG                     | SN 32/16 WG8_1          | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                     | SN 32/16 WGLIQ_1G800B_1 | Validated. No cal required.                   | Validated. No cal required.                   |
| Liquid transition                  | MVG                     | SN 32/16 WGLIQ_1G800H_1 | Validated. No cal required.                   | Validated. No cal required.                   |



## COMOSAR E-FIELD PROBE CALIBRATION REPORT

Ref: ACR.193.11.24.BES.B

|                               |              |                        |                             |                             |
|-------------------------------|--------------|------------------------|-----------------------------|-----------------------------|
| Waveguide                     | MVG          | SN 32/16 WG10_1        | Validated. No cal required. | Validated. No cal required. |
| Liquid transition             | MVG          | SN 32/16 WGLIQ_3G500_1 | Validated. No cal required. | Validated. No cal required. |
| Waveguide                     | MVG          | SN 32/16 WG12_1        | Validated. No cal required. | Validated. No cal required. |
| Liquid transition             | MVG          | SN 32/16 WGLIQ_5G000_1 | Validated. No cal required. | Validated. No cal required. |
| Waveguide                     | MVG          | SN 32/16 WG14_1        | Validated. No cal required. | Validated. No cal required. |
| Liquid transition             | MVG          | SN 32/16 WGLIQ_7G000_1 | Validated. No cal required. | Validated. No cal required. |
| Temperature / Humidity Sensor | Testo 184 H1 | 44235403               | 02/2024                     | 02/2027                     |



## SAR Reference Dipole Calibration Report

Ref : ACR.75.6.23.SATU.A

**Waltek Testing Group (Shenzhen) Co., Ltd.**  
**1/F, Building A, Hongwei Industrial Park, Liuxian 2<sup>nd</sup> Road**  
**BAO'AN DISTRICT**  
**SHENZHEN, P.R.C. (518101)**  
**MVG COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 750 MHZ**  
**SERIAL NO.: SN 47/12 DIP 0G750-203**

**Calibrated at MVG**  
**Z.I. de la pointe du diable**  
**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**  
**29280 PLOUZANE - FRANCE**

**Calibration date: 08/20/2023**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

### *Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>    |
|----------------------|--------------|---------------------|-------------|---------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 08/20/2023  | <i>Yann TOUTAIN</i> |

2023.08.20

11:51:55 +01'00'

|                       | <i>Customer Name</i>                            |
|-----------------------|-------------------------------------------------|
| <i>Distribution :</i> | Waltek Testing<br>Group (Shenzhen)<br>Co., Ltd. |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|-------------|----------------------|
| A            | Jérôme Luc  | 08/20/2023  | Initial release      |
|              |             |             |                      |
|              |             |             |                      |
|              |             |             |                      |

## TABLE OF CONTENTS

|     |                                                |    |
|-----|------------------------------------------------|----|
| 1   | Introduction.....                              | 4  |
| 2   | Device Under Test .....                        | 4  |
| 3   | Product Description .....                      | 4  |
| 3.1 | General Information .....                      | 4  |
| 4   | Measurement Method .....                       | 5  |
| 4.1 | Return Loss Requirements .....                 | 5  |
| 4.2 | Mechanical Requirements .....                  | 5  |
| 5   | Measurement Uncertainty .....                  | 5  |
| 5.1 | Return Loss .....                              | 5  |
| 5.2 | Dimension Measurement .....                    | 5  |
| 5.3 | Validation Measurement .....                   | 5  |
| 6   | Calibration Measurement Results .....          | 6  |
| 6.1 | Return Loss and Impedance In Head Liquid ..... | 6  |
| 6.2 | Return Loss and Impedance In Body Liquid ..... | 6  |
| 6.3 | Mechanical Dimensions .....                    | 7  |
| 7   | Validation measurement .....                   | 7  |
| 7.1 | Head Liquid Measurement .....                  | 8  |
| 7.2 | SAR Measurement Result With Head Liquid .....  | 8  |
| 7.3 | Body Liquid Measurement .....                  | 11 |
| 7.4 | SAR Measurement Result With Body Liquid .....  | 12 |
| 8   | List of Equipment .....                        | 13 |

## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                  |
|--------------------------------|----------------------------------|
| Device Type                    | COMOSAR 750 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                              |
| Model                          | SID750                           |
| Serial Number                  | SN 47/12 DIP 0G750-203           |
| Product Condition (new / used) | New                              |

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

## 4 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

### 4.2 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of  $k=2$ , traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.08 LIN                            |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 0 - 300     | 0.20 mm                        |
| 300 - 450   | 0.44 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 19 % (SAR)           |
| 10 g        | 19 % (SAR)           |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

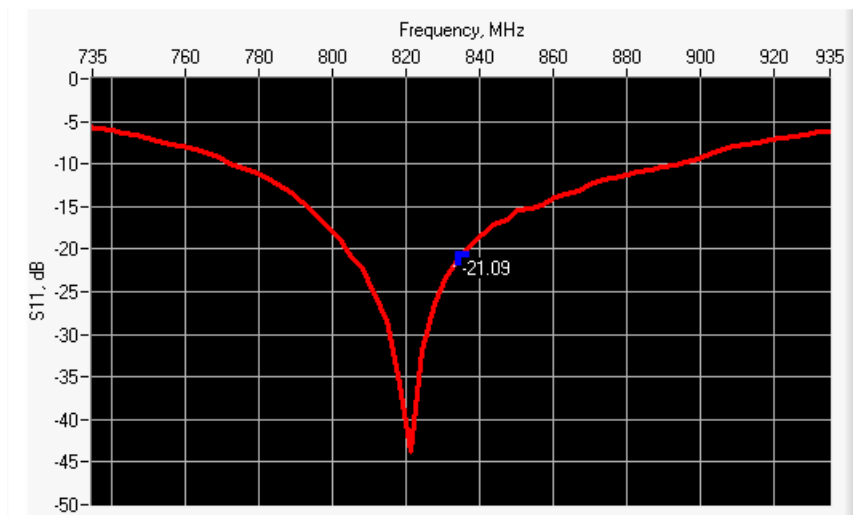

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                      |
|-----------------|------------------|------------------|--------------------------------|
| 750             | -21.09           | -20              | 59.5 $\Omega$ - 1.2 j $\Omega$ |

### 6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

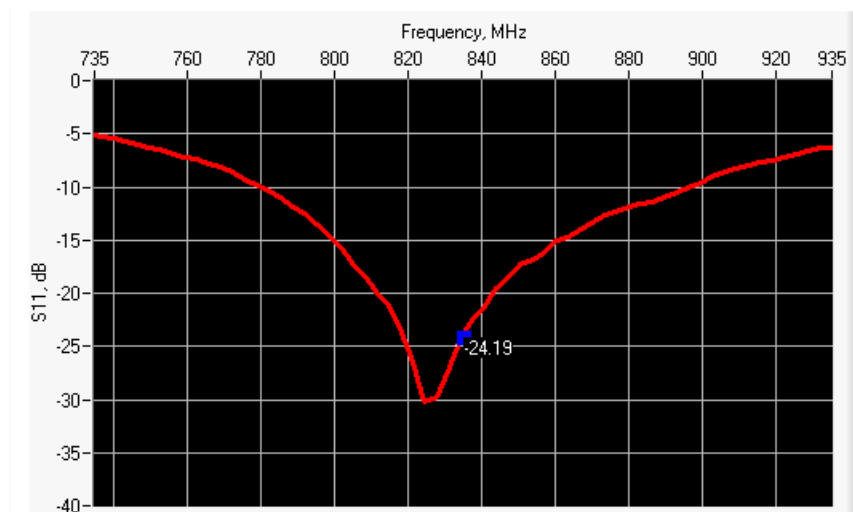

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                      |
|-----------------|------------------|------------------|--------------------------------|
| 750             | -24.19           | -20              | 55.8 $\Omega$ + 3.0 j $\Omega$ |

### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm        |          | h mm        |          | d mm       |          |
|---------------|-------------|----------|-------------|----------|------------|----------|
|               | required    | measured | required    | measured | required   | measured |
| 300           | 420.0 ±1 %. |          | 250.0 ±1 %. |          | 6.35 ±1 %. |          |
| 450           | 290.0 ±1 %. |          | 166.7 ±1 %. |          | 6.35 ±1 %. |          |
| 750           | 176.0 ±1 %. | 177.28   | 100.0 ±1 %. | 99.79    | 6.35 ±1 %. | 6.35     |
| 835           | 161.0 ±1 %. |          | 89.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 900           | 149.0 ±1 %. |          | 83.3 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1450          | 89.1 ±1 %.  |          | 51.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1500          | 86.2 ±1 %.  |          | 50.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1640          | 79.0 ±1 %.  |          | 45.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1750          | 75.2 ±1 %.  |          | 42.9 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1800          | 72.0 ±1 %.  |          | 41.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1900          | 68.0 ±1 %.  |          | 39.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1950          | 66.3 ±1 %.  |          | 38.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2000          | 64.5 ±1 %.  |          | 37.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2100          | 61.0 ±1 %.  |          | 35.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2300          | 55.5 ±1 %.  |          | 32.6 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2450          | 51.5 ±1 %.  |          | 30.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2600          | 48.5 ±1 %.  |          | 28.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3000          | 41.5 ±1 %.  |          | 25.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3300          | -           |          | -           |          | -          |          |
| 3500          | 37.0 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3700          | 34.7 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3900          | -           |          | -           |          | -          |          |
| 4200          | -           |          | -           |          | -          |          |
| 4600          | -           |          | -           |          | -          |          |
| 4900          | -           |          | -           |          | -          |          |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

## 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         | 41.0     | 0.89 $\pm$ 10 %               | 0.82     |
| 835              | 41.5 $\pm$ 10 %                         |          | 0.90 $\pm$ 10 %               |          |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1900             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         |          | 1.67 $\pm$ 10 %               |          |
| 2450             | 39.2 $\pm$ 10 %                         |          | 1.80 $\pm$ 10 %               |          |
| 2600             | 39.0 $\pm$ 10 %                         |          | 1.96 $\pm$ 10 %               |          |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |


## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.



|                                           |                                                         |
|-------------------------------------------|---------------------------------------------------------|
| Software                                  | OPENSAR V5                                              |
| Phantom                                   | SN 13/09 SAM68                                          |
| Probe                                     | SN 41/18 EPGO333                                        |
| Liquid                                    | Head Liquid Values: $\epsilon_p$ : 41.0 $\sigma$ : 0.82 |
| Distance between dipole center and liquid | 15.0 mm                                                 |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                         |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                  |
| Frequency                                 | 750 MHz                                                 |
| Input power                               | 20 dBm                                                  |
| Liquid Temperature                        | 20 +/- 1 °C                                             |
| Lab Temperature                           | 20 +/- 1 °C                                             |
| Lab Humidity                              | 30-70 %                                                 |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |             | 10 g SAR (W/kg/W) |             |
|------------------|------------------|-------------|-------------------|-------------|
|                  | required         | measured    | required          | measured    |
| 300              | 2.85             |             | 1.94              |             |
| 450              | 4.58             |             | 3.06              |             |
| 750              | 8.49             | 8.78 (0.88) | 5.55              | 5.72 (0.57) |
| 835              | 9.56             |             | 6.22              |             |
| 900              | 10.9             |             | 6.99              |             |
| 1450             | 29               |             | 16                |             |
| 1500             | 30.5             |             | 16.8              |             |
| 1640             | 34.2             |             | 18.4              |             |
| 1750             | 36.4             |             | 19.3              |             |
| 1800             | 38.4             |             | 20.1              |             |
| 1900             | 39.7             |             | 20.5              |             |
| 1950             | 40.5             |             | 20.9              |             |
| 2000             | 41.1             |             | 21.1              |             |
| 2100             | 43.6             |             | 21.9              |             |
| 2300             | 48.7             |             | 23.3              |             |
| 2450             | 52.4             |             | 24                |             |
| 2600             | 55.3             |             | 24.6              |             |
| 3000             | 63.8             |             | 25.7              |             |
| 3300             | -                |             | -                 |             |
| 3500             | 67.1             |             | 25                |             |
| 3700             | 67.4             |             | 24.2              |             |
| 3900             | -                |             | -                 |             |
| 4200             | -                |             | -                 |             |
| 4600             | -                |             | -                 |             |
| 4900             | -                |             | -                 |             |

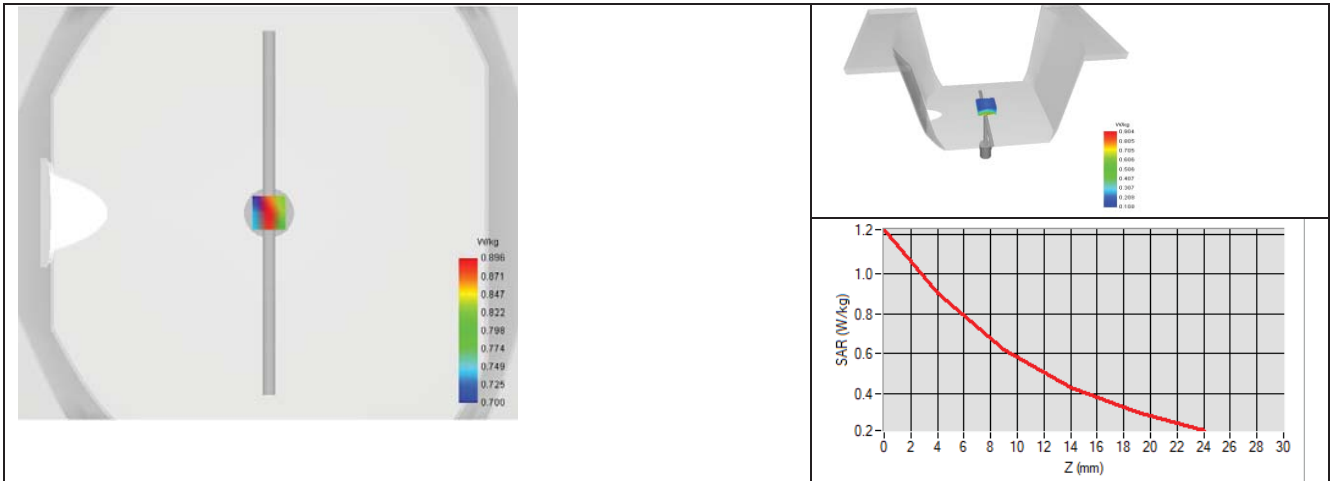


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         | 52.9     | 0.96 $\pm$ 10 %               | 0.89     |
| 835              | 55.2 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 1900             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         |          | 1.81 $\pm$ 10 %               |          |
| 2450             | 52.7 $\pm$ 10 %                         |          | 1.95 $\pm$ 10 %               |          |
| 2600             | 52.5 $\pm$ 10 %                         |          | 2.16 $\pm$ 10 %               |          |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

#### 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                       |
|-------------------------------------------|-------------------------------------------------------|
| Software                                  | OPENSAR V5                                            |
| Phantom                                   | SN 13/09 SAM68                                        |
| Probe                                     | SN 41/18 EPG0333                                      |
| Liquid                                    | Body Liquid Values: $\epsilon_s'$ : 52.9 sigma : 0.89 |
| Distance between dipole center and liquid | 15.0 mm                                               |
| Area scan resolution                      | dx=8mm/dy=8mm                                         |
| Zoon Scan Resolution                      | dx=8mm/dy=8mm/dz=5mm                                  |
| Frequency                                 | 750 MHz                                               |
| Input power                               | 20 dBm                                                |
| Liquid Temperature                        | 20 +/- 1 °C                                           |
| Lab Temperature                           | 20 +/- 1 °C                                           |
| Lab Humidity                              | 30-70 %                                               |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 750              | 8.59 (0.86)      | 5.74 (0.57)       |

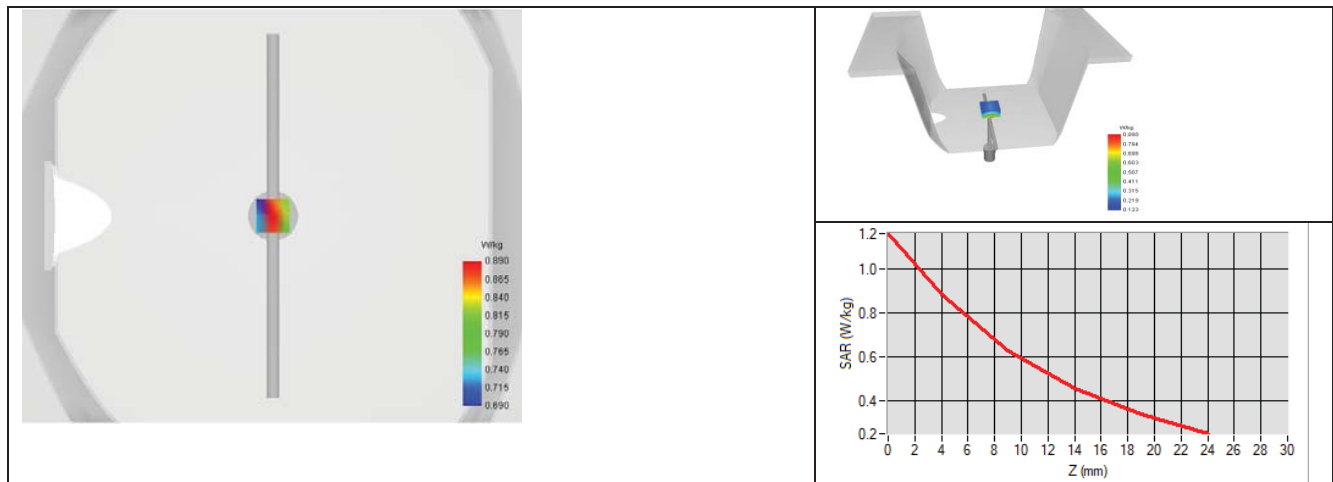



## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2022                                       | 10/2023                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2021                                       | 06/2024                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2021                                       | 06/2024                                       |

Appendix A. Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole SID750– serial no. SN 47/12 DIP 0G750-203

| Head                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -21.09           | /         | 59.5                 | /           | 1.2                        | /            |
| 2024-08-19          | -21.32           | 5.44      | 58.8                 | 0.7         | 1.0                        | 0.2          |

| Body                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -24.19           | /         | 55.8                 | /           | 3.0                        | /            |
| 2024-08-19          | -24.38           | 4.47      | 55.1                 | 0.7         | 2.6                        | 0.4          |

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended.



# SAR Reference Dipole Calibration Report

Ref : ACR.75.1.23.SATU.A

**Waltek Testing Group (Shenzhen) Co., Ltd.**  
**1/F, Building A, Hongwei Industrial Park, Liuxian 2<sup>nd</sup> Road**  
**BAO'AN DISTRICT**  
**SHENZHEN, P.R.C. (518101)**  
**MVG COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 835 MHZ**  
**SERIAL NO.: SN 47/12 DIP 0G835-204**

**Calibrated at MVG**  
**Z.I. de la pointe du diable**  
**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**  
**29280 PLOUZANE - FRANCE**

**Calibration date: 08/20/2023**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

## Summary:

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>    |
|----------------------|--------------|---------------------|-------------|---------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 08/20/2023  | <i>Yann TOUTAIN</i> |

2023.08.20  
11:52:29 +01'00'

|                       | <i>Customer Name</i>                            |
|-----------------------|-------------------------------------------------|
| <i>Distribution :</i> | Waltek Testing<br>Group (Shenzhen)<br>Co., Ltd. |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|-------------|----------------------|
| A            | Jérôme Luc  | 08/20/2023  | Initial release      |
|              |             |             |                      |
|              |             |             |                      |
|              |             |             |                      |

## TABLE OF CONTENTS

|     |                                                |    |
|-----|------------------------------------------------|----|
| 1   | Introduction.....                              | 4  |
| 2   | Device Under Test .....                        | 4  |
| 3   | Product Description .....                      | 4  |
| 3.1 | General Information .....                      | 4  |
| 4   | Measurement Method .....                       | 5  |
| 4.1 | Return Loss Requirements .....                 | 5  |
| 4.2 | Mechanical Requirements .....                  | 5  |
| 5   | Measurement Uncertainty .....                  | 5  |
| 5.1 | Return Loss .....                              | 5  |
| 5.2 | Dimension Measurement .....                    | 5  |
| 5.3 | Validation Measurement .....                   | 5  |
| 6   | Calibration Measurement Results .....          | 6  |
| 6.1 | Return Loss and Impedance In Head Liquid ..... | 6  |
| 6.2 | Return Loss and Impedance In Body Liquid ..... | 6  |
| 6.3 | Mechanical Dimensions .....                    | 7  |
| 7   | Validation measurement .....                   | 7  |
| 7.1 | Head Liquid Measurement .....                  | 8  |
| 7.2 | SAR Measurement Result With Head Liquid .....  | 8  |
| 7.3 | Body Liquid Measurement .....                  | 11 |
| 7.4 | SAR Measurement Result With Body Liquid .....  | 12 |
| 8   | List of Equipment .....                        | 13 |

## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                  |
|--------------------------------|----------------------------------|
| Device Type                    | COMOSAR 835 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                              |
| Model                          | SID835                           |
| Serial Number                  | SN 47/12 DIP 0G835-204           |
| Product Condition (new / used) | New                              |

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

## 4 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

### 4.2 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of  $k=2$ , traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.08 LIN                            |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 0 - 300     | 0.20 mm                        |
| 300 - 450   | 0.44 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 19 % (SAR)           |
| 10 g        | 19 % (SAR)           |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

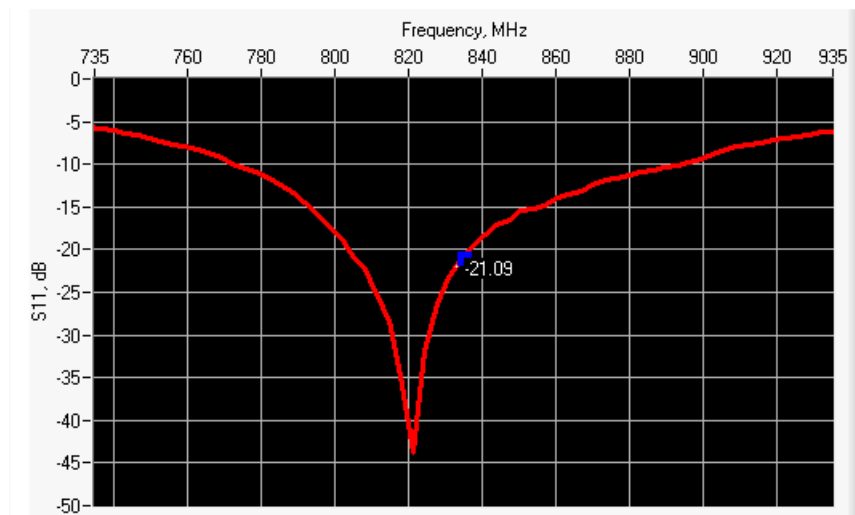

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                      |
|-----------------|------------------|------------------|--------------------------------|
| 835             | -21.09           | -20              | 59.5 $\Omega$ - 1.2 j $\Omega$ |

### 6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

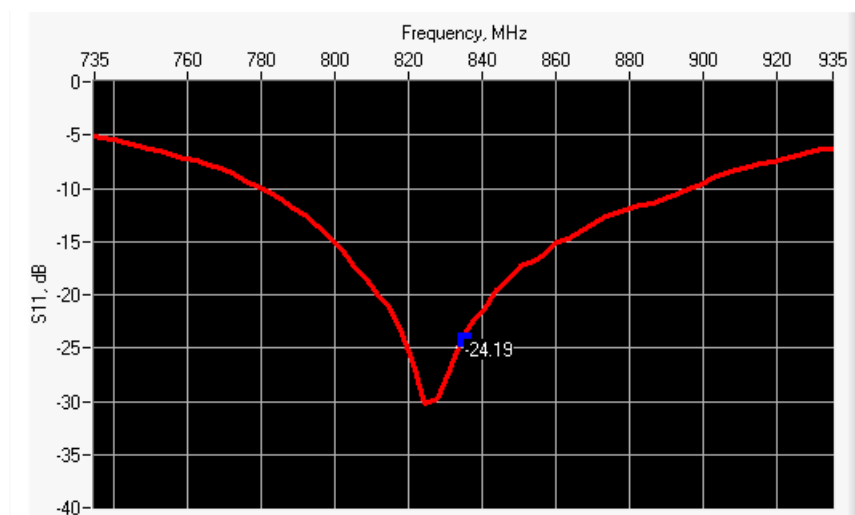

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                      |
|-----------------|------------------|------------------|--------------------------------|
| 835             | -24.19           | -20              | 55.8 $\Omega$ - 3.0 j $\Omega$ |

### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm        |          | h mm        |          | d mm       |          |
|---------------|-------------|----------|-------------|----------|------------|----------|
|               | required    | measured | required    | measured | required   | measured |
| 300           | 420.0 ±1 %. |          | 250.0 ±1 %. |          | 6.35 ±1 %. |          |
| 450           | 290.0 ±1 %. |          | 166.7 ±1 %. |          | 6.35 ±1 %. |          |
| 750           | 176.0 ±1 %. |          | 100.0 ±1 %. |          | 6.35 ±1 %. |          |
| 835           | 161.0 ±1 %. | 160.52   | 89.8 ±1 %.  | 89.37    | 3.6 ±1 %.  | 3.61     |
| 900           | 149.0 ±1 %. |          | 83.3 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1450          | 89.1 ±1 %.  |          | 51.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1500          | 86.2 ±1 %.  |          | 50.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1640          | 79.0 ±1 %.  |          | 45.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1750          | 75.2 ±1 %.  |          | 42.9 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1800          | 72.0 ±1 %.  |          | 41.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1900          | 68.0 ±1 %.  |          | 39.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1950          | 66.3 ±1 %.  |          | 38.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2000          | 64.5 ±1 %.  |          | 37.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2100          | 61.0 ±1 %.  |          | 35.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2300          | 55.5 ±1 %.  |          | 32.6 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2450          | 51.5 ±1 %.  |          | 30.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2600          | 48.5 ±1 %.  |          | 28.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3000          | 41.5 ±1 %.  |          | 25.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3300          | -           |          | -           |          | -          |          |
| 3500          | 37.0 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3700          | 34.7 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3900          | -           |          | -           |          | -          |          |
| 4200          | -           |          | -           |          | -          |          |
| 4600          | -           |          | -           |          | -          |          |
| 4900          | -           |          | -           |          | -          |          |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

## 7.1 HEAD LIQUID MEASUREMENT


| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         |          | 0.89 $\pm$ 10 %               |          |
| 835              | 41.5 $\pm$ 10 %                         | 42.1     | 0.90 $\pm$ 10 %               | 0.92     |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1900             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         |          | 1.67 $\pm$ 10 %               |          |
| 2450             | 39.2 $\pm$ 10 %                         |          | 1.80 $\pm$ 10 %               |          |
| 2600             | 39.0 $\pm$ 10 %                         |          | 1.96 $\pm$ 10 %               |          |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |

## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|                                           |                                                      |
|-------------------------------------------|------------------------------------------------------|
| Software                                  | OPENSAR V5                                           |
| Phantom                                   | SN 13/09 SAM68                                       |
| Probe                                     | SN 41/18 EPGO333                                     |
| Liquid                                    | Head Liquid Values: $\epsilon_p$ : 42.1 sigma : 0.92 |
| Distance between dipole center and liquid | 15.0 mm                                              |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                      |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                               |
| Frequency                                 | 835 MHz                                              |
| Input power                               | 20 dBm                                               |
| Liquid Temperature                        | 20 +/- 1 °C                                          |
| Lab Temperature                           | 20 +/- 1 °C                                          |
| Lab Humidity                              | 30-70 %                                              |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |             | 10 g SAR (W/kg/W) |             |
|------------------|------------------|-------------|-------------------|-------------|
|                  | required         | measured    | required          | measured    |
| 300              | 2.85             |             | 1.94              |             |
| 450              | 4.58             |             | 3.06              |             |
| 750              | 8.49             |             | 5.55              |             |
| 835              | 9.56             | 9.65 (0.97) | 6.22              | 6.26 (0.63) |
| 900              | 10.9             |             | 6.99              |             |
| 1450             | 29               |             | 16                |             |
| 1500             | 30.5             |             | 16.8              |             |
| 1640             | 34.2             |             | 18.4              |             |
| 1750             | 36.4             |             | 19.3              |             |
| 1800             | 38.4             |             | 20.1              |             |
| 1900             | 39.7             |             | 20.5              |             |
| 1950             | 40.5             |             | 20.9              |             |
| 2000             | 41.1             |             | 21.1              |             |
| 2100             | 43.6             |             | 21.9              |             |
| 2300             | 48.7             |             | 23.3              |             |
| 2450             | 52.4             |             | 24                |             |
| 2600             | 55.3             |             | 24.6              |             |
| 3000             | 63.8             |             | 25.7              |             |
| 3300             | -                |             | -                 |             |
| 3500             | 67.1             |             | 25                |             |
| 3700             | 67.4             |             | 24.2              |             |
| 3900             | -                |             | -                 |             |
| 4200             | -                |             | -                 |             |
| 4600             | -                |             | -                 |             |
| 4900             | -                |             | -                 |             |

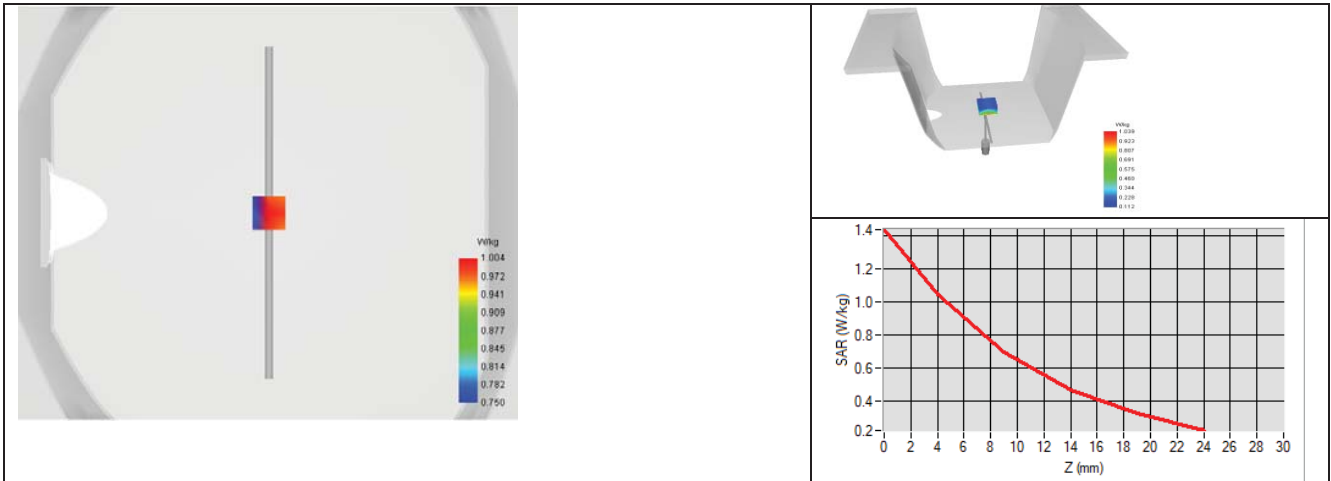


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         |          | 0.96 $\pm$ 10 %               |          |
| 835              | 55.2 $\pm$ 10 %                         | 53.8     | 0.97 $\pm$ 10 %               | 0.98     |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 1900             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         |          | 1.81 $\pm$ 10 %               |          |
| 2450             | 52.7 $\pm$ 10 %                         |          | 1.95 $\pm$ 10 %               |          |
| 2600             | 52.5 $\pm$ 10 %                         |          | 2.16 $\pm$ 10 %               |          |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

## 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPGO333                                         |
| Liquid                                    | Body Liquid Values: $\epsilon_{ps}'$ : 53.8 sigma : 0.98 |
| Distance between dipole center and liquid | 15.0 mm                                                  |
| Area scan resolution                      | dx=8mm/dy=8mm                                            |
| Zoon Scan Resolution                      | dx=8mm/dy=8mm/dz=5mm                                     |
| Frequency                                 | 835 MHz                                                  |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 835              | 9.36 (0.94)      | 6.19 (0.62)       |

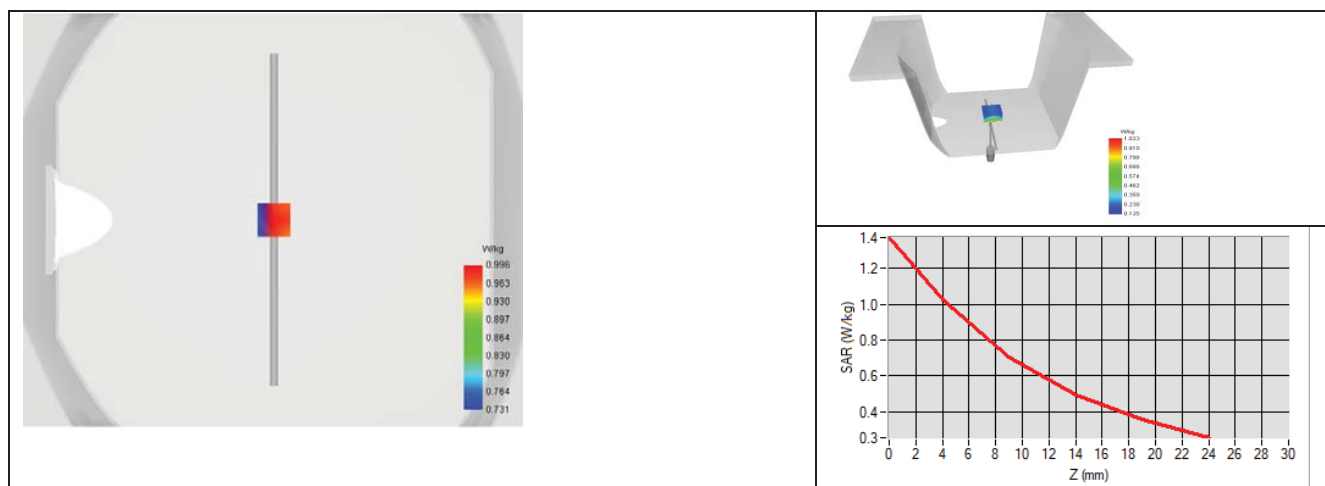



## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2022                                       | 10/2023                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2021                                       | 06/2024                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2021                                       | 06/2024                                       |

Appendix A. Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole SID835– serial no. SN 47/12 DIP 0G835-204

| Head                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -21.09           | /         | 59.5                 | /           | 1.2                        | /            |
| 2024-08-19          | -20.75           | 7.53      | 59.1                 | 0.4         | 1.1                        | 0.1          |

| Body                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -24.19           | /         | 55.8                 | /           | 3.0                        | /            |
| 2024-08-19          | -24.31           | 2.80      | 55.1                 | 0.7         | 2.6                        | 0.4          |

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended.



## SAR Reference Dipole Calibration Report

Ref : ACR.75.3.23.SATU.A

**Waltek Testing Group (Shenzhen) Co., Ltd.**  
**1/F, Building A, Hongwei Industrial Park, Liuxian 2<sup>nd</sup> Road**  
**BAO'AN DISTRICT**  
**SHENZHEN, P.R.C. (518101)**  
**MVG COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 1800 MHZ**  
**SERIAL NO.: SN 47/12 DIP 1G800-206**

**Calibrated at MVG**  
**Z.I. de la pointe du diable**  
**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**  
**29280 PLOUZANE - FRANCE**

**Calibration date: 08/20/2023**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

### *Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>    |
|----------------------|--------------|---------------------|-------------|---------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 08/20/2023  | <i>Yann TOUTAIN</i> |

2023.08.20

11:53:42 +01'00'

|                       | <i>Customer Name</i>                            |
|-----------------------|-------------------------------------------------|
| <i>Distribution :</i> | Waltek Testing<br>Group (Shenzhen)<br>Co., Ltd. |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|-------------|----------------------|
| A            | Jérôme Luc  | 08/20/2023  | Initial release      |
|              |             |             |                      |
|              |             |             |                      |
|              |             |             |                      |

## TABLE OF CONTENTS

|     |                                                |    |
|-----|------------------------------------------------|----|
| 1   | Introduction.....                              | 4  |
| 2   | Device Under Test .....                        | 4  |
| 3   | Product Description .....                      | 4  |
| 3.1 | General Information .....                      | 4  |
| 4   | Measurement Method .....                       | 5  |
| 4.1 | Return Loss Requirements .....                 | 5  |
| 4.2 | Mechanical Requirements .....                  | 5  |
| 5   | Measurement Uncertainty .....                  | 5  |
| 5.1 | Return Loss .....                              | 5  |
| 5.2 | Dimension Measurement .....                    | 5  |
| 5.3 | Validation Measurement .....                   | 5  |
| 6   | Calibration Measurement Results .....          | 6  |
| 6.1 | Return Loss and Impedance In Head Liquid ..... | 6  |
| 6.2 | Return Loss and Impedance In Body Liquid ..... | 6  |
| 6.3 | Mechanical Dimensions .....                    | 7  |
| 7   | Validation measurement .....                   | 7  |
| 7.1 | Head Liquid Measurement .....                  | 8  |
| 7.2 | SAR Measurement Result With Head Liquid .....  | 8  |
| 7.3 | Body Liquid Measurement .....                  | 11 |
| 7.4 | SAR Measurement Result With Body Liquid .....  | 12 |
| 8   | List of Equipment .....                        | 13 |

## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 1800 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                               |
| Model                          | SID1800                           |
| Serial Number                  | SN 47/12 DIP 1G800-206            |
| Product Condition (new / used) | New                               |

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

## 4 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

### 4.2 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.08 LIN                            |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 0 - 300     | 0.20 mm                        |
| 300 - 450   | 0.44 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 19 % (SAR)           |
| 10 g        | 19 % (SAR)           |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

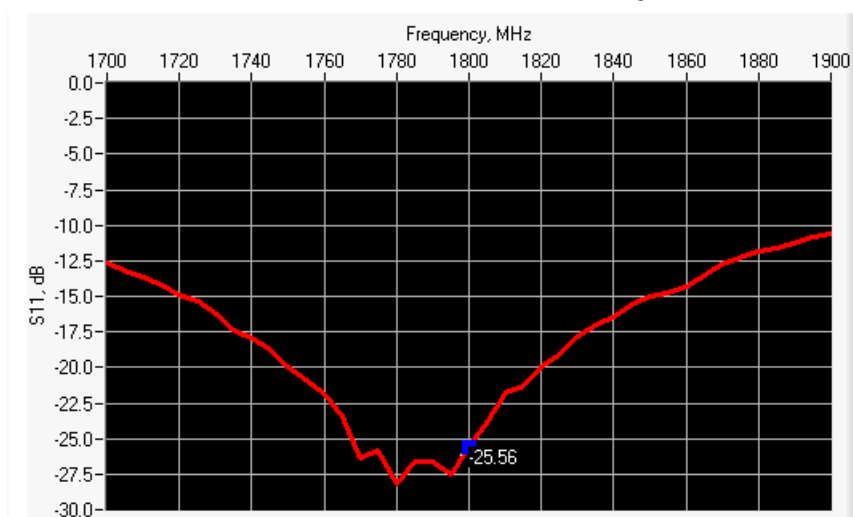

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                      |
|-----------------|------------------|------------------|--------------------------------|
| 1800            | -25.56           | -20              | 48.1 $\Omega$ + 4.8 j $\Omega$ |

### 6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

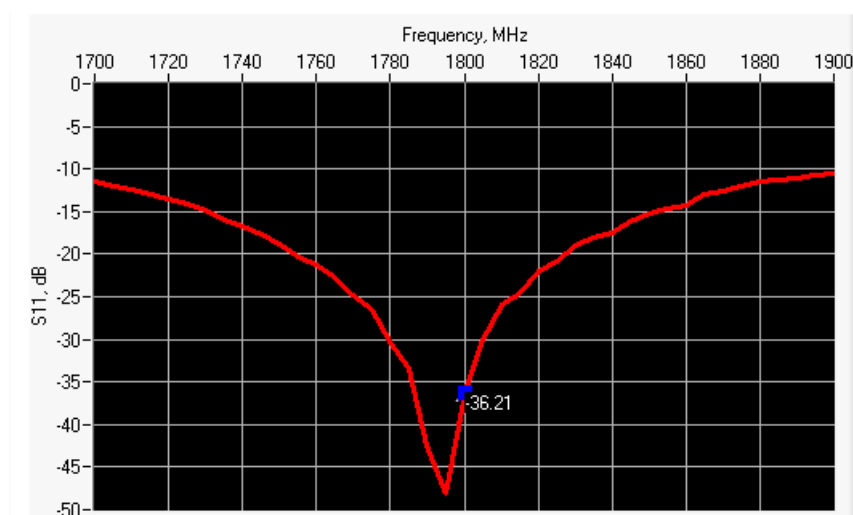

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                      |
|-----------------|------------------|------------------|--------------------------------|
| 1800            | -36.21           | -20              | 48.5 $\Omega$ - 0.2 j $\Omega$ |

### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm        |          | h mm        |          | d mm       |          |
|---------------|-------------|----------|-------------|----------|------------|----------|
|               | required    | measured | required    | measured | required   | measured |
| 300           | 420.0 ±1 %. |          | 250.0 ±1 %. |          | 6.35 ±1 %. |          |
| 450           | 290.0 ±1 %. |          | 166.7 ±1 %. |          | 6.35 ±1 %. |          |
| 750           | 176.0 ±1 %. |          | 100.0 ±1 %. |          | 6.35 ±1 %. |          |
| 835           | 161.0 ±1 %. |          | 89.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 900           | 149.0 ±1 %. |          | 83.3 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1450          | 89.1 ±1 %.  |          | 51.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1500          | 86.2 ±1 %.  |          | 50.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1640          | 79.0 ±1 %.  |          | 45.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1750          | 75.2 ±1 %.  |          | 42.9 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1800          | 72.0 ±1 %.  | 71.51    | 41.7 ±1 %.  | 41.39    | 3.6 ±1 %.  | 3.59     |
| 1900          | 68.0 ±1 %.  |          | 39.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1950          | 66.3 ±1 %.  |          | 38.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2000          | 64.5 ±1 %.  |          | 37.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2100          | 61.0 ±1 %.  |          | 35.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2300          | 55.5 ±1 %.  |          | 32.6 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2450          | 51.5 ±1 %.  |          | 30.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2600          | 48.5 ±1 %.  |          | 28.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3000          | 41.5 ±1 %.  |          | 25.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3300          | -           |          | -           |          | -          |          |
| 3500          | 37.0 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3700          | 34.7 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3900          | -           |          | -           |          | -          |          |
| 4200          | -           |          | -           |          | -          |          |
| 4600          | -           |          | -           |          | -          |          |
| 4900          | -           |          | -           |          | -          |          |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

## 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         |          | 0.89 $\pm$ 10 %               |          |
| 835              | 41.5 $\pm$ 10 %                         |          | 0.90 $\pm$ 10 %               |          |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         | 41.1     | 1.40 $\pm$ 10 %               | 1.39     |
| 1900             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         |          | 1.67 $\pm$ 10 %               |          |
| 2450             | 39.2 $\pm$ 10 %                         |          | 1.80 $\pm$ 10 %               |          |
| 2600             | 39.0 $\pm$ 10 %                         |          | 1.96 $\pm$ 10 %               |          |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |


## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.



|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPGO333                                         |
| Liquid                                    | Head Liquid Values: $\epsilon_s'$ : 41.1 $\sigma$ : 1.39 |
| Distance between dipole center and liquid | 10.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                   |
| Frequency                                 | 1800 MHz                                                 |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |              | 10 g SAR (W/kg/W) |              |
|------------------|------------------|--------------|-------------------|--------------|
|                  | required         | measured     | required          | measured     |
| 300              | 2.85             |              | 1.94              |              |
| 450              | 4.58             |              | 3.06              |              |
| 750              | 8.49             |              | 5.55              |              |
| 835              | 9.56             |              | 6.22              |              |
| 900              | 10.9             |              | 6.99              |              |
| 1450             | 29               |              | 16                |              |
| 1500             | 30.5             |              | 16.8              |              |
| 1640             | 34.2             |              | 18.4              |              |
| 1750             | 36.4             |              | 19.3              |              |
| 1800             | 38.4             | 38.49 (3.85) | 20.1              | 20.67 (2.07) |
| 1900             | 39.7             |              | 20.5              |              |
| 1950             | 40.5             |              | 20.9              |              |
| 2000             | 41.1             |              | 21.1              |              |
| 2100             | 43.6             |              | 21.9              |              |
| 2300             | 48.7             |              | 23.3              |              |
| 2450             | 52.4             |              | 24                |              |
| 2600             | 55.3             |              | 24.6              |              |
| 3000             | 63.8             |              | 25.7              |              |
| 3300             | -                |              | -                 |              |
| 3500             | 67.1             |              | 25                |              |
| 3700             | 67.4             |              | 24.2              |              |
| 3900             | -                |              | -                 |              |
| 4200             | -                |              | -                 |              |
| 4600             | -                |              | -                 |              |
| 4900             | -                |              | -                 |              |

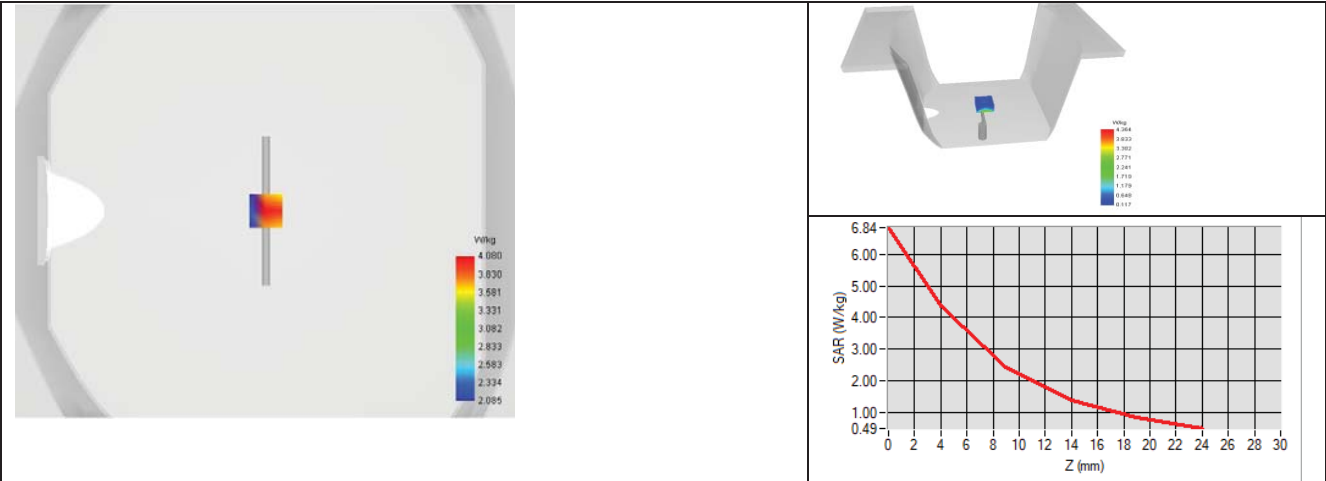


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         |          | 0.96 $\pm$ 10 %               |          |
| 835              | 55.2 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         | 53.0     | 1.52 $\pm$ 10 %               | 1.52     |
| 1900             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         |          | 1.81 $\pm$ 10 %               |          |
| 2450             | 52.7 $\pm$ 10 %                         |          | 1.95 $\pm$ 10 %               |          |
| 2600             | 52.5 $\pm$ 10 %                         |          | 2.16 $\pm$ 10 %               |          |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

## 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPG0333                                         |
| Liquid                                    | Body Liquid Values: $\epsilon_s' : 53.0$ $\sigma : 1.52$ |
| Distance between dipole center and liquid | 10.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                   |
| Frequency                                 | 1800 MHz                                                 |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 1800             | 38.29 (3.83)     | 20.88 (2.09)      |

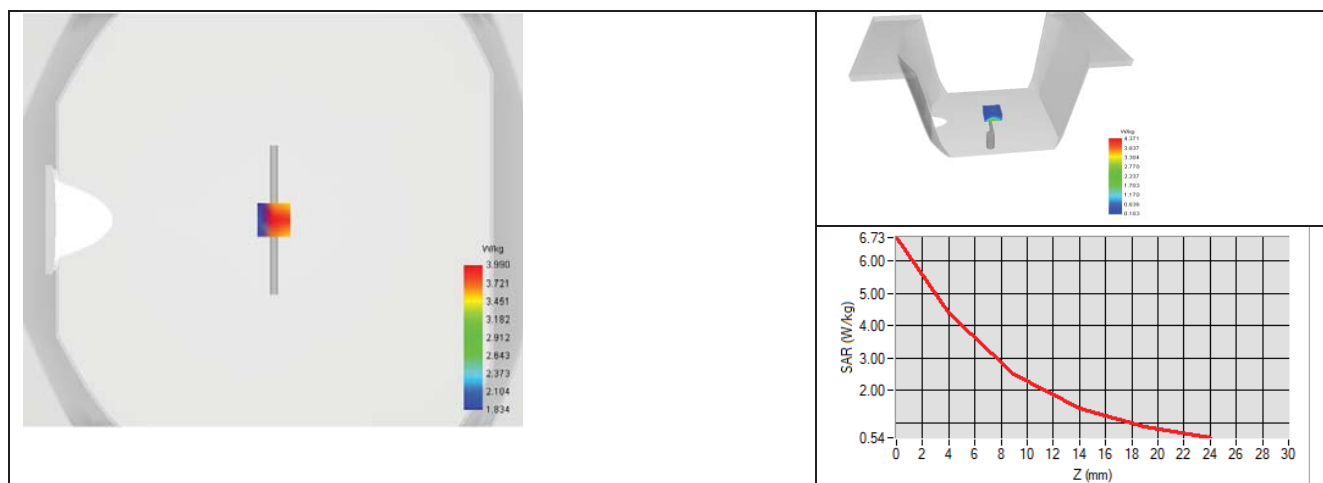



## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2022                                       | 10/2023                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2021                                       | 06/2024                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2021                                       | 06/2024                                       |

Appendix A. Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole SID1800 serial no. SN 47/12 DIP 1G800-206

| Head                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -25.56           | /         | 48.1                 | /           | 4.8                        | /            |
| 2024-08-19          | -25.42           | 3.17      | 49.0                 | 0.9         | 4.2                        | 0.6          |

| Body                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -36.21           | /         | 48.5                 | /           | 0.2                        | /            |
| 2024-08-19          | -36.38           | 3.99      | 49.1                 | 0.6         | 0.6                        | 0.4          |

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended.



## SAR Reference Dipole Calibration Report

Ref : ACR.75.4.23.SATU.A

**Waltek Testing Group (Shenzhen) Co., Ltd.**  
**1/F, Building A, Hongwei Industrial Park, Liuxian 2<sup>nd</sup> Road**  
**BAO'AN DISTRICT**  
**SHENZHEN, P.R.C. (518101)**  
**MVG COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 1900 MHZ**  
**SERIAL NO.: SN 47/12 DIP 1G900-207**

**Calibrated at MVG**  
**Z.I. de la pointe du diable**  
**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**  
**29280 PLOUZANE - FRANCE**

**Calibration date: 08/20/2023**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

### *Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.

|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>    |
|----------------------|--------------|---------------------|-------------|---------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 08/20/2023  | <i>Yann TOUTAIN</i> |

2023.08.20  
11:54:31 +01'00'

|                       | <i>Customer Name</i>                            |
|-----------------------|-------------------------------------------------|
| <i>Distribution :</i> | Waltek Testing<br>Group (Shenzhen)<br>Co., Ltd. |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|-------------|----------------------|
| A            | Jérôme Luc  | 08/20/2023  | Initial release      |
|              |             |             |                      |
|              |             |             |                      |
|              |             |             |                      |

## TABLE OF CONTENTS

|     |                                                |    |
|-----|------------------------------------------------|----|
| 1   | Introduction.....                              | 4  |
| 2   | Device Under Test .....                        | 4  |
| 3   | Product Description .....                      | 4  |
| 3.1 | General Information .....                      | 4  |
| 4   | Measurement Method .....                       | 5  |
| 4.1 | Return Loss Requirements .....                 | 5  |
| 4.2 | Mechanical Requirements .....                  | 5  |
| 5   | Measurement Uncertainty .....                  | 5  |
| 5.1 | Return Loss .....                              | 5  |
| 5.2 | Dimension Measurement .....                    | 5  |
| 5.3 | Validation Measurement .....                   | 5  |
| 6   | Calibration Measurement Results .....          | 6  |
| 6.1 | Return Loss and Impedance In Head Liquid ..... | 6  |
| 6.2 | Return Loss and Impedance In Body Liquid ..... | 6  |
| 6.3 | Mechanical Dimensions .....                    | 7  |
| 7   | Validation measurement .....                   | 7  |
| 7.1 | Head Liquid Measurement .....                  | 8  |
| 7.2 | SAR Measurement Result With Head Liquid .....  | 8  |
| 7.3 | Body Liquid Measurement .....                  | 11 |
| 7.4 | SAR Measurement Result With Body Liquid .....  | 12 |
| 8   | List of Equipment .....                        | 13 |

## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 1900 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                               |
| Model                          | SID1900                           |
| Serial Number                  | SN 47/12 DIP 1G900-207            |
| Product Condition (new / used) | New                               |

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

## 4 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

### 4.2 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.08 LIN                            |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 0 - 300     | 0.20 mm                        |
| 300 - 450   | 0.44 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 19 % (SAR)           |
| 10 g        | 19 % (SAR)           |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

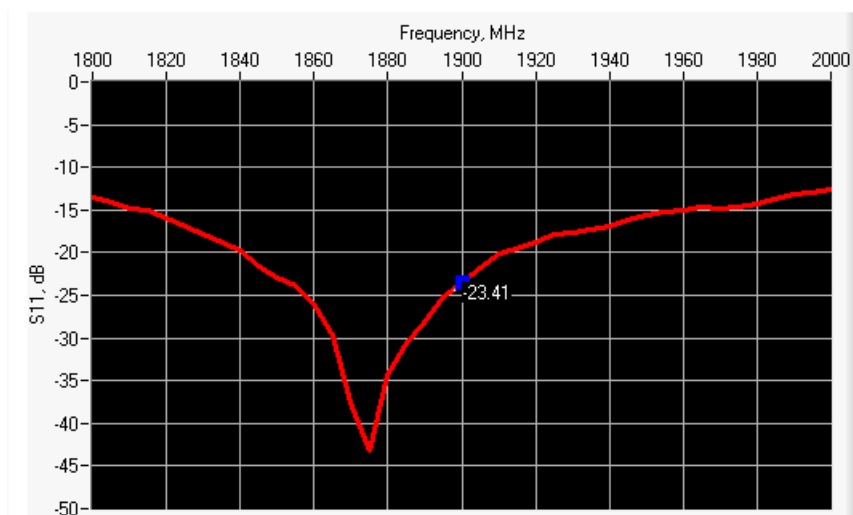

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                   |
|-----------------|------------------|------------------|-----------------------------|
| 1900            | -23.41           | -20              | $53.3 \Omega + 6.2 j\Omega$ |

### 6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

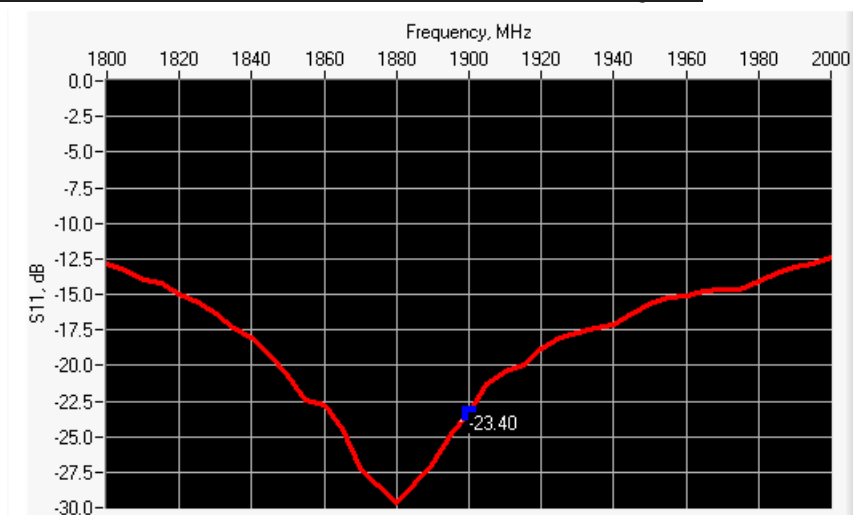

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                   |
|-----------------|------------------|------------------|-----------------------------|
| 1900            | -23.40           | -20              | $47.9 \Omega + 6.3 j\Omega$ |



### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm             |          | h mm             |          | d mm            |          |
|---------------|------------------|----------|------------------|----------|-----------------|----------|
|               | required         | measured | required         | measured | required        | measured |
| 300           | 420.0 $\pm$ 1 %. |          | 250.0 $\pm$ 1 %. |          | 6.35 $\pm$ 1 %. |          |
| 450           | 290.0 $\pm$ 1 %. |          | 166.7 $\pm$ 1 %. |          | 6.35 $\pm$ 1 %. |          |
| 750           | 176.0 $\pm$ 1 %. |          | 100.0 $\pm$ 1 %. |          | 6.35 $\pm$ 1 %. |          |
| 835           | 161.0 $\pm$ 1 %. |          | 89.8 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 900           | 149.0 $\pm$ 1 %. |          | 83.3 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 1450          | 89.1 $\pm$ 1 %.  |          | 51.7 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 1500          | 86.2 $\pm$ 1 %.  |          | 50.0 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 1640          | 79.0 $\pm$ 1 %.  |          | 45.7 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 1750          | 75.2 $\pm$ 1 %.  |          | 42.9 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 1800          | 72.0 $\pm$ 1 %.  |          | 41.7 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 1900          | 68.0 $\pm$ 1 %.  | 67.69    | 39.5 $\pm$ 1 %.  | 39.49    | 3.6 $\pm$ 1 %.  | 3.60     |
| 1950          | 66.3 $\pm$ 1 %.  |          | 38.5 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 2000          | 64.5 $\pm$ 1 %.  |          | 37.5 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 2100          | 61.0 $\pm$ 1 %.  |          | 35.7 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 2300          | 55.5 $\pm$ 1 %.  |          | 32.6 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 2450          | 51.5 $\pm$ 1 %.  |          | 30.4 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 2600          | 48.5 $\pm$ 1 %.  |          | 28.8 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 3000          | 41.5 $\pm$ 1 %.  |          | 25.0 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 3300          | -                |          | -                |          | -               |          |
| 3500          | 37.0 $\pm$ 1 %.  |          | 26.4 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 3700          | 34.7 $\pm$ 1 %.  |          | 26.4 $\pm$ 1 %.  |          | 3.6 $\pm$ 1 %.  |          |
| 3900          | -                |          | -                |          | -               |          |
| 4200          | -                |          | -                |          | -               |          |
| 4600          | -                |          | -                |          | -               |          |
| 4900          | -                |          | -                |          | -               |          |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

## 7.1 HEAD LIQUID MEASUREMENT


| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         |          | 0.89 $\pm$ 10 %               |          |
| 835              | 41.5 $\pm$ 10 %                         |          | 0.90 $\pm$ 10 %               |          |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1900             | 40.0 $\pm$ 10 %                         | 40.9     | 1.40 $\pm$ 10 %               | 1.43     |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         |          | 1.67 $\pm$ 10 %               |          |
| 2450             | 39.2 $\pm$ 10 %                         |          | 1.80 $\pm$ 10 %               |          |
| 2600             | 39.0 $\pm$ 10 %                         |          | 1.96 $\pm$ 10 %               |          |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |

## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|                                           |                                                         |
|-------------------------------------------|---------------------------------------------------------|
| Software                                  | OPENSAR V5                                              |
| Phantom                                   | SN 13/09 SAM68                                          |
| Probe                                     | SN 41/18 EPGO333                                        |
| Liquid                                    | Head Liquid Values: $\epsilon_p$ : 40.9 $\sigma$ : 1.43 |
| Distance between dipole center and liquid | 10.0 mm                                                 |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                         |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                  |
| Frequency                                 | 1900 MHz                                                |
| Input power                               | 20 dBm                                                  |
| Liquid Temperature                        | 20 +/- 1 °C                                             |
| Lab Temperature                           | 20 +/- 1 °C                                             |
| Lab Humidity                              | 30-70 %                                                 |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |              | 10 g SAR (W/kg/W) |              |
|------------------|------------------|--------------|-------------------|--------------|
|                  | required         | measured     | required          | measured     |
| 300              | 2.85             |              | 1.94              |              |
| 450              | 4.58             |              | 3.06              |              |
| 750              | 8.49             |              | 5.55              |              |
| 835              | 9.56             |              | 6.22              |              |
| 900              | 10.9             |              | 6.99              |              |
| 1450             | 29               |              | 16                |              |
| 1500             | 30.5             |              | 16.8              |              |
| 1640             | 34.2             |              | 18.4              |              |
| 1750             | 36.4             |              | 19.3              |              |
| 1800             | 38.4             |              | 20.1              |              |
| 1900             | 39.7             | 39.59 (3.96) | 20.5              | 20.73 (2.07) |
| 1950             | 40.5             |              | 20.9              |              |
| 2000             | 41.1             |              | 21.1              |              |
| 2100             | 43.6             |              | 21.9              |              |
| 2300             | 48.7             |              | 23.3              |              |
| 2450             | 52.4             |              | 24                |              |
| 2600             | 55.3             |              | 24.6              |              |
| 3000             | 63.8             |              | 25.7              |              |
| 3300             | -                |              | -                 |              |
| 3500             | 67.1             |              | 25                |              |
| 3700             | 67.4             |              | 24.2              |              |
| 3900             | -                |              | -                 |              |
| 4200             | -                |              | -                 |              |
| 4600             | -                |              | -                 |              |
| 4900             | -                |              | -                 |              |

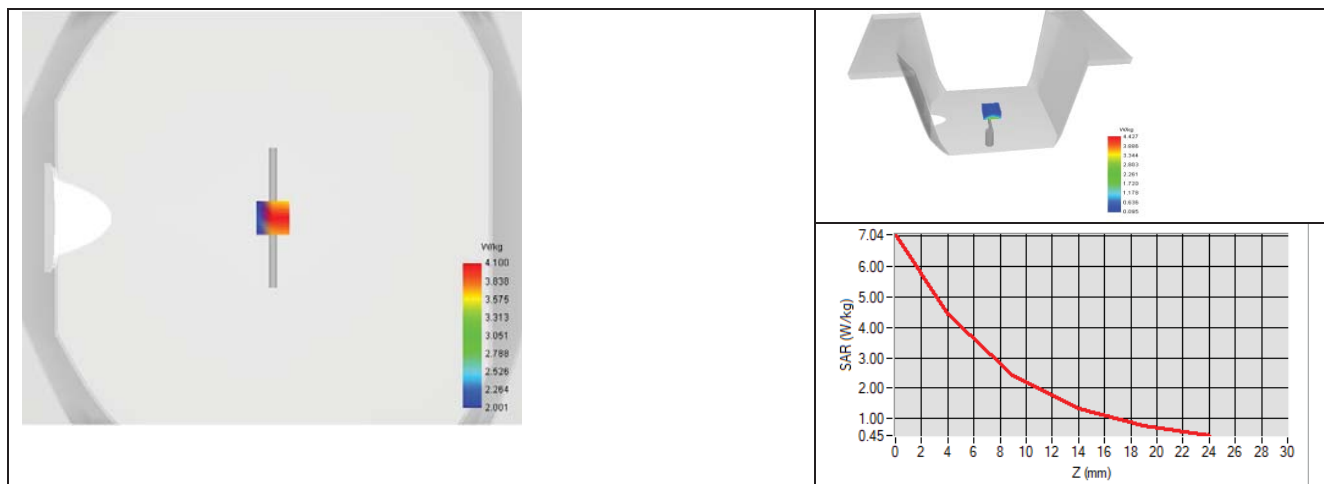


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         |          | 0.96 $\pm$ 10 %               |          |
| 835              | 55.2 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 1900             | 53.3 $\pm$ 10 %                         | 53.9     | 1.52 $\pm$ 10 %               | 1.55     |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         |          | 1.81 $\pm$ 10 %               |          |
| 2450             | 52.7 $\pm$ 10 %                         |          | 1.95 $\pm$ 10 %               |          |
| 2600             | 52.5 $\pm$ 10 %                         |          | 2.16 $\pm$ 10 %               |          |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

## 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPG0333                                         |
| Liquid                                    | Body Liquid Values: $\epsilon_{ps}'$ : 55.0 sigma : 1.57 |
| Distance between dipole center and liquid | 10.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                   |
| Frequency                                 | 1900 MHz                                                 |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 1900             | 39.01 (3.90)     | 20.62 (2.06)      |

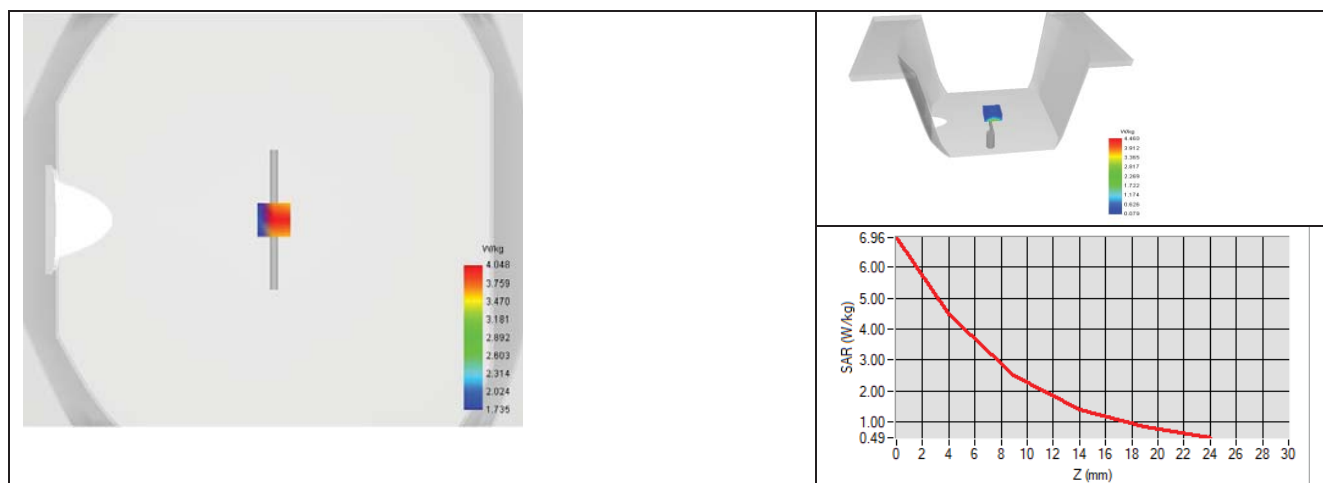



## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2022                                       | 10/2023                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2021                                       | 06/2024                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2021                                       | 06/2024                                       |

Appendix A. Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole SID1900– serial no. SN 47/12 DIP 1G900-207

| Head                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -23.41           | /         | 53.3                 | /           | 6.2                        | /            |
| 2024-08-19          | -23.62           | 4.95      | 52.8                 | 0.5         | 5.7                        | 0.5          |

| Body                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -23.40           | /         | 47.9                 | /           | 6.3                        | /            |
| 2024-08-19          | -23.58           | 4.23      | 46.8                 | 1.1         | 5.6                        | 0.7          |

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended.



## SAR Reference Dipole Calibration Report

Ref : ACR.75.7.23.SATU.A

**Waltek Testing Group (Shenzhen) Co., Ltd.**  
**1/F, Building A, Hongwei Industrial Park, Liuxian 2<sup>nd</sup> Road**  
**BAO'AN DISTRICT**  
**SHENZHEN, P.R.C. (518101)**  
**MVG COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 2300 MHZ**  
**SERIAL NO.: SN 47/12 DIP 2G300-209**

**Calibrated at MVG**  
**Z.I. de la pointe du diable**  
**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**  
**29280 PLOUZANE - FRANCE**

**Calibration date: 08/20/2023**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

### *Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>    |
|----------------------|--------------|---------------------|-------------|---------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>           |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 08/20/2023  | <i>Yann TOUTAIN</i> |

2023.08.20  
11:55:25  
+01'00'

|                       | <i>Customer Name</i>                            |
|-----------------------|-------------------------------------------------|
| <i>Distribution :</i> | Waltek Testing<br>Group (Shenzhen)<br>Co., Ltd. |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|-------------|----------------------|
| A            | Jérôme Luc  | 08/20/2023  | Initial release      |
|              |             |             |                      |
|              |             |             |                      |
|              |             |             |                      |

## TABLE OF CONTENTS

|     |                                                |    |
|-----|------------------------------------------------|----|
| 1   | Introduction.....                              | 4  |
| 2   | Device Under Test .....                        | 4  |
| 3   | Product Description .....                      | 4  |
| 3.1 | General Information .....                      | 4  |
| 4   | Measurement Method .....                       | 5  |
| 4.1 | Return Loss Requirements .....                 | 5  |
| 4.2 | Mechanical Requirements .....                  | 5  |
| 5   | Measurement Uncertainty .....                  | 5  |
| 5.1 | Return Loss .....                              | 5  |
| 5.2 | Dimension Measurement .....                    | 5  |
| 5.3 | Validation Measurement .....                   | 5  |
| 6   | Calibration Measurement Results .....          | 6  |
| 6.1 | Return Loss and Impedance In Head Liquid ..... | 6  |
| 6.2 | Return Loss and Impedance In Body Liquid ..... | 6  |
| 6.3 | Mechanical Dimensions .....                    | 7  |
| 7   | Validation measurement .....                   | 7  |
| 7.1 | Head Liquid Measurement .....                  | 8  |
| 7.2 | SAR Measurement Result With Head Liquid .....  | 8  |
| 7.3 | Body Liquid Measurement .....                  | 11 |
| 7.4 | SAR Measurement Result With Body Liquid .....  | 12 |
| 8   | List of Equipment .....                        | 13 |

## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 2300 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                               |
| Model                          | SID2300                           |
| Serial Number                  | SN 47/12 DIP 2G300-209            |
| Product Condition (new / used) | New                               |

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

## 4 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

### 4.2 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.08 LIN                            |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 0 - 300     | 0.20 mm                        |
| 300 - 450   | 0.44 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 19 % (SAR)           |
| 10 g        | 19 % (SAR)           |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

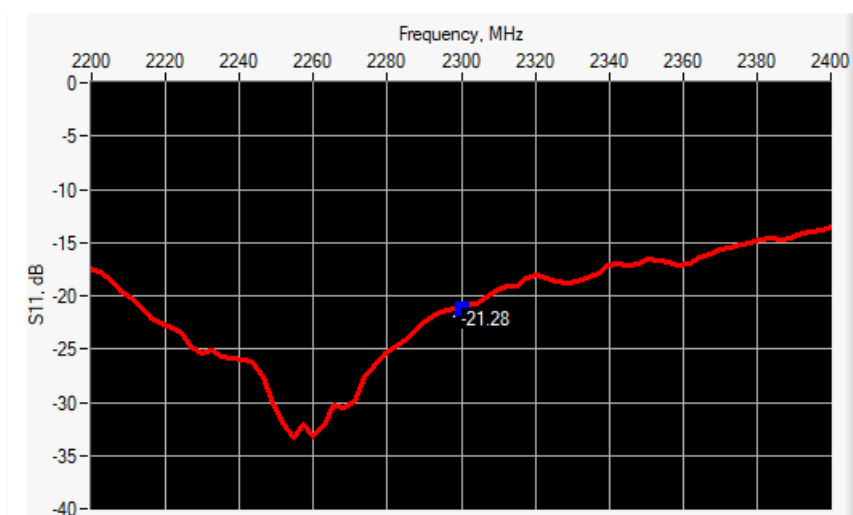

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                   |
|-----------------|------------------|------------------|-----------------------------|
| 2300            | -21.28           | -20              | $56.0 \Omega + 6.1 j\Omega$ |

### 6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

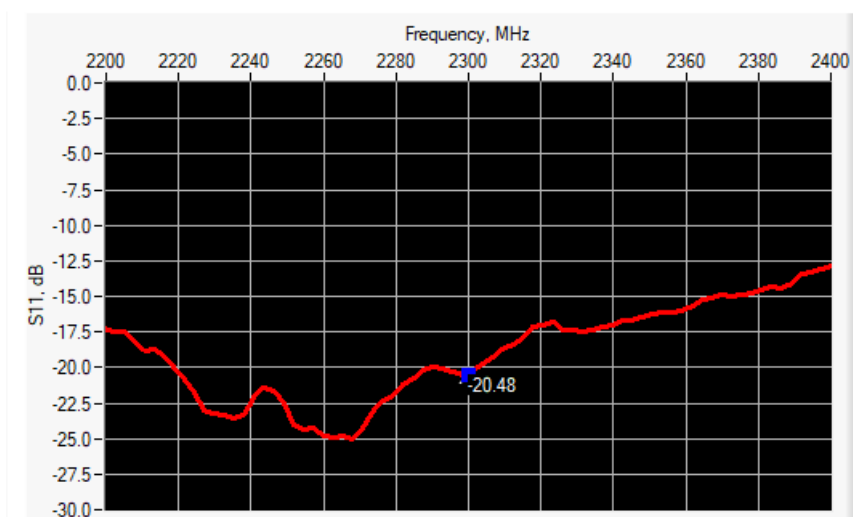

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                   |
|-----------------|------------------|------------------|-----------------------------|
| 2300            | -20.48           | -20              | $53.6 \Omega + 9.2 j\Omega$ |



### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm        |          | h mm        |          | d mm       |          |
|---------------|-------------|----------|-------------|----------|------------|----------|
|               | required    | measured | required    | measured | required   | measured |
| 300           | 420.0 ±1 %. |          | 250.0 ±1 %. |          | 6.35 ±1 %. |          |
| 450           | 290.0 ±1 %. |          | 166.7 ±1 %. |          | 6.35 ±1 %. |          |
| 750           | 176.0 ±1 %. |          | 100.0 ±1 %. |          | 6.35 ±1 %. |          |
| 835           | 161.0 ±1 %. |          | 89.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 900           | 149.0 ±1 %. |          | 83.3 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1450          | 89.1 ±1 %.  |          | 51.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1500          | 86.2 ±1 %.  |          | 50.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1640          | 79.0 ±1 %.  |          | 45.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1750          | 75.2 ±1 %.  |          | 42.9 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1800          | 72.0 ±1 %.  |          | 41.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1900          | 68.0 ±1 %.  |          | 39.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1950          | 66.3 ±1 %.  |          | 38.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2000          | 64.5 ±1 %.  |          | 37.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2100          | 61.0 ±1 %.  |          | 35.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2300          | 55.5 ±1 %.  | 55.56    | 32.6 ±1 %.  | 32.64    | 3.6 ±1 %.  | 3.62     |
| 2450          | 51.5 ±1 %.  |          | 30.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2600          | 48.5 ±1 %.  |          | 28.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3000          | 41.5 ±1 %.  |          | 25.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3300          | -           |          | -           |          | -          |          |
| 3500          | 37.0 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3700          | 34.7 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3900          | -           |          | -           |          | -          |          |
| 4200          | -           |          | -           |          | -          |          |
| 4600          | -           |          | -           |          | -          |          |
| 4900          | -           |          | -           |          | -          |          |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

## 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         |          | 0.89 $\pm$ 10 %               |          |
| 835              | 41.5 $\pm$ 10 %                         |          | 0.90 $\pm$ 10 %               |          |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1900             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         | 42.2     | 1.67 $\pm$ 10 %               | 1.75     |
| 2450             | 39.2 $\pm$ 10 %                         |          | 1.80 $\pm$ 10 %               |          |
| 2600             | 39.0 $\pm$ 10 %                         |          | 1.96 $\pm$ 10 %               |          |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |


## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.



|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPGO333                                         |
| Liquid                                    | Head Liquid Values: $\epsilon_s'$ : 37.7 $\sigma$ : 1.61 |
| Distance between dipole center and liquid | 10.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=5mm/dy=5mm/dz=5mm$                                   |
| Frequency                                 | 2300 MHz                                                 |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |              | 10 g SAR (W/kg/W) |              |
|------------------|------------------|--------------|-------------------|--------------|
|                  | required         | measured     | required          | measured     |
| 300              | 2.85             |              | 1.94              |              |
| 450              | 4.58             |              | 3.06              |              |
| 750              | 8.49             |              | 5.55              |              |
| 835              | 9.56             |              | 6.22              |              |
| 900              | 10.9             |              | 6.99              |              |
| 1450             | 29               |              | 16                |              |
| 1500             | 30.5             |              | 16.8              |              |
| 1640             | 34.2             |              | 18.4              |              |
| 1750             | 36.4             |              | 19.3              |              |
| 1800             | 38.4             |              | 20.1              |              |
| 1900             | 39.7             |              | 20.5              |              |
| 1950             | 40.5             |              | 20.9              |              |
| 2000             | 41.1             |              | 21.1              |              |
| 2100             | 43.6             |              | 21.9              |              |
| 2300             | 48.7             | 49.27 (4.93) | 23.3              | 22.91 (2.29) |
| 2450             | 52.4             |              | 24                |              |
| 2600             | 55.3             |              | 24.6              |              |
| 3000             | 63.8             |              | 25.7              |              |
| 3300             | -                |              | -                 |              |
| 3500             | 67.1             |              | 25                |              |
| 3700             | 67.4             |              | 24.2              |              |
| 3900             | -                |              | -                 |              |
| 4200             | -                |              | -                 |              |
| 4600             | -                |              | -                 |              |
| 4900             | -                |              | -                 |              |

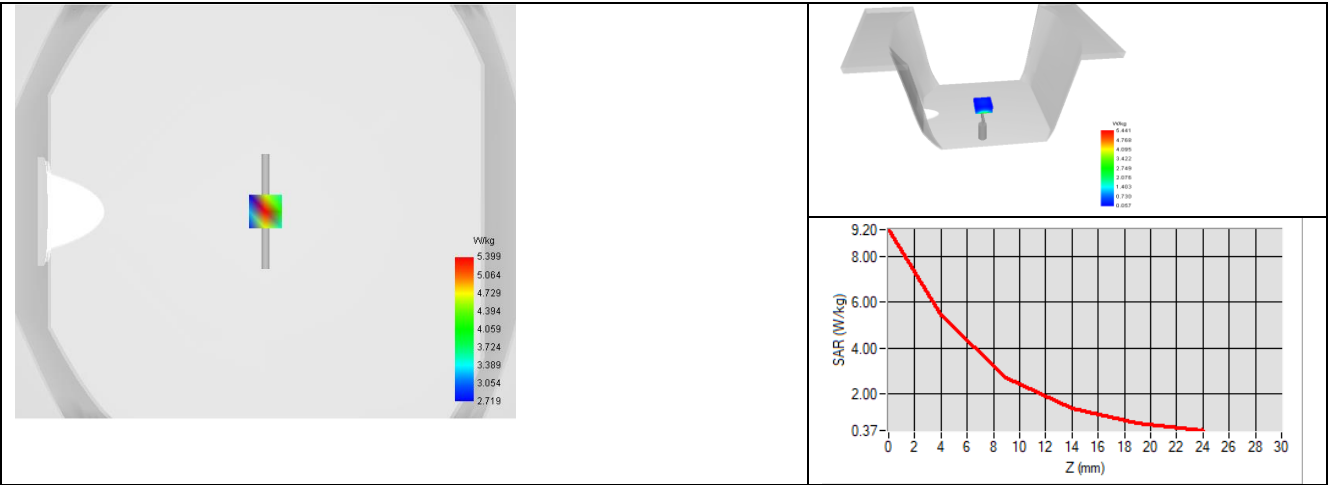


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         |          | 0.96 $\pm$ 10 %               |          |
| 835              | 55.2 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 1900             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         | 54.3     | 1.81 $\pm$ 10 %               | 1.96     |
| 2450             | 52.7 $\pm$ 10 %                         |          | 1.95 $\pm$ 10 %               |          |
| 2600             | 52.5 $\pm$ 10 %                         |          | 2.16 $\pm$ 10 %               |          |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

#### 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPGO333                                         |
| Liquid                                    | Body Liquid Values: $\epsilon_s' : 55.1$ $\sigma : 1.77$ |
| Distance between dipole center and liquid | 10.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=5mm/dy=5mm/dz=5mm$                                   |
| Frequency                                 | 2300 MHz                                                 |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 2300             | 50.42 (5.04)     | 22.61 (2.26)      |

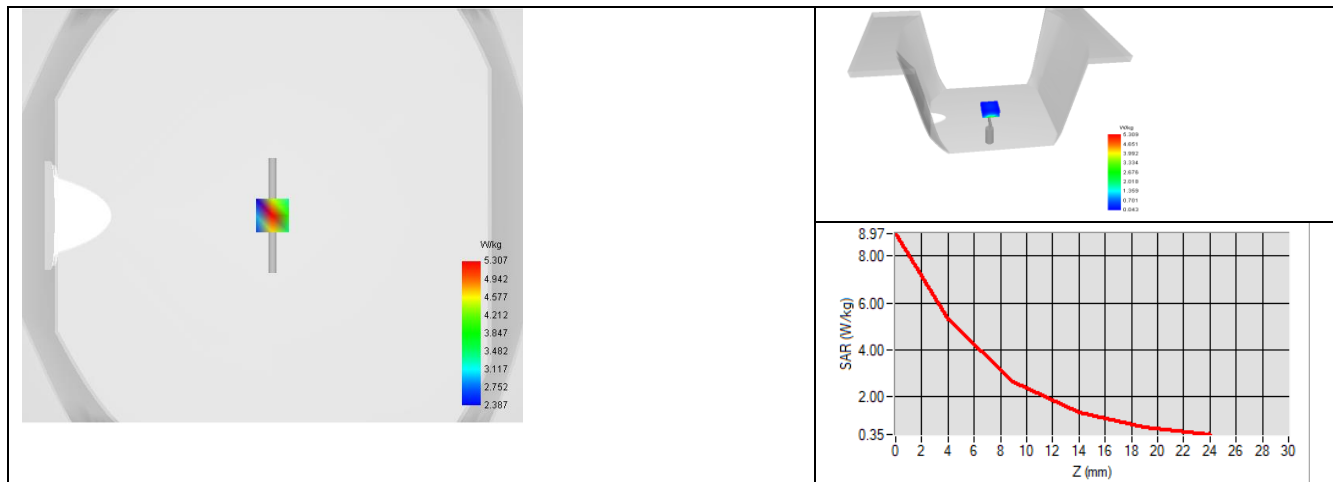



## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2022                                       | 10/2023                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2021                                       | 06/2024                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2021                                       | 06/2024                                       |

Appendix A. Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole SID2300– serial no. SN 47/12 DIP 2G300-209

| Head                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -21.28           | /         | 56.0                 | /           | 6.1                        | /            |
| 2024-08-19          | -21.57           | 6.91      | 55.6                 | 0.4         | 5.2                        | 0.9          |

| Body                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -20.48           | /         | 53.6                 | /           | 9.2                        | /            |
| 2024-08-19          | -20.72           | 5.68      | 53.9                 | 0.3         | 8.1                        | 1.1          |

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended.



## SAR Reference Dipole Calibration Report

Ref : ACR.104.1.23.SATU.A

**Waltek Testing Group (Shenzhen) Co., Ltd.**  
**1/F, Building A, Hongwei Industrial Park, Liuxian 2<sup>nd</sup> Road**  
**BAO'AN DISTRICT**  
**SHENZHEN, P.R.C. (518101)**  
**MVG COMOSAR REFERENCE DIPOLE**  
**FREQUENCY: 2450 MHZ**  
**SERIAL NO.: SN 13/15 DIP 2G450-364**

**Calibrated at MVG**  
**Z.I. de la pointe du diable**  
**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**  
**29280 PLOUZANE - FRANCE**

**Calibration date: 08/20/2023**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

### *Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>                                      |
|----------------------|--------------|---------------------|-------------|-------------------------------------------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>                                             |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 08/20/2023  | <i>JS</i>                                             |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 08/20/2023  | <i>Yann TOUTAIN</i><br>2023.08.20<br>11:56:55 +01'00' |

|                       | <i>Customer Name</i>                            |
|-----------------------|-------------------------------------------------|
| <i>Distribution :</i> | Waltek Testing<br>Group (Shenzhen)<br>Co., Ltd. |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|-------------|----------------------|
| A            | Jérôme Luc  | 08/20/2023  | Initial release      |
|              |             |             |                      |
|              |             |             |                      |
|              |             |             |                      |

## TABLE OF CONTENTS

|     |                                                |    |
|-----|------------------------------------------------|----|
| 1   | Introduction.....                              | 4  |
| 2   | Device Under Test .....                        | 4  |
| 3   | Product Description .....                      | 4  |
| 3.1 | General Information .....                      | 4  |
| 4   | Measurement Method .....                       | 5  |
| 4.1 | Return Loss Requirements .....                 | 5  |
| 4.2 | Mechanical Requirements .....                  | 5  |
| 5   | Measurement Uncertainty .....                  | 5  |
| 5.1 | Return Loss .....                              | 5  |
| 5.2 | Dimension Measurement .....                    | 5  |
| 5.3 | Validation Measurement .....                   | 5  |
| 6   | Calibration Measurement Results .....          | 6  |
| 6.1 | Return Loss and Impedance In Head Liquid ..... | 6  |
| 6.2 | Return Loss and Impedance In Body Liquid ..... | 6  |
| 6.3 | Mechanical Dimensions .....                    | 7  |
| 7   | Validation measurement .....                   | 7  |
| 7.1 | Head Liquid Measurement .....                  | 8  |
| 7.2 | SAR Measurement Result With Head Liquid .....  | 8  |
| 7.3 | Body Liquid Measurement .....                  | 11 |
| 7.4 | SAR Measurement Result With Body Liquid .....  | 12 |
| 8   | List of Equipment .....                        | 13 |

## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 2450 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                               |
| Model                          | SID2450                           |
| Serial Number                  | SN 13/15 DIP 2G450-364            |
| Product Condition (new / used) | New                               |

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

## 4 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

### 4.2 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of  $k=2$ , traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.08 LIN                            |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 0 - 300     | 0.20 mm                        |
| 300 - 450   | 0.44 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 19 % (SAR)           |
| 10 g        | 19 % (SAR)           |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

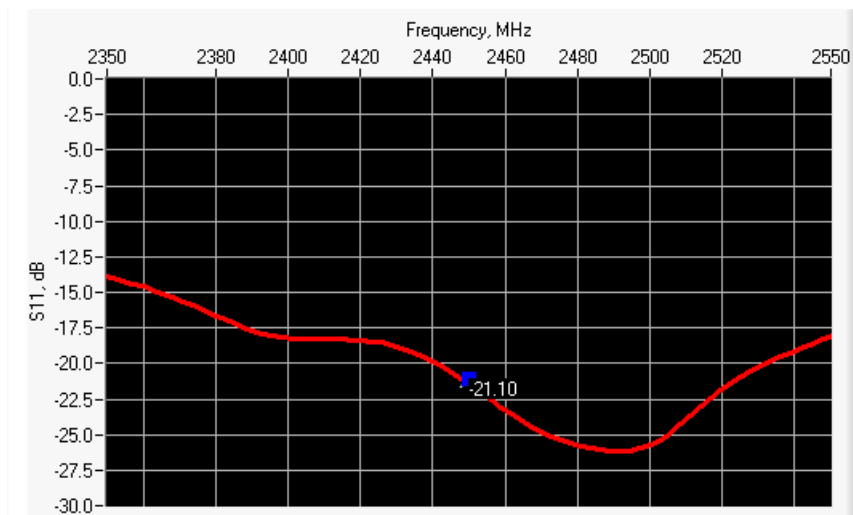

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                   |
|-----------------|------------------|------------------|-----------------------------|
| 2450            | -21.10           | -20              | $45.2 \Omega + 7.3 j\Omega$ |

### 6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

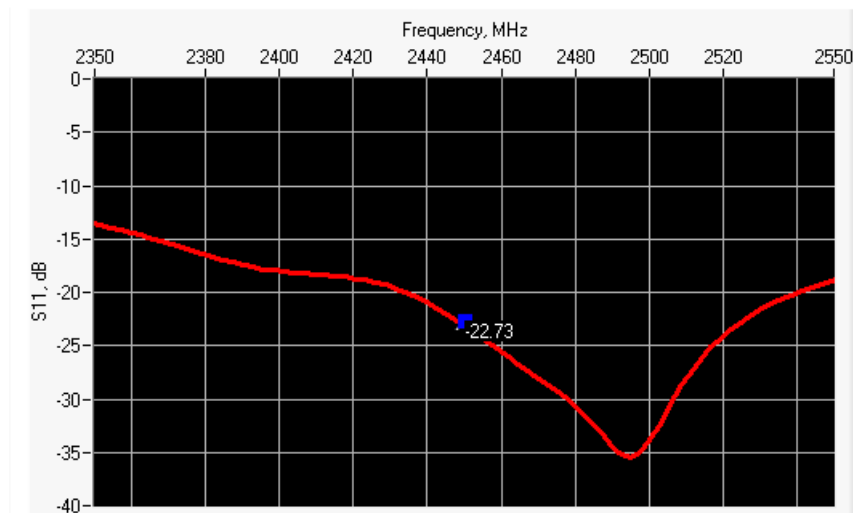

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                   |
|-----------------|------------------|------------------|-----------------------------|
| 2450            | -22.73           | -20              | $48.7 \Omega + 7.2 j\Omega$ |

### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm        |          | h mm        |          | d mm       |          |
|---------------|-------------|----------|-------------|----------|------------|----------|
|               | required    | measured | required    | measured | required   | measured |
| 300           | 420.0 ±1 %. |          | 250.0 ±1 %. |          | 6.35 ±1 %. |          |
| 450           | 290.0 ±1 %. |          | 166.7 ±1 %. |          | 6.35 ±1 %. |          |
| 750           | 176.0 ±1 %. |          | 100.0 ±1 %. |          | 6.35 ±1 %. |          |
| 835           | 161.0 ±1 %. |          | 89.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 900           | 149.0 ±1 %. |          | 83.3 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1450          | 89.1 ±1 %.  |          | 51.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1500          | 86.2 ±1 %.  |          | 50.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1640          | 79.0 ±1 %.  |          | 45.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1750          | 75.2 ±1 %.  |          | 42.9 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1800          | 72.0 ±1 %.  |          | 41.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1900          | 68.0 ±1 %.  |          | 39.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1950          | 66.3 ±1 %.  |          | 38.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2000          | 64.5 ±1 %.  |          | 37.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2100          | 61.0 ±1 %.  |          | 35.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2300          | 55.5 ±1 %.  |          | 32.6 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2450          | 51.5 ±1 %.  | 51.79    | 30.4 ±1 %.  | 30.69    | 3.6 ±1 %.  | 3.60     |
| 2600          | 48.5 ±1 %.  |          | 28.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3000          | 41.5 ±1 %.  |          | 25.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3300          | -           |          | -           |          | -          |          |
| 3500          | 37.0 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3700          | 34.7 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3900          | -           |          | -           |          | -          |          |
| 4200          | -           |          | -           |          | -          |          |
| 4600          | -           |          | -           |          | -          |          |
| 4900          | -           |          | -           |          | -          |          |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

## 7.1 HEAD LIQUID MEASUREMENT


| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         |          | 0.89 $\pm$ 10 %               |          |
| 835              | 41.5 $\pm$ 10 %                         |          | 0.90 $\pm$ 10 %               |          |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1900             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         |          | 1.67 $\pm$ 10 %               |          |
| 2450             | 39.2 $\pm$ 10 %                         | 38.9     | 1.80 $\pm$ 10 %               | 1.79     |
| 2600             | 39.0 $\pm$ 10 %                         |          | 1.96 $\pm$ 10 %               |          |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |

## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.

|                                           |                                                         |
|-------------------------------------------|---------------------------------------------------------|
| Software                                  | OPENSAR V5                                              |
| Phantom                                   | SN 13/09 SAM68                                          |
| Probe                                     | SN 41/18 EPGO333                                        |
| Liquid                                    | Head Liquid Values: $\epsilon_p$ : 38.9 $\sigma$ : 1.79 |
| Distance between dipole center and liquid | 10.0 mm                                                 |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                         |
| Zoon Scan Resolution                      | $dx=5mm/dy=5mm/dz=5mm$                                  |
| Frequency                                 | 2450 MHz                                                |
| Input power                               | 20 dBm                                                  |
| Liquid Temperature                        | 20 +/- 1 °C                                             |
| Lab Temperature                           | 20 +/- 1 °C                                             |
| Lab Humidity                              | 30-70 %                                                 |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |              | 10 g SAR (W/kg/W) |              |
|------------------|------------------|--------------|-------------------|--------------|
|                  | required         | measured     | required          | measured     |
| 300              | 2.85             |              | 1.94              |              |
| 450              | 4.58             |              | 3.06              |              |
| 750              | 8.49             |              | 5.55              |              |
| 835              | 9.56             |              | 6.22              |              |
| 900              | 10.9             |              | 6.99              |              |
| 1450             | 29               |              | 16                |              |
| 1500             | 30.5             |              | 16.8              |              |
| 1640             | 34.2             |              | 18.4              |              |
| 1750             | 36.4             |              | 19.3              |              |
| 1800             | 38.4             |              | 20.1              |              |
| 1900             | 39.7             |              | 20.5              |              |
| 1950             | 40.5             |              | 20.9              |              |
| 2000             | 41.1             |              | 21.1              |              |
| 2100             | 43.6             |              | 21.9              |              |
| 2300             | 48.7             |              | 23.3              |              |
| 2450             | 52.4             | 53.76 (5.38) | 24                | 24.32 (2.43) |
| 2600             | 55.3             |              | 24.6              |              |
| 3000             | 63.8             |              | 25.7              |              |
| 3300             | -                |              | -                 |              |
| 3500             | 67.1             |              | 25                |              |
| 3700             | 67.4             |              | 24.2              |              |
| 3900             | -                |              | -                 |              |
| 4200             | -                |              | -                 |              |
| 4600             | -                |              | -                 |              |
| 4900             | -                |              | -                 |              |

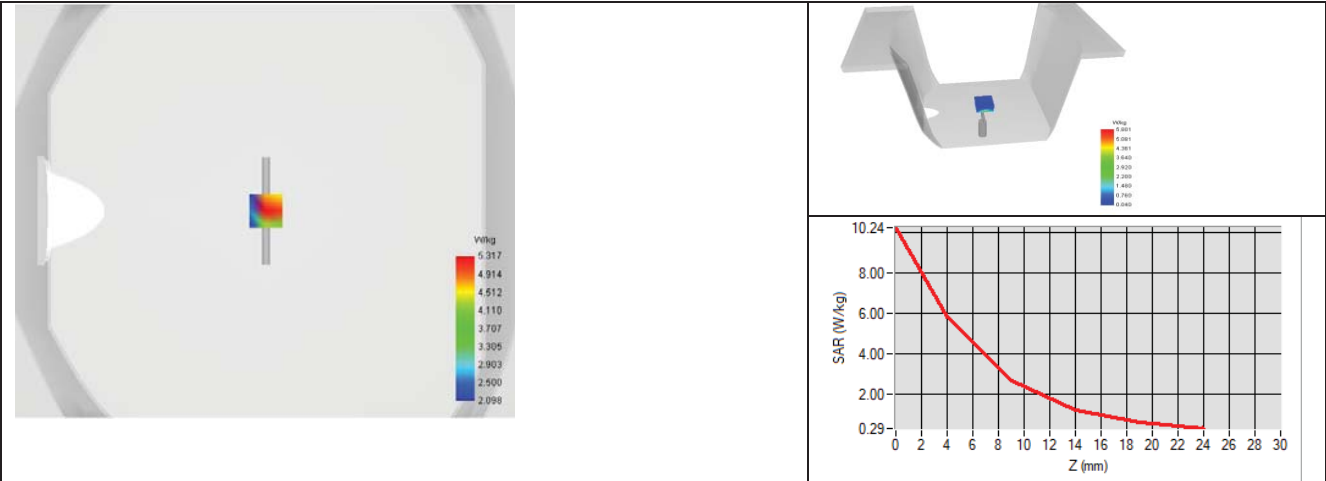


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         |          | 0.96 $\pm$ 10 %               |          |
| 835              | 55.2 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 1900             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         |          | 1.81 $\pm$ 10 %               |          |
| 2450             | 52.7 $\pm$ 10 %                         | 52.7     | 1.95 $\pm$ 10 %               | 1.94     |
| 2600             | 52.5 $\pm$ 10 %                         |          | 2.16 $\pm$ 10 %               |          |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

## 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPG0333                                         |
| Liquid                                    | Body Liquid Values: $\epsilon_s' : 52.7$ $\sigma : 1.94$ |
| Distance between dipole center and liquid | 10.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=5mm/dy=5mm/dz=5mm$                                   |
| Frequency                                 | 2450 MHz                                                 |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 2450             | 50.33 (5.03)     | 23.38 (2.34)      |

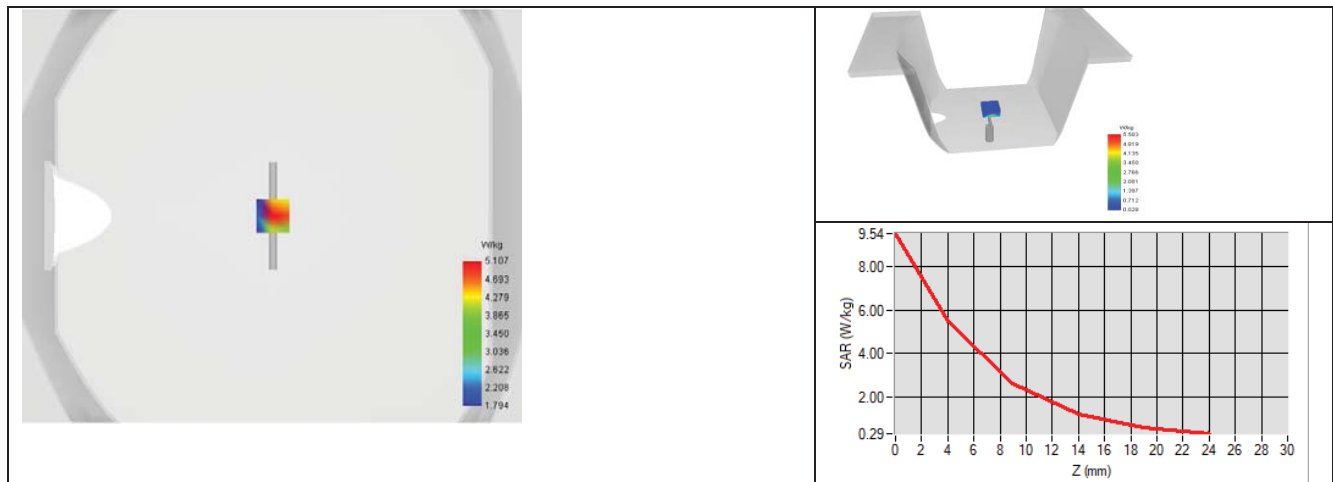



## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2022                                       | 10/2023                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2021                                       | 06/2024                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2021                                       | 06/2024                                       |

Appendix A. Extended Calibration SAR Dipole

Referring to KDB865664 D01, if dipoles are verified in return loss (<-20dBm, within 20% of prior calibration), and in impedance (within 5 ohm of prior calibration), the annual calibration is not necessary and the calibration interval can be extended.

Justification of Extended Calibration SAR Dipole SID2450– serial no. SN 1/315 DIP 2G450-364

| Head                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -21.10           | /         | 45.2                 | /           | 7.3                        | /            |
| 2024-08-19          | -21.32           | 5.20      | 46.4                 | 1.2         | 6.2                        | 1.1          |

| Body                |                  |           |                      |             |                            |              |
|---------------------|------------------|-----------|----------------------|-------------|----------------------------|--------------|
| Date of Measurement | Return-Loss (dB) | Delta (%) | Real Impedance (ohm) | Delta (ohm) | Imaginary Impedance (johm) | Delta (johm) |
| 2023-08-20          | -22.73           | /         | 48.7                 | /           | 7.2                        | /            |
| 2024-08-19          | -22.48           | 5.59      | 48.1                 | 0.6         | 6.3                        | 0.9          |

The Return-Loss is <-20dB, and within 20% of prior calibration; the impedance is within 5 ohm of prior calibration. Therefore the value result should support extended.



## SAR Reference Dipole Calibration Report

Ref : ACR.200.3.24.BES.B

Cancel and replace the report ACR.200.3.24.BES.A

### **WALTEK TESTING GROUP (SHENZHEN) CO., LTD**

**1/F., ROOM 101, BUILDING 1, HONGWEI INDUSTRIAL  
PARK, LIUXIAN 2ND ROAD, BLOCK 70  
BAO'AN DISTRICT, SHENZHEN, GUANGDONG , CHINA  
MVG COMOSAR REFERENCE DIPOLE**

**FREQUENCY: 2600 MHZ**

**SERIAL NO.: SN 28/21 DIP 2G600-590**

**Calibrated at MVG**

**Z.I. de la pointe du diable**

**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**

**29280 PLOUZANE - FRANCE**

**Calibration date: 07/11/2024**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

#### *Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>    |
|----------------------|--------------|---------------------|-------------|---------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 7/11/2024   | <i>JS</i>           |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 7/11/2024   | <i>JS</i>           |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 7/15/2024   | <i>Yann TOUTAIN</i> |

2024.07.11  
15:51:25 +01'05'

|                       | <i>Customer Name</i>                           |
|-----------------------|------------------------------------------------|
| <i>Distribution :</i> | Waltek Testing<br>Group (Shenzhen)<br>Co., Ltd |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i>         |
|--------------|-------------|-------------|------------------------------|
| A            | Jérôme Luc  | 7/11/2024   | Initial release              |
| B            | Jérôme Luc  | 7/12/2024   | Change customer name/address |
|              |             |             |                              |
|              |             |             |                              |

## TABLE OF CONTENTS

|     |                                                |    |
|-----|------------------------------------------------|----|
| 1   | Introduction.....                              | 4  |
| 2   | Device Under Test .....                        | 4  |
| 3   | Product Description .....                      | 4  |
| 3.1 | General Information .....                      | 4  |
| 4   | Measurement Method .....                       | 5  |
| 4.1 | Return Loss Requirements .....                 | 5  |
| 4.2 | Mechanical Requirements.....                   | 5  |
| 5   | Measurement Uncertainty.....                   | 5  |
| 5.1 | Return Loss .....                              | 5  |
| 5.2 | Dimension Measurement .....                    | 5  |
| 5.3 | Validation Measurement.....                    | 5  |
| 6   | Calibration Measurement Results.....           | 6  |
| 6.1 | Return Loss and Impedance In Head Liquid ..... | 6  |
| 6.2 | Return Loss and Impedance In Body Liquid ..... | 6  |
| 6.3 | Mechanical Dimensions .....                    | 7  |
| 7   | Validation measurement .....                   | 7  |
| 7.1 | Head Liquid Measurement .....                  | 8  |
| 7.2 | SAR Measurement Result With Head Liquid.....   | 8  |
| 7.3 | Body Liquid Measurement .....                  | 11 |
| 7.4 | SAR Measurement Result With Body Liquid .....  | 12 |
| 8   | List of Equipment .....                        | 13 |

## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                   |
|--------------------------------|-----------------------------------|
| Device Type                    | COMOSAR 2600 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                               |
| Model                          | SID2600                           |
| Serial Number                  | SN 28/21 DIP 2G600-590            |
| Product Condition (new / used) | New                               |

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

## 4 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

### 4.2 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.08 LIN                            |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 0 - 300     | 0.20 mm                        |
| 300 - 450   | 0.44 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 19 % (SAR)           |
| 10 g        | 19 % (SAR)           |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS AND IMPEDANCE IN HEAD LIQUID

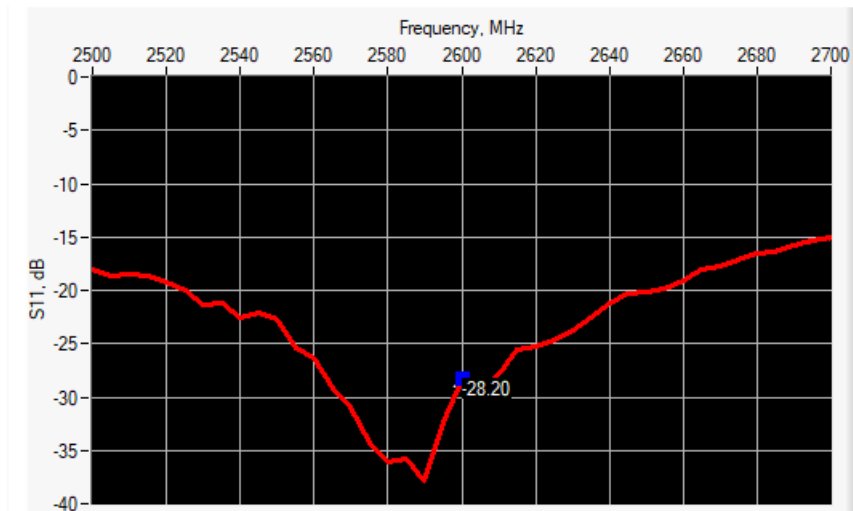

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                   |
|-----------------|------------------|------------------|-----------------------------|
| 2600            | -28.20           | -20              | $52.7 \Omega + 2.8 j\Omega$ |

### 6.2 RETURN LOSS AND IMPEDANCE IN BODY LIQUID

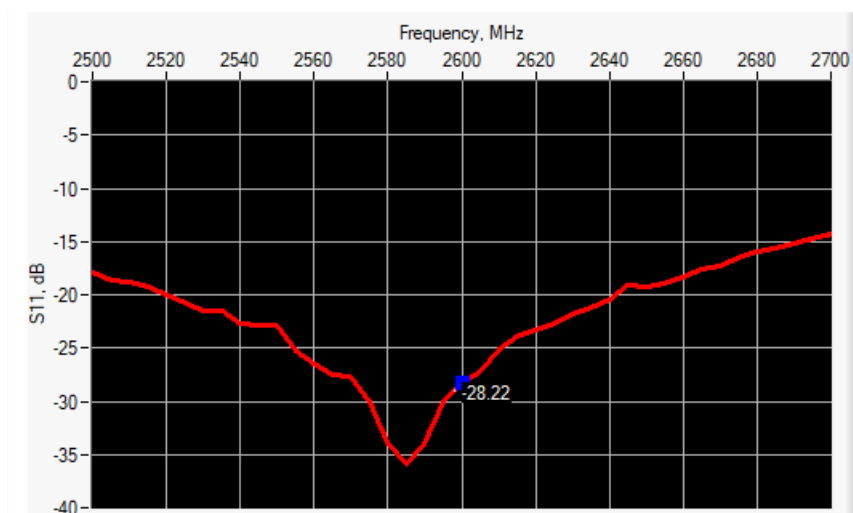

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                   |
|-----------------|------------------|------------------|-----------------------------|
| 2600            | -28.22           | -20              | $49.5 \Omega + 3.8 j\Omega$ |

### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm        |          | h mm        |          | d mm       |          |
|---------------|-------------|----------|-------------|----------|------------|----------|
|               | required    | measured | required    | measured | required   | measured |
| 300           | 420.0 ±1 %. |          | 250.0 ±1 %. |          | 6.35 ±1 %. |          |
| 450           | 290.0 ±1 %. |          | 166.7 ±1 %. |          | 6.35 ±1 %. |          |
| 750           | 176.0 ±1 %. |          | 100.0 ±1 %. |          | 6.35 ±1 %. |          |
| 835           | 161.0 ±1 %. |          | 89.8 ±1 %.  |          | 3.6 ±1 %.  |          |
| 900           | 149.0 ±1 %. |          | 83.3 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1450          | 89.1 ±1 %.  |          | 51.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1500          | 80.5 ±1 %.  |          | 50.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1640          | 79.0 ±1 %.  |          | 45.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1750          | 75.2 ±1 %.  |          | 42.9 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1800          | 72.0 ±1 %.  |          | 41.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1900          | 68.0 ±1 %.  |          | 39.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 1950          | 66.3 ±1 %.  |          | 38.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2000          | 64.5 ±1 %.  |          | 37.5 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2100          | 61.0 ±1 %.  |          | 35.7 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2300          | 55.5 ±1 %.  |          | 32.6 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2450          | 51.5 ±1 %.  |          | 30.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 2600          | 48.5 ±1 %.  | 48.79    | 28.8 ±1 %.  | 28.60    | 3.6 ±1 %.  | 3.61     |
| 3000          | 41.5 ±1 %.  |          | 25.0 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3300          | -           |          | -           |          | -          |          |
| 3500          | 37.0 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3700          | 34.7 ±1 %.  |          | 26.4 ±1 %.  |          | 3.6 ±1 %.  |          |
| 3900          | -           |          | -           |          | -          |          |
| 4200          | -           |          | -           |          | -          |          |
| 4600          | -           |          | -           |          | -          |          |
| 4900          | -           |          | -           |          | -          |          |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

## 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         |          | 0.89 $\pm$ 10 %               |          |
| 835              | 41.5 $\pm$ 10 %                         |          | 0.90 $\pm$ 10 %               |          |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1900             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         |          | 1.67 $\pm$ 10 %               |          |
| 2450             | 39.2 $\pm$ 10 %                         |          | 1.80 $\pm$ 10 %               |          |
| 2600             | 39.0 $\pm$ 10 %                         | 41.5     | 1.96 $\pm$ 10 %               | 2.03     |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |


## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.



|                                           |                                                         |
|-------------------------------------------|---------------------------------------------------------|
| Software                                  | OPENSAR V5                                              |
| Phantom                                   | SN 13/09 SAM68                                          |
| Probe                                     | SN 41/18 EPGO333                                        |
| Liquid                                    | Head Liquid Values: $\epsilon_p$ : 41.5 $\sigma$ : 2.03 |
| Distance between dipole center and liquid | 10.0 mm                                                 |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                         |
| Zoon Scan Resolution                      | $dx=5mm/dy=5mm/dz=5mm$                                  |
| Frequency                                 | 2600 MHz                                                |
| Input power                               | 20 dBm                                                  |
| Liquid Temperature                        | 20 +/- 1 °C                                             |
| Lab Temperature                           | 20 +/- 1 °C                                             |
| Lab Humidity                              | 30-70 %                                                 |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |              | 10 g SAR (W/kg/W) |              |
|------------------|------------------|--------------|-------------------|--------------|
|                  | required         | measured     | required          | measured     |
| 300              | 2.85             |              | 1.94              |              |
| 450              | 4.58             |              | 3.06              |              |
| 750              | 8.49             |              | 5.55              |              |
| 835              | 9.56             |              | 6.22              |              |
| 900              | 10.9             |              | 6.99              |              |
| 1450             | 29               |              | 16                |              |
| 1500             | 30.5             |              | 16.8              |              |
| 1640             | 34.2             |              | 18.4              |              |
| 1750             | 36.4             |              | 19.3              |              |
| 1800             | 38.4             |              | 20.1              |              |
| 1900             | 39.7             |              | 20.5              |              |
| 1950             | 40.5             |              | 20.9              |              |
| 2000             | 41.1             |              | 21.1              |              |
| 2100             | 43.6             |              | 21.9              |              |
| 2300             | 48.7             |              | 23.3              |              |
| 2450             | 52.4             |              | 24                |              |
| 2600             | 55.3             | 56.81 (5.68) | 24.6              | 24.63 (2.46) |
| 3000             | 63.8             |              | 25.7              |              |
| 3300             | -                |              | -                 |              |
| 3500             | 67.1             |              | 25                |              |
| 3700             | 67.4             |              | 24.2              |              |
| 3900             | -                |              | -                 |              |
| 4200             | -                |              | -                 |              |
| 4600             | -                |              | -                 |              |
| 4900             | -                |              | -                 |              |

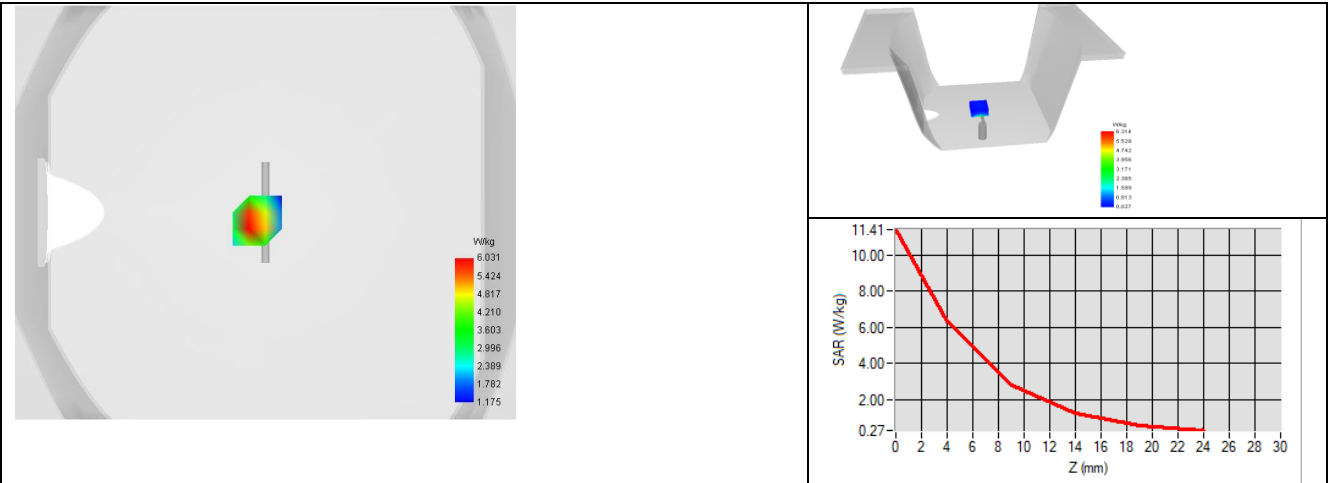


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         |          | 0.96 $\pm$ 10 %               |          |
| 835              | 55.2 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 1900             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         |          | 1.81 $\pm$ 10 %               |          |
| 2450             | 52.7 $\pm$ 10 %                         |          | 1.95 $\pm$ 10 %               |          |
| 2600             | 52.5 $\pm$ 10 %                         | 52.7     | 2.16 $\pm$ 10 %               | 2.36     |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

## 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                      |
|-------------------------------------------|------------------------------------------------------|
| Software                                  | OPENSAR V5                                           |
| Phantom                                   | SN 13/09 SAM68                                       |
| Probe                                     | SN 41/18 EPGO333                                     |
| Liquid                                    | Body Liquid Values: $\epsilon_s$ : 52.7 sigma : 2.36 |
| Distance between dipole center and liquid | 10.0 mm                                              |
| Area scan resolution                      | dx=8mm/dy=8mm                                        |
| Zoon Scan Resolution                      | dx=5mm/dy=5mm/dz=5mm                                 |
| Frequency                                 | 2600 MHz                                             |
| Input power                               | 20 dBm                                               |
| Liquid Temperature                        | 20 +/- 1 °C                                          |
| Lab Temperature                           | 20 +/- 1 °C                                          |
| Lab Humidity                              | 30-70 %                                              |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 2600             | 55.79 (5.58)     | 23.42 (2.34)      |

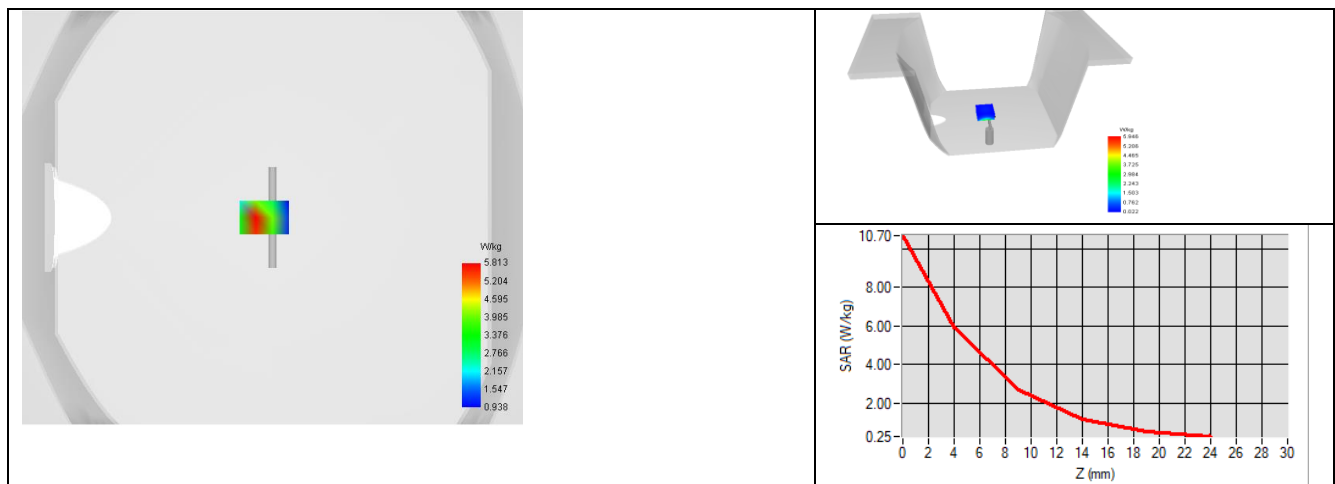



## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2023                                       | 10/2024                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2024                                       | 06/2027                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2024                                       | 06/2027                                       |



## SAR Reference Dipole Calibration Report

Ref : ACR.202.4.24.BES.B

Cancel and replace the report ACR.202.4.24.BES.A

### **WALTEK TESTING GROUP (SHENZHEN) CO., LTD**

**1/F., ROOM 101, BUILDING 1, HONGWEI INDUSTRIAL  
PARK, LIUXIAN 2ND ROAD, BLOCK 70  
BAO'AN DISTRICT, SHENZHEN, GUANGDONG , CHINA  
MVG COMOSAR REFERENCE DIPOLE**

**FREQUENCY: 5200-5800 MHZ**

**SERIAL NO.: SN 02/21 DIP 5G000-543**

**Calibrated at MVG**

**Z.I. de la pointe du diable**

**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**

**29280 PLOUZANE - FRANCE**

**Calibration date: 07/11/2024**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

#### *Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed at MVG, using the COMOSAR test bench. The test results covered by accreditation are traceable to the International System of Units (SI).



|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>    |
|----------------------|--------------|---------------------|-------------|---------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 7/11/2024   | <i>JS</i>           |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 7/11/2024   | <i>JS</i>           |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 7/11/2024   | <i>Yann TOUTAIN</i> |

2024.07.11

15:51:25 +01'05'

|                       | <i>Customer Name</i>                           |
|-----------------------|------------------------------------------------|
| <i>Distribution :</i> | Waltek Testing<br>Group (Shenzhen)<br>Co., Ltd |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|-------------|----------------------|
| A            | Jérôme Luc  | 7/11/2024   | Initial release      |
|              |             |             |                      |
|              |             |             |                      |
|              |             |             |                      |

## TABLE OF CONTENTS

|     |                                               |    |
|-----|-----------------------------------------------|----|
| 1   | Introduction.....                             | 4  |
| 2   | Device Under Test .....                       | 4  |
| 3   | Product Description .....                     | 4  |
| 3.1 | General Information .....                     | 4  |
| 4   | Measurement Method .....                      | 5  |
| 4.1 | Return Loss Requirements .....                | 5  |
| 4.2 | Mechanical Requirements.....                  | 5  |
| 5   | Measurement Uncertainty.....                  | 5  |
| 5.1 | Return Loss .....                             | 5  |
| 5.2 | Dimension Measurement .....                   | 5  |
| 5.3 | Validation Measurement.....                   | 5  |
| 6   | Calibration Measurement Results.....          | 6  |
| 6.1 | Return Loss In Head Liquid .....              | 6  |
| 6.2 | Return Loss In Body Liquid .....              | 6  |
| 6.3 | Mechanical Dimensions .....                   | 7  |
| 7   | Validation measurement .....                  | 7  |
| 7.1 | Head Liquid Measurement .....                 | 7  |
| 7.2 | SAR Measurement Result With Head Liquid.....  | 8  |
| 7.3 | Body Liquid Measurement .....                 | 11 |
| 7.4 | SAR Measurement Result With Body Liquid ..... | 11 |
| 8   | List of Equipment .....                       | 14 |

## 1 INTRODUCTION

This document contains a summary of the requirements set forth by the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards for reference dipoles used for SAR measurement system validations and the measurements that were performed to verify that the product complies with the fore mentioned standards.

## 2 DEVICE UNDER TEST

| Device Under Test              |                                        |
|--------------------------------|----------------------------------------|
| Device Type                    | COMOSAR 5200-5800 MHz REFERENCE DIPOLE |
| Manufacturer                   | MVG                                    |
| Model                          | SID5000                                |
| Serial Number                  | SN 02/21 DIP 5G000-543                 |
| Product Condition (new / used) | New                                    |

## 3 PRODUCT DESCRIPTION

### 3.1 GENERAL INFORMATION

MVG's COMOSAR Validation Dipoles are built in accordance to the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards. The product is designed for use with the COMOSAR test bench only.



**Figure 1 – MVG COMOSAR Validation Dipole**

## 4 MEASUREMENT METHOD

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards provide requirements for reference dipoles used for system validation measurements. The following measurements were performed to verify that the product complies with the fore mentioned standards.

### 4.1 RETURN LOSS REQUIREMENTS

The dipole used for SAR system validation measurements and checks must have a return loss of -20 dB or better. The return loss measurement shall be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. A direct method is used with a network analyser and its calibration kit, both with a valid ISO17025 calibration.

### 4.2 MECHANICAL REQUIREMENTS

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards specify the mechanical components and dimensions of the validation dipoles, with the dimension's frequency and phantom shell thickness dependent. The COMOSAR test bench employs a 2 mm phantom shell thickness therefore the dipoles sold for use with the COMOSAR test bench comply with the requirements set forth for a 2 mm phantom shell thickness. A direct method is used with a ISO17025 calibrated caliper.

## 5 MEASUREMENT UNCERTAINTY

All uncertainties listed below represent an expanded uncertainty expressed at approximately the 95% confidence level using a coverage factor of k=2, traceable to the Internationally Accepted Guides to Measurement Uncertainty.

### 5.1 RETURN LOSS

The following uncertainties apply to the return loss measurement:

| Frequency band | Expanded Uncertainty on Return Loss |
|----------------|-------------------------------------|
| 400-6000MHz    | 0.08 LIN                            |

### 5.2 DIMENSION MEASUREMENT

The following uncertainties apply to the dimension measurements:

| Length (mm) | Expanded Uncertainty on Length |
|-------------|--------------------------------|
| 0 - 300     | 0.20 mm                        |


### 5.3 VALIDATION MEASUREMENT

The guidelines outlined in the IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards were followed to generate the measurement uncertainty for validation measurements.

| Scan Volume | Expanded Uncertainty |
|-------------|----------------------|
| 1 g         | 19 % (SAR)           |
| 10 g        | 19 % (SAR)           |


## 6 CALIBRATION MEASUREMENT RESULTS

### 6.1 RETURN LOSS IN HEAD LIQUID

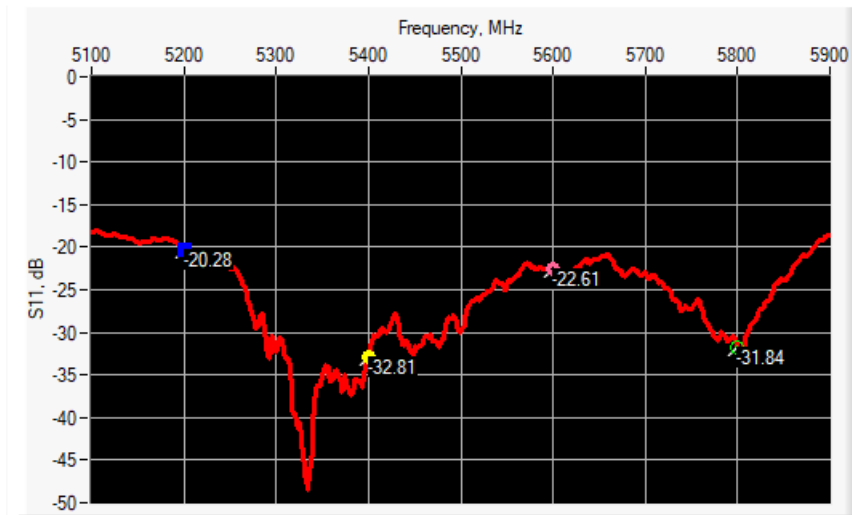

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                        |
|-----------------|------------------|------------------|----------------------------------|
| 5200            | -20.28           | -20              | 50.15 $\Omega$ - 9.64 j $\Omega$ |
| 5400            | -32.81           | -20              | 52.29 $\Omega$ - 0.09 j $\Omega$ |
| 5600            | -22.61           | -20              | 53.96 $\Omega$ - 6.22 j $\Omega$ |
| 5800            | -31.84           | -20              | 49.17 $\Omega$ + 2.42 j $\Omega$ |

### 6.2 RETURN LOSS IN BODY LIQUID

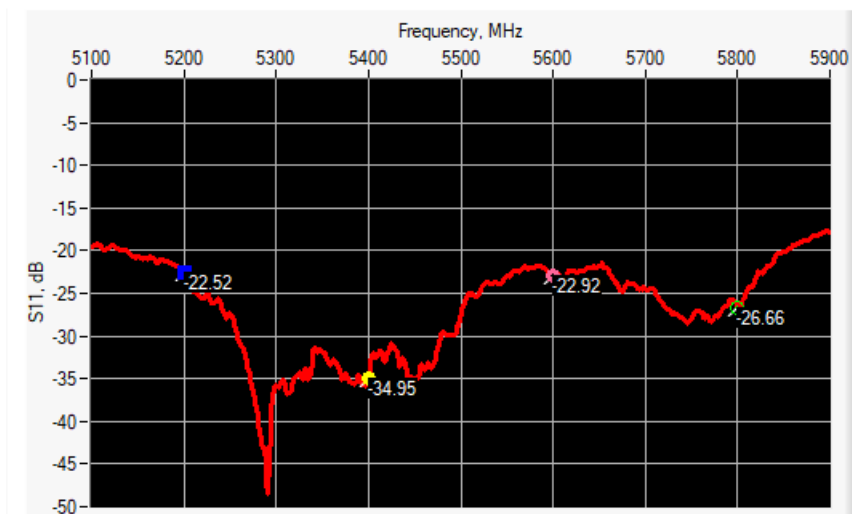

| Frequency (MHz) | Return Loss (dB) | Requirement (dB) | Impedance                        |
|-----------------|------------------|------------------|----------------------------------|
| 5200            | -22.52           | -20              | 50.89 $\Omega$ - 7.40 j $\Omega$ |
| 5400            | -34.95           | -20              | 51.59 $\Omega$ + 0.81 j $\Omega$ |
| 5600            | -22.92           | -20              | 56.03 $\Omega$ - 3.77 j $\Omega$ |
| 5800            | -26.66           | -20              | 49.02 $\Omega$ + 4.53 j $\Omega$ |

### 6.3 MECHANICAL DIMENSIONS

| Frequency MHz | L mm           |          | h mm           |          | d mm          |          |
|---------------|----------------|----------|----------------|----------|---------------|----------|
|               | required       | measured | required       | measured | required      | measured |
| 5000 to 6000  | 20.6 $\pm$ 1 % | 20.78    | 40.3 $\pm$ 1 % | 40.41    | 3.6 $\pm$ 1 % | 3.58     |

## 7 VALIDATION MEASUREMENT

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements must be performed using a reference dipole meeting the fore mentioned return loss and mechanical dimension requirements. The validation measurement must be performed against a liquid filled flat phantom, with the phantom constructed as outlined in the fore mentioned standards. Per the standards, the dipole shall be positioned below the bottom of the phantom, with the dipole length centered and parallel to the longest dimension of the flat phantom, with the top surface of the dipole at the described distance from the bottom surface of the phantom.

### 7.1 HEAD LIQUID MEASUREMENT

| Frequency MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|---------------|-----------------------------------------|----------|-------------------------------|----------|
|               | required                                | measured | required                      | measured |
| 5000          | 36.2 $\pm$ 10 %                         |          | 4.45 $\pm$ 10 %               |          |
| 5100          | 36.1 $\pm$ 10 %                         |          | 4.56 $\pm$ 10 %               |          |
| 5200          | 36.0 $\pm$ 10 %                         | 34.06    | 4.66 $\pm$ 10 %               | 4.70     |
| 5300          | 35.9 $\pm$ 10 %                         |          | 4.76 $\pm$ 10 %               |          |
| 5400          | 35.8 $\pm$ 10 %                         | 33.39    | 4.86 $\pm$ 10 %               | 4.91     |
| 5500          | 35.6 $\pm$ 10 %                         |          | 4.97 $\pm$ 10 %               |          |
| 5600          | 35.5 $\pm$ 10 %                         | 32.77    | 5.07 $\pm$ 10 %               | 5.13     |
| 5700          | 35.4 $\pm$ 10 %                         |          | 5.17 $\pm$ 10 %               |          |
| 5800          | 35.3 $\pm$ 10 %                         | 32.40    | 5.27 $\pm$ 10 %               | 5.34     |
| 5900          | 35.2 $\pm$ 10 %                         |          | 5.38 $\pm$ 10 %               |          |
| 6000          | 35.1 $\pm$ 10 %                         |          | 5.48 $\pm$ 10 %               |          |


## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

At those frequencies, the target SAR value can not be generic. Hereunder is the target SAR value defined by MVG, within the uncertainty for the system validation. All SAR values are normalized to 1 W net power. In bracket, the measured SAR is given with the used input power.


|                                    |                                                                                                                                                                                                                                  |
|------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Software                           | OPENSAR V5                                                                                                                                                                                                                       |
| Phantom                            | SN 13/09 SAM68                                                                                                                                                                                                                   |
| Probe                              | SN 41/18 EPGO333                                                                                                                                                                                                                 |
| Liquid                             | Head Liquid Values 5200 MHz: eps' :34.06 sigma : 4.70<br>Head Liquid Values 5400 MHz: eps' :33.39 sigma : 4.91<br>Head Liquid Values 5600 MHz: eps' :32.77 sigma : 5.13<br>Head Liquid Values 5800 MHz: eps' :32.40 sigma : 5.34 |
| Distance between dipole and liquid | 10 mm                                                                                                                                                                                                                            |
| Area scan resolution               | dx=8mm/dy=8mm                                                                                                                                                                                                                    |
| Zoon Scan Resolution               | dx=4mm/dy=4m/dz=2mm                                                                                                                                                                                                              |
| Frequency                          | 5200 MHz<br>5400 MHz<br>5600 MHz<br>5800 MHz                                                                                                                                                                                     |
| Input power                        | 20 dBm                                                                                                                                                                                                                           |
| Liquid Temperature                 | 20 +/- 1 °C                                                                                                                                                                                                                      |
| Lab Temperature                    | 20 +/- 1 °C                                                                                                                                                                                                                      |
| Lab Humidity                       | 30-70 %                                                                                                                                                                                                                          |

| Frequency (MHz) | 1 g SAR (W/kg) |              | 10 g SAR (W/kg) |              |
|-----------------|----------------|--------------|-----------------|--------------|
|                 | required       | measured     | required        | measured     |
| 5200            | 76.50          | 75.31 (7.53) | 21.60           | 22.23 (2.22) |
| 5400            | -              | 79.56 (7.96) | -               | 23.40 (2.34) |
| 5600            | -              | 78.31 (7.83) | -               | 23.25 (2.33) |
| 5800            | 78.00          | 78.05 (7.80) | 21.90           | 22.86 (2.29) |


## SAR MEASUREMENT PLOTS @ 5200 MHz

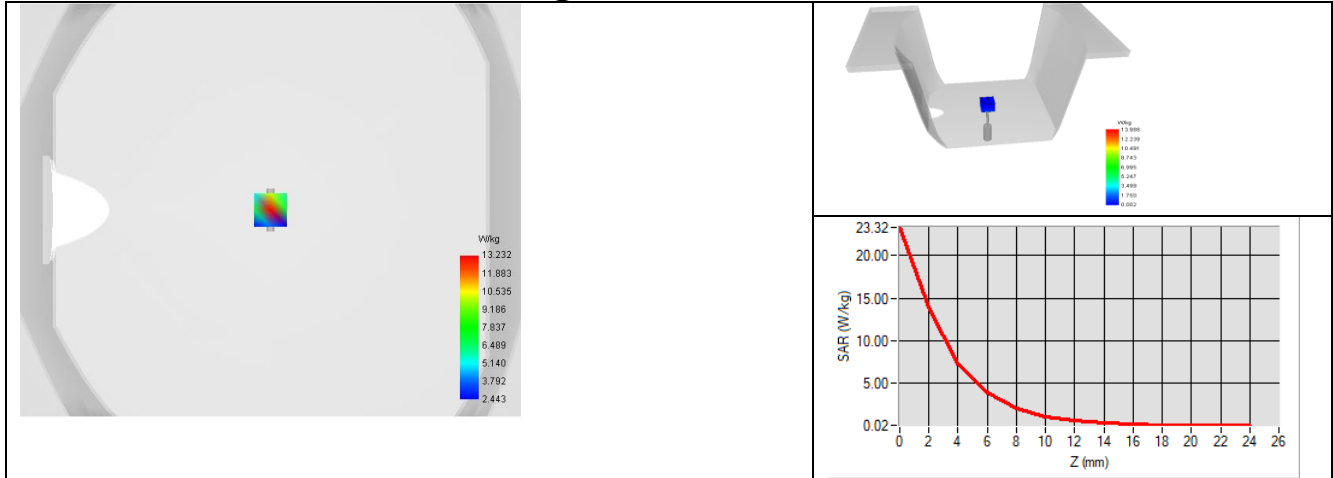


## SAR MEASUREMENT PLOTS @ 5400 MHz

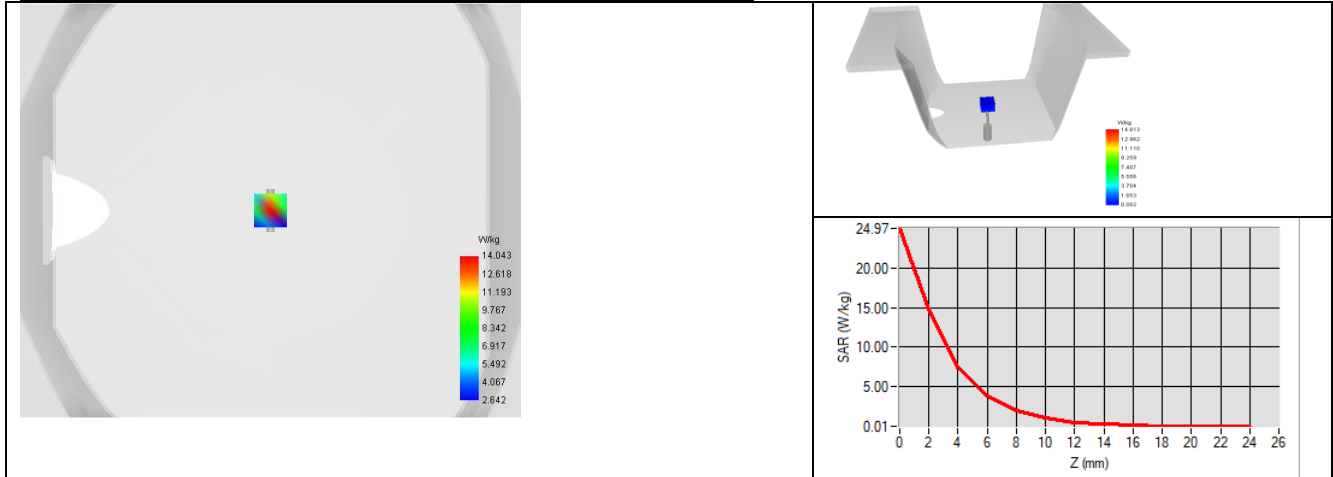

## SAR MEASUREMENT PLOTS @ 5600 MHz

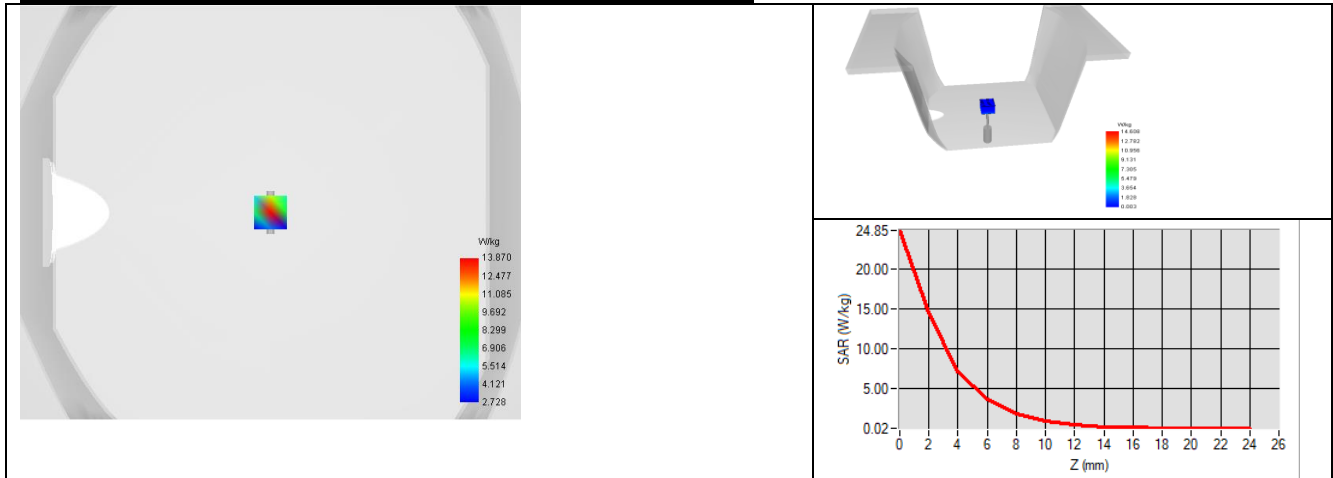

# SAR MEASUREMENT PLOTS @ 5800 MHz

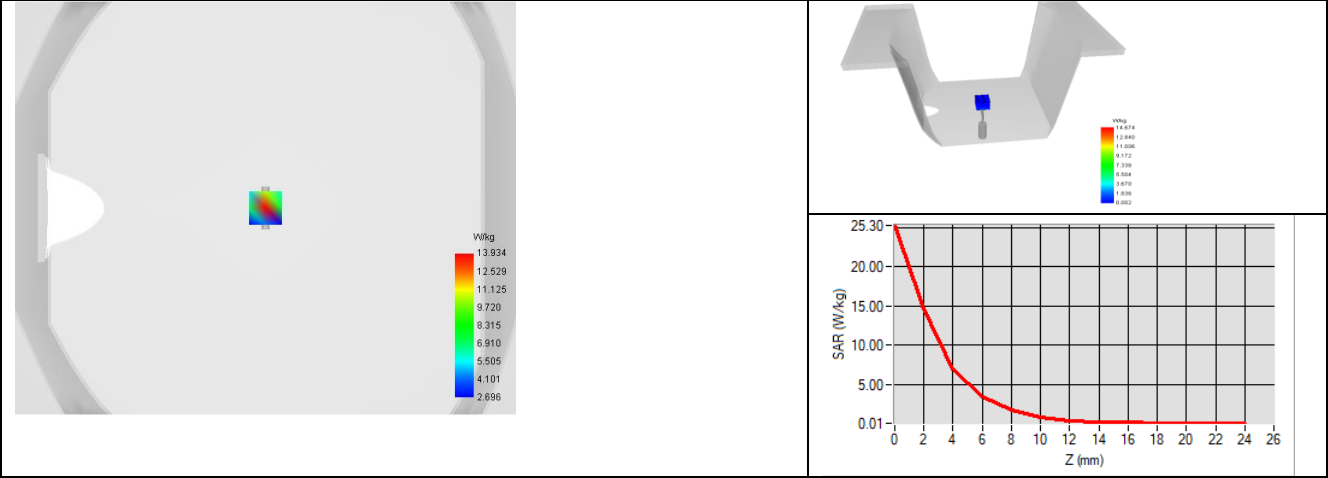

### 7.3 BODY LIQUID MEASUREMENT


| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 5200             | 49.0 $\pm$ 10 %                         | 45.50    | 5.30 $\pm$ 10 %               | 5.63     |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         | 44.78    | 5.53 $\pm$ 10 %               | 5.95     |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         | 44.85    | 5.77 $\pm$ 10 %               | 6.26     |
| 5800             | 48.2 $\pm$ 10 %                         | 44.45    | 6.00 $\pm$ 10 %               | 6.58     |

### 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID


|                                    |                                                                                                                                                                                                                                                                      |
|------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Software                           | OPENSAR V5                                                                                                                                                                                                                                                           |
| Phantom                            | SN 13/09 SAM68                                                                                                                                                                                                                                                       |
| Probe                              | SN 41/18 EPGO333                                                                                                                                                                                                                                                     |
| Liquid                             | Body Liquid Values 5200 MHz: $\epsilon_r'$ :45.50 sigma : 5.63<br>Body Liquid Values 5400 MHz: $\epsilon_r'$ :44.78 sigma : 5.95<br>Body Liquid Values 5600 MHz: $\epsilon_r'$ :44.85 sigma : 6.26<br>Body Liquid Values 5800 MHz: $\epsilon_r'$ :44.45 sigma : 6.58 |
| Distance between dipole and liquid | 10 mm                                                                                                                                                                                                                                                                |
| Area scan resolution               | dx=8mm/dy=8mm                                                                                                                                                                                                                                                        |
| Zoon Scan Resolution               | dx=4mm/dy=4m/dz=2mm                                                                                                                                                                                                                                                  |
| Frequency                          | 5200 MHz<br>5400 MHz<br>5600 MHz<br>5800 MHz                                                                                                                                                                                                                         |
| Input power                        | 20 dBm                                                                                                                                                                                                                                                               |
| Liquid Temperature                 | 20 +/- 1 °C                                                                                                                                                                                                                                                          |
| Lab Temperature                    | 20 +/- 1 °C                                                                                                                                                                                                                                                          |
| Lab Humidity                       | 30-70 %                                                                                                                                                                                                                                                              |

| Frequency (MHz) | 1 g SAR (W/kg) | 10 g SAR (W/kg) |
|-----------------|----------------|-----------------|
|                 | measured       | measured        |
| 5200            | 72.47 (7.25)   | 21.16 (2.12)    |
| 5400            | 79.06 (7.91)   | 22.85 (2.29)    |
| 5600            | 78.50 (7.85)   | 22.96 (2.30)    |
| 5800            | 72.20 (7.22)   | 21.13 (2.11)    |


## BODY SAR MEASUREMENT PLOTS @ 5200 MHz

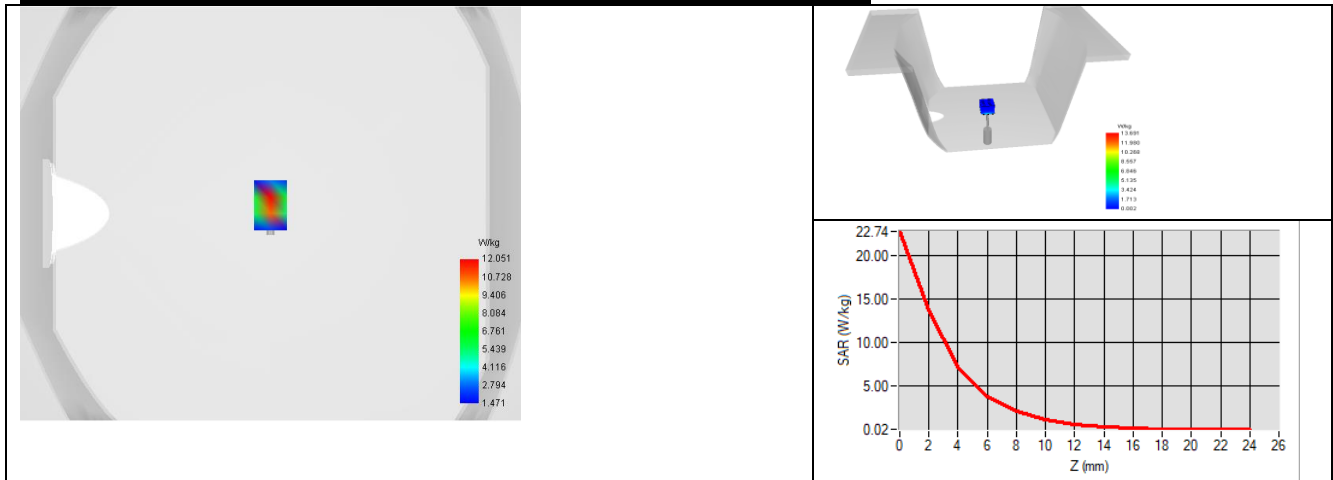


## BODY SAR MEASUREMENT PLOTS @ 5400 MHz

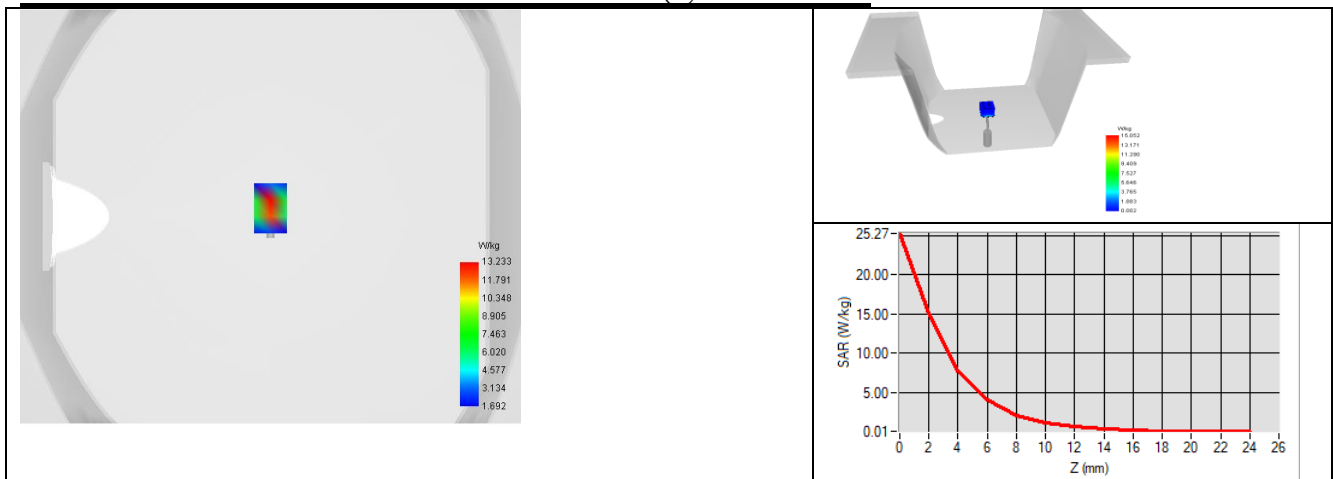

## BODY SAR MEASUREMENT PLOTS @ 5600 MHz

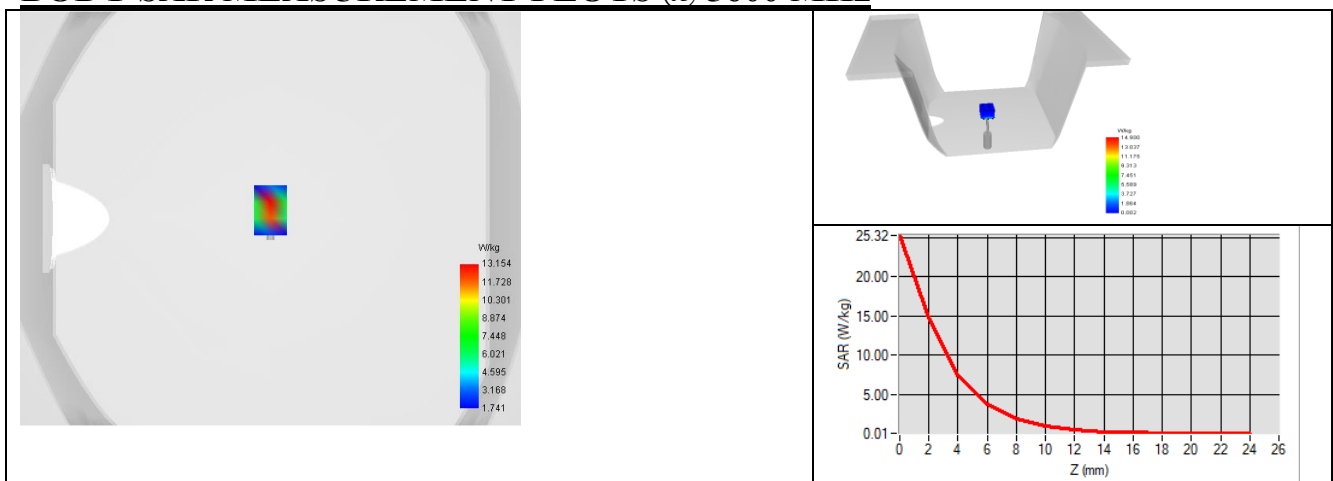

## BODY SAR MEASUREMENT PLOTS @ 5800 MHz

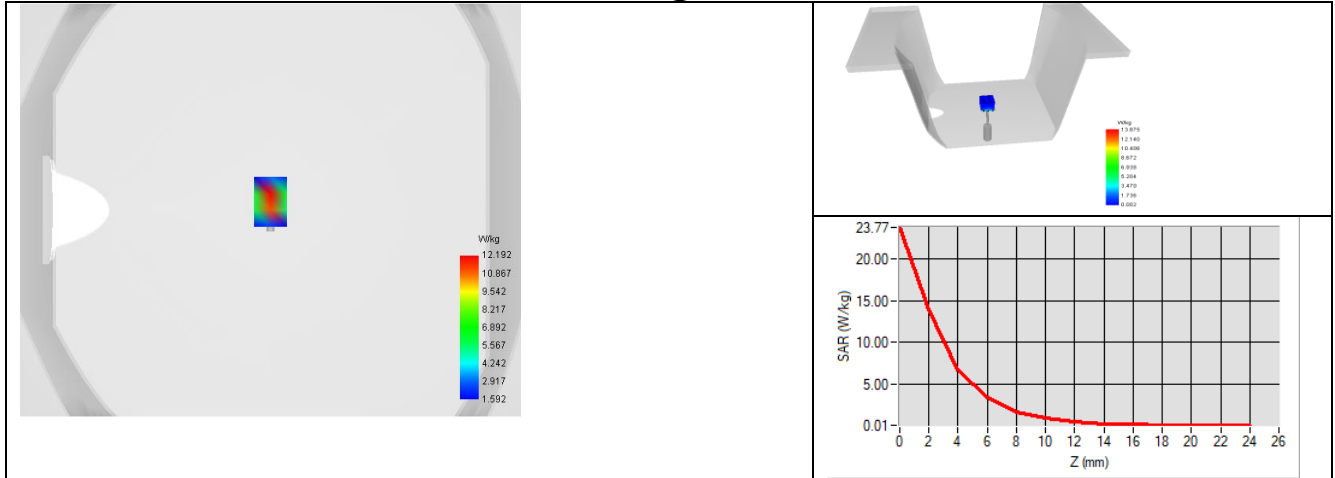



## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2021                                       | 08/2024                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 05/2022                                       | 05/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2023                                       | 10/2024                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2024                                       | 06/2027                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2024                                       | 06/2027                                       |