


Appendix D

Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

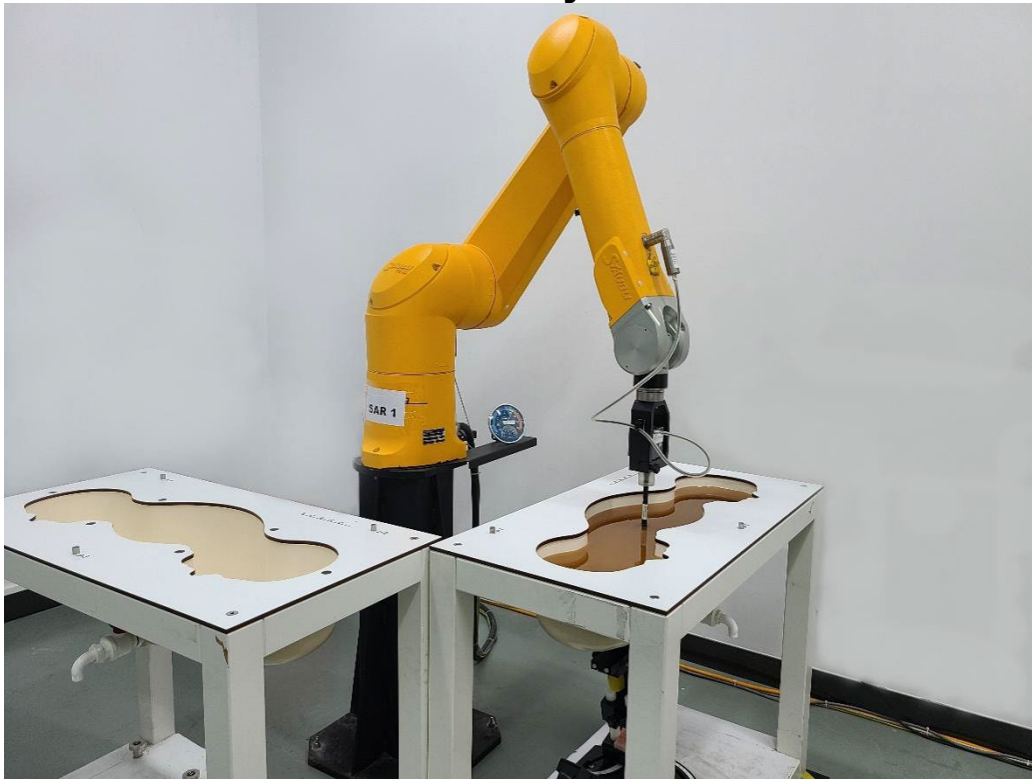

2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for HBBL600-10000MHz	NA
 A photograph showing a cross-section of a container filled with a yellowish, translucent liquid. A metal ruler is placed vertically next to the container, with the 10 cm mark visible. The container has a blue outer rim and a white inner lining. The liquid is contained within the white lining.	NA

3. Photographs of EUT test position

Photo 2: Back side open 0mm

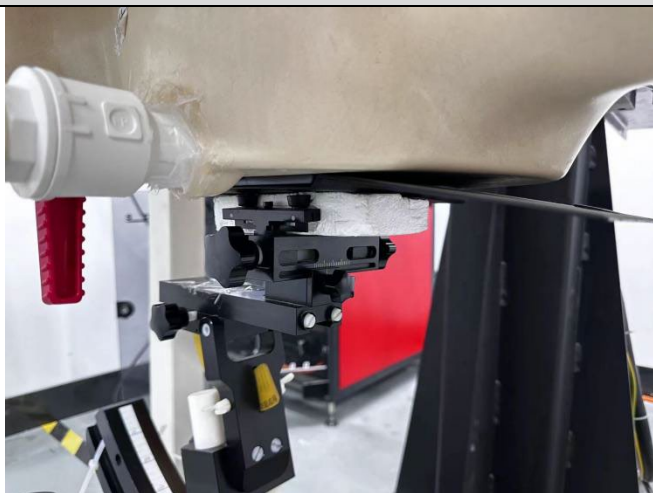


Photo 3: Back side close 0mm



Photo 4: Left Side 0mm



Photo 5: Right Side 0mm



Photo 6: Top Side 0mm





Photo 7: Bottom Side 0mm





4. EUT Constructional Details

Photo 8: Front open View



Photo 9: Back open View

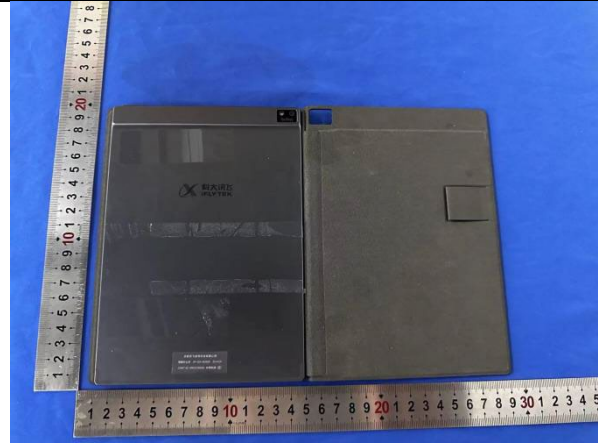


Photo 10: Front close View



Photo 11: Back close View

