


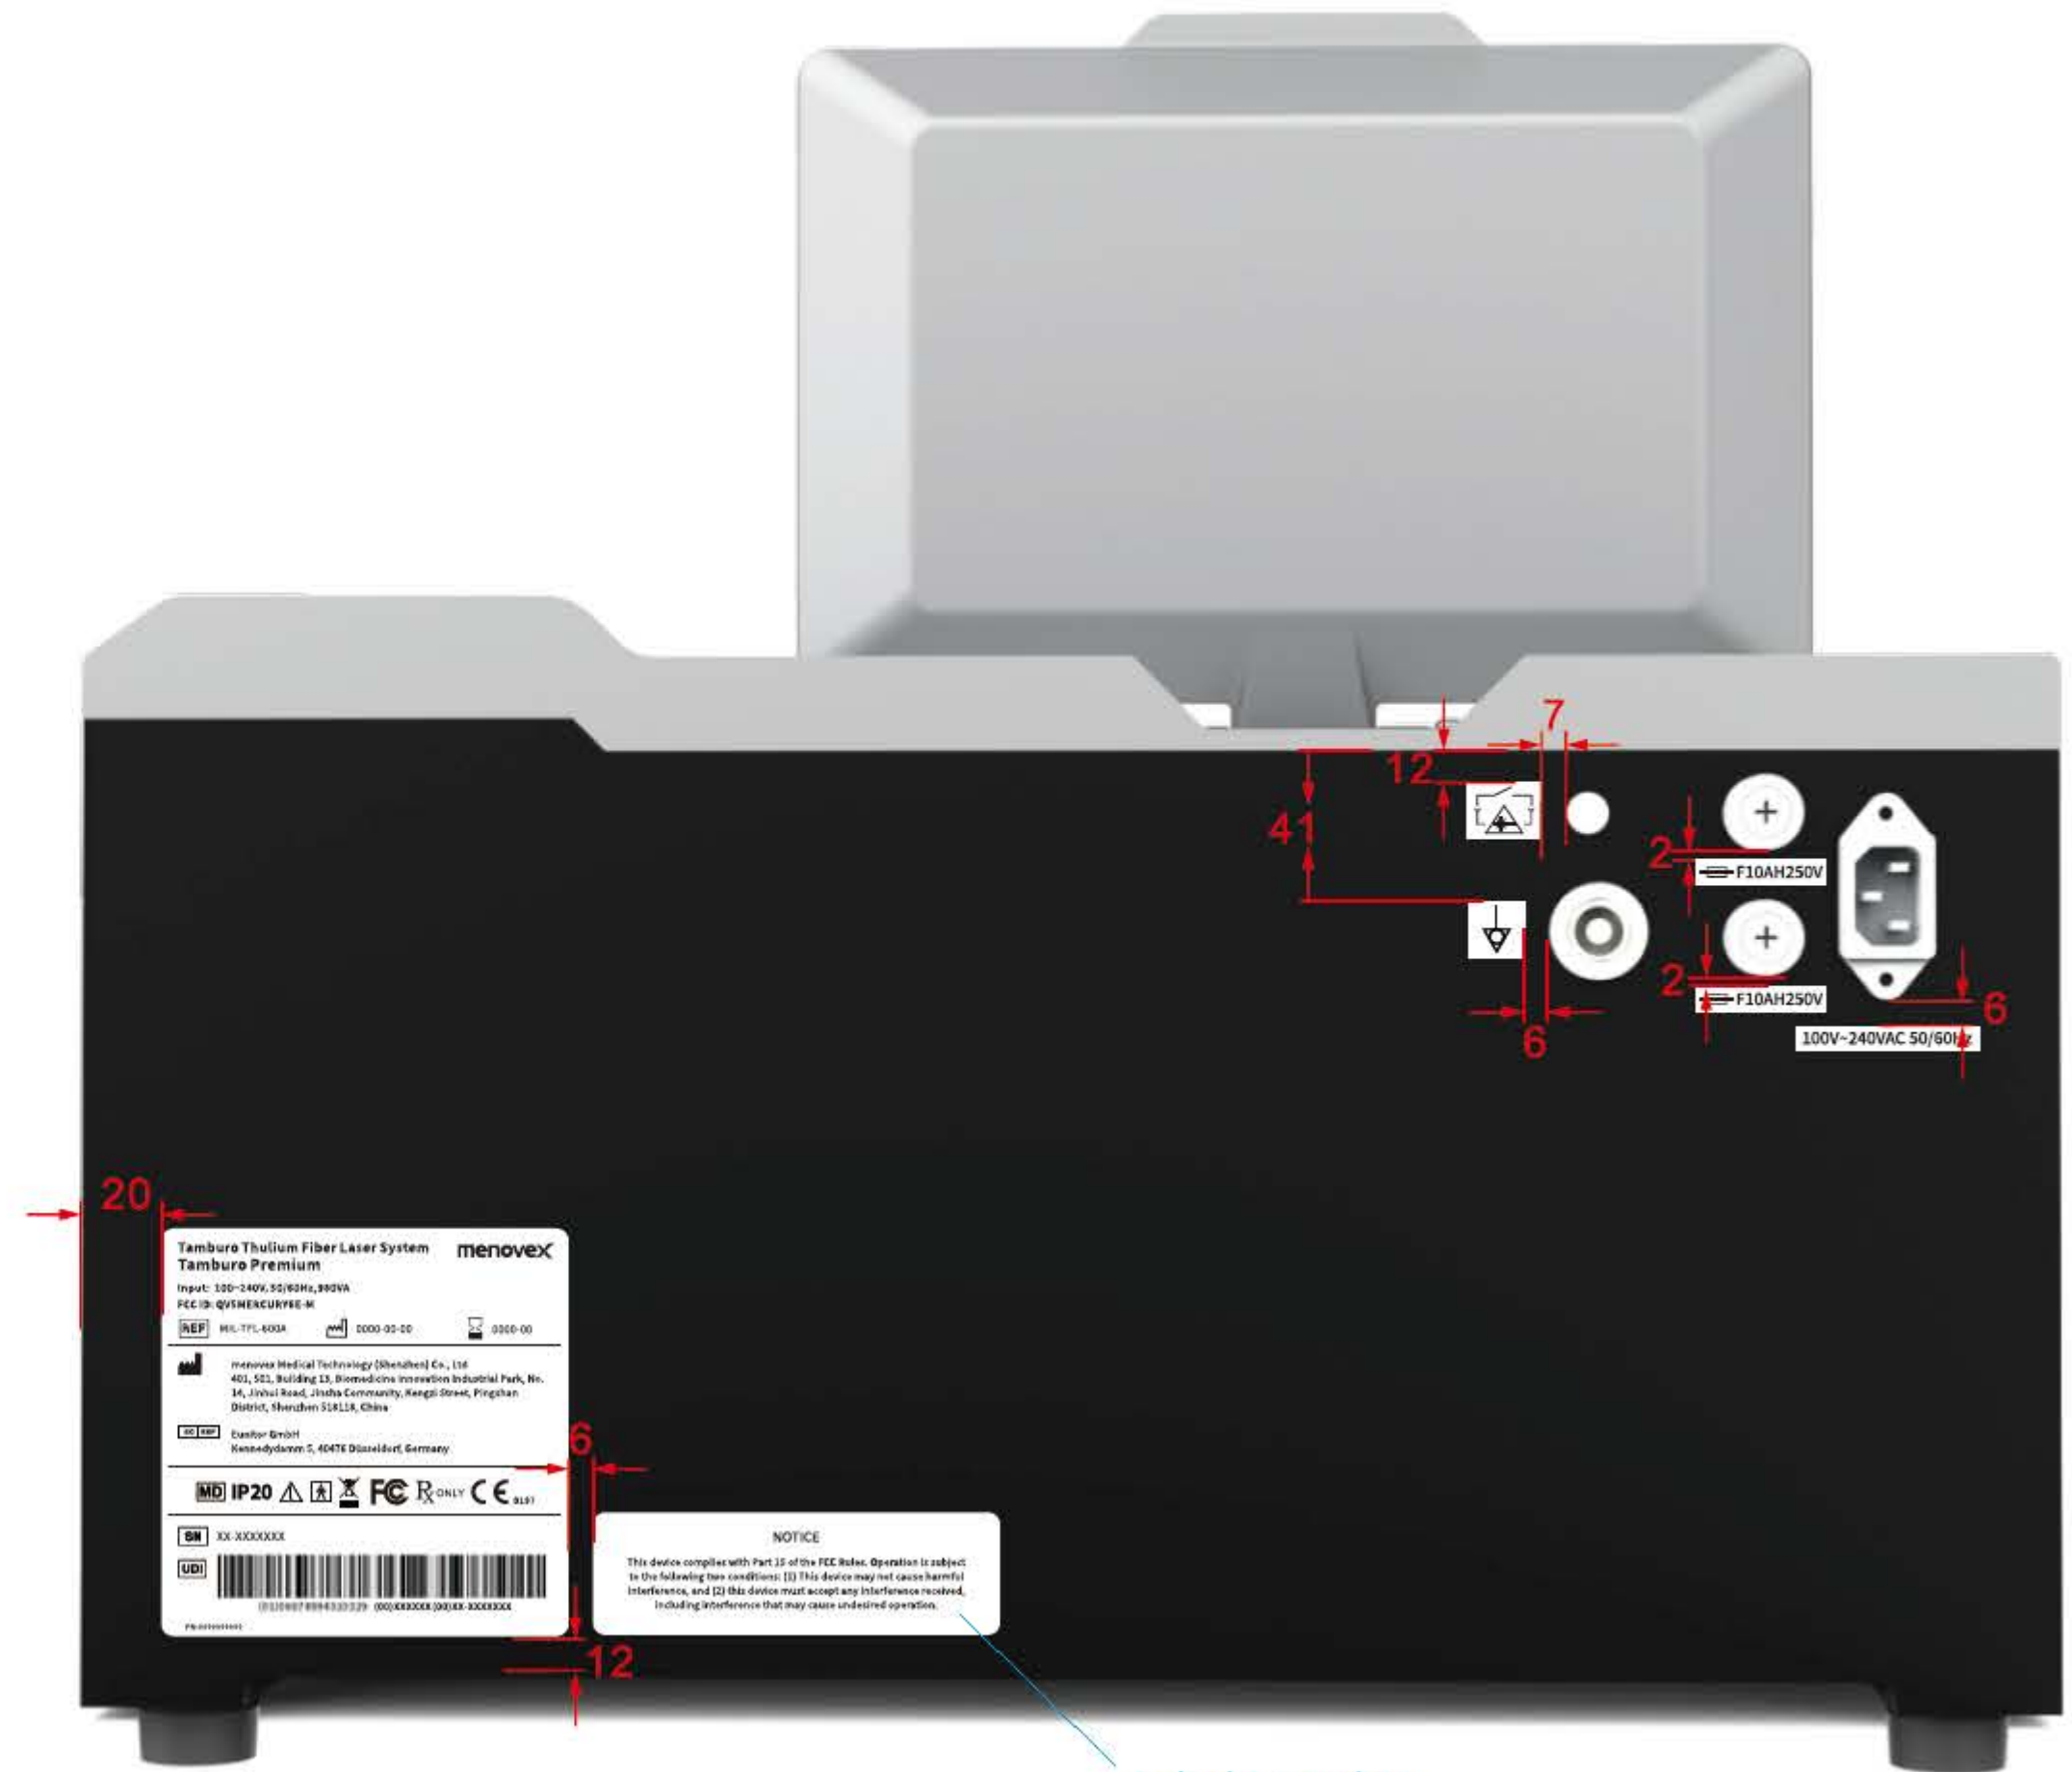

Label Location

NOTICE

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

密尔机密，未经许可不得扩散

1

2

3

4

5

6

7

8

9

10

A

B

C

D

E

F

G

H

A

B

C

D


E

F

G

H

版本	变更内容	日期
A0	初次发行	2024-04-25
A1	按《产品需求规格说明书》V03版更新	2024-10-10

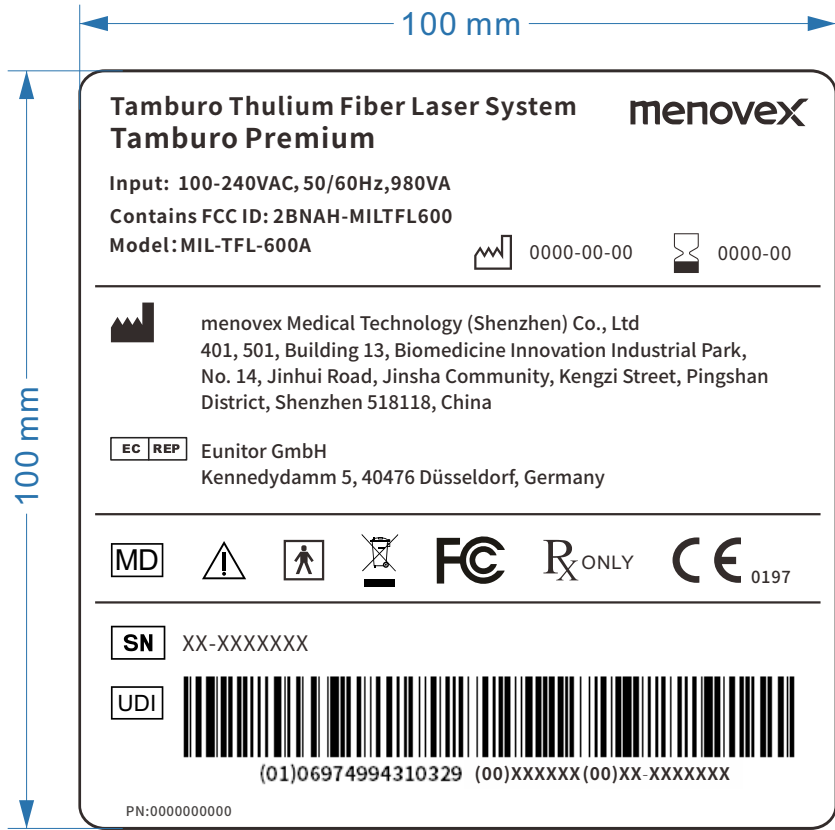

技术要求：

- 1、尺寸要求：如图所示
- 2、材质要求：合成纸+PM胶，耐磨；
- 3、其他要求：要求产品用料符合RoHS认证；图中生产日期、使用期限、SN码、LOT号、UDI（固定DI为06974994310329）、PN码按需求填写。

设计	MIL25	RA2301-B-04-18	材料	/
审核		设备标签-英文	重量	/
批准		RA2301	比例	1:1
				共3张第1张
				密尔医疗

1

2

3

4

5

6

7

8

9

10

A4