

## 7.1 HEAD LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 300              | 45.3 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 450              | 43.5 $\pm$ 10 %                         |          | 0.87 $\pm$ 10 %               |          |
| 750              | 41.9 $\pm$ 10 %                         |          | 0.89 $\pm$ 10 %               |          |
| 835              | 41.5 $\pm$ 10 %                         | 39.9     | 0.90 $\pm$ 10 %               | 0.92     |
| 900              | 41.5 $\pm$ 10 %                         |          | 0.97 $\pm$ 10 %               |          |
| 1450             | 40.5 $\pm$ 10 %                         |          | 1.20 $\pm$ 10 %               |          |
| 1500             | 40.4 $\pm$ 10 %                         |          | 1.23 $\pm$ 10 %               |          |
| 1640             | 40.2 $\pm$ 10 %                         |          | 1.31 $\pm$ 10 %               |          |
| 1750             | 40.1 $\pm$ 10 %                         |          | 1.37 $\pm$ 10 %               |          |
| 1800             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1900             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1950             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2000             | 40.0 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 2100             | 39.8 $\pm$ 10 %                         |          | 1.49 $\pm$ 10 %               |          |
| 2300             | 39.5 $\pm$ 10 %                         |          | 1.67 $\pm$ 10 %               |          |
| 2450             | 39.2 $\pm$ 10 %                         |          | 1.80 $\pm$ 10 %               |          |
| 2600             | 39.0 $\pm$ 10 %                         |          | 1.96 $\pm$ 10 %               |          |
| 3000             | 38.5 $\pm$ 10 %                         |          | 2.40 $\pm$ 10 %               |          |
| 3300             | 38.2 $\pm$ 10 %                         |          | 2.71 $\pm$ 10 %               |          |
| 3500             | 37.9 $\pm$ 10 %                         |          | 2.91 $\pm$ 10 %               |          |
| 3700             | 37.7 $\pm$ 10 %                         |          | 3.12 $\pm$ 10 %               |          |
| 3900             | 37.5 $\pm$ 10 %                         |          | 3.32 $\pm$ 10 %               |          |
| 4200             | 37.1 $\pm$ 10 %                         |          | 3.63 $\pm$ 10 %               |          |
| 4600             | 36.7 $\pm$ 10 %                         |          | 4.04 $\pm$ 10 %               |          |
| 4900             | 36.3 $\pm$ 10 %                         |          | 4.35 $\pm$ 10 %               |          |

## 7.2 SAR MEASUREMENT RESULT WITH HEAD LIQUID

The IEC/IEEE 62209-1528 and FCC KDB865664 D01 standards state that the system validation measurements should produce the SAR values shown below (for phantom thickness of 2 mm), within the uncertainty for the system validation. All SAR values are normalized to 1 W forward power. In bracket, the measured SAR is given with the used input power.




## SAR REFERENCE DIPOLE CALIBRATION REPORT

Ref: ACR.42.11.25.BES.A

|                                           |                                                          |
|-------------------------------------------|----------------------------------------------------------|
| Software                                  | OPENSAR V5                                               |
| Phantom                                   | SN 13/09 SAM68                                           |
| Probe                                     | SN 41/18 EPGO333                                         |
| Liquid                                    | Head Liquid Values: $\epsilon_s'$ : 39.9 $\sigma$ : 0.91 |
| Distance between dipole center and liquid | 15.0 mm                                                  |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                          |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                   |
| Frequency                                 | 835 MHz                                                  |
| Input power                               | 20 dBm                                                   |
| Liquid Temperature                        | 20 +/- 1 °C                                              |
| Lab Temperature                           | 20 +/- 1 °C                                              |
| Lab Humidity                              | 30-70 %                                                  |

| Frequency<br>MHz | 1 g SAR (W/kg/W) |             | 10 g SAR (W/kg/W) |             |
|------------------|------------------|-------------|-------------------|-------------|
|                  | required         | measured    | required          | measured    |
| 300              | 2.85             |             | 1.94              |             |
| 450              | 4.58             |             | 3.06              |             |
| 750              | 8.49             |             | 5.55              |             |
| 835              | 9.56             | 9.73 (0.97) | 6.22              | 6.19 (0.62) |
| 900              | 10.9             |             | 6.99              |             |
| 1450             | 29               |             | 16                |             |
| 1500             | 30.5             |             | 16.8              |             |
| 1640             | 34.2             |             | 18.4              |             |
| 1750             | 36.4             |             | 19.3              |             |
| 1800             | 38.4             |             | 20.1              |             |
| 1900             | 39.7             |             | 20.5              |             |
| 1950             | 40.5             |             | 20.9              |             |
| 2000             | 41.1             |             | 21.1              |             |
| 2100             | 43.6             |             | 21.9              |             |
| 2300             | 48.7             |             | 23.3              |             |
| 2450             | 52.4             |             | 24                |             |
| 2600             | 55.3             |             | 24.6              |             |
| 3000             | 63.8             |             | 25.7              |             |
| 3300             | -                |             | -                 |             |
| 3500             | 67.1             |             | 25                |             |
| 3700             | 67.4             |             | 24.2              |             |
| 3900             | -                |             | -                 |             |
| 4200             | -                |             | -                 |             |
| 4600             | -                |             | -                 |             |
| 4900             | -                |             | -                 |             |

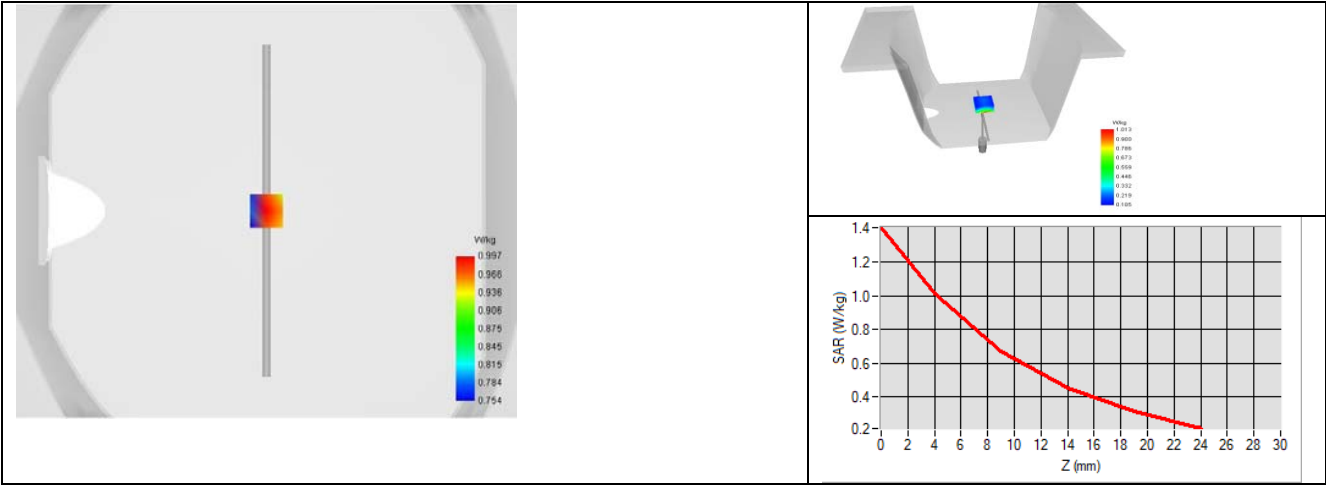


### 7.3 BODY LIQUID MEASUREMENT

| Frequency<br>MHz | Relative permittivity ( $\epsilon_r'$ ) |          | Conductivity ( $\sigma$ ) S/m |          |
|------------------|-----------------------------------------|----------|-------------------------------|----------|
|                  | required                                | measured | required                      | measured |
| 150              | 61.9 $\pm$ 10 %                         |          | 0.80 $\pm$ 10 %               |          |
| 300              | 58.2 $\pm$ 10 %                         |          | 0.92 $\pm$ 10 %               |          |
| 450              | 56.7 $\pm$ 10 %                         |          | 0.94 $\pm$ 10 %               |          |
| 750              | 55.5 $\pm$ 10 %                         |          | 0.96 $\pm$ 10 %               |          |
| 835              | 55.2 $\pm$ 10 %                         | 52.5     | 0.97 $\pm$ 10 %               | 0.95     |
| 900              | 55.0 $\pm$ 10 %                         |          | 1.05 $\pm$ 10 %               |          |
| 915              | 55.0 $\pm$ 10 %                         |          | 1.06 $\pm$ 10 %               |          |
| 1450             | 54.0 $\pm$ 10 %                         |          | 1.30 $\pm$ 10 %               |          |
| 1610             | 53.8 $\pm$ 10 %                         |          | 1.40 $\pm$ 10 %               |          |
| 1800             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 1900             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2000             | 53.3 $\pm$ 10 %                         |          | 1.52 $\pm$ 10 %               |          |
| 2100             | 53.2 $\pm$ 10 %                         |          | 1.62 $\pm$ 10 %               |          |
| 2300             | 52.9 $\pm$ 10 %                         |          | 1.81 $\pm$ 10 %               |          |
| 2450             | 52.7 $\pm$ 10 %                         |          | 1.95 $\pm$ 10 %               |          |
| 2600             | 52.5 $\pm$ 10 %                         |          | 2.16 $\pm$ 10 %               |          |
| 3000             | 52.0 $\pm$ 10 %                         |          | 2.73 $\pm$ 10 %               |          |
| 3300             | 51.6 $\pm$ 10 %                         |          | 3.08 $\pm$ 10 %               |          |
| 3500             | 51.3 $\pm$ 10 %                         |          | 3.31 $\pm$ 10 %               |          |
| 3700             | 51.0 $\pm$ 10 %                         |          | 3.55 $\pm$ 10 %               |          |
| 3900             | 50.8 $\pm$ 10 %                         |          | 3.78 $\pm$ 10 %               |          |
| 4200             | 50.4 $\pm$ 10 %                         |          | 4.13 $\pm$ 10 %               |          |
| 4600             | 49.8 $\pm$ 10 %                         |          | 4.60 $\pm$ 10 %               |          |
| 4900             | 49.4 $\pm$ 10 %                         |          | 4.95 $\pm$ 10 %               |          |
| 5200             | 49.0 $\pm$ 10 %                         |          | 5.30 $\pm$ 10 %               |          |
| 5300             | 48.9 $\pm$ 10 %                         |          | 5.42 $\pm$ 10 %               |          |
| 5400             | 48.7 $\pm$ 10 %                         |          | 5.53 $\pm$ 10 %               |          |
| 5500             | 48.6 $\pm$ 10 %                         |          | 5.65 $\pm$ 10 %               |          |
| 5600             | 48.5 $\pm$ 10 %                         |          | 5.77 $\pm$ 10 %               |          |
| 5800             | 48.2 $\pm$ 10 %                         |          | 6.00 $\pm$ 10 %               |          |

#### 7.4 SAR MEASUREMENT RESULT WITH BODY LIQUID

|                                           |                                                             |
|-------------------------------------------|-------------------------------------------------------------|
| Software                                  | OPENSAR V5                                                  |
| Phantom                                   | SN 13/09 SAM68                                              |
| Probe                                     | SN 41/18 EPGO333                                            |
| Liquid                                    | Body Liquid Values: $\epsilon_{ps}'$ : 52.3 $\sigma$ : 0.94 |
| Distance between dipole center and liquid | 15.0 mm                                                     |
| Area scan resolution                      | $dx=8mm/dy=8mm$                                             |
| Zoon Scan Resolution                      | $dx=8mm/dy=8mm/dz=5mm$                                      |
| Frequency                                 | 835 MHz                                                     |
| Input power                               | 20 dBm                                                      |
| Liquid Temperature                        | 20 +/- 1 °C                                                 |
| Lab Temperature                           | 20 +/- 1 °C                                                 |
| Lab Humidity                              | 30-70 %                                                     |

| Frequency<br>MHz | 1 g SAR (W/kg/W) | 10 g SAR (W/kg/W) |
|------------------|------------------|-------------------|
|                  | measured         | measured          |
| 835              | 9.77 (0.98)      | 6.34 (0.63)       |

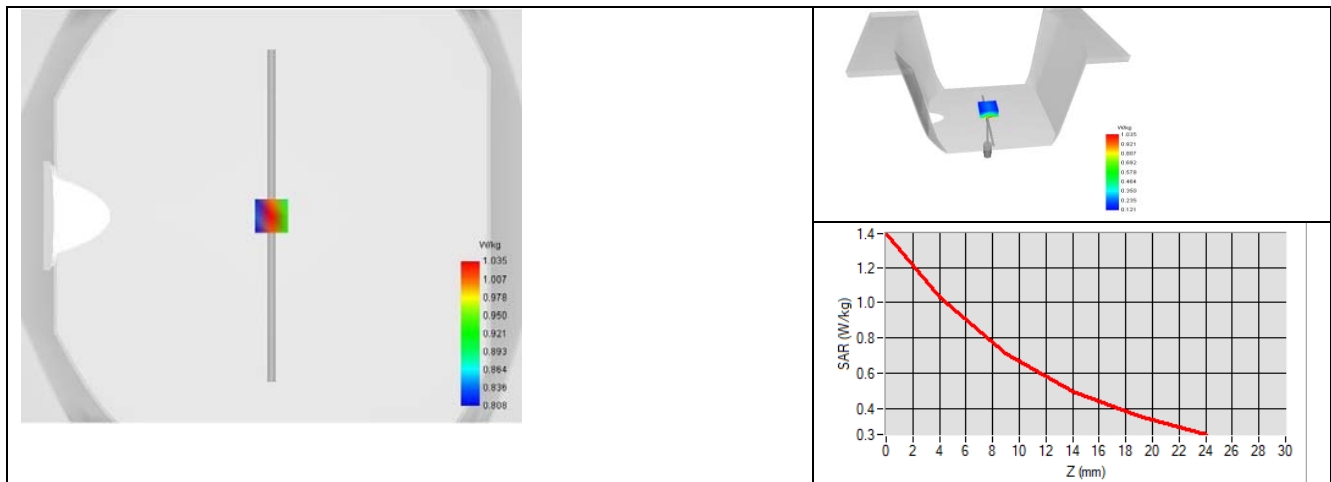

## 8 LIST OF EQUIPMENT

| Equipment Summary Sheet            |                         |                    |                                               |                                               |
|------------------------------------|-------------------------|--------------------|-----------------------------------------------|-----------------------------------------------|
| Equipment Description              | Manufacturer / Model    | Identification No. | Current Calibration Date                      | Next Calibration Date                         |
| SAM Phantom                        | MVG                     | SN 13/09 SAM68     | Validated. No cal required.                   | Validated. No cal required.                   |
| COMOSAR Test Bench                 | Version 3               | NA                 | Validated. No cal required.                   | Validated. No cal required.                   |
| Network Analyzer                   | Rohde & Schwarz ZVM     | 100203             | 08/2024                                       | 08/2027                                       |
| Network Analyzer                   | Agilent 8753ES          | MY40003210         | 10/2022                                       | 10/2025                                       |
| Network Analyzer – Calibration kit | Rohde & Schwarz ZV-Z235 | 101223             | 07/2022                                       | 07/2025                                       |
| Network Analyzer – Calibration kit | HP 85033D               | 3423A08186         | 06/2021                                       | 06/2027                                       |
| Calipers                           | Mitutoyo                | SN 0009732         | 10/2022                                       | 10/2025                                       |
| Reference Probe                    | MVG                     | SN 41/18 EPGO333   | 10/2024                                       | 10/2025                                       |
| Multimeter                         | Keithley 2000           | 1160271            | 02/2023                                       | 02/2026                                       |
| Signal Generator                   | Rohde & Schwarz SMB     | 106589             | 04/2022                                       | 04/2025                                       |
| Amplifier                          | MVG                     | MODU-023-C-0002    | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Power Meter                        | NI-USB 5680             | 170100013          | 06/2021                                       | 06/2026                                       |
| Power Meter                        | Rohde & Schwarz NRVD    | 832839-056         | 11/2022                                       | 11/2025                                       |
| Directional Coupler                | Krytar 158020           | 131467             | Characterized prior to test. No cal required. | Characterized prior to test. No cal required. |
| Temperature / Humidity Sensor      | Testo 184 H1            | 44225320           | 06/2024                                       | 06/2027                                       |



## SAR Reference Dipole Calibration Report

Ref : ACR.42.13.25.BES.A

### **LGT(SHENZHEN) TEST TECHNOLOGY CO., LTD.**

**13-B205, ZONE B, CHEN HSONG INDUSTRIAL  
PARK(SHENZHEN), NO.33 RENMIN MIDDLE ROAD,  
JINSHA COMMUNITY**

**KENGZI SUBDISTRICT, PINGSHAN NEW DISTRICT,  
SHENZHEN, GUANGDONG, CHINA**

### **MVG COMOSAR REFERENCE DIPOLE**

**FREQUENCY: 1900 MHZ**

**SERIAL NO.: SN 06/22 DIP1G900-641**

**Calibrated at MVG**

**Z.I. de la pointe du diable**

**Technopôle Brest Iroise – 295 avenue Alexis de Rochon**

**29280 PLOUZANE - FRANCE**

**Calibration date: 02/05/2025**



Accreditations #2-6789 and #2-6814  
Scope available on [www.cofrac.fr](http://www.cofrac.fr)

**The use of the Cofrac brand and the accreditation references is prohibited from any reproduction.**

#### *Summary:*

This document presents the method and results from an accredited SAR reference dipole calibration performed in MVG using the COMOSAR test bench. All calibration results are traceable to national metrology institutions.



|                      | <i>Name</i>  | <i>Function</i>     | <i>Date</i> | <i>Signature</i>    |
|----------------------|--------------|---------------------|-------------|---------------------|
| <i>Prepared by :</i> | Jérôme Luc   | Technical Manager   | 2/05/2025   | <i>JS</i>           |
| <i>Checked by :</i>  | Jérôme Luc   | Technical Manager   | 2/05/2025   | <i>JS</i>           |
| <i>Approved by :</i> | Yann Toutain | Laboratory Director | 2/05/2025   | <i>Yann TOUTAIN</i> |

2025.02.05  
13:26:59 +01'00'

|                       | <i>Customer Name</i>                          |
|-----------------------|-----------------------------------------------|
| <i>Distribution :</i> | LGT(Shenzhen)<br>Test Technology<br>Co., Ltd. |

| <i>Issue</i> | <i>Name</i> | <i>Date</i> | <i>Modifications</i> |
|--------------|-------------|-------------|----------------------|
| A            | Jérôme Luc  | 2/05/2025   | Initial release      |
|              |             |             |                      |
|              |             |             |                      |
|              |             |             |                      |



## TABLE OF CONTENTS

|     |                                                |    |
|-----|------------------------------------------------|----|
| 1   | Introduction.....                              | 4  |
| 2   | Device Under Test .....                        | 4  |
| 3   | Product Description .....                      | 4  |
| 3.1 | General Information .....                      | 4  |
| 4   | Measurement Method .....                       | 5  |
| 4.1 | Return Loss Requirements .....                 | 5  |
| 4.2 | Mechanical Requirements .....                  | 5  |
| 5   | Measurement Uncertainty .....                  | 5  |
| 5.1 | Return Loss .....                              | 5  |
| 5.2 | Dimension Measurement .....                    | 5  |
| 5.3 | Validation Measurement .....                   | 5  |
| 6   | Calibration Measurement Results .....          | 6  |
| 6.1 | Return Loss and Impedance In Head Liquid ..... | 6  |
| 6.2 | Return Loss and Impedance In Body Liquid ..... | 6  |
| 6.3 | Mechanical Dimensions .....                    | 7  |
| 7   | Validation measurement .....                   | 7  |
| 7.1 | Head Liquid Measurement .....                  | 8  |
| 7.2 | SAR Measurement Result With Head Liquid .....  | 8  |
| 7.3 | Body Liquid Measurement .....                  | 11 |
| 7.4 | SAR Measurement Result With Body Liquid .....  | 12 |
| 8   | List of Equipment .....                        | 13 |