

# Label Information - ICU\_301\_APF\_03\_N

DOCUMENT HISTORY

| VERSION | DATE        | STATUS  | DESCRIPTION     | ROLE | AUTHOR          |
|---------|-------------|---------|-----------------|------|-----------------|
| 0.1     | 06.05.2024. | Draft   | Initial version | EHW  | Matija Ratkajec |
| 0.2     | 04.02.2025  | Release | Update          | PM   | Radomir Čituš   |
| 0.3     | 27.07.2025  | release | Update          | PM   | Radomir Čituš   |
|         |             |         |                 |      |                 |
|         |             |         |                 |      |                 |

## TABLE OF CONTENTS

|   |                      |   |
|---|----------------------|---|
| 1 | Label .....          | 5 |
| 2 | Label location ..... | 5 |

LIST OF FIGURES

|                              |   |
|------------------------------|---|
| Figure 1 Label .....         | 5 |
| Figure 2 Label location..... | 5 |

CONFID. STATEMENT

## 1 Label

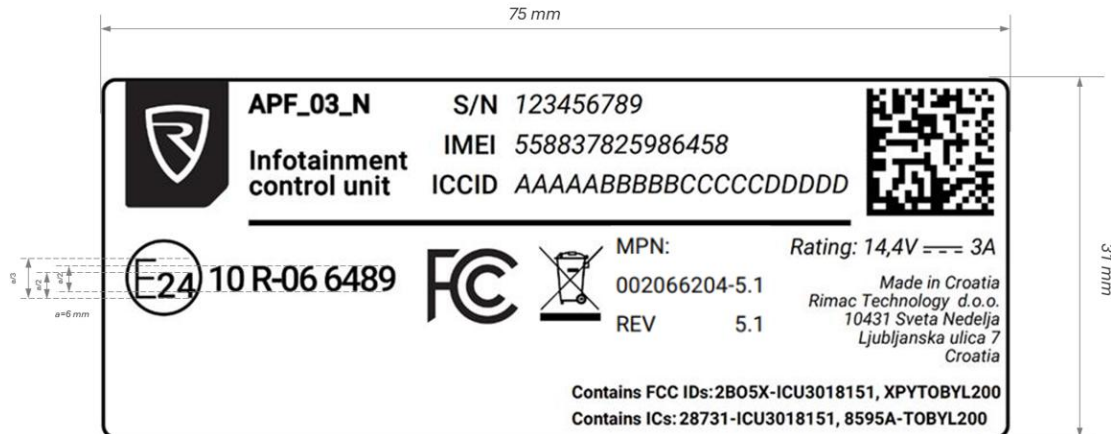


Figure 1 Label

## 2 Label location

Label is located on the bottom side of the device, as illustrated in Figure 2. All dimensions are in millimeters (mm).

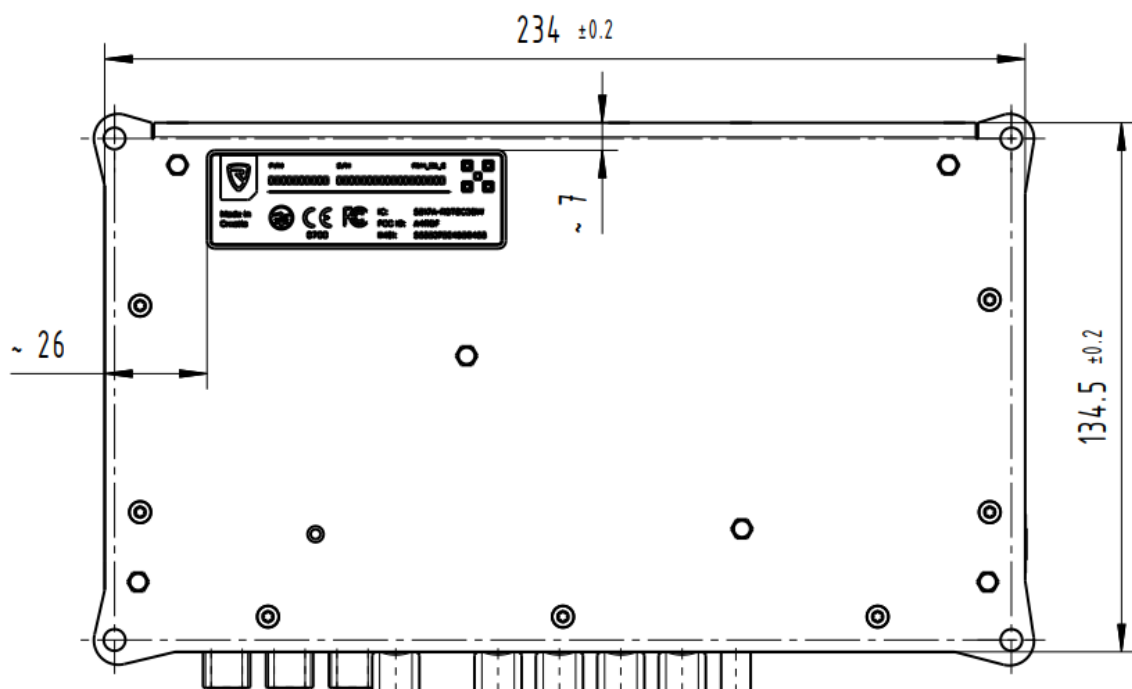


Figure 2 Label location