



Appendix D


Photographs

- | |
|--|
| 1. SAR measurement System |
| 2. Photographs of Tissue Simulate Liquid |
| 3. Photographs of EUT test position |
| 4. EUT Constructional Details |





1. SAR measurement System

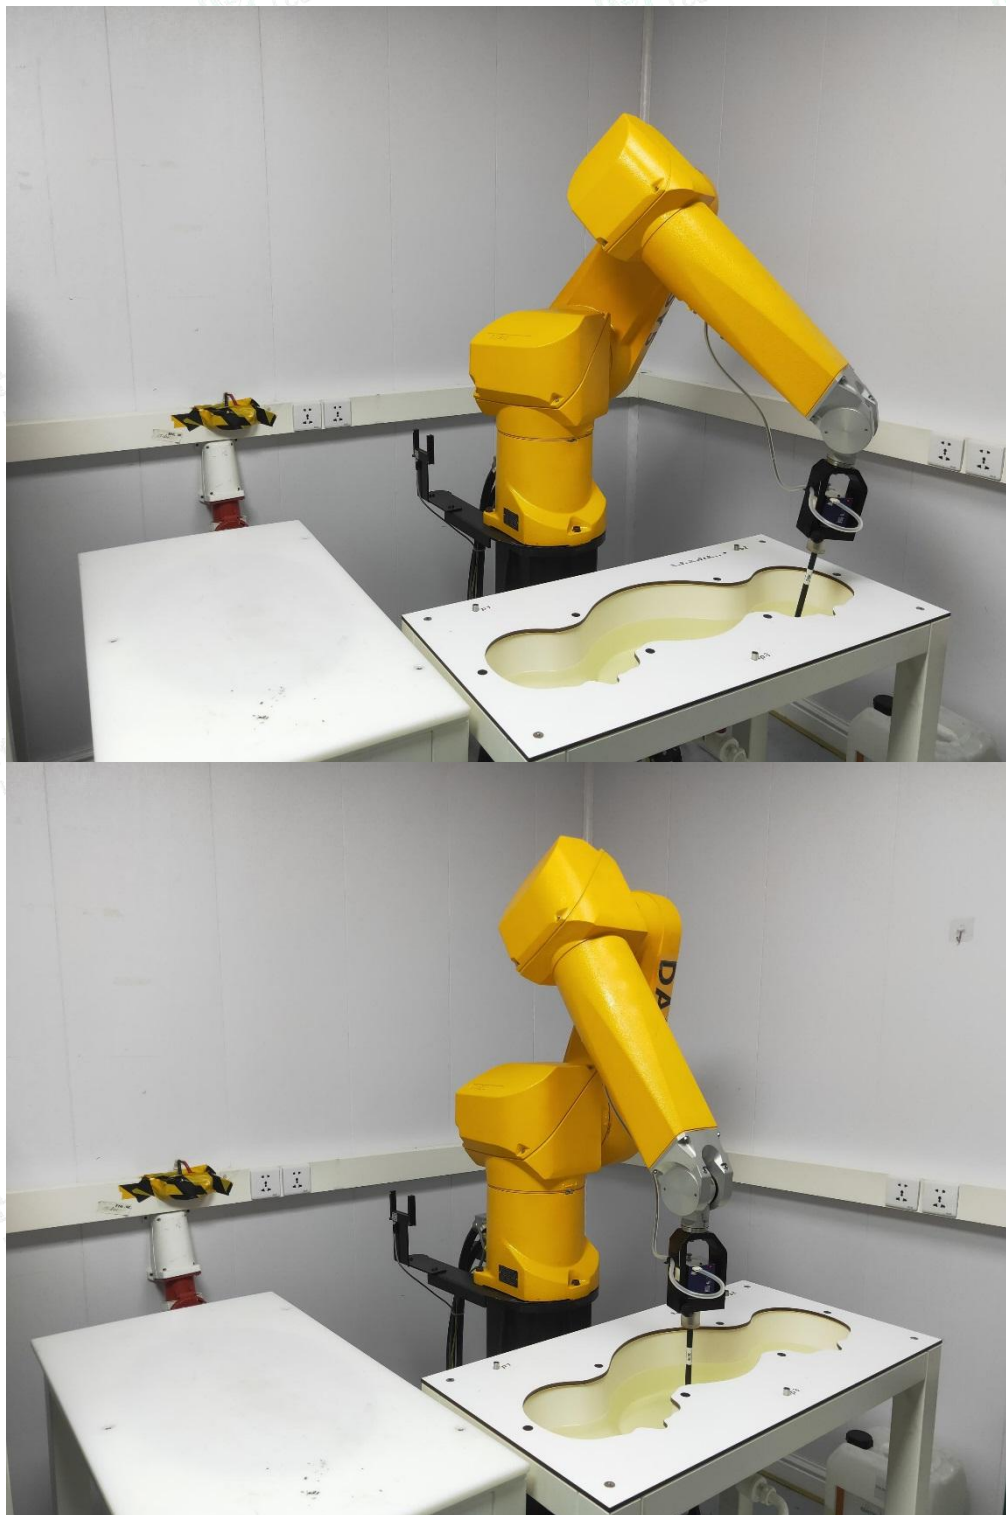



2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 300-3000 Mhz


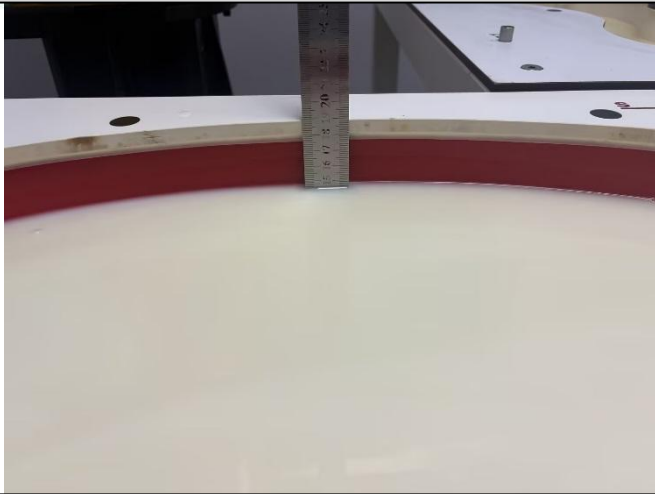


Photo 2: Tissue Simulant Liquid for Head 3000-8000 Mhz



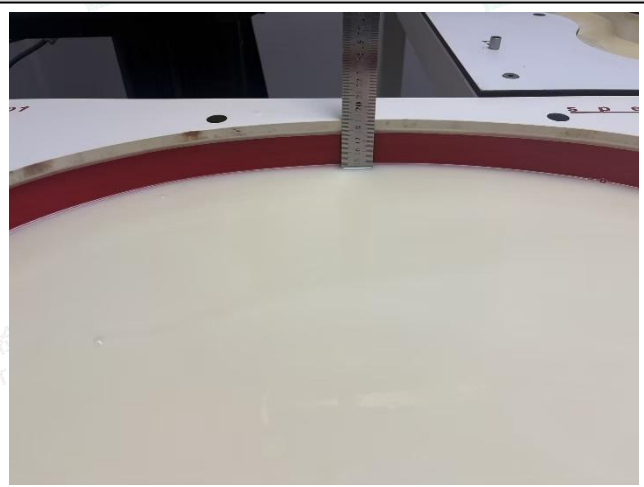

3. Photographs of EUT test position

Photo 3: Rear side 0mm





4. EUT Constructional Details

Photo 4: View 1

Photo 5: View 2

Photo 6: View 3

